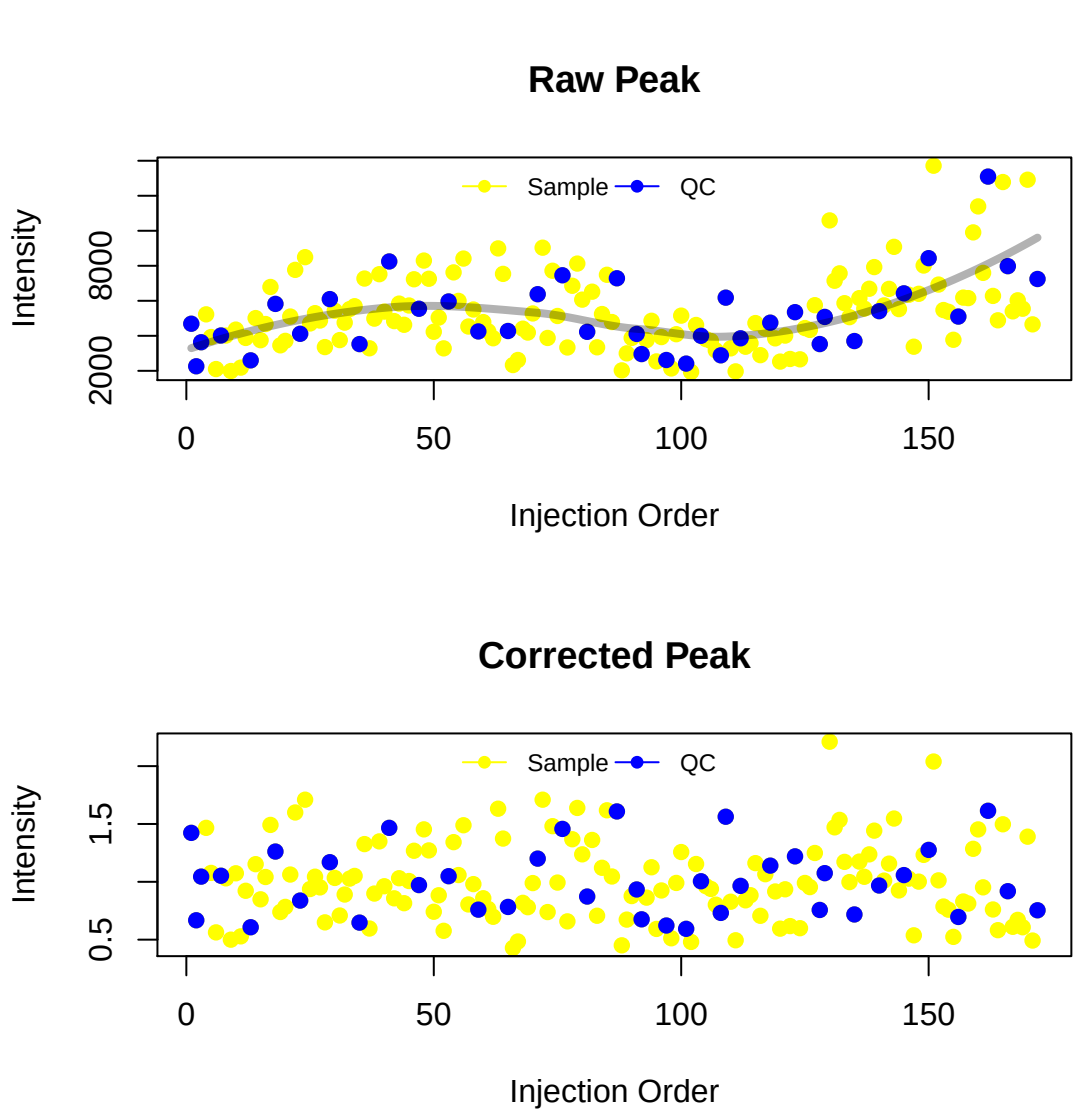
Raw Peak
Sample
QC
Intensity
2000
8000
0
50
100
150
Injection Order
Corrected Peak
Sample
QC
Intensity
0.5
1.5
0
50
100
150
Injection Order