




Quality Assurance Management, Inc.
1620 Valwood Pkwy, Ste. 128
Carrollton, TX 75006
972-331-5800
QAM.com

Oxygen Test Report

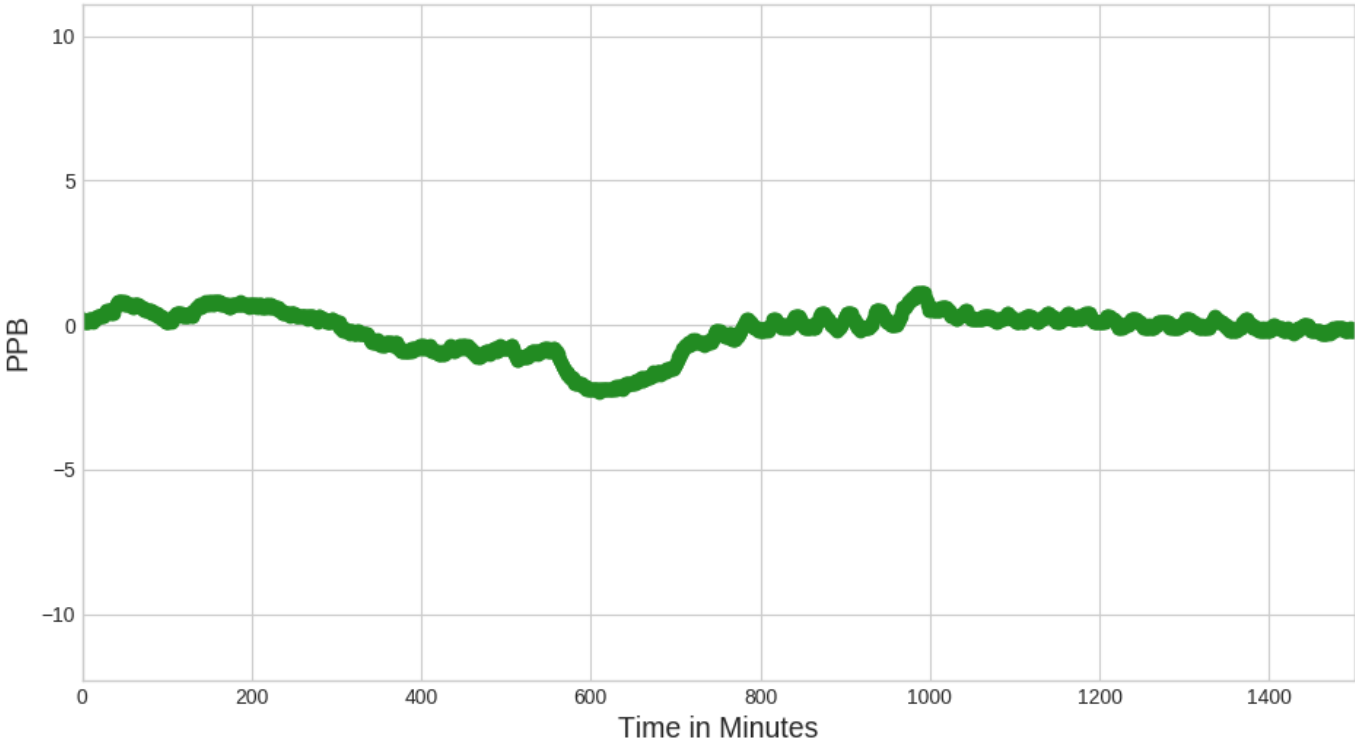

Client:	TEST CLIENT	Oxygen Analyzer:	Delta F
Facility:	QAM HQ	Serial Number:	PT-23473-V6
Tool / Equipment ID:		Calibration Due:	Not calibrated
System:		Instrument Flow (SCFH):	2.0 SCFH
Source ID:		Start Time / Date:	16:03 06/16/21
Test Point ID:		Stop Time / Date:	17:04 06/17/21
Test Gas:		Test Duration:	1 hours 1 minutes
Test Flow:	4.3 SCFH	Average:	-0.2 PPB
Technician:		Final:	-0.2 PPB
		Specification:	20 PPB

Comments: