

Automated PMSM Parameter Identification

by: Josef Tkadlec

1 Introduction

Advanced motor control techniques, such as the sensorless Field Oriented Control (FOC), require knowledge of motor parameters to properly set current controllers and the BEMF observer. Conventional Permanent Magnet Synchronous Motor (PMSM) measurement techniques are described in-depth in [Reference \[1\]](#). On the one hand, the techniques are accurate and reliable, on the other hand, they are time-consuming, require extra equipment, and the user must have background knowledge of motor control. For this reason, Freescale has developed easy to use electrical parameter measurement routines. These routines are delivered as a part of a motor control application and controlled using the Motor Control Application Tuning (MCAT) Tool and FreeMASTER.

This application note describes the MCAT *motor identification tab*, briefly explains how the measurement routines work, provides step-by-step instructions to run the identification process in MCAT, and explains how to troubleshoot faults and warnings that occur during the measurement process. This motor parameter identification process is an extension of the PMSM sensorless control application, however, this application note describes only the *motor identification tab* of the MCAT tool.

Contents

1	Introduction.....	1
2	MCAT motor identification tab description.....	2
2.1	Power stage characterization.....	4
2.2	Measurement.....	5
2.3	Number of pole-pair assistant.....	6
3	Using the motor identification tab.....	7
4	Fault handling.....	8
5	References.....	9

2 MCAT motor identification tab description

The MCAT motor identification tab shown in [Figure 1](#) consists of the following sections:

- **Application scales**—includes quantities that cannot be measured, such as hardware scales, nominal speed, and the number of pole-pairs.
- **Rs and Ls measurement**—defines the parameters of stator resistance (R_s) and stator inductance (L_s) within the measured signal.
- **Number of pole-pairs assistant**—enables the user to determine the number of pole-pairs.
- **Measured Rs and Ls**—displays identified motor parameters.

MCAT offers two tuning modes:

- **Basic**—highly recommended for users who are not experienced in motor control theory. The number of required input parameters is reduced. The fields that require user input are displayed with a white background. The fields that are automatically preset by MCAT are displayed with a gray background and are read-only.
- **Expert**—all input parameters are accessible and editable by the user. However, their setting requires a certain level of expertise in motor control theory.

freescal[™] **Motor Control Application Tuning Tool**

Motor 1: PMSM Tuning Mode: Basic

Introduction | Motor Identif | **Parameters** | Current Loop | Speed Loop | Sensors | Sensorless | Control Struc | Output File

Parameters measurement

Application scales

HW board: TWR-MC-LV3PH

I max: 8 [A]

U DCB max: 36.3 [V]

Fast Loop Period: 0.0001 [sec]

N nom: 4000 [rpm]

pp: 2 [-]

Number of pp assistant

Start Stop

Rs and Ls measurement

Id meas: 1 [A]

Id ampli: 0.8 [A]

Freq meas start: 999 [Hz]

Freq meas min: 400 [Hz]

Ud inc: 0.5 [V]

Freq dec: 100 [Hz]

Measure

Measured Rs and Ls

Rs: 0.48 [Ω]

Ld: 0.00039 [H]

Lq: 0.000451 [H]

Ke: 0.0142 [V*s/rad]

Status

Ready for measurement ...

Reload Data Store Data

Freescal Semiconductor, Inc.
Designed by Motor Control Teams / Roznov CSC

Figure 1. Motor identification tab

Table 1 lists the input parameters including their physical units, description, and accessibility.

Table 1. Motor identification tab parameter descriptions

Parameter	Unit	Description	Write Enable?
HW board	N/A	Selects the power stage (PS). There are three possible options depicted in Figure 2. Freescale low voltage power stage (TWR-MC-LV3PH) and Freescale high voltage power stage (FSL-HV-PS) have predefined hardware scales (I max and U DCB max) and Fast Loop Period . The third option, User HW , enables users to specify hardware scales and Fast Loop Period according to their own power stage and application.	Always
I max	[A]	Hardware board current scale.	User hardware board selected
U DCB max	[V]	Hardware board DC bus voltage scale.	User hardware board selected

Table continues on the next page...

Table 1. Motor identification tab parameter descriptions (continued)

Parameter	Unit	Description	Write Enable?
Fast Loop Period	[s]	Control loop period. In most cases inverted value of PWM frequency.	User hardware board selected
N nom	[rpm]	Motor nominal speed in rpm. This value can be found in the motor control datasheet.	Always
pp	[-]	Motor number of pole-pairs. If the pp is unknown, it can be determined using the <i>Number of pp assistant</i>	Always
Calib Rs	[Ω]	Resistance of the connected motor for power stage characterization purposes. Must be measured manually prior to characterization process. Be aware, that the resistance of the calibration resistor must be low enough to reach measurement current 2A. See Power stage characterization for more information	If hardware board == User HW
Id meas	[A]	DC current for R_s measurement. Id meas may be set as half of the motor nominal current, however, the maximum Id meas is 2A because the characterization is done from -2A to 2A.	Always
Id ampl	[A]	Amplitude of AC sinusoidal current for L_s measurement. Id ampl may be set as half of the motor nominal current.	Always
F meas start	[Hz]	Starting frequency of sinusoidal signal for L_s measurement. See Measurement for more information.	Expert tuning mode selected
F meas min	[Hz]	Minimal (end) frequency of sinusoidal signal for L_s measurement. See Measurement for more information.	Expert tuning mode selected
Ud inc	[V]	Voltage increment when measuring L_s . See Measurement for more information.	Expert tuning mode selected
Freq dec	[Hz]	Frequency decrement when measuring L_s . See Measurement for more information.	Expert tuning mode selected
Rs	[Ω]	R_s result.	Never
Ld	[H]	L_d result.	Never
Lq	[H]	L_q result.	Never
Ke	[V.s/rad]	K_e result.	Never

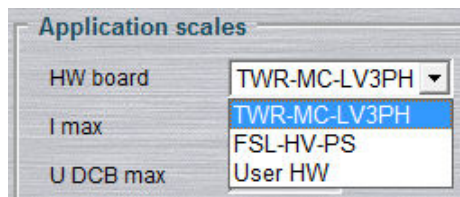


Figure 2. Hardware board selector

2.1 Power stage characterization

Each inverter introduces a total error count which includes dead-time, a current clamping effect, and transistor voltage drop. The total error count depends on the phase current and this dependency is measured during the power stage characterization process from -2A to +2A. An example of the inverter error characteristic is depicted in [Figure 3](#). The acquired characterization data is saved to a file and used later for phase voltage correction during the R_s measurement process. Before performing characterization, a motor with a known R_s must be connected to the inverter and the value of its R_s set as

Calib Rs. Afterward, characterization may begin by pressing the **Calibrate** button. Characterization performs 65 current steps gradually, from -2A to +2A, each for 300 ms, so be aware that the process takes about 20s and the motor must withstand this load. It is recommended to use a motor with a low R_s for characterization purposes.

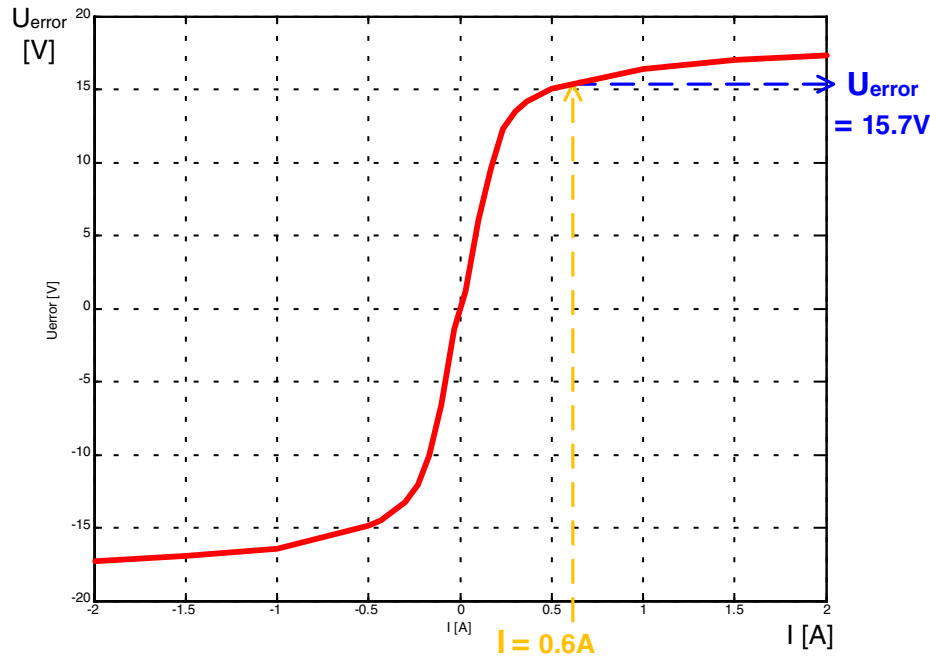


Figure 3. Transfer characteristic

Power stage characterization is necessary only for the user's hardware board. When Freescale power stages are used with the application, the characterization process can be omitted. The acquired characterization data is saved in a file, therefore, it is only necessary to do the characterization once, depending on the user's hardware.

2.2 Measurement

The motor parameter identification process measures R_s , L_d , L_q and K_e respectively.

Stator resistance (R_s) is measured with the DC current **Id meas** value, which is applied to the motor for 600 ms. Current control is enabled during R_s measurement and the current controllers' parameters are set to satisfy a slow response. R_s is calculated from Ohm's law when the actual phase voltage value is corrected using chracterization data.

For stator inductance (L_s) identification purposes, a sinusoidal measurement voltage is applied to the motor. During L_s measurement, the voltage control is enabled. The frequency and amplitude of the sinusoidal voltage are obtained before actual measurement, during the tuning process. The tuning process begins with a 0V amplitude and **F start** frequency, which are applied to the motor. The amplitude is gradually increased by **Ud inc** up to half of the DC bus voltage (DCbus/2) until **Id ampl** is reached. If **Id ampl** is not reached even with DCbus/2 and **F start**, the frequency of the measuring signal is gradually decreased by **F dec** down to **F min** again until **Id ampl** is reached. If **Id ampl** is still not reached, measurement will continue with DCbus/2 and **F min**. The tuning process is depicted in Figure 4. When the tuning process is complete, the sinusoidal measurement signal (with amplitude and frequency obtained during the tuning process) is applied to the motor. The total impedance of the RL circuit is then calculated from the voltage and current amplitudes and L_s is calculated from the total impedance of the RL circuit.

Direct inductance (L_d) and quadrature inductance (L_q) measurements are completed in the same way as L_s . Before the L_d and L_q measurement is taken, a DC current is applied to the D-axis, which aligns the rotor. For L_d measurement, the sinusoidal voltage is applied in the D-axis, and for L_q measurement, the sinusoidal voltage is applied in the Q-axis.

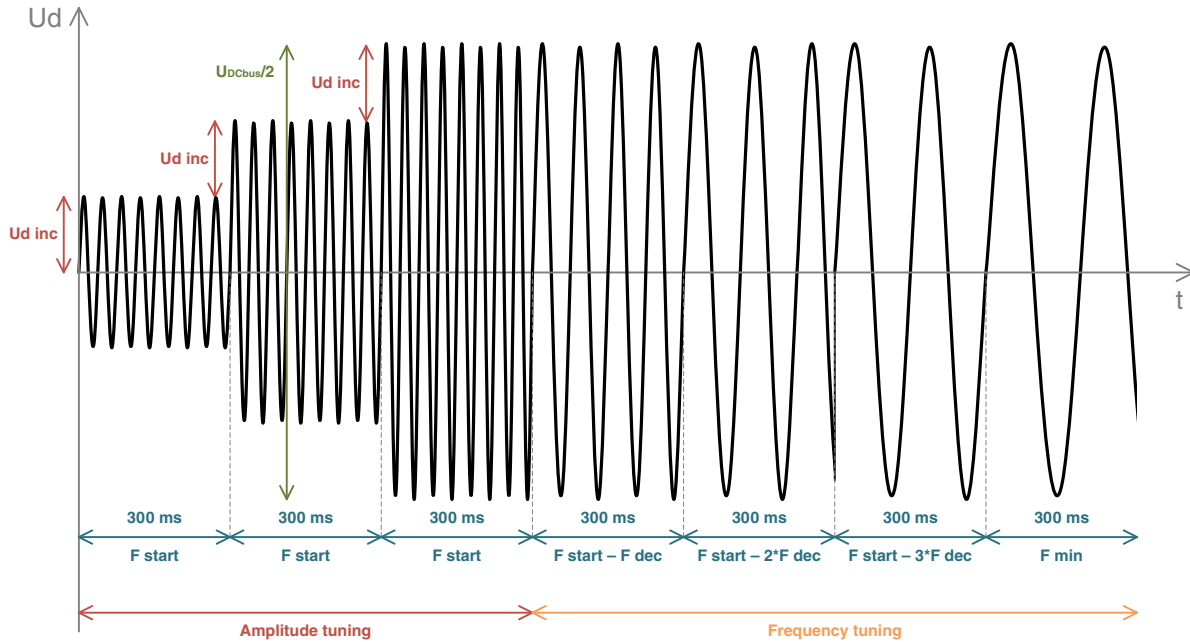


Figure 4. Sinusoidal signal tuning

Prior to the actual k_e measurement, the MCAT tool calculates the current controllers and BEMF observer constants from the previously measured R_s , L_d , and L_q . To be able to measure k_e , the motor must spin. I_d is controlled through **I_d meas** and the electrical open-loop position is generated by integrating the required speed, which is derived from **N nom**. When the motor reaches the required speed, BEMF voltages obtained by the BEMF observer are filtered and k_e is calculated:

$$k_e = \frac{U_{BEMF}}{\omega_{el}}$$

Equation 1

When k_e is being measured, the user must visually check to determine whether the motor is spinning properly. If the motor is not spinning properly use the following steps:

- Ensure that the number of **pp** is correct. The required speed for k_e measurement is also calculated from **pp**, therefore, an inaccuracy in **pp** causes inaccuracy in the resultant k_e .
- Increase **I_d meas** to produce higher torque when spinning during the open-loop.
- Decrease **N nom** to decrease the required speed for the k_e measurement.

As soon as identification is complete, the motor parameters are passed to the *Parameters* tab in MCAT automatically.

2.3 Number of pole-pair assistant

The number of pole-pairs cannot be measured without a position sensor, however, there is a simple assist to determine the number of pole-pairs (**pp**). The *Number of pp assistant* performs one electrical revolution and stops for 2.4s, and then repeats. Because the **pp** value is a ratio between electrical and mechanical speeds, it can be determined as the number of stops per one mechanical revolution. It is recommended not to count the stops during the first mechanical revolution because an alignment occurs during the first revolution which affects the number of stops. During the **pp** measurement, the current loop is enabled and current I_d is controlled by **I_d meas**. The electrical position is generated by integrating the open-loop speed. If the rotor does not move after the start of the *Number of pp assistant*, stop the assistant, increase **I_d meas**, and start the assistant again.

3 Using the motor identification tab

1. Select your hardware board.
 - When using the TWR-LV-3PH power stage with DC bus voltage of 24 V, PWM frequency of 10 kHz, and dead-time of 0.5 μ s, select TWR-LV-3PH.
 - When using the Freescale high-voltage power stage with DC bus voltage of 325 V, PWM frequency of 10 kHz, and dead-time of 0.5 μ s, select FSL-HV-PS.
 - When using a different configuration than mentioned above, select User HW.
2. Enter **I max**, **U DCB max**, **Fast Loop Period** and **N nom** if accessible. For more information, see [Table 1](#).
3. Enter **Id meas** and **Id ampl**. For more information, see [Table 1](#).
4. Enter **F start**, **F min**, **Ud inc**, **F dec** if you are in Expert mode. For more information, see [Measurement](#).
5. Enter **pp** if you already know it, or use the *Number of pp assistant*. For more information, see [Number of pole-pair assistant](#).
6. Perform characterization when not using a Freescale power stage. For more information, see [Power stage characterization](#).
7. Start the identification by pressing the **Measure** button.
8. If a fault or warning occurs, check [Fault handling](#) to troubleshoot.
9. If measurement is successful, read the motor control parameters and remember that these parameters are fed to the *Parameters* tab automatically.
10. Continue with the controllers' parameters tuning according to [Reference \[2\]](#).

This entire step-by-step process is depicted in [Figure 5](#).

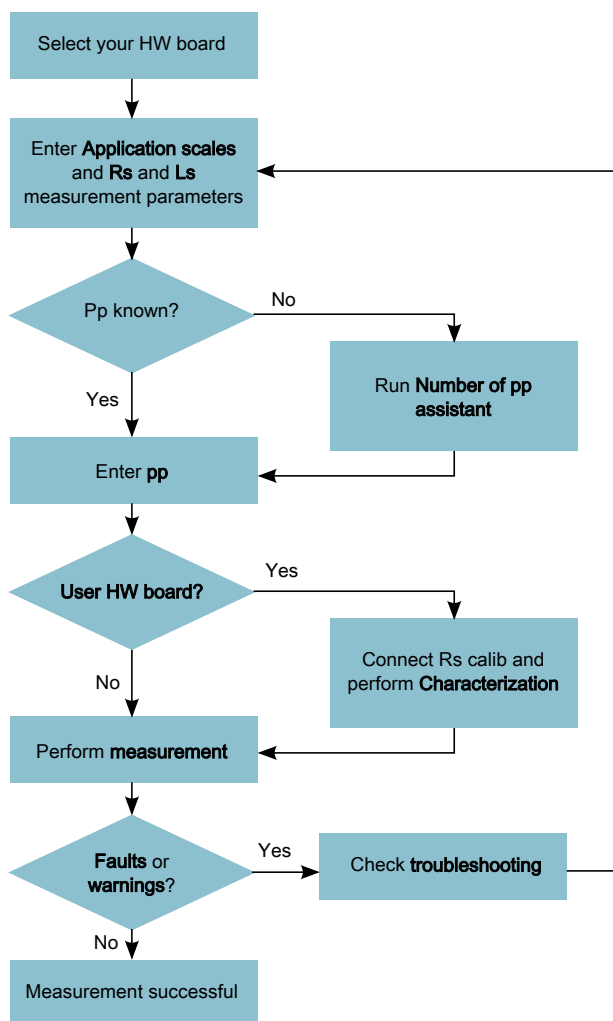


Figure 5. Step-by-step flow chart

4 Fault handling

There are several faults and warnings which can occur during the measurement or calibration processes. These measurement faults are not be confused with application faults, such as DC bus undervoltage or overspeed. The measurement faults and warnings serve to inform the user that something went wrong during the measurement process. There are 3 measurement faults described in [Table 2](#), together with their reason and possible troubleshooting. If one of these faults occurs, the identification process ends immediately and informs the user by a message depicted in [Figure 6](#).

Table 2. Faults description

Fault No.	Fault description	Fault reason	Troubleshooting
01	Motor not connected	Id > 50mA cannot be reached with the available DC bus voltage.	Confirm that a motor is connected.

Table continues on the next page...

Table 2. Faults description (continued)

Fault No.	Fault description	Fault reason	Troubleshooting
02	Rs too high for calibration	Id = 2A cannot be reached with the available DC bus voltage.	Use a motor with a lower Rs for power stage characterization.
03	Wrong characteristic data	Characteristic data, which is used for voltage correction, does not correspond to the actual power stage.	Select User HW and perform the calibration.

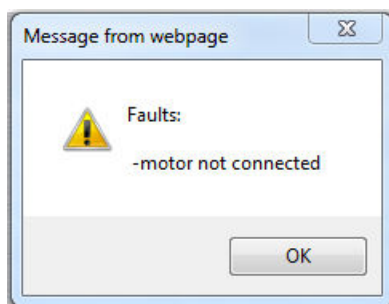


Figure 6. Fault example

Unlike faults, warnings do not stop the identification process immediately, but instead inform the user that something nonessential failed. There are two warnings that can occur during the measurement process, described in Table 3.

Table 3. Warnings description

Warning No.	Warning description	Warning reason	Troubleshooting
01	Current measurement Id_meas not reached	User defined Id meas was not reached, so the measurement was taken with a lower Id meas .	Raise the DC bus voltage to reach the Id meas or lower the Id meas to avoid this warning.
02	Current amplitude measurement Id_ampl not reached	User defined Id_ampl was not reached, so the measurement was taken with a lower Id_ampl .	Raise the DC bus voltage or lower the F min to reach the Id_ampl or lower the Id_ampl to avoid this warning.

5 References

The following references are available on <http://www.freescale.com> :

1. *PMSM Electrical Parameters Measurement* (Document AN4680).
2. *Tuning 3-Phase PMSM Sensorless Control Application Using MCAT Tool* (Document AN4912).

How to Reach Us:

Home Page:

freescale.com

Web Support:

freescale.com/support

Information in this document is provided solely to enable system and software implementers to use Freescale products. There are no express or implied copyright licenses granted hereunder to design or fabricate any integrated circuits based on the information in this document. Freescale reserves the right to make changes without further notice to any products herein.

Freescale makes no warranty, representation, or guarantee regarding the suitability of its products for any particular purpose, nor does Freescale assume any liability arising out of the application or use of any product or circuit, and specifically disclaims any and all liability, including without limitation consequential or incidental damages.

“Typical” parameters that may be provided in Freescale data sheets and/or specifications can and do vary in different applications, and actual performance may vary over time. All operating parameters, including “typicals,” must be validated for each customer application by customer's technical experts. Freescale does not convey any license under its patent rights nor the rights of others. Freescale sells products pursuant to standard terms and conditions of sale, which can be found at the following address: freescale.com/SalesTermsandConditions.

Freescale and the Freescale logo, are trademarks of Freescale Semiconductor, Inc., Reg. U.S. Pat. & Tm. Off. All other product or service names are the property of their respective owners.

© 2014 Freescale Semiconductor, Inc.