


# cronologic

Ndigo6G-PCIe  
USER GUIDE

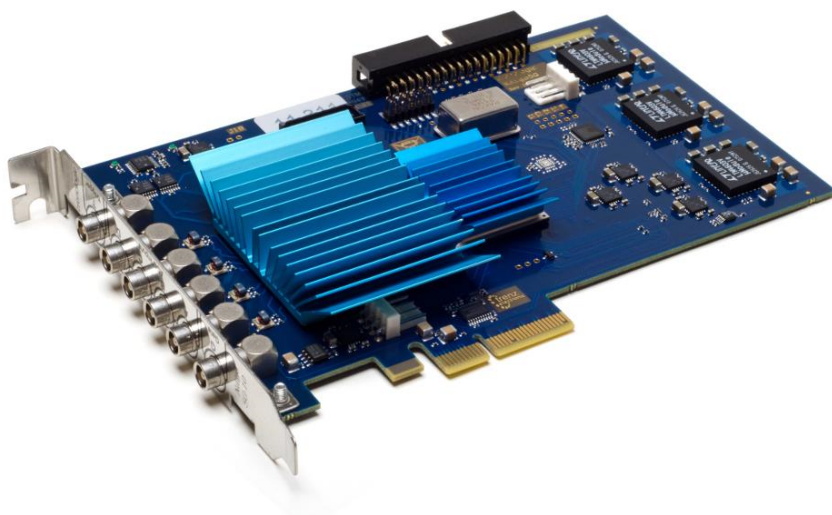

[www.cronologic.de](http://www.cronologic.de)

**Ndigo6G-PCIe**

# Contents

<b>1</b>	<b>Introduction</b>	<b>4</b>
1.1	Features	4
<b>2</b>	<b>Hardware</b>	<b>5</b>
2.1	Installing the Board	5
2.2	Ndigo6G External Inputs and Connectors	5
2.2.1	Connectors	5
2.2.2	Analog Inputs	7
2.2.3	Digital Inputs	8
2.3	Extension Card	8
2.4	Ndigo5G Functionality	9
2.4.1	ADC Modes	9
2.4.2	Zero Suppression	11
2.4.3	Trigger Blocks	12
2.4.4	Gating Blocks	18
2.4.5	Auto Triggering Function Generator	21
2.4.6	Timestamp Channel	21
2.4.7	Data Lookup Table	21
2.5	Multiple Ndigo boards synchronization	22
2.5.1	Calibration Procedure	23
2.5.2	Synchronizing a Ndigo5G and an HPTDC8-PCI	26
2.6	Performing a firmware update	26
2.7	Calibrating the TDC	27
<b>3</b>	<b>Driver Programming API</b>	<b>29</b>
3.1	Constants	29
3.2	Initialization	29
3.2.1	Structure <code>ndigo6g12_init_parameters</code>	29
3.3	Status Information	31
3.3.1	Functions for Information Retrieval	31
3.3.2	Structure <code>ndigo6g12_static_info</code>	31
3.3.3	Structure <code>ndigo6g12_param_info</code>	32
3.3.4	Structure <code>ndigo6g12_fast_info</code>	33
3.3.5	Structure <code>ndigo_slow_info</code>	35
3.4	Configuration	36
3.4.1	Structure <code>ndigo_configuration</code>	36
3.4.2	Structure <code>ndigo_trigger</code>	38
3.4.3	Structure <code>ndigo_trigger_block</code>	38
3.4.4	Structure <code>ndigo_extension_block</code>	40
3.4.5	Run Time Control	40
3.5	Readout	40
3.5.1	Input Structure <code>ndigo_read_in</code>	40
3.5.2	Output Structure <code>ndigo_read_out</code>	41
3.6	Other Functions	41
3.6.1	LED control	41
<b>4</b>	<b>Packet Format</b>	<b>42</b>
4.1	Output Structure <code>ndigo_packet</code>	42
<b>5</b>	<b>C-Example</b>	<b>44</b>
<b>6</b>	<b>Technical Data</b>	<b>46</b>
6.1	Digitizer Characteristics	46
6.1.1	1-Channel-Mode (5 Gsps)	46
6.1.2	2-Channel-Mode (2.5 Gsps)	46

6.1.3	4-Channel-Mode (1.25 Gbps)	46
6.2	Electrical Characteristics	47
6.2.1	Oscillator	47
6.2.2	Environmental Conditions for Operation	47
6.2.3	Environmental Conditions for Storage	47
6.2.4	Power Supply	47
6.2.5	Analog Input	47
6.2.6	Analog inputs	48
6.3	Information Required by DIN EN 61010-1	48
6.3.1	Manufacturer	48
6.3.2	Intended Use and System Integration	48
6.3.3	Cooling	49
6.3.4	Environmental Conditions	49
6.3.5	Inputs	49
6.3.6	Known Bugs	49
6.3.7	Workarounds	49
6.3.8	Recycling	49
6.3.9	Export Control	49
<b>7</b>	<b>Revision History</b>	<b>50</b>
7.1	Firmware	50
7.2	Driver & Applications	50
7.3	User Guide	50

**Caution:** This User Guide is under active development and therefore, not accurate.

# 1 Introduction

The Ndigo6G-12 offers up to 6.4 Gsps sample rate, 12 bits resolution and a greatly improved readout rate of 6000 MB/s.

The unit is a combined ADC/TDC board for the acquisition of pulses in time-of-flight applications. It builds on the established platform of the Ndigo5G-10, but takes it to the next level both in performance and flexibility.

The Ndigo6g-12 was specifically designed for time-of-flight applications like LIDAR or TOF mass spectrometry. Pulse arrival times can be measured with an accuracy down to 5 ps together with information on the pulse shape, such as area or amplitude.

Four channels with 1.6 Gsps at 12 bit resolution can be acquired independently. Alternatively, the four channels can be combined to two or to one channel, increasing either the dynamic range or the sample rate.

## 1.1 Features

- **12 bit** dynamic range
- Up to **6.4 Gsps** sample rate (in 1 channel mode) for increased resolution in time domain.
- Up to **four ADC channels** for your individual measurement setups.
- **Four TDC channels** with a resolution of **12 ns**.
- Digital input with TDC that can also be used for gating and triggering.
- 2<sup>nd</sup> digital input for gating or triggering.
- PCIe3 x8 1.1 with **XYZ MB/s throughput** for simple and fast data transfer to most PCs.
- **Synchronization of up to eight boards** via reference clock if more channels are required.
- **Unlimited multihit** capabilities.
- Continuous ADC readout rate of approx. **6000 MB/s**.
- **Zero suppression** reducing PCIe load.

## 2 Hardware

### 2.1 Installing the Board


The **Ndigo6G** board can be installed in any  $\times 8$  (or higher amount of lanes) PCIe slot. **If the slot electrically supports less than eight lanes, the board will operate at lower data throughput rates.**

Please ensure proper cooling of the device. The **Ndigo6G** has an onboard temperature detection. If the ADC chip temperature exceeds  $90^{\circ}\text{C}$  a warning is issued to the device driver. In case the temperature is higher than  $95^{\circ}\text{C}$  the ADC is disabled to avoid damage. Using a PCI-slot cooler is in many cases an appropriate solution to circumvent problems caused by overheating if the board is used inside a PC. The Ndigo-Crate will provide sufficient cooling under normal operating conditions. Using a single **Ndigo6G**, no further connections need to be made.

For applications that require more than four ADC channels, several Ndigo boards can be operated in sync. Any board of the **Ndigo product line** can be synced to other Ndigo boards, allowing, for instance, for a combination of high speed ADCs (e.g., **Ndigo5G**) and slower high resolution ADCs (**Ndigo250M-14**).

The signals used for board synchronization and inter-board triggering are transferred on a bus between the boards. Join all C2 connectors (see [Figure 2.3](#)) on the boards using a ribbon cable. Both ends of the bus need to be terminated properly. In case a **Ndigo-Crate** is used, connectors providing proper termination are located on the crate mainboard next to the PCIe slots to the extreme left and right (for more details, please refer to the *Ndigo-Crate User Guide* <[https://download.cronologic.de/PCIe-Crates/Ndigo\\_Crate\\_User\\_Guide.pdf](https://download.cronologic.de/PCIe-Crates/Ndigo_Crate_User_Guide.pdf)>\_) In applications that use only a few Ndigo boards directly inside a PC, termination PCBs available from cronologic can be used.

The standard device driver of the **Ndigo6G** can be used to read out all boards and acquire data. For more complex scenarios, using the *cronoSync-library*, which is part of *cronoTools*, is recommended. The *cronoSync-library* is provided with the Ndigo device driver. Please refer to the **cronoTools User Guide** for more information.

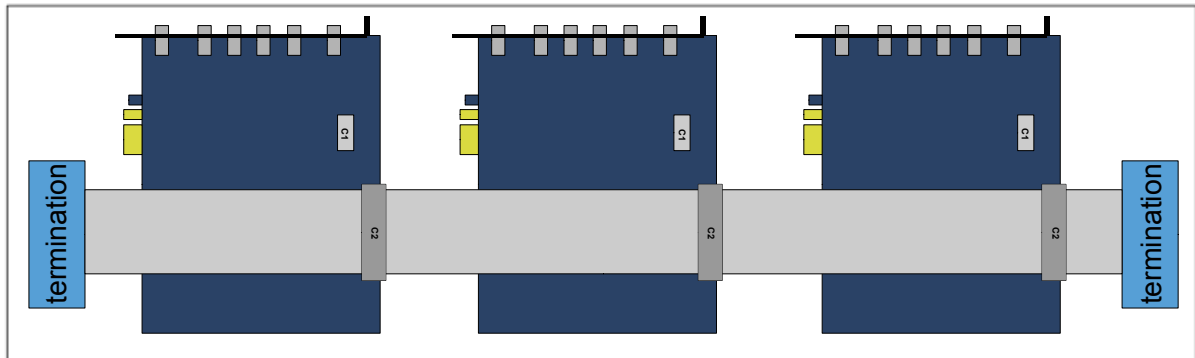

**Figure 2.1:** If several Ndigo boards are connected to work in sync, the boards must be connected using a ribbon cable as a bus for synchronization and trigger signals. Proper termination is required at both ends of the cable.

### 2.2 Ndigo6G External Inputs and Connectors

#### 2.2.1 Connectors

The inputs of the **Ndigo6G** are located on the PCI bracket. [Figure 2.3](#) shows the location of the four analog inputs A to D, the four digital TDC inputs E to H, and the two digital FPGA inputs 0 and 1. Furthermore, two board inter-connection connectors can be found at the top edge of the **Ndigo6G** board, as displayed in [Figure 2.3](#). Connector C1 is used for a board-to-board connection (e.g., to link a **HPTDC8-PCI** and an **Ndigo6G** via an **Ndigo Extension Board**, see [Chapter 2.3](#)). Connector C2 is used as a bus interface between multiple Ndigo boards distributing clock, trigger and sync signals. Proper termination must be placed at both ends of the bus interconnection ribbon cable.

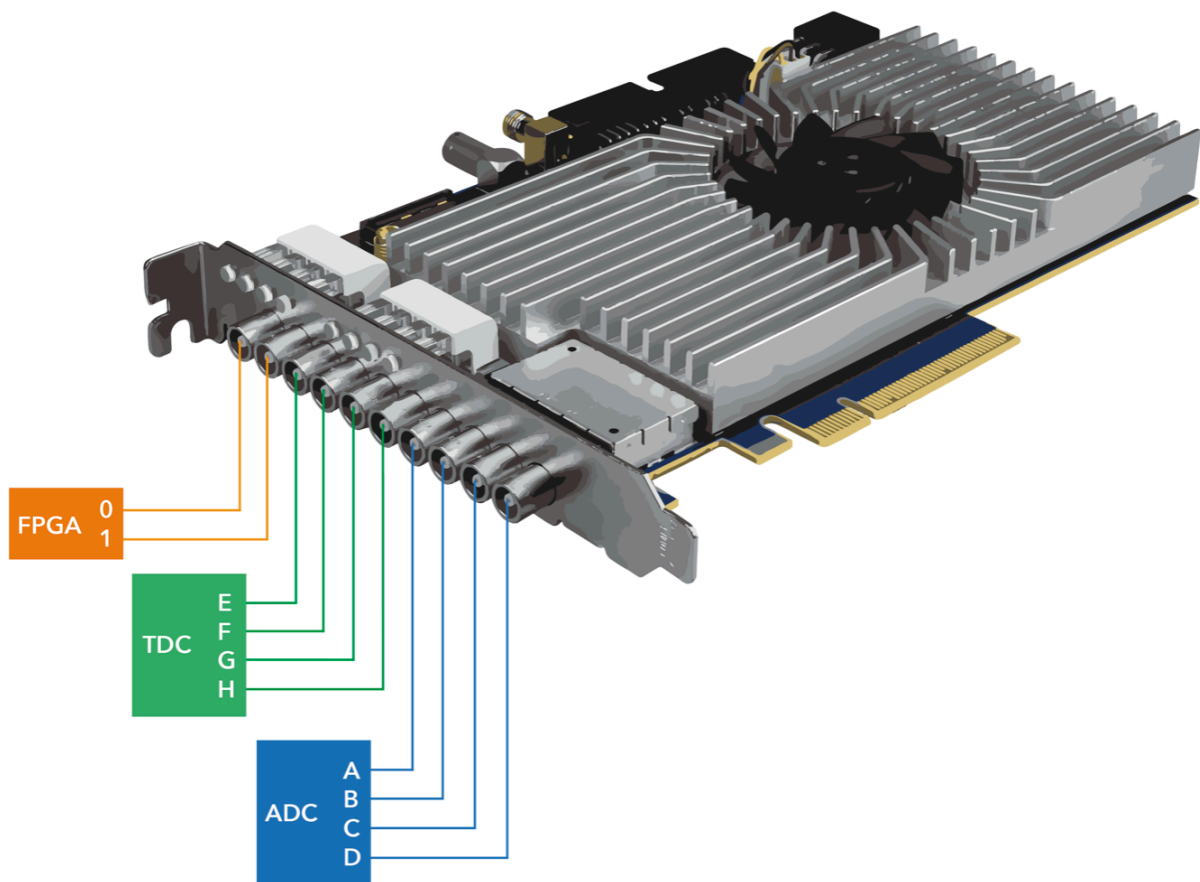


Figure 2.2: Input connectors of an **Ndigo6G** board located on the PCI bracket.


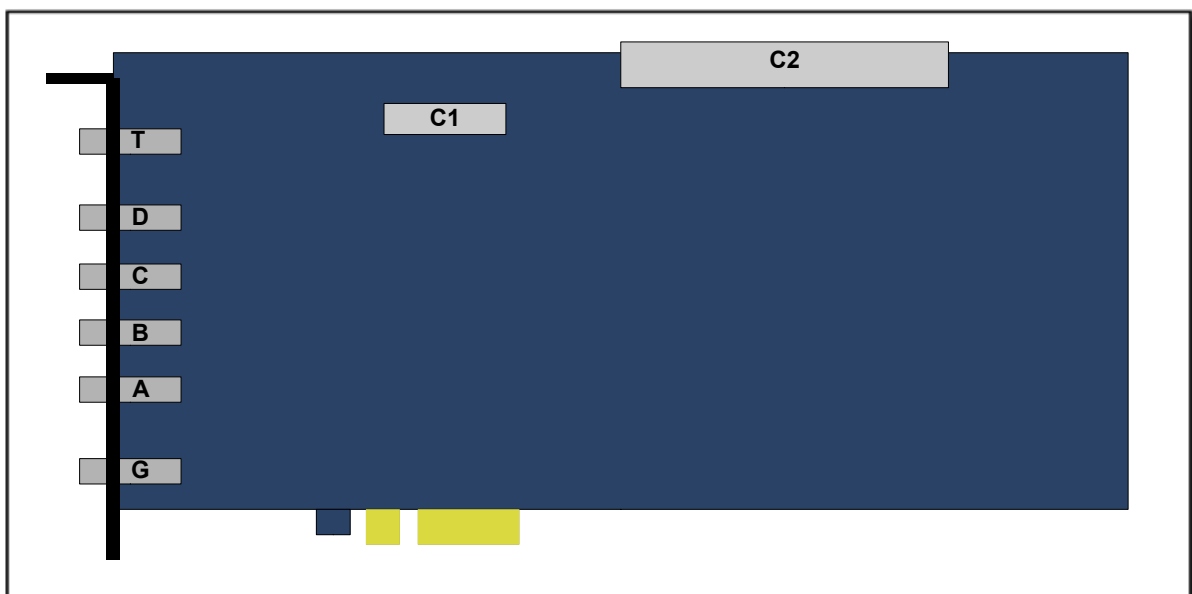


Figure 2.3: Schematic of an **Ndigo6G** board showing inter-board connectors C1 and C2. TODO update schematic

## 2.2.2 Analog Inputs

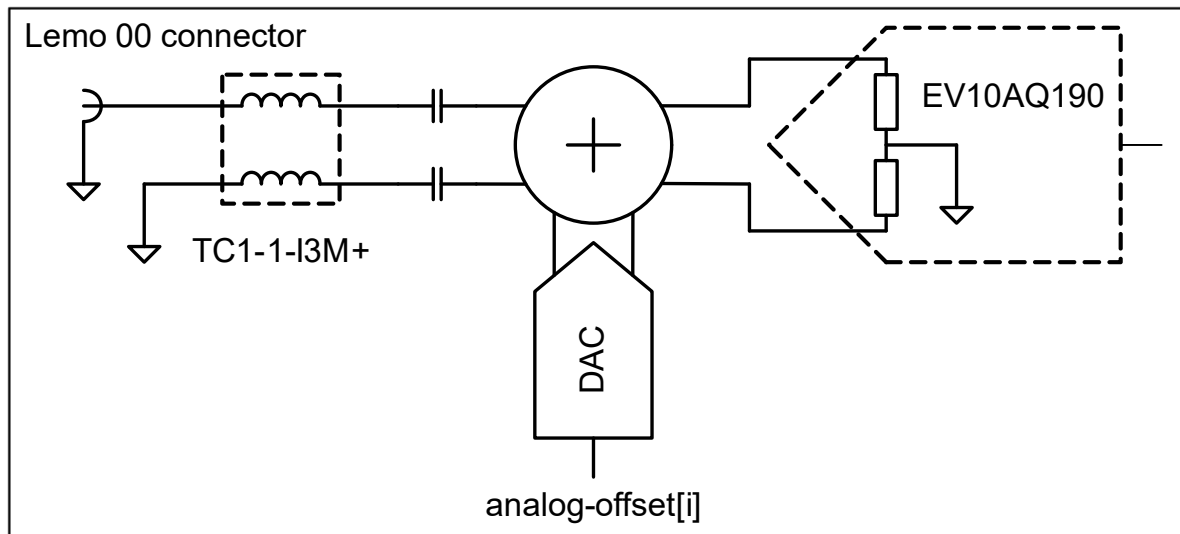


**Figure 2.4:** Input circuit for each of the four analog channels.

The analog inputs of the ADC are single ended LEMO00 coax connectors. The inputs have a  $50\ \Omega$  impedance and are AC coupled. The inputs are converted to a differential signal using a balun.

### Analog Offsets

AC coupling removes the common mode voltage from the input signal. Users can move the common mode voltage to a value of their choice using the `analogoffset` parameter of each channel before sampling.

This feature is useful for highly asymmetric signals, such as pulses from TOF spectrometers or LIDAR systems. Without analog offset compensation, the pulses would begin in the middle of the ADC range, effectively cutting the dynamic range in half (see Figure 2.6). By shifting the DC baseline to one end of the ADC range, the input range can be used fully, providing the maximum dynamic range. The analog offset can be set between  $\pm 0.25\text{ V}$ .

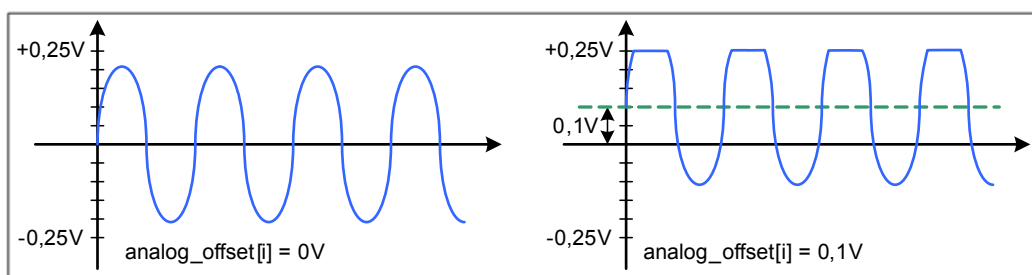

**Figure 2.5:** Users can add analog offset to the input before sampling

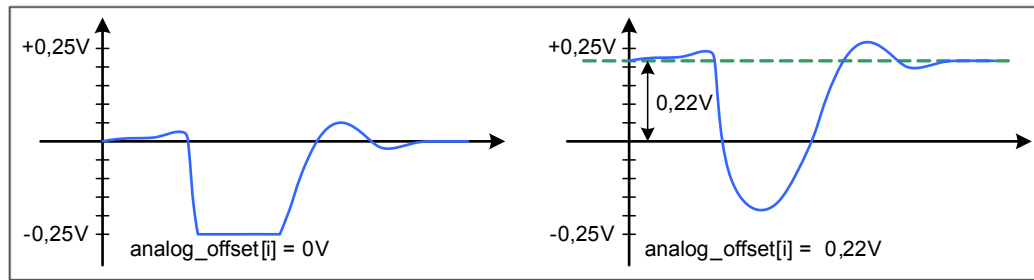


Figure 2.6: Asymmetric signal shifted to increase dynamic range

### 2.2.3 Digital Inputs

There are two digital inputs on the front slot cover called *Trigger* (T) and *Gate* (G).

Both inputs provide a digital input signal routed to the trigger matrix. These signals can be used to trigger any of the trigger state machines and gating blocks. The inputs are AC coupled. A DC offset is configurable via `dc_offset_parameter` in the *configurations structure* to support positive and negative input pulses.

The configuration is set via the structure's `trigger [8]` and `trigger [9]` in the *configuration structure*. The input circuit is shown in Figure 2.17.

#### TDC on Trigger Input

A time-to-digital (TDC) connected to the Trigger input. The TDC creates packets of **type 8**. These packets first contain a coarse timestamp and a payload that can be used to calculate the trigger position with higher precision. The function `ndigo_process_tdc_packet` can be used to replace the coarse timestamp with the precise timestamp. This function is described in Chapter 3.5. TDC pulses must have a minimum duration of 3.3 ns. The dead-time of the TDC is 32 ns.

---

**Note:** When used with the TDC, the Trigger input supports negative pulses only.

---

## 2.3 Extension Card

The **Ndigo Extension Card** provides additional inputs or outputs to the FPGA. It is connected to the C1 (Samtec QSS-025) connector on an **Ndigo5G** by an Samtec SQCD cable assembly.

The **Ndigo Extension Card** provides up to ten single ended LEMO00 connectors. The circuit connecting to each of these circuits can be chosen to provide inputs or outputs. These can be AC or DC coupled. AC coupled inputs support NIM signaling.

The signals connect to 2.5 V IO Pins of the Xilinx Virtex-5 FPGA. The current firmware revision provides the following signal connections.



Connector	QSS Pin	FPGA Pin	Direction	Signal
LEMO00: CH0	22	AD9	Input	Ndigo Extension digital channel 0
LEMO00: CH1	18	AE10	Input	Ndigo Extension digital channel 1
LEMO00: CH2	14	D10		not connected
LEMO00: CH3	10	AF9	Output	39.0625 MHz clock for HPTDC
LEMO00: CH4	6	AD11	Output	39.0625 MHz clock for HPTDC
LEMO00: CH5	5	AE7	Output	39.0625 MHz clock for HPTDC
LEMO00: CH6	9	AF7	Output	39.0625 MHz clock for HPTDC
LEMO00: CH7	13	D9		not connected
LEMO00: CH8	17	V9	Input	Ndigo Extension digital channel 2
LEMO00: CH9	21	W9	Input	Ndigo Extension digital channel 3
SYNC1: Sync-TDC8	26	F9		not connected
SYNC1: Sync-HPTDC	44	AA7	Output	Sync for HPTDC

The four digital inputs are routed to the bus inputs of the trigger matrix to be used for triggering. The routing can be configured to either *OR*ing the sync bus and extension channels or use the extension channels exclusively.

Connector	Extension Card	Trigger matrix input	Trigger matrix input
	Digital Channel	ignorecable = 0	ignorecable = 1
LEMO00: CH0	0	BUS0 = EXT0 Sync Cable 0	BUS0 = EXT0
LEMO00: CH1	1	BUS1 = EXT1 Sync Cable 1	BUS1 = EXT1
LEMO00: CH8	2	BUS2 = EXT2 Sync Cable 2	BUS2 = EXT2
LEMO00: CH9	3	BUS3 = EXT3 Sync Cable 3	BUS3 = EXT3

## 2.4 Ndigo5G Functionality

### 2.4.1 ADC Modes

Depending on board configuration, the analog input signal is quantized to 8 or 10 bits. However, the board always scales and offsets the data to 16 bit signed data centered around 0.

Data processing such as trigger detection or packet building are always performed on 3.2 ns intervals. Depending on the ADC mode, this interval may contain 4, 8 or 16 samples.

The board supports using one, two or four channels:

#### 1 Channel Modes A, B, C and D

In these modes, only a single channel is used. The analog signal on that channel is digitized at 5Gsps. Packet size is always a multiple of 16 samples per 3.2 ns (See [Figures 2.9](#) and [2.15](#)).

#### 2 Channel Modes AC, BC, AD and BD

In these modes, two channels are used simultaneously. The analog signals on these channels are digitized at **2.5 Gsps** each. Packet size is always a multiple of 8 samples per 3.2 ns (See [Figures 2.8](#) and [2.14](#)).

#### 4 Channel Mode ABCD

In this mode, all four channels are digitized independently at 1.25 Gsps each. The packet size is always a multiple of 4 samples per 3.2 ns. (See Figures 2.7 and 2.13).

#### Multiple Sampling Modes AAAA, BBBB, CCCC and DDDD

In these modes, only one analog input channel is used, but the channel is sampled independently and simultaneously by four ADCs at **1.25 Gsps**. The board creates four independent streams with 4 samples each per **3.2 ns**.

Using the same trigger setting on all ADCs, can be used to reduce noise by averaging the four channels. To deal with complex triggering conditions, different trigger settings on each of the ADCs can be used.

The **Ndigo5G** provides four ADCs sampling at **1.25 Gsps** each. Higher speed modes are implemented by interleaving two or four of these ADCs.

During interleaving, the **Ndigo5G** firmware reorders and groups the data into a linear sample stream. The process is fully transparent. For users, the only difference is that a **3.2 ns** cycle can contain 4, 8 or 16 samples, depending on mode.

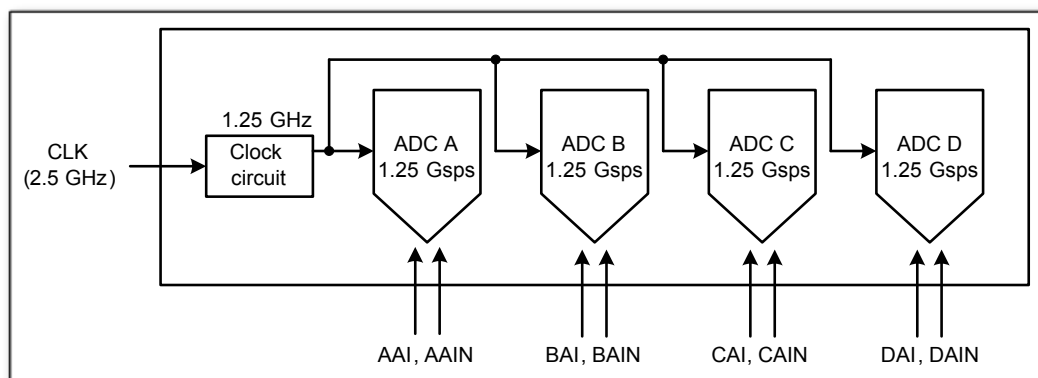


Figure 2.7: ADCs in 4 channel mode ABCD at 1.25 Gsps.

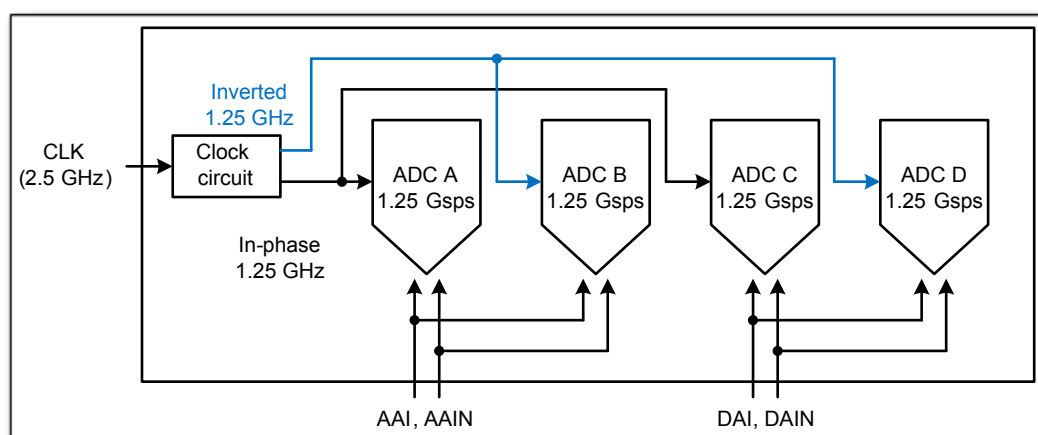


Figure 2.8: ADCs in 2 channel mode AD, interleaved for 2.5 Gsps.


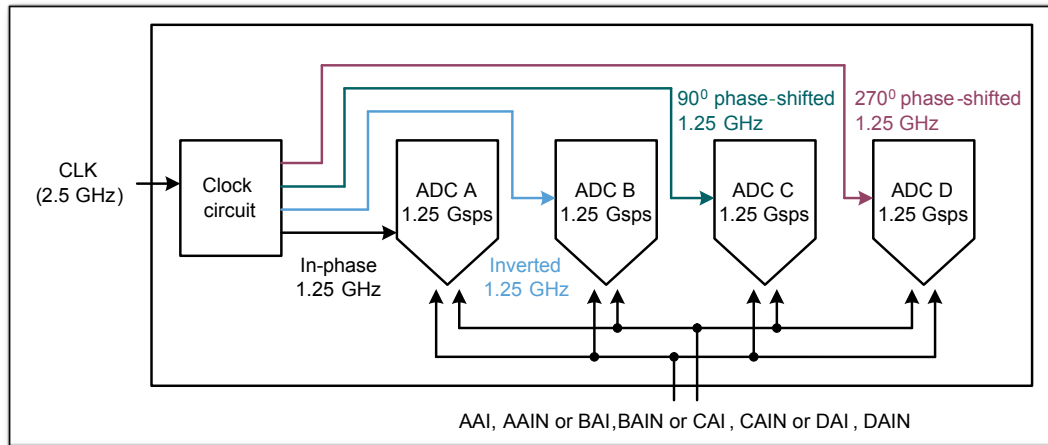


Figure 2.9: ADCs in 1 channel mode A, B, C or D interleaved for 5 Gsps.

### 2.4.2 Zero Suppression

One key features of the **Ndigo6g** is on-board zero suppression to reduce PCIe bus load. Only data that passes specifications predefined by the user is transmitted. This guide refers to transmitted waveform data as “packets”. A packet contains the waveform data and a timestamp giving the absolute time (i.e. the time since start of data acquisition) of the packet's last sample.

Figure 2.14 shows a simple example: Data is written to the PC only if values exceed a specified threshold. Expanding on that, **Ndigo5G**'s zero suppression can be used to realize much more complex scenarios.

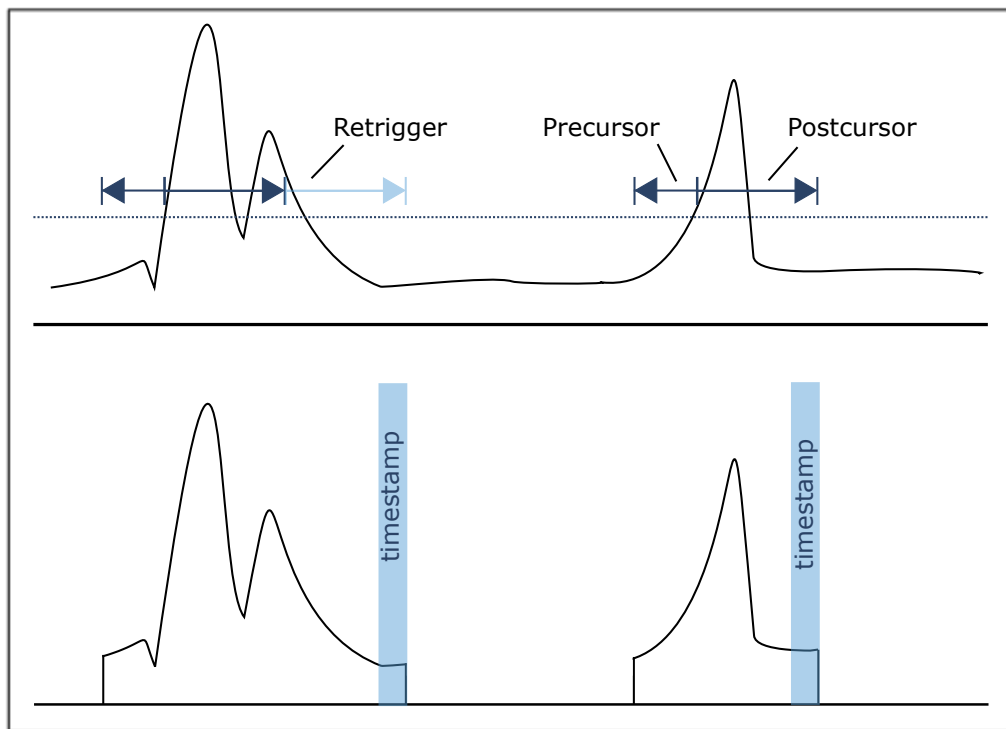

**Figure 2.10:** Simple zero suppression: Only data with values above a threshold are written to the PC.

### 2.4.3 Trigger Blocks

**Ndigo5G-10** and **Ndigo5G-8** record analog waveforms using zero suppression. Whenever a relevant waveform is detected, data is written to an internal FIFO memory. Each ADC channel has one trigger block determining whether data is written to the FIFO. The parameters are set in Structure **ndigo\_trigger\_block** (See [Chapter 3.3.5](#)).

Each trigger block consists of two independent units that check the incoming raw data stream for trigger conditions ([Figure 2.10](#)). Users can specify a threshold and can choose whether triggering is used whenever incoming data is below or above the threshold (level triggering) or only if data exceeds the threshold (edge triggering).

A gate length can be set to extend the trigger window by multiples of **3.2 ns**. Furthermore, if users choose precursor values  $> 0$ , the trigger unit will start writing data to the FIFO precursor 3.2 ns before the trigger event.

When using edge triggering, all packets have the same length ([Figure 2.11](#)): precursor + length + 1 cycles of **3.2 ns**. For level triggering, packet length is data dependent ([Figure 2.12](#)).

Please note that triggering is not accurate to sample. For each **3.2 ns** clock cycle, it is determined whether on any sample during that clock cycle a trigger condition is met. The clock cycle is then selected as the trigger point. As a result, the trigger sample can be anywhere within a range of up to 16 samples in single channel mode ([Figure 2.15](#)) at 16 samples per 3.2 ns.

If retriggering is active, the current trigger window is extended if a trigger event is detected inside the window.

A trigger block can use several input sources:

- The 8 trigger decision units of all four ADC channels ([Figure 2.16](#))
- The GATE input ([Figure 2.17](#))
- The Trigger or TDC input ([Figure 2.17](#))
- A function trigger providing random or periodic triggering.

- Triggers originating from other cards connected with the sync cable or from the Ndigo Extension card (BUS0, BUS1, BUS2, BUS3)
- A second set of trigger units with names ending in pe for the digital inputs Trigger, GATE, BUS0, BUS1, BUS2, and BUS3 configured for positive edge triggering. Together with the regular trigger units on this inputs, both edges of a pulse can be used in the trigger logic. This set of triggers is not available as inputs for the gate blocks.

Trigger inputs from the above sources can be concatenated using logical OR (Figure 2.19) by setting the appropriate bits in the trigger blocks source mask.

Triggers can be fed into the gate blocks as described in Chapter 2.4.4 (Figure 2.20). Gate blocks can be used to block writing data to the FIFO. That way, only zero suppressed data occurring when the selected gate is active is transmitted. This procedure reduces PCIe bus load even further (Figure 2.20).

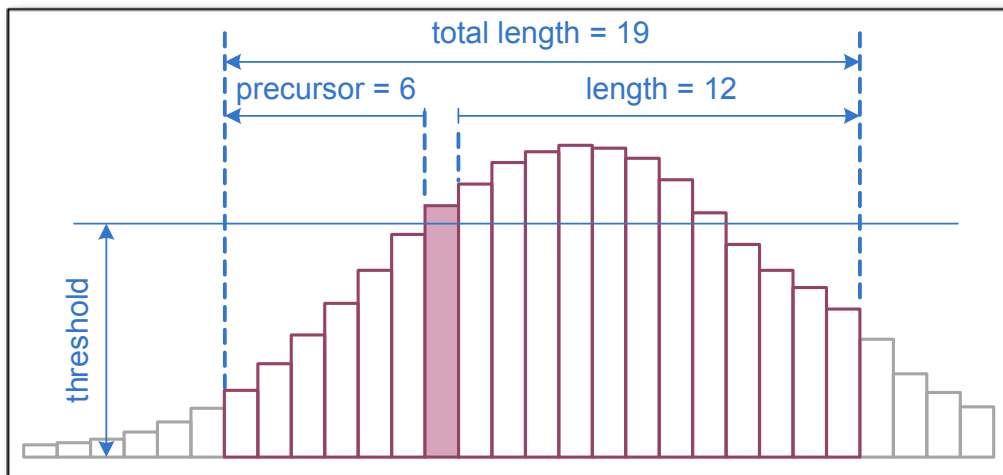


Figure 2.11: Parameters for edge triggering.



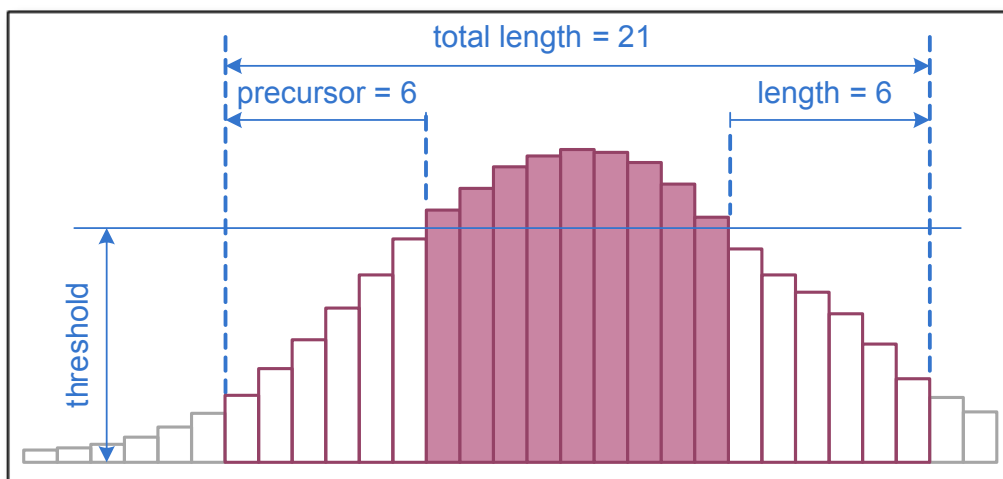



Figure 2.12: Parameters for level triggering.

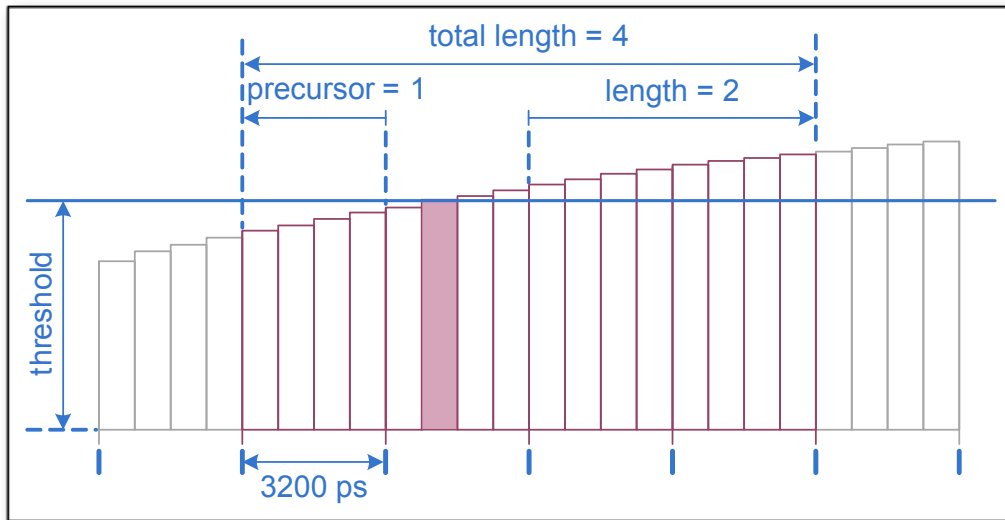


**Figure 2.13:** Triggering in 4 channel mode at 4 samples per clock cycle.

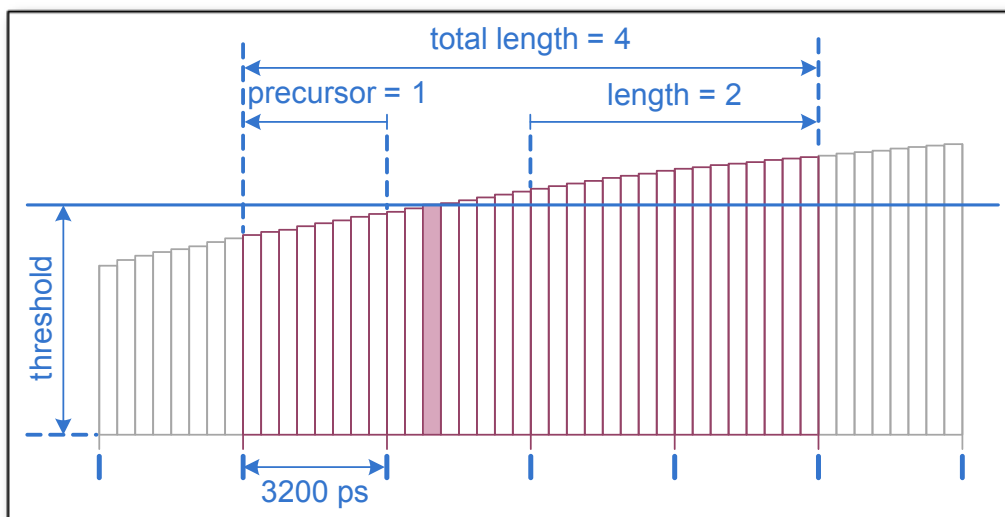


**Figure 2.14:** Triggering in 2 channel mode at 8 samples per clock cycle.

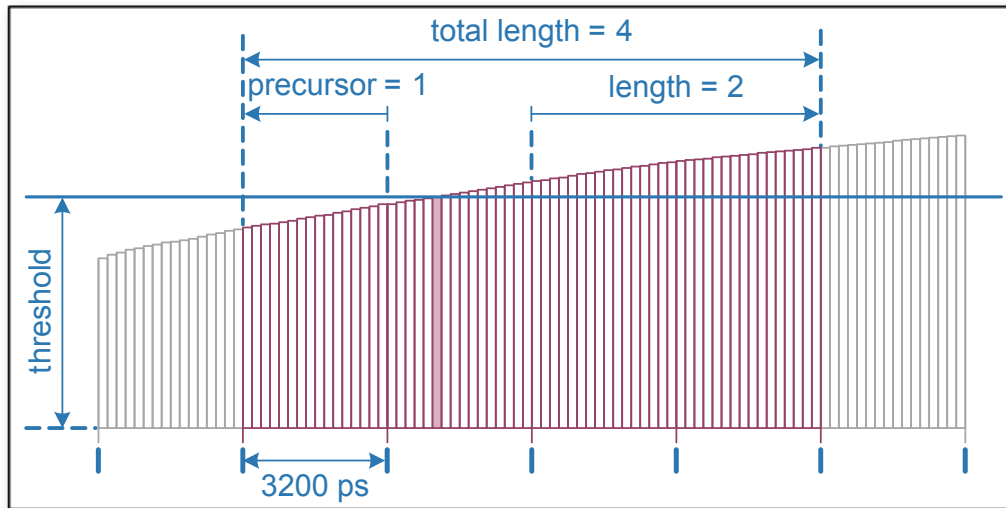


**Figure 2.15:** Triggering in 1 channel mode at 16 samples per clock cycle.

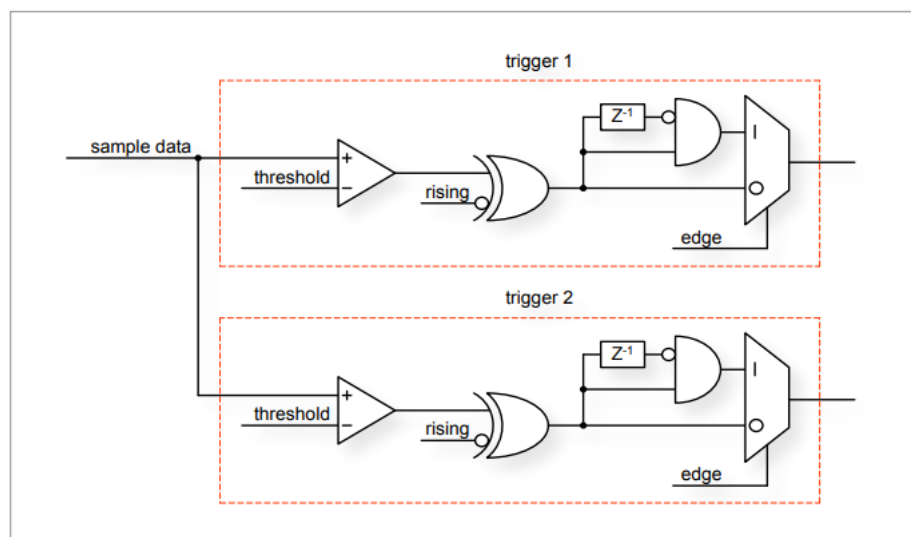

**Figure 2.16:** From the ADC inputs, a trigger unit creates an input flag for the trigger matrix. Each digitizer channel (A, B, C, D) has two trigger units.

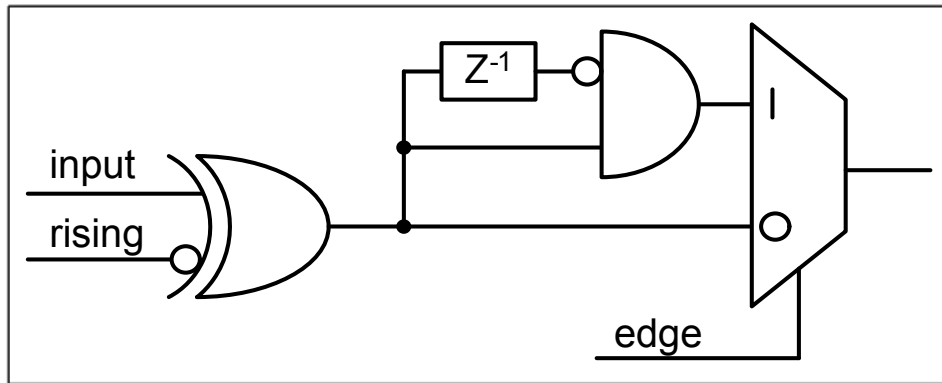


**Figure 2.17:** The digital inputs Trigger, GATE, BUS0, BUS1, BUS2 and BUS3 have simpler trigger units.

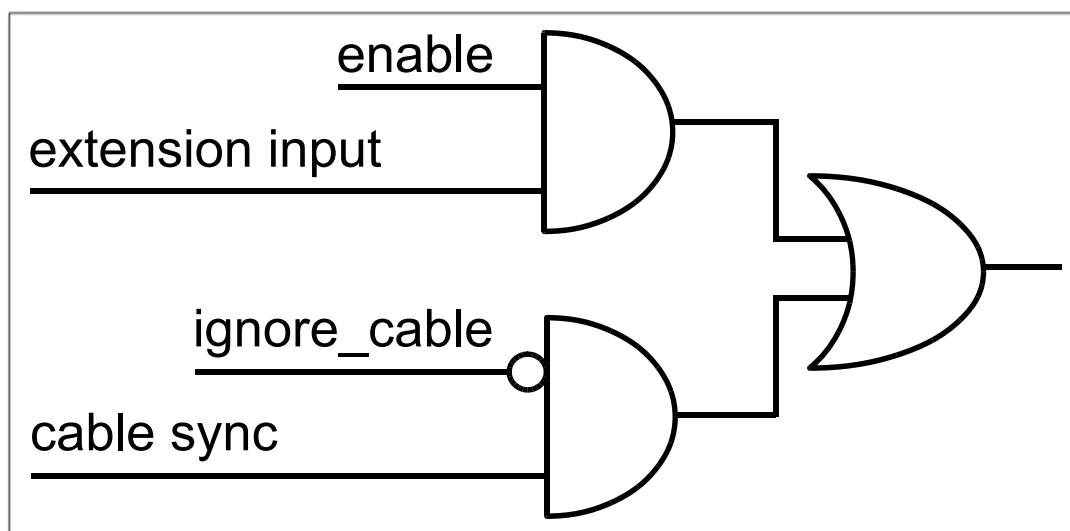


**Figure 2.18:** The extension block combines signals from the optional extension board and the sync cable.



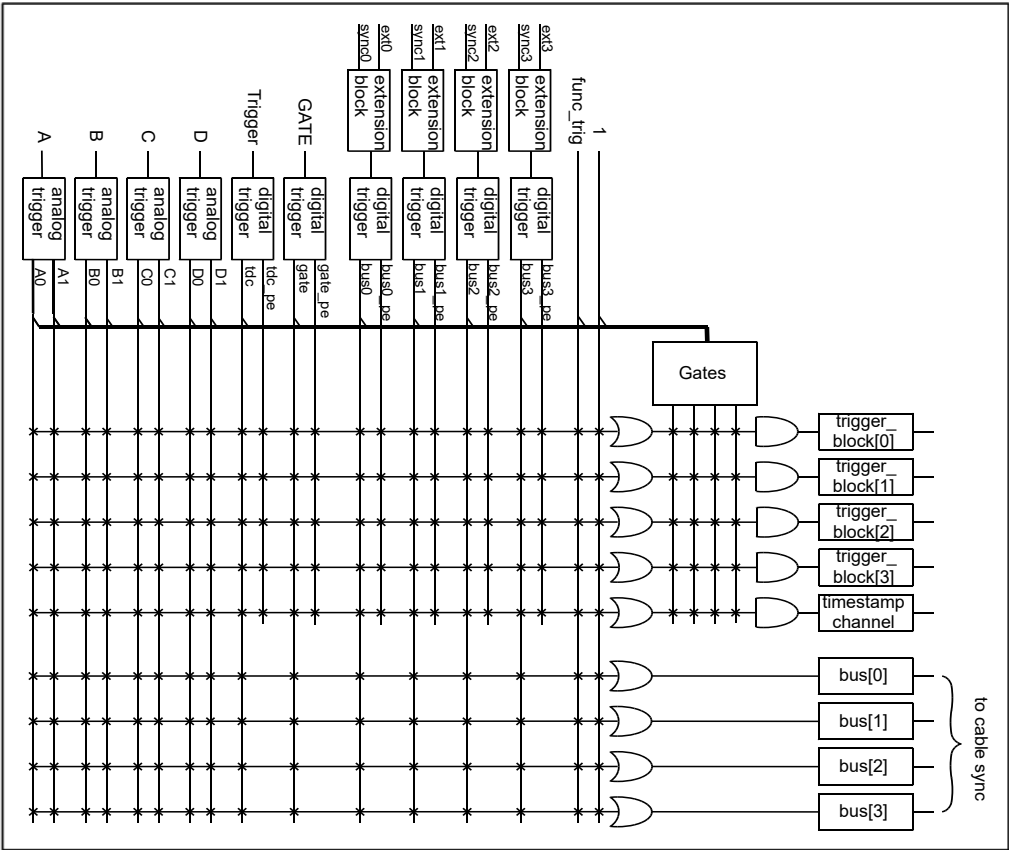

**Figure 2.19:** Trigger Matrix: The trigger signals of each ADC channel, the trigger input, the GATE input or the sync cable can be combined to create a trigger input for each trigger block. The four gate signals can be used to suppress triggers during certain time frames.

### 2.4.4 Gating Blocks

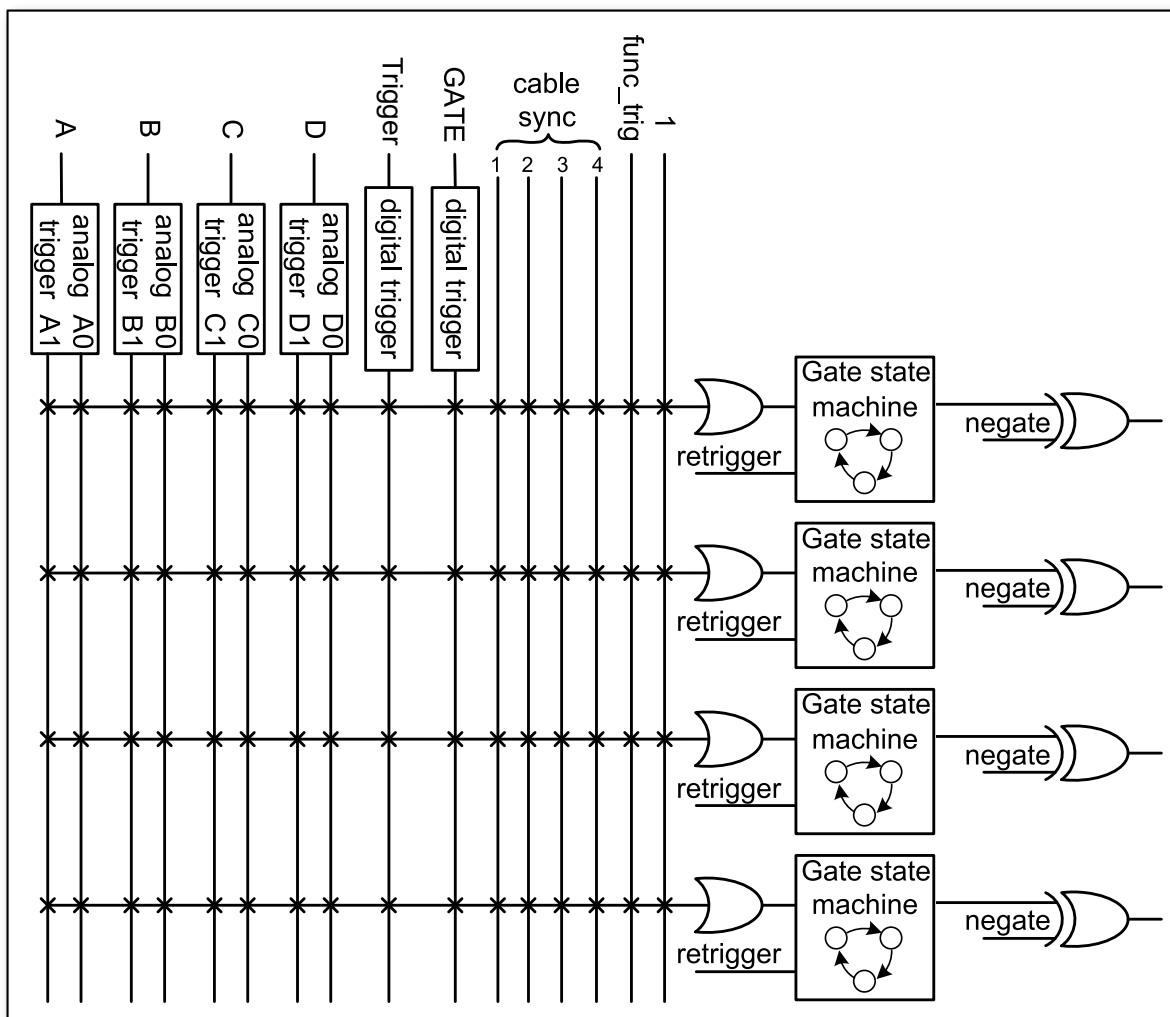

**Figure 2.20:** Gating Blocks: Each gating block can use an arbitrary combination of inputs to trigger its state machine. The outputs can be individually inverted and routed to the AND-gate feeding the trigger blocks.

To decrease the amount of data transmitted to the PC, **Ndigo6G** includes four independent gate and delay units. A gate and delay unit creates a gate window starting at a specified time after a trigger, closing the window at gate stop. Both timing values — gate start and gate stop — must be set as multiples of 3.2 ns.


Trigger blocks can use the gate signal to suppress data acquisition: Only data that fulfills zero suppression specifications occurring in an active gate window is written to the PC.

As input, any trigger from the four trigger blocks, the GATE and Trigger inputs, a trigger from a connected board and the function generator can be used.

The retrigger feature will create a new gate if a trigger occurs during an active gate window. The gate signal can be inverted, causing an active gate to close for a time defined by the user.

The parameters of a gating block are set in Structure `ndigo_gating_block` described in [Section 3.4.4](#).

[Figure 2.21](#) shows the functionality of the gate timing and delay unit. The active gate time is marked in green.

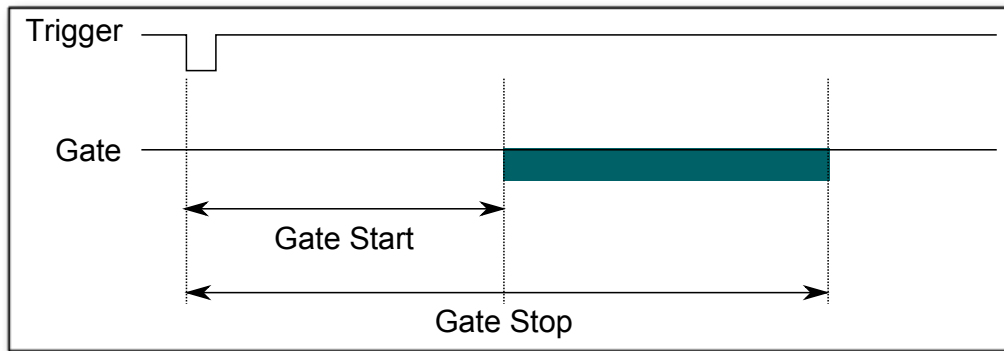

**Figure 2.21:** Gate and delay functionality: When a trigger occurs, the gate opens after a set period of time “gate start” and closes when it reaches “gate stop”.

#### **Gating Example 1: Suppression of Noise After Starting an Acquisition**

In mass spectrometer and other experiments, noise while starting data acquisition can result in undesired trigger events for that time period. To prevent noise in the output data, a gating block could be used to suppress all triggers during start-up.

The following example illustrates the use of a gating block to prevent noise: The GATE input transmits a pulse on each acquisition start. The trigger structure of the GATE input is used to select pulse polarity. Then, the GATE trigger is selected as gating block input and the gating block's start parameter is set to 0. The stop parameter is set to the desired length measured in 3.2 ns clock cycle and negate is set to true. The gating block will now output a low pulse of the desired length whenever there is a pulse on the GATE input.

Enabling this gating block as an AND input to the trigger block, for which noise shall be suppressed.

#### **Gating Example 2: Delayed Trigger**

To sample a short window at a specified time after a trigger event on a channel, the gating block can be used to create a delayed trigger. To do this, one of the triggers of the channel of interested is configured to the desired parameters by selecting the threshold, setting the edge polarity and enabling edge triggering.

Instead of directly using this trigger as input to the trigger block's input matrix, the trigger is selected as an input to a gating block. The block is configured to `start = delay` (in 3.2 ns clock cycles) and `stop = start+1`, `negate = false`. This causes the gating block to produce a one clock cycle pulse on its output after the specified delay.


To send this pulse to the trigger block, the gating block must be enabled in the trigger block's AND matrix and the ONE trigger source must be selected.

#### **Gating Example 3: Dual Level Trigger**


The gates provide AND connections between each other (see Figure 2.19) which can be used for example in a dual level trigger. For the acquisition of signal data with amplitudes between a lower and an upper bound, for example, two level triggers can be connected (see Figure 2.22): a falling level trigger with an upper threshold and a rising level trigger with a lower threshold.

Since the triggers are only connected by OR in the triggerblock logic (see Figure 2.19) they are assigned to one of the gates each and connected with AND via the gating block region of the trigger matrix (see Figures 2.19 and 2.23). Because of the dead times of the gates it is important to enable the retriggering feature. Furthermore a precursor of 2 clock cycles is needed, because the gates are delayed in relation to the ADC samples.

Config settings can be found in the following code [snippet](#).

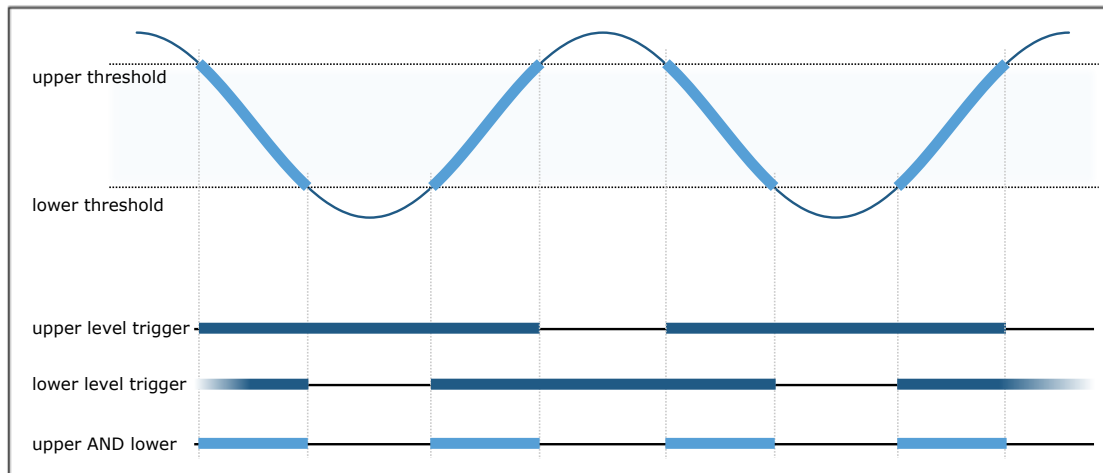

**Figure 2.22:** Measuring data with amplitude between an upper and a lower threshold by means of two level triggers.

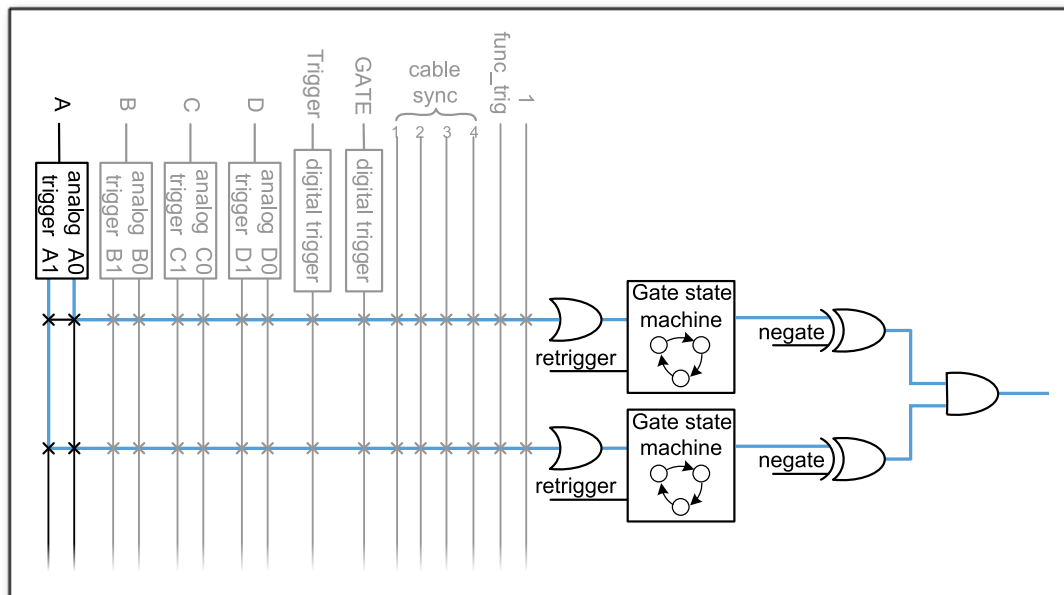

**Figure 2.23:** Gating block logic for the AND connection of two triggers.

```

config.trigger_block[0].enabled = 1;
config.trigger_block[0].precursor = 2;
config.trigger_block[0].length = 0;
config.trigger_block[0].sources = NDIGO_TRIGGER_SOURCE_ONE;
config.trigger_block[0].gates = NDIGO_TRIGGER_GATE_0 | NDIGO_TRIGGER_GATE_1;
config.gating_block[0].retrigger = 1;
config.gating_block[0].stop = 0;
config.gating_block[0].sources = NDIGO_TRIGGER_A0;
config.gating_block[1].retrigger = 1;
config.gating_block[1].stop = 0;
config.gating_block[1].sources = NDIGO_TRIGGER_A1;
config.trigger[NDIGO_TRIGGER_A0].rising = 0;
config.trigger[NDIGO_TRIGGER_A0].threshold = 10000;
config.trigger[NDIGO_TRIGGER_A1].rising = 1;
config.trigger[NDIGO_TRIGGER_A1].threshold = -10000;

```

### 2.4.5 Auto Triggering Function Generator

Some applications require periodic or random triggering. **Ndigo5G**'s function generator provides this functionality.

The delay between two trigger pulses of this trigger generator is the sum of two components: A fixed value  $M$  and a pseudo-random value given by the exponent  $N$ .

The period is

$$T = 1 + M + [1...2^N]$$

clock cycles with a duration of 3.2 ns per cycle.

This allows to monitor input signals at times the current trigger configuration does not trigger, e. g., to get base line information in mass spectrometry applications. It can also be used to determine a suitable threshold level for the trigger by first getting random statistics on the input signal.

### 2.4.6 Timestamp Channel

The timestamp channel produces a stream of small packets that denote the time of the trigger event. An arbitrary set of trigger sources can be selected in the trigger matrix to cause the creation of a packet.

The packets have a fixed length of 16 bytes. The format is described in [Chapter 4.1](#). The length field of the packet contains a 32-bit pattern that contains the levels of all trigger sources at the time of the trigger event except for the period monitor. Only one packet is created, no matter how many trigger sources caused the timestamp channel to trigger.

### 2.4.7 Data Lookup Table

In some applications it might be useful to modify the ADC sample data by a user defined function  $f(x)$ . In this case the onboard FPGA is able to perform this task such that the data stream consists of data words  $f(sample)$  instead of  $sample$ . The function  $f(x)$  is applied using a 1024 word lookup table (LUT) which needs to be provided by the user. This is done by defining the corresponding function as a custom\_lut-member of the ndigo\_configuration structure. Please feel free to contact cronologic if you plan the use this feature. The onboard INL correction is applied prior to mapping the LUT values.

## 2.5 Multiple Ndigo boards synchronization

Using several Ndigo devices in applications that use more channels than a single board can provide requires synchronized operation. To ensure exact synchronization, a delay parameter needs to be set for each board. This parameter might change in case boards are swapped, added or removed and in some cases might change after a firmware update.

The calibration tool “MultiboardCalibration.exe” is available after installing the Ndigo device driver. It is used to find appropriate delay values for each board in a given board setup. After starting, the application lists all Ndigo boards found (Figure 2.24).

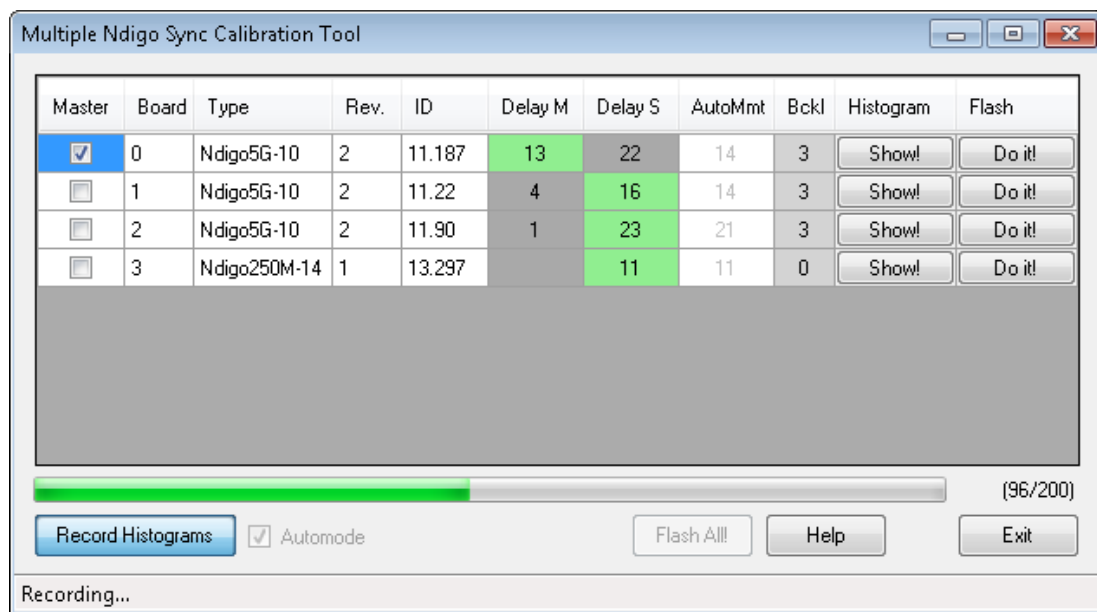



Figure 2.24: Main window of the multiple boards sync calibration tool.

A board's appropriate delay depends on whether it operates in master or slave mode. The respective values can be set in the column “Delay M” (for master boards) and “Delay S” (for slave boards). The designated master board can be selected in the column “Master”. The calibration procedure creates a histogram for each board displaying the current delay between the boards. The histogram can be viewed by clicking on “Show!”. When the appropriate delay values are found they can be stored in the on-board flash PROM by clicking “Do it!” separately for each board. Clicking “Flash All!” will write the values to all boards at once. Please note: Flashing the values might take up to 10 seconds during which the program might not respond.

**Note:** If the application reports a “PLL not locked” error check the cable. If the recording of histograms does not make progress check the cable. Make sure the cable is properly terminated at both ends and firmly attached to each card.


### 2.5.1 Calibration Procedure

1. Make sure “Automode” is selected.
2. Record the calibration histograms by pressing “Record histograms”. The program will perform up to 200 measurements of the sync delay. After accumulating some data, the delay values found are reported in the column “AutoMmt”. The values can be verified by examining the histogram that was recorded. A board’s histogram should look like the one shown in [Figure 2.25](#). During normal operation the delay will be adjusted such that the data points accumulated roughly coincide with the vertical markers in the upper panel. As the delay pattern is periodic valid delay values are between 0 and 31. Thus, the delay value found by the auto measurement should correspond to the distance between the vertical markers and accumulated data points. Hint: When moving the mouse pointer across the histogram the delay value of the current location is displayed.
3. After stopping the data acquisition, by pressing “Record Histograms” again or waiting for 200 measurements to complete, the delay values of the auto measurement need to be copied to the columns “Delay M” or “Delay S” depending on the corresponding board being a master or a slave. The correct field to copy the value to is highlighted in green.
4. You may record a new dataset as a crosscheck that the delay is now set to an appropriate value. By disabling “Automode” the new delay values are used. Press “Record Histograms” in order to start the data acquisition. After some time the histogram should look similar to the one in [Figure 2.26](#).
5. The delay values for all boards in a set needs to be found. For the case a board acts as a master, the value “Delay M” needs to be adjusted, in case it is a slave, the “Delay S” parameter needs to be changed. In order to find the master-case delay values for all boards, the calibration procedure needs to be performed with every board acting as a master once. After changing the master board, the slave values of the other boards don’t need to be readjusted. Only Ndigo5G boards may be set as masters. Therefore, a Ndigo250M board only needs to be calibrated as a slave.
6. After finding all delay values, write the values to the on-board flash PROMs by pressing “Flash All!”.

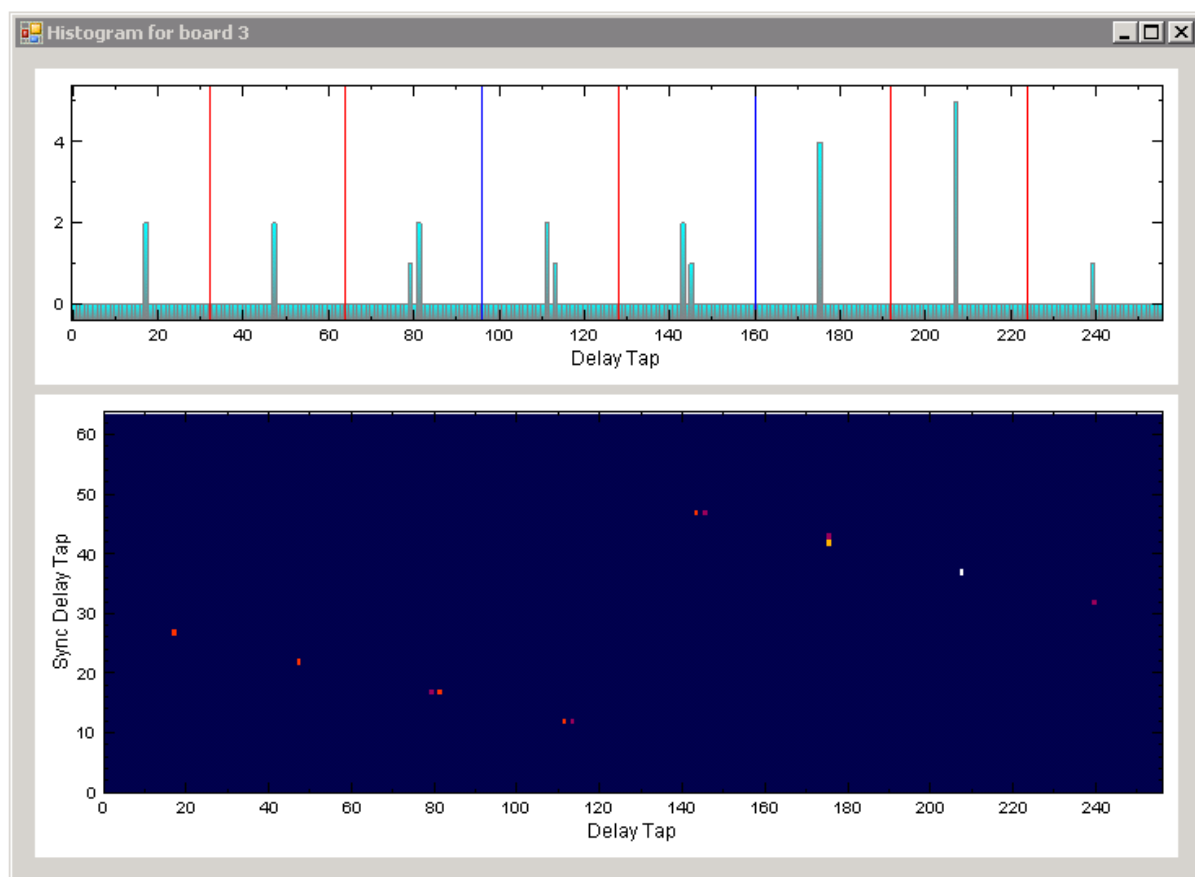

**Figure 2.25:** Histogram for the case that the delay value for the board is not set correctly. Please note that the lower panel might differ from board to board, with the “step” being at a different position.



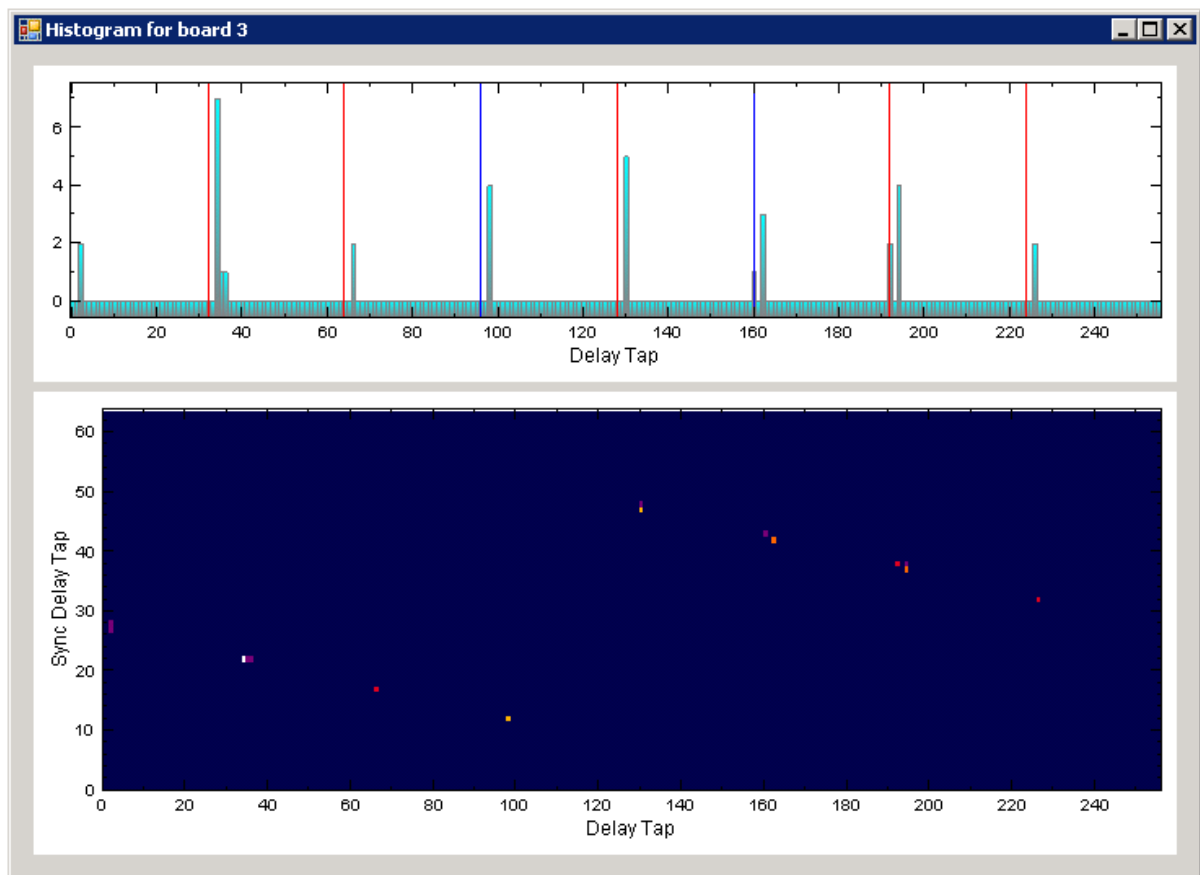


**Figure 2.26:** Histogram for the case that the delay value of the board is set correctly. Please note that the lower panel might differ from board to board, with the “step” being at a different position.

## 2.5.2 Synchronizing a Ndigo5G and an HPTDC8-PCI

In order to operate a Ndigo5G in sync with one or more HPTDC8-PCI boards, a board to board interconnection using a Ndigo Extension Board needs to be done. The Ndigo Extension Board has four clock outputs. One of them needs to be connected to the external clock input of the HPTDC using a standard Lemo 00 cable. The Ndigo5G is connected to the Ndigo Extension Board using the Samtec ribbon cable provided with the Ndigo Extension Board. The signals used for synchronization of the boards are transmitted by a standard 10pin ribbon cable connecting the Ndigo Extension Board and the HPTDC. A schematic of all necessary connections is shown in Figure 2.27.

In principle the user can use the standard device drivers of the Ndigo5G and the HPTDC8-PCI to perform data acquisition. It is, however, recommended to use the cronoSync-library, which is a part of the cronoTools provided with the Ndigo5G device driver. CronoSync offers an easy group-based access to the data recorded and handles the synchronization of all cronologic data acquisition devices used. A detailed description of cronoTools and cronoSync can be found in the cronoTools user guide.

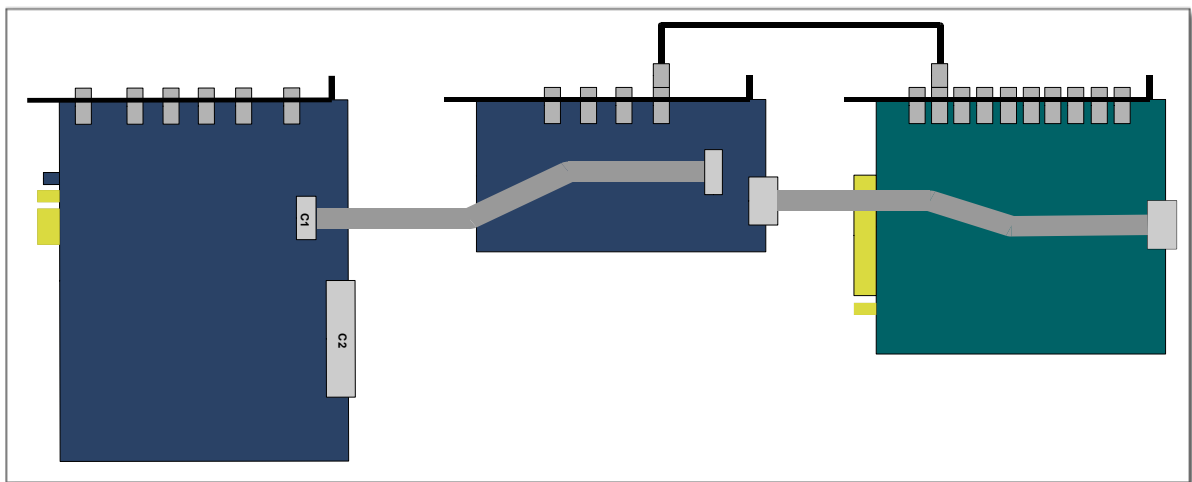


**Figure 2.27:** Interconnection scheme of a Ndigo5G (left) and a HPTDC8-PCI (right) using a Ndigo Extension Board (middle).

## 2.6 Performing a firmware update

After installing the Ndigo device driver, a firmware update tool is available. By choosing “NdigoFirmwareGUI.exe” a firmware update can be performed. After invoking the application a window as shown in Figure 2.28 will appear. The tool can be used for updating the firmware and to create a backup of the on-board calibration data of the Ndigo unit. If several boards are present, the one which is going to be used can be selected in the upper left corner of the window. Pressing the “Backup” buttons a backup of the firmware or the calibration data will be created, respectively. In order to perform a firmware update, choose the “.ndigorom”-file to be used by pressing “Browse”. The file contains the firmware PROMs for all boards of the Ndigo product line. By pressing “Flash” the firmware is written to the board. “Verify” can be used to compare the data stored inside the PROM to the one inside a file.

**Note:** The new firmware will only be used after a power cycle, i.e., after switching the PC (or Ndigo crate) off and back on. A simple reboot is not sufficient. Therefore the information shown in the upper half of the application window does not change right after flashing a new firmware.

After flashing and shutting the PC or the crate off and on again it is recommended to perform a window calibration. The tool “WindowCalibration” is provided for that purpose within the driver installation. The omission of the calibration process leads to longer execution times of applications using that firmware, since the calibration is performed then instead.

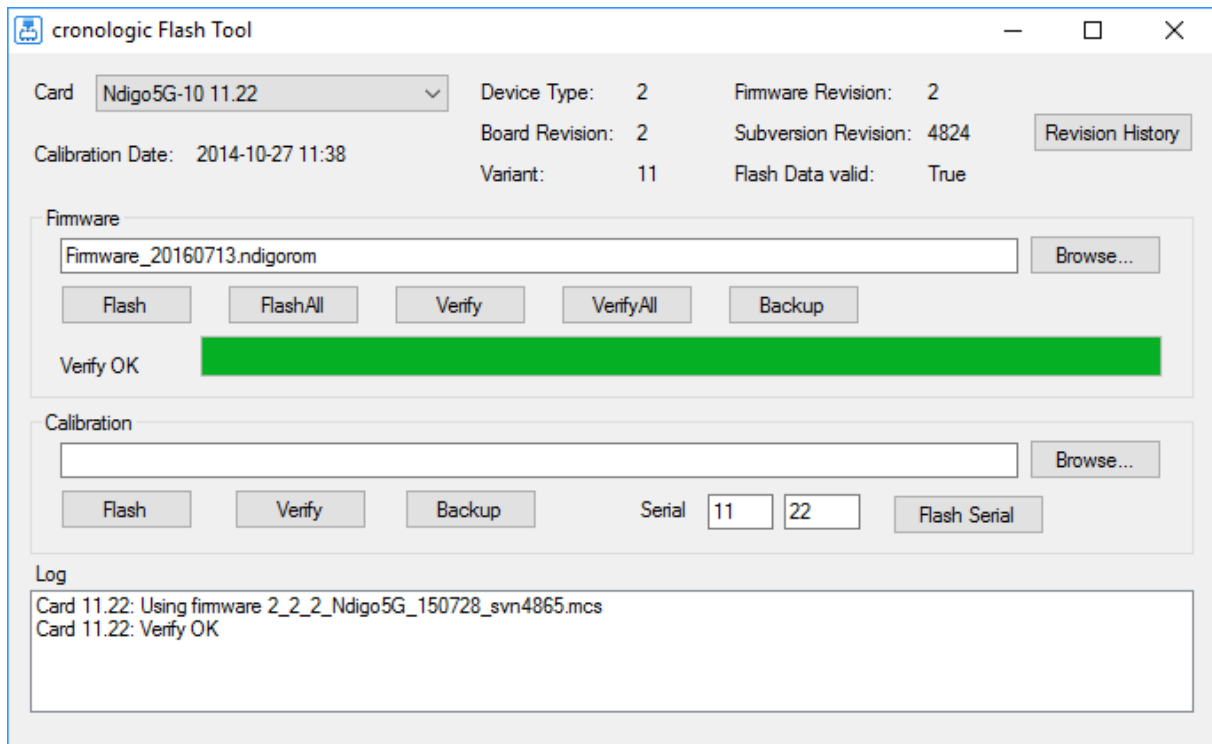

**Figure 2.28:** The firmware update and calibration data backup tool as provided with the Ndigo device driver.

## 2.7 Calibrating the TDC


After each update of the Ndigo5G-10 firmware the TDC has to be calibrated. The calibration is done with the tool “TDCCalibration.exe” which is available after installing the Ndigo device driver. After invoking the application a window as shown in [Figure 2.29](#) will appear.

The calibration procedure is as follows:

1. Connect an external pulse signal to the Trigger input. The signal should be low active with a frequency in the kHz range. It must not be synchronized to the clock source of the Ndigo5G-10. The input frequency must not exceed 10 MHz. The pulse low and high width has to be at least 10ns each.
2. Set *Serial Number* according to the sticker on the card if the shown value is not correct.
3. Start capturing pulse events by pressing the *Start* button.
4. Adjust the *Input Offset* so that *First Bin* is in the range of 4 to 16. If *First Bin* is less than 4, increment *Input Offset* by one. If *First Bin* is greater than 16 decrement *Input Offset* by one. Repeat increment/decrement until *First Bin* is in the range of 4 to 16. Depending on the firmware revision the *Input Offset* value for a successful calibration may be in the range of 6–10 or 28–32.
5. When the *Write Calibration Data* button becomes enabled press it to update the calibration data on the card.
6. Calibration done!

The card can only be successfully calibrated if:

- *First Bin* is in the range of 4 to 16
- *Empty Bins* is less than (First Bin + 4)
- at least 10,000 events have been captured
- a valid serial number is set.

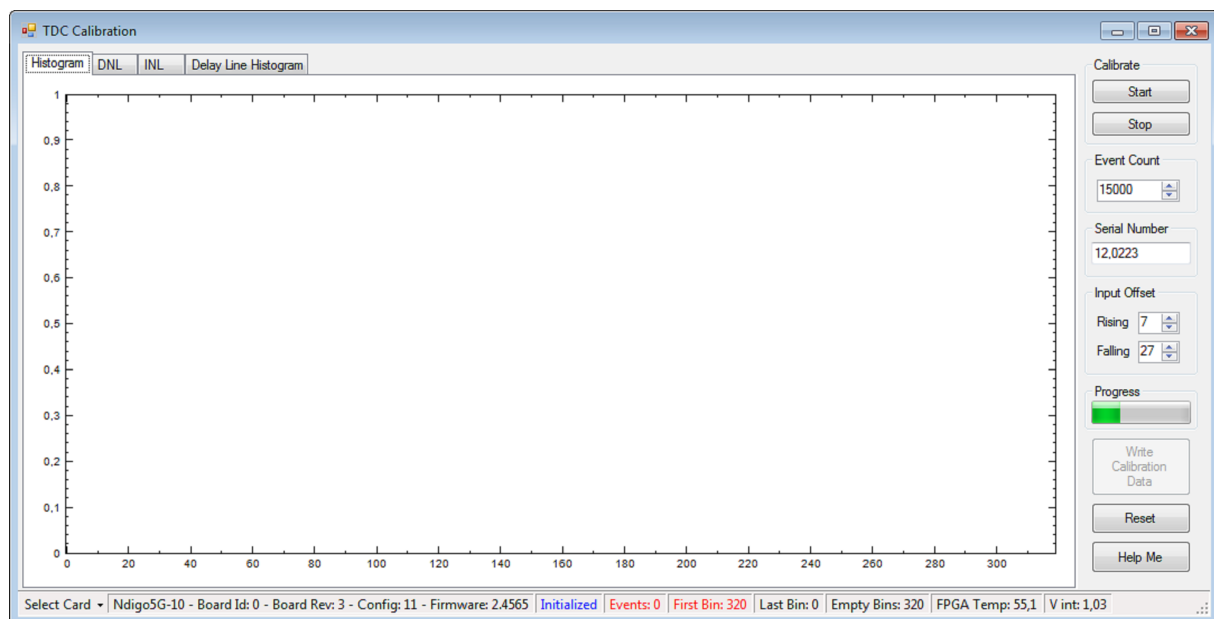

**Figure 2.29:** The TDC calibration tool as provided with the Ndigo device driver.

**Note:** If the application reports an error check if the input pulse is within specification.

## 3 Driver Programming API

The API is a DLL with C linkage. The functions provided by the DLL are declared in `ndigo6g12_interface.h`.

### 3.1 Constants

**#define NDIGO6G12\_CHANNEL\_COUNT 4**

The number of analog input channels.

**#define NDIGO6G12\_GATE\_COUNT 4**

The number of gating blocks.

**#define NDIGO6G12\_TRIGGER\_COUNT 16**

The number of triggers. Two per analog input, one per digital input plus some specials. **TODO check**

**#define NDIGO6G12\_ADD\_TRIGGER\_COUNT 6**

Additional set of triggers for digital inputs.

### 3.2 Initialization

**int ndigo6g12\_count\_devices(int \*error\_code, const char \*\*error\_message)**

Return the number of boards that are supported by this driver in the system.

**int ndigo6g12\_get\_default\_init\_parameters(ndigo6g12\_init\_parameters \*init)**

Get a set of default parameters to feed into `ndigo6g12_init()`. This must always be used to initialize the `ndigo6g12_init_parameter` structure.

**ndigo6g12\_device \*ndigo6g12\_init(ndigo6g12\_init\_parameters \*params, int \*error\_code, char \*\*error\_message)**

Open and initialize the **Ndigo6G12** board with the given index. With `error_code` and `error_message` the user must provide pointers where to buffers where error information should be written by the driver. The buffer for the error message must be at least **80 chars** long. `params` is a structure of type `ndigo6g12_init_parameters` that must be completely initialized.

**int ndigo6g12\_close(ndigo6g12\_device \*device)**

Finalize the driver for this device.

#### 3.2.1 Structure `ndigo6g12_init_parameters`

**int version**

Must be set to `NDIGO6G12_API_VERSION`

**int card\_index**

The index in the list of **Ndigo6G** boards that should be initialized. There might be multiple boards in the system that are handled by this driver as reported by `ndigo6g12_count_devices()`. This index selects one of them. Boards are enumerated depending on the PCIe slot. The lower the bus number and the lower the slot number, the lower the card index.

**int board\_id**

This 8-bit number is filled into each packet created by the board and is useful if data streams of multiple boards will be merged. If only **Ndigo6G12** cards are used this number can be set to the card index. If boards of different types that use a compatible data format are used in a system each board should get a unique id.

**int64\_t buffer\_size[8]**

The minimum size of the DMA buffer. If set to 0, the default size of 64 MiBytes is used. For the Ndigo6G12, only the first entry is used.

**int dma\_read\_delay**

The update delay of the writing pointer after a packet has been send over PCIe. Default value is 8192. Do not change.

**int perf\_derating**

Default 0: 1.6/3.2/6.4 Gsps. Do not change.

**int led\_flashing\_mode**

Controls the LED flashing mode. - 0: off - 1: light all colors once - 2: - 3:

**int adc\_channel\_mask**

Mask with a bit set for each enabled ADC channel. By default, all channels are enabled. Do not change.

**crono\_bool\_t no\_reference\_clock**

Default is false. Do not change.

**crono\_bool\_t use\_external\_clock**

Use 10 MHz clock as a reference. Input is either the internal SMA or external LEMO connector depending on use\_aux2\_clock. Default is false.

**crono\_bool\_t use\_aux2\_clock**

If enabled, use slot bracket LEMO as external reference clock input. Otherwise, the internal SMA connector is used. Has no effect if use\_external\_clock is false. Default is false.

**crono\_bool\_t ignore\_lane\_errors**

Default is false. Do not change.

**crono\_bool\_t ignore\_clock\_erros**

Default is false. Do not change.

**crono\_bool\_t adc\_full\_swing**

Default is false. Do not change.

**int application\_type**

Select four, two, or one channel, or averaging mode. - 0 use currently isntalled type - 1 one ADC channel at 6.4 Gsps - 2 two ADC channels at 3.2 Gsps - 4 four ADC channels at 1.6 Gsps - 5 averaging mode

**crono\_bool\_t force\_bitstream\_update**

Update partial bitstream even if the application type matches.

**int partial\_bitstream\_size**

Size of the partial bitstream.

**uint32\_t \*partial\_bitstream**

Pointer to the buffer with the partial bitstream data. Can be nullptr if application\_type matches application\_type of the currently installed firmware.

**const char \*firmware\_locations**

Pointer to a list of paths (separated by ;). Can be nullptr if application\_type matches application\_type of the currently installed firmware.

### 3.3 Status Information

#### 3.3.1 Functions for Information Retrieval

The driver provides functions to retrieve detailed information on the type of board, its configuration, settings and state. The information is split according to its scope and the computational requirements to query the information from the board.

**int** ndigo6g12\_get\_driver\_revision()

Returns the driver version, same format as `ndigo_static_info::driver_revision`.

**const char\*** ndigo\_get\_driver\_revision\_str()

Returns the driver version including SVN build revision as a string. with format `x.y.z.svn`

**int** ndigo\_get\_static\_info(ndigo\_device \*device, ndigo\_static\_info \*info)

This structure contains information about the board that does not change during run time.

**int** ndigo\_get\_param\_info(ndigo\_device \*device, ndigo\_param\_info \*info)

The structure returned by this call contains information that changes indirectly due to configuration changes.

**int** ndigo\_get\_fast\_info(ndigo\_device \*device, ndigo\_fast\_info \*info)

This call returns a structure that contains dynamic information that can be obtained within a few microseconds.

**int** ndigo\_get\_slow\_info(ndigo\_device \*device, ndigo\_slow\_info \*info)

The data reported in this structure requires milliseconds to be obtained. The application should only call it in situation where the program flow can cope with an interruption of that magnitude.

**const char\*** ndigo\_get\_last\_error\_message(ndigo\_device \*device)

#### 3.3.2 Structure ndigo6g12\_static\_info

This structure contains information about the board that does not change during run time. It is provided by the function `ndigo_get_static_info()`.

**int** size

The number of bytes occupied by the structure.

**int** version

A version number that is increased when the definition of the structure is changed. The increment can be larger than one to match driver version numbers or similar. Set to 0 for all versions up to first release.

**int** board\_id

Index of the board as passed to the constructor or set via

`int` ndigosetboardid(ndigodevice \*device, `int` boardid).

**char** bitstream\_date[NDIGO6G\_BITSTREAM\_DATE\_LEN]

Bitstream creation date

DIN EN ISO 8601 string YYYY-MM-DD HH:DD:SS describing the time when the bitstream was created.

**int** board\_revision

Board revision number.

The board revision number can be read from a register. It is a four bit number that changes when the schematic of the board is changed. - 0: Experimental first board Version. Labeled "Rev. 1" - 2: First commercial Version. Labeled "Rev. 2"

**int** board\_serial

Serial number

With year and running number in 8.24 format. The number is identical to the one printed on the silvery sticker on the board.

**char calibration\_date**[NDIG06G\_CALIBRATION\_DATE\_LEN]

Calibration date

DIN EN ISO 8601 string YYYY-MM-DD HH:DD describing the time when the card was calibrated.

**int chip\_id;**

16bit factory ID of the ADC chip.

This is the chipID as read from the 16 bit ADC chip ID register.

**crono\_bool\_t dc\_coupled**

Shows if the inputs are DC-coupled. Default is **false**, i.e., AC-coupled.

**int driver\_build\_revision**

The build number of the driver according to cronologic's internal versioning system.

**crono\_bool\_t flash\_valid**

Calibration data read from flash is valid.

If not **false**, the driver found valid calibration data in the flash on the board and is using it.

**int fw\_revision**

Revision number of the FPGA configuration

**int fw\_type**

Type of firmware, always **5**, i.e., Ndigo6G-12.

**int pcb\_serial**

Trenz serial number

**int svn\_revision**

Subversion revision ID of the FPGA configuration.

A number to track builds of the firmware in more detail than the firmware revision. It changes with every change in the firmware, even if there is no visible effect for the user. The subversion revision number can be read from a register.

**int application\_type**

Shows the initialized mode **0**: keep currently used application type **1**: one ADC channel @6.4 Gsps **2**: two ADC channels @3.2 Gsps **4**: four ADC channels @1.6 Gsps **5**: averaging mode See NDIG06G\_APP\_TYPE\_\* constants

**char config\_flash\_signature\_primary**[NDIG06G\_FLASH\_SIG\_LEN]

Shows the signature of the primary flash

**char config\_flash\_signature\_secondary**[NDIG06G\_FLASH\_SIG\_LEN]

Shows the signature of the secondary flash

### 3.3.3 Structure `ndigo6g12_param_info`

**int size**

The number of bytes occupied by the structure.

**int version**

A version number that is increased when the definition of the structure is changed. The increment can be larger than one to match driver version numbers or similar. Set to **0** for all versions up to first release.

**double bandwidth**

Bandwidth setting of the ADC. **4.5** or **6.5** (GHz) depending on the configuration.

**double resolution**

ADC sample resolution. Always **12.0** (bit).

**double sample\_rate**

Actual ADC sample rate of currently sampled data. Depends on ADC mode:  $sample\_rate = 6.4 / \#channels$



**double sample\_period**

The period one sample in the data represents in ps.

**double tdc\_period**

The period one TDC bin in the data represents in ps.

**double packet\_ts\_period**

The period one tick of the packet timestamp represents in ps.

**uint64\_t tdc\_packet\_timestamp\_offset**

TDC packets carry the timestamp of the end of packet. To calculate the start, subtract the offset.

**uint32\_t tdc\_rollover\_period**

The time span in TDC bins of one TDC timestamp rollover period.

**adc\_sample\_delay**

The ID the board uses to identify itself in the output data stream. Takes values 0 to 255.

**int board\_id**

The number the board uses to identify the data source in the output data stream.

**int channels**

Number of channels in the current mode.

**int channel\_mask**

Mask with a set bit for each enabled input channel.

**int tdc\_channels**

Number of TDC channels in the current mode.

**int64\_t total\_buffer**

The total amount of the DMA buffer in bytes.

**3.3.4 Structure ndigo6g12\_fast\_info****int size**

The number of bytes occupied by the structure.

**int version**

A version number that is increased when the definition of the structure is changed. The increment can be larger than one to match driver version numbers or similar. Set to 0 for all versions up to first release.

**int state**

The current state of the device. Should be one of the values NDIGO6G12\_DEVICE\_STATE\_\*

**int fan\_speed**

Speed of the FPGA fan in rounds per minute. Reports 0, if no fan is present.

**double fpga\_temperature**

Temperature of the FPGA in °C.

**double fpga\_vccint**

Internal Voltage of the FPGA in V? TODO.

**double fpga\_vccaux**

Auxillary Voltage of the FPGA

**double fpga\_vccbram**

BRAM Voltage of the FPGA in V? TODO.

**double mgt\_0v9**

Shows measured Voltage for the mgt\_0v9 supply in V? TODO.

**double mgt\_1v2**

Shows measured Voltage for the mgt\_1v2 supply in V? TODO.

**double adc\_2v5**

Shows measured Voltage for the 2v5 supply in V? TODO.

**double clk\_3v3**

Shows measured Voltage for the clk\_3v3 supply in V? TODO.

**double adc\_3v3**

Shows measured Voltage for the adc\_3v3 supply in V? TODO.

**double pcie\_3v3**

Shows measured Voltage for the pcie\_3v3 supply in V? TODO.

**double opamp\_5v2**

Shows measured Voltage for the opamp\_5v2 supply in V? TODO.

**double temp4633\_1**

Shows temperature of temp4633\_1 in °C

**double temp4633\_2**

Shows temperature of temp4633\_2 in °C

**double temp4644**

Shows temperature of temp4644 in °C

**double tdc1\_temp**

Temperature of the TDC in °C.

**double ev12\_cmiref**

Shows voltage for ev12\_cmiref supply. Measured or calibration target depending on board revision and assembly variant.

**double ev12\_temp**

Temperature of the ADC in °C.

**int alerts**

Alert bits from temperature sensor and the system monitor.

Bit 0 is set if the TDC temperature exceeds 140 °C. In this case the TDC did shut down and the device needs to be reinitialized.

**int pcie\_link\_width**

Number of PCIe lanes the card uses. Should always be 8 for the Ndigo6G12.

**int pcie\_link\_speed**

Data rate of the PCIe card. Should always be x TODO for the Ndigo6G12.

**int pcie\_max\_payload**

Maximum size for a single PCIe transaction in bytes. Depends on system configuration.

**crono\_bool\_t adc\_data\_pll\_locked**

ADC data clock is PLL locked

**crono\_bool\_t adc\_data\_pll\_lost\_lock**

ADC data clock PLL lost lock (Sticky Bit)

**int adc\_lanes\_synced;**

Shows the synced ADC lanes each bit corresponds to one lane

**int adc\_lanes\_lost\_sync**

Shows the ADC lanes that lost sync each bit corresponds to one lane

**int adc\_lanes\_fifo\_empty**

Shows which ADC lanes have an empty FIFO each bit corresponds to one lane

**int adc\_lanes\_fifo\_full**

Shows which ADC lanes have a full FIFO each bit corresponds to one lane

**int adc\_lanes\_running**

Shows which ADC lanes are running each bit corresponds to one lane

**int** `adc_lanes_sync_timeout`

Shows which ADC lanes were unable to sync before a timeout each bit corresponds to one lane

**int** `adc_sync_retry_count`

The number of ADC lane synchronization retries Default is set to 0

**int** `adc_sync_strobe_retry_count`

The number of ADC strobe synchronization retries Default is set to 0

**int** `adc_sync_delay_count`

16 Bit number showing when the last ADC lane synchronization was achieved

**crono\_bool\_t** `adc_mgt_power_good`

Shows if the supplied mgt power is sufficient

**crono\_bool\_t** `lmk_pll1_locked`

Shows if lmk\_pll1 is locked

**crono\_bool\_t** `lmk_pll2_locked`

Shows if lmk\_pll2 is locked

**crono\_bool\_t** `lmk_lost_lock`

Shows if lmk lost lock

**int** `lmk_lock_wait_count`

Wait count of the lmk

**int** `lmk_ctrl_vcxo`

TODO

**crono\_bool\_t** `lmx_locked`

lmx locked

**crono\_bool\_t** `lmx_lost_lock`

lmx lost lock

**int** `lmx_lock_wait_count`

TODO

### 3.3.5 Structure `ndigo_slow_info`

**int** `size`

The number of bytes occupied by the structure.

**int** `version`

A version number that is increased when the definition of the structure is changed. The increment can be larger than one to match driver version numbers or similar. Set to 0 for all versions up to first release.

**double** `adc_temperature`

ADC temperature in degree Celsius as measured on die.

**double** `board_temperature`

Board temperature in degree celsius.

## 3.4 Configuration

The device is configured with a configuration structure. The user should first obtain a structure that contains the default settings of the device read from an on board ROM, then modify the structure as needed for the user application and use the result to configure the device.

**int** ndigo\_get\_default\_configuration(ndigo\_device \*device, ndigo\_configuration \*config)

**int** ndigo\_get\_current\_configuration(ndigo\_device \*device, ndigo\_configuration \*config)

**int** ndigo\_configure(ndigo\_device \*device, ndigo\_configuration \*config)

**int** ndigo\_set\_board\_id(ndigo\_device \*device, int board\_id)

The board\_id can be changed after initialization of the card. If *cronotools* are used, the board\_id changes have to be done before *cronotools* initialization.

### 3.4.1 Structure ndigo\_configuration

This is the structure containing the configuration information. It is used in conjunction with ndigo\_get\_default\_configuration, ndigo\_get\_current\_configuration and ndigo\_configure.

It uses internally the structures ndigo\_trigger\_block and ndigo\_trigger.

**int** size

The number of bytes occupied by the structure.

**int** version

A version number that is increased when the definition of the structure is changed. The increment can be larger than one to match driver version numbers or similar. Set to 0 for all versions up to first release.

**int** reserved1

Reserved for internal usage. Do not change.

**int** adc\_mode

Constant describing the ADC mode

```
#define NDIGO_ADC_MODE_ABCD 0
#define NDIGO_ADC_MODE_AC 4
#define NDIGO_ADC_MODE_BC 5
#define NDIGO_ADC_MODE_AD 6
#define NDIGO_ADC_MODE_BD 7
#define NDIGO_ADC_MODE_A 8
#define NDIGO_ADC_MODE_B 9
#define NDIGO_ADC_MODE_C 10
#define NDIGO_ADC_MODE_D 11
#define NDIGO_ADC_MODE_AAAA 12
#define NDIGO_ADC_MODE_BBBB 13
#define NDIGO_ADC_MODE_CCCC 14
#define NDIGO_ADC_MODE_DDDD 15
#define NDIGO_ADC_MODE_A12 28 // not available on all boards
#define NDIGO_ADC_MODE_B12 29 // not available on all boards
#define NDIGO_ADC_MODE_C12 30 // not available on all boards
#define NDIGO_ADC_MODE_D12 31 // not available on all boards
```

**double** bandwidth

Set to the minimum bandwidth required for the application. Lower bandwidth results in reduced noise. The driver will set the ADC to the minimum setting that has at least the desired bandwidth and report the selected bandwidth in the ndigo\_param\_info structure. Versions -8, -10 and -12 currently support 1 GHz and 3 GHz bandwidth, version -8AQ supports 2 GHz, 1.5 GHz, 600 MHz and 500 MHz.

**ndigo\_bool\_t** reserved

Reserved for internal use, do not change.

**ndigo\_bool\_t tdc\_enabled**

Enable capturing of TDC measurements on external digital input channel.

**ndigo\_bool\_t tdc\_fb\_enabled**

Enable enhanced TDC resolution. Currently not implemented.

**double analog\_offset[NDIGO\_CHANNEL\_COUNT]**

Sets the input DC offset-values to  $\pm$  this value in V. Defaults to 0.

**double dc\_offset[2]**

Sets the DC offset in volts for the TDC trigger input (index 1) and the GATE input (index 0). The trigger threshold is zero. For **negative 0.8 V NIM** pulses, this value should be set to 0.4.

**ndigo\_trigger trigger[NDIGO\_TRIGGER\_COUNT + NDIGO\_ADD\_TRIGGER\_COUNT]**

Configuration of the external trigger sources. Threshold is ignored for entries **8 and above**.

The trigger indexes refer to the entry in the trigger array and are defined like this:

```
#define NDIGO_TRIGGER_A0 0
#define NDIGO_TRIGGER_A1 1
#define NDIGO_TRIGGER_B0 2
#define NDIGO_TRIGGER_B1 3
#define NDIGO_TRIGGER_C0 4
#define NDIGO_TRIGGER_C1 5
#define NDIGO_TRIGGER_D0 6
#define NDIGO_TRIGGER_1 7
#define NDIGO_TRIGGER_TDC 8
#define NDIGO_TRIGGER_GATE 9
#define NDIGO_TRIGGER_BUS0 10
#define NDIGO_TRIGGER_BUS1 11
#define NDIGO_TRIGGER_BUS2 12
#define NDIGO_TRIGGER_BUS3 13
#define NDIGO_TRIGGER_UTO 14
#define NDIGO_TRIGGER_ONE 15
```

Always positive edge-sensitive sources:

```
#define NDIGO_TRIGGER_TDC PE 16
#define NDIGO_TRIGGER_GATE PE 17
#define NDIGO_TRIGGER_BUS0 PE 18
#define NDIGO_TRIGGER_BUS1 PE 19
#define NDIGO_TRIGGER_BUS2 PE 20
#define NDIGO_TRIGGER_BUS3 PE 21
```

**ndigo\_trigger\_block trigger\_block[NDIGO\_CHANNEL\_COUNT + 1]**

A structure describing the trigger settings of the four channels plus the timestamp channel. In some modes not all channels are used.

**ndigo\_gating\_block gating\_block[4]**

A structure describing the gating blocks that can be used by the trigger blocks to filter triggers.

**ndigo\_extension\_block extension\_block[NDIGO\_EXTENSION\_COUNT]**

A structure describing the routing of the 4 digital channels of the **Ndigo extension board** to the trigger matrix.

**int drive\_bus[4]**

Enable output drive for each of the four external sync lines. Each integer represents a bitmask selecting the trigger sources for that line. The bit mapping is described in [Section 3.4.3](#)

**int auto\_trigger\_period****int auto\_trigger\_random\_exponent**

Create a trigger either periodically or randomly. With  $M = \text{auto\_trigger\_period}$  and  $N = \text{auto\_trigger\_random\_exponent}$ , the number of clock cycles  $T$  between triggers will be

$$T = 1 + M + [1 \dots 2^N]$$

where  $0 \leq M < 2^{32}$  and  $0 \leq N < 32$ .

There is no enable or reset as the usage of this trigger can be configured in the trigger block channel source field.

#### **int** output\_mode

Defines the data representation in the output. Signed16 scales and CUTSOM\_INL corrects the input. RAW directly presents the ADC values.

```
#define NDIGO_OUTPUT_MODE_SIGNED16 0
#define NDIGO_OUTPUT_MODE_RAW 1
#define NDIGO_OUTPUT_MODE_CUSTOM 2
#define NDIGO_OUTPUT_MODE_CUSTOM_INL 3
```

#### **lut\_func** custom\_lut

Look-up table. If the output\_mode is set to NDIGO\_OUTPUT\_MODE\_CUSTOM or to NDIGO\_OUTPUT\_MODE\_CUSTOM\_INL, this function is used for mapping from ADC value to output value. The driver will call this function with a value from -1 to +1 and the function must return the corresponding signed 16-bit value that the board should return for an input voltage relative to the full scale range.

#### **typedef short** (\*lut\_func)(**int** channel, **float** x)

This can be used, e.g., for custom INL, offset and gain correction that covers user front end electronics. It can also invert the signal or correct the effect of logarithmic input amplifiers etc.

The look-up table is applied on the board, thus using it does not cause any additional CPU load. In the mode NDIGO\_OUTPUT\_MODE\_CUSTOM\_INL the on-board INL correction table is applied before the user function, while NDIGO\_OUTPUT\_MODE\_CUSTOM does not perform INL correction. In order to use the user LUT functionality, lut\_func must be set to a pointer to the LUT-function

### 3.4.2 Structure ndigo\_trigger

#### **short** threshold

Sets the threshold for the trigger block within the range of the ADC data of -32768 and +32768.

For trigger indices NDIGO\_TRIGGER\_TDC to NDIGO\_TRIGGER\_BUS3\_PE, the threshold is ignored.

#### **ndigo\_bool\_t** edge

If set, this trigger implements edge trigger functionality. Else, this is a level trigger.

For trigger indices NDIGO\_TRIGGER\_AUTO and NDIGO\_TRIGGER\_ONE, this is ignored.

For trigger indices NDIGO\_TRIGGER\_TDC\_PE to NDIGO\_TRIGGER\_BUS3\_PE, this must be set.

#### **ndigo\_bool\_t** rising

If set, trigger on rising edges or when above threshold.

For trigger indices NDIGO\_TRIGGER\_AUTO and NDIGO\_TRIGGER\_ONE this is ignored.

For trigger indices NDIGO\_TRIGGER\_TDC\_PE to NDIGO\_TRIGGER\_BUS3\_PE this must be set.

### 3.4.3 Structure ndigo\_trigger\_block

#### **ndigo\_bool\_t** enabled

Activate triggers on this channel.

#### **ndigo\_bool\_t** retrigger

If a new trigger condition occurs while the postcursor is acquired, the packet is extended by starting a new postcursor. Otherwise the new trigger is ignored and the packet ends after the precursor of the first trigger.

The retrigger setting is ignored for the timestamp channel.

**ndigo\_bool\_t reserved1**

Defaults to **false**. Do not change.

**ndigo\_bool\_t reserved2**

Defaults to **false**. Do not change.

**int precursor**

Precursor in multiples of 3.2ns. The amount of data preceding a trigger that is captured. The precursor setting is ignored for the timestamp channel.

**int length**

In multiples of 3.2 ns.

The total amount of data that is recorded in addition to the trigger window. Precursor determines how many of these are ahead of the trigger and how many are appended after the trigger. In **edge trigger mode** the trigger window always is **3.2 ns** wide. In **level trigger mode** it is as long as the trigger condition is fulfilled.

The length setting is ignored for the timestamp channel.

**int sources**

A bit mask with a bit set for all trigger sources that can trigger this channel.

```
#define NDIGO_TRIGGER_SOURCE_A0 0x00000001
#define NDIGO_TRIGGER_SOURCE_A1 0x00000002
#define NDIGO_TRIGGER_SOURCE_B0 0x00000004
#define NDIGO_TRIGGER_SOURCE_B1 0x00000008
#define NDIGO_TRIGGER_SOURCE_C0 0x00000010
#define NDIGO_TRIGGER_SOURCE_C1 0x00000020
#define NDIGO_TRIGGER_SOURCE_D0 0x00000040
#define NDIGO_TRIGGER_SOURCE_D1 0x00000080
#define NDIGO_TRIGGER_SOURCE_TDC 0x00000100
#define NDIGO_TRIGGER_SOURCE_GATE 0x00000200
#define NDIGO_TRIGGER_SOURCE_BUS0 0x00000400
#define NDIGO_TRIGGER_SOURCE_BUS1 0x00000800
#define NDIGO_TRIGGER_SOURCE_BUS2 0x00001000
#define NDIGO_TRIGGER_SOURCE_BUS3 0x00002000
#define NDIGO_TRIGGER_SOURCE_AUTO 0x00004000
#define NDIGO_TRIGGER_SOURCE_ONE 0x00008000
#define NDIGO_TRIGGER_SOURCE_TDC PE 0x01000000
#define NDIGO_TRIGGER_SOURCE_GATE PE 0x02000000
#define NDIGO_TRIGGER_SOURCE_BUS0 PE 0x04000000
#define NDIGO_TRIGGER_SOURCE_BUS1 PE 0x08000000
#define NDIGO_TRIGGER_SOURCE_BUS2 PE 0x10000000
#define NDIGO_TRIGGER_SOURCE_BUS3 PE 0x20000000
```

**int gates**

```
#define NDIGO_TRIGGER_GATE_NONE 0x0000
#define NDIGO_TRIGGER_GATE_0 0x0001
#define NDIGO_TRIGGER_GATE_1 0x0002
#define NDIGO_TRIGGER_GATE_2 0x0004
#define NDIGO_TRIGGER_GATE_3 0x0008
```

**double minimum\_free\_packets**

This parameter sets how many packets are supposed to fit into the on-board FIFO before a new packet is recorded after the FIFO was full, i.e., a certain amount of free space in the FIFO is demanded before a new packet is written after the FIFO was full.

As a measure for the packet length the gate length set by the user is used. The on-board algorithm checks the free FIFO space only in case the FIFO is full. Therefore, if this number is **1.0** or more, at least every second packet in the DMA buffer is guaranteed to have the full length set by the gate length parameters. In many cases smaller values will also result in full length packets. But below a certain value multiple packets that are cut off at the end will show up.

### 3.4.4 Structure `ndigo_extension_block`

This structure configures how the inputs from the optional extension board and signals from the synchronization bus are merged.

#### `ndigo_bool_t enable`

Enable routing of digital signal from Ndigo extension board to the according BUSx trigger unit.

#### `ndigo_bool_t ignore_cable`

If `false` input signal and BUS signal are *OR\*ed* before routing to the according BUSx trigger unit. Otherwise only the signal from *\*\*Ndigo extension board\** is used.

### 3.4.5 Run Time Control

`int ndigo_start_capture(ndigo_device *device)`

`int ndigo_pause_capture(ndigo_device *device)`

`int ndigo_continue_capture(ndigo_device *device)`

Call this to resume data acquisition after a call to `ndigo_pause_capture`.

`int ndigo_stop_capture(ndigo_device *device)`

## 3.5 Readout

`int ndigo_read(ndigo_device *device, ndigo_read_in *in, ndigo_read_out *out)`

Return a pointer to an array of captured data in `read_out`. The result can contain any number of packets of type `ndigo_packet`. `read_in` provides parameters to the driver. A call to this method automatically allows the driver to reuse the memory returned in the previous call.

Returns an error code as defined in the structure `ndigo_read_out`.

`int ndigo_acknowledge(ndigo_device *device, ndigo_packet *packet)`

Acknowledge all data up to the packet provided as parameter. This is mandatory if `acknowledge_last_read` in the `ndigo_read_in` structure is set to `false` for calls to `ndigo_read`.

This feature allows to either free up partial DMA space early if there will be no call to `ndigo_read` anytime soon. It also allows to keep data over multiple calls to `ndigo_read` to avoid unnecessary copying of data.

`int ndigo_process_tdc_packet(ndigo_device *device, ndigo_packet *packet)`

Call on a TDC packet to update the timestamp of the packet with a more accurate value. If called more than once on a packet the timestamp will be invalid.

### 3.5.1 Input Structure `ndigo_read_in`

#### `ndigo_bool_t acknowledge_last_read`

If set `ndigo_read` automatically acknowledges packets from the last read.



### 3.5.2 Output Structure `ndigo_read_out`

`ndigo_packet *first_packet`

Pointer to the first packet that was capture by the call of `ndigo_read`.

`ndigo_packet *last_packet`

Address of header of the last packet in the buffer.

`int error_code`

```
#define NDIGO_READ_OK 0
#define NDIGO_READ_NO_DATA 1
#define NDIGO_READ_INTERNAL_ERROR 2
```

`const char *error_message`

## 3.6 Other Functions

### 3.6.1 LED control

There are six LEDs on the front panel. The intensity of the red and green part can be set from 0 to 255. There is no blue component in the current version. Per default all LEDs are set to auto mode. This means that used channels are lit **green**, activity is shown as **yellow** on overflow is shown as **red**.

`int ndigo_set_led_color(ndigo device *device, int led, unsigned short r, unsigned short g, unsigned short b)`

Set the LED to the selected color. No automatic updates are performed.

`int ndigo_set_led_automode(ndigo device *device, int led)`

Let the selected LED be controlled by hardware.

## 4 Packet Format

### 4.1 Output Structure `ndigo_packet`

**unsigned char** `channel`

0 to 3 for the ADC input channels, 4 for the TDC, 5 for the timestamp channel.

**unsigned char** `card`

Identifies the source card in case there are multiple boards present. Defaults to 0 if no value is assigned to the parameter `boardid` in Structure `ndigoinitparameters` or set via **int** `ndigosetboardid(ndigodevice *device, int boardid)`.

**unsigned char** `type`

For the ADC channels this is set to 1 to signify 16-bit signed data.

For the TDC channel it is set to 8 to signify 64-bit unsigned data.

If the type field is 128 or greater then there is no data present, even if length is not 0. In this cases the length field may contain other data.

Type	Length Field	Description
1	Number of payload words	16 bit signed samples from one of the ADCs
8	Number of payload words	64 Bit unsigned TDC Data, only for internal processing
128	Bit pattern of trigger sources	Whenever at least one of the sources that is enabled for the timestamp channel triggers, one of these packets is generated. The length field contains the triggers active when this packet was created.

**unsigned char** `flags`

**#define** `NDIGO_PACKET_FLAG_SHORTENED 1`

If the bit with **weight 1** is set, the packet was truncated because the internal FIFO was full. Less than the requested number of samples have been written due to the full FIFO.

**#define** `NDIGO_PACKET_FLAG_PACKETS_LOST 2`

If the bit with **weight 2** is set, there are lost triggers immediately preceding this packet due to insufficient DMA buffers. The DMA controller has discarded packets due to full host buffer.

**#define** `NDIGO_PACKET_FLAG_OVERFLOW 4`

If the bit with **weight 4** is set, the packet contains ADC sample overflows.

**#define** `NDIGO_PACKET_FLAG_TRIGGER_MISSED 8`

If the bit with **weight 8** is set, there are lost triggers immediately preceding this packet due to insufficient buffers. The trigger unit has discarded packets due to full FIFO.

**#define** `NDIGO_PACKET_FLAG_DMA_FIFO_FULL 16`

If the bit with **weight 16** is set, the internal DMA FIFO was full. Triggers only got lost if a subsequent package has the bit with **weight 8** set.

**#define** `NDIGO_PACKET_FLAG_HOST_BUFFER_FULL 32`

If the bit with **weight 32** is set, the host buffer was full. Triggers only got lost if a subsequent package has the bit with **weight 8** set.

```
#define NDIGO_PACKET_FLAG_TDC_NO_EDGE 64
```

If the bit with **weight 64** is set, the packet from the TDC does not contain valid data and the timestamp is not corrected. No valid edge was found in TDC packet.

```
unsigned int length
```

Number of **64-bit** elements (each containing four samples) in the data array if type < 128.

If type == 128 this is the pattern of trigger sources that were active in the clock cycle given by the timestamp. Bits are set according to the trigger sources, i.e., **bit 0** is set if **trigger A0** was active, **bit 29** is set if **trigger BUS3 PE** was active. Use the NDIGO\_TRIGGER\_SOURCE\_\*-defines to check for the bits set.

```
unsigned __int64 timestamp
```

ADC channels **A** to **D**: Timestamp of the last word in the packet in ps.

TDC: Timestamp of the trigger event (falling edge) on the TDC channel in ps. When ndigo\_process\_tdc\_packet() is called once on the packet, the timestamp is replaced with the precise timestamp for the edge.

Timestamp channel: Timestamp of the trigger event in ps.

```
unsigned __int64 data[]
```

Sample data. For the **Ndigo5G** each **64-bit** word contains four **16-bit** signed words from the ADC. The user can cast the array to **short** to directly operate on the sample data.

## 5 C-Example

```
1  #include "Ndigo_interface.h"
2  #include <stdio.h>
3  #include <stdlib.h>
4
5  int main(int argc, char* argv[])
6  {
7      ndigo_init_parameters params;
8      ndigo_get_default_init_parameters(&params);
9
10     params.card_index = 0;
11     params.buffer_size[0] = 1<<23;
12     params.drive_external_clock = true;
13     params.is_slave = false;
14     params.use_external_clock = false;
15
16     int error_code;
17     const char* error_message;
18     ndigo_device* ndgo = ndigo_init(&params, &error_code, &error_message);
19     if( error_code != NDIGO_OK ) {
20         printf("\nError %d: %s\n", error_code, error_message);
21         exit(-1);
22     }
23
24     ndigo_configuration config;
25     ndigo_get_default_configuration(ndgo, &config);
26     config.adc_mode = NDIGO_ADC_MODE_ABCD;
27
28     // disable unused trigger blocks
29     config.trigger_block[1].enabled = false;
30     config.trigger_block[2].enabled = false;
31     config.trigger_block[3].enabled = false;
32     config.trigger_block[4].enabled = false;
33
34     // configure trigger block 0
35     config.trigger_block[0].enabled = true;
36     config.trigger_block[0].minimum_free_packets = 1.0;
37     config.trigger_block[0].precursor = 0;
38     config.trigger_block[0].retrigger = 0;
39
40     config.trigger_block[0].sources = NDIGO_TRIGGER_SOURCE_A0;
41     config.trigger_block[0].length = 16;
42     config.trigger_block[0].gates = NDIGO_TRIGGER_GATE_NONE;
43
44     config.analog_offset[0] = 0.1;
45
46     config.trigger[NDIGO_TRIGGER_A0].edge = true;
47     config.trigger[NDIGO_TRIGGER_A0].rising = false;
48     config.trigger[NDIGO_TRIGGER_A0].threshold = 0;
49
50     if( ndigo_configure(ndgo, &config) != NDIGO_OK ) {
51         printf("\nFatal configuration error. Aborting...\n");
52         exit(-1);
53     }
54
55     ndigo_start_capture(ndgo);
56
57     // counts the number of packets received
58     int count = 0;
```

(continues on next page)

(continued from previous page)

```

58
59 while( count < 10 ) {
60     ndigo_read_in in;
61     // Do not wait for data
62     // (if set to 1 the ndigo_acknowledge function has to be removed)
63     in.acknowledge_last_read = 0;
64     ndigo_read_out out;
65     int result = ndigo_read(ndgo, &in, &out);
66     if( !result ) {
67         // buffer received with one or more packets
68         ndigo_packet *packet = out.first_packet;
69         while( packet <= out.last_packet ) {
70             int length = 0;
71             if( !(packet->type & NDIGO_PACKET_TYPE_TIMESTAMP_ONLY) )
72                 length = packet->length;
73
74             printf("Card %02x, Channel %02x, Flags %02x, Length %6d, Timestamp %llu \n",
75 packet->card, packet->channel, packet->flags, length, packet->timestamp);
76             if( !(packet->type & NDIGO_PACKET_TYPE_TIMESTAMP_ONLY) ){
77                 short* data = (short*) packet->data;
78                 for( inti = 0; i < packet->length * 4; i++ )
79                     printf("%6d, ", *(data++));
80                 printf("\n\n");
81             }
82             // current packet pointer is invalid after call to ndigo_acknowledge
83             ndigo_packet *next_packet = ndigo_next_packet(packet);
84             ndigo_acknowledge(ndgo, packet);
85             packet = next_packet;
86             count++;
87         }
88     }
89     ndigo_close(ndgo);
90     return 0;
91 }

```

## 6 Technical Data

- Input Passband: **4.5 MHz** to **950 MHz**
- Power Requirements: **25 W**
- Mechanical Dimensions: **170 mm × 106 mm**
- Throughput: **800 MByte/s** on PCIe x4

### 6.1 Digitizer Characteristics

Each board is tested against the values listed in the “Min” column. “Typical” is the mean value of the first 10 boards produced.

#### 6.1.1 1-Channel-Mode (5 Gps)

Symbol	Parameter	Min	Typical	Max	Units
THD1	Total Harmonic Distortion	56	60		dB
SNR1	Signal to Noise Ration	47	49		dB
SFDR <sub>incl</sub> 1	Spurious Free Dynamic Range (including Harmonics)	55	59		dB
SFDR <sub>excl</sub> 1	Spurious Free Dynamic Range (excluding Harmonics)	55	60		dB
SINAD1	Signal-to-Interference Ratio including Noise and Distortion	47	48		dB
ENOB1	Effective Number of Bits	7.5	7.7		

#### 6.1.2 2-Channel-Mode (2.5 Gps)

Symbol	Parameter	Min	Typical	Max	Units
THD2	Total Harmonic Distortion	56	60		dB
SNR2	Signal to Noise Ration	49	51		dB
SFDR <sub>incl</sub> 2	Spurious Free Dynamic Range (including Harmonics)	58	60		dB
SFDR <sub>excl</sub> 2	Spurious Free Dynamic Range (excluding Harmonics)	58	61		dB
SINAD2	Signal-to-Interference Ratio including Noise and Distortion	49	50		dB
ENOB2	Effective Number of Bits	7.8	8.1		

#### 6.1.3 4-Channel-Mode (1.25 Gps)

Symbol	Parameter	Min	Typical	Max	Units
THD4	Total Harmonic Distortion	56	60		dB
SNR4	Signal to Noise Ration	49	51		dB
SFDR <sub>incl</sub> 4	Spurious Free Dynamic Range (including Harmonics)	58	60		dB
SFDR <sub>excl</sub> 4	Spurious Free Dynamic Range (excluding Harmonics)	68	73		dB
SINAD4	Signal-to-Interference Ratio including Noise and Distortion	49	51		dB
ENOB4	Effective Number of Bits	7.9	8.1		

## 6.2 Electrical Characteristics

### 6.2.1 Oscillator

The **Ndigo5G** uses an OCXO oscillator with **25 ppb** stability. After power up the oscillator needs to run for **10 minutes** to reach this stability.

### 6.2.2 Environmental Conditions for Operation

The board is designed to be operated under the following conditions:

Symbol	Parameter	Min	Typical	Max	Units
T	ambient temperature	5		40	°C
RH	relative humidity at 31°C	20		75	%

### 6.2.3 Environmental Conditions for Storage

The board shall be stored between operation under the following conditions:

Symbol	Parameter	Min	Typical	Max	Units
T	ambient temperature	-30		60	°C
RH	relative humidity at 31°C non condensing	10		70	%

### 6.2.4 Power Supply

Symbol	Parameter	Min	Typical	Max	Units
I	PCIe 3,3V rail power consumption			4	mA
VCC	PCIe 3,3V rail power supply	3.1	3.3	3.6	V
I	PCIe 12V rail power consumption			2.1	A
VCC	PCIe 12V rail power supply	11.1	12	12.9	V
I	PCIe 3,3VAux rail power consumption		0		A
VCC	PCIe 3,3VAux rail power supply		3.3		V

### 6.2.5 Analog Input

AC coupled single-ended analog inputs (standard version).

Symbol	Parameter	Min	Typical	Max	Units
V <sub>p-p</sub>	Peak to peak input voltage			0,5	V
Z <sub>p</sub>	Input impedance Analog offset	-0.25	50	0.25	Ω V

AC coupled differential analog inputs (S version).

Symbol	Parameter	Min	Typical	Max	Units
V <sub>com</sub>	Input common mode	-4		6	V
V <sub>p-p</sub>	Differential input Voltage	-125		125	mV
Z <sub>p</sub>	Input impedance Analog offset	-0.25	100	+0.25	Ω V

## 6.2.6 Analog inputs

Single ended AC coupled inputs Trigger and GATE with configurable DC offset bias.

Symbol	Parameter	Min	Typical	Max	Units
$V_{\text{trig}}$	Pulse height			5.0	V
$V_{\text{trigoffset}}$	DC offset	-1.25		1.25	V
$V_{\text{tdcoffset}}$	DC offset for TDC	-1.25		-0.01	V
$Z_{\text{trig}}$	Input impedance		50		$\Omega$
$t_{\text{pulse}}$	pulse width	7		100	ns

## 6.3 Information Required by DIN EN 61010-1

### 6.3.1 Manufacturer

The **Ndigo5G** is a product of:

cronologic GmbH & Co. KG  
Jahnstraße 49  
60318 Frankfurt

HRA 42869 beim Amtsgericht Frankfurt/M  
VAT-ID: DE235184378

### 6.3.2 Intended Use and System Integration

The devices are not ready to use as delivered by cronologic. It requires the development of specialized software to fulfill the application of the end user. The device is provided to system integrators to be built into measurement systems that are distributed to end users. These systems usually consist of a the **Ndigo5G**, a main board, a case, application software and possible additional electronics to attach the system to some type of detector. They might also be integrated with the detector.

The **Ndigo5G** is designed to comply with **DIN EN 61326-1** when operated on a PCIe compliant main board housed in a properly shielded enclosure. When operated in a closed standard compliant PC enclosure the device does not pose any hazards as defined by **EN 61010-1**.

Radiated emissions, noise immunity and safety highly depend on the quality of the enclosure. It is the responsibility of the system integrator to ensure that the assembled system is compliant to applicable standards of the country that the system is operated in, especially with regards to user safety and electromagnetic interference. Compliance was only tested for attached cables shorter than 3 m.

When handling the board, adequate measures have to be taken to protect the circuits against electrostatic discharge (ESD). All power supplied to the system must be turned off before installing the board.



### 6.3.3 Cooling

The **Ndigo5G** in its base configuration has passive cooling that requires a certain amount of air flow. If the case design can't provide enough air flow to the board, a slot cooler like Zalman ZM-SC100 can be placed next to the board. Active cooling is also available as an option to the board.

### 6.3.4 Environmental Conditions

See Section 6.2.2 and Section 6.2.4.

### 6.3.5 Inputs

All inputs are AC coupled. The inputs have very high input bandwidth requirements and therefore there are no circuits that provide over voltage protection for these signals. Any voltage on the inputs above **5V** or below **-5V** relative to the voltage of the slot cover can result in permanent damage to the board.

### 6.3.6 Known Bugs

The Ndigo5G does not work in most Thunderbolt PCIe extension enclosures. The reason is unknown.

### 6.3.7 Workarounds

Use **Ndigo6G** All other cronologic products work reliably in Thunderbolt enclosures. The **Ndigo6G** offers very similar functionality to the **Ndigo5G** at a higher performance. When using the Ndigo6G as a replacement, there are some software changes required in the device configuration. The readout data format and API is identical. See [www.cronologic.de/products/adcs/ndigo6g-12](http://www.cronologic.de/products/adcs/ndigo6g-12) for details.

Use Ndigo Crate Up to eight **Ndigo5G** can be used in an Ndigo Crate connected to a PC. Electrically the setup is similar to an external Thunderbolt enclosure, but the PC must have a vacant PCIe slot. See [www.cronologic.de/products/pcie/pcie-crates](http://www.cronologic.de/products/pcie/pcie-crates) for details.

All other cronologic products work reliably in Thunderbolt enclosure. Consider using an **Ndigo6G** as a replacement.

### 6.3.8 Recycling

cronologic is registered with the "Stiftung Elektro-Altgeräte Register" as a manufacturer of electronic systems with **Registration ID DE 77895909**.

The **Ndigo5G** belongs to **category 9, "Überwachungs und Kontrollinstrumente für ausschließlich gewerbliche Nutzung"**. The last owner of an **Ndigo5G** must recycle it, treat the board in compliance with **§11** and **§12** of the German ElektroG, or return it to the manufacturer's address listed in [Section 6.3.1](#).

### 6.3.9 Export Control

The **Ndigo5G** product line is a dual use item under [Council Regulation \(EC\) No 428/2009 of 5 May 2009 setting up a Community regime for the control of exports, transfer, brokering and transit of dual-use items in section 3A002h](#). Similar regulations exist in many countries outside Europe.

An export permit is required to export this product from the European Community (EC) which will cause additional lead time. When ordering from outside the EC, the seller will ask you for additional information needed to obtain this permit.

Before reexporting an **Ndigo5G** or any product containing an Ndigo5G as a component please check your local regulations whether an export permit is required.

## 7 Revision History

### 7.1 Firmware

Revision	Date	Comments
1.4865	2015-07-28	Internal optimizations
1.4824	2015-02-27	Fixed intel PCIe link training issues

### 7.2 Driver & Applications

Revision	Date	Comments
1.4.3	2019-10-21	Fixed a card initialization error in x64 32 mode
1.4.0	2019-06-04	Added Windows 10 support
1.3.0	2017-06-08	NdigoScope application now supports Ndigo250M-14

### 7.3 User Guide

Revision	Date	Comments
1.1.0	2019-08-27	API clarifications