
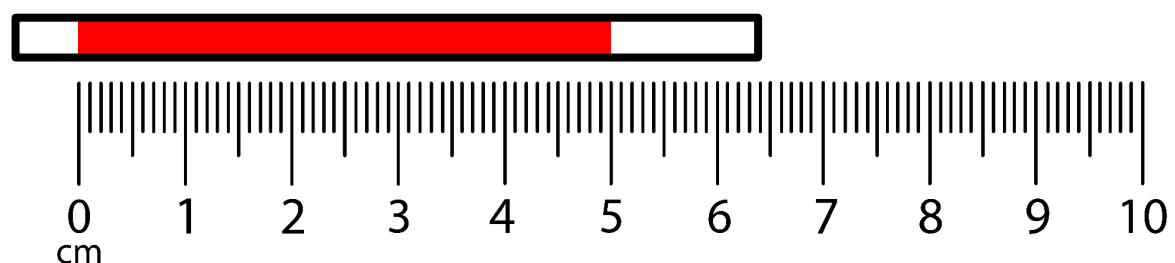




Field sampling & laboratory analysis

Measure volume of blood sample in capillary tube following venipuncture

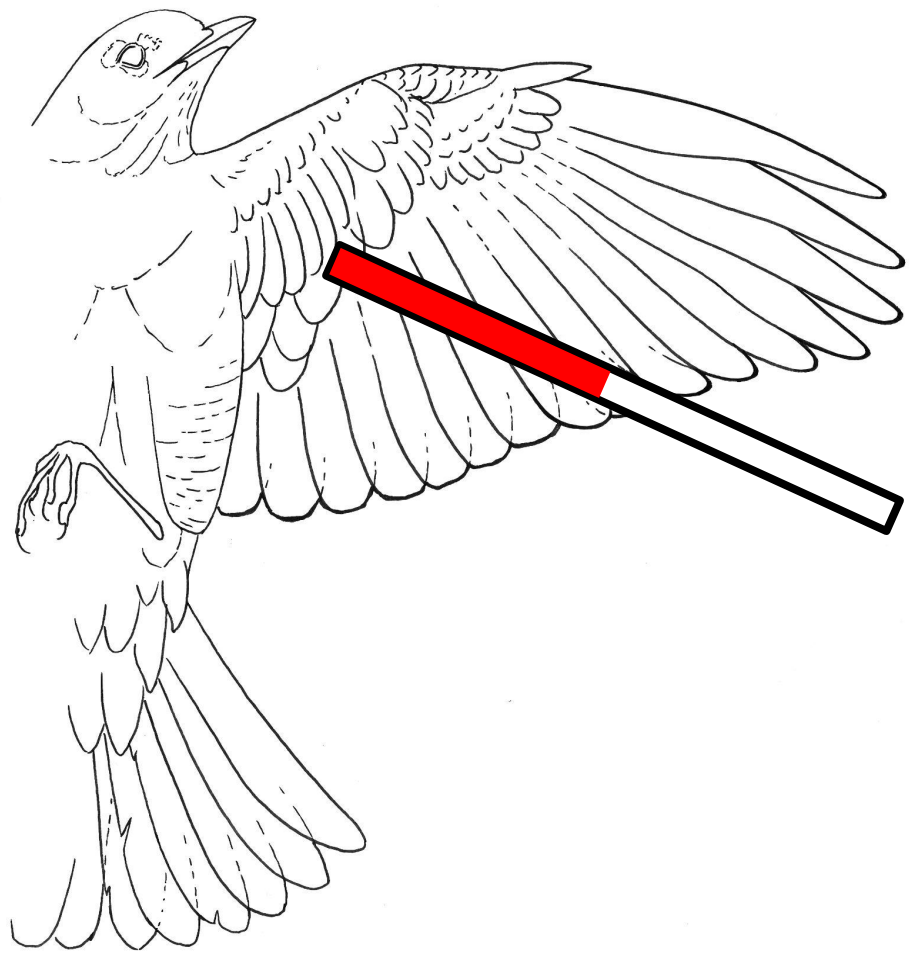


Length (mm) = Volume (μL)
50 mm = 50 μL

Create dried blood spot on filter paper card and extract for Hg analysis

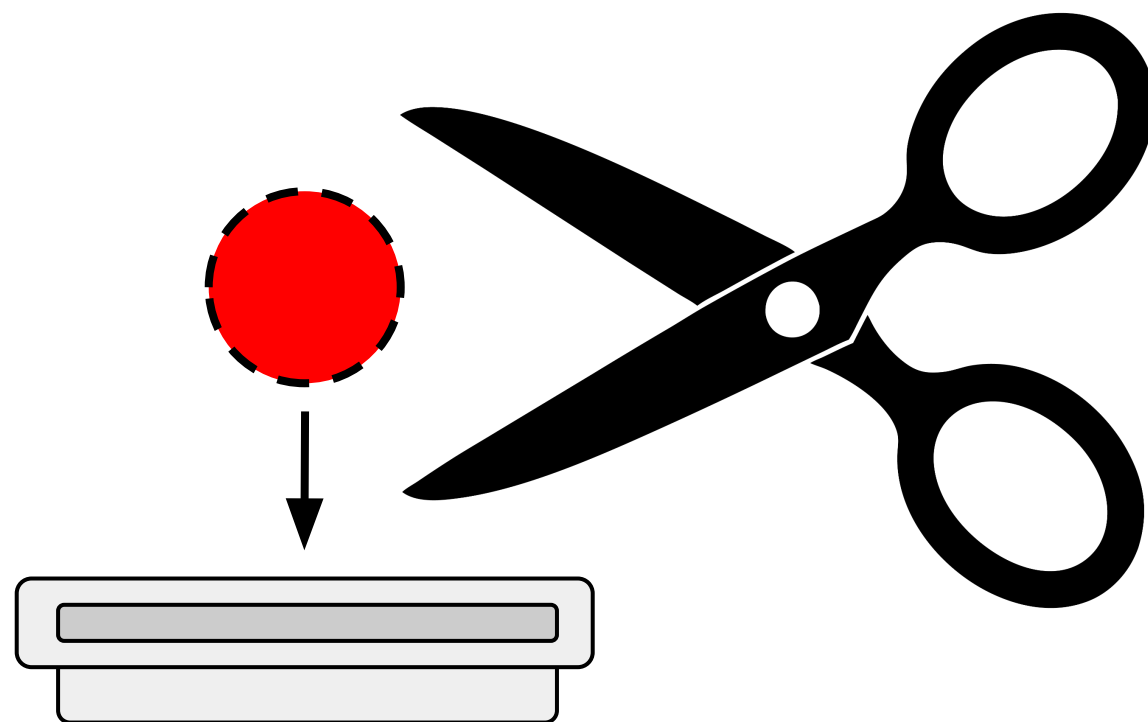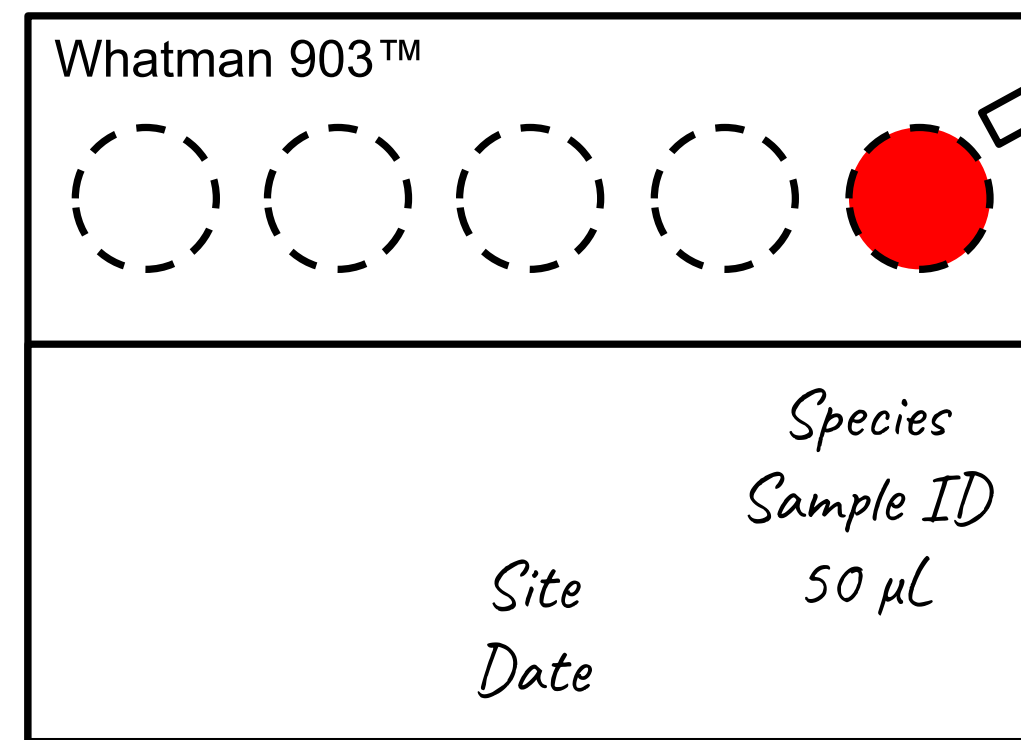


Validation

Bayesian error-in-variables
linear regression of paired samples

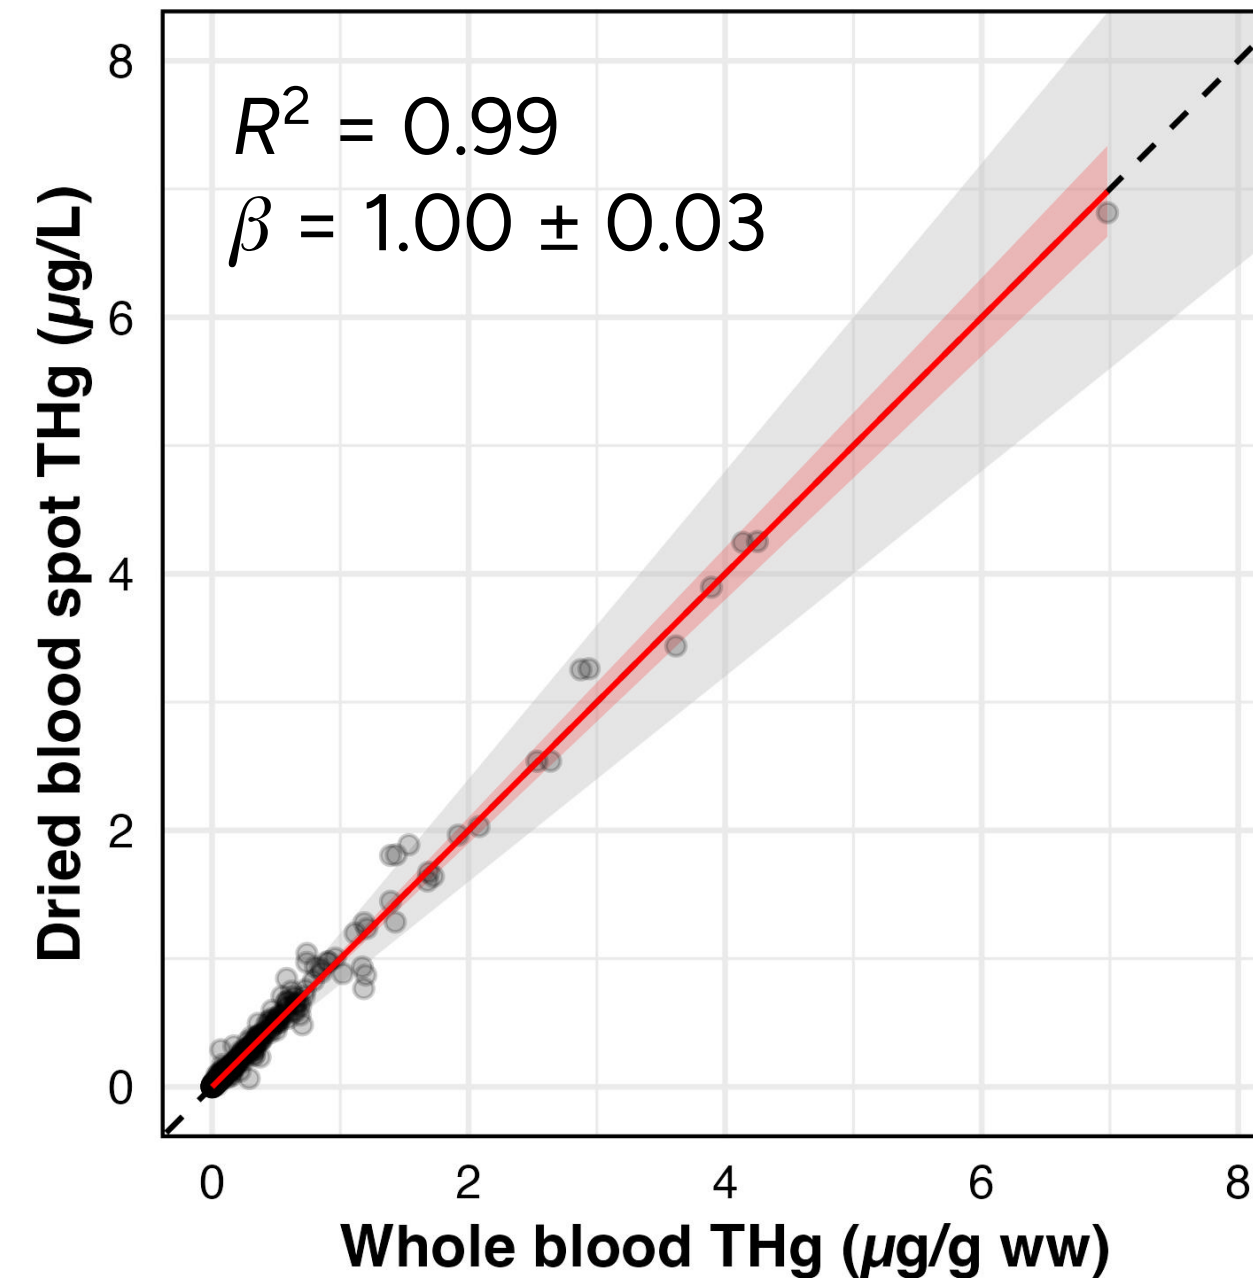

Conclusions

Dried blood spots...



Can be stored at
ambient temperatures





Are less expensive &
reduce operational costs



Allow variably sized blood
draws for animal welfare




Are practical & reliable in
remote field conditions

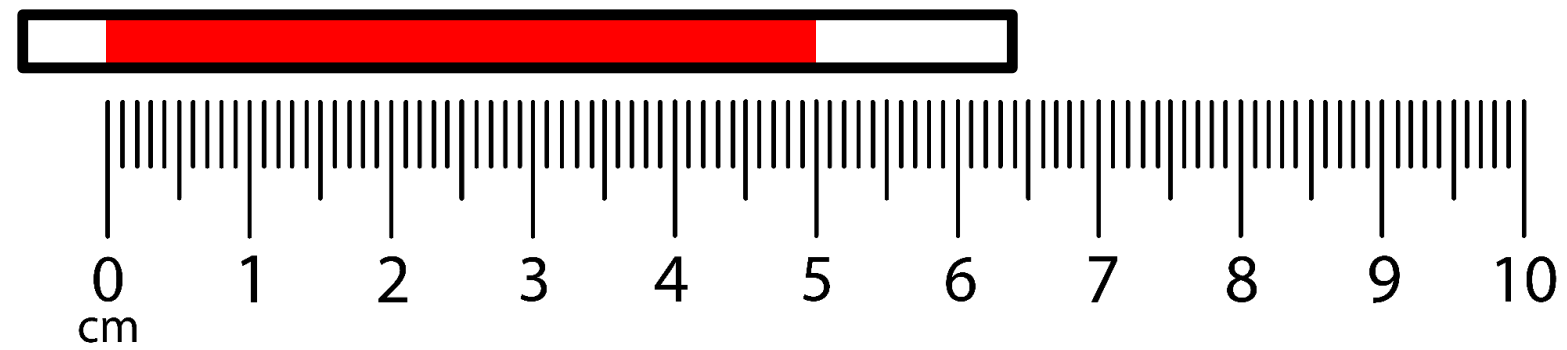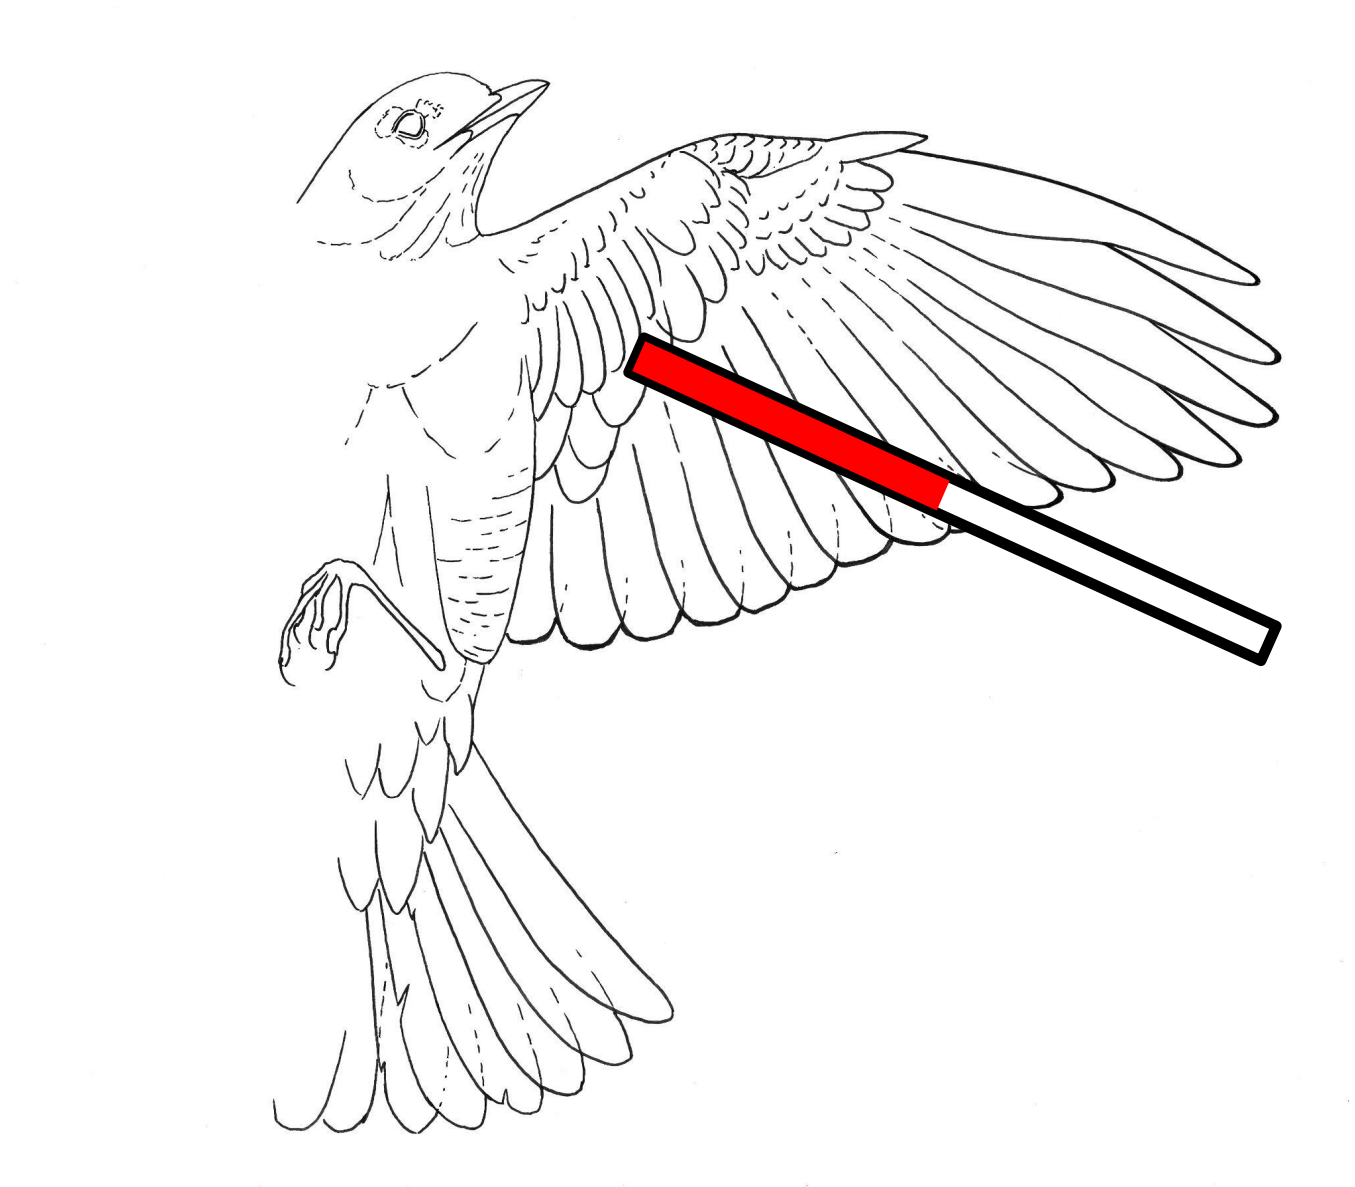

50 mm = 50 μ L

Whatman 903™				
			Species	
			Sample ID	
			50 μ L	
Site				
Date				

(1) Measure volume of blood sample in the field

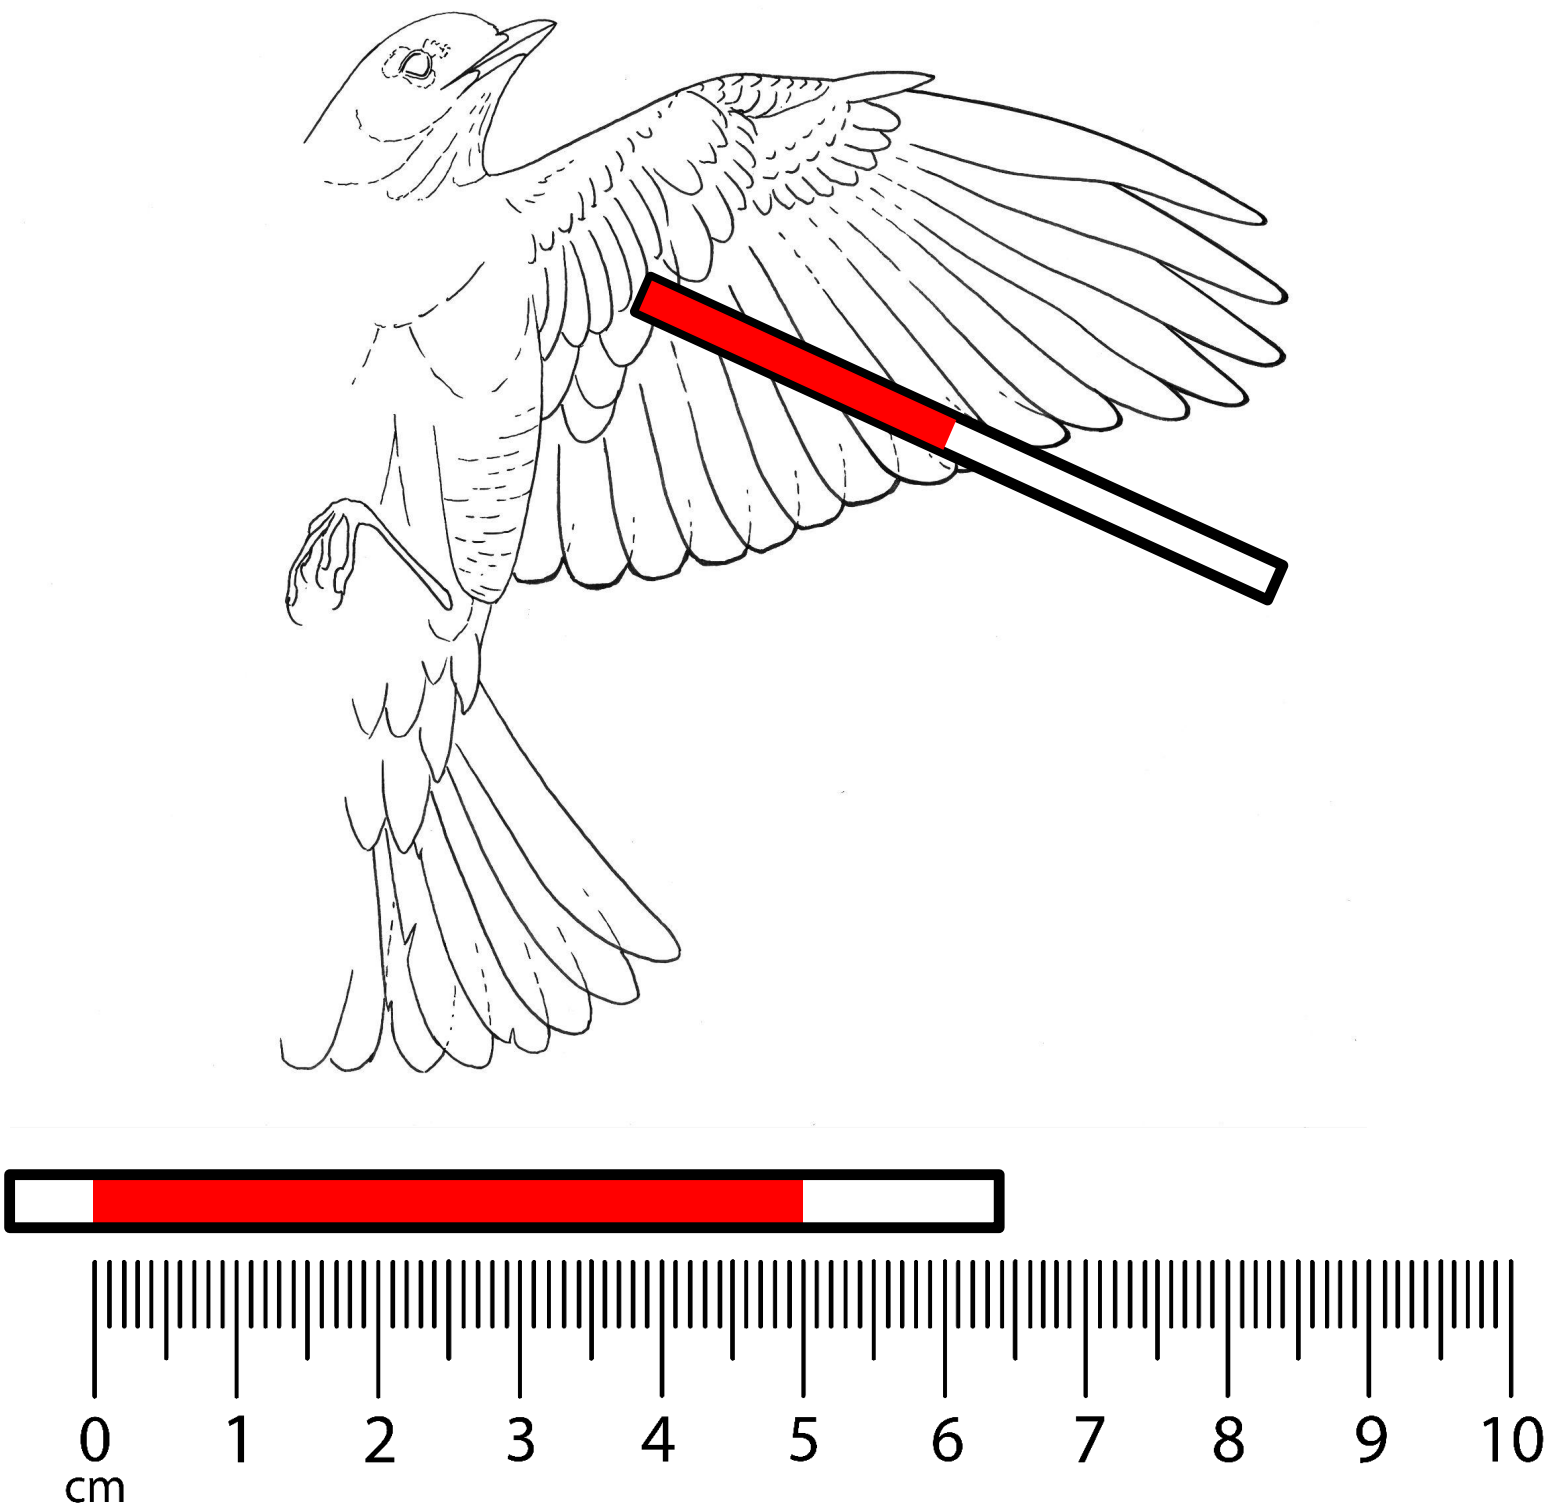

Length (mm) = Volume (μL)
50 mm = 50 μL

Create dried blood spot onto filter paper card


Whatman 903™



Site Date

Species Sample ID

50 μL

Create dried blood spot onto filter paper card

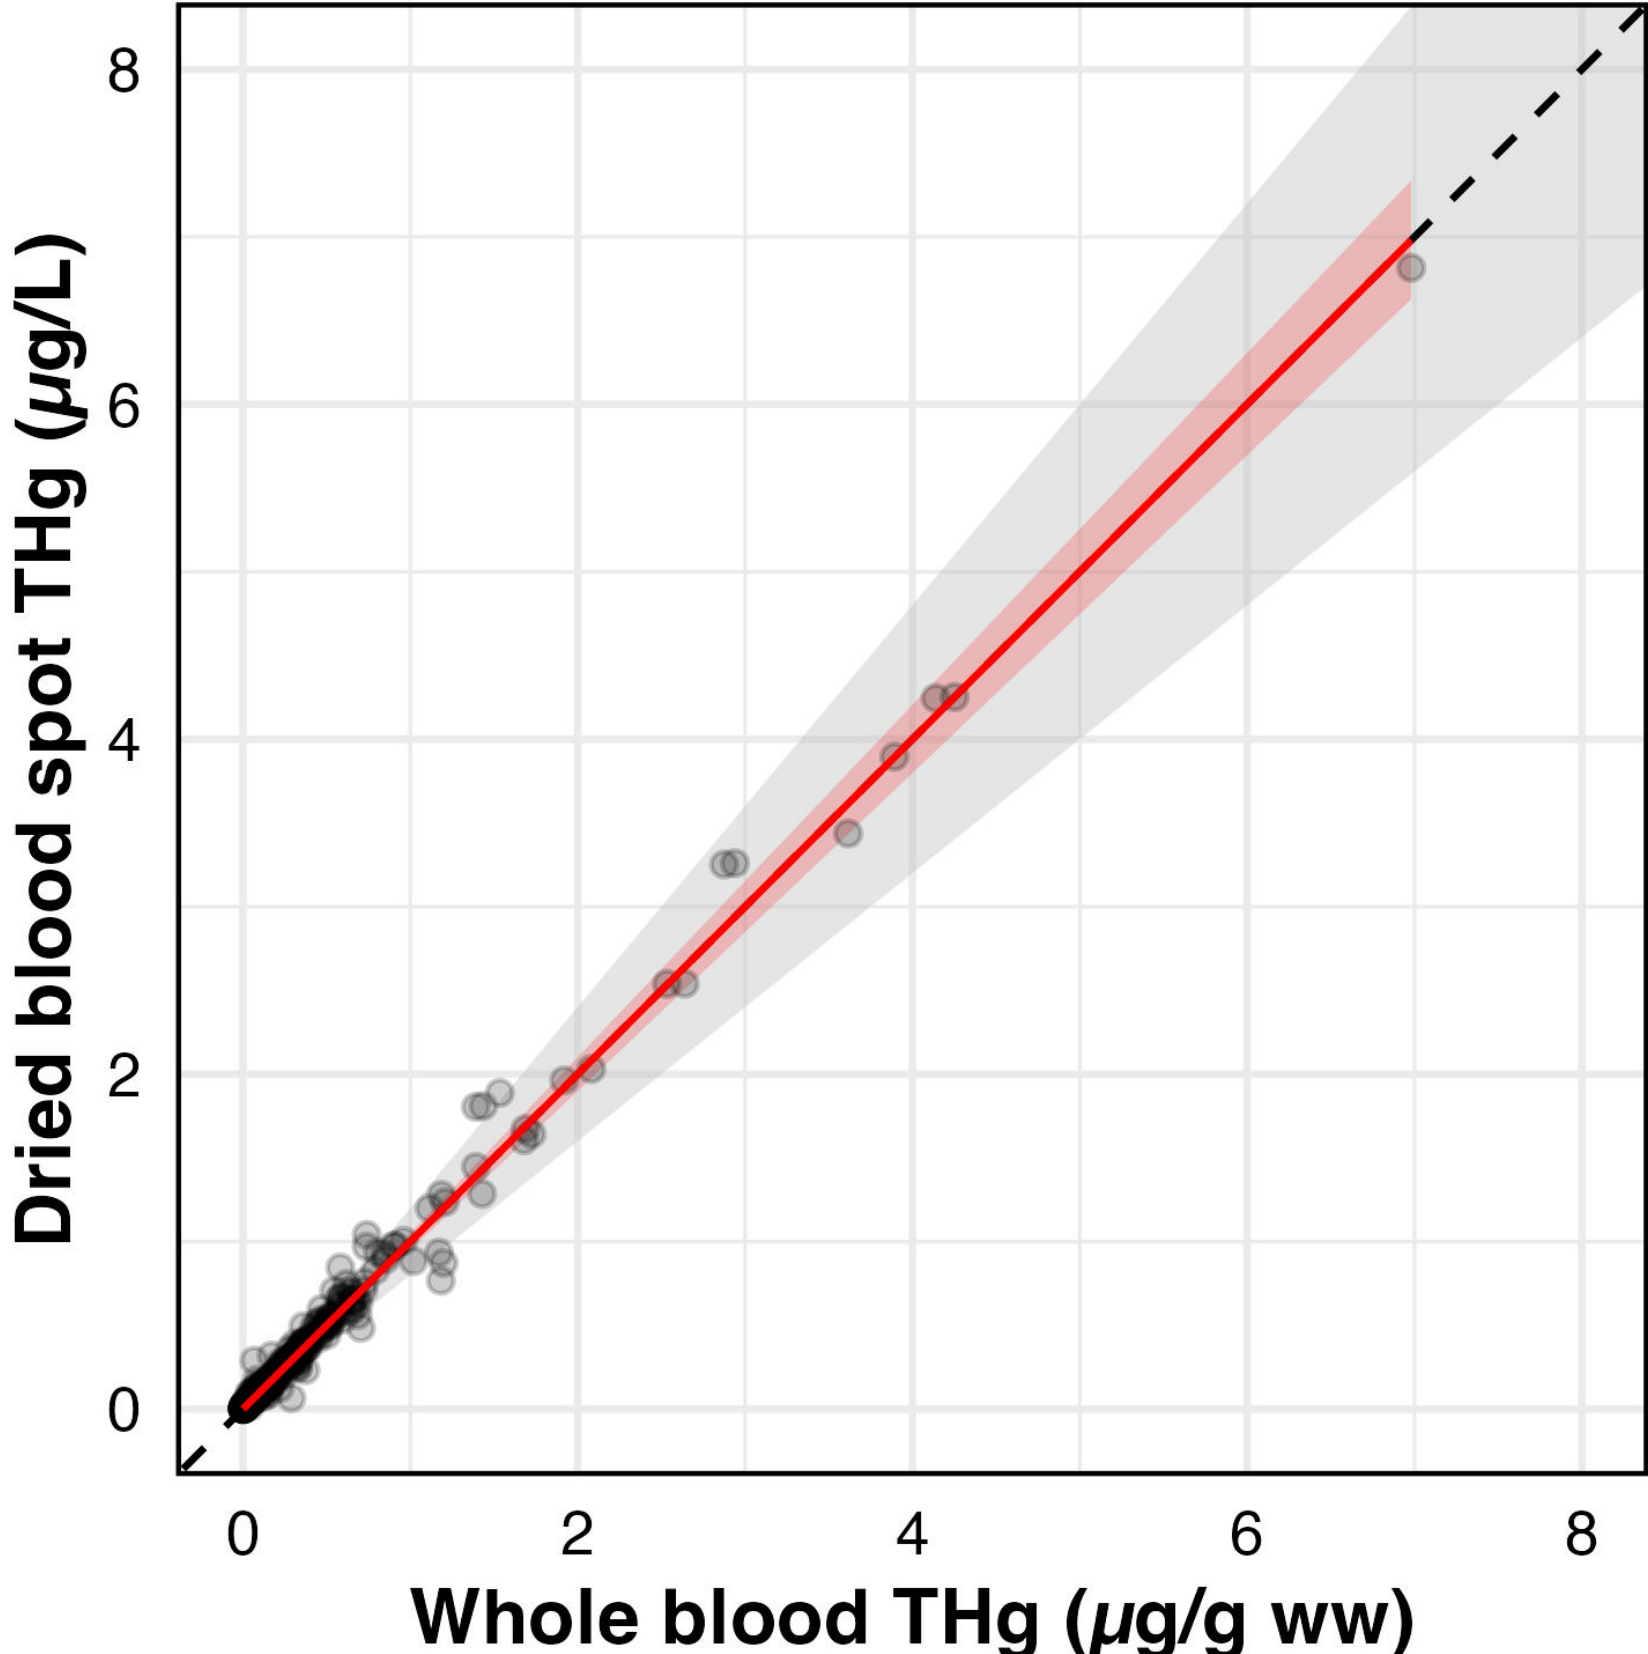

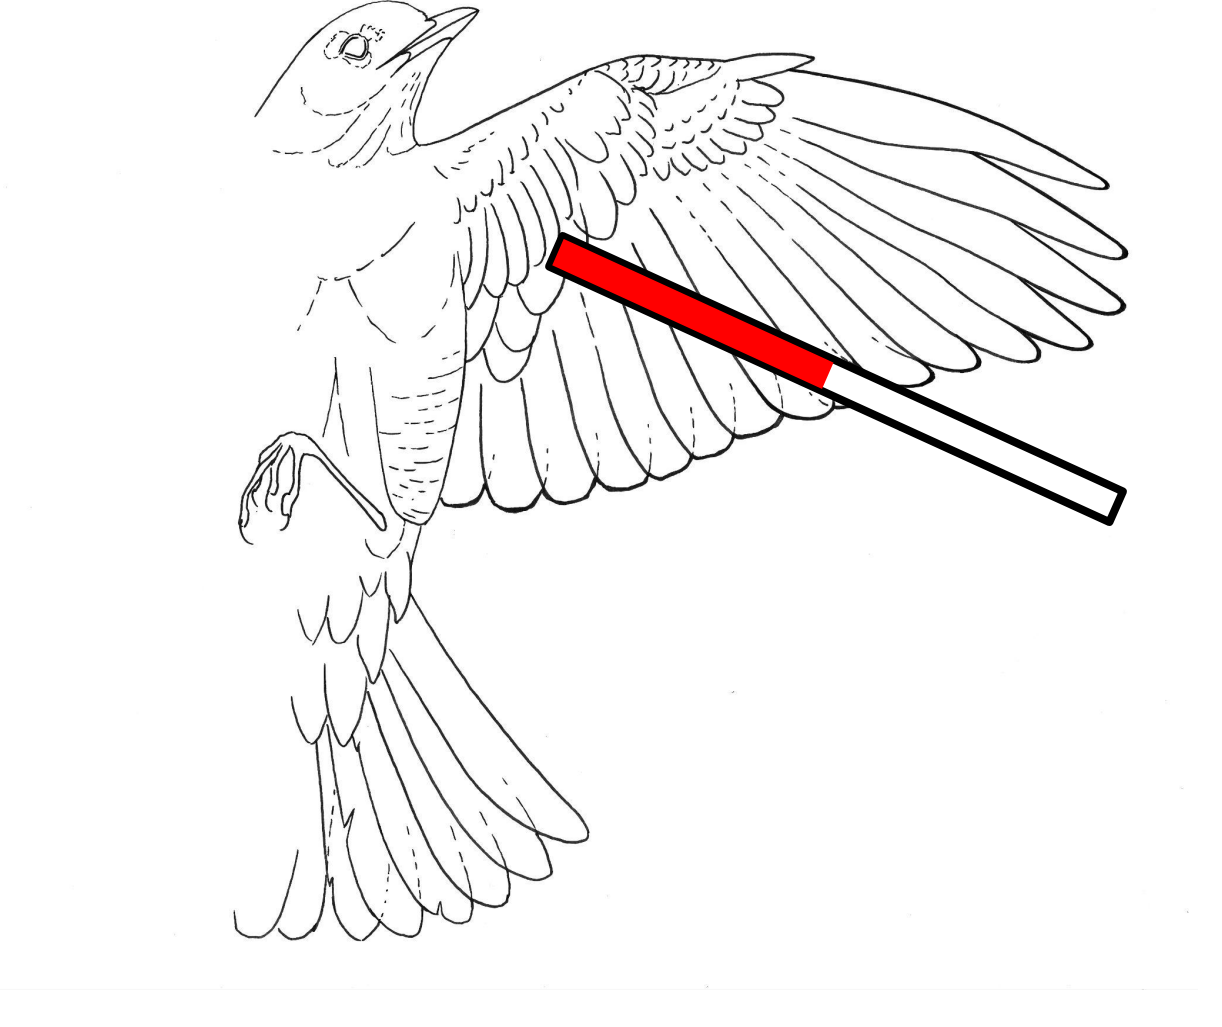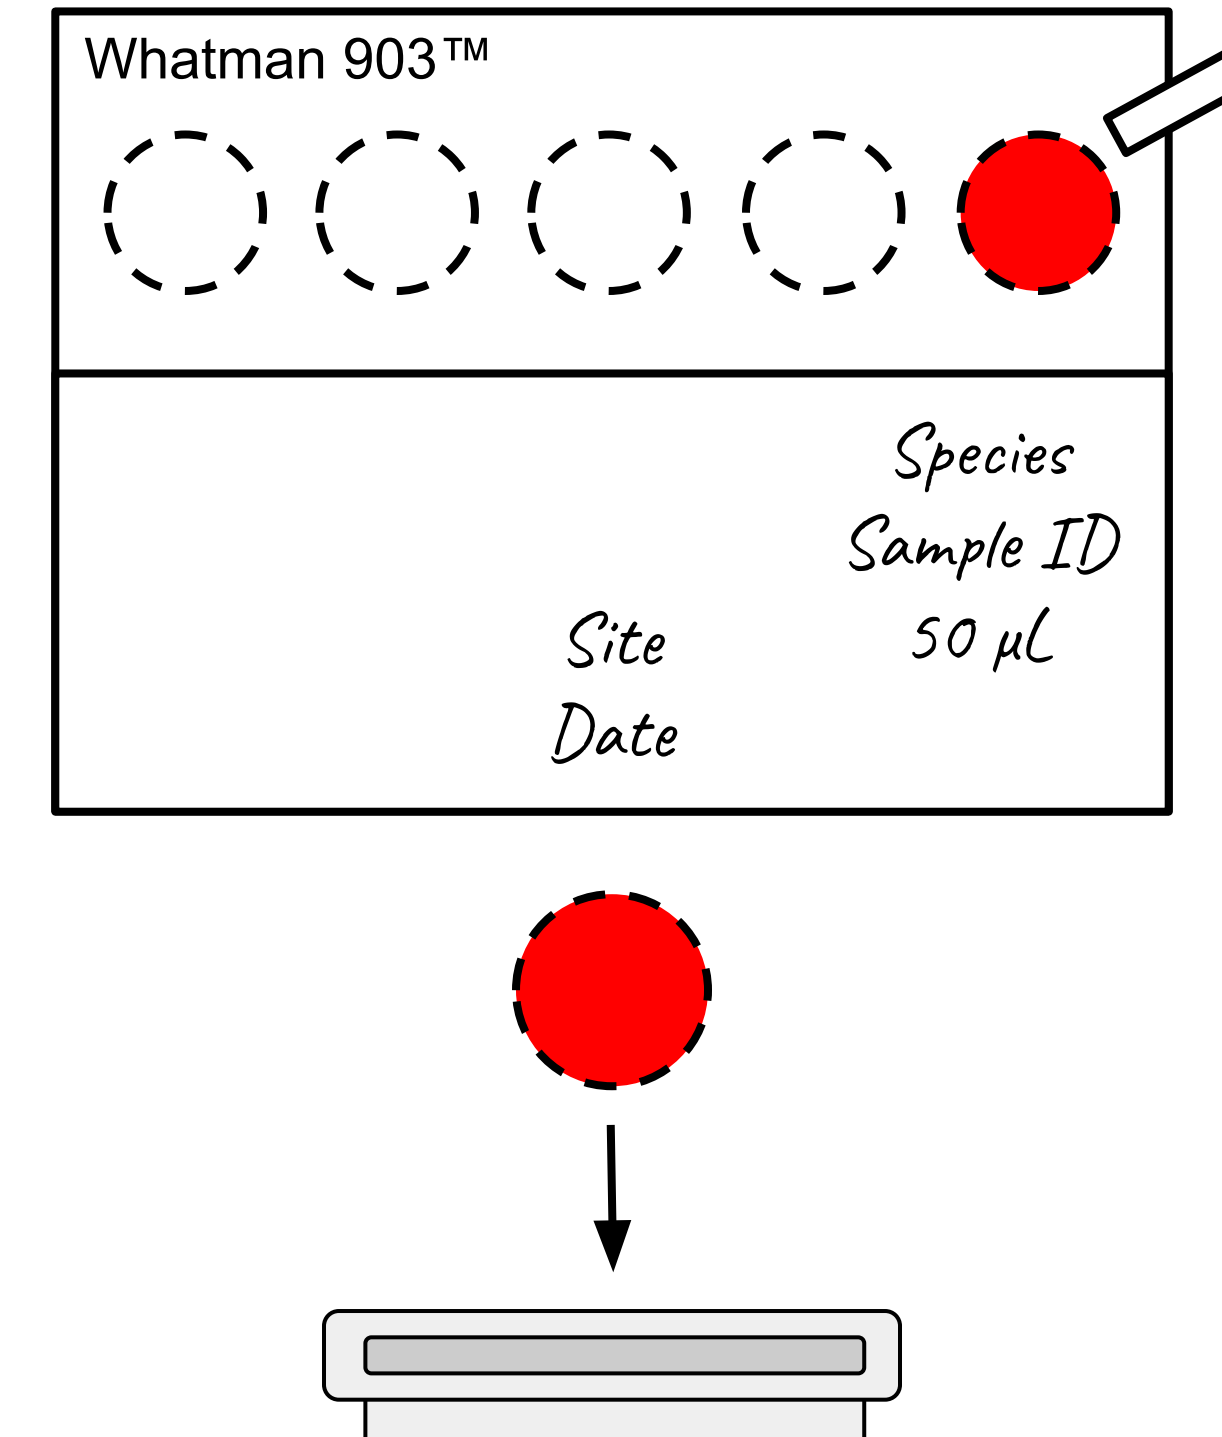Field sampling	Laboratory analysis	Validation	Conclusions
Measure volume of blood sample in capillary tube following venipuncture  Length (mm) = Volume (μL) 50 mm = 50 μL	Create dried blood spot on filter paper card and extract for Hg analysis 	Bayesian error-in-variables linear regression 