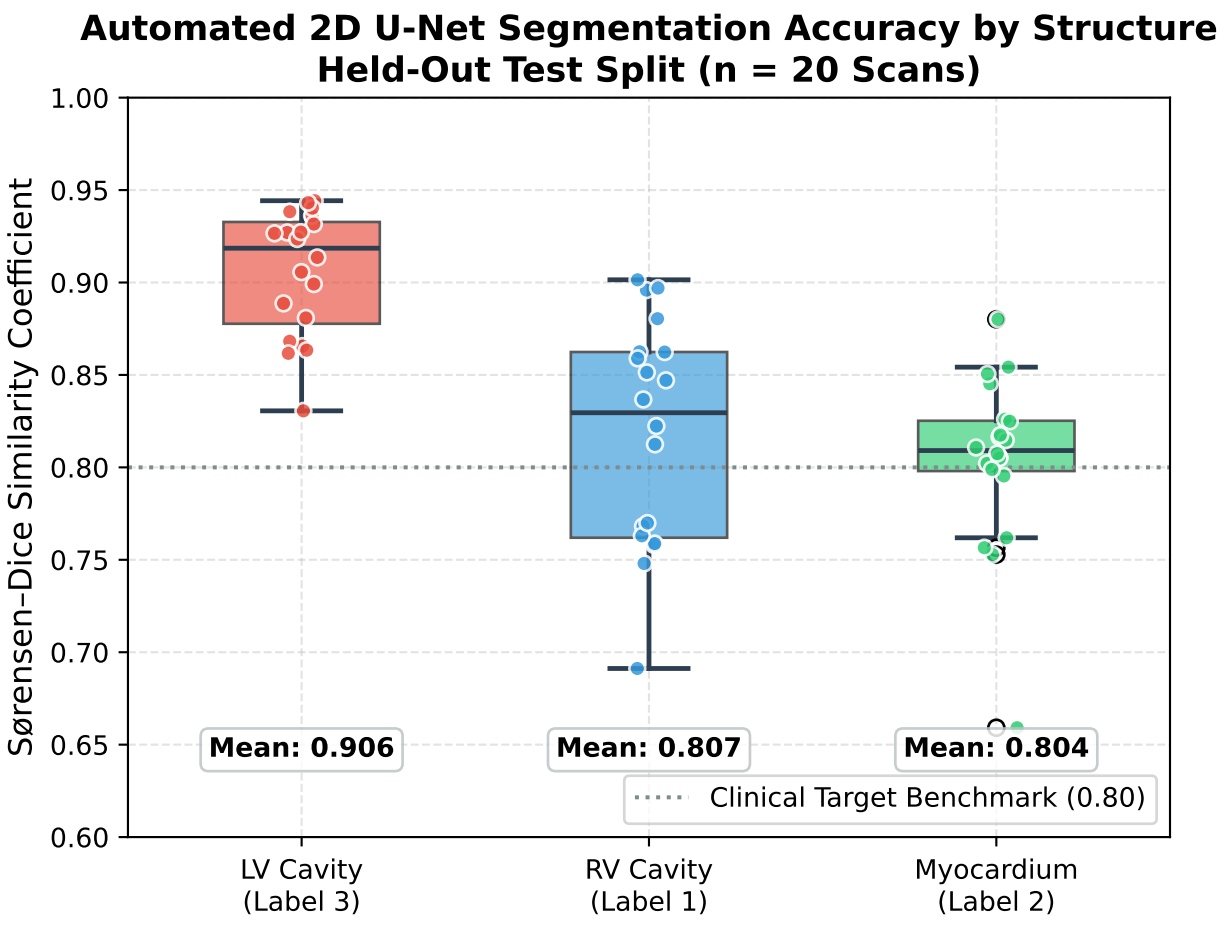
Automated 2D U-Net Segmentation Accuracy by Structure
Held-Out Test Split (n = 20 Scans)
Sørensen–Dice Similarity Coefficient
1.00
0.95
0.90
0.85
0.80
0.75
0.70
0.65
0.60
Mean: 0.906
Mean: 0.807
Mean: 0.804
Clinical Target Benchmark (0.80)
LV Cavity
(Label 3)
RV Cavity
(Label 1)
Myocardium
(Label 2)