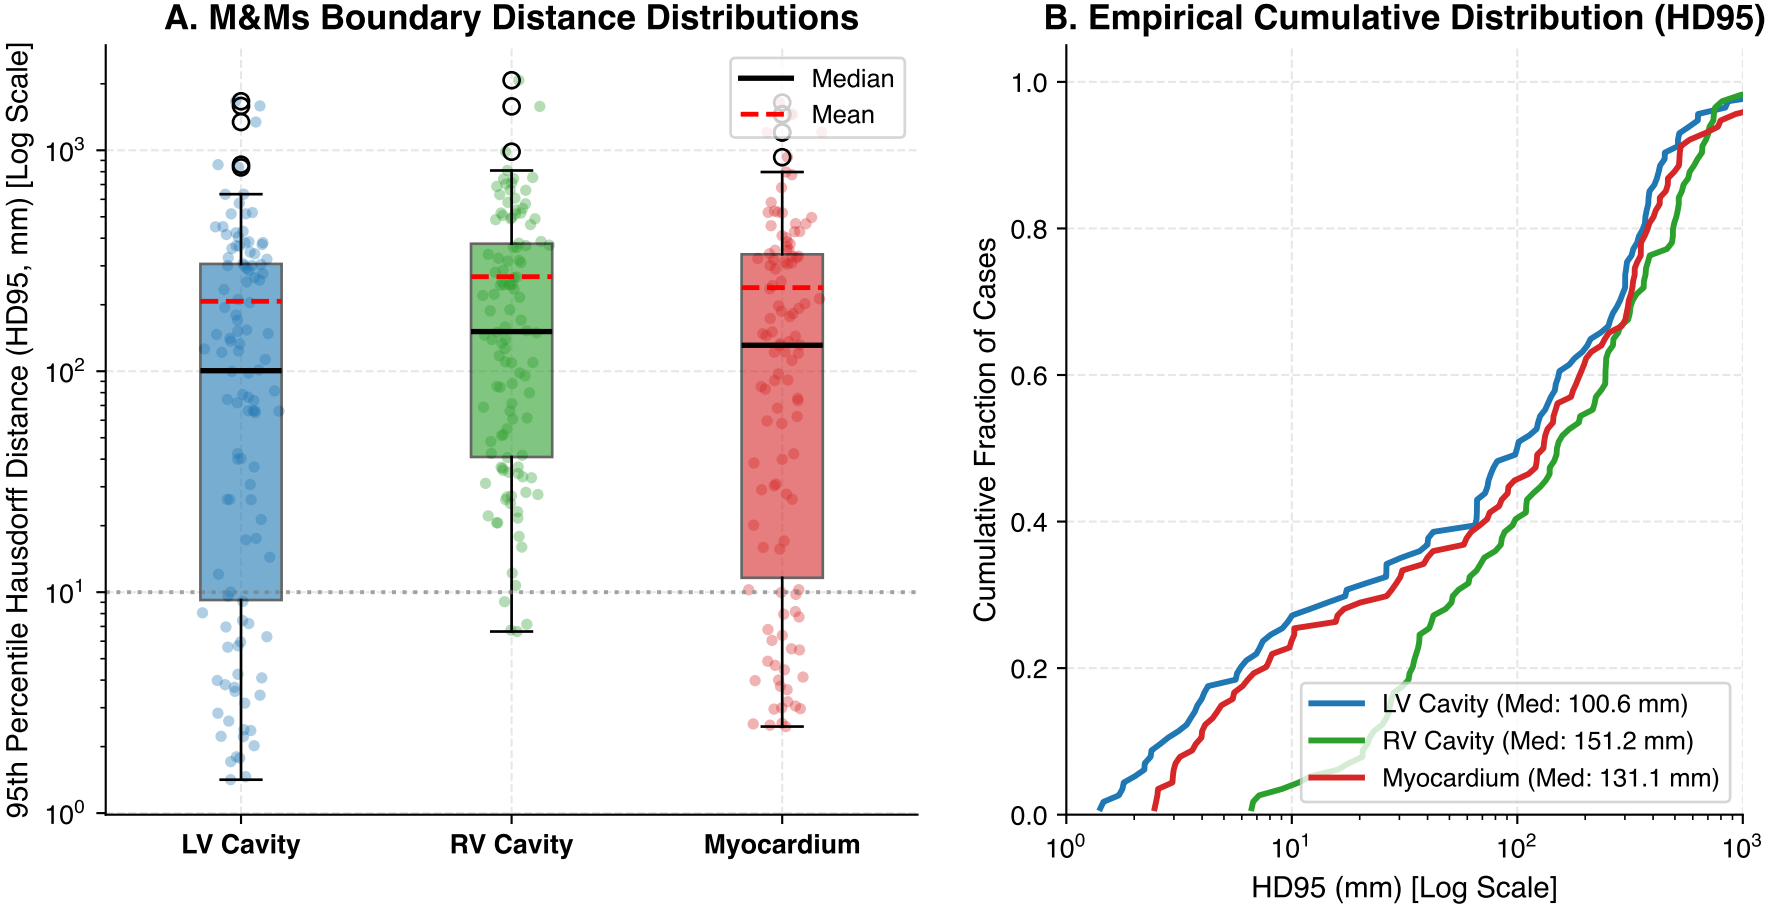

Figure 2: M&Ms External Boundary Surface Distances (N=114). Outliers (>100mm) reflect false-positive basal/apical slice components.
Medians: LV = 100.6 mm, RV = 151.2 mm, Myo = 131.1 mm.