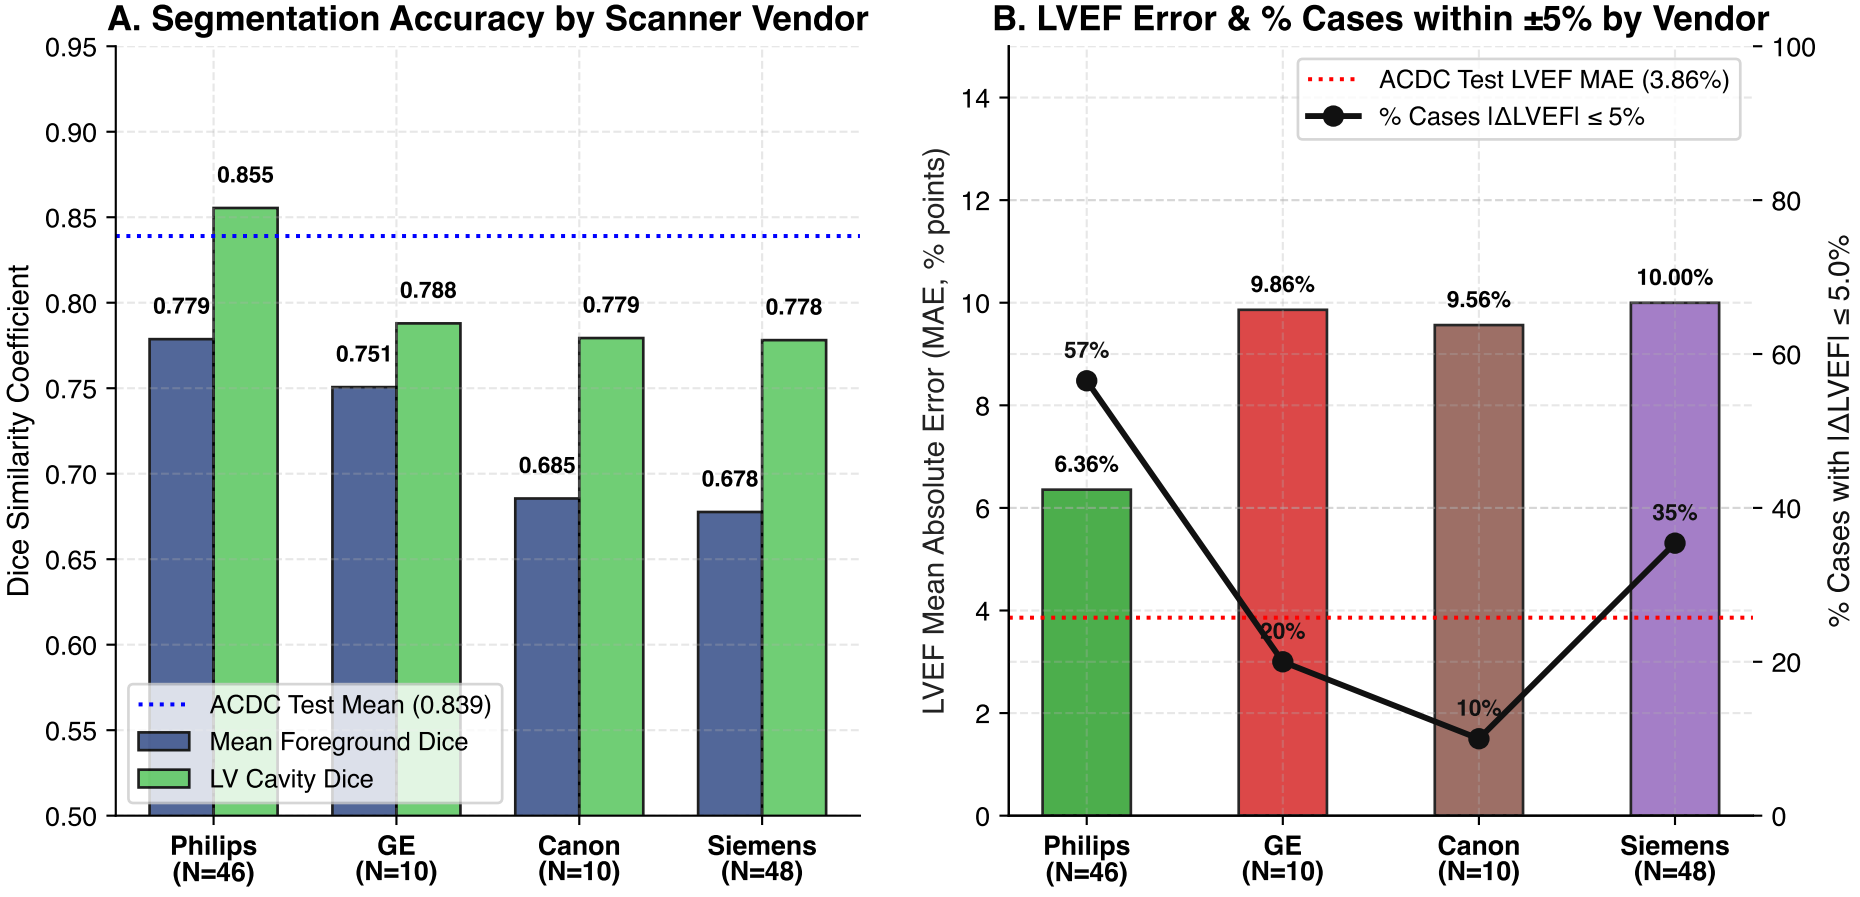

Figure 3: Performance breakdown across 4 MRI vendors. Philips demonstrates highest out-of-domain transfer (Mean DSC 0.779, LVEF MAE 6.36%). Siemens exhibits lower RV accuracy (DSC 0.618) likely due to slice thickness and coil profile differences from ACDC.