

Device: Evera MRI™ XT DR DDMB1D4

Serial Number: PFZ214965H

Date of Interrogation: 19-Jun-2025 19:55:18


Patient: PETERSON, MURPHY

Physician: Anthony Johnson 717-217-6944

History: Primary Prevention, AT/AF + Normal Sinus, Normal AV Conduction, NYHA Class II

Device Status (Implanted: 29-Aug-2016)

Remaining Longevity 19 months (19-Jun-2025)



(based on initial interrogation)

	Atrial(5076)	RV(6935M)
Pacing Impedance	456 ohms	399 ohms
Defibrillation Impedance		RV=71 ohms
Capture Threshold	0.750 V @ 0.40 ms	0.750 V @ 0.40 ms
Measured On	19-Jun-2025	19-Jun-2025
Programmed Amplitude/Pulse Width	1.50 V / 0.40 ms	2.00 V / 0.40 ms
Measured P/ R Wave	0.8 mV	6.3 mV
Programmed Sensitivity	0.15 mV	0.30 mV

Parameter Summary

Mode	AAI<=>DDD	Lower Rate	60 bpm	Paced AV	180 ms
Mode Switch	171 bpm	Upper Track	130 bpm	Sensed AV	150 ms
		Upper Sensor	130 bpm		

Detection		Rates	Therapies
AT/AF	Monitor	>171 bpm	All Rx Off
VF	On	>200 bpm	ATP During Charging, 35J x 6
FVT	via VF	200-231 bpm	Burst(3), 25J, 35J x 4
VT	OFF		All Rx Off

Enhancements On: VT Monitor, AF/Afl, Sinus Tach, Wavelet, TWave, Noise(Timeout)

Clinical Status Since 28-Mar-2025 Cardiac Compass Trends (Apr-2024 to Jun-2025)
Treated


VF	0
FVT	0
VT (Off)	
AT/AF(Monitor)	

Monitored

VT (140-200 bpm)	0
VT-NS (>4 beats, >200 bpm)	0
High Rate-NS	0
SVT: VT/VF Rx Withheld	0
V. Oversensing-TWave Rx Withheld	0
V. Oversensing-Noise Rx Withheld	0
AT/AF	0
Time in AT/AF	<0.1 hr/day (<0.1%)

Functional

Patient Activity	Last Week
	0.7 hr/day

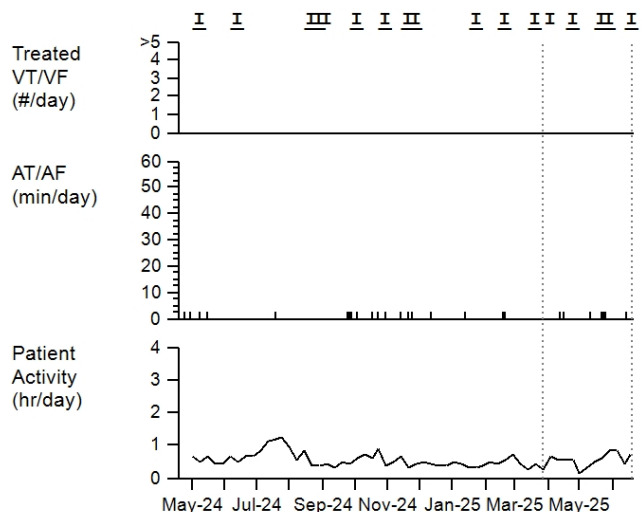

Therapy Summary	VT/VF	AT/AF	Pacing	(% of Time Since 28-Mar-2025)
Pace-Terminated Episodes	0	0	Total VP	0.2% (MVP On)
Shock-Terminated Episodes	0	0	AS-VS	90.2%
Total Shocks	0	0	AS-VP	0.1%
Aborted Charges	0	0	AP-VS	9.6%