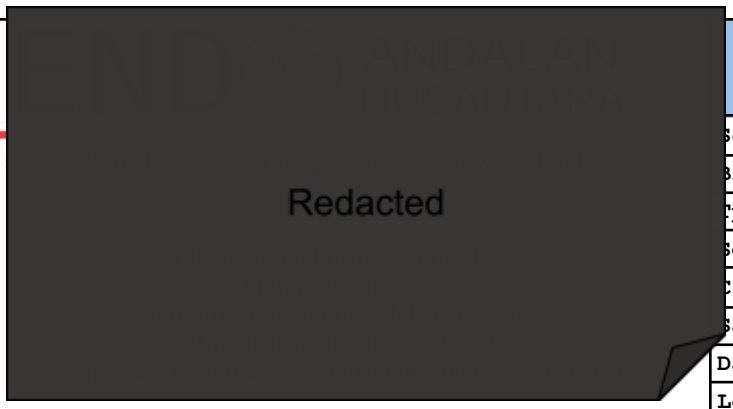


Evaluation Report

Incoming Technical Report

Scope Type	Flexible Scope
Brand/Product No.	OLYMPUS
Type	BF-H190
Serial No.	[redacted]
Client	[redacted]
Sales Person	
Date	[redacted]
Location	[redacted]

Complaint		
Leak Test	Yes	No ☐
Sterilizers	Yes	No ☐
Additional Report	Image Static, IT Buckle, CB Leak, EL Housing Leak and rust, Light Dim, Snaking	

#	ENDOSCOPE ANATOMY	TEST (Ok/Failed)	DESCRIPTIONS	#	ENDOSCOPE ANATOMY	TEST (Ok/Failed)	DESCRIPTIONS
1	Bending Rubber	F		19	Suction Channel	OK	
2	Distal Head	OK		20	Switch Electrical 1,2,3,4	OK	
3	Nozzle Air/Water	N/A		21	Stress Rubber Booth #2	OK	
4	Camera Lens	OK	Scratched	22	Light Guide Tube	OK	
5	Light Guide Lens	OK	Scratched / Dim	23	Stress Rubber Booth #3	OK	
6	Biopsy Channel	F	Leak	24	Electrical Housing	F	Leak, Rust
7	Bending Section	OK		25	Electrical Pin Unit	OK	
8	Insertion Tube	F	Buckle	26	Light Guide Prong	OK	
9	Stress Rubber Booth #1	OK		27	Auxiliary Water Inlet/Jet	N/A	
10	Biopsy Inlet Port	F	Leak	28	Tensioner	N/A	
11	Control Body	F	Leak	29	Camera CCD/NBI/Eyescan	F	Static
12	Angulation Up	OK	-30°		**ERCP**		
13	Angulation Down	OK	-20°	1	Elevator Lever		
14	Angulation Left	N/A		2	Channel Elevator		
15	Angulation Right	N/A		3	Actuator Arm		
16	Brake U/D	N/A			**FIBER**		
17	Brake L/R	N/A		1	Fiber Image		
18	Air/Water Channel	N/A		2	Ocular Tower		

Service Contract	Yes	☐ No	Contract Number :
Customer Visit Record			
Accessories Included in the Box	Box Alat, Suction Valve, Biopsy Cap		
Person in Charged for Repair			
Department			
Pre-Approval for Repair Bellow			

	P.I.C	Sales Technician
Minor Repair *		
Medium Repair *		
Major Repair * + CCD		
Overhaul Repair *	(NN)	A , M

Redacted

Evaluation Report

Incoming Technical Report

Scope Type	Flexible Scope
Brand/Product No.	OLYMPUS
Type	BF-H190
Serial No.	[redacted]
Client	[redacted]
Sales Person	
Date	[redacted]
Location	[redacted]


Pic 1 - Biopsy Inlet Leak




Pic 2- Electric Housing Leak




Pic 3 - Electric Housing Corrosion

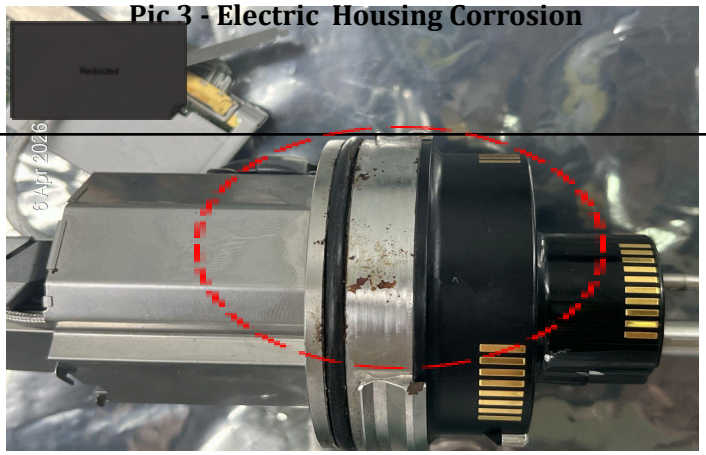

Pic 4 - Insertion Tube Buckle

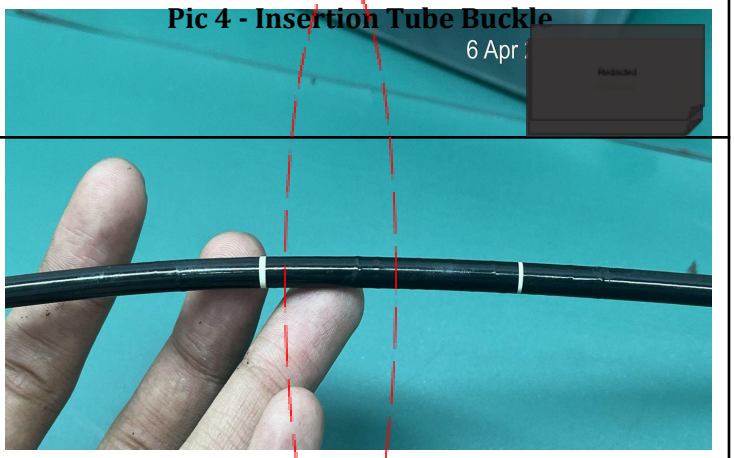

Pic 5- Image Static

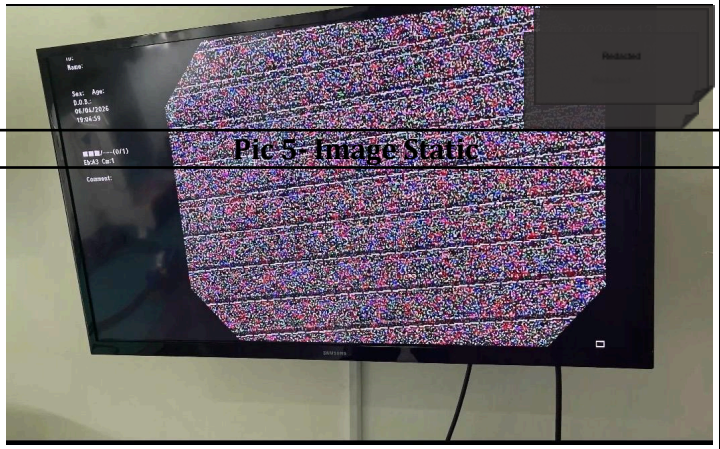

Pic 6- Control Body Leak

