Sunburst Sensors, LLC
1226 W Broadway Ave
Missoula, MT 59802
+1 406 532 3247

SAMI^2 CO_2 Calibration Certificate February 11, 2025

Serial Number:	C0062
Board Version:	E Board
Technician:	BW
Reagent:	606
Reagent Remaining:	65%

Table 1: SAMI^2 CO_2 calibration parameters.

A	B	C	K_{434}	K_{620}	T_{avg}	Range (ppm)
0.0636	0.5328	-1.4839	1.0248	1.1558	8.9474	201–1996

Table 2: Blank intensities.

Source	Reference	Signal
Dark	45	34
434 nm	3083	3149
620 nm	2691	3094

Build Notes

Pressure Test: 200 psi

Modifications:

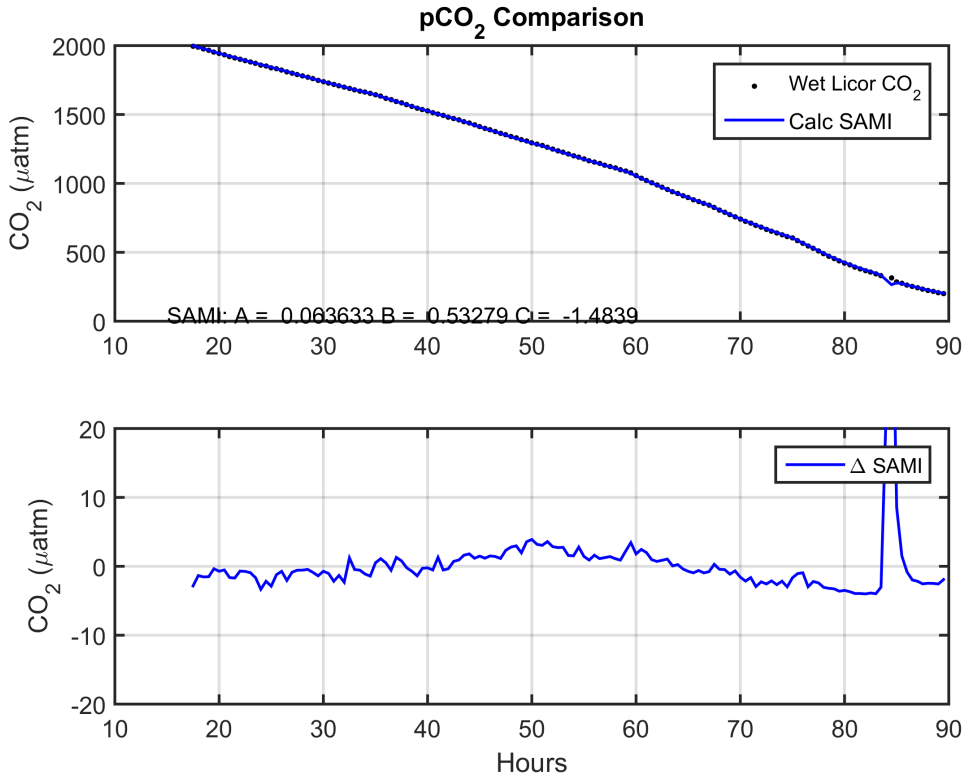
65

standard refurb

IR testing

2x sem filters

ext cal


pCO2 Comparison
Wet Licor CO2
Calc SAMI
SAMI: A = 0.063633 B = 0.53279 C = -1.4839
CO2 (μatm)
Δ SAMI
Hours