

Spectrometer Mount

- Allows Spectrometers to be mounted.
- Slips on the Sensor Housing four outer Posts. Requires the Electronics Housing to be modified by trimming the four outer posts by 0.15in (circled in red in Image 2).
- One Spectrometer Mount per sensor. Same mount works for both.
- The Spectrometer Mount should be printed using PETG or similar material

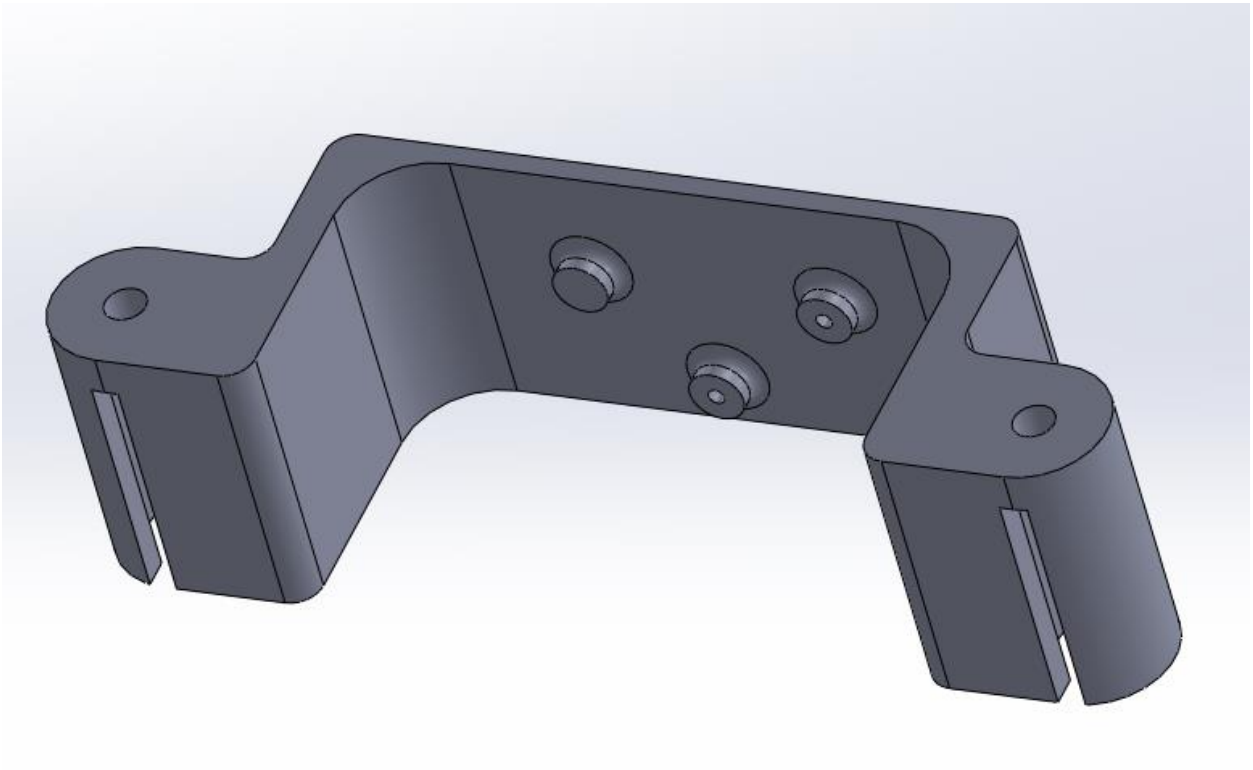


Image 1



Image 2