


REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS




TOP

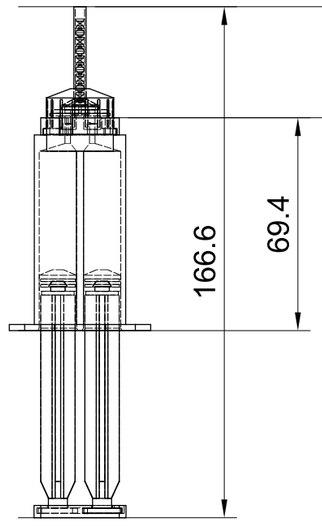

FRONT



RIGHT

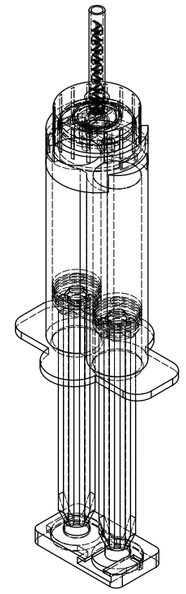


ISOMETRIC (0.65:1)


NOTES: 1. TOLERANCES PER ISO 2768-m UNLESS OTHERWISE SPECIFIED.
2. STERILIZATION: ETO OR GAMMA COMPATIBLE.
3. BARREL CAPACITY: 2 X 4.0 ML WORKING (5.0 ML MAX).
4. POKA-YOKE BAYONET PREVENTS 180-DEG MIS-ASSEMBLY.

DUAL/SINGLE-BARREL SEALANT MIXING DEVICE - DISPENSE ASSY	SCALE 1:2 MM THIRD ANGLE
CSL-ASSY-001 · MEDICAL COC / PP / SILICONE · ANTIGRAVITY CAD	SHEET 1 OF 12 REV B coseal_engineering_drawings


REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS

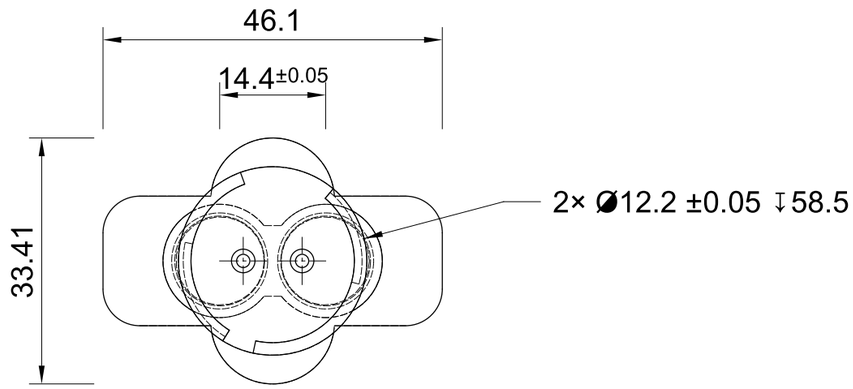


TOP

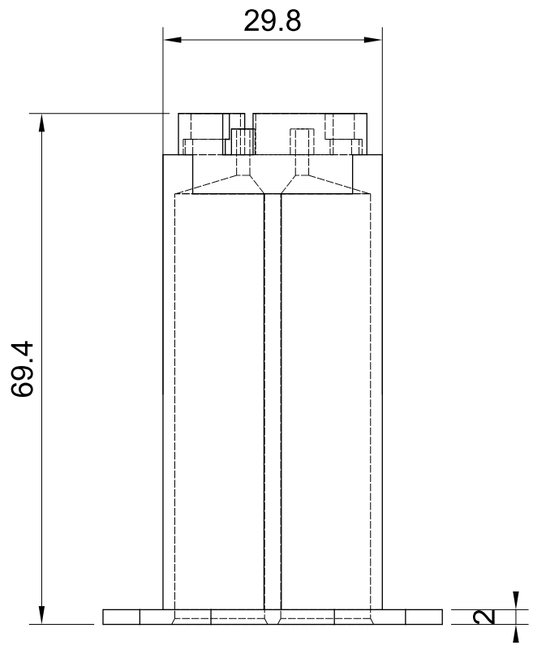

FRONT

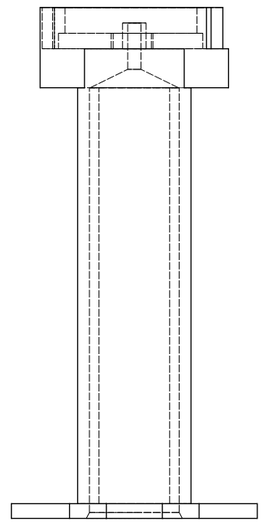

RIGHT

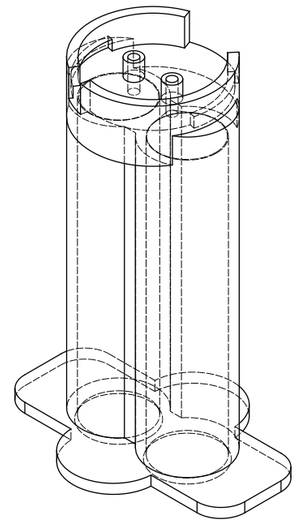


ISOMETRIC (1.1:1)


NOTES: 1. TOLERANCES PER ISO 2768-m UNLESS OTHERWISE SPECIFIED.
2. ASYMMETRIC BAYONET GAPS: +Y 60 DEG / -Y 20 DEG.
3. INTERNAL BORE SURFACE FINISH Ra <= 0.4 um.
4. NOZZLE BORE PITCH 8.00 +-0.03 MM; OD 3.20 / ID 1.80.

DUAL-BARREL SYRINGE BODY (POKA-YOKE BAYONET)	SCALE 1.2:1 MM THIRD ANGLE
CSL-PRT-101 · MEDICAL GRADE PP / COC (CLEAR) · ANTIGRAVITY CAD	SHEET 2 OF 12 REV B coseal_engineering_drawings


REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS

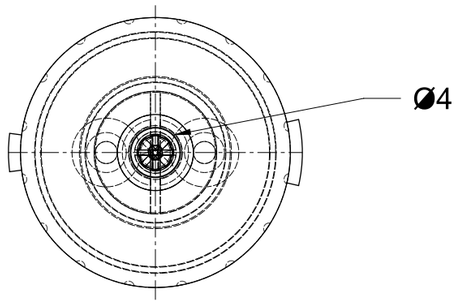


TOP

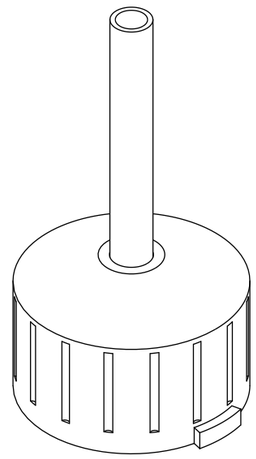

ISOMETRIC 1.76:1

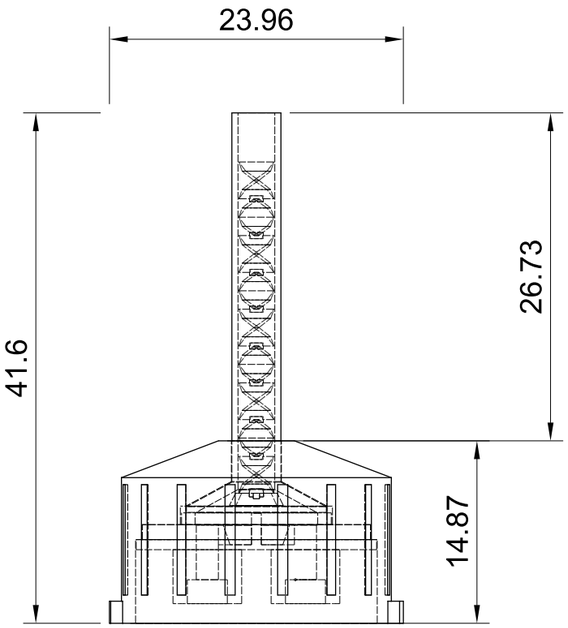

FRONT

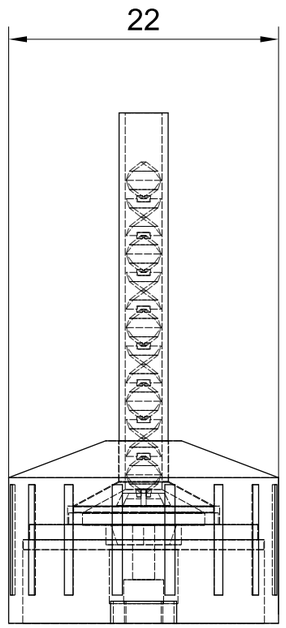


RIGHT


NOTES: 1. TOLERANCES PER ISO 2768-m UNLESS OTHERWISE SPECIFIED.
2. 4-PART SUBASSEMBLY: CAP + SEAL + 1-PC BELL TUBE + HELIX.
3. 9-ELEMENT KENICS CORE WITH 4.40 MM ANTI-EJECTION BASE.
4. SEAL SOCKET MOLDED ID 3.10 +-0.05 MM (INTERFERENCE).

PART 1 - 4-PART HELICAL STATIC MIXER DUAL-BARREL CAP ASSY	SCALE 2:1 MM THIRD ANGLE
CSL-CAP-201 · ABS / SILICONE / CLEAR PC / POM · ANTIGRAVITY CAD	SHEET 3 OF 12 REV C coseal_engineering_drawings


REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS

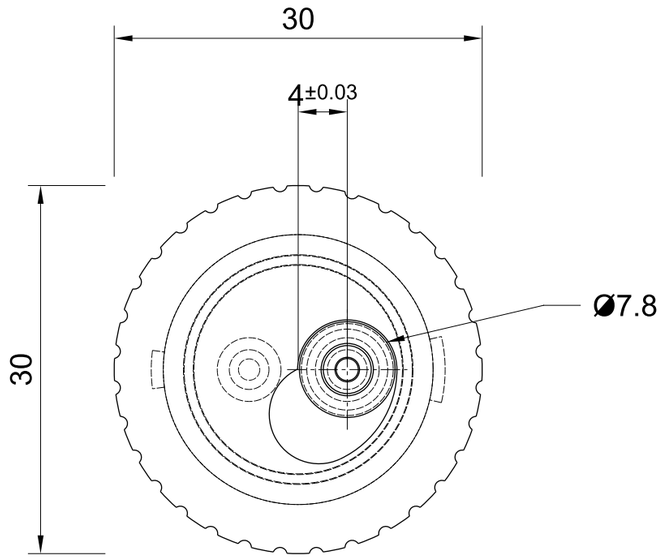


TOP

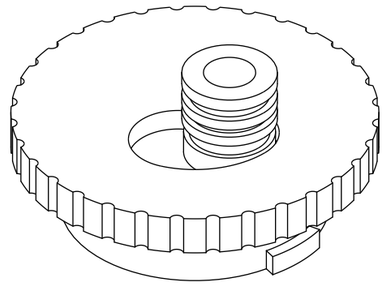

ISOMETRIC

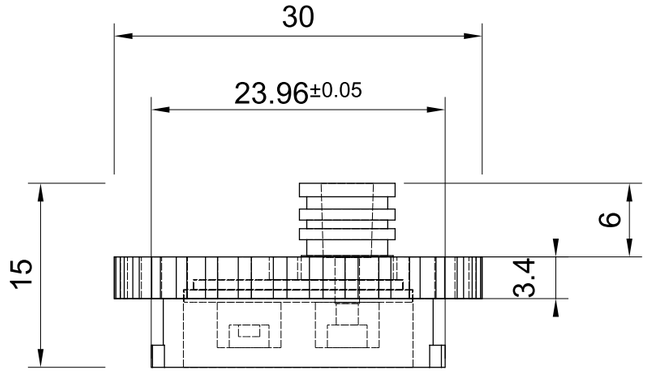

FRONT

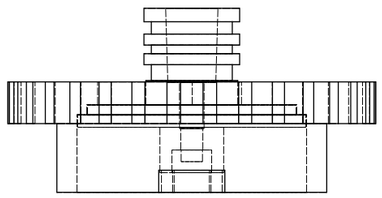


RIGHT


NOTES: 1. TOLERANCES PER ISO 2768-m UNLESS OTHERWISE SPECIFIED.
2. FEMALE LUER-LOCK PER ISO 80369-7 (6% TAPER).
3. PORT A (+4.00 MM) OPEN; PORT B (-4.00 MM) BLIND.
4. OUTER RING ROTATES 65 DEG AROUND STATIONARY INSERT.

PART 2 - LUER RECONSTITUTION SINGLE-BARREL CAP	SCALE 2:1 MM THIRD ANGLE
CSL-CAP-202 · MEDICAL PP + TPE / PC · ANTIGRAVITY CAD	SHEET 4 OF 12 REV B coseal_engineering_drawings


REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS

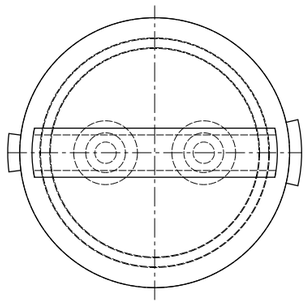


TOP

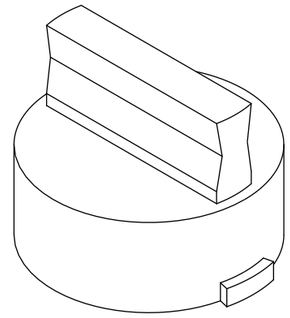

ISOMETRIC

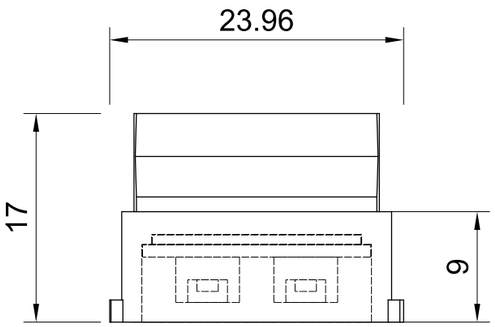

FRONT

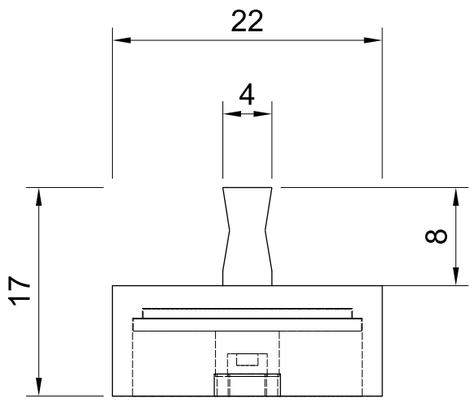


RIGHT


NOTES: 1. TOLERANCES PER ISO 2768-m UNLESS OTHERWISE SPECIFIED.
2. DUAL BLIND ELASTOMER PLUGS SEAL BOTH BARRELS.
3. OUTER CAP SPINS FREELY AROUND STATIONARY PLUG PAD.
4. MOLDED SOCKET ID 3.10 +-0.05 MM; BORE PIN OD 1.86 MM.

PART 3 - INITIAL PLUG VALVE SEALING CAP	SCALE 2:1 MM THIRD ANGLE
CSL-CAP-203 · MEDICAL PP + BUTYL / SILICONE · ANTIGRAVITY CAD	SHEET 5 OF 12 REV B coseal_engineering_drawings


REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS

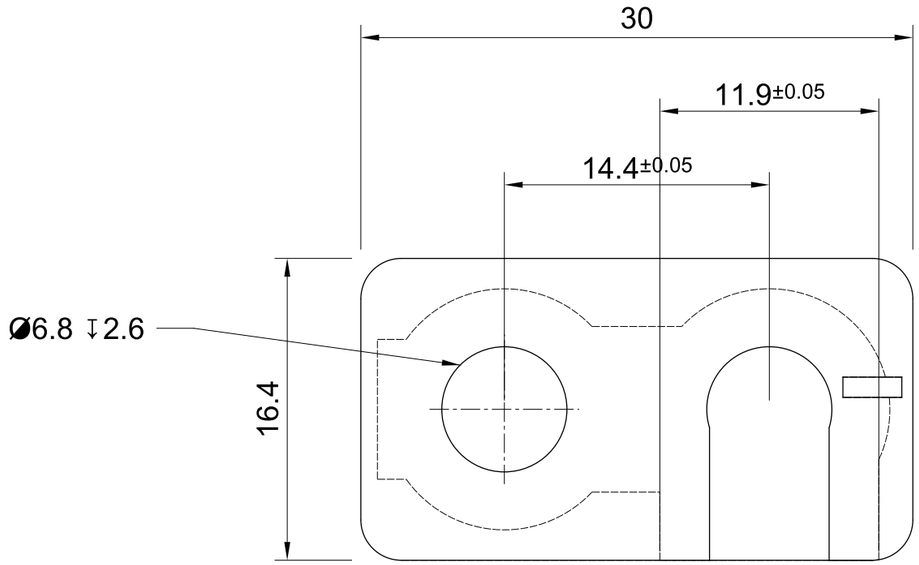

TOP

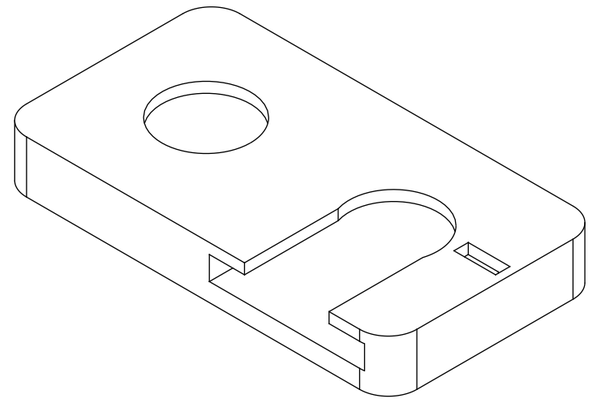

ISOMETRIC

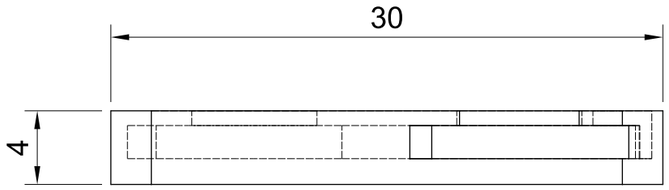


FRONT

RIGHT


NOTES: 1. TOLERANCES PER ISO 2768-m UNLESS OTHERWISE SPECIFIED.
2. CAPTIVE PIVOT ON BARREL B (-7.20 MM) ROTATES 90 DEG.
3. SIDE SNAP C-JAW ON BARREL A (+7.20 MM): 0.90 MM DETENT.
4. INTERNAL SLOT WIDTH 1.80 +0.10/-0.00 MM FOR 1.60 MM DISC.

PART 4 - SINGLE/DUAL PLUNGER SELECTOR CLIP	SCALE 3:1 MM THIRD ANGLE
CSL-PRT-104 · MEDICAL POM (DELRIN) / TOUGHENED PP · ANTIGRAVITY CAD	SHEET 6 OF 12 REV B coseal_engineering_drawings


REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS

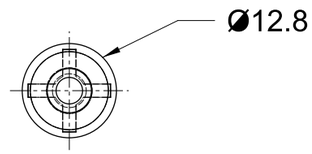


TOP

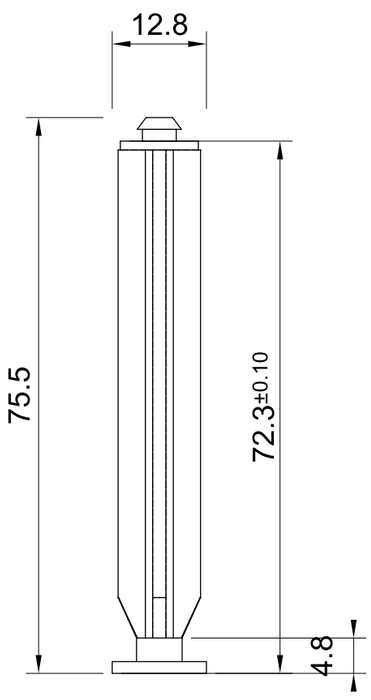

FRONT



RIGHT




ISOMETRIC (1.2:1)


NOTES: 1. TOLERANCES PER ISO 2768-m UNLESS OTHERWISE SPECIFIED.
2. QTY PER SYSTEM: 2 PCS (IDENTICAL FOR BARREL A & B).
3. THUMB DISC 12.80 X 1.60 MM MATES WITH SELECTOR CLIP #4.
4. NECK JOURNAL DIA 6.20 MM X 3.20 MM LENGTH.

CRUCIFORM PLUNGER ROD (DUAL-BARREL DRIVE)	SCALE 1.2:1 MM THIRD ANGLE
CSL-PRT-102 · MEDICAL GRADE PP / ABS · ANTIGRAVITY CAD	SHEET 7 OF 12 REV B coseal_engineering_drawings


REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS

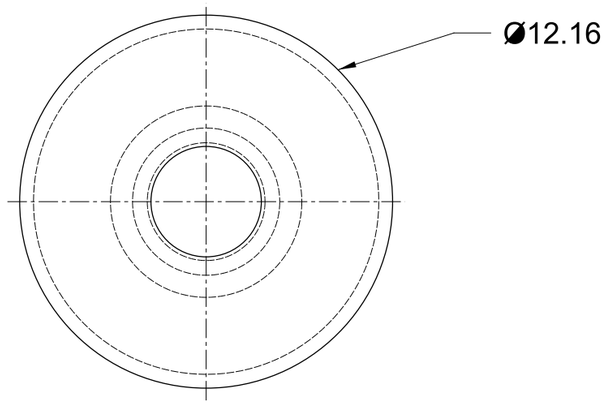


TOP

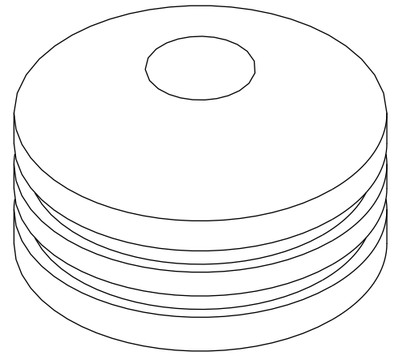

ISOMETRIC

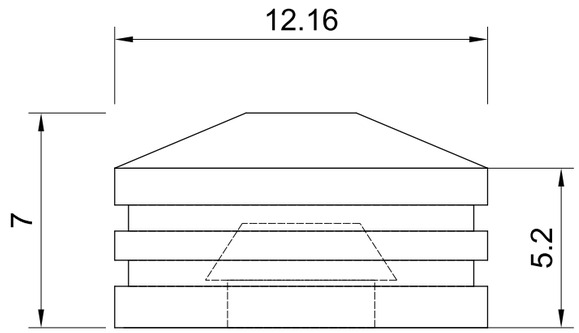

FRONT

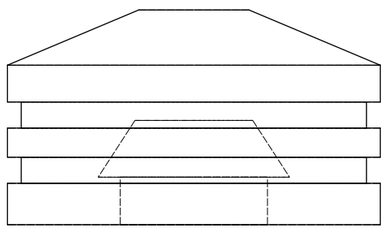


RIGHT


NOTES: 1. TOLERANCES PER ISO 2768-m UNLESS OTHERWISE SPECIFIED.
2. QTY PER SYSTEM: 2 PCS (MEDICAL SILICONE OIL COATED).
3. MOLDED SEALING RIB OD 12.50 +-0.10 MM FOR 12.20 BORE.
4. CONICAL TIP MINIMIZES RESIDUAL HOLD-UP VOLUME.

TRIPLE-RIB ELASTOMER PISTON STOPPER	SCALE 5:1 MM THIRD ANGLE
CSL-PRT-103 · MEDICAL BROMOBUTYL / SILICONE (SHORE A 55) · ANTIGRAVITY CAD	SHEET 8 OF 12 REV B coseal_engineering_drawings


REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS

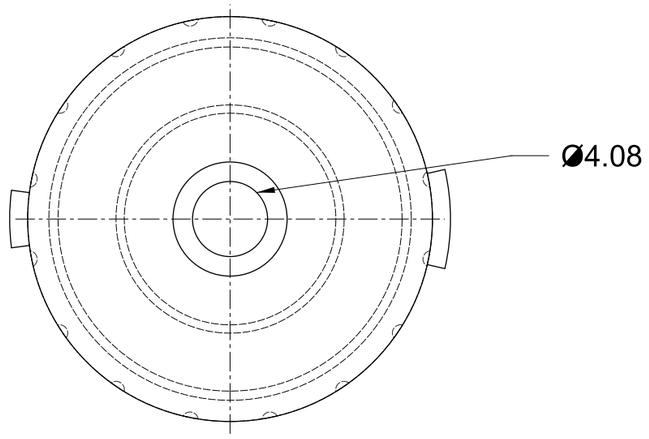


TOP

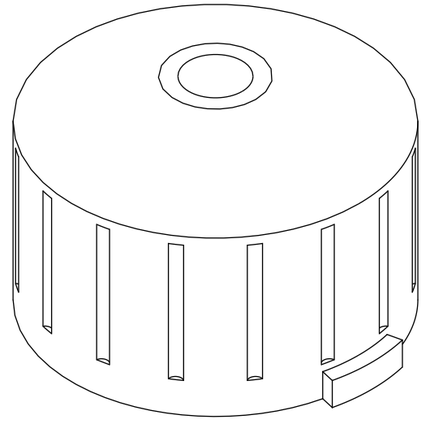

ISOMETRIC

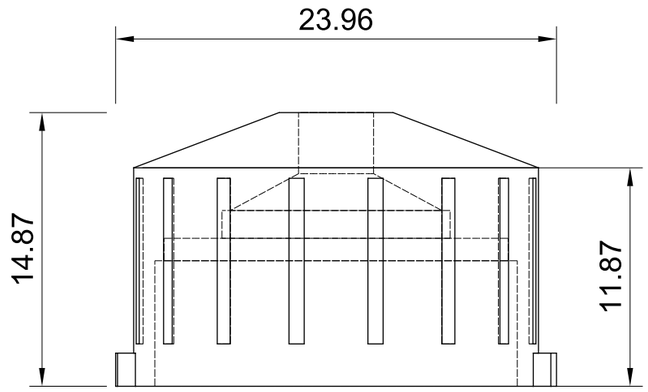

FRONT

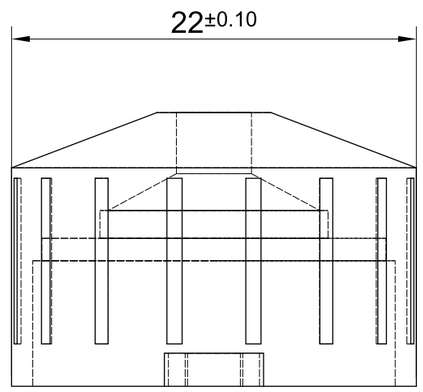


RIGHT


NOTES: 1. TOLERANCES PER ISO 2768-f UNLESS OTHERWISE SPECIFIED.
2. ASYMMETRIC BAYONET LUGS: +X 26 DEG / -X 15 DEG.
3. INTERNAL CONICAL SHOULDER CLAMPS BELL CANNULA WITHOUT GLUE.
4. SINGLE-PULL 2-PLATE MOLDABLE STEPPED CAVITY.

PART 1-1 - MIXER BAYONET RETAINING OUTER CAP	SCALE 3:1 MM THIRD ANGLE
CSL-CAP-201-1 · MEDICAL GRADE ABS / PP (OLIVE GREEN) · ANTIGRAVITY CAD	SHEET 9 OF 12 REV C coseal_engineering_drawings


REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS

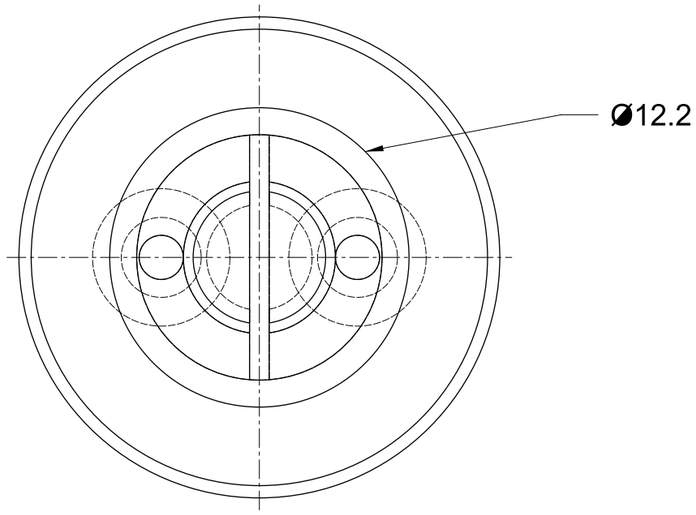


TOP

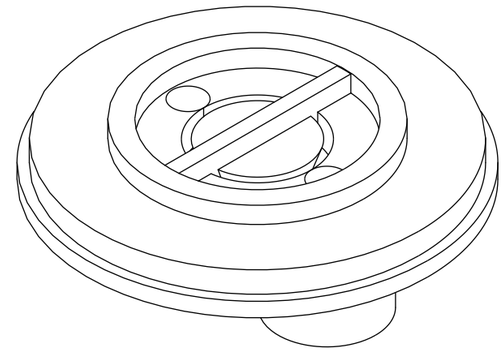

ISOMETRIC

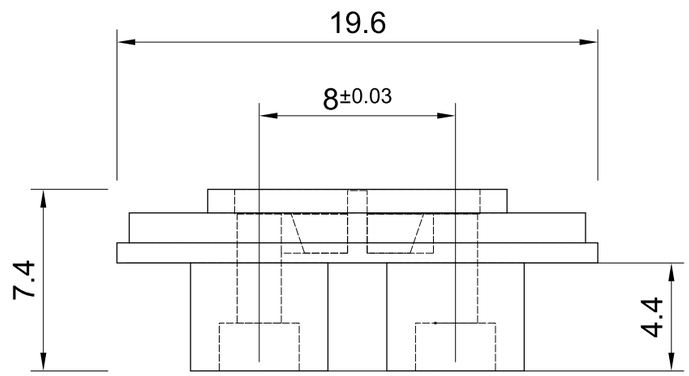

FRONT

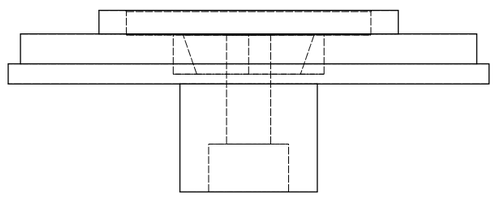


RIGHT


NOTES: 1. TOLERANCES PER ISO 2768-m UNLESS OTHERWISE SPECIFIED.
2. MOLDED FEMALE NOZZLE SOCKETS ID 3.10 +-0.05 MM (2X).
3. DUAL STRAIGHT 1.80 MM RISERS ON 8.00 +-0.03 MM PITCH.
4. CENTRAL PARTITION RIB ISOLATES CHANNELS A & B.

PART 1-2 - DUAL-CHANNEL MANIFOLD ELASTOMER SEAL SEAT	SCALE 4:1 MM THIRD ANGLE
CSL-CAP-201-2 · MEDICAL SILICONE / TPE (SHORE A 60) · ANTIGRAVITY CAD	SHEET 10 OF 12 REV C coseal_engineering_drawings

REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS

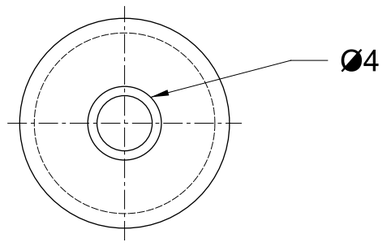


TOP

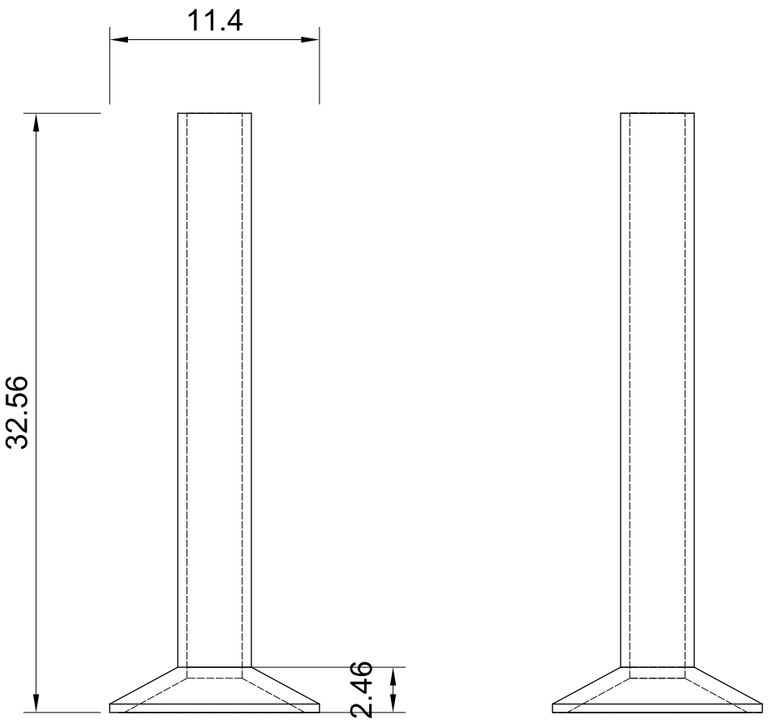

FRONT

RIGHT

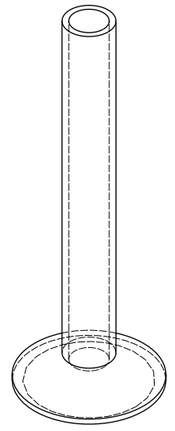


ISOMETRIC (2.2:1)


NOTES: 1. TOLERANCES PER ISO 2768-f UNLESS OTHERWISE SPECIFIED.
2. INTEGRATED FLARED BELL MOUTH & STRAIGHT CANNULA (NO SEAM).
3. OPTICAL TRANSMITTANCE >= 88% FOR VISUAL BUBBLE CHECK.
4. SINGLE POLISHED CORE PIN EXTRACTION ALONG -Z.

PART 1-3 - ONE-PIECE BELL-MOUTH CLEAR MIXING CANNULA	SCALE 3:1 MM THIRD ANGLE
CSL-CAP-201-3 · MEDICAL CLEAR POLYCARBONATE (PC) / COC · ANTIGRAVITY CAD	SHEET 11 OF 12 REV C coseal_engineering_drawings

REV	DATE	DESCRIPTION
A	2026-10-28	VENDOR CONCEPT LAYOUT
B	2026-11-03	COMPLETE 3D CAD, POKA-YOKE & ISO TOLERANCES
C	2026-11-04	VERIFIED 4-PART MIXER DETAIL DRAWINGS



TOP

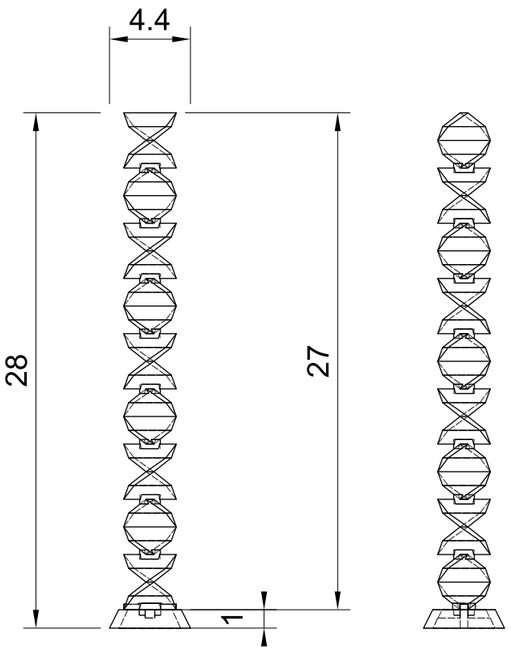

FRONT

RIGHT



ISOMETRIC (2.4:1)

NOTES: 1. TOLERANCES PER ISO 2768-f UNLESS OTHERWISE SPECIFIED.
2. REAR CONICAL COLLAR OD 4.40->3.40 MM PREVENTS TIP BLOWOUT.
3. 9 ALTERNATING L/R 180-DEG ELEMENTS (3.00 MM PITCH, 512 LAYERS).
4. LEFT/RIGHT SPLIT-CAVITY PRECISION INJECTION MOLD.

PART 1-4 - 9-ELEMENT KENICS HELICAL CORE (ANTI-EJECTION)	SCALE 3:1 MM THIRD ANGLE
CSL-CAP-201-4 · MEDICAL GRADE POM (ACETAL COPOLYMER) · ANTIGRAVITY CAD	SHEET 12 OF 12 REV C coseal_engineering_drawings