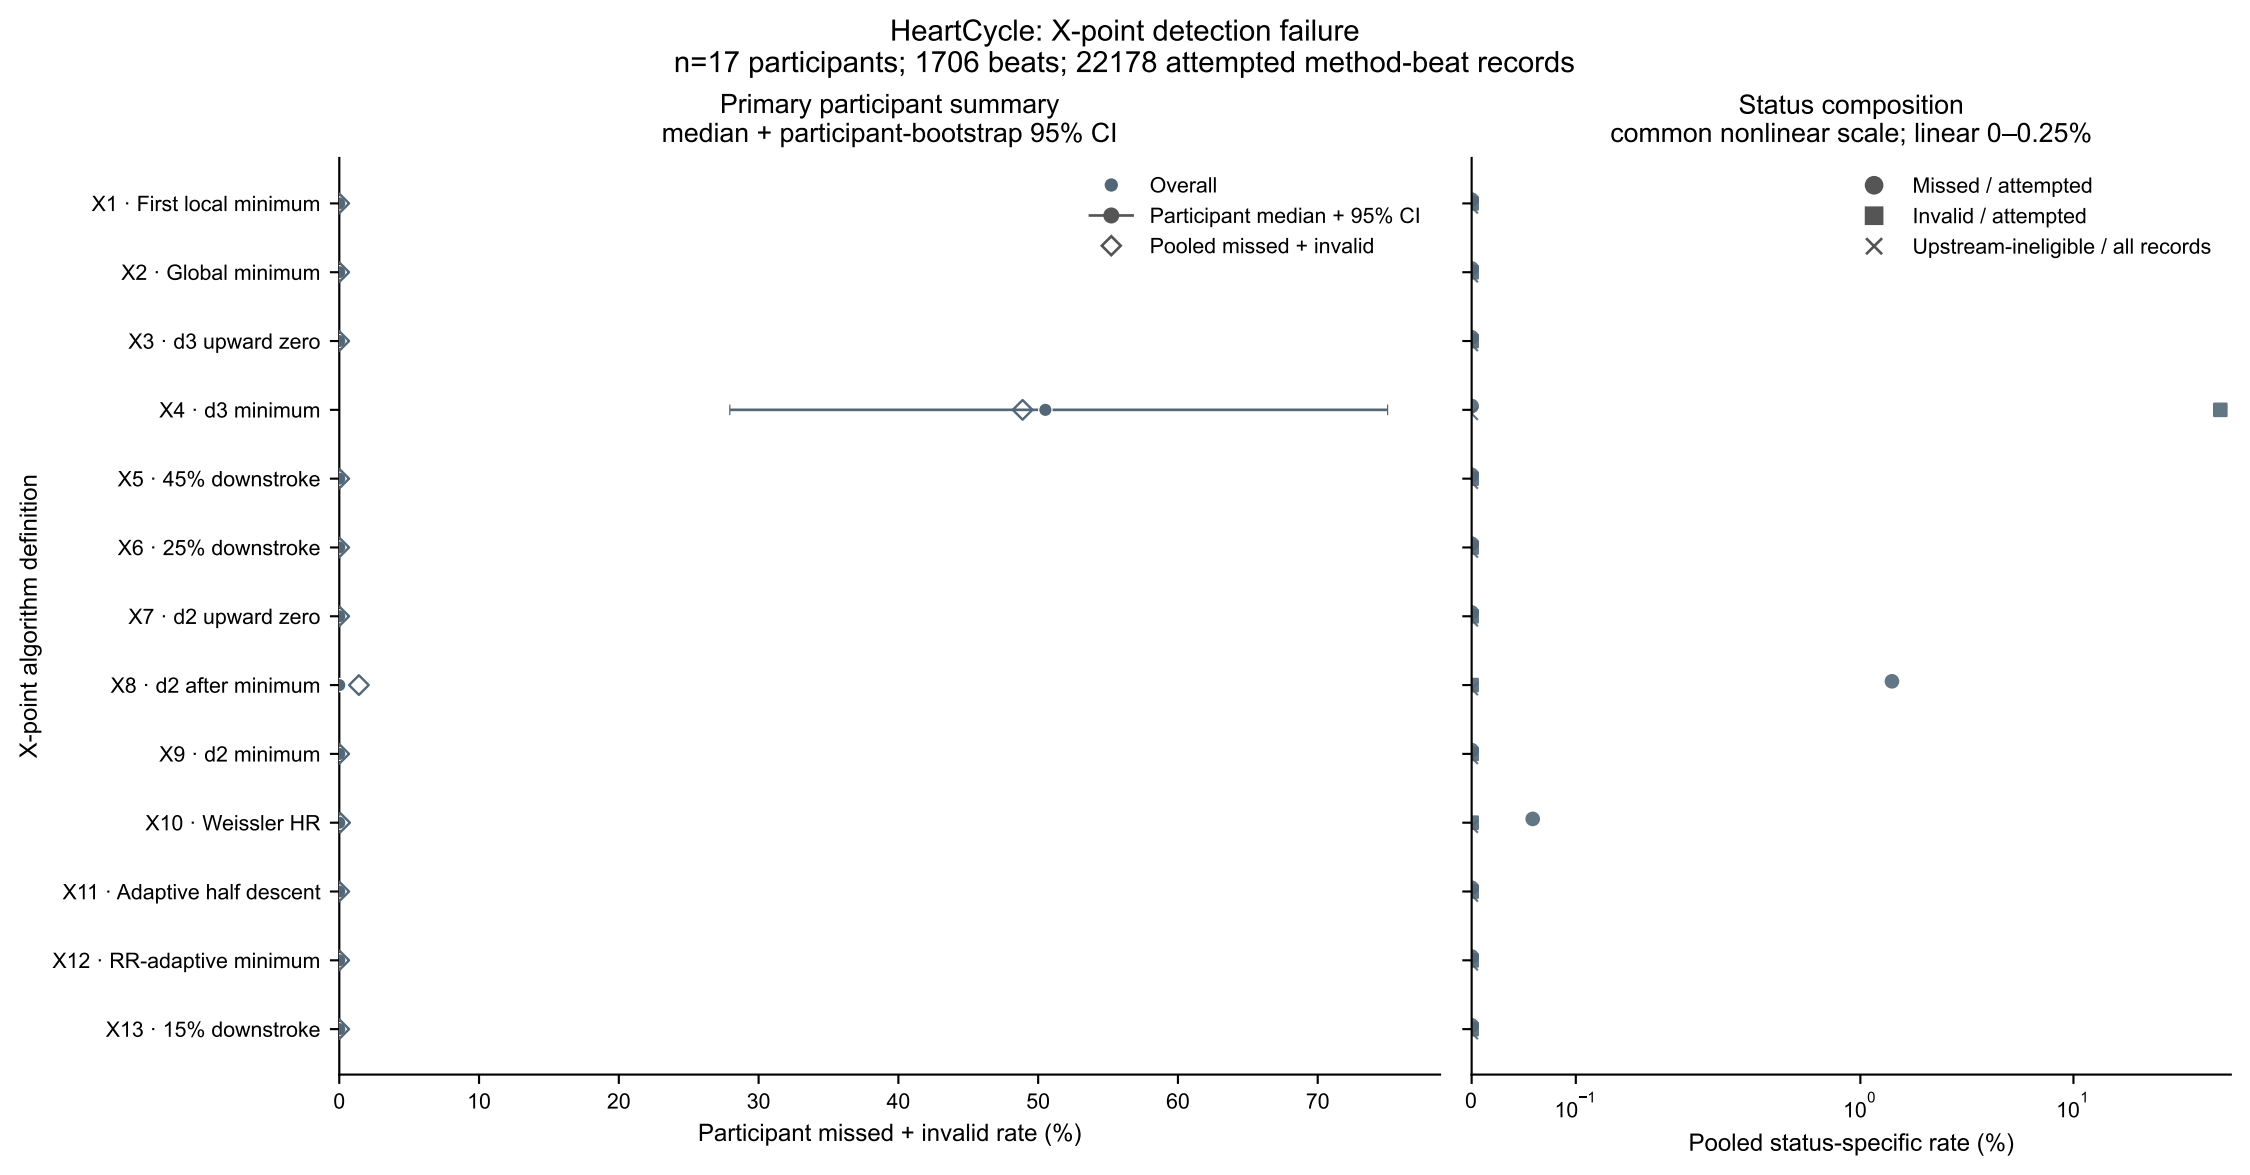
HeartCycle: X-point detection failure
n=17 participants; 1706 beats; 22178 attempted method-beat records
Primary participant summary
median + participant-bootstrap 95% CI
Status composition
common nonlinear scale; linear 0–0.25%
X-point algorithm definition
X1 · First local minimum
X2 · Global minimum
X3 · d3 upward zero
X4 · d3 minimum
X5 · 45% downstroke
X6 · 25% downstroke
X7 · d2 upward zero
X8 · d2 after minimum
X9 · d2 minimum
X10 · Weissler HR
X11 · Adaptive half descent
X12 · RR-adaptive minimum
X13 · 15% downstroke
Overall
Participant median + 95% CI
Pooled missed + invalid
Missed / attempted
Invalid / attempted
Upstream-ineligible / all records
0
10
20
30
40
50
60
70
Participant missed + invalid rate (%)
0
10^{-1}
10^{0}
10^{1}
Pooled status-specific rate (%)