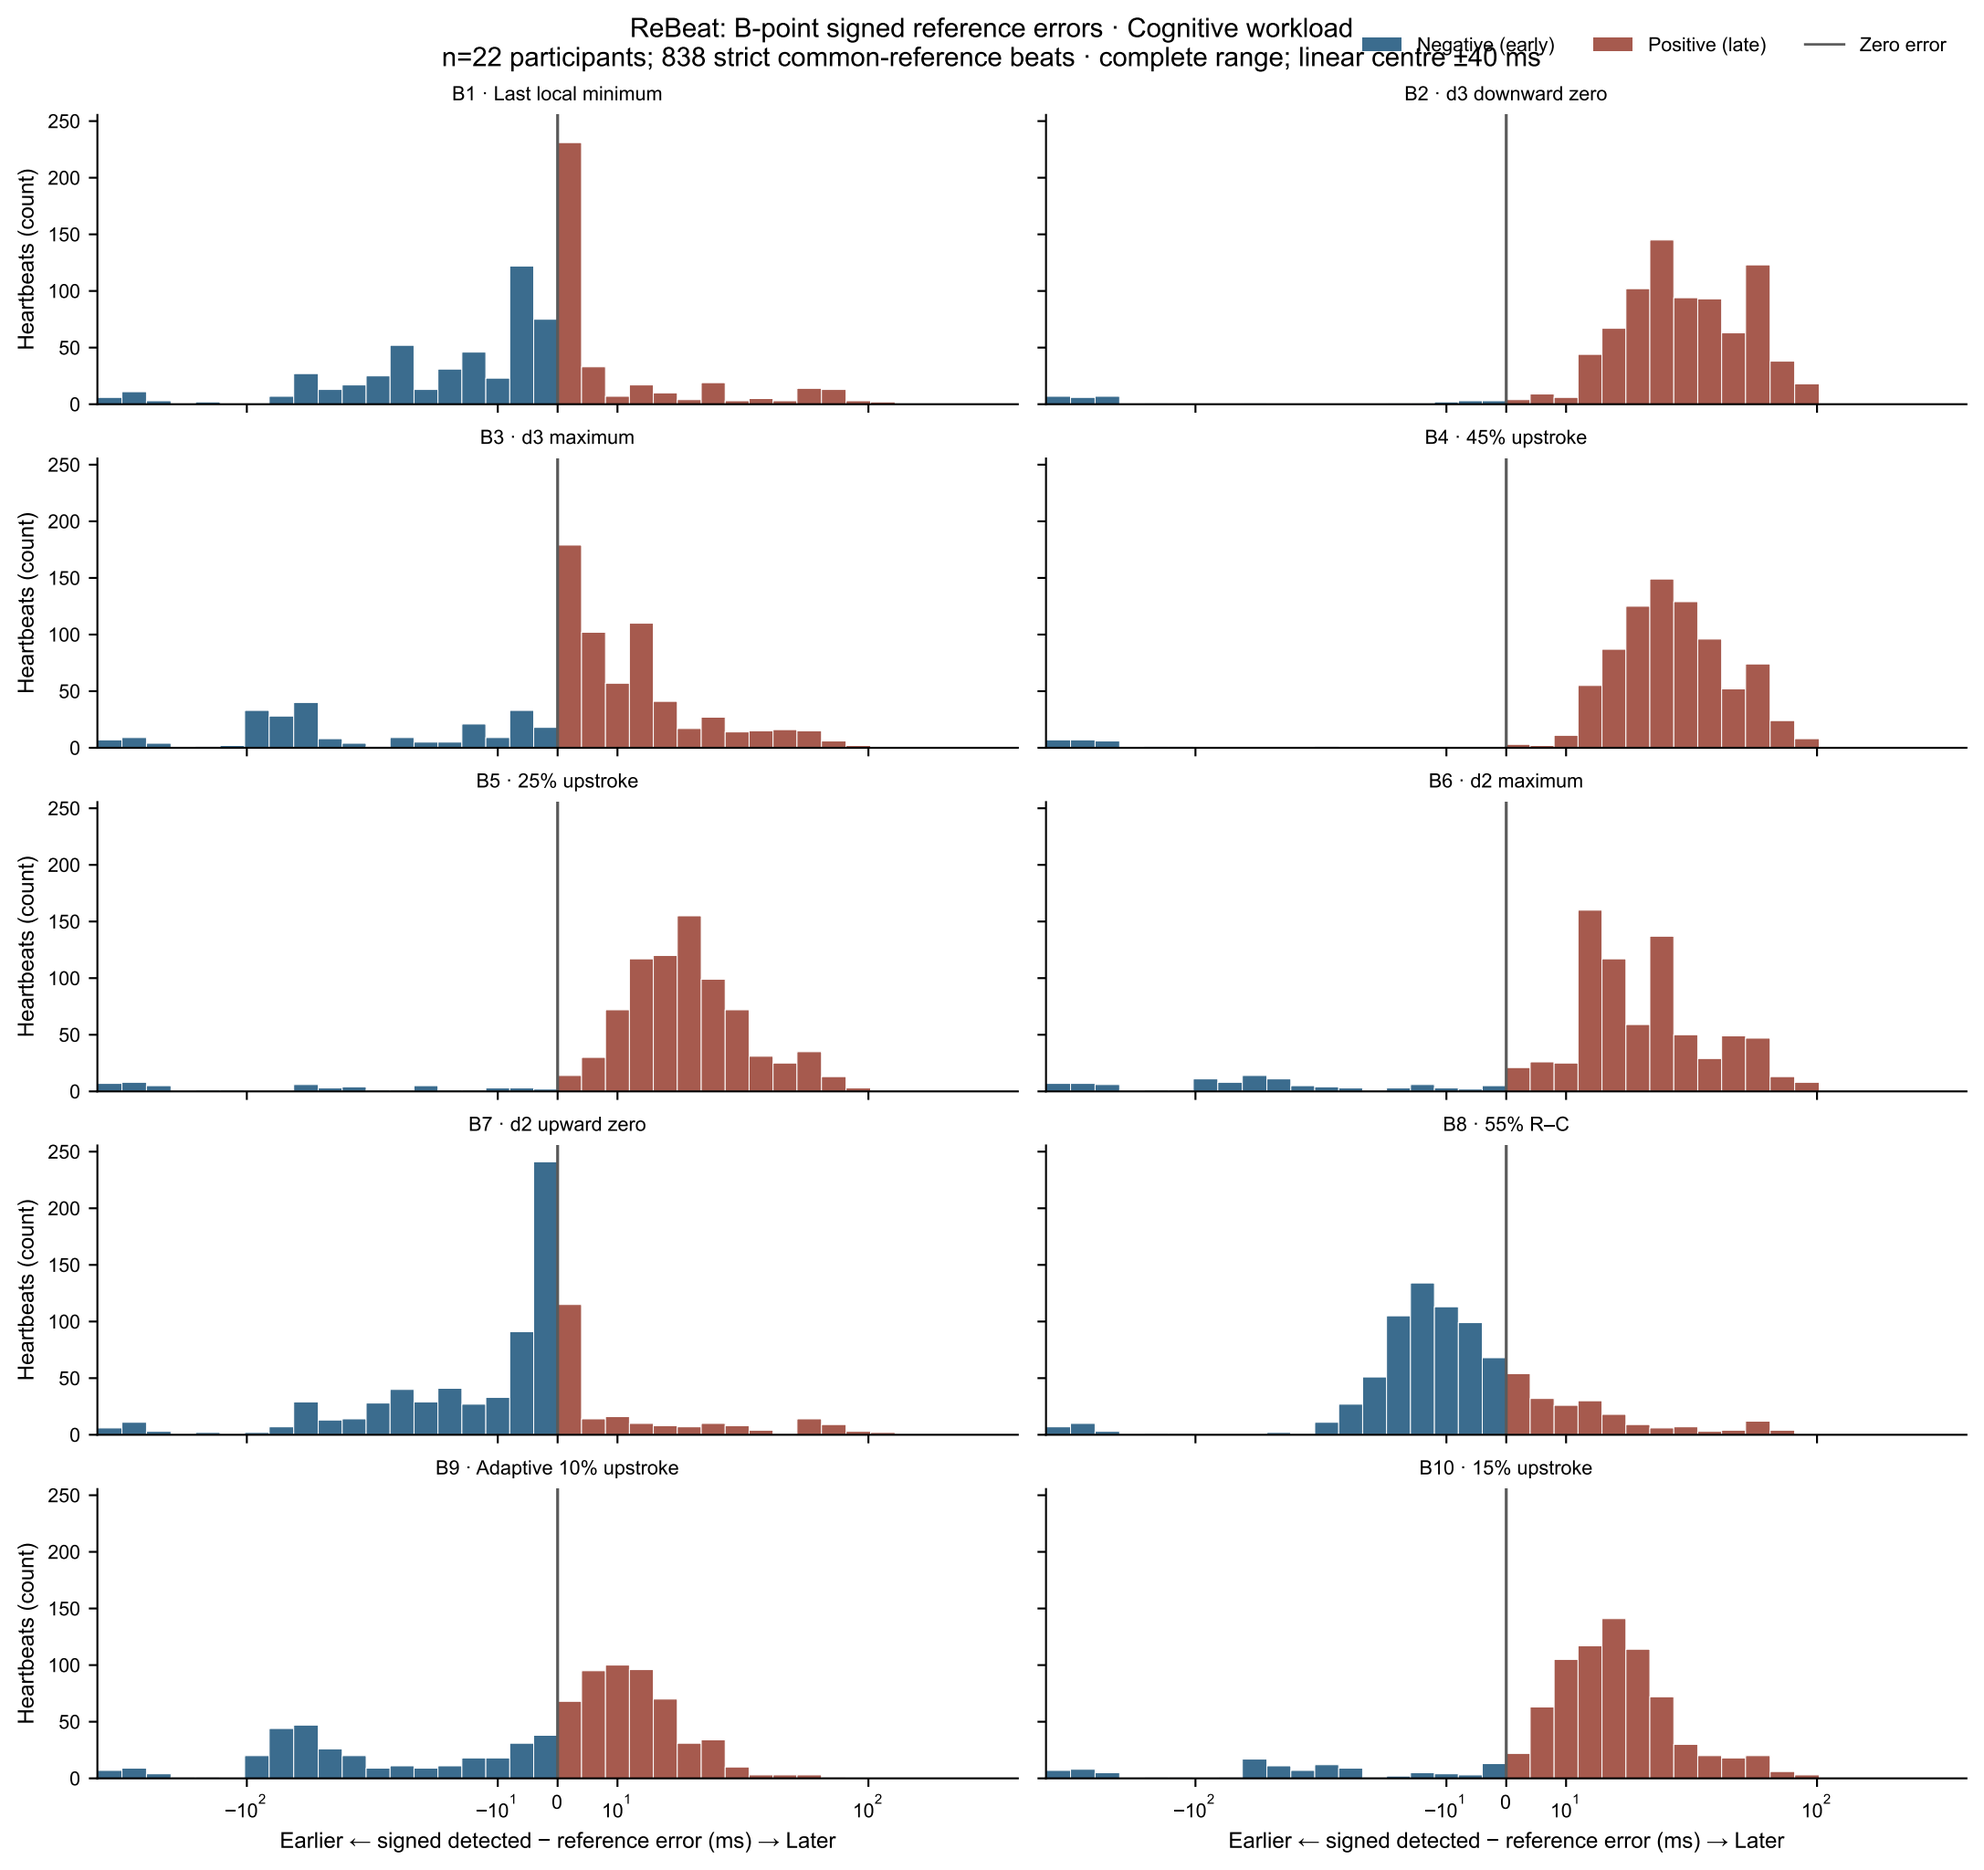
ReBeat: B-point signed reference errors · Cognitive workload
n=22 participants; 838 strict common-reference beats · complete range; linear centre ±40 ms
Negative (early)
Positive (late)
Zero error
B1 · Last local minimum
B2 · d3 downward zero
B3 · d3 maximum
B4 · 45% upstroke
B5 · 25% upstroke
B6 · d2 maximum
B7 · d2 upward zero
B8 · 55% R–C
B9 · Adaptive 10% upstroke
B10 · 15% upstroke
Heartbeats (count)
0
50
100
150
200
250
−10²
−10¹
0
10¹
10²
Earlier ← signed detected − reference error (ms) → Later