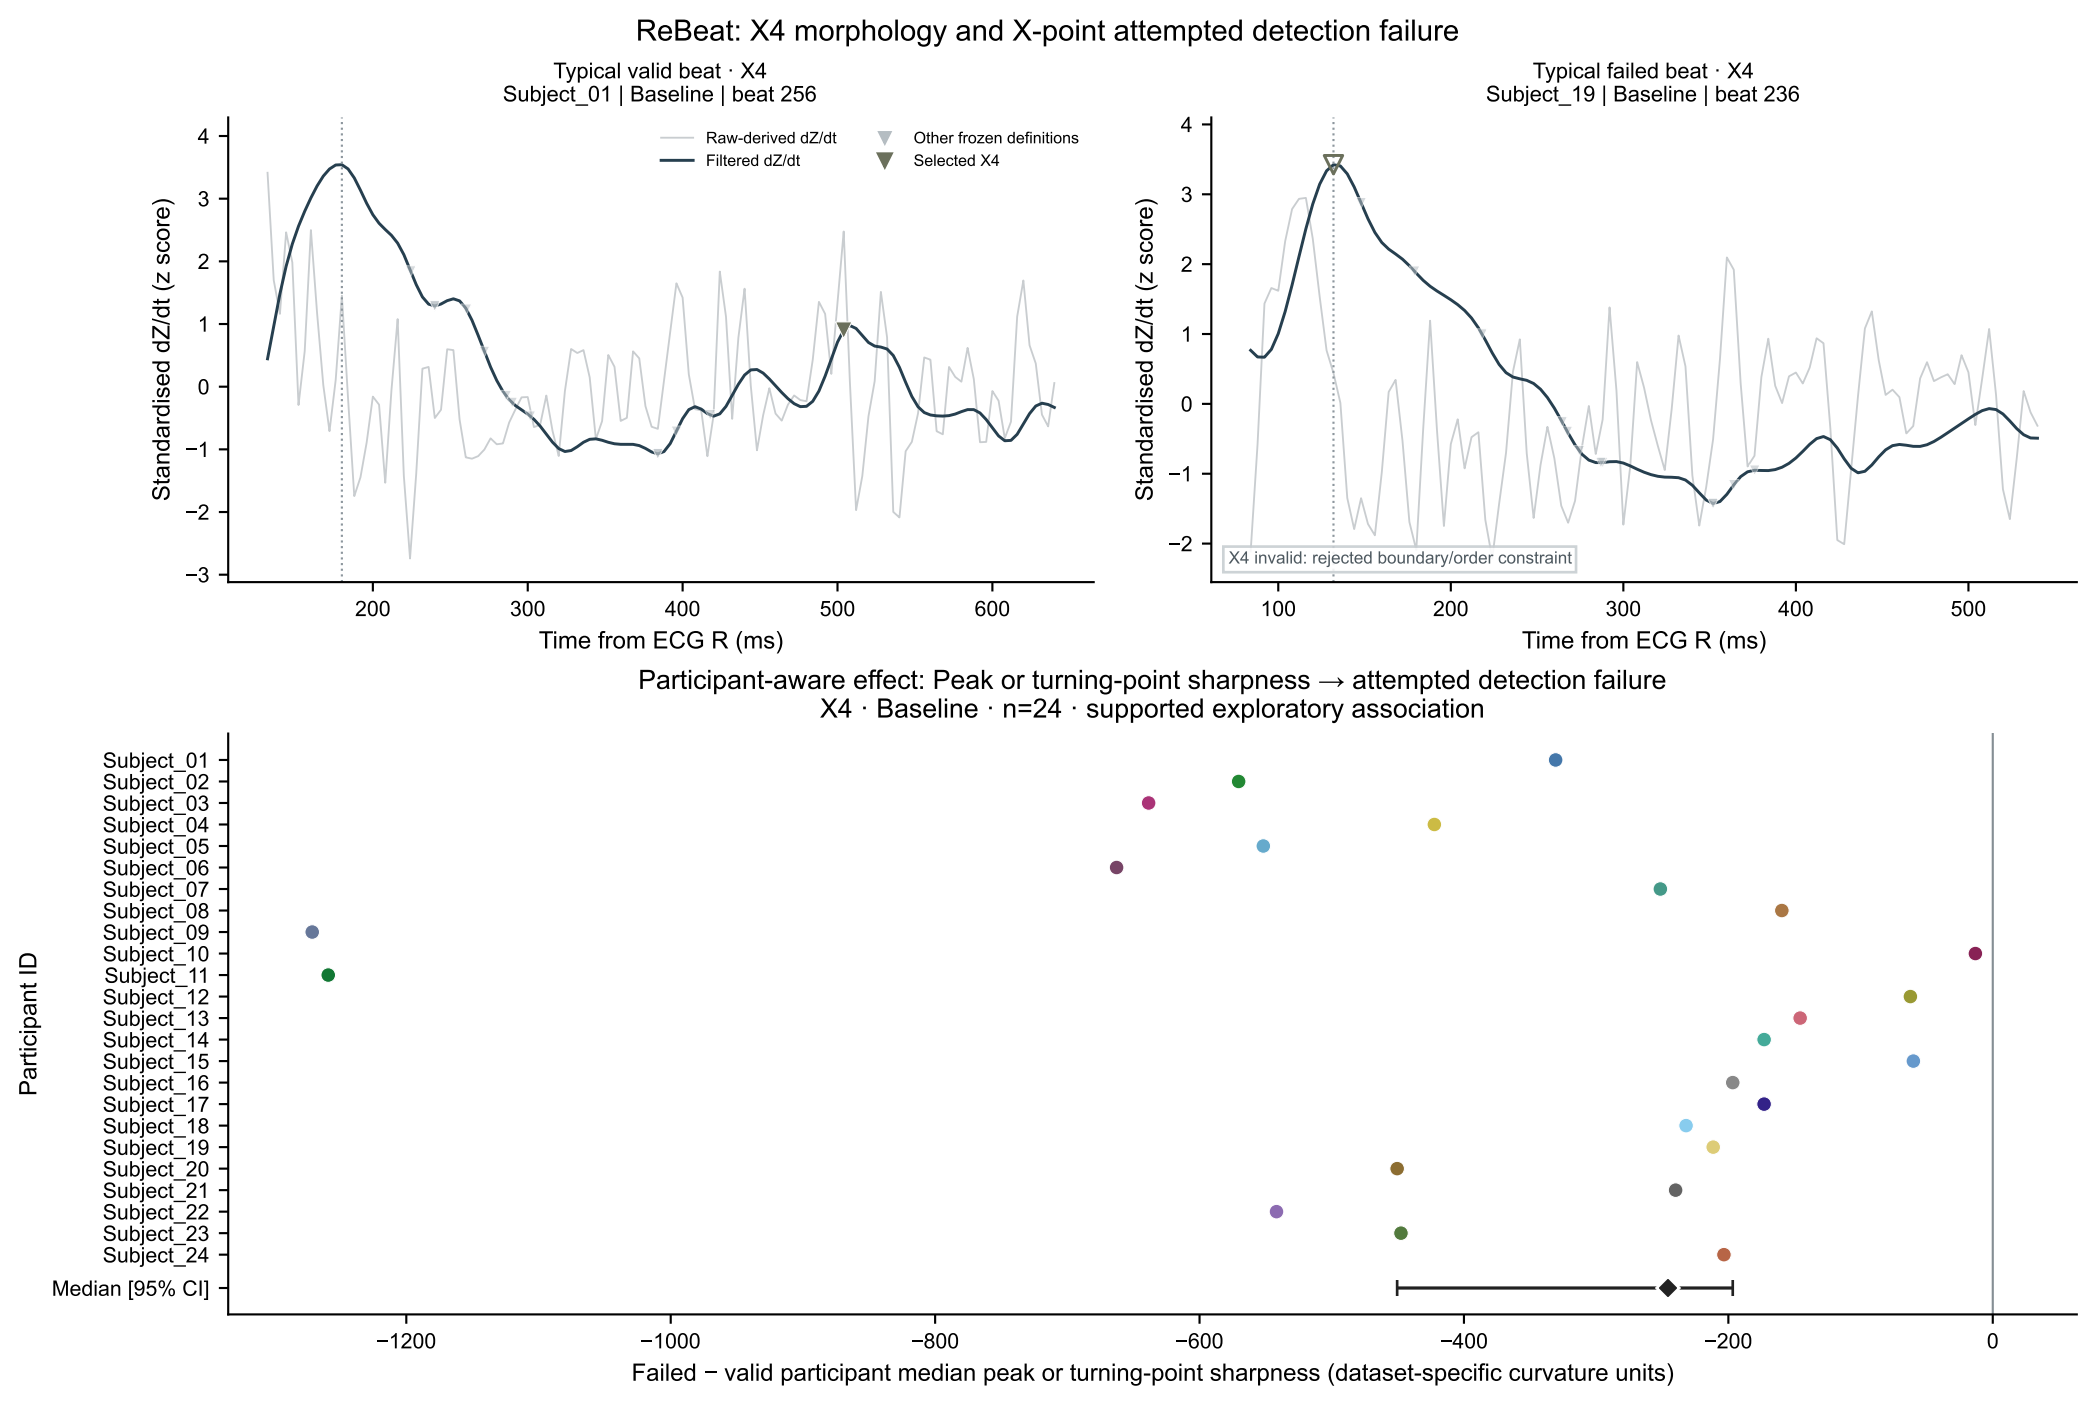
ReBeat: X4 morphology and X-point attempted detection failure
Typical valid beat · X4
Subject_01 | Baseline | beat 256
Raw-derived dZ/dt
Filtered dZ/dt
Other frozen definitions
Selected X4
Standardised dZ/dt (z score)
Time from ECG R (ms)
Typical failed beat · X4
Subject_19 | Baseline | beat 236
X4 invalid: rejected boundary/order constraint
Participant-aware effect: Peak or turning-point sharpness → attempted detection failure
X4 · Baseline · n=24 · supported exploratory association
Participant ID
Subject_01
Subject_02
Subject_03
Subject_04
Subject_05
Subject_06
Subject_07
Subject_08
Subject_09
Subject_10
Subject_11
Subject_12
Subject_13
Subject_14
Subject_15
Subject_16
Subject_17
Subject_18
Subject_19
Subject_20
Subject_21
Subject_22
Subject_23
Subject_24
Median [95% CI]
Failed − valid participant median peak or turning-point sharpness (dataset-specific curvature units)