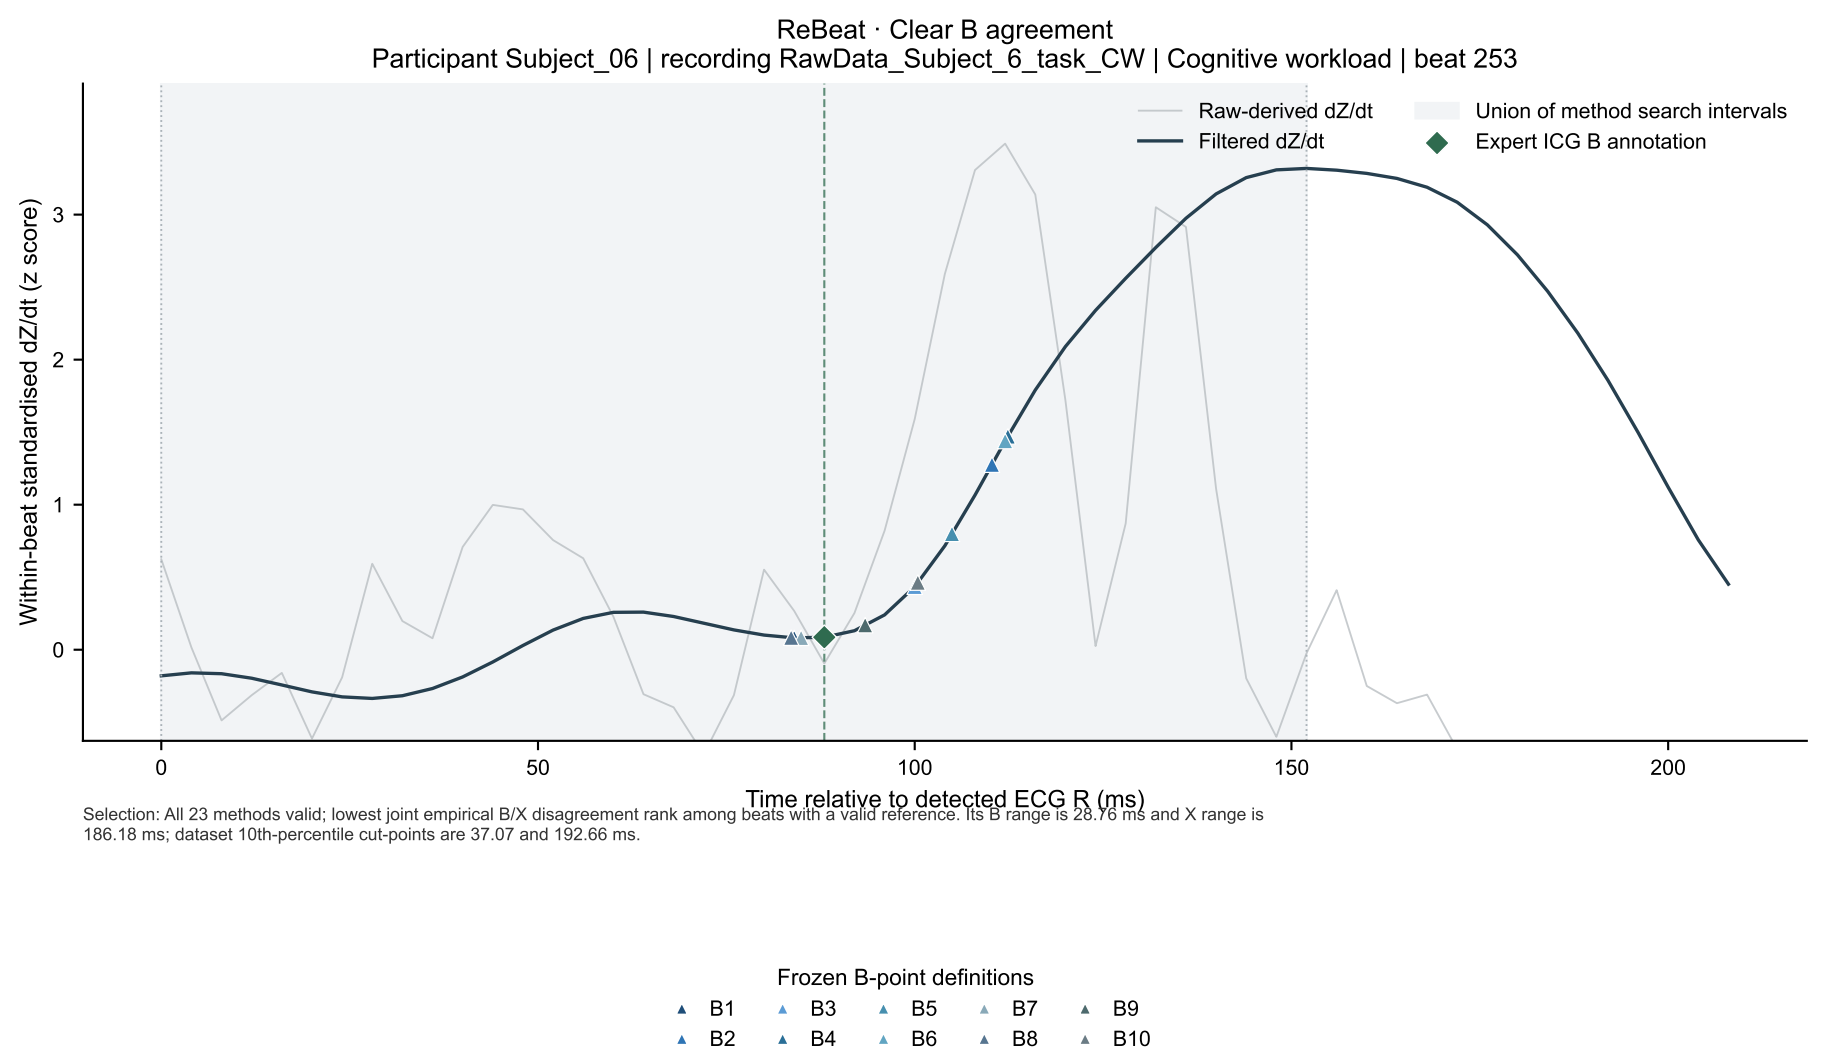
ReBeat · Clear B agreement
Participant Subject_06 | recording RawData_Subject_6_task_CW | Cognitive workload | beat 253
Raw-derived dZ/dt
Filtered dZ/dt
Union of method search intervals
Expert ICG B annotation
Within-beat standardised dZ/dt (z score)
3
2
1
0
0
50
100
150
200
Time relative to detected ECG R (ms)
Selection: All 23 methods valid; lowest joint empirical B/X disagreement rank among beats with a valid reference. Its B range is 28.76 ms and X range is 186.18 ms; dataset 10th-percentile cut-points are 37.07 and 192.66 ms.
Frozen B-point definitions
B1
B2
B3
B4
B5
B6
B7
B8
B9
B10