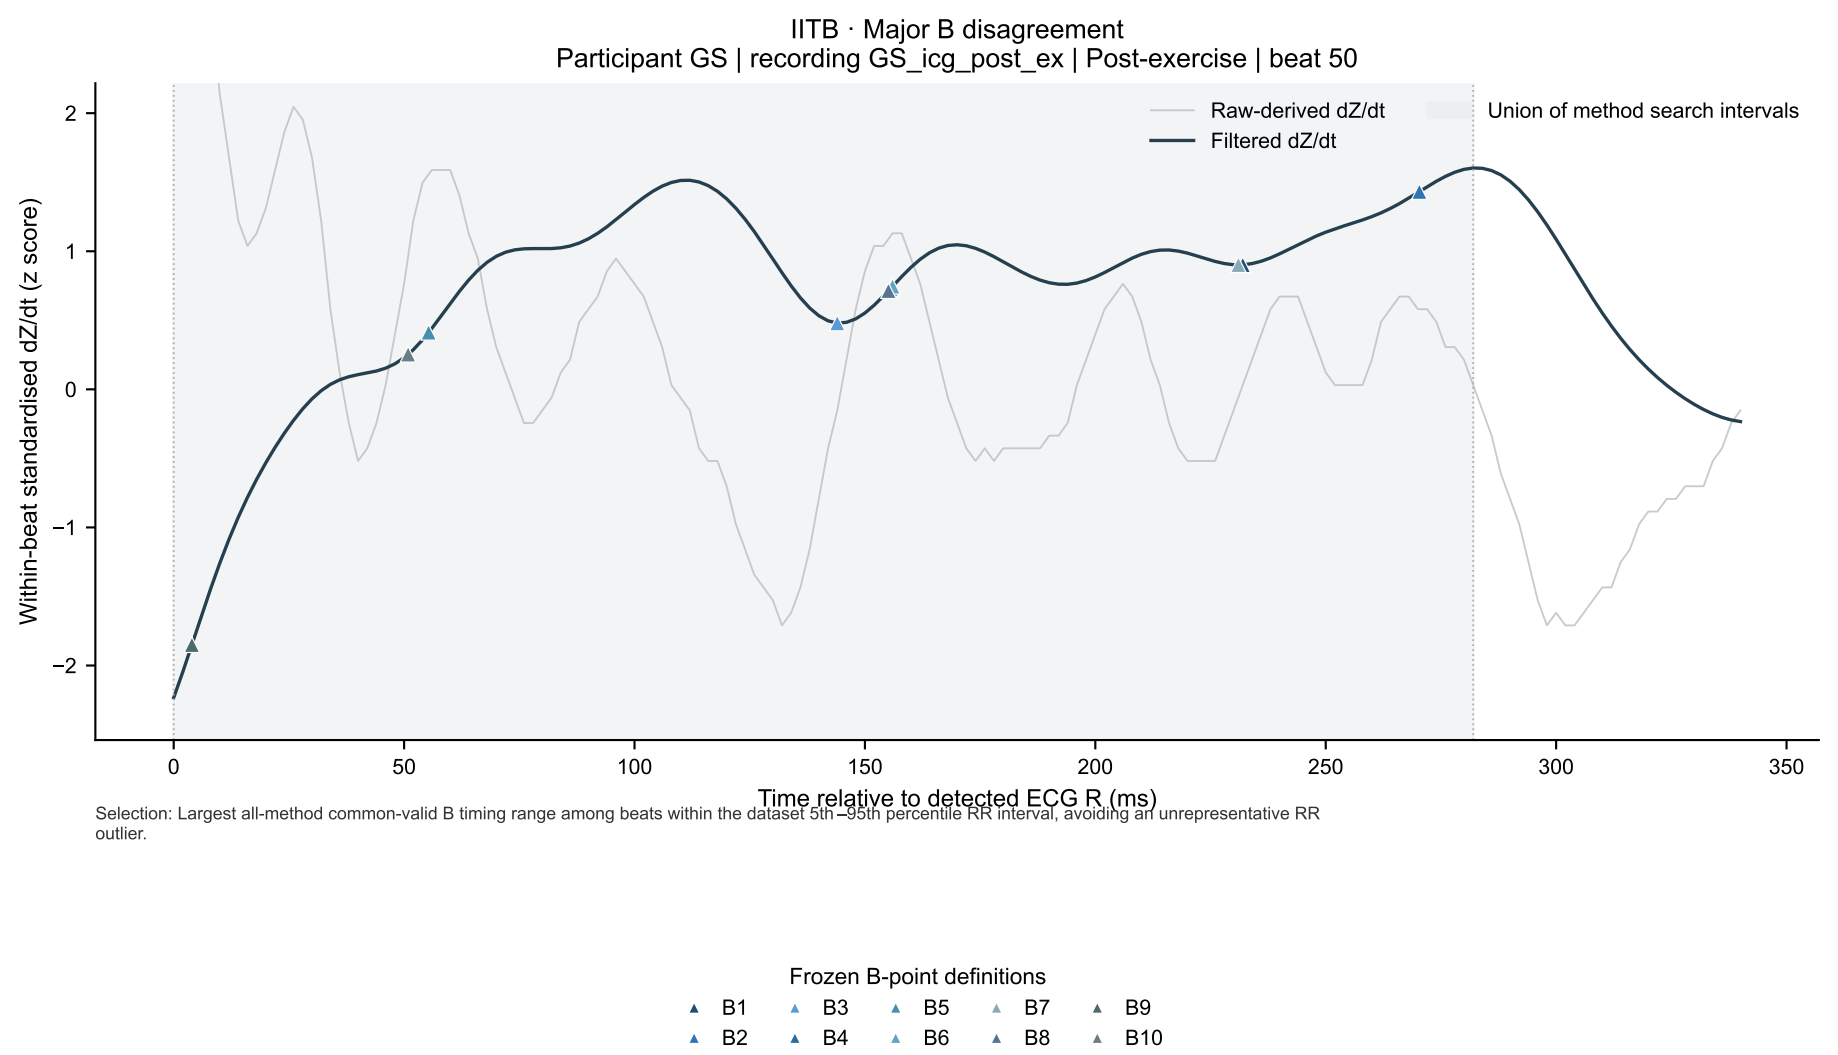
IITB · Major B disagreement
Participant GS | recording GS_icg_post_ex | Post-exercise | beat 50
Raw-derived dZ/dt
Filtered dZ/dt
Union of method search intervals
Within-beat standardised dZ/dt (z score)
2
1
0
−1
−2
0
50
100
150
200
250
300
350
Time relative to detected ECG R (ms)
Selection: Largest all-method common-valid B timing range among beats within the dataset 5th–95th percentile RR interval, avoiding an unrepresentative RR outlier.
Frozen B-point definitions
B1
B2
B3
B4
B5
B6
B7
B8
B9
B10