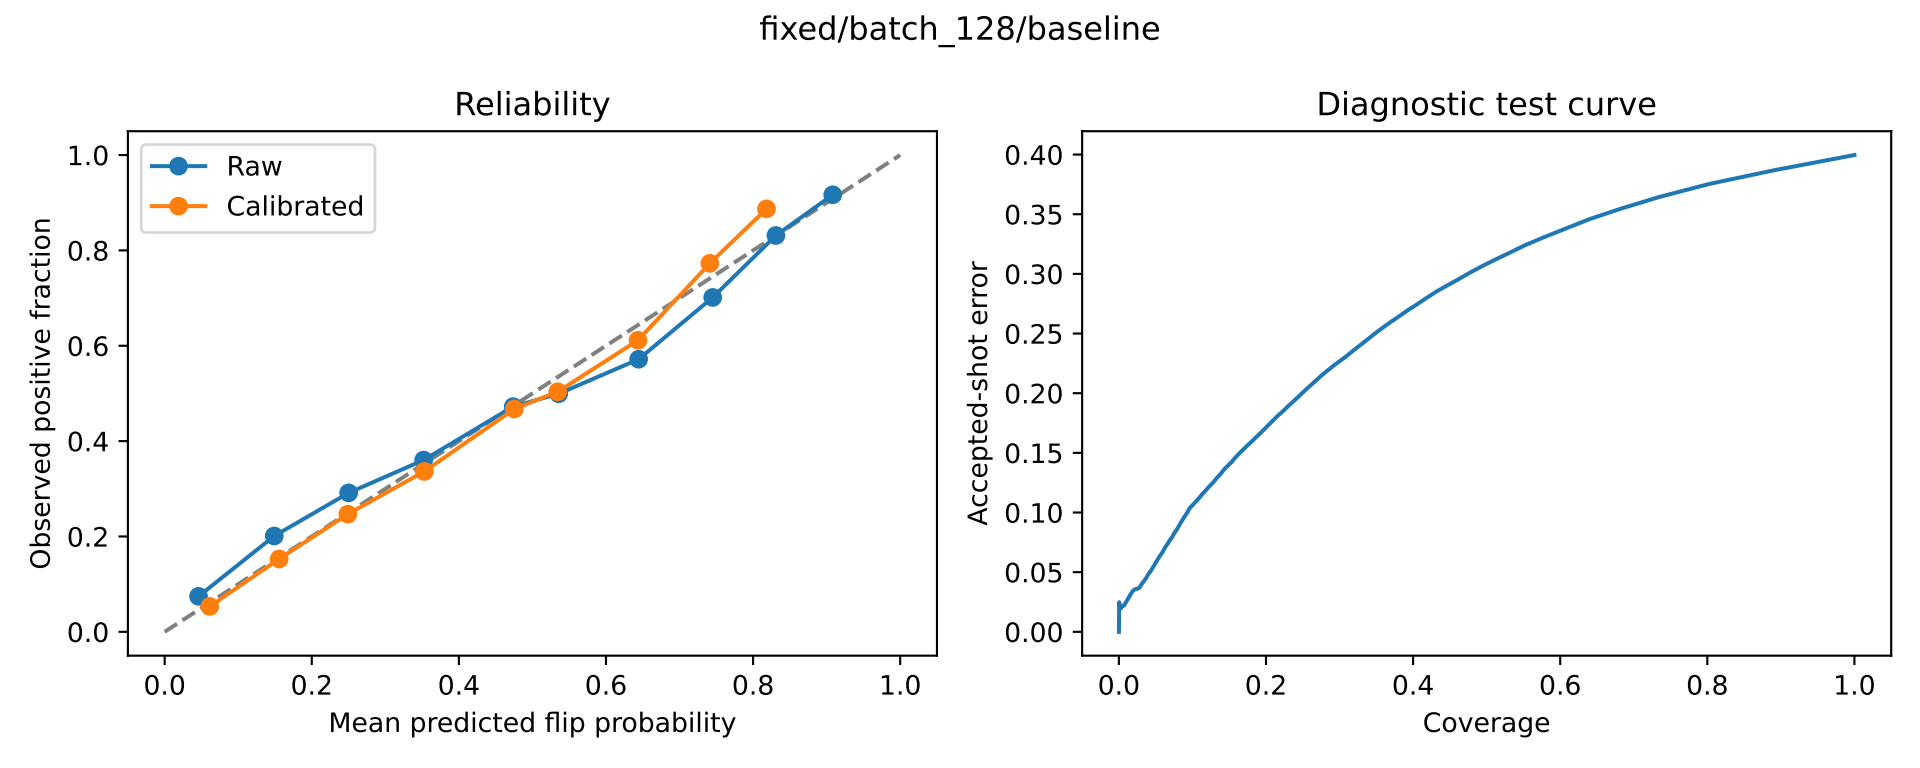
fixed/batch_128/baseline
Reliability
Raw
Calibrated
Observed positive fraction
Mean predicted flip probability
0.0
0.2
0.4
0.6
0.8
1.0
Diagnostic test curve
Accepted-shot error
Coverage
0.00
0.05
0.10
0.15
0.20
0.25
0.30
0.35
0.40