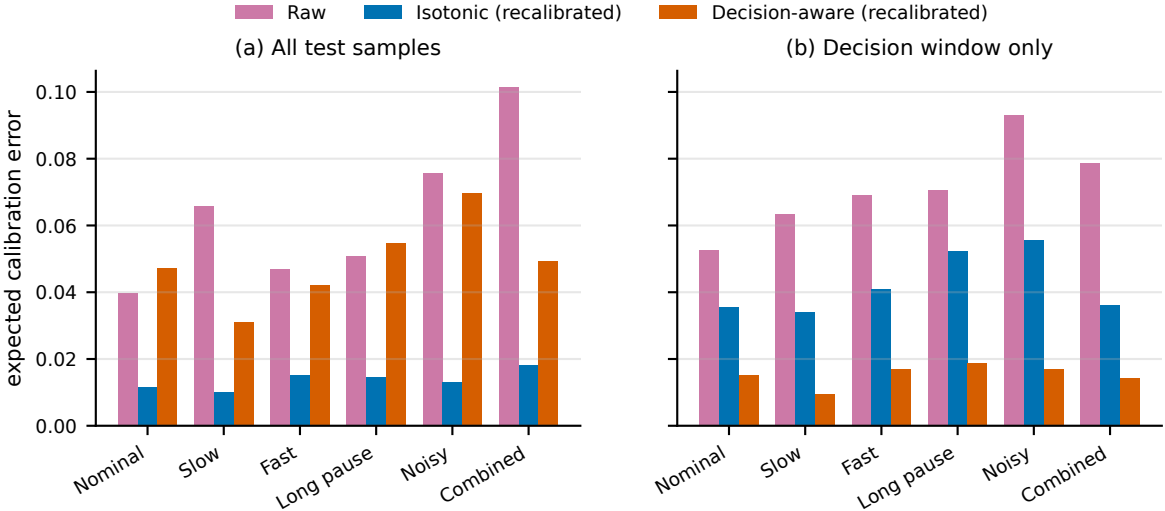
Raw
Isotonic (recalibrated)
Decision-aware (recalibrated)
(a) All test samples
(b) Decision window only
expected calibration error
0.00
0.02
0.04
0.06
0.08
0.10
Nominal
Slow
Fast
Long pause
Noisy
Combined