


Comparison: Reason vs Anti-Reason - Sample ECG200_-1_4

X INCORRECT: Predicted=-1, Actual=1

Maximal REASON (cost=54.1172, 13 intervals)

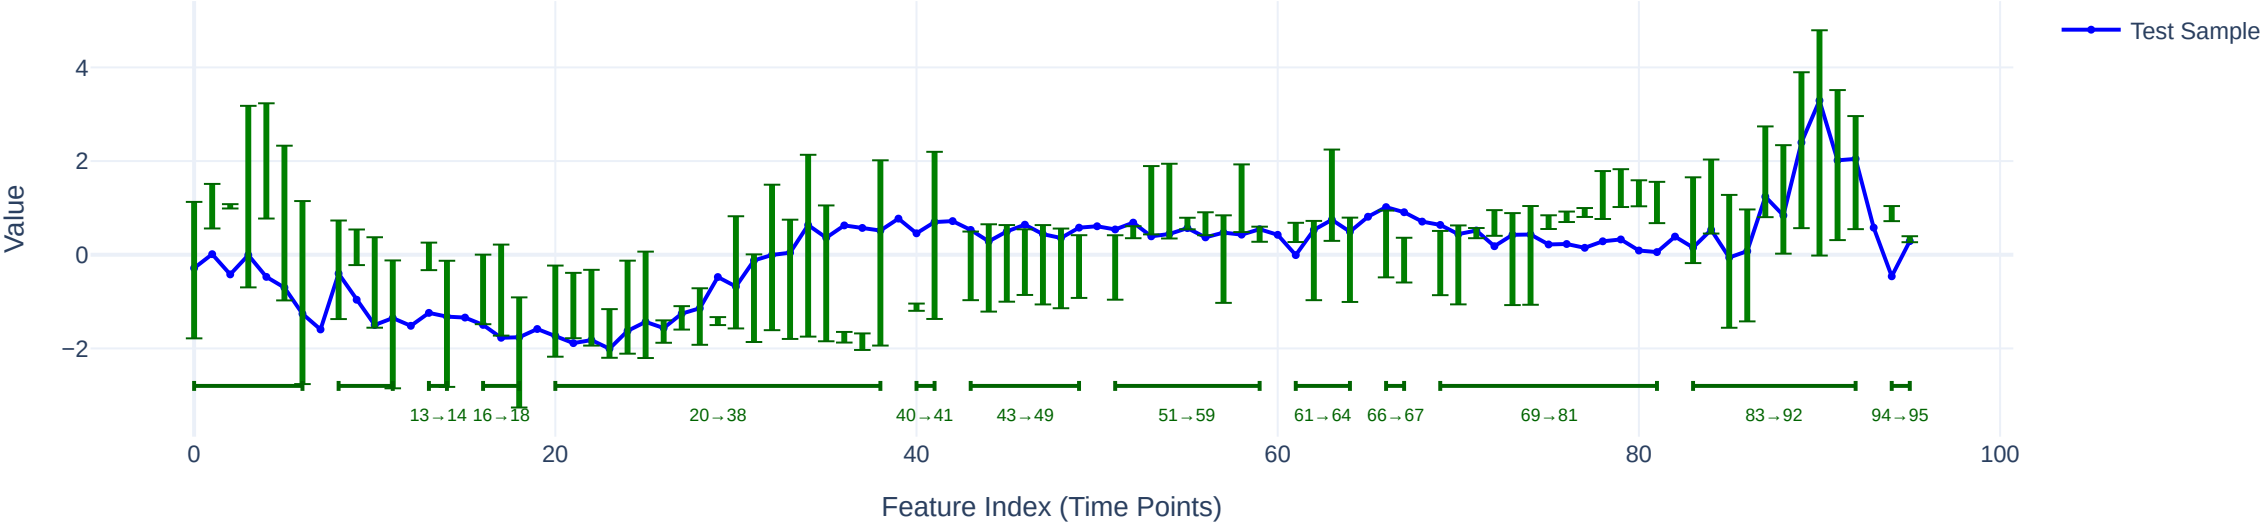

Maximal ANTI-REASON (cost=44.3773, 12 intervals)

