SEALER LOCATIONS (Continued)

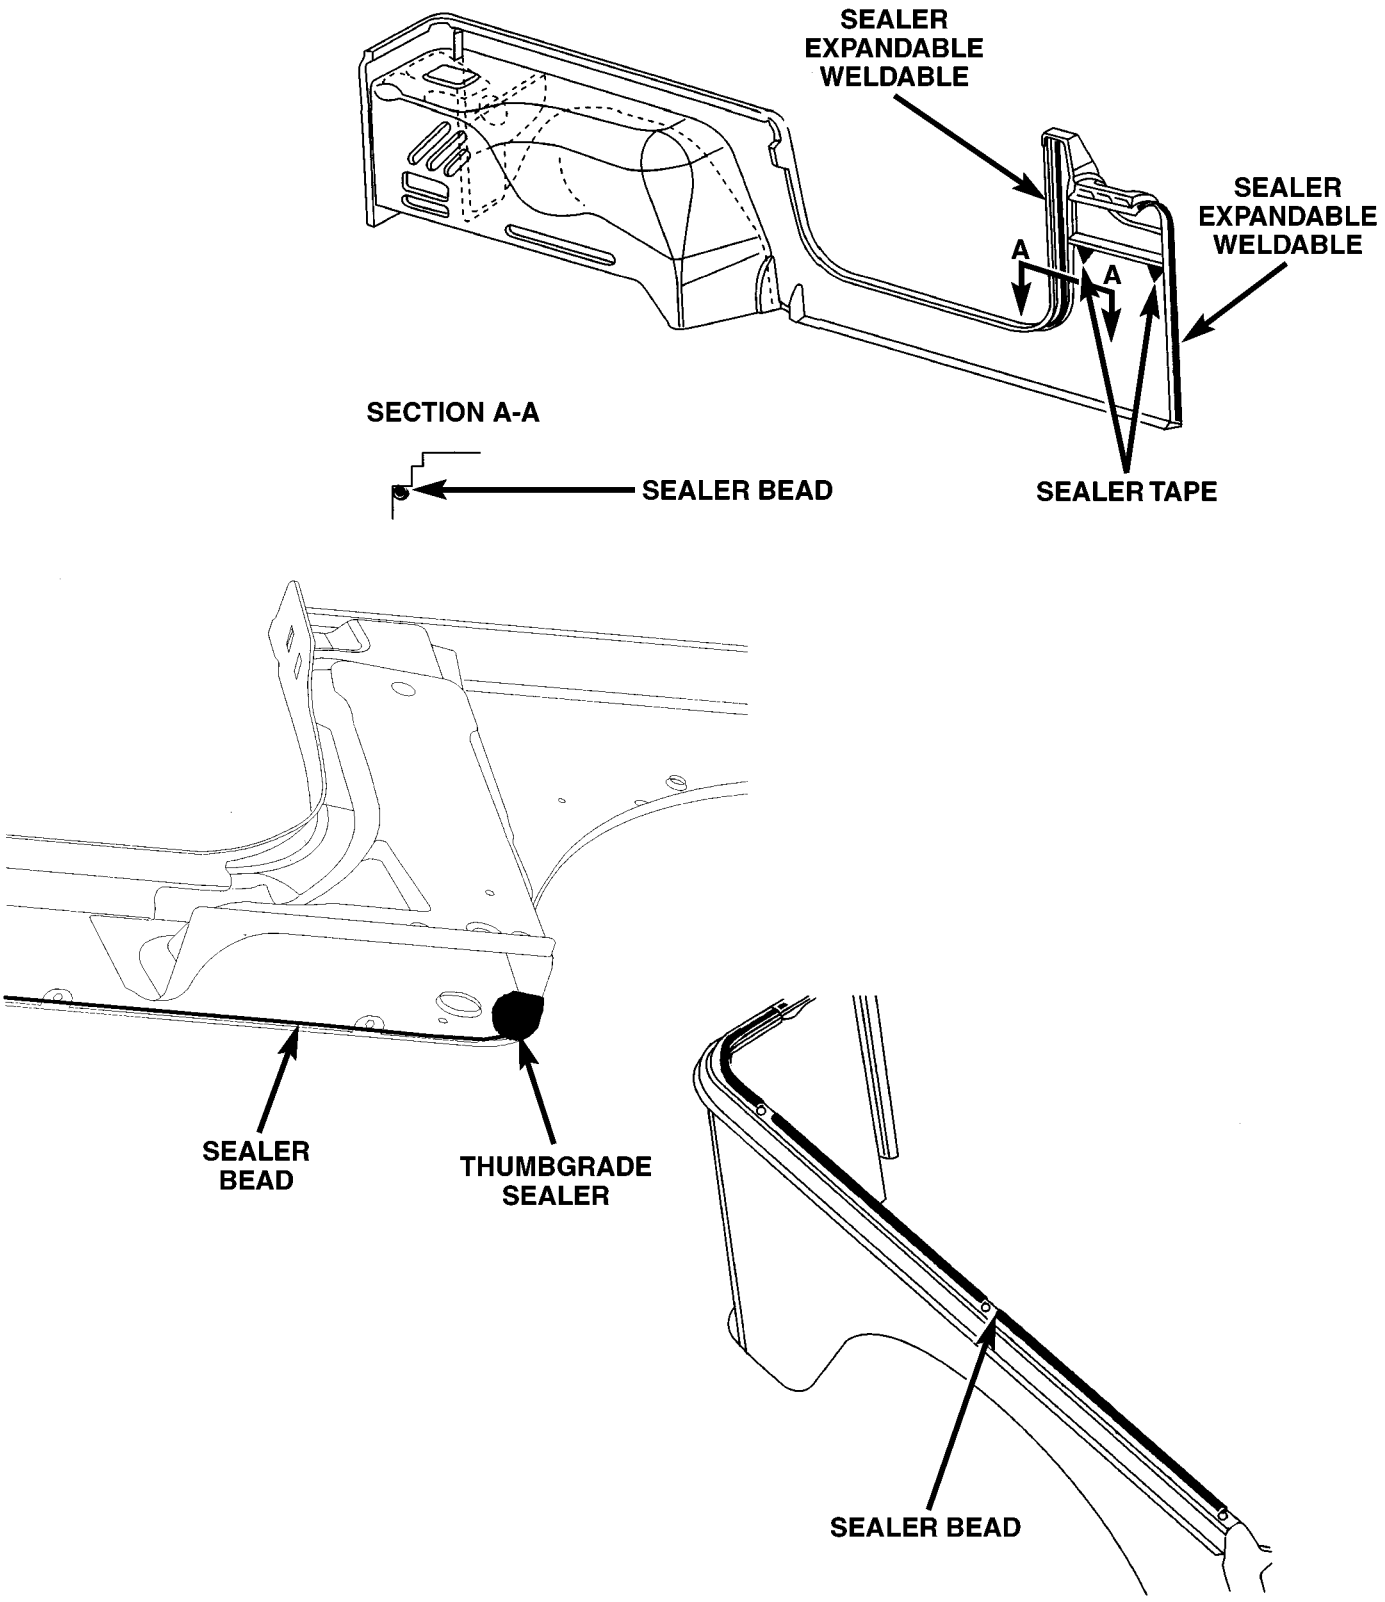

Fig. 24 BODY SIDE APERTURE