

MMS Flowmaster: Uroflow


Test



Gender: Male
Date of birth: 12/12/2000
Patient number:

Investigation date/time: 10/03/2025 / 10:57
Investigation number:
Hospital: MMS, the Netherlands

Print date: 10/03/2025
Print time: 10:57
Flowmaster: MMS FLOWMETER - PE14-9FLMB5900

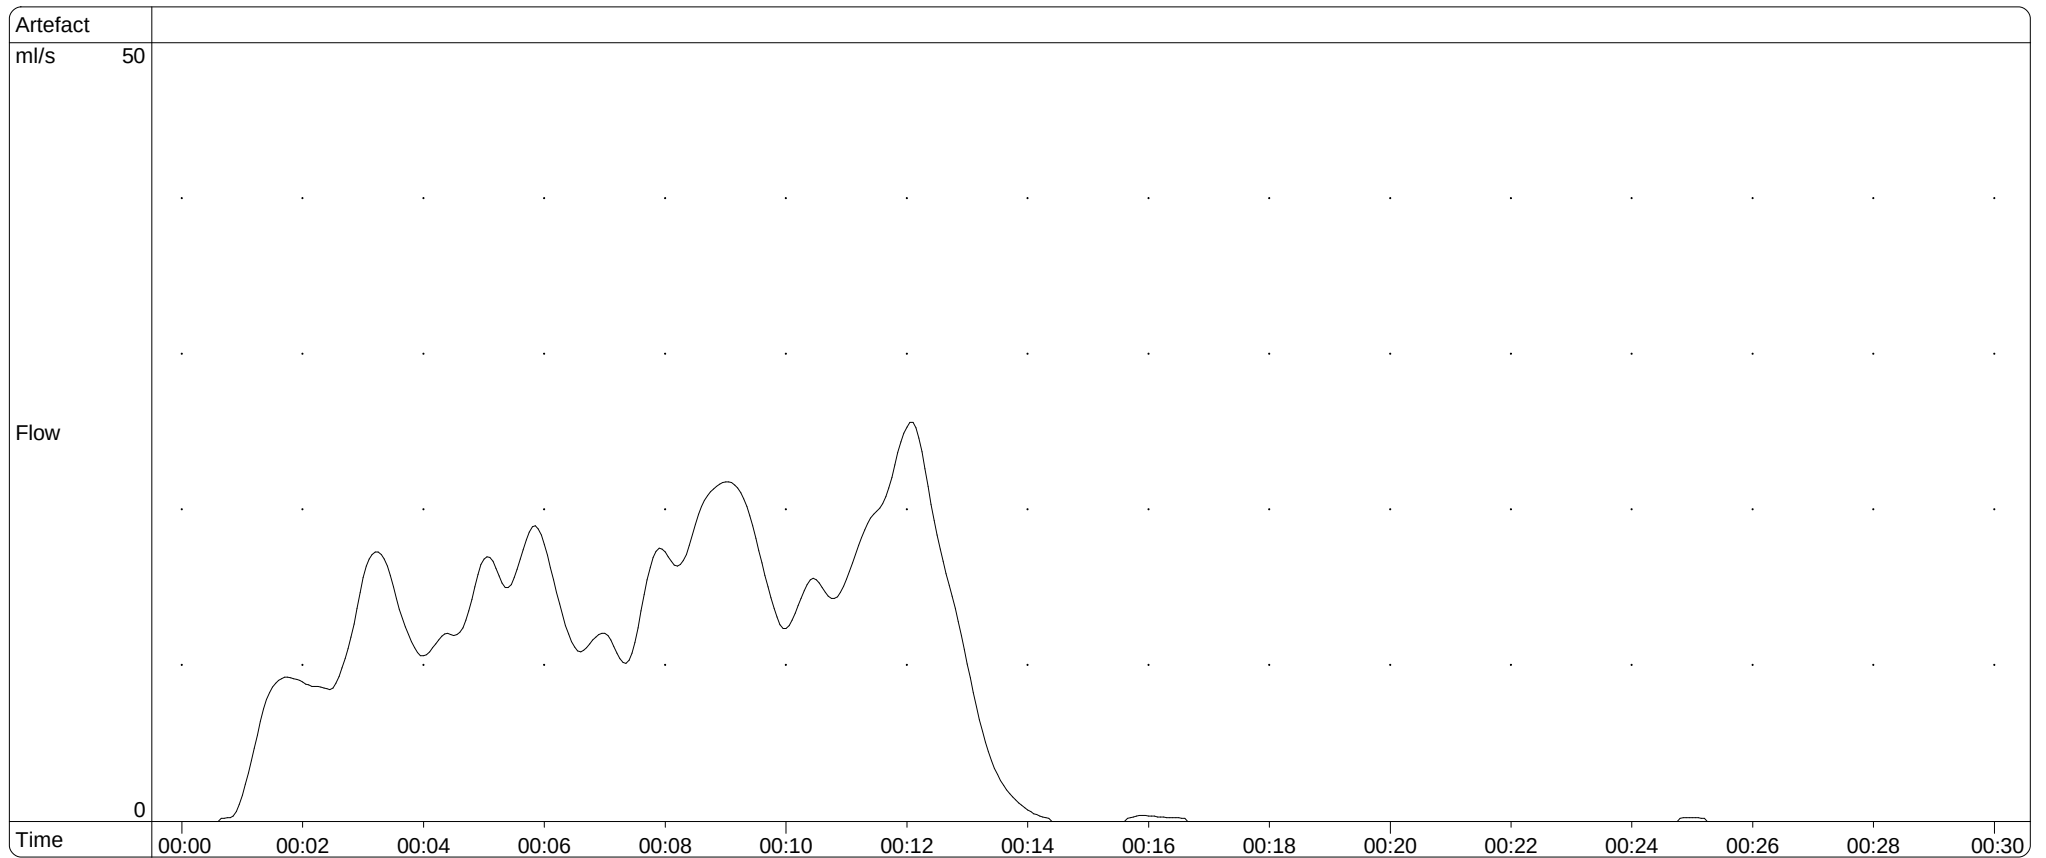

Results

Average flow rate : 12.4 ml/s
Maximum flow rate : 25.6 ml/s
Time to maximum flow : 11.2 s
Voided volume : 183.1 ml
Flow time : 14.0 s
Voiding time : 15.5 s
Intervals : 2

Comments
