

MMS Flowmaster: Uroflow


Test



Gender: Male
Date of birth: 11/11/1997
Patient number:

Investigation date/time: 22/01/2025 / 12:22
Investigation number:
Hospital: MMS, the Netherlands

Print date: 22/01/2025
Print time: 12:27
Flowmaster: MMS FLOWMETER - PE14-9FLMB5900

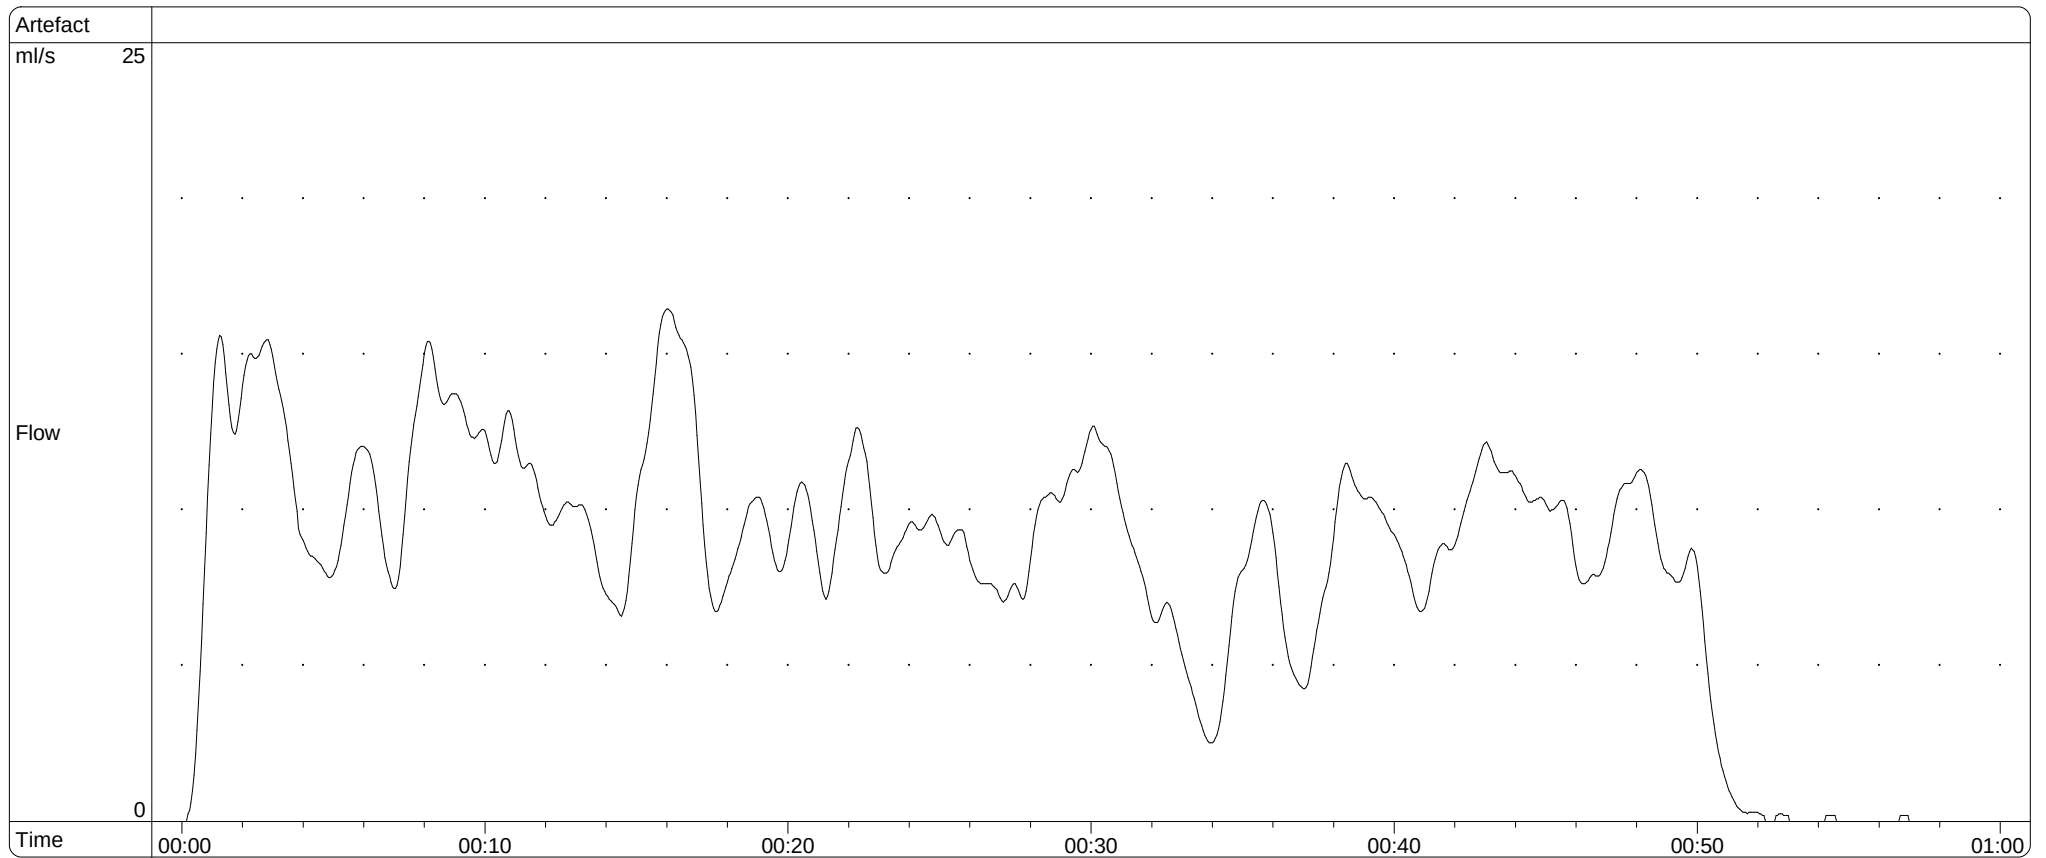

Results

Average flow rate : 9.2 ml/s
Maximum flow rate : 16.5 ml/s
Time to maximum flow : 15.8 s
Voided volume : 489.6 ml
Flow time : 51.8 s
Voiding time : 51.8 s
Intervals : 1

Comments
