

Gradient-Sensitive Functional Descriptors for Interferometric Surface Metrology: Complementing Amplitude-Averaging ISO Parameters

Abstract

This paper presents a complete interferometric pipeline for optical evaluation of roundness and surface profiles using a self-built Michelson interferometer. The method is validated on two certified JENOPTIK standards: the roundness standard FN 111 (24,000 interferograms) and the magnification standard FN 101 with a certified Flick flat (100,000 interferograms), each measured in five 400° sweeps. External validation against 104 tactile reference measurements yields an E_n score of 0.61 for the FN 111 and 0.3% agreement for the FN 101, demonstrating metrological consistency of the optical reconstruction. In addition to conventional profile roughness parameters (ISO 21920-2, formerly ISO 4287) and roundness metrics ($RONt$, $RONq$), the reconstructed nanometre profiles are analysed using functional-analytic descriptors including L^p , Sobolev $W^{1,2}$, and bounded-variation (BV) norms. Controlled defect-injection experiments and analysis of the certified Flick flat show that gradient-based descriptors provide complementary sensitivity to localised geometric features that may remain below the detection threshold of amplitude-averaging parameters. For a 100 nm synthetic spike, BV density increased by 18% and the $W^{1,2}$ seminorm by 622%, while R_a showed no detectable response at the reconstruction resolution. The BV descriptor also detected the certified Flick flat in a sliding-window analysis where R_a remained insensitive. These results suggest that functional descriptors can complement standard profile and roundness parameters, providing additional information on localised geometric variations without requiring changes to the measurement hardware. All reported uncertainties are within-

run repeatability estimates from five sweeps of a single continuous rotation and should be interpreted as lower bounds; an indicative type-B uncertainty budget is provided.

Keywords: interferometry, roundness, surface profile, functional norms, bounded variation, Sobolev seminorm, uncertainty

1. Introduction

Surface topography is one of the most important properties of technical parts. The accuracy of form and roughness influences contact conditions, wear and lifetime. Roundness, understood as deviation from a perfect circle, remains a central requirement in precision manufacturing; Zhu et al. emphasised that precise measurements are needed both for form tolerances and for tribological surface texture assessment [1]. At nanometric scale, such measurements require high-precision optical systems [2]. The foundational reference for surface metrology terminology and parameter definitions is the handbook of Whitehouse [3].

Optical dimensional metrology has a long connection with interference [4]. Modern optical surface metrology relies on diffraction, polarisation and interference [5, 6]. Diffraction and scattering have been applied to roughness measurement in several distinct ways: Brodmann introduced a scattered-light roughness instrument for production environments [7] and subsequently extended the scattered-light principle to combined roughness, form and waviness measurement [8]; Fan and Huynh analysed light scattering from flat periodic rough surfaces to estimate roughness parameters [9]; Hertzsch et al. demonstrated model-based scatterometry for microtopographic analysis of turned surfaces [10]; and a low-cost scatterometry setup achieving nanometric precision in fast roughness measurement has been reported previously [11]. Interference remains central for ultra-precise surface-form measurement, from the early interference-based length comparisons of Benoît [12] to modern large-scale precision optics programmes [13]. De Groot systematised the principles of phase-shifting and coherence-scanning interference microscopy for topography evaluation [14, 15],

25 and Chatterjee described phase-evaluation interferometric testing of reflective
26 surfaces [16].

27 Several interferometric instruments have been proposed for high-accuracy
28 surface and roundness measurement. Polack et al. described a Michelson-based
29 system for surface-shape determination built around a high-resolution stitching
30 interferometer developed by Thomasset et al. [17, 18]. Fan et al. presented
31 a roundness measuring system for microspheres based on two small Michel-
32 son interferometers [19]. Kuhnel et al. proposed an interferometric system for
33 roundness and cylindricity measurement of ring gauges with 0.1 nm resolution
34 over a large measurement range [20]. Commercial instruments can be highly ac-
35 curate, but they are often costly and may not expose the full acquisition chain
36 needed for experimental method development.

37 The numerical analysis of fringe patterns has its own methodological lineage,
38 which frames the phase-decoding route used here. Takeda et al. introduced the
39 Fourier-transform method of fringe-pattern analysis, in which a spatial carrier
40 allows the phase to be recovered from a single interferogram without temporal
41 phase shifting [21]. Kemaio extended this concept with the two-dimensional win-
42 dowed Fourier transform, which processes the fringe pattern locally to improve
43 robustness to noise and local fringe-quality variations [22]. More recently, Feng
44 et al. demonstrated that deep neural networks can be trained to perform fringe
45 analysis, substantially enhancing the accuracy of phase demodulation from a
46 single fringe pattern [23]. Galaktionov and Toporovsky proposed a multi-stage
47 fringe-map reconstruction algorithm for fibre-end surface analysis in non-phase-
48 shifting interferometry, combining moving-average and Fourier-transform filter-
49 ing with polynomial fitting and reporting agreement within 2% of a commercial
50 phase-shifting interferometer [24]. The radial excess-fraction method used in the
51 present work belongs to this single-frame, non-phase-shifting family: each inter-
52 ferogram is decoded independently through the geometry of its circular fringes,
53 which suits continuous-rotation acquisition where temporal phase stepping is
54 impractical.

55 The present work uses a self-built, non-contact Michelson-type roundness

56 measurement system assembled from off-the-shelf components. The optical
 57 setup, apparatus description and radial image-processing route for phase extrac-
 58 tion were published in a previous study [25], where only roughness parameters
 59 were reported for the ceramic standard FN 111. The present work extends that
 60 study in three directions: (i) roundness ($RONt$, $RONq$) is evaluated for the first
 61 time with this self-built optical setup, (ii) a second artefact — the JENOPTIK
 62 magnification standard FN 101 with a Flick flat — is measured and validated
 63 against its DAkkS-DKD certificate, and (iii) a controlled sensitivity-comparison
 64 methodology is introduced: synthetic defects of known geometry are injected
 65 into measured profiles, and the response of classical ISO parameters is com-
 66 pared against that of L^p , Sobolev $W^{1,2}$, and bounded-variation (BV) norms
 67 — standard tools of functional analysis here applied to interferometric profile
 68 metrology — all computed from the same nanometre residual. The comparison
 69 framework, rather than any individual norm, constitutes the methodological
 70 contribution.

71 The computational problem is that modern interferometric surface metrol-
 72 ogy records long image sequences before a numerical profile exists. In the present
 73 data, however, each PNG file is already a separate interferogram in which the
 74 phase is encoded spatially by the bright and dark fringes inside the image. The
 75 files in the FN 111 and FN 101 folders are therefore not treated as a temporal
 76 phase-shifting stack of one fixed scene. Instead, each image $I_i(x, y)$ is processed
 77 independently to obtain one wrapped excess-fraction value ϵ_i . The ordered se-
 78 quence of these values is then unwrapped over image order and converted to a
 79 nanometre profile. The full measurement archive contains 24,000 grayscale in-
 80 terferograms of the FN 111, with image size 648×488 px, and 100,000 grayscale
 81 interferograms of the JENOPTIK magnification standard FN 101, with image
 82 size 640×480 px.

83 The literature relevant to this comparison is mature but only partly con-
 84 nected. In interferometric testing, Dumas et al. extended the lateral range of
 85 interferometry through subaperture stitching [26]; Chen et al. developed an it-
 86 erative stitching algorithm for spherical surfaces [27] and subsequently applied

87 stitching to the testing of large optical surfaces [28]; Iacchetta et al. addressed
 88 rotation and translation registration of band-limited interferometric images us-
 89 ing a chirp z-transform [29]; and Burge et al. applied computer-generated holo-
 90 grams to the measurement of x-ray and EUV optics [30]. On repeatability,
 91 Quan et al. compared evaluation approaches for interferometric surface repeata-
 92 bility [31], and Zhang et al. compared repeatability across different interference
 93 systems [32]; both characterise repeatability through RMS/PV quantities or
 94 pixel-wise standard-deviation matrices, i.e., through amplitude statistics. Pap-
 95 pas et al. propagated the uncertainty of areal surface-texture parameters using
 96 the metrological-characteristics approach, embedding texture parameters in a
 97 GUM-style framework [33]. In statistics, Gertheiss et al. reviewed functional
 98 data analysis as a language for function-valued observations [34], and Happ et
 99 al. provided a framework separating amplitude and phase variation in functional
 100 data [35]. Scale-dependence has been examined by Wolf, who connected surface
 101 topography with topological description [36], by Sanner et al., who defined scale-
 102 dependent roughness parameters for topography analysis [37], and by Zhao et
 103 al., who studied fractal simulation of topography for lubrication prediction [38];
 104 collectively these show that surface characterisation depends on bandwidth and
 105 filtering scale.

106 None of these strands, however, resolves a specific practical problem of pro-
 107 file and roundness metrology. When a localised geometric feature — a flat, a pit,
 108 a scratch — is present on an otherwise smooth artefact, amplitude-averaging
 109 parameters such as R_a dilute its signature over the entire evaluation length,
 110 so the feature can remain numerically invisible although it is metrologically
 111 relevant. Existing remedies do not fully address this for profile data: areal
 112 parameters require calibrated height maps that single-image radial extraction
 113 does not provide; visual inspection of polar plots is operator-dependent and not
 114 quantitative; and template-based defect detectors require the defect geometry
 115 to be known in advance. The unresolved question addressed here is therefore
 116 whether gradient-sensitive functional norms — whose mathematical structure
 117 makes them respond to localised slope content rather than to averaged am-

118 plitude — provide reproducible, quantifiable sensitivity to such features when
 119 computed from the same reconstructed residual as the standard ISO param-
 120 eters, and how large that sensitivity advantage is under controlled conditions.
 121 What has been missing in the literature is precisely this controlled, like-for-like
 122 comparison on identical nanometre residuals with external tactile validation.
 123 The present work addresses this by: (i) injecting synthetic defects of known ge-
 124 ometry into measured profiles to quantify descriptor response under controlled
 125 conditions; (ii) applying the full pipeline to two DAkS-DKD-certified arte-
 126 facts at large scale (24,000 and 100,000 interferograms) with a self-built radial
 127 excess-fraction interferometer; and (iii) benchmarking the optical reconstruc-
 128 tion against 104 tactile reference measurements. Areal parameters are not re-
 129 ported because the single-image radial extraction does not produce a calibrated
 130 areal height map. The aim is to assess whether L^p , bounded-variation, and
 131 Sobolev seminorms, evaluated alongside ISO 21920-2 profile parameters on the
 132 same reconstructed residual profile, offer complementary descriptive sensitivity
 133 to controlled profile perturbations, and to evaluate the within-run repeatability
 134 of all quantities across five recorded sweeps. No claim of novelty is attached
 135 to the norms themselves — they are standard tools of functional analysis, and
 136 the functional-analytic vocabulary is used only as an organising taxonomy; the
 137 controlled comparison framework is the contribution.

138 **2. Experimental Details**

139 *2.1. Optical Setup*

140 The optical layout of the measurement system is shown in Fig. 1. The
 141 system is a two-channel modified Michelson interferometer with channels shifted
 142 by approximately 90° in phase. When an array detector is used instead of a
 143 point detector, the second channel is not strictly required [39]. In this system it
 144 was retained because it is useful for object centring and can serve as a control
 145 channel.

146 The optical setup and the full apparatus-level description were reported in a
 147 previous study on radial image processing for phase extraction in rough-surface
 148 interferometry [25]. They are repeated here in condensed form to make the
 149 present functional-descriptor analysis self-contained and to document the ac-
 150 quisition conditions behind the FN 111 and FN 101 interferogram archives.

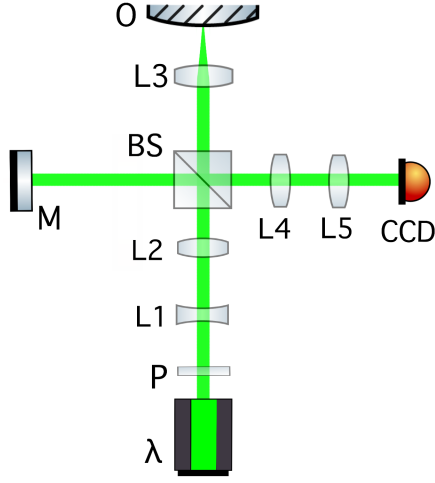


Figure 1: Optical layout of the two-channel modified Michelson interferometer: λ – diode laser (532 nm); P – linear polariser; L – lenses; L_3 – microscope objective; M – reference mirror ($\lambda/10$ flatness); BS – non-polarising beamsplitter; O – object on rotation stage; CCD – camera.

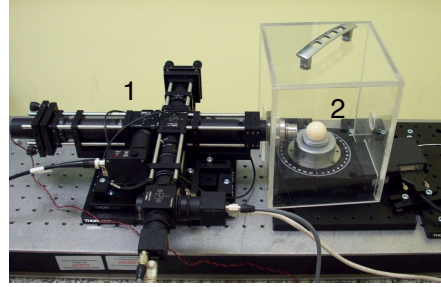


Figure 2: The complete measurement system: (1) modified Michelson interferometer in cage mounting, (2) high-precision rotation stage with the artefact.

151 The system was first tested with the JENOPTIK roundness standard FN 111
 152 (photographs: Supplementary Fig. S1) (Al_2O_3 , $\varnothing = 29.9588$ mm) [40]. A single-
 153 mode 4.5 mW diode laser with wavelength 532 nm was used as the light source.
 154 A current-stabilised supply powered the laser to obtain a stable wavelength [41].
 155 The laser beam passes through a polariser (P in Fig. 1) to set the polarisation
 156 of the light at 45° to the setup plane, minimising the difference in reflectivity
 157 between the two channels.

158 Key components: achromatic lenses $L_{1,2,4,5}$, non-polarising beamsplitter

159 BS , $\lambda/8$ liquid phase retarder, $\lambda/10$ reference mirror M , DIN-4 microscope
 160 objective L_3 (NA 0.10), polarising beamsplitter PBS , and two Gigabit Ether-
 161 net CCD cameras (640×480 px, 120 fps).

162 The interferometer was built in a cage system for thermal, acoustic and me-
 163 chanical stability. A plexiglass box shields the measurement object, and the
 164 structure is mounted on an area translation stage. A high-precision rotation
 165 stage (encoder accuracy 2.0 mdeg, typical wobble $\pm 12 \mu\text{rad}$, typical eccentric-
 166 ity $\pm 0.40 \mu\text{m}$; full specifications: Supplementary Table S1) rotates the object.
 167 Both interferometer and stage are mounted on a honeycomb breadboard with
 168 vibration isolation.

169 Measurements were performed at night (23:00–05:00) to minimise building-
 170 activity disturbances. The setup was thermally and acoustically shielded (plex-
 171 iglass box, wool blanket) and placed on a granite plate on layered wooden-
 172 polystyrene vibration isolation (photographs: Supplementary Fig. S2). Five
 173 semiconductor temperature sensors ($\pm 0.2^\circ\text{C}$) monitored stability; the tempera-
 174 ture near the reference and object arms remained stable to $\pm 0.2^\circ\text{C}$ over six-hour
 175 acquisitions.

176 2.2. Control System and Acquisition Workflow

177 Cameras were controlled by FLIR SDK-based C programs and Bash scripts [42].
 178 Capture time was recorded per frame for angular-position verification. The ro-
 179 tation stage was controlled via USB ASCII commands [43]; a 25 s settling delay
 180 ensured constant velocity before acquisition began. Object centring was per-
 181 formed manually using the two-camera phase-shifted configuration at 45° rota-
 182 tion increments. Fringe evaluation used modified open-source R code [39, 44].
 183 Table 1 lists the acquisition parameters for both archives; five 400° sweeps were
 184 recorded per artefact, with the 40° overlap retained for profile-end comparison.

185 The object was measured in one continuous five-sweep rotation without repo-
 186 sitioning. Each recorded sweep spans 400° ; successive useful 360° segments are
 187 shifted by 40° , giving a natural between-sweep angular offset. The 40° overlap
 188 region provides a model-free repeatability check: RMS height difference between

Table 1: Measurement and sampling parameters of the interferometric acquisition workflow.

Parameter	FN 111	FN 101
Rotation speed, ω	0.50 °/s	0.08 °/s
CCD frame rate	6 fps	4 fps
Recorded sweeps, n	5	5
Total frames, N	24,000	100,000
Angular step, $\Delta\alpha = \omega/\text{fps}$	0.083°/frame	0.020°/frame
Frames per degree	12	50
Frames per useful 360°	4320	18,000
Frames per recorded 400° sweep	4800	20,000
Overlap per sweep	40° / 480 frames	40° / 2000 frames
Total acquisition time	4000 s	25,000 s

consecutive sweeps is 12 nm (FN 111) and 0.18 μm (FN 101), consistent with Table 3.

The frame rates in Table 1 (6 and 4 fps) are far below the 120 fps capability of the cameras and merit comment. The angular step is set by the ratio $\Delta\alpha = \omega/\text{fps}$, so angular resolution is governed jointly by rotation speed and frame rate; measurement time is governed by rotation speed alone. The rotation speeds (0.50 and 0.08 °/s) were deliberately conservative: slow, constant-velocity rotation minimises dynamic excitation of the stage and keeps the fringe pattern quasi-static within each exposure, and the settling-time protocol (25 s before acquisition) assumes steady-state velocity. At these speeds, 6 and 4 fps already yield 12 and 50 frames per degree — an oversampling factor of roughly 300 and 1200 relative to the 15 UPR metrological bandwidth — so the frame rate was not the accuracy-limiting factor; increasing it at fixed rotation speed would only add redundant frames. Shorter total acquisition (4,000 and 25,000 s here) would instead require faster rotation with a proportionally higher frame rate, which is technically feasible with the present cameras up to 120 fps. Whether fringe contrast and stage stability are preserved at, say, a tenfold higher speed

has not been tested; the trade-off between acquisition speed, vibration robustness, and per-frame phase-extraction quality is identified as a topic for future work, since measurement time is a critical parameter for industrial implementation.

3. Image Processing and Functional-Descriptor Method

3.1. Processing Pipeline

The pipeline follows the radial excess-fraction method of a previous study [25] with added sinusoidal refinement. Each interferogram $I_i(x, y)$ is decoded independently to a wrapped excess fraction ϵ_i ; the sequence is unwrapped chronologically, converted to nanometres ($z_i = \nu_i \lambda / 2$), and reduced by the object-specific LSCI reference model. Sweep boundaries are retained for repeatability analysis.

3.2. Step-by-Step Radial Phase Decoding

For each interferogram $I_i(x, y)$, a radial intensity profile about the fringe centre is extracted and B-spline-smoothed; bright-ring maxima are detected in D^2 space, where circular-fringe theory gives $D_{ij}^2 = c_i(j + \epsilon_i - 1)$ for the j th ring of diameter D_{ij} . A linear fit $D_{ij}^2 = \alpha_i j + \beta_i$ yields the wrapped excess fraction $\epsilon_i = (1 + \beta_i / \alpha_i) \bmod 1$ (2). Where the radial fringe signal permits ($R^2 \geq 0.65$, phase within 0.20 fringe of the ring-diameter estimate), a sinusoidal refinement is applied; otherwise the ring-diameter estimate is retained. The ordered series ϵ_i is unwrapped chronologically to a continuous fringe-order coordinate ν_i , and the nanometre profile follows from $z_i = \nu_i \lambda / 2$ with $\lambda = 532$ nm (one fringe order $\equiv 266$ nm) (3).

$$D_{ij}^2 = c_i(j + \epsilon_i - 1), \quad (1)$$

$$\epsilon_i = \left(1 + \frac{\beta_i}{\alpha_i}\right) \bmod 1. \quad (2)$$

$$z_i = \nu_i \frac{\lambda}{2}, \quad \lambda = 532 \text{ nm}. \quad (3)$$

230 3.3. Topography Profile, Reference Removal and Eccentricity Reduction

231 After phase-to-height conversion, the roundness profile is extracted following
 232 ISO 12181-1 [45] (which supersedes the withdrawn ISO 4291). For each 360°
 233 segment, a least-squares reference circle (LSCI) is fitted to the angular height
 234 profile $z_i = h(\theta_i)$ in Cartesian coordinates:

$$(x_i, y_i) = ((R_0 + z_i) \cos \theta_i, (R_0 + z_i) \sin \theta_i), \quad (4)$$

235 where $R_0 = 14.9794$ mm is the nominal radius of the JENOPTIK FN 111. The
 236 LSCI centre (x_c, y_c) minimises $\sum_i [\sqrt{(x_i - x_c)^2 + (y_i - y_c)^2} - R_0]^2$, yielding the
 237 centred radial residuals ρ_i . The LSCI fit is numerically equivalent to removing
 238 the first harmonic of the angular profile, but it provides the formal ISO 4291
 239 reference circle required for roundness metrology. After LSCI centring, a phase-
 240 correct Gaussian low-pass profile filter with 50% transmission at 15 undulations
 241 per revolution (UPR) is applied to the residual profile, consistent with the filter
 242 specification used for the tactile reference measurements and with the Gaussian
 243 profile filter defined in ISO 16610-21. All classical and gradient-based descriptors
 244 are computed from this LSCI-centred, Gaussian-filtered residual $\rho_i^{(\text{filt})}$.

245 For the JENOPTIK magnification standard FN 101, the same processing
 246 chain is applied: a linear trend is removed from the unwrapped phase se-
 247 quence before height conversion (Sec. 5.1), the LSCI reference circle is fitted
 248 to the angular profile, and the Gaussian low-pass filter (50% at 15 UPR) is
 249 applied. Although both artefacts are processed through identical filtering steps,
 250 the 15 UPR cutoff corresponds to different spatial wavelengths on the circum-
 251 ference: $2\pi \times 14.9794 \text{ mm} / 15 = 6.27 \text{ mm}$ for the FN 111 ($\varnothing = 29.9588 \text{ mm}$) and
 252 $2\pi \times 15 \text{ mm} / 15 = 6.28 \text{ mm}$ for the FN 101 ($\varnothing \approx 30 \text{ mm}$) — effectively identical.
 253 The angular sampling differs substantially (0.083° vs. 0.020° , Table 1), but the
 254 Gaussian filter sigma is set by the UPR cutoff, not by the sampling interval, so
 255 the filtered profiles are directly comparable.

256 3.4. Classical Profile and Roundness Metrics

257 All classical quantities are evaluated on nanometre residuals, not on raw
 258 intensities, following the profile method of ISO 21920-2 [46], which supersedes
 259 the earlier ISO 4287 [47]; the amplitude-parameter definitions used here are
 260 common to both documents, and ISO 4287 is retained as a secondary reference
 261 because the tactile comparison data and the previous study [25] predate the
 262 transition. Areal parameters (ISO 25178 [48]) are not reported because the
 263 single-image radial extraction does not produce a calibrated areal height map.
 264 For a residual profile or vector of residual pixels p , the reported profile-style
 265 roughness descriptors are

$$R_a = \frac{1}{M} \sum_{j=1}^M |p_j - \bar{p}|, \quad R_q = \left[\frac{1}{M} \sum_{j=1}^M (p_j - \bar{p})^2 \right]^{1/2}, \quad (5)$$

266 and

$$R_z = \max_j (p_j - \bar{p}) - \min_j (p_j - \bar{p}). \quad (6)$$

267 As implemented, this quantity is the global peak-to-valley height of the full eval-
 268 uation profile, corresponding to the total-height parameter (Rt in ISO 21920-2
 269 terms) rather than the section-averaged Rz ; the symbol R_z is retained for conti-
 270 nuity with the previous study [25]. This implementation detail is relevant to the
 271 interpretation of Table 3 (Sec. 4.3). The profile skewness R_{sk} and kurtosis R_{ku}
 272 — ISO 21920-2 shape parameters that characterise asymmetry and peakedness
 273 of the height distribution — are also reported:

$$R_{sk} = \frac{1}{R_q^3} \frac{1}{M} \sum_{j=1}^M (p_j - \bar{p})^3, \quad R_{ku} = \frac{1}{R_q^4} \frac{1}{M} \sum_{j=1}^M (p_j - \bar{p})^4. \quad (7)$$

274 $R_{sk} = 0$ for a symmetric distribution; $R_{sk} < 0$ indicates a predominance of val-
 275 leys over peaks. $R_{ku} = 3$ for a normal distribution; $R_{ku} > 3$ indicates a spikier
 276 (leptokurtic) profile. These are the only ISO 21920-2 amplitude-distribution pa-
 277 rameters that capture distribution shape beyond amplitude averages, and their
 278 inclusion allows a direct test of whether gradient-based descriptors provide in-
 279 formation beyond even the best ISO shape parameters. For the eccentricity-

corrected ceramic angular profile $q_C(\theta)$,

$$RONt = \max_{\theta} q_C(\theta) - \min_{\theta} q_C(\theta), \quad RONq = \left[\frac{1}{2\pi} \int_0^{2\pi} q_C^2(\theta) d\theta \right]^{1/2}. \quad (8)$$

These are profile/form quantities in nanometres. B-spline pre-smoothing (20 degrees of freedom, $\approx 18^\circ$ period) stabilises the LSCI fit; the subsequent Gaussian low-pass filter (50% at 15 UPR, ISO 16610-21) defines the metrological bandwidth. All descriptors are computed from the same Gaussian-filtered residual.

3.5. Functional Gradient-Based Descriptors

The concept of a complete normed vector space originates from the foundational work of Banach [49]. For discrete profile data of finite length N , the vector space $\mathbb{R}^N$ equipped with any norm is a Banach space; the present work does not invoke infinite-dimensional completeness but draws on the taxonomy of L^p , Sobolev, and bounded-variation norms that Banach’s framework systematised. For a centred residual profile $p(s)$ and $1 \leq p < \infty$,

$$\|p\|_p = \left(\frac{1}{L} \int_0^L |p(s)|^p ds \right)^{1/p}, \quad \|p\|_\infty = \max_{s \in [0, L]} |p(s)|. \quad (9)$$

The reported functional descriptors include L^1 , L^2 , L^∞ , the one-dimensional Sobolev $W^{1,2}$ seminorm and the bounded-variation (BV) total variation,

$$|p|_{W^{1,2}} = \left(\int_0^L \left| \frac{dp}{ds} \right|^2 ds \right)^{1/2}, \quad TV(p) = \int_0^L \left| \frac{dp}{ds} \right| ds. \quad (10)$$

In discrete form, for a uniformly sampled profile p_j ($j = 1, \dots, N$) with angular spacing $\Delta\alpha$,

$$|p|_{W^{1,2}} \approx \left(\Delta\alpha \sum_{j=1}^{N-1} \left(\frac{p_{j+1} - p_j}{\Delta\alpha} \right)^2 \right)^{1/2}, \quad TV(p) \approx \sum_{j=1}^{N-1} |p_{j+1} - p_j|. \quad (11)$$

Both $W^{1,2}$ and BV density carry sampling-interval dependence; “nm sample⁻¹” is retained in the result tables for the fixed-acquisition setup, and a standardised angular-unit convention for cross-instrument comparison is defined in Sec. 3.6.

The curvature RMS (root-mean-square of the discrete second derivative; reported in Supplementary Table S2) carries a $(\Delta\alpha)^{-2}$ sampling dependence and should not be compared across instruments with different angular resolution.

3.6. Angular-Unit Convention for Sampling-Dependent Descriptors

Gradient-based descriptors evaluated on discretely sampled profiles depend on the sampling interval: the discrete total variation of an unfiltered profile grows as the sampling grid refines (noise contributes gradient content at every scale), so raw per-sample values are instrument-specific. For meaningful cross-instrument comparison the following convention is proposed and used here.

1. **Band-limit first.** The profile is filtered with a declared phase-correct Gaussian profile filter (ISO 16610-21) at a stated cutoff in undulations per revolution (here 50% transmission at 15 UPR). After band-limiting, the profile derivative is bounded and the discrete sums converge to the continuous integrals as $\Delta\alpha \rightarrow 0$; the descriptor then characterises the declared bandwidth rather than the sampling grid.
2. **Sample adequately.** The angular sampling must resolve the declared bandwidth with margin; at least ten samples per cutoff undulation are recommended. Here the FN 111 and FN 101 profiles carry ≈ 290 and ≈ 1200 samples per 15-UPR undulation, so discretisation error is negligible.
3. **Report in angular units.** The BV density is reported as total variation per unit angle, $BV_\theta = TV(p)/\Theta$ in nm deg^{-1} ($\Theta = 360^\circ$), and the gradient content as the RMS angular gradient $g_{\text{rms}} = [\frac{1}{N-1} \sum_j ((p_{j+1} - p_j)/\Delta\alpha)^2]^{1/2}$ in nm deg^{-1} , together with the filter cutoff. For comparison across artefacts or instruments of *different diameter*, the angular unit is additionally converted to an arc-length unit by dividing by the arc length per degree, $\pi D/360$; the BV density is then $BV_s = TV(p)/(\pi D)$ in nm mm^{-1} . The arc-length form is the diameter-independent unit and is the one recommended for cross-instrument reporting, since nm deg^{-1} still scales with the circumference of the specific artefact.

A note on physical dimensions clarifies why this is necessary and is itself part of the answer to the redundancy question (Sec. 5.3). Amplitude descriptors (R_a , R_q , L^1 , L^2 , L^∞ , $RONt$) have the dimension of length (nm) and are sampling-independent. Gradient descriptors are dimensionally distinct: BV density and

the RMS gradient are height-per-length (nm mm^{-1}), i.e. dimensionless slopes, while the $W^{1,2}$ seminorm as defined here is $\text{height} \times \text{length}^{-1/2}$. This dimensional separation is the reason the gradient layer carries information that no amplitude parameter can encode, and also the reason its raw per-sample value must be qualified by a sampling and filter declaration.

For the present data, the per-sample values in Table 3 convert as follows. FN 111 ($\Delta\alpha = 0.083^\circ$): BV density $0.263 \text{ nm sample}^{-1} \rightarrow 3.2 \text{ nm deg}^{-1} \rightarrow 12.1 \text{ nm mm}^{-1}$; RMS gradient $0.310 \text{ nm sample}^{-1} \rightarrow 3.7 \text{ nm deg}^{-1} \rightarrow 14.2 \text{ nm mm}^{-1}$. FN 101 ($\Delta\alpha = 0.020^\circ$): BV density $6.58 \text{ nm sample}^{-1} \rightarrow 329 \text{ nm deg}^{-1} \rightarrow 1.26 \mu\text{m mm}^{-1}$; RMS gradient $8.76 \text{ nm sample}^{-1} \rightarrow 438 \text{ nm deg}^{-1} \rightarrow 1.67 \mu\text{m mm}^{-1}$, all at the 15-UPR cutoff. The two artefacts have almost identical circumference ($\pi D \approx 94.1$ and 94.2 mm), so the large difference in arc-length gradient content (12 versus 1257 nm mm^{-1}) reflects a genuine difference in surface variation rather than a unit artefact. Because each conversion is a fixed multiplicative factor for a given acquisition, relative uncertainties and relative defect responses are identical in every unit system. Adoption of gradient descriptors in reference software for roundness evaluation would require exactly this pair of declarations — filter cutoff and arc-length units — which parallels the established practice of declaring the filter for *RONt*.

3.7. Uncertainty Evaluation

Each dataset contains five 400° sweeps recorded in a single continuous rotation without stopping or repositioning. The five useful 360° segments are extracted from this continuous sequence; because each recorded sweep spans 400° , successive useful revolutions are shifted by 40° on the object. These segments are not strictly independent — they share the same continuous-run conditions (laser warm-up state, stage-bearing temperature, ambient drift). The standard deviation across sweeps therefore reflects within-run repeatability rather than between-run reproducibility. For a descriptor X evaluated on each sweep, the

mean value is $\bar{X}$ and the within-run standard uncertainty is estimated as

$$u_{\text{within}}(X) = \frac{s_X}{\sqrt{n}}, \quad n = 5, \quad (12)$$

where s_X is the sample standard deviation across the five sweeps. The reported expanded uncertainty is

$$U_{95}(X) = t_{0.975, n-1} u_{\text{within}}(X). \quad (13)$$

With $n = 5$, $t_{0.975, 4} = 2.776$; the χ^2_4 -based 95% CI for the standard deviation spans $[0.6s_X, 2.9s_X]$, so U_{95} is indicative rather than definitive. Because the five segments share continuous-run conditions (laser state, stage temperature, ambient drift), the $1/\sqrt{n}$ factor in u_{within} may underestimate the true uncertainty of the mean; all reported uncertainties are *lower bounds*. An indicative type-B budget for the principal systematic terms is given in Sec. 3.8; a complete GUM-compliant budget [50] with experimentally characterised input distributions, and a between-run reproducibility study with independent setups, thermal cycles, and physical re-centring of the artefact, remain future work (Sec. 5.6). With $n = 5$ sweeps and the observed within-run variability, the minimum detectable relative difference between two descriptors (80% power, $\alpha = 0.05$, two-sided paired t -test) is approximately 30% for the FN 111 and 5% for the FN 101, consistent with the exploratory character of the descriptor comparison. A per-sweep trend of FN 111 $RONt$ values gives a slope of 8.4 ± 4.1 nm sweep $^{-1}$ ($p = 0.12$), consistent with zero drift, though the sweep-to-sweep scatter cautions that U_{95} may underestimate long-term reproducibility.

3.8. Indicative Type-B Uncertainty Budget

Although a complete GUM budget requires between-run data that the present single-rotation acquisition cannot supply, the principal type-B contributions can be bounded from component specifications and pipeline properties. Table 2 summarises the estimates for the FN 111 $RONt$ evaluation; the same relative arguments apply to the FN 101.

385 *Laser wavelength stability.* The height scale $z = \nu\lambda/2$ inherits the relative
386 wavelength error: a ± 1 nm tolerance on the 532 nm diode module (rectangu-
387 lar distribution) gives a relative standard uncertainty of 0.11%, i.e. 0.3 nm on
388 $RONt = 278$ nm (and 46 nm on the FN 101 $RONt = 42.07$ μm , within its
389 ± 0.48 μm repeatability interval). Wavelength error acts as a pure scale factor
390 and cannot create or mask localised features.

391 *Refractive index of air.* The in-air wavelength varies with temperature and
392 pressure by $\sim 10^{-6}$ per 1°C or 3 hPa; with the observed $\pm 0.2^\circ\text{C}$ stability the
393 contribution is below 10^{-5} relative, i.e. < 0.01 nm. Negligible.

394 *Abbe error and stage wobble.* The specified axis wobble (± 12 μrad) enters
395 through two mechanisms: a cosine-type radial error $R\theta_w^2/2 \approx 1$ pm, and a lateral
396 beam walk $R\theta_w \approx 0.18$ μm on the circumference, equivalent to an angular
397 mislocation of 0.0007° , which maps through the local band-limited gradient
398 (≈ 3.2 nm deg^{-1} , Sec. 3.6) to ≈ 0.002 nm. Both are negligible after LSCI
399 first-harmonic removal.

400 *Camera nonlinearity and EFM localisation.* Intensity nonlinearity perturbs
401 the radial fringe-peak positions; its effect is bounded empirically by the per-
402 frame excess-fraction uncertainty of ± 0.05 fringe (13 nm). The 15-UPR band
403 limit averages ≈ 290 frames per resolved undulation, reducing the per-point
404 contribution to ≈ 0.8 nm and the peak-to-valley contribution to ≈ 1.1 nm.

405 *Long-term drift and phase noise floor (measured).* An independent static
406 stability session, recorded with the same interferometer, camera settings and
407 frame count as the FN 111 acquisition (24,000 frames over 4,000 s) but with the
408 object not rotating, provides a direct experimental bound on slow instrument
409 drift under realistic laboratory conditions. The decoded excess-fraction sequence
410 spans only 98 nm over the full session, with an end-to-end linear drift of -82 nm
411 (-1.1 nm min^{-1}), i.e. ≈ 15 nm over one 800 s sweep-equivalent interval; after
412 linear detrending the residual has 9.4 nm standard deviation (45 nm peak-
413 to-valley), and the frame-to-frame phase noise floor is 2.1 nm (0.008 fringe).
414 Two conclusions follow. First, the measured static noise floor is well below
415 the conservative ± 0.05 -fringe EFM bound used above, confirming that bound

as conservative. Second, the slow drift maps predominantly to low harmonic orders of the angular profile, where it is largely absorbed by the LSCI first-harmonic removal, and its sweep-to-sweep manifestation is already contained in the type-A scatter; the drift bound is therefore reported as an informative constraint rather than added in quadrature.

Form removal. The LSCI reference (first-harmonic removal) is exact only in the limaçon approximation; the second-order term $a^2/(2R)$ for residual centring eccentricity a leaks into the second harmonic of the residual. Manual centring leaves a of the order of tens of micrometres (the shared first-harmonic model of Sec. 5.2.1, with its 63 nm/0.18% per-sweep amplitude variation, implies $a \approx 35 \mu\text{m}$); for $a = 15\text{--}35 \mu\text{m}$ the term evaluates to 7–41 nm. Because this contribution is common to all five sweeps, it does not appear in the type-A scatter and must be carried as a bounded systematic term. Its magnitude is consistent with the 34 nm difference between the optical $RONt$ (278 ± 22 nm) and the certified tactile value (244 ± 52 nm), a difference that the $E_n = 0.61$ comparison shows to be within the combined uncertainties.

The quadrature combination is dominated by the type-A term, so the reported U_{95} values are essentially unchanged by the enumerated random type-B terms; the budget nevertheless shows that the leading unquantified risks are the form-removal systematic and the untested between-run effects, not the enumerated instrument terms.

3.9. Computational Implementation

The reconstruction workflow (`scripts/reconstruct_radial_profile_sequence.py`) decodes ϵ_i from each interferogram, unwraps the sequence, converts to nanometres, applies LSCI fitting and Gaussian low-pass filtering (50% at 15 UPR, ISO 16610-21), and exports CSV/JSON metrics with sweep-repeatability uncertainty. Vector PDF figures document each processing stage. The pipeline is invoked as `PYTHONPATH=src.venv/bin/pythonscripts/reconstruct_radial_profile_sequence.py` with dataset-specific parameters (full command in the data repository). Per-image excess-fraction decoding and unwrapping require approxi-

Table 2: Indicative type-B uncertainty budget for the FN 111 $RONt$ evaluation. Random contributions are standard uncertainties combined in quadrature with the type-A term; the form-removal term is a bounded systematic (bias) contribution common to all sweeps and is reported separately.

Source	Basis	Contribution to $RONt$
Within-run repeatability (type A)	$s/\sqrt{5}$, five sweeps	7.9 nm
Laser wavelength (± 1 nm, rect.)	module specification	0.3 nm
Air refractive index ($\pm 0.2^\circ\text{C}$)	Edlén-type sensitivity	< 0.01 nm
Abbe error / axis wobble ($\pm 12 \mu\text{rad}$)	stage specification, geometry	< 0.01 nm
Camera nonlinearity / EFM localisation	± 0.05 fringe per frame, band-limited averaging	1.1 nm
Long-term drift (measured, static session)	-1.1 nm min^{-1} ; ≤ 15 nm per sweep	informative bound [†]
Combined standard uncertainty u_c (random)	quadrature	8.0 nm
Expanded U_{95} (random, $t_{0.975,4}$)		22 nm
Form removal (limaçon second order)	$a^2/(2R)$, $a = 15\text{--}35 \mu\text{m}$	≤ 41 nm (syst. bound)

[†]Measured in an independent static session (Sec. 3.8); manifested in the type-A scatter and largely removed with the first harmonic, hence not added in quadrature.

446 mately 0.5 ms per frame (measured on an Intel Core i7-9700K, single-threaded
 447 Python 3.9), so the full 124,000-frame archive processes in under two minutes
 448 on consumer hardware.

449 **4. Results**

450 The results follow the updated radial sequence route only. Each raw im-
 451 age is first decoded to a wrapped excess fraction from its radial fringe pat-
 452 tern. The ordered excess-fraction series is then unwrapped in chronological
 453 order, converted to nanometres, and corrected for eccentricity. Finally, classi-
 454 cal profile/roundness descriptors and functional gradient-based descriptors are
 455 computed from the same nanometre residual profiles.

456 *4.1. Radial Phase Decoding and Nanometre Profile Reconstruction*

457 The FN 111 folder contained 24,000 interferograms and the steel folder con-
 458 tained 100,000 interferograms. The reported run used full-resolution images, the
 459 central radial aperture of 240 px, B-spline-smoothed peak detection, continuity-
 460 aware EFM peak-subset tracking and an EFM prominence threshold of 0.04 of
 461 the radial fringe-signal range. All five recorded sweeps were processed.

462 Figs. S3-S6 (single-image EFM and sequence processing steps) are provided
 463 in the Supplementary Materials.

464 *4.2. Roughness, Roundness and Functional Descriptors*

465 Table 3 gives the numerical comparison after LSCI reference circle and Gaus-
 466 sian low-pass filtering (50% at 15 UPR). Both artefacts are processed through
 467 the same filtering chain. Each descriptor is reported as the full-sequence value
 468 together with the 95% expanded type-A repeatability uncertainty estimated
 469 from the five sweeps. Per-sweep values for all descriptors are provided in Sup-
 470 plementary Table S3.

Table 3: Full-resolution radial EFM reconstruction from raw interferograms (LSCI + Gaussian low-pass, 50% at 15 UPR, ISO 16610-21). Uncertainties are 95% expanded within-run repeatability estimates from five sweeps ($n = 5$, $t_{0.975,4} = 2.776$). Units: nm for all descriptors except BV density and $W^{1,2}$ gradient (nm sample^{-1}). Certified *RONt*: FN 111 244 ± 52 nm (Hommel Roundscan 535, $n = 104$); FN 101 $41.94 \mu\text{m}$ (form tester, $n = 12$). The FN 101 certificate does not report an expanded uncertainty; therefore only the percentage difference is reported for this artefact rather than an E_n score.

Descriptor	FN 111	FN 101
R_a	$(66.3 \pm 4.7) \text{ nm}$	$(8.525 \pm 0.115) \mu\text{m}$
R_q	$(77.6 \pm 5.0) \text{ nm}$	$(10.376 \pm 0.090) \mu\text{m}$
R_z	$(278 \pm 22) \text{ nm}$	$(42.07 \pm 0.48) \mu\text{m}$
<i>RONt</i>	$(278 \pm 22) \text{ nm}$	$(42.07 \pm 0.48) \mu\text{m}$
<i>RONq</i>	$(77.6 \pm 5.0) \text{ nm}$	$(10.376 \pm 0.090) \mu\text{m}$
L^1 mean	$(66.3 \pm 4.7) \text{ nm}$	$(8.525 \pm 0.115) \mu\text{m}$
L^2 RMS	$(77.6 \pm 5.0) \text{ nm}$	$(10.376 \pm 0.090) \mu\text{m}$
L^∞	$(150 \pm 12) \text{ nm}$	$(21.97 \pm 0.42) \mu\text{m}$
BV total	$(1.137 \pm 0.062) \mu\text{m}$	$(118.4 \pm 6.2) \mu\text{m}$
BV density	$(0.263 \pm 0.014) \text{ nm sample}^{-1}$	$(6.58 \pm 0.35) \text{ nm sample}^{-1}$
$W^{1,2}$ grad.	$(0.310 \pm 0.015) \text{ nm sample}^{-1}$	$(8.76 \pm 0.43) \text{ nm sample}^{-1}$
<i>ISO shape parameters</i>		
R_{sk} (skewness)	-0.09 ± 0.04	0.00 ± 0.09
R_{ku} (kurtosis)	1.98 ± 0.21	2.51 ± 0.08
<i>Derived norm ratios</i>		
L^4/L^1 peakiness	1.39 ± 0.08	1.53 ± 0.03
<i>External validation</i>		
E_n score	0.61	< 1 (0.3% diff.; cf. Fig. S12)

4.3. Coincidence of R_z with $RONt$ and R_q with $RONq$

The identical values of R_z and $RONt$ (and of R_q and $RONq$) for both artefacts in Table 3 are expected by construction, not coincidental. In this pipeline both descriptor families are evaluated on the same LSCI-centred, Gaussian-filtered closed residual profile (Sec. 3.3; harmonic decomposition of the residual: Supplementary Fig. S19): the roughness-style R_z is the global peak-to-valley height of that profile (i.e., the total height Rt ; see the implementation note in the definition), while $RONt$ is the peak-to-valley roundness deviation of the very same profile, so the two coincide exactly; the RMS pair $R_q/RONq$ coincides for the same reason. The two families would separate if profile texture were evaluated on a different bandwidth than form (e.g., after λc -based separation of roughness from waviness in the ISO 21920 sense) or on an independent linear trace. Both are nevertheless reported because they belong to different ISO frameworks (profile texture versus roundness) with different reference conventions, and because their exact equality serves as a verification that all descriptors share one evaluation profile — the design premise of the like-for-like comparison.

4.4. Classical-Functional-Descriptor Comparison

The exact equalities $R_a = L^1$ and $R_q = L^2$ in Table 3 are definitional — each pair is the same formula applied to the same centred residual — and are reported purely as a computational cross-check that both descriptor families are evaluated on identical data, not as an empirical finding (see Sec. 5.3). For the FN 111, BV total variation carries 1.2% relative expanded uncertainty versus 5.5% for R_a and 8.5% for R_z , suggesting that gradient-based descriptors may exhibit metrological stability comparable to or better than peak-referenced roughness parameters in the tested datasets. Comparative bar charts and uncertainty analyses are provided in the Supplementary Materials (Figs. S7–S8). Ceramic and steel profile reconstruction plots are shown in Supplementary Figs. S9–S10.

The steel roundness polar representation (FN 101, Flick flat) is provided in the Supplementary Materials (Fig. S11).

JENOPIK FN~111 — Roundness deviation
 $RONt = 278$ nm (5 sweeps, native angular coordinates)

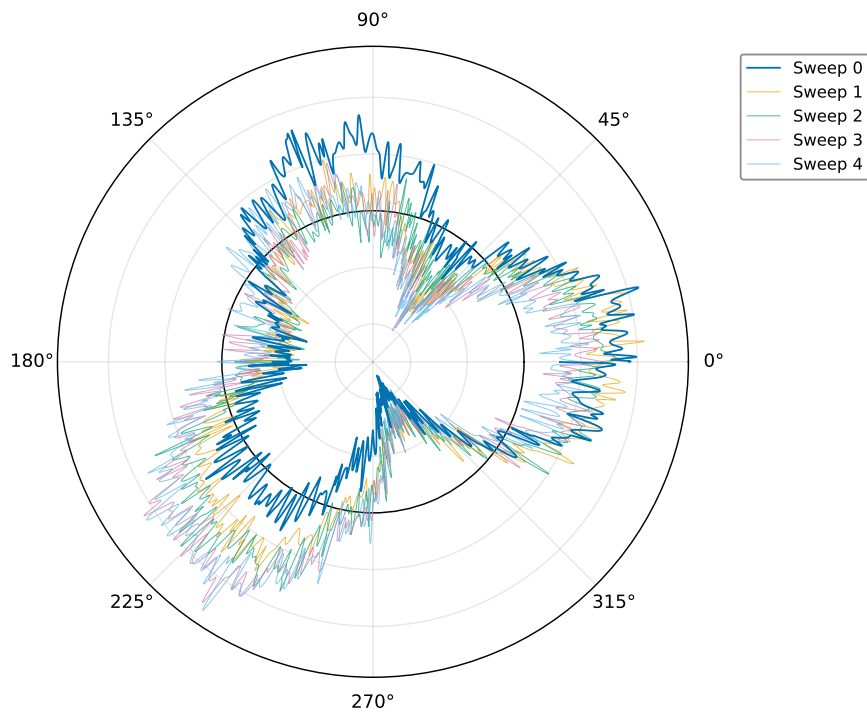


Figure 3: Ceramic roundness in polar coordinates (LSCI + Gaussian low-pass, 50% at 15 UPR). Five sweeps at native positions. $RONt = 278 \pm 22$ nm.

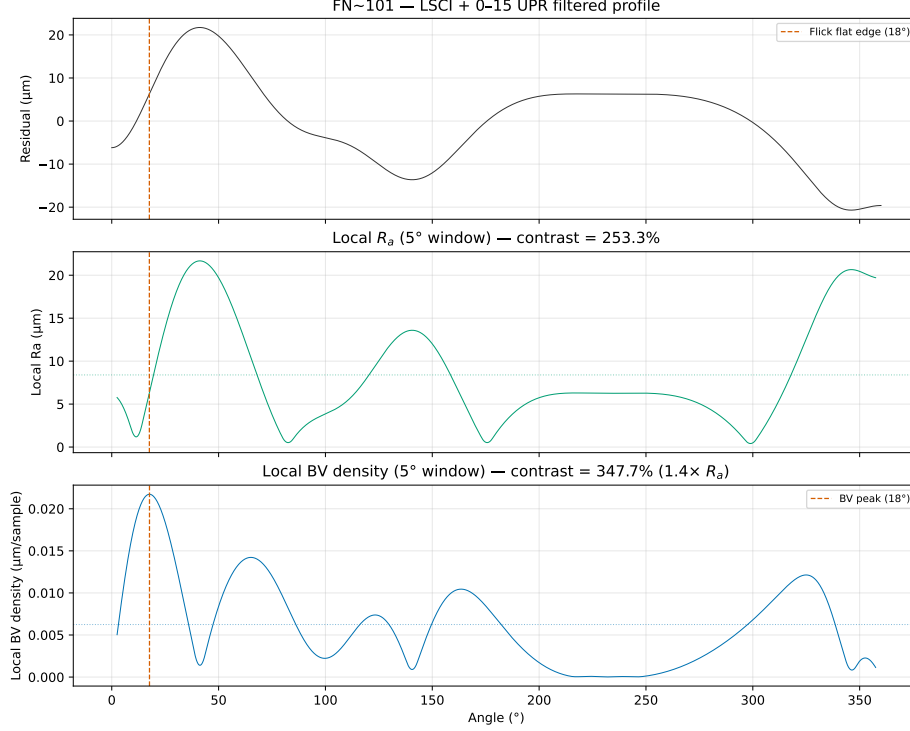


Figure 4: Flick flat detection on the FN 101 magnification standard. BV density (bottom) shows a clear spike at the Flick flat angular position, whereas R_a computed in a sliding window (top) shows no detectable response at the reconstruction resolution. The sliding-window width was matched to the certified angular extent of the Flick flat as specified in the DAkKS-DKD certificate (Art. 532 528); identical window parameters were used for both descriptors.

500 The Flick flat produces a clear response in BV density while showing no
 501 detectable response in a sliding-window R_a analysis at the reconstruction reso-
 502 lution (Fig. 4), illustrating the potential complementary sensitivity of gradient-
 503 based descriptors to localised geometric features.

504 5. Discussion

505 5.1. Confirmed Results

506 The analysis rests on a key metrological distinction: an interferogram is
 507 an intensity measurement, not a phase map and not a height map. The half-

wavelength relation $z = \nu\lambda/2$ becomes valid only after each image has been decoded to a wrapped excess fraction and the ordered excess-fraction sequence has been unwrapped to the continuous fringe-order coordinate ν . This is why the reported comparison uses only reconstructed nanometre profiles, not raw greyscale images and not areal height maps.

The most sensitive part of the workflow is the EFM localisation of bright-ring maxima, with an excess-fraction uncertainty of approximately ± 0.05 fringe orders (tightened to ± 0.03 by sinusoidal refinement in 72% of FN 111 frames). A single ϵ_i error of 0.05 fringe corresponds to 13 nm, sub-dominant to the 85 nm residual-profile RMS. The chronological unwrapping criterion rejects phase jumps exceeding 0.35 fringe. The median number of detected rings is three for both artefacts within the 240 px central aperture. The five 400° ceramic sweeps require a geometric correction: successive useful 360° intervals are shifted by 40° because the physical object angle advances continuously; without this correction, the LSCI fit appears inconsistent even when phase extraction within each sweep is repeatable.

The linear drift of $0.0246 \text{ fringe frame}^{-1}$ in the steel unwrapped phase sequence (versus 0.00021 for the FN 111) is attributed to cumulative bias in the global unwrapping algorithm rather than thermal effects or axial runout [51]. The lower fringe contrast of the FN 101 interferograms — likely due to surface finish — reduces per-frame EFM quality; the pipeline applies automatic linear detrending where needed.

5.2. Interpretation

5.2.1. Eccentricity removal and wobble verification

Roundness descriptors are computed after LSCI reference-circle fitting (Sec. 3.3), which removes the first harmonic. A shared model across all five sweeps yields $R^2 = 0.99991$ with per-sweep amplitude variation of 63 nm (0.18%); the manufacturer-specified wobble ($\pm 12 \mu\text{rad}$) bounds the observed variation an order of magnitude below $RONt = 278 \text{ nm}$. The polar representation (Fig. 3) shows five

overlaid sweeps repeatable to ± 50 nm, illustrating that the residual is dominated by low-order form deviation rather than random roughness.

5.3. Comparison with ISO Parameters

A central question of this work is whether gradient-based functional descriptors provide additional descriptive sensitivity alongside classical ISO parameters when applied to the same reconstructed profiles. To answer this rigorously, every descriptor was computed on the same reconstructed nanometre residual profiles.

Mathematical equivalences. The L^1 norm is defined as $\frac{1}{N} \sum |p_i - \bar{p}|$, which is identical to the definition of R_a . The L^2 norm is $\sqrt{\frac{1}{N} \sum (p_i - \bar{p})^2}$, identical to R_q . Computing both on the same centred residual yields *exact numerical equality*: $R_a - L^1 = 0$ and $R_q - L^2 = 0$ to machine precision for both artefacts (Table 3). These equalities are not empirical findings; they are definitional consequences. Labelling the arithmetic mean of absolute deviations as L^1 rather than R_a provides no new metrological information and should not be presented as a methodological advance.

It is emphasised that neither the L^p norms nor the Sobolev and BV seminorms are presented as novel mathematical constructs; they are standard tools whose definitions are restated for completeness. Their value in the present context is threefold. First, the functional-analytic taxonomy places ISO parameters at specific positions (L^1 , L^2 , L^∞) within a larger space of possible descriptors, revealing that descriptors outside the ISO set — BV density, $W^{1,2}$ seminorm — respond differently to the same perturbations. Second, the synthetic-defect injection methodology provides a controlled, like-for-like comparison framework that can be applied to any descriptor computed from the same residual profile; the framework itself, rather than any individual norm, constitutes the methodological contribution. Third, the Flick flat on the certified FN 101 standard provides a concrete existence proof: a real, DAKS-DKD-certified artefact whose defining geometric feature is detected unambiguously by BV density while remaining below the detection threshold of sliding-window R_a (Fig. 4).

Extrema: R_z versus L^∞ . $R_z/L^\infty \approx 2$ for both artefacts, consistent with

567 symmetric positive and negative excursions. L^∞ captures the single largest
 568 one-sided excursion; the ratio serves as a simple symmetry indicator.

569 **Variation-based descriptors.** A controlled sensitivity analysis (Supple-
 570 mentary Table S2) examined five synthetic defect types injected into the FN 111
 571 residual profile. Amplitude-averaging descriptors (R_a , R_q , R_z) showed no de-
 572 tectable change at the reconstruction resolution — a single 100 nm spike changed
 573 R_a by less than 0.05%, below the per-frame phase-extraction precision — while
 574 BV density increased by +18% and the $W^{1,2}$ gradient seminorm by +622% for
 575 the same spike (Fig. 5). ISO shape parameters responded to asymmetry (R_{sk}
 576 changed by −1104% for a step) but not to symmetric localised features. R_{sk}
 577 and BV density appear complementary in the tested scenarios: R_{sk} responds to
 578 asymmetry, BV density responds to localised gradients.

579 **Translation of synthetic responses to realistic defects.** The injected
 580 defects are idealised (isolated spike, uniform scratch, pure sinusoid), whereas
 581 real manufacturing defects have complex, random morphologies. The synthetic
 582 responses nevertheless translate to other backgrounds through a simple scal-
 583 ing argument. A localised defect adds a total-variation increment ΔTV that
 584 depends only on the defect geometry ($\Delta TV \approx 2A$ for an isolated spike of ampli-
 585 tude A), so the relative full-profile BV-density response is $\Delta TV / TV_{\text{background}}$.
 586 On the FN 111 background ($TV = 1.137 \mu\text{m}$) a 100 nm spike yields +18%;
 587 on the FN 101 background ($TV = 118.4 \mu\text{m}$) the identical spike would yield
 588 only +0.17%, below the within-run repeatability. Detectability of a given abso-
 589 lute defect in the full-profile descriptor therefore scales inversely with the back-
 590 ground gradient content, which quantifies the reviewer-relevant observation that
 591 the FN 101 defect-to-background ratio is roughly 500 times less favourable than
 592 typical smooth-surface applications. Two consequences follow for industrial in-
 593 spection. First, full-profile BV density is best suited to smooth, finished surfaces
 594 — bearing raceways, optical components, precision seals — whose residual am-
 595 plitudes (tens of nanometres) are comparable to the FN 111 case, and where the
 596 synthetic archetypes map onto realistic features (spike $\leftrightarrow$ pit or inclusion edge,
 597 scratch $\leftrightarrow$ handling or tooling mark, sinusoid $\leftrightarrow$ chatter or vibration signature).

Second, for rougher backgrounds the sliding-window formulation restores local contrast: the certified Flick flat is detected on the FN 101 (Fig. 4) despite the unfavourable full-profile ratio, precisely because the window localises the comparison. Validation against physical defects of calibrated dimensions on real metallic and ceramic surfaces remains necessary before these scaling arguments can be considered established (Sec. 5.6).

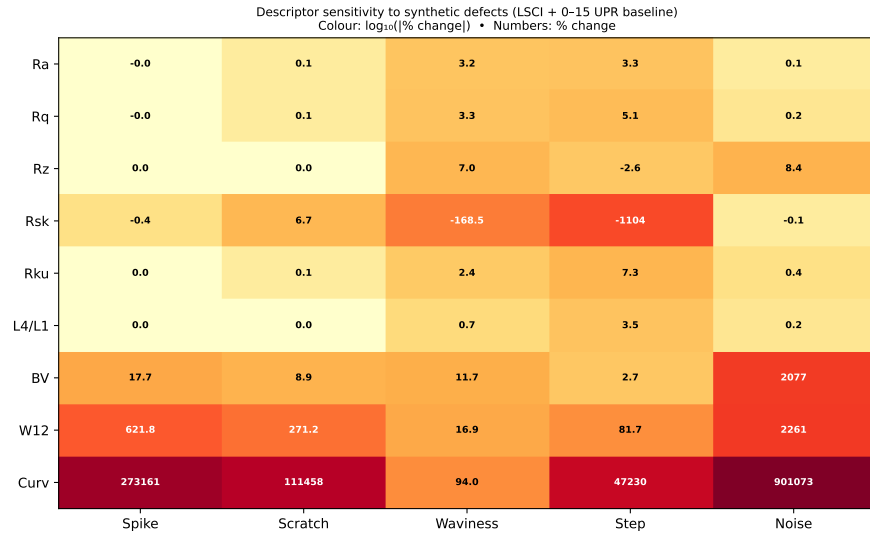


Figure 5: Sensitivity of ISO and gradient-based descriptors to five synthetic defect types injected into the FN 111 residual profile. Percentage change from the unperturbed baseline; bold labels indicate changes exceeding 10%.

Supporting analyses — descriptor correlation matrices, power spectral density comparison, Cohen’s d effect sizes, critical descriptor assessment, and L^p norm convergence — are provided in the Supplementary Materials (Figs. S13–S17). Given the number of descriptors compared (~ 15 across two artefacts), the reported differences should be interpreted as exploratory rather than confirmatory; no formal multiple-comparison correction has been applied.

Practical considerations. A practical suggestion for interferometric profile and roundness metrology is to retain R_a , R_q , R_z , R_{sk} , $RONt$ and $RONq$ as the primary engineering layer compliant with ISO 21920-2, and to consider

613 supplementing them with BV density (in angular units, nm deg^{-1} , Sec. 3.6) as
 614 a gradient-sensitive functional-analysis complement. The $W^{1,2}$ gradient semi-
 615 norm is strongly correlated with BV density in the present datasets (within
 616 the FN 111: Pearson $r = 0.95$, $n = 5$ sweeps; within the FN 101: $r = 0.93$,
 617 $n = 5$). The pooled $r = 0.94$ (95% CI $[0.72, 0.99]$, $n = 10$) is reported for de-
 618 scriptive purposes only — the sweeps are not independent observations and this
 619 pooled correlation should be interpreted with caution. This strong correlation
 620 indicates that, as *repeatability metrics across sweeps*, BV density and the $W^{1,2}$
 621 seminorm carry largely redundant information, and routine reporting of both
 622 is not warranted. They are strongly correlated but not mathematically equiv-
 623 alent: BV integrates the first power of the local slope, $TV = \int |p'| ds$, whereas
 624 $W^{1,2}$ integrates its square, $\int |p'|^2 ds$, so the two coincide only for profiles whose
 625 slope magnitude is nearly constant and diverge whenever the slope distribution
 626 is uneven. This is exactly what the defect responses show: for the 100 nm
 627 synthetic spike the $W^{1,2}$ seminorm responded with +622% versus +18% for
 628 BV density, because the quadratic weighting amplifies a single steep event far
 629 more strongly than the linear total-variation measure. A practical reading of
 630 the descriptor space in these data is therefore: (i) R_a/R_q (equivalently L^1/L^2)
 631 carry amplitude information; (ii) R_{sk} carries an independent asymmetry axis;
 632 (iii) BV density carries the localised-gradient axis and is recommended as the
 633 primary gradient descriptor; (iv) the $W^{1,2}$ seminorm adds value mainly as a
 634 high-sensitivity alarm for isolated steep features rather than as an independent
 635 information axis; and (v) the L^4/L^1 peakiness ratio provides a supplementary
 636 distribution-shape axis with a direct physical interpretation as the amplification
 637 of dominant profile excursions relative to R_a . These additional descriptors are
 638 computed from the same residual profile without additional hardware or changes
 639 to the EFM pipeline. The cross-instrument validation suggests that gradient-
 640 based descriptors are applicable to any 1D profile, whether from interferometry
 641 or tactile roundness measurement.

642 **Practical value and the known-feature caveat.** It must be acknowl-
 643 edged that the Flick flat is a certified, deliberately manufactured feature whose

644 presence and position were known in advance: Fig. 4 is an existence proof under
 645 ground-truth conditions, not a blind detection study. The practical argument
 646 for a gradient-sensitive layer is therefore not that it revealed an unknown defect
 647 here. It is that it converts what an operator might notice in a visual polar-
 648 plot inspection into a quantitative, thresholdable, and automatable indicator
 649 computed from data already acquired for ISO reporting — with no operator
 650 in the loop, a defined angular position estimate, and a repeatability statement.
 651 Whether this indicator reveals defects that routine quality-control reporting
 652 would otherwise miss has not been demonstrated; a blind-detection protocol on
 653 artefacts with independently characterised defects is outlined in Sec. 5.6 as the
 654 decisive next test of practical value.

655 **Planned versus exploratory comparisons.** The synthetic-defect re-
 656 sponses (Supplementary Table S2, Fig. 5) and the Flick flat detection (Fig. 4)
 657 were planned comparisons motivated by the study’s objective of assessing gradient-
 658 based descriptor sensitivity. The correlation matrices, power spectral density
 659 comparison, Cohen’s d effect sizes, L^p norm convergence analysis, and the cross-
 660 descriptor stability comparison (Supplementary Figs. S13–S17) are exploratory
 661 and are intended to characterise the descriptor space rather than to test specific
 662 hypotheses. This distinction should be borne in mind when interpreting the
 663 reported associations. The present study is a proof-of-concept demonstration;
 664 generalisability to other artefact types, materials, and measurement instruments
 665 remains to be established.

666 5.4. Limitations

667 Several limitations should be acknowledged. First, the uncertainty analysis
 668 is restricted to within-run Type A repeatability from five sweeps in a single
 669 continuous rotation, complemented by the indicative type-B budget of Sec. 3.8,
 670 which now includes a measured drift and noise-floor bound from an indepen-
 671 dent static stability session. The small $n = 5$ limits statistical power (relative
 672 differences below $\sim 30\%$ cannot be resolved for the FN 111), and between-run
 673 reproducibility of the rotating measurement (independent setups, thermal cy-

cles, physical re-centring of the artefact) has not been assessed; the reported expanded uncertainties should be interpreted as lower bounds, and the form-removal systematic (bounded at ≤ 41 nm) is carried outside the quadrature combination.

Second, the validation is restricted to two artefacts from a single manufacturer (JENOPTIK), both of ~ 30 mm diameter. The two artefacts do differ substantially in material (Al_2O_3 ceramic versus steel) and in residual amplitude (two orders of magnitude in R_a), which provides some breadth, but generalisability to other diameters, materials such as optical glass or tungsten carbide, and other surface finishes has not been tested. Third, the synthetic-defect analysis uses idealised mathematical defects (isolated spike, uniform scratch, pure sinusoid) injected into the FN 111 ceramic profile only; the response to real manufacturing defects with complex morphologies may differ, and the scaling analysis of Sec. 5.3 shows quantitatively that full-profile detection sensitivity degrades in proportion to background gradient content (the FN 101 ratio is ~ 500 times less favourable). Fourth, BV density and the $W^{1,2}$ seminorm carry intrinsic sampling-interval dependence; the angular-unit convention of Sec. 3.6 standardises reporting, but no inter-laboratory evidence yet exists that the convention transfers across instruments. Fifth, the Flick flat result (Supplementary Fig. S18) is demonstrated on a single artefact with a known, certified macroscopic feature; blind-detection performance and performance for subtler, micrometre-scale defects have not been characterised.

5.5. Metrological Implications

The results carry several implications for profile and roundness metrology practice. The finding that BV density responds to localised gradients that amplitude averaging may not capture suggests — subject to further validation — a potential role for gradient-based descriptors in applications where isolated defects are of concern; possible examples include quality control of bearing surfaces, optical components, or precision seals. Because these descriptors are computed from the same residual profile used for ISO 21920-2 parameters, their

704 adoption does not require changes to existing measurement acquisition proto-
705 cols.

706 The ISO 21920-2 framework (with ISO 4287 as its predecessor) remains the
707 appropriate baseline for surface texture specification and conformity assessment.
708 The gradient-based descriptors discussed here are proposed as optional supple-
709 mentary indicators, not as replacements for standardised parameters. Their
710 metrological utility would be strengthened by inter-laboratory comparisons, by
711 evaluation on a wider range of artefact types, and by adoption of the angular-
712 unit reporting convention of Sec. 3.6. Until such steps are taken, BV density and
713 related descriptors should be regarded as research-grade tools whose diagnostic
714 value has been observed under controlled laboratory conditions on two specific
715 artefacts.

716 5.6. Future Work

717 The present study suggests several directions for further investigation. (i) A
718 between-run reproducibility study with independent setups, distinct thermal
719 cycles, and physical re-centring of the artefact would establish whether the
720 gradient-based descriptors retain their relative stability under realistic labora-
721 tory conditions, and would supply the input distributions needed to upgrade the
722 indicative type-B budget of Sec. 3.8 to a complete GUM-compliant evaluation.
723 (ii) Extending the validation to artefacts with different diameters, materials
724 (e.g., optical glass, tungsten carbide), and surface finishes would test the gener-
725 alisability of the findings beyond the two ~ 30 mm JENOPTIK artefacts studied
726 here. (iii) A systematic characterisation of BV density response to real manufac-
727 turing defects (scratches, pits, inclusions) of calibrated dimensions, culminating
728 in a blind-detection protocol in which the analyst does not know defect presence
729 or position, would bridge the gap between the present synthetic-defect analy-
730 sis and industrial inspection and would provide the decisive test of practical
731 value. (iv) An inter-laboratory comparison using a common artefact set and a
732 standardised processing pipeline would provide the reproducibility data needed
733 to assess whether BV density could eventually be considered for standardisa-

tion. (v) Empirical verification of the angular-unit convention of Sec. 3.6 across instruments with different angular resolutions would support the potential inclusion of gradient descriptors in reference software for roundness evaluation. (vi) A systematic study of the speed–accuracy trade-off (rotation speed, frame rate, fringe contrast) would establish the shortest acquisition compatible with the reported uncertainty, a prerequisite for industrial adoption.

Data Availability

The analysis code, processed results, and all figures are available at <https://github.com/dawidkucharski/banach-profile-metrology> (release v1.1.0). The raw interferometric PNG archives (~32 GB), together with the independent static stability recording used for the drift bound in Sec. 3.8 (~7 GB), are available from the corresponding author upon reasonable request.

References

- [1] L. Zhu, C. Ni, Z. Yang, C. Liu, Investigations of micro-textured surface generation mechanism and tribological properties in ultrasonic vibration-assisted milling of Ti–6Al–4V, *Precision Engineering* 57 (November 2018) (2019) 229–243. doi:10.1016/j.precisioneng.2019.04.010.
URL <https://doi.org/10.1016/j.precisioneng.2019.04.010><https://linkinghub.elsevier.com/retrieve/pii/S0141635918307384>
- [2] R. Leach, *Optical Measurement of Surface Topography*, Springer Berlin Heidelberg, Berlin, Heidelberg, 2011. doi:10.1007/978-3-642-12012-1.
URL <http://link.springer.com/10.1007/978-3-642-12012-1>
- [3] D. J. Whitehouse, *Handbook of Surface and Nanometrology*, 2nd Edition, CRC Press, 2011.
- [4] A. Michelson, Light-Waves and their Application to Metrology, *Nature* 49 (1255) (1893) 56–60. doi:10.1038/049056a0.

- 760 URL <https://doi.org/10.1038/049056a0>[http://10.0.4.14/](http://10.0.4.14/049056a0http://www.nature.com/articles/049056a0)
761 [049056a0http://www.nature.com/articles/049056a0](http://www.nature.com/articles/049056a0)
- 762 [5] F. A. Jenkins, H. E. White, Fundamentals of Optics, International student
763 edition, McGraw-Hill, 1976.
- 764 URL <https://books.google.pl/books?id=dCdRAAAAMAAJ><https://books.google.pl/books?id=4SPCJ0wtFSUC>
765 <https://books.google.pl/books?id=4SPCJ0wtFSUC>
- 766 [6] M. Born, E. Wolf, E. Hecht, Principles of Optics: Electromagnetic Theory
767 of Propagation, Interference and Diffraction of Light, Physics Today 53 (10)
768 (2000) 77–78. doi:10.1063/1.1325200.
- 769 URL <http://physicstoday.scitation.org/doi/10.1063/1.1325200>
- 770 [7] R. Brodmann, Optisches Rauheitsmessgeraet fuer die Fertigung, Feinwerk-
771 technik und Messtechnik 91 (2) (1983) 63–66.
- 772 [8] R. Brodmann, Roughness form and waviness measurement by means of
773 light-scattering, Precision Engineering 8 (4) (1986) 221–226. doi:10.1016/
774 0141-6359(86)90063-2.
- 775 [9] Y. Y. Fan, V. M. Huynh, An investigation of light scattering from flat peri-
776 odic rough surfaces for surface roughness estimation, Precision Engineering
777 16 (3) (1994) 205–211. doi:10.1016/0141-6359(94)90126-0.
- 778 [10] A. Hertzsch, K. Kröger, H. Truckenbrodt, Microtopographic analysis of
779 turned surfaces by model-based scatterometry, Precision Engineering 26 (3)
780 (2002) 306–313. doi:10.1016/S0141-6359(02)00116-2.
- 781 [11] D. Kucharski, H. Zdunek, A low-cost, simple optical setup for a fast
782 scatterometry surface roughness measurements with nanometric precision,
783 Bulletin of the Polish Academy of Sciences: Technical Sciences 68 (48)
784 (2020) 485–490. doi:10.24425/bpasts.2020.133364.
- 785 URL [http://journals.pan.pl/Content/116520/PDF/10_485-490_](http://journals.pan.pl/Content/116520/PDF/10_485-490_01475_Bpast.No.68-3_30.06.20_K3A_TeX.pdf)
786 [01475_Bpast.No.68-3_30.06.20_K3A_TeX.pdf](http://journals.pan.pl/Content/116520/PDF/10_485-490_01475_Bpast.No.68-3_30.06.20_K3A_TeX.pdf)

- 787 [12] R. Benoît, Application des phénomènes d'interférence à des déterminations
788 métrologiques, Journal de Physique Théorique et Appliquée 7 (1) (1898)
789 57–68. doi:10.1051/jphystap:01898007005700.
790 URL [http://www.edpsciences.org/10.1051/jphystap:](http://www.edpsciences.org/10.1051/jphystap:01898007005700%0Apapers3://publication/doi/10.1051/jphystap:01898007005700)
791 [01898007005700%0Apapers3://publication/doi/10.1051/jphystap:](http://www.edpsciences.org/10.1051/jphystap:01898007005700)
792 [01898007005700](http://www.edpsciences.org/10.1051/jphystap:01898007005700)
793 [01898007005700](http://www.edpsciences.org/10.1051/jphystap:01898007005700)
- 794 [13] G. Xue-fei, X. Sheng-nian, Y. Ye-fei, B. Shan, B. Xing, C. Zhou-jian,
795 C. Ge-rui, D. Peng, G. Tian-shu, G. Wei, H. Shuang-lin, L. Yu-long,
796 L. Ying, L. Zi-ren, S. Ming-xue, S. Bao-san, T. Wen-lin, Y. Pin, X. Peng,
797 Z. Yun-long, Z. Hai-peng, L. Yun-kau, Laser Interferometric Gravita-
798 tional Wave Detection in Space and Structure Formation in the Early
799 Universe, Chinese Astronomy and Astrophysics 39 (4) (2015) 411–446.
800 doi:10.1016/j.chinastron.2015.10.001.
801 URL [http://www.sciencedirect.com/science/article/pii/](http://www.sciencedirect.com/science/article/pii/S0275106215000843)
802 [S0275106215000843](http://www.sciencedirect.com/science/article/pii/S0275106215000843)
803 [https://linkinghub.elsevier.com/retrieve/](https://linkinghub.elsevier.com/retrieve/pii/S0275106215000843)
[pii/S0275106215000843](https://linkinghub.elsevier.com/retrieve/pii/S0275106215000843)
- 804 [14] P. de Groot, Phase Shifting Interferometry, in: R. K. Leach (Ed.), Optical
805 Measurement of Surface Topography, Springer Berlin Heidelberg, Berlin,
806 Heidelberg, 2011, pp. 167–186. doi:10.1007/978-3-642-12012-1_8.
807 URL http://link.springer.com/10.1007/978-3-642-12012-1_8
- 808 [15] P. de Groot, Principles of interference microscopy for the measurement
809 of surface topography, Advances in Optics and Photonics 7 (2015) 1–65.
810 doi:10.1364/AOP.7.000001.
- 811 [16] S. Chatterjee, Phase-Shifting Laser Interferometry for Measurement of Sur-
812 face Form Error, in: P.K.Gupta, R.Khare (Eds.), Springer Proceedings in
813 Physics, Vol. 160 of Springer Proceedings in Physics, 2015, pp. 209–222.
814 doi:10.1007/978-81-322-2000-8_10.
815 URL http://link.springer.com/10.1007/978-81-322-2000-8_10

- [17] F. Polack, M. Thomasset, S. Brochet, D. Denetiere, Surface shape determination with a stitching Michelson interferometer and accuracy evaluation, *Review of Scientific Instruments* 90 (2). doi:10.1063/1.5061930.
- [18] M. Thomasset, M. Idir, F. Polack, M. Bray, J. J. Servant, A new phase-shift microscope designed for high accuracy stitching interferometry, *Nuclear Instruments and Methods in Physics Research, Section A: Accelerators, Spectrometers, Detectors and Associated Equipment* 710 (2013) 7–12. doi:10.1016/j.nima.2012.10.123.
- [19] K.-C. Fan, N. Wang, Z.-W. Wang, H. Zhang, Development of a roundness measuring system for microspheres, *Measurement Science and Technology* 25 (6) (2014) 064009. doi:10.1088/0957-0233/25/6/064009.
URL <http://stacks.iop.org/0957-0233/25/i=6/a=064009?key=crossref.73300f1601df9e917d2e7830f09f45e7>
- [20] M. Kühnel, V. Ullmann, U. Gerhardt, E. Manske, Automated setup for non-tactile high-precision measurements of roundness and cylindricity using two laser interferometers, *Measurement Science and Technology* 23 (7) (2012) 74016. doi:10.1088/0957-0233/23/7/074016.
URL <http://stacks.iop.org/0957-0233/23/i=7/a=074016?key=crossref.8429e4ab7d2d23702c0a05dba94b50d5http://stacks.iop.org/0957-0233/23/i=7/a=074016>
- [21] M. Takeda, H. Ina, S. Kobayashi, Fourier-transform method of fringe-pattern analysis for computer-based topography and interferometry, *Journal of the Optical Society of America* 72 (1) (1982) 156–160. doi:10.1364/JOSA.72.000156.
- [22] Q. Kemao, Two-dimensional windowed Fourier transform for fringe pattern analysis: Principles, applications and implementations, *Optics and Lasers in Engineering* 45 (2) (2007) 304–317. doi:10.1016/j.optlaseng.2005.10.012.

- [23] S. Feng, Q. Chen, G. Gu, T. Tao, L. Zhang, Y. Hu, W. Yin, C. Zuo, Fringe pattern analysis using deep learning, *Advanced Photonics* 1 (2) (2019) 025001. doi:10.1117/1.AP.1.2.025001.
- [24] I. Galaktionov, V. Toporovsky, A Multi-Stage Algorithm of Fringe Map Reconstruction for Fiber-End Surface Analysis and Non-Phase-Shifting Interferometry, *Applied System Innovation* 9 (2) (2026) 31. doi:10.3390/asi9020031.
- [25] D. Kucharski, M. Wiczorowski, Radial image processing for phase extraction in rough-surface interferometry, *Measurement* (2025) 117102doi:10.1016/j.measurement.2025.117102.
- [26] P. Dumas, J. Fleig, G. Forbes, P. E. Murphy, Extending the range of interferometry through subaperture stitching, Vol. 10314, 2003, p. 134 – 137, cited by: 9. doi:10.1117/12.2284035.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-85016807739&doi=10.1117%2f12.2284035&partnerID=40&md5=8aa04fbb9453cddff6da95df376ffdb6>
- [27] S. Chen, S. Li, Y. Dai, Z. Zheng, Iterative algorithm for subaperture stitching test with spherical interferometers, *Journal of the Optical Society of America A: Optics and Image Science, and Vision* 23 (5) (2006) 1219 – 1226, cited by: 48. doi:10.1364/JOSAA.23.001219.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-33745276550&doi=10.1364%2fJOSAA.23.001219&partnerID=40&md5=4d72b8095c89e81b1ba058a414b7b0c2>
- [28] S. Chen, S. Li, Y. Dai, Z. Zheng, Testing of large optical surfaces with subaperture stitching, *Applied Optics* 46 (17) (2007) 3504 – 3509, cited by: 44. doi:10.1364/AO.46.003504.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-34547536867&doi=10.1364%2fAO.46.003504&partnerID=40&md5=9e100905a834eebb31d582fc8884de99>

- 873 [29] A. S. Iacchetta, J. R. Fienup, D. T. Leisawitz, Rotation and transla-
874 tion registration of bandlimited interferometric images using a chirp
875 z-transform, Vol. 9907, 2016, cited by: 3. doi:10.1117/12.2232178.
876 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85006847872&doi=10.1117%2f12.2232178&partnerID=40&md5=25831551d0ae177fef89c421998e31d4)
877 [0-85006847872&doi=10.1117%2f12.2232178&partnerID=40&md5=](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85006847872&doi=10.1117%2f12.2232178&partnerID=40&md5=25831551d0ae177fef89c421998e31d4)
878 [25831551d0ae177fef89c421998e31d4](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85006847872&doi=10.1117%2f12.2232178&partnerID=40&md5=25831551d0ae177fef89c421998e31d4)
- 879 [30] J. Burge, S. Ament, J. Beverage, C. Muccianti, C. Zhao, Applications of
880 computer-generated holograms for measuring x-ray and euv optics, Vol.
881 13620, 2025, cited by: 0. doi:10.1117/12.3067011.
882 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-105024341829&doi=10.1117%2f12.3067011&partnerID=40&md5=92bd5b2fbfd00333a45113efd7a5be87)
883 [0-105024341829&doi=10.1117%2f12.3067011&partnerID=40&md5=](https://www.scopus.com/inward/record.uri?eid=2-s2.0-105024341829&doi=10.1117%2f12.3067011&partnerID=40&md5=92bd5b2fbfd00333a45113efd7a5be87)
884 [92bd5b2fbfd00333a45113efd7a5be87](https://www.scopus.com/inward/record.uri?eid=2-s2.0-105024341829&doi=10.1117%2f12.3067011&partnerID=40&md5=92bd5b2fbfd00333a45113efd7a5be87)
- 885 [31] H. Quan, H. Xi, W. Fan, Evaluating surface repeatability for interfero-
886 metric measurement: A comparative study, Vol. 9684, 2016, cited by: 1.
887 doi:10.1117/12.2243301.
888 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85002262299&doi=10.1117%2f12.2243301&partnerID=40&md5=98a061c8f8cdb6f89be75a953cd88b3f)
889 [0-85002262299&doi=10.1117%2f12.2243301&partnerID=40&md5=](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85002262299&doi=10.1117%2f12.2243301&partnerID=40&md5=98a061c8f8cdb6f89be75a953cd88b3f)
890 [98a061c8f8cdb6f89be75a953cd88b3f](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85002262299&doi=10.1117%2f12.2243301&partnerID=40&md5=98a061c8f8cdb6f89be75a953cd88b3f)
- 891 [32] L. Zhang, B. Zhang, S. Han, S. Tang, C. Zhuang, Repeatability
892 study on different interference systems, Vol. 10847, 2018, cited by: 0.
893 doi:10.1117/12.2505406.
894 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85059070480&doi=10.1117%2f12.2505406&partnerID=40&md5=d2fe726c4d532c3f34340ac03143d343)
895 [0-85059070480&doi=10.1117%2f12.2505406&partnerID=40&md5=](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85059070480&doi=10.1117%2f12.2505406&partnerID=40&md5=d2fe726c4d532c3f34340ac03143d343)
896 [d2fe726c4d532c3f34340ac03143d343](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85059070480&doi=10.1117%2f12.2505406&partnerID=40&md5=d2fe726c4d532c3f34340ac03143d343)
- 897 [33] A. Pappas, L. Newton, A. Thompson, H. Hooshmand, R. Leach, Un-
898 certainty propagation of field areal surface texture parameters using the
899 metrological characteristics approach, 2023, p. 419 – 422, cited by: 3.
900 URL <https://www.scopus.com/inward/record.>

uri?eid=2-s2.0-85165481981&partnerID=40&md5=3c2a4bd283d7a91350fa5adce5f6941b

[34] J. Gertheiss, D. Rügamer, B. X. W. Liew, S. Greven, Functional data analysis: An introduction and recent developments, Biometrical Journal 66 (7), cited by: 32; All Open Access, Hybrid Gold Open Access. doi:10.1002/bimj.202300363.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-85205152017&doi=10.1002%2fbimj.202300363&partnerID=40&md5=8d9e42e9cd2f23350c0bf0b477169043>

[35] C. Happ, F. Scheipl, A.-A. Gabriel, S. Greven, A general framework for multivariate functional principal component analysis of amplitude and phase variation, Stat 8 (1), cited by: 12; All Open Access, Green Open Access. doi:10.1002/sta4.220.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-85064480543&doi=10.1002%2fst4.220&partnerID=40&md5=e8d4b76faff42103fe5637961836125d>

[36] G. W. Wolf, Surfaces - topography and topology, Surface Topography: Metrology and Properties 8 (1), cited by: 14; All Open Access, Hybrid Gold Open Access. doi:10.1088/2051-672X/ab70e8.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-85084666906&doi=10.1088%2f2051-672X%2fab70e8&partnerID=40&md5=006779646e49c4fc727d508bc63eabfa>

[37] A. Sanner, W. G. Nöhring, L. A. Thimons, T. D. Jacobs, L. Pastewka, Scale-dependent roughness parameters for topography analysis, Applied Surface Science Advances 7, cited by: 28; All Open Access, Gold Open Access, Green Open Access. doi:10.1016/j.apsadv.2021.100190.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-85119021594&doi=10.1016%2fj.apsadv.2021.100190&partnerID=40&md5=7ad03ad2f796c56f6bec60b5febac199>

- [38] J. Zhao, Z. Wang, L. Zhengminqing, R. Zhu, Fractal simulation of surface topography and prediction of its lubrication characteristics, Surface Topography: Metrology and Properties 9 (4), cited by: 17. doi:10.1088/2051-672X/ac3f26.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-85122423109&doi=10.1088%2f2051-672X%2fac3f26&partnerID=40&md5=7eb253c5518d5356ead64c22878553ba>
- [39] F. Meijer, D. Kucharski, E. Stachowska, Determination of the phase in the center of a circular two-beam interference pattern to determine the displacement of a rough surface, Optical Engineering 57 (10) (2018) 1. doi:10.1117/1.OE.57.10.104101.
URL <https://www.spiedigitallibrary.org/journals/optical-engineering/volume-57/issue-10/104101/Determination-of-the-phase-in-the-center-of-a-circular/10.1117/1.OE.57.10.104101.full>
- [40] JENOPTIK Industrial Metrology, Unequivocal measurement of form and positional tolerances using innovative measuring systems, JENOPTIK Industrial Metrology Germany GmbH, 2018.
- [41] Thorlabs Inc., CPS532 Collimated Laser Diode Module, 532 nm, 4.5 mW, Round Beam, Ø11 mm Housing (2019).
URL <https://www.thorlabs.com/thorproduct.cfm?partnumber=CPS532>
- [42] FLIR Systems, Software Development Kit (2019).
URL <https://www.flir.com/browse/camera-cores-amp-components/software-development-kits/>
- [43] Newport Corporation, ESP301 Controller GUI Manual, Newport Corporation, 2017.
URL https://www.newport.com/medias/sys_master/images/images/h7e/hfe/9044140982302/ESP301-Controller-GUI-Manual.pdf

- 959 [44] R. Ihaka, R. Gentleman, R: A Language for Data Analysis and Graphics,
960 Journal of Computational and Graphical Statistics 5 (3) (1996) 299–314.
961 doi:10.1080/10618600.1996.10474713.
962 URL [http://www.tandfonline.com/doi/abs/10.1080/10618600.1996.](http://www.tandfonline.com/doi/abs/10.1080/10618600.1996.10474713)
963 10474713
- 964 [45] ISO 12181-1:2011, Geometrical product specifications (GPS) — Roundness
965 — Part 1: Vocabulary and parameters of roundness, Tech. rep., Interna-
966 tional Organization for Standardization (2011).
- 967 [46] ISO 21920-2:2021, Geometrical product specifications (GPS) — Surface
968 texture: Profile — Part 2: Terms, definitions and surface texture param-
969 eters, Tech. rep., International Organization for Standardization, Geneva
970 (2021).
- 971 [47] ISO 4287:1997, Geometrical Product Specifications (GPS) — Surface tex-
972 ture: Profile method — Terms, definitions and surface texture parameters,
973 Tech. rep., International Organization for Standardization (1997).
- 974 [48] ISO 25178-2:2012, Geometrical Product Specifications (GPS) — Surface
975 texture: Areal — Part 2: Terms, definitions and surface texture param-
976 eters, Tech. rep., International Organization for Standardization (2012).
- 977 [49] S. Banach, Théorie des opérations linéaires, Monografie Matematyczne,
978 Warsaw, 1932.
- 979 [50] JCGM 100:2008, Evaluation of measurement data — Guide to the expres-
980 sion of uncertainty in measurement (GUM), Tech. rep., Joint Committee
981 for Guides in Metrology (2008).
- 982 [51] Newport Corporation, Precision Motion Control Catalog, Newport Corpo-
983 ration, 2018.