

Gradient-Sensitive Functional Descriptors for Interferometric Surface Metrology: Complementing Amplitude-Averaging ISO Parameters

Abstract

This paper presents a complete interferometric pipeline for optical evaluation of roundness and surface profiles using a self-built Michelson interferometer. The method is validated on two certified JENOPTIK standards: the roundness standard FN 111 (24,000 interferograms) and the magnification standard FN 101 with a certified Flick flat (100,000 interferograms), each measured in five 400° sweeps. External validation against 104 tactile reference measurements yields an E_n score of 0.61 for the FN 111 and 0.3% agreement for the FN 101, demonstrating metrological consistency of the optical reconstruction. In addition to conventional ~~ISO-profile roughness parameters (ISO 21920-2, formerly ISO 4287 roughness parameters)~~ and roundness metrics ($RONt$, $RONq$), the reconstructed nanometre profiles are analysed using functional-analytic descriptors including L^p , Sobolev $W^{1,2}$, and bounded-variation (BV) norms. Controlled defect-injection experiments and analysis of the certified Flick flat show that gradient-based descriptors provide complementary sensitivity to localised geometric features that may remain below the detection threshold of amplitude-averaging parameters. For a 100 nm synthetic spike, BV density increased by 18% and the $W^{1,2}$ seminorm by 622%, while R_a showed no detectable response at the reconstruction resolution. The BV descriptor also detected the certified Flick flat in a sliding-window analysis where R_a remained insensitive. These results suggest that functional descriptors can complement standard profile and roundness parameters, providing additional information on localised geometric variations without requiring changes to the measurement hardware. [All reported](#)

uncertainties are within-run repeatability estimates from five sweeps of a single continuous rotation and should be interpreted as lower bounds; an indicative type-B uncertainty budget is provided.

Keywords: interferometry, roundness, surface profile, functional norms, bounded variation, Sobolev seminorm, uncertainty

1. Introduction

Surface topography is one of the most important properties of technical parts. The accuracy of form and roughness influences contact conditions, wear and lifetime. Roundness, understood as deviation from a perfect circle, remains a central requirement in precision manufacturing; Zhu et al. emphasised that precise measurements are needed both for form tolerances and for tribological surface texture assessment [1]. At nanometric scale, such measurements require high-precision optical systems [2]. The foundational reference for surface metrology terminology and parameter definitions is the handbook of Whitehouse [3].

Optical dimensional metrology has a long connection with interference [4]. Modern optical surface metrology relies on diffraction, polarisation and interference [5, 6]. Diffraction and scattering have been applied to roughness measurement ~~[7–11], while interference in several distinct ways:~~ Brodmann introduced a scattered-light roughness instrument for production environments [7] and subsequently extended the scattered-light principle to combined roughness, form and waviness measurement [8]; Fan and Huynh analysed light scattering from flat periodic rough surfaces to estimate roughness parameters [9]; Hertzsch et al. demonstrated model-based scatterometry for microtopographic analysis of turned surfaces [10]; and Kucharski and Zdunek reported a low-cost scatterometry setup achieving nanometric precision in fast roughness measurement [11]. Interference remains central for ultra-precise surface-form measurement ~~[12, 13] and,~~ from the early interference-based length comparisons of Benoît [12] to modern large-scale precision optics programmes [13]. De Groot systematised the principles of phase-shifting interferometry is widely used in and coherence-scanning interference microscopy

25 for topography evaluation [14–16][14, 16], and Chatterjee described phase-evaluation
26 interferometric testing of reflective surfaces [15].

27 Several interferometric instruments have been proposed for high-accuracy
28 surface and roundness measurement. Polack et al. described a Michelson-based
29 system for surface-shape determination built around a high-resolution stitching
30 interferometer developed by Thomasset et al. [17, 18]. Fan et al. presented
31 a roundness measuring system for microspheres based on two small Michel-
32 son interferometers [19]. Kuhnel et al. proposed an interferometric system for
33 roundness and cylindricity measurement of ring gauges with 0.1 nm resolution
34 over a large measurement range [20]. Commercial instruments can be highly ac-
35 curate, but they are often costly and may not expose the full acquisition chain
36 needed for experimental method development.

37 The ~~present work~~ numerical analysis of fringe patterns has its own methodological
38 lineage, which frames the phase-decoding route used here. Takeda et al. introduced
39 the Fourier-transform method of fringe-pattern analysis, in which a spatial
40 carrier allows the phase to be recovered from a single interferogram without
41 temporal phase shifting [21]. Kemaio extended this concept with the two-dimensional
42 windowed Fourier transform, which processes the fringe pattern locally to improve
43 robustness to noise and local fringe-quality variations [22]. More recently,
44 Feng et al. demonstrated that deep neural networks can be trained to perform
45 fringe analysis, substantially enhancing the accuracy of phase demodulation
46 from a single fringe pattern [23]. Galaktionov and Toporovsky proposed a
47 multi-stage fringe-map reconstruction algorithm for fibre-end surface analysis in
48 non-phase-shifting interferometry, combining moving-average and Fourier-transform
49 filtering with polynomial fitting and reporting agreement within 2% of a commercial
50 phase-shifting interferometer [24]. The radial excess-fraction method used in
51 the present work belongs to this single-frame, non-phase-shifting family: each
52 interferogram is decoded independently through the geometry of its circular
53 fringes, which suits continuous-rotation acquisition where temporal phase stepping
54 is impractical.

55 The present work uses a self-built, non-contact Michelson-type roundness

56 measurement system assembled from off-the-shelf components. The optical
 57 setup, apparatus description and radial image-processing route for phase extrac-
 58 tion were published in a previous study [25], where only roughness parameters
 59 were reported for the ceramic standard FN 111. The present work extends that
 60 study in three directions: (i) roundness ($RONt$, $RONq$) is evaluated for the first
 61 time with this self-built optical setup, (ii) a second artefact — the JENOPTIK
 62 magnification standard FN 101 with a Flick flat — is measured and validated
 63 against its DAkkS-DKD certificate, and (iii) a controlled sensitivity-comparison
 64 methodology is introduced: synthetic defects of known geometry are injected
 65 into measured profiles, and the response of classical ISO parameters is com-
 66 pared against that of L^p , Sobolev $W^{1,2}$, and bounded-variation (BV) norms
 67 — standard tools of functional analysis here applied to interferometric profile
 68 metrology — all computed from the same nanometre residual. The comparison
 69 framework, rather than any individual norm, constitutes the methodological
 70 contribution.

71 The computational problem is that modern interferometric surface metrol-
 72 ogy records long image sequences before a numerical profile exists. In the present
 73 data, however, each PNG file is already a separate interferogram in which the
 74 phase is encoded spatially by the bright and dark fringes inside the image. The
 75 files in the FN 111 and FN 101 folders are therefore not treated as a temporal
 76 phase-shifting stack of one fixed scene. Instead, each image $I_i(x, y)$ is processed
 77 independently to obtain one wrapped excess-fraction value ϵ_i . The ordered se-
 78 quence of these values is then unwrapped over image order and converted to a
 79 nanometre profile. The full measurement archive contains 24,000 grayscale in-
 80 terferograms of the FN 111, with image size 648×488 px, and 100,000 grayscale
 81 interferograms of the JENOPTIK magnification standard FN 101, with image
 82 size 640×480 px.

83 The literature relevant to this comparison is mature but only partly con-
 84 nected. ~~Interferometric testing has developed approaches for stitching, registration~~
 85 ~~;, motion-error compensation, and systematic-error control [26–30]. Repeatability~~
 86 ~~is commonly evaluated~~ In interferometric testing, Dumas et al. extended the

lateral range of interferometry through subaperture stitching [26]; Chen et al. developed an iterative stitching algorithm for spherical surfaces [27] and subsequently applied stitching to the testing of large optical surfaces [28]; Iacchetta et al. addressed rotation and translation registration of band-limited interferometric images using a chirp z-transform [29]; and Burge et al. applied computer-generated holograms to the measurement of x-ray and EUV optics [30]. On repeatability, Quan et al. compared evaluation approaches for interferometric surface repeatability [31], and Zhang et al. compared repeatability across different interference systems [32]; both characterise repeatability through RMS/PV quantities or pixel-wise standard-deviation matrices [31, 32]. ~~Uncertainty-oriented surface metrology embeds~~, i.e., through amplitude statistics. Pappas et al. propagated the uncertainty of areal surface-texture parameters ~~in~~ using the metrological-characteristics approach, embedding texture parameters in a GUM-style ~~propagation framework~~ [33]. ~~Functional data analysis provides a statistical~~ In statistics, Gertheiss et al. reviewed functional data analysis as a language for function-valued observations [34, 35], and [34], and Happ et al. provided a framework separating amplitude and phase variation in functional data [35]. Scale-dependence has been examined by Wolf, who connected surface topography with topological description [36], by Sanner et al., who defined scale-dependent roughness ~~studies show that characterisation can depend~~ parameters for topography analysis [37], and by Zhao et al., who studied fractal simulation of topography for lubrication prediction [38]; collectively these show that surface characterisation depends on bandwidth and filtering scale [36–38].

The research gap is therefore specific – Existing interferometric literature provides robust instrumentation and phase reconstruction; standards-oriented work provides scalar profile and form parameters with uncertainty evaluation; and functional data analysis provides a mathematical language for function-valued observations. What has received less attention is a controlled, within-profile comparison of the sensitivity of classical ISO amplitude parameters against variation-based functional norms. None of these strands, however, resolves a specific practical problem of profile and roundness metrology. When a localised

118 geometric feature — a flat, a pit, a scratch — is present on an otherwise smooth
 119 artefact, amplitude-averaging parameters such as R_a dilute its signature over
 120 the entire evaluation length, so the feature can remain numerically invisible
 121 although it is metrologically relevant. Existing remedies do not fully address
 122 this for profile data: areal parameters require calibrated height maps that
 123 single-image radial extraction does not provide; visual inspection of polar plots
 124 is operator-dependent and not quantitative; and template-based defect detectors
 125 require the defect geometry to be known in advance. The unresolved question
 126 addressed here is therefore whether gradient-sensitive functional norms — whose
 127 mathematical structure makes them respond to localised slope content rather
 128 than to averaged amplitude — provide reproducible, quantifiable sensitivity to
 129 such features when computed from the same ~~nanometre residual and validated~~
 130 ~~against an external tactile reference~~ reconstructed residual as the standard ISO
 131 parameters, and how large that sensitivity advantage is under controlled conditions.
 132 What has been missing in the literature is precisely this controlled, like-for-like
 133 comparison on identical nanometre residuals with external tactile validation.
 134 The present work addresses this by: (i) injecting synthetic defects of known ge-
 135 ometry into measured profiles to quantify descriptor response under controlled
 136 conditions; (ii) applying the full pipeline to two DAkkS-DKD-certified arte-
 137 facts at large scale (24,000 and 100,000 interferograms) with a self-built radial
 138 excess-fraction interferometer; and (iii) benchmarking the optical reconstruction
 139 against 104 tactile reference measurements. Areal parameters are not reported
 140 because the single-image radial extraction does not produce a calibrated areal
 141 height map. The aim is to assess whether L^p , bounded-variation, and Sobolev
 142 seminorms, evaluated alongside ISO ~~4287-21920-2~~ profile parameters on the
 143 same reconstructed residual profile, offer complementary descriptive sensitivity
 144 to controlled profile perturbations, and to evaluate the within-run repeatability
 145 of all quantities across five recorded sweeps. No claim of novelty is attached
 146 to the norms themselves — they are standard tools of functional analysis, and
 147 the functional-analytic vocabulary is used only as an organising taxonomy; the
 148 controlled comparison framework is the contribution.

2. Experimental Details

2.1. Optical Setup

The optical layout of the measurement system is shown in Fig. 1. The system is a two-channel modified Michelson interferometer with channels shifted by approximately 90° in phase. When an array detector is used instead of a point detector, the second channel is not strictly required [39]. In this system it was retained because it is useful for object centring and can serve as a control channel.

The optical setup and the full apparatus-level description were reported in a previous study on radial image processing for phase extraction in rough-surface interferometry [25]. They are repeated here in condensed form to make the present functional-descriptor analysis self-contained and to document the acquisition conditions behind the FN 111 and FN 101 interferogram archives.

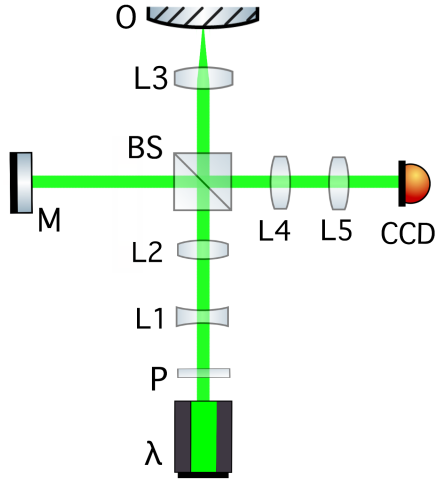


Figure 1: Optical layout of the two-channel modified Michelson interferometer: λ – diode laser (532 nm); P – linear polariser; L – lenses; L_3 – microscope objective; M – reference mirror ($\lambda/10$ flatness); BS – non-polarising beamsplitter; O – object on rotation stage; CCD – camera.

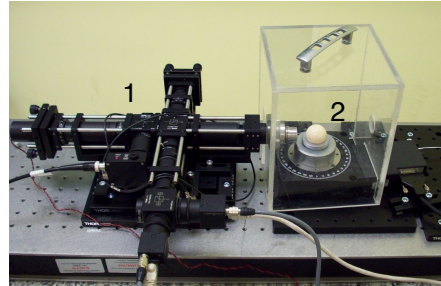


Figure 2: The complete measurement system: (1) modified Michelson interferometer in cage mounting, (2) high-precision rotation stage with the artefact.

162 The system was first tested with the JENOPTIK roundness standard FN 111
 163 (photographs: Supplementary Fig. S1) (Al_2O_3 , $\varnothing = 29.9588$ mm) [40]. A single-
 164 mode 4.5 mW diode laser with wavelength 532 nm was used as the light source.
 165 A current-stabilised supply powered the laser to obtain a stable wavelength [41].
 166 The laser beam passes through a polariser (P in Fig. 1) to set the polarisation
 167 of the light at 45° to the setup plane, minimising the difference in reflectivity
 168 between the two channels.

169 Key components: achromatic lenses $L_{1,2,4,5}$, non-polarising beamsplitter
 170 BS , $\lambda/8$ liquid phase retarder, $\lambda/10$ reference mirror M , DIN-4 microscope
 171 objective L_3 (NA 0.10), polarising beamsplitter PBS , and two Gigabit Ether-
 172 net CCD cameras (640×480 px, 120 fps).

173 The interferometer was built in a cage system for thermal, acoustic and me-
 174 chanical stability. A plexiglass box shields the measurement object, and the
 175 structure is mounted on an area translation stage. A high-precision rotation
 176 stage (encoder accuracy 2.0 mdeg, typical wobble $\pm 12 \mu\text{rad}$, typical eccentric-
 177 ity $\pm 0.40 \mu\text{m}$; full specifications: Supplementary Table S1) rotates the object.
 178 Both interferometer and stage are mounted on a honeycomb breadboard with
 179 vibration isolation.

180 Measurements were performed at night (23:00–05:00) to minimise building-
 181 activity disturbances. The setup was thermally and acoustically shielded (plex-
 182 iglass box, wool blanket) and placed on a granite plate on layered wooden-
 183 polystyrene vibration isolation (photographs: Supplementary Fig. S2). Five
 184 semiconductor temperature sensors ($\pm 0.2^\circ\text{C}$) monitored stability; the tempera-
 185 ture near the reference and object arms remained stable to $\pm 0.2^\circ\text{C}$ over six-hour
 186 acquisitions.

187 2.2. Control System and Acquisition Workflow

188 Cameras were controlled by FLIR SDK-based C programs and Bash scripts [42].
 189 Capture time was recorded per frame for angular-position verification. The ro-
 190 tation stage was controlled via USB ASCII commands [43]; a 25 s settling delay
 191 ensured constant velocity before acquisition began. Object centring was per-

192 formed manually using the two-camera phase-shifted configuration at 45° rota-
193 tion increments. Fringe evaluation used modified open-source R code [39, 44].
194 Table 1 lists the acquisition parameters for both archives; five 400° sweeps were
195 recorded per artefact, with the 40° overlap retained for profile-end comparison.

Table 1: Measurement and sampling parameters of the interferometric acquisition workflow.

Parameter	FN 111	FN 101
Rotation speed, ω	$0.50^\circ/\text{s}$	$0.08^\circ/\text{s}$
CCD frame rate	6 fps	4 fps
Recorded sweeps, n	5	5
Total frames, N	24,000	100,000
Angular step, $\Delta\alpha = \omega/\text{fps}$	$0.083^\circ/\text{frame}$	$0.020^\circ/\text{frame}$
Frames per degree	12	50
Frames per useful 360°	4320	18,000
Frames per recorded 400° sweep	4800	20,000
Overlap per sweep	$40^\circ / 480 \text{ frames}$	$40^\circ / 2000 \text{ frames}$
Total acquisition time	4000 s	25,000 s

196 The object was measured in one continuous five-sweep rotation without repo-
197 sitioning. Each recorded sweep spans 400° ; successive useful 360° segments are
198 shifted by 40° , giving a natural between-sweep angular offset. The 40° overlap
199 region provides a model-free repeatability check: RMS height difference between
200 consecutive sweeps is 12 nm (FN 111) and $0.18 \mu\text{m}$ (FN 101), consistent with
201 Table 3.

202 The frame rates in Table 1 (6 and 4 fps) are far below the 120 fps capability
203 of the cameras and merit comment. The angular step is set by the ratio
204 $\Delta\alpha = \omega/\text{fps}$, so angular resolution is governed jointly by rotation speed and
205 frame rate; measurement time is governed by rotation speed alone. The rotation
206 speeds (0.50 and $0.08^\circ/\text{s}$) were deliberately conservative: slow, constant-velocity
207 rotation minimises dynamic excitation of the stage and keeps the fringe pattern
208 quasi-static within each exposure, and the settling-time protocol (25 s before

acquisition) assumes steady-state velocity. At these speeds, 6 and 4 fps already yield 12 and 50 frames per degree — an oversampling factor of roughly 300 and 1200 relative to the 15 UPR metrological bandwidth — so the frame rate was not the accuracy-limiting factor; increasing it at fixed rotation speed would only add redundant frames. Shorter total acquisition (4,000 and 25,000 s here) would instead require faster rotation with a proportionally higher frame rate, which is technically feasible with the present cameras up to 120 fps. Whether fringe contrast and stage stability are preserved at, say, a tenfold higher speed has not been tested; the trade-off between acquisition speed, vibration robustness, and per-frame phase-extraction quality is identified as a topic for future work, since measurement time is a critical parameter for industrial implementation.

3. Image Processing and Functional-Descriptor Method

3.1. Processing Pipeline

The pipeline follows the radial excess-fraction method of a previous study [25] with added sinusoidal refinement. Each interferogram $I_i(x, y)$ is decoded independently to a wrapped excess fraction ϵ_i ; the sequence is unwrapped chronologically, converted to nanometres ($z_i = \nu_i \lambda / 2$), and reduced by the object-specific LSCI reference model. Sweep boundaries are retained for repeatability analysis.

3.2. Step-by-Step Radial Phase Decoding

For each interferogram $I_i(x, y)$, a radial intensity profile about the fringe centre is extracted and B-spline-smoothed; bright-ring maxima are detected in D^2 space, where circular-fringe theory gives $D_{ij}^2 = c_i(j + \epsilon_i - 1)$ for the j th ring of diameter D_{ij} . A linear fit $D_{ij}^2 = \alpha_i j + \beta_i$ yields the wrapped excess fraction $\epsilon_i = (1 + \beta_i / \alpha_i) \bmod 1$ (2). Where the radial fringe signal permits ($R^2 \geq 0.65$, phase within 0.20 fringe of the ring-diameter estimate), a sinusoidal refinement is applied; otherwise the ring-diameter estimate is retained. The ordered series ϵ_i is unwrapped chronologically to a continuous fringe-order coordinate ν_i , and

the nanometre profile follows from $z_i = \nu_i \lambda / 2$ with $\lambda = 532$ nm (one fringe order $\equiv 266$ nm) (3).

$$D_{ij}^2 = c_i(j + \epsilon_i - 1), \quad (1)$$

$$\epsilon_i = \left(1 + \frac{\beta_i}{\alpha_i}\right) \bmod 1. \quad (2)$$

$$z_i = \nu_i \frac{\lambda}{2}, \quad \lambda = 532 \text{ nm}. \quad (3)$$

3.3. Topography Profile, Reference Removal and Eccentricity Reduction

After phase-to-height conversion, the roundness profile is extracted following ISO 12181-1 [45] (which supersedes the withdrawn ISO 4291). For each 360° segment, a least-squares reference circle (LSCI) is fitted to the angular height profile $z_i = h(\theta_i)$ in Cartesian coordinates:

$$(x_i, y_i) = ((R_0 + z_i) \cos \theta_i, (R_0 + z_i) \sin \theta_i), \quad (4)$$

where $R_0 = 14.9794$ mm is the nominal radius of the JENOPTIK FN 111. The LSCI centre (x_c, y_c) minimises $\sum_i [\sqrt{(x_i - x_c)^2 + (y_i - y_c)^2} - R_0]^2$, yielding the centred radial residuals ρ_i . The LSCI fit is numerically equivalent to removing the first harmonic of the angular profile, but it provides the formal ISO 4291 reference circle required for roundness metrology. After LSCI centring, a phase-correct Gaussian low-pass profile filter with 50% transmission at 15 undulations per revolution (UPR) is applied to the residual profile, consistent with the filter specification used for the tactile reference measurements and with the Gaussian profile filter defined in ISO 16610-21. All classical and gradient-based descriptors are computed from this LSCI-centred, Gaussian-filtered residual $\rho_i^{(\text{filt})}$.

For the JENOPTIK magnification standard FN 101, the same processing chain is applied: a linear trend is removed from the unwrapped phase sequence before height conversion (Sec. 5.1), the LSCI reference circle is fitted to the angular profile, and the Gaussian low-pass filter (50% at 15 UPR) is applied. Although both artefacts are processed through identical filtering steps, the 15 UPR cutoff corresponds to different spatial wavelengths on the circumference: $2\pi \times 14.9794 \text{ mm} / 15 = 6.27 \text{ mm}$ for the FN 111 ($\varnothing = 29.9588 \text{ mm}$) and

262 $2\pi \times 15 \text{ mm}/15 = 6.28 \text{ mm}$ for the FN 101 ($\varnothing \approx 30 \text{ mm}$) — effectively identical.
 263 The angular sampling differs substantially (0.083° vs. 0.020° , Table 1), but the
 264 Gaussian filter sigma is set by the UPR cutoff, not by the sampling interval, so
 265 the filtered profiles are directly comparable.

266 3.4. Classical Profile and Roundness Metrics

267 All classical quantities are evaluated on nanometre residuals, not on raw
 268 intensities, following the profile method of ISO [21920-2 \[46\]](#), [which supersedes](#)
 269 [the earlier ISO 4287 \[47\]](#); [the amplitude-parameter definitions used here are](#)
 270 [common to both documents, and ISO 4287 is retained as a secondary reference](#)
 271 [because the tactile comparison data and the previous study \[25\] predate the](#)
 272 [transition](#). Areal parameters (ISO 25178 [48]) are not reported because the
 273 single-image radial extraction does not produce a calibrated areal height map.
 274 For a residual profile or vector of residual pixels p , the reported profile-style
 275 roughness descriptors are

$$R_a = \frac{1}{M} \sum_{j=1}^M |p_j - \bar{p}|, \quad R_q = \left[\frac{1}{M} \sum_{j=1}^M (p_j - \bar{p})^2 \right]^{1/2}, \quad (5)$$

276 and

$$R_z = \max_j (p_j - \bar{p}) - \min_j (p_j - \bar{p}). \quad (6)$$

277 [As implemented, this quantity is the global peak-to-valley height of the full](#)
 278 [evaluation profile, corresponding to the total-height parameter \(\$R_t\$ in ISO 21920-2](#)
 279 [terms\) rather than the section-averaged \$R_z\$; the symbol \$R_z\$ is retained for](#)
 280 [continuity with the previous study \[25\]. This implementation detail is relevant](#)
 281 [to the interpretation of Table 3 \(Sec. 4.3\).](#) The profile skewness R_{sk} and kurtosis
 282 R_{ku} — ISO [4287-21920-2](#) shape parameters that characterise asymmetry and
 283 peakedness of the height distribution — are also reported:

$$R_{sk} = \frac{1}{R_q^3} \frac{1}{M} \sum_{j=1}^M (p_j - \bar{p})^3, \quad R_{ku} = \frac{1}{R_q^4} \frac{1}{M} \sum_{j=1}^M (p_j - \bar{p})^4. \quad (7)$$

284 $R_{sk} = 0$ for a symmetric distribution; $R_{sk} < 0$ indicates a predominance
 285 of valleys over peaks. $R_{ku} = 3$ for a normal distribution; $R_{ku} > 3$ indi-
 286 cates a spikier (leptokurtic) profile. These are the only ISO [4287-21920-2](#)

287 [amplitude-distribution](#) parameters that capture distribution shape beyond am-
 288 plitude averages, and their inclusion allows a direct test of whether gradient-
 289 based descriptors provide information beyond even the best ISO shape param-
 290 eters. For the eccentricity-corrected ceramic angular profile $q_C(\theta)$,

$$RONt = \max_{\theta} q_C(\theta) - \min_{\theta} q_C(\theta), \quad RONq = \left[\frac{1}{2\pi} \int_0^{2\pi} q_C^2(\theta) d\theta \right]^{1/2}. \quad (8)$$

291 These are profile/form quantities in nanometres. B-spline pre-smoothing (20 de-
 292 grees of freedom, $\approx 18^\circ$ period) stabilises the LSCI fit; the subsequent Gaussian
 293 low-pass filter (50% at 15 UPR, ISO 16610-21) defines the metrological band-
 294 width. All descriptors are computed from the same Gaussian-filtered residual.

295 3.5. Functional Gradient-Based Descriptors

296 The concept of a complete normed vector space originates from the founda-
 297 tional work of Banach [49]. For discrete profile data of finite length N , the vector
 298 space $\mathbb{R}^N$ equipped with any norm is a Banach space; the present work does
 299 not invoke infinite-dimensional completeness but draws on the taxonomy of L^p ,
 300 Sobolev, and bounded-variation norms that Banach's framework systematised.
 301 For a centred residual profile $p(s)$ and $1 \leq p < \infty$,

$$\|p\|_p = \left(\frac{1}{L} \int_0^L |p(s)|^p ds \right)^{1/p}, \quad \|p\|_\infty = \max_{s \in [0, L]} |p(s)|. \quad (9)$$

302 The reported functional descriptors include L^1 , L^2 , L^∞ , the one-dimensional
 303 Sobolev $W^{1,2}$ seminorm and the bounded-variation (BV) total variation,

$$|p|_{W^{1,2}} = \left(\int_0^L \left| \frac{dp}{ds} \right|^2 ds \right)^{1/2}, \quad TV(p) = \int_0^L \left| \frac{dp}{ds} \right| ds. \quad (10)$$

304 In discrete form, for a uniformly sampled profile p_j ($j = 1, \dots, N$) with angular
 305 spacing $\Delta\alpha$,

$$|p|_{W^{1,2}} \approx \left(\Delta\alpha \sum_{j=1}^{N-1} \left(\frac{p_{j+1} - p_j}{\Delta\alpha} \right)^2 \right)^{1/2}, \quad TV(p) \approx \sum_{j=1}^{N-1} |p_{j+1} - p_j|. \quad (11)$$

306 Both $W^{1,2}$ and BV density carry sampling-interval dependence ~~and require conversion~~
 307 ~~to angular units ($\text{nm deg}^{-1/2}$ and nm deg^{-1} , respectively) for cross-instrument~~

308 ~~comparison~~; “nm sample⁻¹” is retained in the result tables for the fixed-acquisition
 309 setup~~-, and a standardised angular-unit convention for cross-instrument comparison~~
 310 is defined in Sec. 3.6.

311 The curvature RMS (root-mean-square of the discrete second derivative;
 312 reported in Supplementary Table S2) carries a $(\Delta\alpha)^{-2}$ sampling dependence and
 313 should not be compared across instruments with different angular resolution.

314 3.6. ~~Repeatability Uncertainty~~Angular-Unit Convention for Sampling-Dependent 315 Descriptors

316 Gradient-based descriptors evaluated on discretely sampled profiles depend
 317 on the sampling interval: the discrete total variation of an unfiltered profile
 318 grows as the sampling grid refines (noise contributes gradient content at every
 319 scale), so raw per-sample values are instrument-specific. For meaningful cross-instrument
 320 comparison the following convention is proposed and used here.

- 321 1. **Band-limit first.** The profile is filtered with a declared phase-correct
 322 Gaussian profile filter (ISO 16610-21) at a stated cutoff in undulations
 323 per revolution (here 50% transmission at 15 UPR). After band-limiting,
 324 the profile derivative is bounded and the discrete sums converge to the
 325 continuous integrals as $\Delta\alpha \rightarrow 0$; the descriptor then characterises the
 326 declared bandwidth rather than the sampling grid.
- 327 2. **Sample adequately.** The angular sampling must resolve the declared
 328 bandwidth with margin: at least ten samples per cutoff undulation are
 329 recommended. Here the FN 111 and FN 101 profiles carry ≈ 290 and
 330 ≈ 1200 samples per 15-UPR undulation, so discretisation error is negligible.
 331
- 332 3. **Report in angular units.** The BV density is reported as total variation
 333 per unit angle, $BV_\theta = TV(p)/\Theta$ in nm deg⁻¹ ($\Theta = 360^\circ$), and the gradient
 334 content as the RMS angular gradient $g_{\text{rms}} = [\frac{1}{N-1} \sum_j ((p_{j+1} - p_j)/\Delta\alpha)^2]^{1/2}$
 335 in nm deg⁻¹, together with the filter cutoff. For comparison across artefacts
 336 or instruments of different diameter, the angular unit is additionally converted

to an arc-length unit by dividing by the arc length per degree, $\pi D/360$; the BV density is then $BV_s = TV(p)/(\pi D)$ in nm mm^{-1} . The arc-length form is the diameter-independent unit and is the one recommended for cross-instrument reporting, since nm deg^{-1} still scales with the circumference of the specific artefact.

A note on physical dimensions clarifies why this is necessary and is itself part of the answer to the redundancy question (Sec. 5.3). Amplitude descriptors (R_a , R_q , L^1 , L^2 , L^∞ , $RONt$) have the dimension of length (nm) and are sampling-independent. Gradient descriptors are dimensionally distinct: BV density and the RMS gradient are height-per-length (nm mm^{-1}), i.e. dimensionless slopes, while the $W^{1,2}$ seminorm as defined here is $\text{height} \times \text{length}^{-1/2}$. This dimensional separation is the reason the gradient layer carries information that no amplitude parameter can encode, and also the reason its raw per-sample value must be qualified by a sampling and filter declaration.

For the present data, the per-sample values in Table 3 convert as follows. FN 111 ($\Delta\alpha = 0.083^\circ$): BV density $0.263 \text{ nm sample}^{-1} \rightarrow 3.2 \text{ nm deg}^{-1} \rightarrow 12.1 \text{ nm mm}^{-1}$; RMS gradient $0.310 \text{ nm sample}^{-1} \rightarrow 3.7 \text{ nm deg}^{-1} \rightarrow 14.2 \text{ nm mm}^{-1}$. FN 101 ($\Delta\alpha = 0.020^\circ$): BV density $6.58 \text{ nm sample}^{-1} \rightarrow 329 \text{ nm deg}^{-1} \rightarrow 1.26 \text{ } \mu\text{m mm}^{-1}$; RMS gradient $8.76 \text{ nm sample}^{-1} \rightarrow 438 \text{ nm deg}^{-1} \rightarrow 1.67 \text{ } \mu\text{m mm}^{-1}$, all at the 15-UPR cutoff. The two artefacts have almost identical circumference ($\pi D \approx 94.1$ and 94.2 mm), so the large difference in arc-length gradient content (12 versus 1257 nm mm^{-1}) reflects a genuine difference in surface variation rather than a unit artefact. Because each conversion is a fixed multiplicative factor for a given acquisition, relative uncertainties and relative defect responses are identical in every unit system. Adoption of gradient descriptors in reference software for roundness evaluation would require exactly this pair of declarations — filter cutoff and arc-length units — which parallels the established practice of declaring the filter for $RONt$.

3.7. Uncertainty Evaluation

Each dataset contains five 400° sweeps recorded in a single continuous rotation without stopping or repositioning. The five useful 360° segments are extracted from this continuous sequence; because each recorded sweep spans 400° , successive useful revolutions are shifted by 40° on the object. These segments are not strictly independent — they share the same continuous-run conditions (laser warm-up state, stage-bearing temperature, ambient drift). The standard deviation across sweeps therefore reflects within-run repeatability rather than between-run reproducibility. For a descriptor X evaluated on each sweep, the mean value is $\bar{X}$ and the within-run standard uncertainty is estimated as

$$u_{\text{within}}(X) = \frac{s_X}{\sqrt{n}}, \quad n = 5, \quad (12)$$

where s_X is the sample standard deviation across the five sweeps. The reported expanded uncertainty is

$$U_{95}(X) = t_{0.975, n-1} u_{\text{within}}(X). \quad (13)$$

With $n = 5$, $t_{0.975, 4} = 2.776$; the χ^2_4 -based 95% CI for the standard deviation spans $[0.6s_X, 2.9s_X]$, so U_{95} is indicative rather than definitive. Because the five segments share continuous-run conditions (laser state, stage temperature, ambient drift), the $1/\sqrt{n}$ factor in u_{within} may underestimate the true uncertainty of the mean; all reported uncertainties are *lower bounds*. ~~A full GUM-compliant budget (An indicative type-B terms: laser wavelength stability, refractive-index variations, Abbe error [50], camera nonlinearity, form-removal uncertainty) is beyond the present scope~~ budget for the principal systematic terms is given in Sec. 3.8; a complete GUM-compliant budget [51] with experimentally characterised input distributions, and a between-run reproducibility study with independent setups, thermal cycles, and physical re-centring of the artefact, remain future work (Sec. 5.6). With $n = 5$ sweeps and the observed within-run variability, the minimum detectable relative difference between two descriptors (80% power, $\alpha = 0.05$, two-sided paired t -test) is approximately 30% for the FN 111 and

5% for the FN 101, consistent with the exploratory character of the descriptor comparison. A per-sweep trend of FN 111 $RONt$ values gives a slope of $8.4 \pm 4.1 \text{ nm sweep}^{-1}$ ($p = 0.12$), consistent with zero drift, though the sweep-to-sweep scatter cautions that U_{95} may underestimate long-term reproducibility.

3.8. *Indicative Type-B Uncertainty Budget*

Although a complete GUM budget requires between-run data that the present single-rotation acquisition cannot supply, the principal type-B contributions can be bounded from component specifications and pipeline properties. Table 2 summarises the estimates for the FN 111 $RONt$ evaluation; the same relative arguments apply to the FN 101.

Laser wavelength stability. The height scale $z = \nu\lambda/2$ inherits the relative wavelength error: a $\pm 1 \text{ nm}$ tolerance on the 532 nm diode module (rectangular distribution) gives a relative standard uncertainty of 0.11%, i.e. 0.3 nm on $RONt = 278 \text{ nm}$ (and 46 nm on the FN 101 $RONt = 42.07 \mu\text{m}$, within its $\pm 0.48 \mu\text{m}$ repeatability interval). Wavelength error acts as a pure scale factor and cannot create or mask localised features.

Refractive index of air. The in-air wavelength varies with temperature and pressure by $\sim 10^{-6}$ per 1°C or 3 hPa; with the observed $\pm 0.2^\circ\text{C}$ stability the contribution is below 10^{-5} relative, i.e. $< 0.01 \text{ nm}$. Negligible.

Abbe error and stage wobble. The specified axis wobble ($\pm 12 \mu\text{rad}$) enters through two mechanisms: a cosine-type radial error $R\theta_w^2/2 \approx 1 \text{ pm}$, and a lateral beam walk $R\theta_w \approx 0.18 \mu\text{m}$ on the circumference, equivalent to an angular mislocation of 0.0007° , which maps through the local band-limited gradient ($\approx 3.2 \text{ nm deg}^{-1}$, Sec. 3.6) to $\approx 0.002 \text{ nm}$. Both are negligible after LSCI first-harmonic removal.

Camera nonlinearity and EFM localisation. Intensity nonlinearity perturbs the radial fringe-peak positions; its effect is bounded empirically by the per-frame excess-fraction uncertainty of ± 0.05 fringe (13 nm). The 15-UPR band limit averages ≈ 290 frames per resolved undulation, reducing the per-point contribution to $\approx 0.8 \text{ nm}$ and the peak-to-valley contribution to $\approx 1.1 \text{ nm}$.

421 *Long-term drift and phase noise floor (measured).* An independent static
422 stability session, recorded with the same interferometer, camera settings and
423 frame count as the FN 111 acquisition (24,000 frames over 4,000 s) but with the
424 object not rotating, provides a direct experimental bound on slow instrument
425 drift under realistic laboratory conditions. The decoded excess-fraction sequence
426 spans only 98 nm over the full session, with an end-to-end linear drift of -82 nm
427 (-1.1 nm min $^{-1}$), i.e. ≈ 15 nm over one 800 s sweep-equivalent interval; after
428 linear detrending the residual has 9.4 nm standard deviation (45 nm peak-to-valley),
429 and the frame-to-frame phase noise floor is 2.1 nm (0.008 fringe). Two conclusions
430 follow. First, the measured static noise floor is well below the conservative
431 ± 0.05 -fringe EFM bound used above, confirming that bound as conservative.
432 Second, the slow drift maps predominantly to low harmonic orders of the angular
433 profile, where it is largely absorbed by the LSCI first-harmonic removal, and
434 its sweep-to-sweep manifestation is already contained in the type-A scatter; the
435 drift bound is therefore reported as an informative constraint rather than added
436 in quadrature.

437 *Form removal.* The LSCI reference (first-harmonic removal) is exact only in
438 the limaçon approximation; the second-order term $a^2/(2R)$ for residual centring
439 eccentricity a leaks into the second harmonic of the residual. Manual centring
440 leaves a of the order of tens of micrometres (the shared first-harmonic model
441 of Sec. 5.2.1, with its 63 nm/0.18% per-sweep amplitude variation, implies
442 $a \approx 35$ μ m); for $a = 15$ – 35 μ m the term evaluates to 7–41 nm. Because this
443 contribution is common to all five sweeps, it does not appear in the type-A
444 scatter and must be carried as a bounded systematic term. Its magnitude is
445 consistent with the 34 nm difference between the optical *RONT* (278 ± 22 nm)
446 and the certified tactile value (244 ± 52 nm), a difference that the $E_n = 0.61$
447 comparison shows to be within the combined uncertainties.

448 The quadrature combination is dominated by the type-A term, so the reported
449 U_{95} values are essentially unchanged by the enumerated random type-B terms;
450 the budget nevertheless shows that the leading unquantified risks are the form-removal
451 systematic and the untested between-run effects, not the enumerated instrument

Table 2: Indicative type-B uncertainty budget for the FN 111 $RONt$ evaluation. Random contributions are standard uncertainties combined in quadrature with the type-A term; the form-removal term is a bounded systematic (bias) contribution common to all sweeps and is reported separately.

Source	Basis	Contribution to $RONt$
Within-run repeatability (type A)	$s/\sqrt{5}$, five sweeps	7.9 nm
Laser wavelength (± 1 nm, rect.)	module specification	0.3 nm
Air refractive index ($\pm 0.2^\circ\text{C}$)	Edlén-type sensitivity	< 0.01 nm
Abbe error / axis wobble ($\pm 12 \mu\text{rad}$)	stage specification, geometry	< 0.01 nm
Camera nonlinearity / EFM localisation	± 0.05 fringe per frame, band-limited averaging	1.1 nm
Long-term drift (measured, static session)	-1.1 nm min^{-1} , < 15 nm per sweep	informative bound [†]
Combined standard uncertainty u_c (random)	quadrature	8.0 nm
Expanded U_{95} (random, $t_{0.975,4}$)		22 nm
Form removal (limaçon second order)	$a^2/(2R)$, $a = 15\text{--}35 \mu\text{m}$	< 41 nm (syst. bound)

[†]Measured in an independent static session (Sec. 3.8); manifested in the type-A scatter and largely removed with the first harmonic, hence not added in quadrature.

452 [terms.](#)

453 *3.9. Computational Implementation*

454 The reconstruction workflow (`scripts/reconstruct_radial_profile_sequence.py`) decodes ϵ_i from each interferogram, unwraps the sequence, converts to
455 nanometres, applies LSCI fitting and Gaussian low-pass filtering (50% at 15 UPR,
456 ISO 16610-21), and exports CSV/JSON metrics with sweep-repeatability uncertainty. Vector PDF figures document each processing stage. The pipeline is in-
457 voked as `PYTHONPATH=src.venv/bin/pythonscripts/reconstruct_radial_profile_`
458 `sequence.py` with dataset-specific parameters (full command in the data repository). Per-image excess-fraction decoding and unwrapping require approxi-
459 mately 0.5 ms per frame (measured on an Intel Core i7-9700K, single-threaded
460 Python 3.9), so the full 124,000-frame archive processes in under two minutes
461 on consumer hardware.

465 **4. Results**

466 The results follow the updated radial sequence route only. Each raw im-
467 age is first decoded to a wrapped excess fraction from its radial fringe pat-
468 tern. The ordered excess-fraction series is then unwrapped in chronological
469 order, converted to nanometres, and corrected for eccentricity. Finally, classi-
470 cal profile/roundness descriptors and functional gradient-based descriptors are
471 computed from the same nanometre residual profiles.

472 *4.1. Radial Phase Decoding and Nanometre Profile Reconstruction*

473 The FN 111 folder contained 24,000 interferograms and the steel folder con-
474 tained 100,000 interferograms. The reported run used full-resolution images, the
475 central radial aperture of 240 px, B-spline-smoothed peak detection, continuity-
476 aware EFM peak-subset tracking and an EFM prominence threshold of 0.04 of
477 the radial fringe-signal range. All five recorded sweeps were processed.

478 Figs. S3-S6 (single-image EFM and sequence processing steps) are provided
479 in the Supplementary Materials.

480 4.2. Roughness, Roundness and Functional Descriptors

481 Table 3 gives the numerical comparison after LSCI reference circle and Gaus-
482 sian low-pass filtering (50% at 15 UPR). Both artefacts are processed through
483 the same filtering chain. Each descriptor is reported as the full-sequence value
484 together with the 95% expanded type-A repeatability uncertainty estimated
485 from the five sweeps. Per-sweep values for all descriptors are provided in Sup-
486 plementary Table S3.

Table 3: Full-resolution radial EFM reconstruction from raw interferograms (LSCI + Gaussian low-pass, 50% at 15 UPR, ISO 16610-21). Uncertainties are 95% expanded within-run repeatability estimates from five sweeps ($n = 5$, $t_{0.975,4} = 2.776$). Units: nm for all descriptors except BV density and $W^{1,2}$ gradient (nm sample⁻¹). Certified *RONt*: FN 111 244 ± 52 nm (Hommel Roundscan 535, $n = 104$); FN 101 $41.94 \mu\text{m}$ (form tester, $n = 12$). The FN 101 certificate does not report an expanded uncertainty; therefore only the percentage difference is reported for this artefact rather than an E_n score.

Descriptor	FN 111	FN 101
R_a	66.3 ± 4.7 (<u>66.3 ± 4.7</u>) nm	8.525 ± 0.115 (<u>8.525 ± 0.115</u>) μm
R_q	77.6 ± 5.0 (<u>77.6 ± 5.0</u>) nm	10.376 ± 0.090 (<u>10.376 ± 0.090</u>) μm
R_z	278 ± 22 (<u>278 ± 22</u>) nm	42.07 ± 0.48 (<u>42.07 ± 0.48</u>) μm
<i>RONt</i>	278 ± 22 (<u>278 ± 22</u>) nm	42.07 ± 0.48 (<u>42.07 ± 0.48</u>) μm
<i>RONq</i>	77.6 ± 5.0 (<u>77.6 ± 5.0</u>) nm	10.376 ± 0.090 (<u>10.376 ± 0.090</u>) μm
L^1 mean	66.3 ± 4.7 (<u>66.3 ± 4.7</u>) nm	8.525 ± 0.115 (<u>8.525 ± 0.115</u>) μm
L^2 RMS	77.6 ± 5.0 (<u>77.6 ± 5.0</u>) nm	10.376 ± 0.090 (<u>10.376 ± 0.090</u>) μm
L^∞	150 ± 12 (<u>150 ± 12</u>) nm	21.97 ± 0.42 (<u>21.97 ± 0.42</u>) μm
BV total	1.137 ± 0.062 (<u>1.137 ± 0.062</u>) μm	118.4 ± 6.2 (<u>118.4 ± 6.2</u>) μm
BV density	0.263 ± 0.014 (<u>0.263 ± 0.014</u>) nm sample ⁻¹	6.58 ± 0.35 (<u>6.58 ± 0.35</u>) nm sample ⁻¹
$W^{1,2}$ grad.	0.310 ± 0.015 (<u>0.310 ± 0.015</u>) nm sample ⁻¹	8.76 ± 0.43 (<u>8.76 ± 0.43</u>) nm sample ⁻¹
<i>ISO shape parameters</i>		
R_{sk} (skewness)	-0.09 ± 0.04	0.00 ± 0.09
R_{ku} (kurtosis)	1.98 ± 0.21	2.51 ± 0.08
<i>Derived norm ratios</i>		
L^4/L^1 peakiness	1.39 ± 0.08	1.53 ± 0.03
<i>External validation</i>		
E_n score	0.61	< 1 (0.3% diff.; cf. Fig. S12)

487 ~~The numerical identity $R_{ONt} = R_z$~~

488 *4.3. Coincidence of R_z with R_{ONt} and R_q with R_{ONq}*

489 ~~The identical values of R_z and R_{ONt} (and of R_q and R_{ONq}) for both~~
490 ~~artefacts (in Table 3) reflects the fact that after LSCI centring and Gaussian~~
491 ~~low-pass filtering (50% at 15 UPR), the residual profile is dominated by a single~~
492 ~~lobe (harmonic decomposition are expected by construction, not coincidental. In~~
493 ~~this pipeline both descriptor families are evaluated on the same LSCI-centred,~~
494 ~~Gaussian-filtered closed residual profile (Sec. 3.3; harmonic decomposition of~~
495 ~~the residual: Supplementary Fig. S19); the: the roughness-style R_z is the~~
496 ~~global peak-to-valley height of that profile (i.e., the total height R_t ; see the~~
497 ~~implementation note in the definition), while R_{ONt} is the peak-to-valley round-~~
498 ~~ness deviation and the profile roughness peak-to-valley therefore coincide . This~~
499 ~~identity is specific to the present artefact-filter combination and should not be~~
500 ~~expected to hold for artefacts with multi-lobed form deviations or for different~~
501 ~~filter cutoffs of the very same profile, so the two coincide exactly; the RMS pair~~
502 ~~R_q/R_{ONq} coincides for the same reason. The two families would separate if~~
503 ~~profile texture were evaluated on a different bandwidth than form (e.g., after~~
504 ~~λ_c -based separation of roughness from waviness in the ISO 21920 sense) or on an~~
505 ~~independent linear trace. Both are nevertheless reported because they belong~~
506 ~~to different ISO frameworks (profile texture versus roundness) with different~~
507 ~~reference conventions, and because their exact equality serves as a verification~~
508 ~~that all descriptors share one evaluation profile — the design premise of the~~
509 ~~like-for-like comparison.~~

510 *4.4. Classical-Functional-Descriptor Comparison*

511 ~~The numerical identity exact equalities $R_a = L^1$ and $R_q = L^2$ (in Table 3)~~
512 ~~confirms are definitional — each pair is the same formula applied to the same~~
513 ~~centred residual — and are reported purely as a computational cross-check that~~
514 ~~both descriptor families are evaluated on the same nanometre residual identical~~
515 ~~data, not as an empirical finding (see Sec. 5.3). For the FN 111, BV total~~

516 variation carries 1.2% relative expanded uncertainty versus 5.5% for R_a and
517 8.5% for R_z , suggesting that gradient-based descriptors may exhibit metrological
518 stability comparable to or better than peak-referenced roughness parameters
519 in the tested datasets. Comparative bar charts and uncertainty analyses are
520 provided in the Supplementary Materials (Figs. S7–S8). Ceramic and steel
521 profile reconstruction plots are shown in Supplementary Figs. S9–S10.

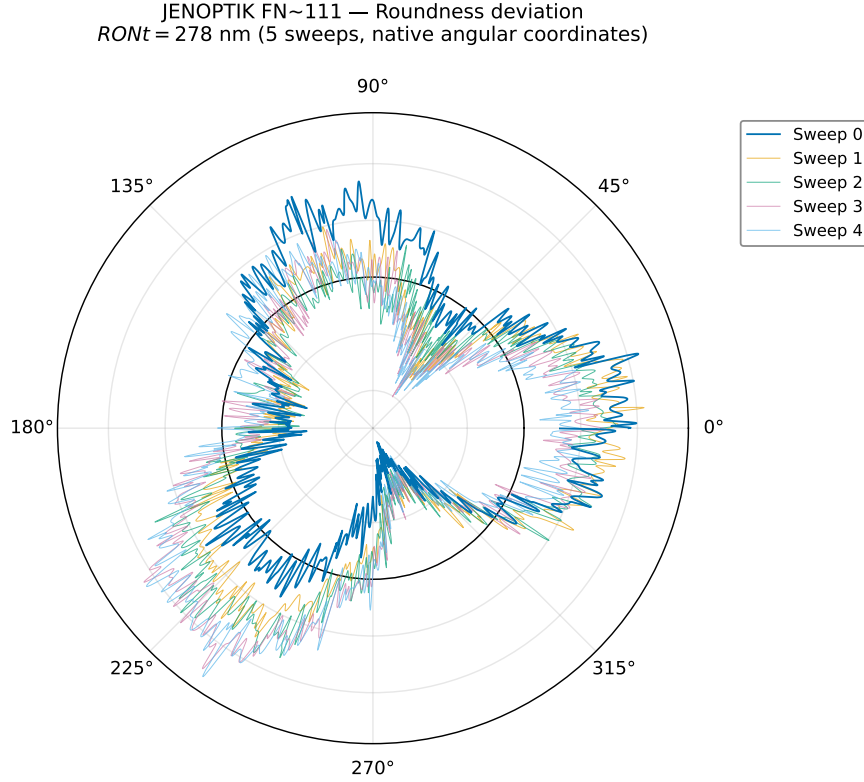


Figure 3: Ceramic roundness in polar coordinates (LSCI + Gaussian low-pass, 50% at 15 UPR). Five sweeps at native positions. $RONt = 278 \pm 22$ nm.

522 The steel roundness polar representation (FN 101, Flick flat) is provided in

523 the Supplementary Materials (Fig. S11).

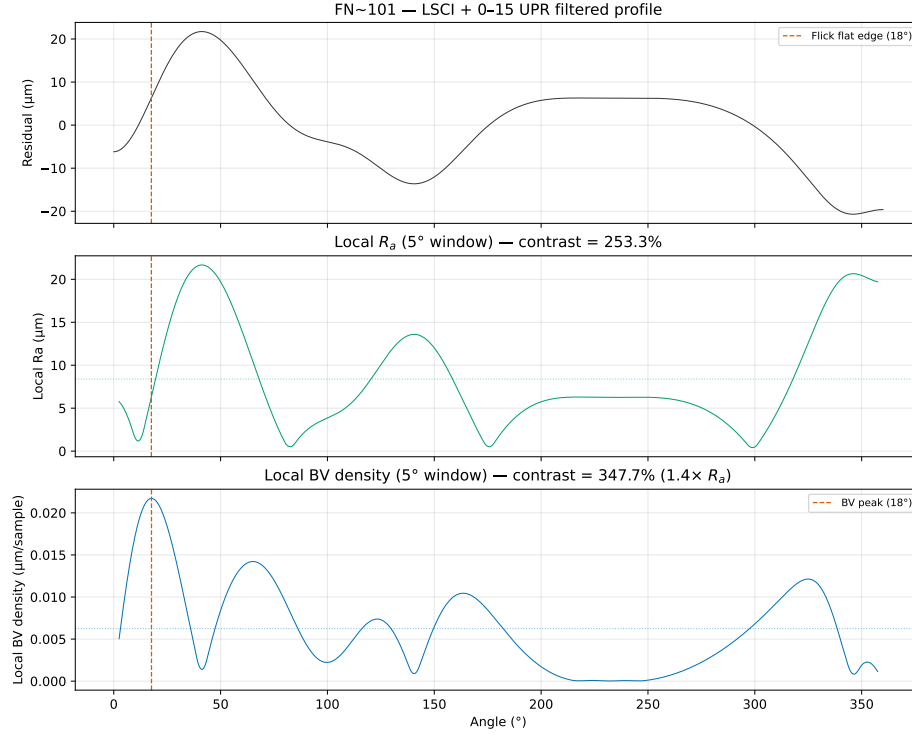


Figure 4: Flick flat detection on the FN 101 magnification standard. BV density (bottom) shows a clear spike at the Flick flat angular position, whereas R_a computed in a sliding window (top) shows no detectable response at the reconstruction resolution. The sliding-window width was matched to the certified angular extent of the Flick flat as specified in the DAkKS-DKD certificate (Art. 532 528); identical window parameters were used for both descriptors.

524 The Flick flat produces a clear response in BV density while showing no
 525 detectable response in a sliding-window R_a analysis at the reconstruction reso-
 526 lution (Fig. 4), illustrating the potential complementary sensitivity of gradient-
 527 based descriptors to localised geometric features.

528 5. Discussion

529 5.1. Confirmed Results

530 The analysis rests on a key metrological distinction: an interferogram is
531 an intensity measurement, not a phase map and not a height map. The half-
532 wavelength relation $z = \nu\lambda/2$ becomes valid only after each image has been
533 decoded to a wrapped excess fraction and the ordered excess-fraction sequence
534 has been unwrapped to the continuous fringe-order coordinate ν . This is why
535 the reported comparison uses only reconstructed nanometre profiles, not raw
536 greyscale images and not areal height maps.

537 The most sensitive part of the workflow is the EFM localisation of bright-
538 ring maxima, with an excess-fraction uncertainty of approximately ± 0.05 fringe
539 orders (tightened to ± 0.03 by sinusoidal refinement in 72% of FN 111 frames).
540 A single ϵ_i error of 0.05 fringe corresponds to 13 nm, sub-dominant to the
541 85 nm residual-profile RMS. The chronological unwrapping criterion rejects
542 phase jumps exceeding 0.35 fringe. The median number of detected rings is
543 three for both artefacts within the 240 px central aperture. The five 400° ce-
544 ramic sweeps require a geometric correction: successive useful 360° intervals are
545 shifted by 40° because the physical object angle advances continuously; without
546 this correction, the LSCI fit appears inconsistent even when phase extraction
547 within each sweep is repeatable.

548 The linear drift of $0.0246 \text{ fringe frame}^{-1}$ in the steel unwrapped phase se-
549 quence (versus 0.00021 for the FN 111) is attributed to cumulative bias in the
550 global unwrapping algorithm rather than thermal effects or axial runout [50].
551 The lower fringe contrast of the FN 101 interferograms — likely due to surface
552 finish — reduces per-frame EFM quality; the pipeline applies automatic linear
553 detrending where needed.

554 5.2. Interpretation

555 5.2.1. Eccentricity removal and wobble verification

556 Roundness descriptors are computed after LSCI reference-circle fitting (Sec. 3.3),
557 which removes the first harmonic. A shared model across all five sweeps yields

558 $R^2 = 0.99991$ with per-sweep amplitude variation of 63 nm (0.18%); the manufacturer-
559 specified wobble ($\pm 12 \mu\text{rad}$) bounds the observed variation an order of magni-
560 tude below $RONt = 278$ nm. The polar representation (Fig. 3) shows five
561 overlaid sweeps repeatable to ± 50 nm, illustrating that the residual is domi-
562 nated by low-order form deviation rather than random roughness.

563 5.3. Comparison with ISO Parameters

564 A central question of this work is whether gradient-based functional descrip-
565 tors provide additional descriptive sensitivity alongside classical ISO parameters
566 when applied to the same reconstructed profiles. To answer this rigorously, every
567 descriptor was computed on the same reconstructed nanometre residual profiles.

568 **Mathematical equivalences.** The L^1 norm is defined as $\frac{1}{N} \sum |p_i - \bar{p}|$,
569 which is identical to the definition of R_a . The L^2 norm is $\sqrt{\frac{1}{N} \sum (p_i - \bar{p})^2}$,
570 identical to R_q . Computing both on the same centred residual yields *exact*
571 *numerical equality*: $R_a - L^1 = 0$ and $R_q - L^2 = 0$ to machine precision for
572 both artefacts (Table 3). These equalities are not empirical findings; they are
573 definitional consequences. Labelling the arithmetic mean of absolute deviations
574 as L^1 rather than R_a provides no new metrological information and should not
575 be presented as a methodological advance.

576 It is emphasised that neither the L^p norms nor the Sobolev and BV semi-
577 norms are presented as novel mathematical constructs; they are standard tools
578 whose definitions are restated for completeness. Their value in the present con-
579 text is threefold. First, the functional-analytic taxonomy places ISO parameters
580 at specific positions (L^1 , L^2 , L^∞) within a larger space of possible descriptors,
581 revealing that descriptors outside the ISO set — BV density, $W^{1,2}$ seminorm
582 — respond differently to the same perturbations. Second, the synthetic-defect
583 injection methodology provides a controlled, like-for-like comparison framework
584 that can be applied to any descriptor computed from the same residual profile;
585 the framework itself, rather than any individual norm, constitutes the method-
586 ological contribution. Third, the Flick flat on the certified FN 101 standard pro-
587 vides a concrete existence proof: a real, DAkkS-DKD-certified artefact whose

defining geometric feature is detected unambiguously by BV density while remaining below the detection threshold of sliding-window R_a (Fig. 4).

Extrema: R_z versus L^∞ . $R_z/L^\infty \approx 2$ for both artefacts, consistent with symmetric positive and negative excursions. L^∞ captures the single largest one-sided excursion; the ratio serves as a simple symmetry indicator.

Variation-based descriptors. A controlled sensitivity analysis (Supplementary Table S2) examined five synthetic defect types injected into the FN 111 residual profile. Amplitude-averaging descriptors (R_a , R_q , R_z) showed no detectable change at the reconstruction resolution — a single 100 nm spike changed R_a by less than 0.05%, below the per-frame phase-extraction precision — while BV density increased by +18% and the $W^{1,2}$ gradient seminorm by +622% for the same spike (Fig. 5). ISO shape parameters responded to asymmetry (R_{sk} changed by −1104% for a step) but not to symmetric localised features. R_{sk} and BV density appear complementary in the tested scenarios: R_{sk} responds to asymmetry, BV density responds to localised gradients.

Translation of synthetic responses to realistic defects. The injected defects are idealised (isolated spike, uniform scratch, pure sinusoid), whereas real manufacturing defects have complex, random morphologies. The synthetic responses nevertheless translate to other backgrounds through a simple scaling argument. A localised defect adds a total-variation increment ΔTV that depends only on the defect geometry ($\Delta TV \approx 2A$ for an isolated spike of amplitude A), so the relative full-profile BV-density response is $\Delta TV/TV_{\text{background}}$. On the FN 111 background ($TV = 1.137 \mu\text{m}$) a 100 nm spike yields +18%; on the FN 101 background ($TV = 118.4 \mu\text{m}$) the identical spike would yield only +0.17%, below the within-run repeatability. Detectability of a given absolute defect in the full-profile descriptor therefore scales inversely with the background gradient content, which quantifies the reviewer-relevant observation that the FN 101 defect-to-background ratio is roughly 500 times less favourable than typical smooth-surface applications. Two consequences follow for industrial inspection. First, full-profile BV density is best suited to smooth, finished surfaces — bearing raceways, optical components, precision seals — whose

residual amplitudes (tens of nanometres) are comparable to the FN 111 case, and where the synthetic archetypes map onto realistic features (spike ↔ pit or inclusion edge, scratch ↔ handling or tooling mark, sinusoid ↔ chatter or vibration signature). Second, for rougher backgrounds the sliding-window formulation restores local contrast: the certified Flick flat is detected on the FN 101 (Fig. 4) despite the unfavourable full-profile ratio, precisely because the window localises the comparison. Validation against physical defects of calibrated dimensions on real metallic and ceramic surfaces remains necessary before these scaling arguments can be considered established (Sec. 5.6).

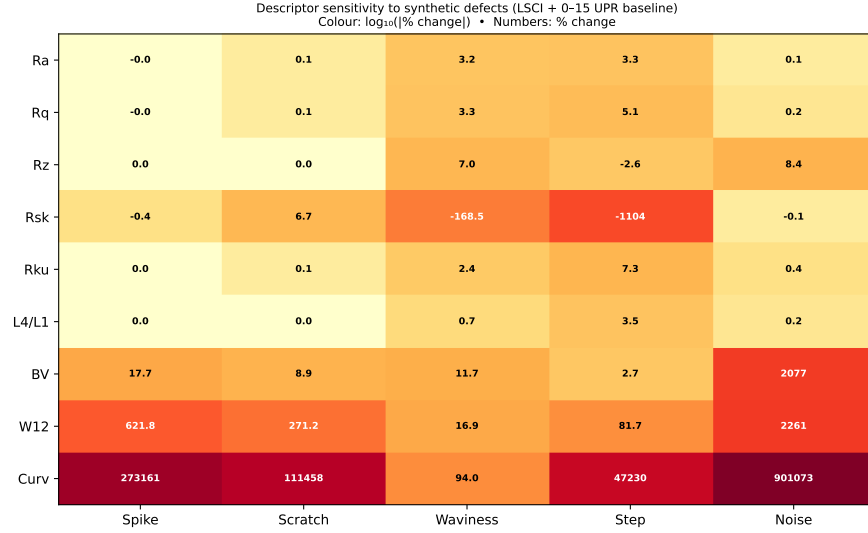


Figure 5: Sensitivity of ISO and gradient-based descriptors to five synthetic defect types injected into the FN 111 residual profile. Percentage change from the unperturbed baseline; bold labels indicate changes exceeding 10%.

Supporting analyses — descriptor correlation matrices, power spectral density comparison, Cohen’s d effect sizes, critical descriptor assessment, and L^p norm convergence — are provided in the Supplementary Materials (Figs. S13–S17). Given the number of descriptors compared (~ 15 across two artefacts), the reported differences should be interpreted as exploratory rather than confirmatory; no formal multiple-comparison correction has been applied.

Practical considerations. A practical suggestion for interferometric profile and roundness metrology is to retain R_a , R_q , R_z , R_{sk} , $RONt$ and $RONq$ as the primary engineering layer compliant with ISO 4287:2019-2, and to consider supplementing them with BV density (in angular units, nm deg^{-1} , Sec. 3.6) as a gradient-sensitive functional-analysis complement. The $W^{1,2}$ gradient seminorm is strongly correlated with BV density in the present datasets (within the FN 111: Pearson $r = 0.95$, $n = 5$ sweeps; within the FN 101: $r = 0.93$, $n = 5$). The pooled $r = 0.94$ (95% CI $[0.72, 0.99]$, $n = 10$) is reported for descriptive purposes only — the sweeps are not independent observations and this pooled correlation should be interpreted with caution. This strong correlation indicates that, as repeatability metrics across sweeps, BV density and the $W^{1,2}$ may add limited independent information beyond BV density alone given the small sample. The seminorm carry largely redundant information, and routine reporting of both is not warranted. They are strongly correlated but not mathematically equivalent: BV integrates the first power of the local slope, $TV = \int |p'| ds$, whereas $W^{1,2}$ integrates its square, $\int |p'|^2 ds$, so the two coincide only for profiles whose slope magnitude is nearly constant and diverge whenever the slope distribution is uneven. This is exactly what the defect responses show: for the 100 nm synthetic spike the $W^{1,2}$ seminorm responded with +622% versus +18% for BV density, because the quadratic weighting amplifies a single steep event far more strongly than the linear total-variation measure. A practical reading of the descriptor space in these data is therefore: (i) R_a/R_q (equivalently L^1/L^2) carry amplitude information; (ii) R_{sk} carries an independent asymmetry axis; (iii) BV density carries the localised-gradient axis and is recommended as the primary gradient descriptor; (iv) the $W^{1,2}$ seminorm adds value mainly as a high-sensitivity alarm for isolated steep features rather than as an independent information axis; and (v) the L^4/L^1 peakiness ratio provides a supplementary distribution-shape axis with a direct physical interpretation as the amplification of dominant profile excursions relative to R_a . These additional descriptors are computed from the same residual profile without additional hardware or changes to the EFM pipeline. The cross-instrument validation suggests that gradient-

665 based descriptors are applicable to any 1D profile, whether from interferometry
666 or tactile roundness measurement.

667 **Practical value and the known-feature caveat.** It must be acknowledged
668 that the Flick flat is a certified, deliberately manufactured feature whose presence
669 and position were known in advance: Fig. 4 is an existence proof under ground-truth
670 conditions, not a blind detection study. The practical argument for a gradient-sensitive
671 layer is therefore not that it revealed an unknown defect here. It is that
672 it converts what an operator might notice in a visual polar-plot inspection
673 into a quantitative, thresholdable, and automatable indicator computed from
674 data already acquired for ISO reporting — with no operator in the loop, a
675 defined angular position estimate, and a repeatability statement. Whether this
676 indicator reveals defects that routine quality-control reporting would otherwise
677 miss has not been demonstrated; a blind-detection protocol on artefacts with
678 independently characterised defects is outlined in Sec. 5.6 as the decisive next
679 test of practical value.

680 **Planned versus exploratory comparisons.** The synthetic-defect re-
681 sponses (Supplementary Table S2, Fig. 5) and the Flick flat detection (Fig. 4)
682 were planned comparisons motivated by the study’s objective of assessing gradient-
683 based descriptor sensitivity. The correlation matrices, power spectral density
684 comparison, Cohen’s d effect sizes, L^p norm convergence analysis, and the cross-
685 descriptor stability comparison (Supplementary Figs. S13–S17) are exploratory
686 and are intended to characterise the descriptor space rather than to test specific
687 hypotheses. This distinction should be borne in mind when interpreting the
688 reported associations. The present study is a proof-of-concept demonstration;
689 generalisability to other artefact types, materials, and measurement instruments
690 remains to be established.

691 5.4. Limitations

692 Several limitations should be acknowledged. First, the uncertainty anal-
693 ysis is restricted to within-run Type A repeatability from five sweeps in a
694 single continuous rotation—, complemented by the indicative type-B budget

of Sec. 3.8, which now includes a measured drift and noise-floor bound from
an independent static stability session. The small $n = 5$ limits statistical
power (relative differences below $\sim 30\%$ cannot be resolved for the FN 111),
and between-run reproducibility of the rotating measurement (independent se-
tups, thermal cycles, physical re-centring of the artefact) has not been assessed.
A full GUM-compliant uncertainty budget, incorporating type-B evaluations
of laser wavelength stability, refractive-index variations, Abbe error, camera
nonlinearity, and form-removal uncertainty, is beyond the scope of this study;
the reported expanded uncertainties should be interpreted as lower bounds,
and the form-removal systematic (bounded at < 41 nm) is carried outside the
quadrature combination.

Second, the validation is restricted to two artefacts from a single manufac-
turer (JENOPTIK), both of ~ 30 mm diameter. The two artefacts do differ
substantially in material (Al_2O_3 ceramic versus steel) and in residual amplitude
(two orders of magnitude in R_a), which provides some breadth, but generalis-
ability to other sizes, materials, or diameters, materials such as optical glass
or tungsten carbide, and other surface finishes has not been tested. Third,
the synthetic-defect analysis uses idealised mathematical defects (isolated spike,
uniform scratch, pure sinusoid) injected into the FN 111 ceramic profile only;
the response to real manufacturing defects with complex morphologies may dif-
fer, and the defect-to-background ratio for scaling analysis of Sec. 5.3 shows
quantitatively that full-profile detection sensitivity degrades in proportion to
background gradient content (the FN 101 is approximately ratio is ~ 500 times
smaller, so the detection sensitivity reported here may not generalise to artefacts
with substantially larger form deviations less favourable). Fourth, BV density
and the $W^{1,2}$ seminorm carry intrinsic sampling-interval dependence requiring
conversion to angular units for cross-instrument comparison; the angular-unit
convention of Sec. 3.6 standardises reporting, but no inter-laboratory evidence
yet exists that the convention transfers across instruments. Fifth, the Flick flat
result (Supplementary Fig. S18) is demonstrated on a single artefact with a
known, certified macroscopic feature; performance blind-detection performance

726 and performance for subtler, micrometre-scale defects ~~has~~ have not been char-
727 acterised.

728 5.5. Metrological Implications

729 The results carry several implications for profile and roundness metrology
730 practice. The finding that BV density responds to localised gradients that am-
731 plitude averaging may not capture suggests — subject to further validation —
732 a potential role for gradient-based descriptors in applications where isolated
733 defects are of concern; possible examples include quality control of bearing sur-
734 faces, optical components, or precision seals. Because these descriptors are
735 computed from the same residual profile used for ISO ~~4287~~ 21920-2 parameters,
736 their adoption does not require changes to existing measurement acquisition
737 protocols.

738 The ISO ~~4287 framework~~ 21920-2 framework (with ISO 4287 as its predecessor)
739 remains the appropriate baseline for surface texture specification and confor-
740 mity assessment. The gradient-based descriptors discussed here are proposed
741 as optional supplementary indicators, not as replacements for standardised pa-
742 rameters. Their metrological utility would be strengthened by inter-laboratory
743 comparisons, by evaluation on a wider range of artefact types, and by ~~the~~
744 ~~development of agreed procedures for converting sampling-dependent units to~~
745 ~~instrument-independent angular gradient units.~~ adoption of the angular-unit reporting
746 convention of Sec. 3.6. Until such steps are taken, BV density and related de-
747 scriptors should be regarded as research-grade tools whose diagnostic value has
748 been observed under controlled laboratory conditions on two specific artefacts.

749 5.6. Future Work

750 The present study suggests several directions for further investigation. (i) A
751 between-run reproducibility study with independent setups ~~and~~ distinct thermal
752 cycles, and physical re-centring of the artefact would establish whether the
753 gradient-based descriptors retain their relative stability under realistic labo-
754 ratory conditions. ~~—, and would supply the input distributions needed to upgrade~~

755 the indicative type-B budget of Sec. 3.8 to a complete GUM-compliant evaluation.
 756 (ii) Extending the validation to artefacts with different diameters, materials
 757 (e.g., ~~glass, optical glass, tungsten~~ carbide), and surface finishes would test the
 758 generalisability of the findings beyond the two ~30 mm JENOPTIK artefacts
 759 studied here. (iii) A systematic characterisation of BV density response to real
 760 manufacturing defects (scratches, pits, inclusions) of ~~controlled dimensions~~ calibrated
 761 dimensions, culminating in a blind-detection protocol in which the analyst does
 762 not know defect presence or position, would bridge the gap between the present
 763 synthetic-defect analysis and industrial inspection ~~scenarios~~ and would provide
 764 the decisive test of practical value. (iv) An inter-laboratory comparison using
 765 a common artefact set and a standardised processing pipeline would provide
 766 the reproducibility data needed to assess whether BV density could eventually
 767 be considered for standardisation. (v) ~~The development of agreed Empirical~~
 768 ~~verification of the~~ angular-unit ~~conventions for sampling-dependent gradient~~
 769 ~~descriptors would facilitate cross-instrument comparison and potential inclusion~~
 770 ~~convention of Sec. 3.6 across instruments with different angular resolutions~~
 771 ~~would support the potential inclusion of gradient descriptors~~ in reference soft-
 772 ware for roundness evaluation. (vi) A systematic study of the speed-accuracy
 773 trade-off (rotation speed, frame rate, fringe contrast) would establish the shortest
 774 acquisition compatible with the reported uncertainty, a prerequisite for industrial
 775 adoption.

776 Data Availability

777 The analysis code, processed results, and all figures are available at [https:](https://github.com/dawidkucharski/banach-profile-metrology)
 778 [//github.com/dawidkucharski/banach-profile-metrology](https://github.com/dawidkucharski/banach-profile-metrology) (release v1.1.0).
 779 The raw interferometric PNG archives (~32 GB), together with the independent
 780 static stability recording used for the drift bound in Sec. 3.8 (~7 GB), are
 781 available from the corresponding author upon reasonable request.

782 References

- 783 [1] L. Zhu, C. Ni, Z. Yang, C. Liu, Investigations of micro-textured surface
 784 generation mechanism and tribological properties in ultrasonic vibration-
 785 assisted milling of Ti-6Al-4V, Precision Engineering 57 (November 2018)
 786 (2019) 229–243. doi:10.1016/j.precisioneng.2019.04.010.
 787 URL <https://doi.org/10.1016/j.precisioneng.2019.04.010https://linkinghub.elsevier.com/retrieve/pii/S0141635918307384>
 788
- 789 [2] R. Leach, Optical Measurement of Surface Topography, Springer Berlin
 790 Heidelberg, Berlin, Heidelberg, 2011. doi:10.1007/978-3-642-12012-1.
 791 URL <http://link.springer.com/10.1007/978-3-642-12012-1>
- 792 [3] D. J. Whitehouse, Handbook of Surface and Nanometrology, 2nd Edition,
 793 CRC Press, 2011.
- 794 [4] A. Michelson, Light-Waves and their Application to Metrology, Nature
 795 49 (1255) (1893) 56–60. doi:10.1038/049056a0.
 796 URL <https://doi.org/10.1038/049056a0http://10.0.4.14/049056a0http://www.nature.com/articles/049056a0>
 797
- 798 [5] F. A. Jenkins, H. E. White, Fundamentals of Optics, International student
 799 edition, McGraw-Hill, 1976.
 800 URL <https://books.google.pl/books?id=dCdRAAAAMAAJhttps://books.google.pl/books?id=4SPCJ0wtFSUC>
 801
- 802 [6] M. Born, E. Wolf, E. Hecht, Principles of Optics: Electromagnetic Theory
 803 of Propagation, Interference and Diffraction of Light, Physics Today 53 (10)
 804 (2000) 77–78. doi:10.1063/1.1325200.
 805 URL <http://physicstoday.scitation.org/doi/10.1063/1.1325200>
- 806 [7] R. Brodmann, Optisches Rauheitsmessgeraet fuer die Fertigung, Feinwerk-
 807 technik und Messtechnik 91 (2) (1983) 63–66.

- [8] R. Brodmann, Roughness form and waviness measurement by means of light-scattering, Precision Engineering 8 (4) (1986) 221–226. doi:10.1016/0141-6359(86)90063-2.
- [9] Y. Y. Fan, V. M. Huynh, An investigation of light scattering from flat periodic rough surfaces for surface roughness estimation, Precision Engineering 16 (3) (1994) 205–211. doi:10.1016/0141-6359(94)90126-0.
- [10] A. Hertzsch, K. Kröger, H. Truckenbrodt, Microtopographic analysis of turned surfaces by model-based scatterometry, Precision Engineering 26 (3) (2002) 306–313. doi:10.1016/S0141-6359(02)00116-2.
- [11] D. Kucharski, H. Zdunek, A low-cost, simple optical setup for a fast scatterometry surface roughness measurements with nanometric precision, Bulletin of the Polish Academy of Sciences: Technical Sciences 68 (48) (2020) 485–490. doi:10.24425/bpasts.2020.133364.
URL http://journals.pan.pl/Content/116520/PDF/10_485-490_01475_Bpast.No.68-3_30.06.20_K3A_TeX.pdf
- [12] R. Benoît, Application des phénomènes d’interférence à des déterminations métrologiques, Journal de Physique Théorique et Appliquée 7 (1) (1898) 57–68. doi:10.1051/jphystap:01898007005700.
URL <http://www.edpsciences.org/10.1051/jphystap:01898007005700%0Apapers3://publication/doi/10.1051/jphystap:01898007005700http://www.edpsciences.org/10.1051/jphystap:01898007005700>
- [13] G. Xue-fei, X. Sheng-nian, Y. Ye-fei, B. Shan, B. Xing, C. Zhou-jian, C. Ge-rui, D. Peng, G. Tian-shu, G. Wei, H. Shuang-lin, L. Yu-long, L. Ying, L. Zi-ren, S. Ming-xue, S. Bao-san, T. Wen-lin, Y. Pin, X. Peng, Z. Yun-long, Z. Hai-peng, L. Yun-kau, Laser Interferometric Gravitational Wave Detection in Space and Structure Formation in the Early Universe, Chinese Astronomy and Astrophysics 39 (4) (2015) 411–446. doi:10.1016/j.chinastron.2015.10.001.

- 837 URL [http://www.sciencedirect.com/science/article/pii/](http://www.sciencedirect.com/science/article/pii/S0275106215000843)
838 [S0275106215000843https://linkinghub.elsevier.com/retrieve/](https://linkinghub.elsevier.com/retrieve/pii/S0275106215000843)
839 [pii/S0275106215000843](https://linkinghub.elsevier.com/retrieve/pii/S0275106215000843)
- 840 [14] P. de Groot, Phase Shifting Interferometry, in: R. K. Leach (Ed.), Optical
841 Measurement of Surface Topography, Springer Berlin Heidelberg, Berlin,
842 Heidelberg, 2011, pp. 167–186. doi:10.1007/978-3-642-12012-1_8.
843 URL http://link.springer.com/10.1007/978-3-642-12012-1_8
- 844 [15] S. Chatterjee, Phase-Shifting Laser Interferometry for Measurement of Sur-
845 face Form Error, in: P.K.Gupta, R.Khare (Eds.), Springer Proceedings in
846 Physics, Vol. 160 of Springer Proceedings in Physics, 2015, pp. 209–222.
847 doi:10.1007/978-81-322-2000-8_10.
848 URL http://link.springer.com/10.1007/978-81-322-2000-8_10
- 849 [16] P. de Groot, Principles of interference microscopy for the measurement
850 of surface topography, Advances in Optics and Photonics 7 (2015) 1–65.
851 doi:10.1364/AOP.7.000001.
- 852 [17] F. Polack, M. Thomasset, S. Brochet, D. Denetiere, Surface shape deter-
853 mination with a stitching Michelson interferometer and accuracy evalua-
854 tion, Review of Scientific Instruments 90 (2). doi:10.1063/1.5061930.
- 855 [18] M. Thomasset, M. Idir, F. Polack, M. Bray, J. J. Servant, A new phase-shift
856 microscope designed for high accuracy stitching interferometry, Nuclear
857 Instruments and Methods in Physics Research, Section A: Accelerators,
858 Spectrometers, Detectors and Associated Equipment 710 (2013) 7–12. doi:
859 10.1016/j.nima.2012.10.123.
- 860 [19] K.-C. Fan, N. Wang, Z.-W. Wang, H. Zhang, Development of a roundness
861 measuring system for microspheres, Measurement Science and Technology
862 25 (6) (2014) 064009. doi:10.1088/0957-0233/25/6/064009.
863 URL [http://stacks.iop.org/0957-0233/25/i=6/a=064009?key=](http://stacks.iop.org/0957-0233/25/i=6/a=064009?key=crossref.73300f1601df9e917d2e7830f09f45e7)
864 [crossref.73300f1601df9e917d2e7830f09f45e7](http://stacks.iop.org/0957-0233/25/i=6/a=064009?key=crossref.73300f1601df9e917d2e7830f09f45e7)

- [20] M. Kühnel, V. Ullmann, U. Gerhardt, E. Manske, Automated setup for non-tactile high-precision measurements of roundness and cylindricity using two laser interferometers, *Measurement Science and Technology* 23 (7) (2012) 74016. doi:10.1088/0957-0233/23/7/074016.
URL <http://stacks.iop.org/0957-0233/23/i=7/a=074016?key=crossref.8429e4ab7d2d23702c0a05dba94b50d5><http://stacks.iop.org/0957-0233/23/i=7/a=074016>
- [21] M. Takeda, H. Ina, S. Kobayashi, Fourier-transform method of fringe-pattern analysis for computer-based topography and interferometry, *Journal of the Optical Society of America* 72 (1) (1982) 156–160. doi:10.1364/JOSA.72.000156.
- [22] Q. Kemao, Two-dimensional windowed Fourier transform for fringe pattern analysis: Principles, applications and implementations, *Optics and Lasers in Engineering* 45 (2) (2007) 304–317. doi:10.1016/j.optlaseng.2005.10.012.
- [23] S. Feng, Q. Chen, G. Gu, T. Tao, L. Zhang, Y. Hu, W. Yin, C. Zuo, Fringe pattern analysis using deep learning, *Advanced Photonics* 1 (2) (2019) 025001. doi:10.1117/1.AP.1.2.025001.
- [24] I. Galaktionov, V. Toporovsky, A Multi-Stage Algorithm of Fringe Map Reconstruction for Fiber-End Surface Analysis and Non-Phase-Shifting Interferometry, *Applied System Innovation* 9 (2) (2026) 31. doi:10.3390/asi9020031.
- [25] D. Kucharski, M. Wiczorowski, Radial image processing for phase extraction in rough-surface interferometry, *Measurement* (2025) 117102doi:10.1016/j.measurement.2025.117102.
- [26] P. Dumas, J. Fleig, G. Forbes, P. E. Murphy, Extending the range of interferometry through subaperture stitching, Vol. 10314, 2003, p. 134 – 137, cited by: 9. doi:10.1117/12.2284035.

893 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
894 0-85016807739&doi=10.1117%2f12.2284035&partnerID=40&md5=
895 8aa04fbb9453cddff6da95df376ffdb6

896 [27] S. Chen, S. Li, Y. Dai, Z. Zheng, Iterative algorithm for subaperture
897 stitching test with spherical interferometers, Journal of the Optical Society
898 of America A: Optics and Image Science, and Vision 23 (5) (2006) 1219 –
899 1226, cited by: 48. doi:10.1364/JOSA.23.001219.

900 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
901 0-33745276550&doi=10.1364%2fJOSA.23.001219&partnerID=40&
902 md5=4d72b8095c89e81b1ba058a414b7b0c2

903 [28] S. Chen, S. Li, Y. Dai, Z. Zheng, Testing of large optical surfaces with
904 subaperture stitching, Applied Optics 46 (17) (2007) 3504 – 3509, cited
905 by: 44. doi:10.1364/AO.46.003504.

906 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
907 0-34547536867&doi=10.1364%2fAO.46.003504&partnerID=40&md5=
908 9e100905a834eebb31d582fc8884de99

909 [29] A. S. Iacchetta, J. R. Fienup, D. T. Leisawitz, Rotation and transla-
910 tion registration of bandlimited interferometric images using a chirp
911 z-transform, Vol. 9907, 2016, cited by: 3. doi:10.1117/12.2232178.

912 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
913 0-85006847872&doi=10.1117%2f12.2232178&partnerID=40&md5=
914 25831551d0ae177fef89c421998e31d4

915 [30] J. Burge, S. Ament, J. Beverage, C. Muccianti, C. Zhao, Applications of
916 computer-generated holograms for measuring x-ray and euv optics, Vol.
917 13620, 2025, cited by: 0. doi:10.1117/12.3067011.

918 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
919 0-105024341829&doi=10.1117%2f12.3067011&partnerID=40&md5=
920 92bd5b2fbfd00333a45113efd7a5be87

- [31] H. Quan, H. Xi, W. Fan, Evaluating surface repeatability for interferometric measurement: A comparative study, Vol. 9684, 2016, cited by: 1. doi:10.1117/12.2243301.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-85002262299&doi=10.1117%2f12.2243301&partnerID=40&md5=98a061c8f8cdb6f89be75a953cd88b3f>
- [32] L. Zhang, B. Zhang, S. Han, S. Tang, C. Zhuang, Repeatability study on different interference systems, Vol. 10847, 2018, cited by: 0. doi:10.1117/12.2505406.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-85059070480&doi=10.1117%2f12.2505406&partnerID=40&md5=d2fe726c4d532c3f34340ac03143d343>
- [33] A. Pappas, L. Newton, A. Thompson, H. Hooshmand, R. Leach, Uncertainty propagation of field areal surface texture parameters using the metrological characteristics approach, 2023, p. 419 – 422, cited by: 3.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-85165481981&partnerID=40&md5=3c2a4bd283d7a91350fa5adce5f6941b>
- [34] J. Gertheiss, D. Rügamer, B. X. W. Liew, S. Greven, Functional data analysis: An introduction and recent developments, Biometrical Journal 66 (7), cited by: 32; All Open Access, Hybrid Gold Open Access. doi:10.1002/bimj.202300363.
URL <https://www.scopus.com/inward/record.uri?eid=2-s2.0-85205152017&doi=10.1002%2fbimj.202300363&partnerID=40&md5=8d9e42e9cd2f23350c0bf0b477169043>
- [35] C. Happ, F. Scheipl, A.-A. Gabriel, S. Greven, A general framework for multivariate functional principal component analysis of amplitude and phase variation, Stat 8 (1), cited by: 12; All Open Access, Green Open Access. doi:10.1002/sta4.220.

950 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
951 0-85064480543&doi=10.1002%2fst4.220&partnerID=40&md5=
952 e8d4b76faff42103fe5637961836125d

953 [36] G. W. Wolf, Surfaces - topography and topology, Surface Topography:
954 Metrology and Properties 8 (1), cited by: 14; All Open Access, Hybrid
955 Gold Open Access. doi:10.1088/2051-672X/ab70e8.
956 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
957 0-85084666906&doi=10.1088%2f2051-672X%2fab70e8&partnerID=
958 40&md5=006779646e49c4fc727d508bc63eabfa

959 [37] A. Sanner, W. G. Nöhring, L. A. Thimons, T. D. Jacobs, L. Pastewka,
960 Scale-dependent roughness parameters for topography analysis, Applied
961 Surface Science Advances 7, cited by: 28; All Open Access, Gold Open
962 Access, Green Open Access. doi:10.1016/j.apsadv.2021.100190.
963 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
964 0-85119021594&doi=10.1016%2fj.apsadv.2021.100190&partnerID=
965 40&md5=7ad03ad2f796c56f6bec60b5febac199

966 [38] J. Zhao, Z. Wang, L. Zhengminqing, R. Zhu, Fractal simulation of
967 surface topography and prediction of its lubrication characteristics,
968 Surface Topography: Metrology and Properties 9 (4), cited by: 17.
969 doi:10.1088/2051-672X/ac3f26.
970 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
971 0-85122423109&doi=10.1088%2f2051-672X%2fac3f26&partnerID=
972 40&md5=7eb253c5518d5356ead64c22878553ba

973 [39] F. Meijer, D. Kucharski, E. Stachowska, Determination of the phase in
974 the center of a circular two-beam interference pattern to determine the
975 displacement of a rough surface, Optical Engineering 57 (10) (2018) 1.
976 doi:10.1117/1.OE.57.10.104101.
977 URL [https://www.spiedigitallibrary.org/journals/](https://www.spiedigitallibrary.org/journals/optical-engineering/volume-57/issue-10/104101/)
978 [optical-engineering/volume-57/issue-10/104101/](https://www.spiedigitallibrary.org/journals/optical-engineering/volume-57/issue-10/104101/)

979 Determination-of-the-phase-in-the-center-of-a-circular/10.
980 1117/1.OE.57.10.104101.full

981 [40] JENOPTIK Industrial Metrology, Unequivocal measurement of form and
982 positional tolerances using innovative measuring systems, JENOPTIK In-
983 dustrial Metrology Germany GmbH, 2018.

984 [41] Thorlabs Inc., CPS532 Collimated Laser Diode Module, 532 nm, 4.5 mW,
985 Round Beam, Ø11 mm Housing (2019).
986 URL [https://www.thorlabs.com/thorproduct.cfm?partnumber=](https://www.thorlabs.com/thorproduct.cfm?partnumber=CPS532)
987 CPS532

988 [42] FLIR Systems, Software Development Kit (2019).
989 URL [https://www.flir.com/browse/camera-cores-amp-components/](https://www.flir.com/browse/camera-cores-amp-components/software-development-kits/)
990 software-development-kits/

991 [43] Newport Corporation, ESP301 Controller GUI Manual, Newport Corpora-
992 tion, 2017.
993 URL [https://www.newport.com/medias/sys_master/images/images/](https://www.newport.com/medias/sys_master/images/images/h7e/hfe/9044140982302/ESP301-Controller-GUI-Manual.pdf)
994 h7e/hfe/9044140982302/ESP301-Controller-GUI-Manual.pdf

995 [44] R. Ihaka, R. Gentleman, R: A Language for Data Analysis and Graphics,
996 Journal of Computational and Graphical Statistics 5 (3) (1996) 299–314.
997 doi:10.1080/10618600.1996.10474713.
998 URL [http://www.tandfonline.com/doi/abs/10.1080/10618600.1996.](http://www.tandfonline.com/doi/abs/10.1080/10618600.1996.10474713)
999 10474713

1000 [45] ISO 12181-1:2011, Geometrical product specifications (GPS) — Roundness
1001 — Part 1: Vocabulary and parameters of roundness, Tech. rep., Interna-
1002 tional Organization for Standardization (2011).

1003 [46] ISO 21920-2:2021, Geometrical product specifications (GPS) — Surface
1004 texture: Profile — Part 2: Terms, definitions and surface texture param-
1005 eters, Tech. rep., International Organization for Standardization, Geneva
1006 (2021).

- 1007 [47] ISO 4287:1997, Geometrical Product Specifications (GPS) — Surface tex-
 1008 ture: Profile method — Terms, definitions and surface texture parameters,
 1009 Tech. rep., International Organization for Standardization (1997).
- 1010 [48] ISO 25178-2:2012, Geometrical Product Specifications (GPS) — Surface
 1011 texture: Areal — Part 2: Terms, definitions and surface texture paramete-
 1012 rs, Tech. rep., International Organization for Standardization (2012).
- 1013 [49] S. Banach, Théorie des opérations linéaires, Monografie Matematyczne,
 1014 Warsaw, 1932.
- 1015 [50] Newport Corporation, Precision Motion Control Catalog, Newport Corpo-
 1016 ration, 2018.
- 1017 [51] JCGM 100:2008, Evaluation of measurement data — Guide to the expres-
 1018 sion of uncertainty in measurement (GUM), Tech. rep., Joint Committee
 1019 for Guides in Metrology (2008).