

Gradient-Sensitive Functional Descriptors for Interferometric Surface Metrology: Complementing Amplitude-Averaging ISO Parameters

Abstract

This paper presents a complete interferometric pipeline for optical evaluation of roundness and surface profiles using a self-built Michelson interferometer. The method is validated on two certified JENOPTIK standards: the roundness standard FN 111 (24,000 interferograms) and the magnification standard FN 101 with a certified Flick flat (100,000 interferograms), each measured in five 400° sweeps. External validation against 104 tactile reference measurements yields an E_n score of 0.61 for the FN 111 and 0.3% agreement for the FN 101, demonstrating metrological consistency of the optical reconstruction. In addition to conventional ~~ISO-profile roughness parameters (ISO 21920-2, formerly ISO 4287 roughness parameters)~~ and roundness metrics ($RONt$, $RONq$), the reconstructed nanometre profiles are analysed using functional-analytic descriptors including L^p , Sobolev $W^{1,2}$, and bounded-variation (BV) norms. Controlled defect-injection experiments and analysis of the certified Flick flat show that gradient-based descriptors provide complementary sensitivity to localised geometric features that may remain below the detection threshold of amplitude-averaging parameters. For a 100 nm synthetic spike, BV density increased by 18% and the $W^{1,2}$ seminorm by 622%, while R_a showed no detectable response at the reconstruction resolution. The BV descriptor also detected the certified Flick flat in a sliding-window analysis where R_a remained insensitive. These results suggest that functional descriptors can complement standard profile and roundness parameters, providing additional information on localised geometric variations without requiring changes to the measurement hardware. [All reported](#)

uncertainties are within-run repeatability estimates from five sweeps of a single continuous rotation and should be interpreted as lower bounds; an indicative type-B uncertainty budget is provided.

Keywords: interferometry, roundness, surface profile, functional norms, bounded variation, Sobolev seminorm, uncertainty

1. Introduction

Surface topography is one of the most important properties of technical parts. The accuracy of form and roughness influences contact conditions, wear and lifetime. Roundness, understood as deviation from a perfect circle, remains a central requirement in precision manufacturing; Zhu et al. emphasised that precise measurements are needed both for form tolerances and for tribological surface texture assessment [1]. At nanometric scale, such measurements require high-precision optical systems [2]. The foundational reference for surface metrology terminology and parameter definitions is the handbook of Whitehouse [3].

Optical dimensional metrology has a long connection with interference [4]. Modern optical surface metrology relies on diffraction, polarisation and interference [5, 6]. Diffraction and scattering have been applied to roughness measurement ~~[7–10], while interference in several distinct ways:~~ Brodmann introduced a scattered-light roughness instrument for production environments [11] and subsequently extended the scattered-light principle to combined roughness, form and waviness measurement [7]; Fan and Huynh analysed light scattering from flat periodic rough surfaces to estimate roughness parameters [8]; Hertzsch et al. demonstrated model-based scatterometry for microtopographic analysis of turned surfaces [9]; and a low-cost scatterometry setup achieving nanometric precision in fast roughness measurement has been reported previously [10]. Interference remains central for ultra-precise surface-form measurement ~~[12, 13] and~~, from the early interference-based length comparisons of Benoît [12] to modern large-scale precision optics programmes [13]. De Groot systematised the principles of phase-shifting ~~interferometry is widely used in and coherence-scanning~~

25 interference microscopy for topography evaluation [14–16][14, 16], and Chatterjee
26 described phase-evaluation interferometric testing of reflective surfaces [15].

27 Several interferometric instruments have been proposed for high-accuracy
28 surface and roundness measurement. Polack et al. described a Michelson-based
29 system for surface-shape determination built around a high-resolution stitching
30 interferometer developed by Thomasset et al. [17, 18]. Fan et al. presented
31 a roundness measuring system for microspheres based on two small Michel-
32 son interferometers [19]. Kuhnel et al. proposed an interferometric system for
33 roundness and cylindricity measurement of ring gauges with 0.1 nm resolution
34 over a large measurement range [20]. Commercial instruments can be highly ac-
35 curate, but they are often costly and may not expose the full acquisition chain
36 needed for experimental method development.

37 The ~~present work~~ numerical analysis of fringe patterns has its own methodological
38 lineage, which frames the phase-decoding route used here. Takeda et al. introduced
39 the Fourier-transform method of fringe-pattern analysis, in which a spatial
40 carrier allows the phase to be recovered from a single interferogram without
41 temporal phase shifting [21]. Kemaio extended this concept with the two-dimensional
42 windowed Fourier transform, which processes the fringe pattern locally to improve
43 robustness to noise and local fringe-quality variations [22]. More recently,
44 Feng et al. demonstrated that deep neural networks can be trained to perform
45 fringe analysis, substantially enhancing the accuracy of phase demodulation
46 from a single fringe pattern [23]. Galaktionov and Toporovsky proposed a
47 multi-stage fringe-map reconstruction algorithm for fibre-end surface analysis in
48 non-phase-shifting interferometry, combining moving-average and Fourier-transform
49 filtering with polynomial fitting and reporting agreement within 2% of a commercial
50 phase-shifting interferometer [24]. The radial excess-fraction method used in
51 the present work belongs to this single-frame, non-phase-shifting family: each
52 interferogram is decoded independently through the geometry of its circular
53 fringes, which suits continuous-rotation acquisition where temporal phase stepping
54 is impractical.

55 The present work uses a self-built, non-contact Michelson-type roundness

measurement system assembled from off-the-shelf components. The optical setup, apparatus description and radial image-processing route for phase extraction were published in a previous study [25], where only roughness parameters were reported for the ceramic standard FN 111. The present work extends that study in three directions: (i) roundness ($RONt$, $RONq$) is evaluated for the first time with this self-built optical setup, (ii) a second artefact — the JENOPTIK magnification standard FN 101 with a Flick flat — is measured and validated against its DAKS-DKD certificate, and (iii) a controlled sensitivity-comparison methodology is introduced: synthetic defects of known geometry are injected into measured profiles, and the response of classical ISO parameters is compared against that of L^p , Sobolev $W^{1,2}$, and bounded-variation (BV) norms — standard tools of functional analysis here applied to interferometric profile metrology — all computed from the same nanometre residual. The comparison framework, rather than any individual norm, constitutes the methodological contribution.

The computational problem is that modern interferometric surface metrology records long image sequences before a numerical profile exists. In the present data, however, each PNG file is already a separate interferogram in which the phase is encoded spatially by the bright and dark fringes inside the image. The files in the FN 111 and FN 101 folders are therefore not treated as a temporal phase-shifting stack of one fixed scene. Instead, each image $I_i(x, y)$ is processed independently to obtain one wrapped excess-fraction value ϵ_i . The ordered sequence of these values is then unwrapped over image order and converted to a nanometre profile. The full measurement archive contains 24,000 grayscale interferograms of the FN 111, with image size 648×488 px, and 100,000 grayscale interferograms of the JENOPTIK magnification standard FN 101, with image size 640×480 px.

The literature relevant to this comparison is mature but only partly connected. ~~Interferometric testing has developed approaches for stitching, registration, motion-error compensation, and systematic-error control [26–30]. Repeatability is commonly evaluated~~ In interferometric testing, Dumas et al. extended the

lateral range of interferometry through subaperture stitching [26]; Chen et al. developed an iterative stitching algorithm for spherical surfaces [27] and subsequently applied stitching to the testing of large optical surfaces [28]; Iacchetta et al. addressed rotation and translation registration of band-limited interferometric images using a chirp z-transform [29]; and Burge et al. applied computer-generated holograms to the measurement of x-ray and EUV optics [30]. On repeatability, Quan et al. compared evaluation approaches for interferometric surface repeatability [31], and Zhang et al. compared repeatability across different interference systems [32]; both characterise repeatability through RMS/PV quantities or pixel-wise standard-deviation matrices [31, 32]. ~~Uncertainty-oriented surface metrology embeds~~, i.e., through amplitude statistics. Pappas et al. propagated the uncertainty of areal surface-texture parameters ~~in~~ using the metrological-characteristics approach, embedding texture parameters in a GUM-style ~~propagation framework~~ [33]. ~~Functional data analysis provides a statistical~~ In statistics, Gertheiss et al. reviewed functional data analysis as a language for function-valued observations [34, 35], and [34], and Happ et al. provided a framework separating amplitude and phase variation in functional data [35]. Scale-dependence has been examined by Wolf, who connected surface topography with topological description [36], by Sanner et al., who defined scale-dependent roughness ~~studies show that characterisation can depend~~ parameters for topography analysis [37], and by Zhao et al., who studied fractal simulation of topography for lubrication prediction [38]; collectively these show that surface characterisation depends on bandwidth and filtering scale [36–38].

The research gap is therefore specific – Existing interferometric literature provides robust instrumentation and phase reconstruction; standards-oriented work provides scalar profile and form parameters with uncertainty evaluation; and functional data analysis provides a mathematical language for function-valued observations. What has received less attention is a controlled, within-profile comparison of the sensitivity of classical ISO amplitude parameters against variation-based functional norms. None of these strands, however, resolves a specific practical problem of profile and roundness metrology. When a localised

118 geometric feature — a flat, a pit, a scratch — is present on an otherwise smooth
 119 artefact, amplitude-averaging parameters such as R_a dilute its signature over
 120 the entire evaluation length, so the feature can remain numerically invisible
 121 although it is metrologically relevant. Existing remedies do not fully address
 122 this for profile data: areal parameters require calibrated height maps that
 123 single-image radial extraction does not provide; visual inspection of polar plots
 124 is operator-dependent and not quantitative; and template-based defect detectors
 125 require the defect geometry to be known in advance. The unresolved question
 126 addressed here is therefore whether gradient-sensitive functional norms — whose
 127 mathematical structure makes them respond to localised slope content rather
 128 than to averaged amplitude — provide reproducible, quantifiable sensitivity to
 129 such features when computed from the same ~~nanometre residual and validated~~
 130 ~~against an external tactile reference~~ reconstructed residual as the standard ISO
 131 parameters, and how large that sensitivity advantage is under controlled conditions.
 132 What has been missing in the literature is precisely this controlled, like-for-like
 133 comparison on identical nanometre residuals with external tactile validation.
 134 The present work addresses this by: (i) injecting synthetic defects of known ge-
 135 ometry into measured profiles to quantify descriptor response under controlled
 136 conditions; (ii) applying the full pipeline to two DAkkS-DKD-certified arte-
 137 facts at large scale (24,000 and 100,000 interferograms) with a self-built radial
 138 excess-fraction interferometer; and (iii) benchmarking the optical reconstruction
 139 against 104 tactile reference measurements. Areal parameters are not reported
 140 because the single-image radial extraction does not produce a calibrated areal
 141 height map. The aim is to assess whether L^p , bounded-variation, and Sobolev
 142 seminorms, evaluated alongside ISO ~~4287-21920-2~~ profile parameters on the
 143 same reconstructed residual profile, offer complementary descriptive sensitivity
 144 to controlled profile perturbations, and to evaluate the within-run repeatability
 145 of all quantities across five recorded sweeps. No claim of novelty is attached
 146 to the norms themselves — they are standard tools of functional analysis, and
 147 the functional-analytic vocabulary is used only as an organising taxonomy; the
 148 controlled comparison framework is the contribution.

2. Experimental Details

2.1. Optical Setup

The optical layout of the measurement system is shown in Fig. 1. The system is a two-channel modified Michelson interferometer with channels shifted by approximately 90° in phase. When an array detector is used instead of a point detector, the second channel is not strictly required [39]. In this system it was retained because it is useful for object centring and can serve as a control channel.

The optical setup and the full apparatus-level description were reported in a previous study on radial image processing for phase extraction in rough-surface interferometry [25]. They are repeated here in condensed form to make the present functional-descriptor analysis self-contained and to document the acquisition conditions behind the FN 111 and FN 101 interferogram archives.

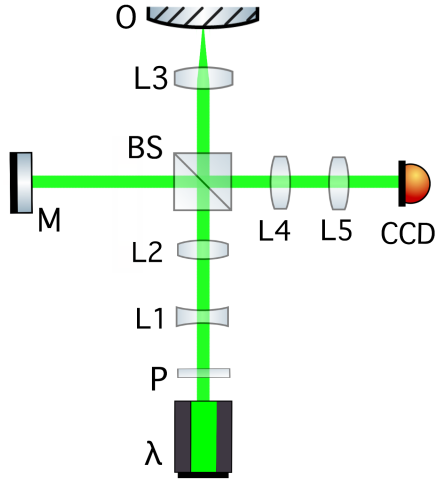


Figure 1: Optical layout of the two-channel modified Michelson interferometer: λ – diode laser (532 nm); P – linear polariser; L – lenses; L_3 – microscope objective; M – reference mirror ($\lambda/10$ flatness); BS – non-polarising beamsplitter; O – object on rotation stage; CCD – camera.

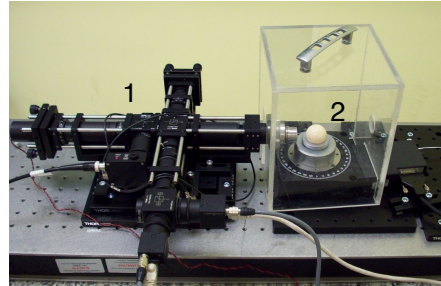


Figure 2: The complete measurement system: (1) modified Michelson interferometer in cage mounting, (2) high-precision rotation stage with the artefact.

162 The system was first tested with the JENOPTIK roundness standard FN 111
 163 (photographs: Supplementary Fig. S1) (Al_2O_3 , $\varnothing = 29.9588$ mm) [40]. A single-
 164 mode 4.5 mW diode laser with wavelength 532 nm was used as the light source.
 165 A current-stabilised supply powered the laser to obtain a stable wavelength [41].
 166 The laser beam passes through a polariser (P in Fig. 1) to set the polarisation
 167 of the light at 45° to the setup plane, minimising the difference in reflectivity
 168 between the two channels.

169 Key components: achromatic lenses $L_{1,2,4,5}$, non-polarising beamsplitter
 170 BS , $\lambda/8$ liquid phase retarder, $\lambda/10$ reference mirror M , DIN-4 microscope
 171 objective L_3 (NA 0.10), polarising beamsplitter PBS , and two Gigabit Ether-
 172 net CCD cameras (640×480 px, 120 fps).

173 The interferometer was built in a cage system for thermal, acoustic and me-
 174 chanical stability. A plexiglass box shields the measurement object, and the
 175 structure is mounted on an area translation stage. A high-precision rotation
 176 stage (encoder accuracy 2.0 mdeg, typical wobble $\pm 12 \mu\text{rad}$, typical eccentric-
 177 ity $\pm 0.40 \mu\text{m}$; full specifications: Supplementary Table S1) rotates the object.
 178 Both interferometer and stage are mounted on a honeycomb breadboard with
 179 vibration isolation.

180 Measurements were performed at night (23:00–05:00) to minimise building-
 181 activity disturbances. The setup was thermally and acoustically shielded (plex-
 182 iglass box, wool blanket) and placed on a granite plate on layered wooden-
 183 polystyrene vibration isolation (photographs: Supplementary Fig. S2). Five
 184 semiconductor temperature sensors ($\pm 0.2^\circ\text{C}$) monitored stability; the tempera-
 185 ture near the reference and object arms remained stable to $\pm 0.2^\circ\text{C}$ over six-hour
 186 acquisitions.

187 2.2. Control System and Acquisition Workflow

188 Cameras were controlled by FLIR SDK-based C programs and Bash scripts [42].
 189 Capture time was recorded per frame for angular-position verification. The ro-
 190 tation stage was controlled via USB ASCII commands [43]; a 25 s settling delay
 191 ensured constant velocity before acquisition began. Object centring was per-

192 formed manually using the two-camera phase-shifted configuration at 45° rota-
 193 tion increments. Fringe evaluation used modified open-source R code [39, 44].
 194 Table 1 lists the acquisition parameters for both archives; five 400° sweeps were
 195 recorded per artefact, with the 40° overlap retained for profile-end comparison.

Table 1: Measurement and sampling parameters of the interferometric acquisition workflow.

Parameter	FN 111	FN 101
Rotation speed, ω	$0.50^\circ/\text{s}$	$0.08^\circ/\text{s}$
CCD frame rate	6 fps	4 fps
Recorded sweeps, n	5	5
Total frames, N	24,000	100,000
Angular step, $\Delta\alpha = \omega/\text{fps}$	$0.083^\circ/\text{frame}$	$0.020^\circ/\text{frame}$
Frames per degree	12	50
Frames per useful 360°	4320	18,000
Frames per recorded 400° sweep	4800	20,000
Overlap per sweep	$40^\circ / 480 \text{ frames}$	$40^\circ / 2000 \text{ frames}$
Total acquisition time	4000 s	25,000 s

196 The object was measured in one continuous five-sweep rotation without repo-
 197 sitioning. Each recorded sweep spans 400° ; successive useful 360° segments are
 198 shifted by 40° , giving a natural between-sweep angular offset. The 40° overlap
 199 region provides a model-free repeatability check: RMS height difference between
 200 consecutive sweeps is 12 nm (FN 111) and $0.18 \mu\text{m}$ (FN 101), consistent with
 201 Table 4.

202 The frame rates in Table 1 (6 and 4 fps) are far below the 120 fps capability
 203 of the cameras and merit comment. The angular step is set by the ratio
 204 $\Delta\alpha = \omega/\text{fps}$, so angular resolution is governed jointly by rotation speed and
 205 frame rate; measurement time is governed by rotation speed alone. The rotation
 206 speeds (0.50 and $0.08^\circ/\text{s}$) were deliberately conservative: slow, constant-velocity
 207 rotation minimises dynamic excitation of the stage and keeps the fringe pattern
 208 quasi-static within each exposure, and the settling-time protocol (25 s before

acquisition) assumes steady-state velocity. At these speeds, 6 and 4 fps already yield 12 and 50 frames per degree — an oversampling factor of roughly 300 and 1200 relative to the 15 UPR metrological bandwidth — so the frame rate was not the accuracy-limiting factor; increasing it at fixed rotation speed would only add redundant frames. Shorter total acquisition (4,000 and 25,000 s here) would instead require faster rotation with a proportionally higher frame rate, which is technically feasible with the present cameras up to 120 fps. Whether fringe contrast and stage stability are preserved at, say, a tenfold higher speed has not been tested; the trade-off between acquisition speed, vibration robustness, and per-frame phase-extraction quality is identified as a topic for future work, since measurement time is a critical parameter for industrial implementation.

3. Image Processing and Functional-Descriptor Method

3.1. Processing Pipeline

The pipeline follows the radial excess-fraction method of a previous study [25] with added sinusoidal refinement. Each interferogram $I_i(x, y)$ is decoded independently to a wrapped excess fraction ϵ_i ; the sequence is unwrapped chronologically, converted to nanometres ($z_i = \nu_i \lambda / 2$), and reduced by the object-specific LSCI reference model. Sweep boundaries are retained for repeatability analysis.

3.2. Step-by-Step Radial Phase Decoding

For each interferogram $I_i(x, y)$, a radial intensity profile about the fringe centre is extracted and B-spline-smoothed; bright-ring maxima are detected in D^2 space, where circular-fringe theory gives $D_{ij}^2 = c_i(j + \epsilon_i - 1)$ for the j th ring of diameter D_{ij} . A linear fit $D_{ij}^2 = \alpha_i j + \beta_i$ yields the wrapped excess fraction $\epsilon_i = (1 + \beta_i / \alpha_i) \bmod 1$ (2). Where the radial fringe signal permits ($R^2 \geq 0.65$, phase within 0.20 fringe of the ring-diameter estimate), a sinusoidal refinement is applied; otherwise the ring-diameter estimate is retained. The ordered series ϵ_i is unwrapped chronologically to a continuous fringe-order coordinate ν_i , and

the nanometre profile follows from $z_i = \nu_i \lambda / 2$ with $\lambda = 532$ nm (one fringe order $\equiv 266$ nm) (3).

$$D_{ij}^2 = c_i(j + \epsilon_i - 1), \quad (1)$$

$$\epsilon_i = \left(1 + \frac{\beta_i}{\alpha_i}\right) \bmod 1. \quad (2)$$

$$z_i = \nu_i \frac{\lambda}{2}, \quad \lambda = 532 \text{ nm}. \quad (3)$$

3.3. Topography Profile, Reference Removal and Eccentricity Reduction

After phase-to-height conversion, the roundness profile is extracted following ISO 12181-1 [45] (which supersedes the withdrawn ISO 4291 [46]). For each 360° segment, a least-squares reference circle (LSCI) is fitted to the angular height profile $z_i = h(\theta_i)$ in Cartesian coordinates:

$$(x_i, y_i) = ((R_0 + z_i) \cos \theta_i, (R_0 + z_i) \sin \theta_i), \quad (4)$$

where $R_0 = 14.9794$ mm is the nominal radius of the JENOPTIK FN 111. The LSCI centre (x_c, y_c) minimises $\sum_i [\sqrt{(x_i - x_c)^2 + (y_i - y_c)^2} - R_0]^2$, yielding the centred radial residuals ρ_i . The LSCI fit is numerically equivalent to removing the first harmonic of the angular profile, but it provides the formal ISO 4291 reference circle required for roundness metrology. After LSCI centring, a phase-correct Gaussian low-pass profile filter with 50% transmission at 15 undulations per revolution (UPR) is applied to the residual profile, consistent with the filter specification used for the tactile reference measurements and with the Gaussian profile filter defined in ISO 16610-21:2025 [47]. All classical and gradient-based descriptors are computed from this LSCI-centred, Gaussian-filtered residual $\rho_i^{(\text{filt})}$.

For the JENOPTIK magnification standard FN 101, the same processing chain is applied: a linear trend is removed from the unwrapped phase sequence before height conversion (Sec. 5.1), the LSCI reference circle is fitted to the angular profile, and the Gaussian low-pass filter (50% at 15 UPR) is applied. Although both artefacts are processed through identical filtering steps,

the 15 UPR cutoff corresponds to different spatial wavelengths on the circumference: $2\pi \times 14.9794 \text{ mm}/15 = 6.27 \text{ mm}$ for the FN 111 ($\varnothing = 29.9588 \text{ mm}$) and $2\pi \times 15 \text{ mm}/15 = 6.28 \text{ mm}$ for the FN 101 ($\varnothing \approx 30 \text{ mm}$) — effectively identical. The angular sampling differs substantially (0.083° vs. 0.020° , Table 1), but the Gaussian filter sigma is set by the UPR cutoff, not by the sampling interval, so the filtered profiles are directly comparable.

3.4. Classical Profile and Roundness Metrics

All classical quantities are evaluated on nanometre residuals, not on raw intensities, following the profile method of ISO [21920-2 \[48\]](#), [which supersedes the earlier ISO 4287 \[49\]](#); [the amplitude-parameter definitions used here are common to both documents, and ISO 4287 is retained as a secondary reference because the tactile comparison data and the previous study \[25\] predate the transition](#). Areal parameters (ISO 25178 [50]) are not reported because the single-image radial extraction does not produce a calibrated areal height map. For a residual profile or vector of residual pixels p , the reported profile-style roughness descriptors are

$$R_a = \frac{1}{M} \sum_{j=1}^M |p_j - \bar{p}|, \quad R_q = \left[\frac{1}{M} \sum_{j=1}^M (p_j - \bar{p})^2 \right]^{1/2}, \quad (5)$$

and

$$R_z = \max_j (p_j - \bar{p}) - \min_j (p_j - \bar{p}). \quad (6)$$

[As implemented, this quantity is the global peak-to-valley height of the full evaluation profile, corresponding to the total-height parameter \(\$R_t\$ in ISO 21920-2 terms\) rather than the section-averaged \$R_z\$; the symbol \$R_z\$ is retained for continuity with the previous study \[25\]. This implementation detail is relevant to the interpretation of Table 4 \(Sec. 4.3\).](#) The profile skewness R_{sk} and kurtosis R_{ku} — ISO [4287-21920-2](#) shape parameters that characterise asymmetry and peakedness of the height distribution — are also reported:

$$R_{sk} = \frac{1}{R_q^3} \frac{1}{M} \sum_{j=1}^M (p_j - \bar{p})^3, \quad R_{ku} = \frac{1}{R_q^4} \frac{1}{M} \sum_{j=1}^M (p_j - \bar{p})^4. \quad (7)$$

285 $R_{sk} = 0$ for a symmetric distribution; $R_{sk} < 0$ indicates a predominance
 286 of valleys over peaks. $R_{ku} = 3$ for a normal distribution; $R_{ku} > 3$ indi-
 287 cates a spikier (leptokurtic) profile. These are the only ISO ~~4287-21920-2~~
 288 [amplitude-distribution](#) parameters that capture distribution shape beyond am-
 289 plitude averages, and their inclusion allows a direct test of whether gradient-
 290 based descriptors provide information beyond even the best ISO shape param-
 291 eters. For the eccentricity-corrected ceramic angular profile $q_C(\theta)$,

$$RONt = \max_{\theta} q_C(\theta) - \min_{\theta} q_C(\theta), \quad RONq = \left[\frac{1}{2\pi} \int_0^{2\pi} q_C^2(\theta) d\theta \right]^{1/2}. \quad (8)$$

292 These are profile/form quantities in nanometres. B-spline pre-smoothing (20
 293 degrees of freedom, $\approx 18^\circ$ period) stabilises the LSCI fit; the subsequent Gaus-
 294 sian low-pass filter (50% at 15 UPR, ISO 16610-21:[2025](#)) defines the metrolog-
 295 ical bandwidth. All descriptors are computed from the same Gaussian-filtered
 296 residual.

297 3.5. Functional Gradient-Based Descriptors

298 The concept of a complete normed vector space originates from the founda-
 299 tional work of Banach [51]. For discrete profile data of finite length N , the vector
 300 space $\mathbb{R}^N$ equipped with any norm is a Banach space; the present work does
 301 not invoke infinite-dimensional completeness but draws on the taxonomy of L^p ,
 302 Sobolev, and bounded-variation norms that Banach's framework systematised.
 303 For a centred residual profile $p(s)$ and $1 \leq p < \infty$,

$$\|p\|_p = \left(\frac{1}{L} \int_0^L |p(s)|^p ds \right)^{1/p}, \quad \|p\|_\infty = \max_{s \in [0, L]} |p(s)|. \quad (9)$$

304 The reported functional descriptors include L^1 , L^2 , L^∞ , the one-dimensional
 305 Sobolev $W^{1,2}$ seminorm and the bounded-variation (BV) total variation,

$$|p|_{W^{1,2}} = \left(\int_0^L \left| \frac{dp}{ds} \right|^2 ds \right)^{1/2}, \quad TV(p) = \int_0^L \left| \frac{dp}{ds} \right| ds. \quad (10)$$

306 In discrete form, for a uniformly sampled profile p_j ($j = 1, \dots, N$) with angular
 307 spacing $\Delta\alpha$,

$$|p|_{W^{1,2}} \approx \left(\Delta\alpha \sum_{j=1}^{N-1} \left(\frac{p_{j+1} - p_j}{\Delta\alpha} \right)^2 \right)^{1/2}, \quad TV(p) \approx \sum_{j=1}^{N-1} |p_{j+1} - p_j|. \quad (11)$$

308 Both $W^{1,2}$ and BV density carry sampling-interval dependence ~~and require conversion~~
 309 ~~to angular units ($\text{nm deg}^{-1/2}$ and nm deg^{-1} , respectively) for cross-instrument~~
 310 ~~comparison~~; “nm sample $^{-1}$ ” is retained in the result tables for the fixed-acquisition
 311 setup, ~~and a standardised angular-unit convention for cross-instrument comparison~~
 312 is defined in Sec. 3.6.

313 The curvature RMS (root-mean-square of the discrete second derivative;
 314 reported in Supplementary Table S2) carries a $(\Delta\alpha)^{-2}$ sampling dependence and
 315 should not be compared across instruments with different angular resolution.

316 3.6. ~~Repeatability Uncertainty~~ Angular-Unit Convention for Sampling-Dependent 317 Descriptors

318 Gradient-based descriptors evaluated on discretely sampled profiles depend
 319 on the sampling interval: the discrete total variation of an unfiltered profile
 320 grows as the sampling grid refines (noise contributes gradient content at every
 321 scale), so raw per-sample values are instrument-specific. For meaningful cross-instrument
 322 comparison the following convention is proposed and used here.

- 323 1. **Band-limit first.** The profile is filtered with a declared phase-correct
 324 Gaussian profile filter (ISO 16610-21:2025) at a stated cutoff in undulations
 325 per revolution (here 50% transmission at 15 UPR). After band-limiting,
 326 the profile derivative is bounded and the discrete sums converge to the
 327 continuous integrals as $\Delta\alpha \rightarrow 0$; the descriptor then characterises the
 328 declared bandwidth rather than the sampling grid.
- 329 2. **Sample adequately.** The angular sampling must resolve the declared
 330 bandwidth with margin; at least ten samples per cutoff undulation are
 331 recommended. Here the FN 111 and FN 101 profiles carry ≈ 290 and

≈ 1200 samples per 15-UPR undulation, so discretisation error is negligible.

3. **Report in angular units.** The BV density is reported as total variation per unit angle, $BV_\theta = TV(p)/\Theta$ in nm deg^{-1} ($\Theta = 360^\circ$), and the gradient content as the RMS angular gradient $g_{\text{rms}} = [\frac{1}{N-1} \sum_j ((p_{j+1} - p_j)/\Delta\alpha)^2]^{1/2}$ in nm deg^{-1} , together with the filter cutoff. For comparison across artefacts or instruments of *different diameter*, the angular unit is additionally converted to an arc-length unit by dividing by the arc length per degree, $\pi D/360$; the BV density is then $BV_s = TV(p)/(\pi D)$ in nm mm^{-1} . The arc-length form is the diameter-independent unit and is the one recommended for cross-instrument reporting, since nm deg^{-1} still scales with the circumference of the specific artefact.

A note on physical dimensions clarifies why this is necessary and is itself part of the answer to the redundancy question (Sec. 5.3). Amplitude descriptors (R_a , R_q , L^1 , L^2 , L^∞ , $RONt$) have the dimension of length (nm) and are sampling-independent. Gradient descriptors are dimensionally distinct: BV density and the RMS gradient are height-per-length (nm mm^{-1}), i.e. dimensionless slopes, while the $W^{1,2}$ seminorm as defined here is $\text{height} \times \text{length}^{-1/2}$. This dimensional separation is the reason the gradient layer carries information that no amplitude parameter can encode, and also the reason its raw per-sample value must be qualified by a sampling and filter declaration.

For the present data, the per-sample values in Table 4 convert as follows.
 FN 111 ($\Delta\alpha = 0.083^\circ$): BV density $0.263 \text{ nm sample}^{-1} \rightarrow 3.2 \text{ nm deg}^{-1} \rightarrow 12.1 \text{ nm mm}^{-1}$; RMS gradient $0.310 \text{ nm sample}^{-1} \rightarrow 3.7 \text{ nm deg}^{-1} \rightarrow 14.2 \text{ nm mm}^{-1}$.
 FN 101 ($\Delta\alpha = 0.020^\circ$): BV density $6.58 \text{ nm sample}^{-1} \rightarrow 329 \text{ nm deg}^{-1} \rightarrow 1.26 \text{ } \mu\text{m mm}^{-1}$; RMS gradient $8.76 \text{ nm sample}^{-1} \rightarrow 438 \text{ nm deg}^{-1} \rightarrow 1.67 \text{ } \mu\text{m mm}^{-1}$, all at the 15-UPR cutoff. The two artefacts have almost identical circumference ($\pi D \approx 94.1$ and 94.2 mm), so the large difference in arc-length gradient content (12 versus 1257 nm mm^{-1}) reflects a genuine difference in surface variation rather than a unit artefact. Because each conversion is a fixed multiplicative

factor for a given acquisition, relative uncertainties and relative defect responses are identical in every unit system. Adoption of gradient descriptors in reference software for roundness evaluation would require exactly this pair of declarations — filter cutoff and arc-length units — which parallels the established practice of declaring the filter for $RONt$.

An empirical demonstration that this convention removes the sampling dependence is obtained by decimating the FN 111 residual of session A from 12 to 1 samples per degree (a factor of 12) and recomputing the descriptors with the 15-UPR Gaussian filter matched to each sampling. The band-limited BV density and RMS gradient change by less than 0.5% across the full decimation range, whereas the unfiltered total variation drops by a factor of 3.3 over the same range. This confirms that the declared filter — not the sampling grid — defines the descriptor value, and shows that the recommendation of at least ten samples per cutoff undulation is conservative: even 24 samples per cutoff undulation reproduce the band-limited values to within 0.5%.

3.7. *Uncertainty Evaluation*

Each dataset contains five 400° sweeps recorded in a single continuous rotation without stopping or repositioning. The five useful 360° segments are extracted from this continuous sequence; because each recorded sweep spans 400° , successive useful revolutions are shifted by 40° on the object. These segments are not strictly independent — they share the same continuous-run conditions (laser warm-up state, stage-bearing temperature, ambient drift). The standard deviation across sweeps therefore reflects within-run repeatability rather than between-run reproducibility. For a descriptor X evaluated on each sweep, the mean value is $\bar{X}$ and the within-run standard uncertainty is estimated as

$$u_{\text{within}}(X) = \frac{s_X}{\sqrt{n}}, \quad n = 5, \quad (12)$$

where s_X is the sample standard deviation across the five sweeps. The reported expanded uncertainty is

$$U_{95}(X) = t_{0.975, n-1} u_{\text{within}}(X). \quad (13)$$

With $n = 5$, $t_{0.975,4} = 2.776$; the χ^2_4 -based 95% CI for the standard deviation spans $[0.6s_X, 2.9s_X]$, so U_{95} is indicative rather than definitive. Because the five segments share continuous-run conditions (laser state, stage temperature, ambient drift), the $1/\sqrt{n}$ factor in u_{within} may underestimate the true uncertainty of the mean; all reported uncertainties are *lower bounds*. ~~A full GUM-compliant budget (An indicative type-B terms: laser wavelength stability, refractive-index variations, Abbe error [52], camera nonlinearity, form-removal uncertainty) is beyond the present scope~~ budget for the principal systematic terms is given in Sec. 3.8; a complete GUM-compliant budget [53] with experimentally characterised input distributions, and a between-run reproducibility study with independent setups, thermal cycles, and physical re-centring of the artefact, remain future work (Sec. 5.6). With $n = 5$ sweeps and the observed within-run variability, the minimum detectable relative difference between two descriptors (80% power, $\alpha = 0.05$, two-sided paired t -test) is approximately 30% for the FN 111 and 5% for the FN 101, consistent with the exploratory character of the descriptor comparison. A per-sweep trend of FN 111 $RONt$ values gives a slope of $8.4 \pm 4.1 \text{ nm sweep}^{-1}$ ($p = 0.12$), consistent with zero drift, though the sweep-to-sweep scatter cautions that U_{95} may underestimate long-term reproducibility.

3.8. Indicative Type-B Uncertainty Budget

Although a complete GUM budget requires between-run data that the present single-rotation acquisition cannot supply, the principal type-B contributions can be bounded from component specifications and pipeline properties. Table 2 summarises the estimates for the FN 111 $RONt$ evaluation; the same relative arguments apply to the FN 101.

Laser wavelength stability. The height scale $z = \nu\lambda/2$ inherits the relative wavelength error: a $\pm 1 \text{ nm}$ tolerance on the 532 nm diode module (rectangular distribution) gives a relative standard uncertainty of 0.11%, i.e. 0.3 nm on $RONt = 278 \text{ nm}$ (and 46 nm on the FN 101 $RONt = 42.07 \mu\text{m}$, within its $\pm 0.48 \mu\text{m}$ repeatability interval). Wavelength error acts as a pure scale factor and cannot create or mask localised features.

419 *Refractive index of air.* The in-air wavelength varies with temperature and
 420 pressure by $\sim 10^{-6}$ per 1°C or 3 hPa; with the observed $\pm 0.2^\circ\text{C}$ stability the
 421 contribution is below 10^{-5} relative, i.e. < 0.01 nm. Negligible.

422 *Abbe error and stage wobble.* The specified axis wobble (± 12 μrad) enters
 423 through two mechanisms: a cosine-type radial error $R\theta_w^2/2 \approx 1$ pm, and a
 424 lateral beam walk $R\theta_w \approx 0.18$ μm on the circumference, equivalent to an angular
 425 mislocation of 0.0007° , which maps through the local band-limited gradient
 426 (≈ 3.2 nm deg^{-1} , Sec. 3.6) to ≈ 0.002 nm. Both are negligible after LSCI
 427 first-harmonic removal.

428 *Camera nonlinearity and EFM localisation.* Intensity nonlinearity perturbs
 429 the radial fringe-peak positions; its effect is bounded empirically by the per-frame
 430 excess-fraction uncertainty of ± 0.05 fringe (13 nm). The 15-UPR band limit
 431 averages ≈ 290 frames per resolved undulation, reducing the per-point contribution
 432 to ≈ 0.8 nm and the peak-to-valley contribution to ≈ 1.1 nm.

433 *Long-term drift and phase noise floor (measured).* An independent static
 434 stability session, recorded with the same interferometer, camera settings and
 435 frame count as the FN 111 acquisition (24,000 frames over 4,000 s) but with the
 436 object not rotating, provides a direct experimental bound on slow instrument
 437 drift under realistic laboratory conditions. The decoded excess-fraction sequence
 438 spans only 98 nm over the full session, with an end-to-end linear drift of -82 nm
 439 (-1.1 nm min^{-1}), i.e. ≈ 15 nm over one 800 s sweep-equivalent interval; after
 440 linear detrending the residual has 9.4 nm standard deviation (45 nm peak-to-valley),
 441 and the frame-to-frame phase noise floor is 2.1 nm (0.008 fringe). Two conclusions
 442 follow. First, the measured static noise floor is well below the conservative
 443 ± 0.05 -fringe EFM bound used above, confirming that bound as conservative.
 444 Second, the slow drift maps predominantly to low harmonic orders of the angular
 445 profile, where it is largely absorbed by the LSCI first-harmonic removal, and
 446 its sweep-to-sweep manifestation is already contained in the type-A scatter; the
 447 drift bound is therefore reported as an informative constraint rather than added
 448 in quadrature.

449 *Form removal.* The LSCI reference (first-harmonic removal) is exact only in

the limaçon approximation; the second-order term $a^2/(2R)$ for residual centring eccentricity a leaks into the second harmonic of the residual. Manual centring leaves a of the order of tens of micrometres (the shared first-harmonic model of Sec. 5.2.1, with its 63 nm/0.18% per-sweep amplitude variation, implies $a \approx 35 \mu\text{m}$); for $a = 15\text{--}35 \mu\text{m}$ the term evaluates to 7–41 nm. Because this contribution is common to all five sweeps, it does not appear in the type-A scatter and must be carried as a bounded systematic term. Its magnitude is consistent with the 34 nm difference between the optical *RONt* (278 ± 22 nm) and the certified tactile value (244 ± 52 nm), a difference that the $E_n = 0.61$ comparison shows to be within the combined uncertainties.

The quadrature combination is dominated by the type-A term, so the reported U_{95} values are essentially unchanged by the enumerated random type-B terms; the budget nevertheless shows that the leading risks are the form-removal systematic and the between-run effects bounded in Sec. 3.9, not the enumerated instrument terms.

3.9. *Between-Run Reproducibility of Independent Sessions*

Two further independent acquisition sessions of the FN 111 were processed through the identical pipeline and descriptor computation (per-sweep LSCI-centred residual, circular Gaussian low-pass filter at 15 UPR) to assess between-run reproducibility with the archived material. The primary archive reported in Tables 1 and 4 is denoted session A. Session B (0.50°/s, 6 fps, 24,000 frames) repeats its acquisition parameters; session C (0.64°/s, 8 fps, 25,000 frames, 0.08°/frame) uses a different rotation speed and frame rate at nearly the same angular sampling. Sessions B and C were recorded on different days with the artefact re-mounted and re-centred. Table 3 reports the relative between-session differences and the E_n compatibility statistic, $E_n = |\Delta|/(2\sqrt{u_A^2 + u_B^2})$, with the standard uncertainties of the per-sweep means ($n = 5$).

For session B, every descriptor agrees with session A within its combined uncertainty ($|E_n| < 1$): the amplitude parameters differ by less than 3% and the gradient descriptors by about 4% (BV density, $E_n = 0.99$, is the largest),

Table 2: Indicative type-B uncertainty budget for the FN 111 $RONt$ evaluation. Random contributions are standard uncertainties combined in quadrature with the type-A term; the form-removal term is a bounded systematic (bias) contribution common to all sweeps and is reported separately.

Source	Basis	Contribution to $RONt$
Within-run repeatability (type A)	$s/\sqrt{5}$, five sweeps	7.9 nm
Laser wavelength (± 1 nm, rect.)	module specification	0.3 nm
Air refractive index ($\pm 0.2^\circ\text{C}$)	Edlén-type sensitivity	< 0.01 nm
Abbe error / axis wobble ($\pm 12 \mu\text{rad}$)	stage specification, geometry	< 0.01 nm
Camera nonlinearity / EFM localisation	± 0.05 fringe per frame, band-limited averaging	1.1 nm
Long-term drift (measured, static session)	-1.1 nm min^{-1} , < 15 nm per sweep	informative bound [†]
Combined standard uncertainty u_c (random)	quadrature	8.0 nm
Expanded U_{95} (random, $t_{0.975,4}$)		22 nm
Form removal (limaçon second order)	$a^2/(2R)$, $a = 15\text{--}35 \mu\text{m}$	< 41 nm (syst. bound)

[†]Measured in an independent static session (Sec. 3.8); manifested in the type-A scatter and largely removed with the first harmonic, hence not added in quadrature.

Table 3: Between-session comparison for the FN 111. Session A is the primary archive reported in Tables 1–3; sessions B and C are independent repeat acquisitions (B: same parameters; C: 0.64°/s, 8 fps) with the artefact re-mounted and re-centred. Relative differences and E_n compatibility values are reported; $E_n < 1$ indicates agreement within the combined standard uncertainties of the per-sweep means.

Descriptor	B vs. A		C vs. A	
	rel. diff.	E_n	rel. diff.	E_n
R_q	−2.4%	0.35	+7.0%	1.45
R_q	−2.0%	0.23	+8.8%	1.51
$RONt$	−2.9%	0.23	+12.3%	1.16
L^∞	−0.1%	0.00	+11.6%	0.79
BV density	−4.0%	0.99	+4.4%	1.25
$W^{1,2}$ grad.	−3.8%	0.88	+4.6%	1.40

showing that BV density and the $W^{1,2}$ seminorm are between-run stable to the same order as the classical parameters under identical acquisition parameters. For session C, the amplitude descriptors differ by 7–12% (E_n up to 1.5); the $RONt$ difference of 42 nm is comparable to the ≤ 41 nm form-removal bound of Sec. 3.8, indicating that the dominant between-session variation arises from re-centring (first-harmonic leakage) rather than from the change of rotation speed or frame rate. The gradient descriptors change by +4% (per-sample) to +9% (angular units), tracking the shared amplitude change with no sampling-induced anomaly. Together with the static-session drift bound (Sec. 3.8), these results establish the first quantitative between-run stability statement for the gradient-based descriptors; a full multi-session campaign remains future work (Sec. 5.6).

3.10. Computational Implementation

The reconstruction workflow (`scripts/reconstruct_radial_profile_sequence.py`) decodes ϵ_i from each interferogram, unwraps the sequence, converts to nanometres, applies LSCI fitting and Gaussian low-pass filtering (50% at 15 UPR, ISO 16610-21:2025), and exports CSV/JSON metrics with sweep-repeatability uncertainty. Vector PDF figures document each processing stage. The pipeline is invoked as `PYTHONPATH=src.venv/bin/pythonscripts/reconstruct_radial_`

498 `profile_sequence.py` with dataset-specific parameters (full command in the
 499 data repository). Per-image excess-fraction decoding and unwrapping require
 500 approximately 0.5 ms per frame (measured on an Intel Core i7-9700K, single-
 501 threaded Python 3.9), so the full 124,000-frame archive processes in under two
 502 minutes on consumer hardware.

503 4. Results

504 The results follow the updated radial sequence route only. Each raw im-
 505 age is first decoded to a wrapped excess fraction from its radial fringe pat-
 506 tern. The ordered excess-fraction series is then unwrapped in chronological
 507 order, converted to nanometres, and corrected for eccentricity. Finally, classi-
 508 cal profile/roundness descriptors and functional gradient-based descriptors are
 509 computed from the same nanometre residual profiles.

510 4.1. Radial Phase Decoding and Nanometre Profile Reconstruction

511 The FN 111 folder contained 24,000 interferograms and the steel folder con-
 512 tained 100,000 interferograms. The reported run used full-resolution images, the
 513 central radial aperture of 240 px, B-spline-smoothed peak detection, continuity-
 514 aware EFM peak-subset tracking and an EFM prominence threshold of 0.04 of
 515 the radial fringe-signal range. All five recorded sweeps were processed.

516 Figs. S3–S6 (single-image EFM and sequence processing steps) are provided
 517 in the Supplementary Materials.

518 4.2. Roughness, Roundness and Functional Descriptors

519 Table 4 gives the numerical comparison after LSCI reference circle and Gaus-
 520 sian low-pass filtering (50% at 15 UPR). Both artefacts are processed through
 521 the same filtering chain. Each descriptor is reported as the full-sequence value
 522 together with the 95% expanded type-A repeatability uncertainty estimated
 523 from the five sweeps. Per-sweep values for all descriptors are provided in Sup-
 524plementary Table S3.

525 ~~The numerical identity $RONt = R_z$~~

Table 4: Full-resolution radial EFM reconstruction from raw interferograms (LSCI + Gaussian low-pass, 50% at 15 UPR, ISO 16610-21:2025). Uncertainties are 95% expanded within-run repeatability estimates from five sweeps ($n = 5$, $t_{0.975,4} = 2.776$). Units: nm for all descriptors except BV density and $W^{1,2}$ gradient (nm sample $^{-1}$). Certified *RONt*: FN 111 244 ± 52 nm (Hommel Roundscan 535, $n = 104$); FN 101 $41.94 \mu\text{m}$ (form tester, $n = 12$). The FN 101 certificate does not report an expanded uncertainty; therefore only the percentage difference is reported for this artefact rather than an E_n score.

Descriptor	FN 111	FN 101
R_a	66.3 ± 4.7 (<u>66.3 ± 4.7</u>) nm	8.525 ± 0.115 (<u>8.525 ± 0.115</u>) μm
R_q	77.6 ± 5.0 (<u>77.6 ± 5.0</u>) nm	10.376 ± 0.090 (<u>10.376 ± 0.090</u>) μm
R_z	278 ± 22 (<u>278 ± 22</u>) nm	42.07 ± 0.48 (<u>42.07 ± 0.48</u>) μm
<i>RONt</i>	278 ± 22 (<u>278 ± 22</u>) nm	42.07 ± 0.48 (<u>42.07 ± 0.48</u>) μm
<i>RONq</i>	77.6 ± 5.0 (<u>77.6 ± 5.0</u>) nm	10.376 ± 0.090 (<u>10.376 ± 0.090</u>) μm
L^1 mean	66.3 ± 4.7 (<u>66.3 ± 4.7</u>) nm	8.525 ± 0.115 (<u>8.525 ± 0.115</u>) μm
L^2 RMS	77.6 ± 5.0 (<u>77.6 ± 5.0</u>) nm	10.376 ± 0.090 (<u>10.376 ± 0.090</u>) μm
L^∞	150 ± 12 (<u>150 ± 12</u>) nm	21.97 ± 0.42 (<u>21.97 ± 0.42</u>) μm
BV total	1.137 ± 0.062 (<u>1.137 ± 0.062</u>) μm	118.4 ± 6.2 (<u>118.4 ± 6.2</u>) μm
BV density	0.263 ± 0.014 (<u>0.263 ± 0.014</u>) nm sample $^{-1}$	6.58 ± 0.35 (<u>6.58 ± 0.35</u>) nm sample $^{-1}$
$W^{1,2}$ grad.	0.310 ± 0.015 (<u>0.310 ± 0.015</u>) nm sample $^{-1}$	8.76 ± 0.43 (<u>8.76 ± 0.43</u>) nm sample $^{-1}$
<i>ISO shape parameters</i>		
R_{sk} (skewness)	-0.09 ± 0.04	0.00 ± 0.09
R_{ku} (kurtosis)	1.98 ± 0.21	2.51 ± 0.08
<i>Derived norm ratios</i>		
L^4/L^1 peakiness	1.39 ± 0.08	1.53 ± 0.03
<i>External validation</i>		
E_n score	0.61	< 1 (0.3% diff.; cf. Fig. S12)

526 4.3. *Coincidence of R_z with $RONt$ and R_q with $RONq$*

527 The identical values of R_z and $RONt$ (and of R_q and $RONq$) for both
528 artefacts (in Table 4) ~~reflects the fact that after LSCI centring and Gaussian~~
529 ~~low-pass filtering (50% at 15 UPR), the residual profile is dominated by a single~~
530 ~~lobe (harmonic decomposition are expected by construction, not coincidental. In~~
531 ~~this pipeline both descriptor families are evaluated on the same LSCI-centred,~~
532 ~~Gaussian-filtered closed residual profile (Sec. 3.3; harmonic decomposition of~~
533 ~~the residual: Supplementary Fig. S19); the~~ the roughness-style R_z is the
534 global peak-to-valley height of that profile (i.e., the total height Rt ; see the
535 implementation note in the definition), while $RONt$ is the peak-to-valley round-
536 ness deviation ~~and the profile roughness peak-to-valley therefore coincide. This~~
537 ~~identity is specific to the present artefact-filter combination and should not be~~
538 ~~expected to hold for artefacts with multi-lobed form deviations or for different~~
539 ~~filter cutoffs~~ of the very same profile, so the two coincide exactly; the RMS pair
540 $R_q/RONq$ coincides for the same reason. The two families would separate if
541 profile texture were evaluated on a different bandwidth than form (e.g., after
542 λc -based separation of roughness from waviness in the ISO 21920 sense) or on an
543 independent linear trace. Both are nevertheless reported because they belong
544 to different ISO frameworks (profile texture versus roundness) with different
545 reference conventions, and because their exact equality serves as a verification
546 that all descriptors share one evaluation profile — the design premise of the
547 like-for-like comparison.

548 4.4. *Classical-Functional-Descriptor Comparison*

549 The ~~numerical identity~~ exact equalities $R_a = L^1$ and $R_q = L^2$ (in Table 4)
550 ~~confirms~~ are definitional — each pair is the same formula applied to the same
551 centred residual — and are reported purely as a computational cross-check that
552 both descriptor families are evaluated on ~~the same nanometre residual identical~~
553 ~~data, not as an empirical finding (see Sec. 5.3).~~ For the FN 111, BV total
554 variation carries 1.2% relative expanded uncertainty versus 5.5% for R_a and
555 8.5% for R_z , suggesting that gradient-based descriptors may exhibit metrological

556 stability comparable to or better than peak-referenced roughness parameters
 557 in the tested datasets. Comparative bar charts and uncertainty analyses are
 558 provided in the Supplementary Materials (Figs. S7–S8). Ceramic and steel
 559 profile reconstruction plots are shown in Supplementary Figs. S9–S10.

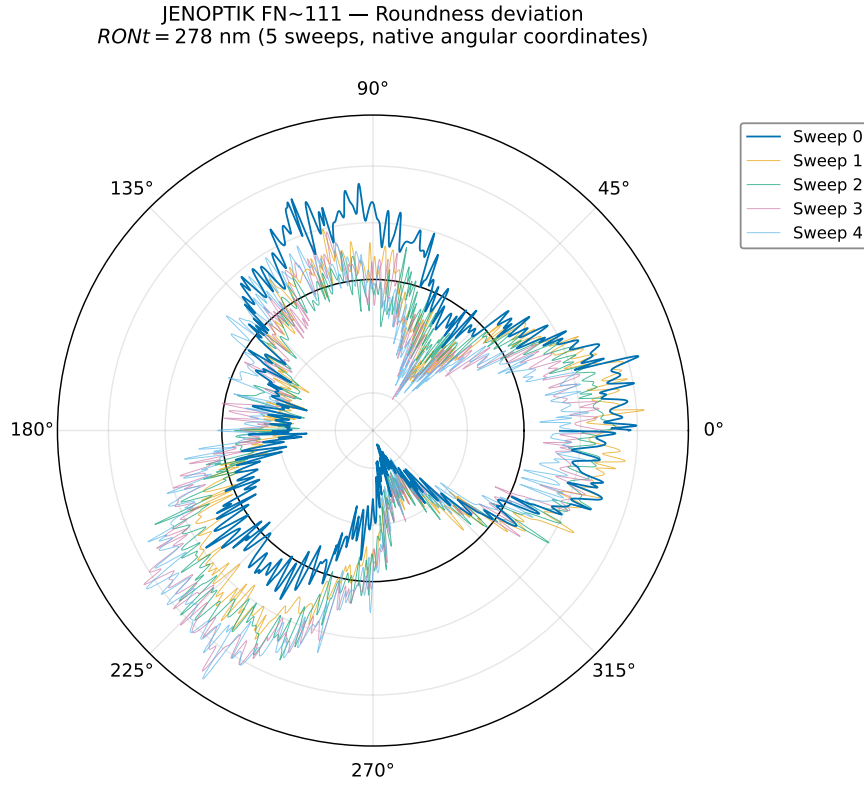


Figure 3: Ceramic roundness in polar coordinates (LSCI + Gaussian low-pass, 50% at 15 UPR). Five sweeps at native positions. $RONt = 278 \pm 22$ nm.

560 The steel roundness polar representation (FN 101, Flick flat) is provided in
 561 the Supplementary Materials (Fig. S11).

562 The Flick flat produces a clear response in BV density while showing no

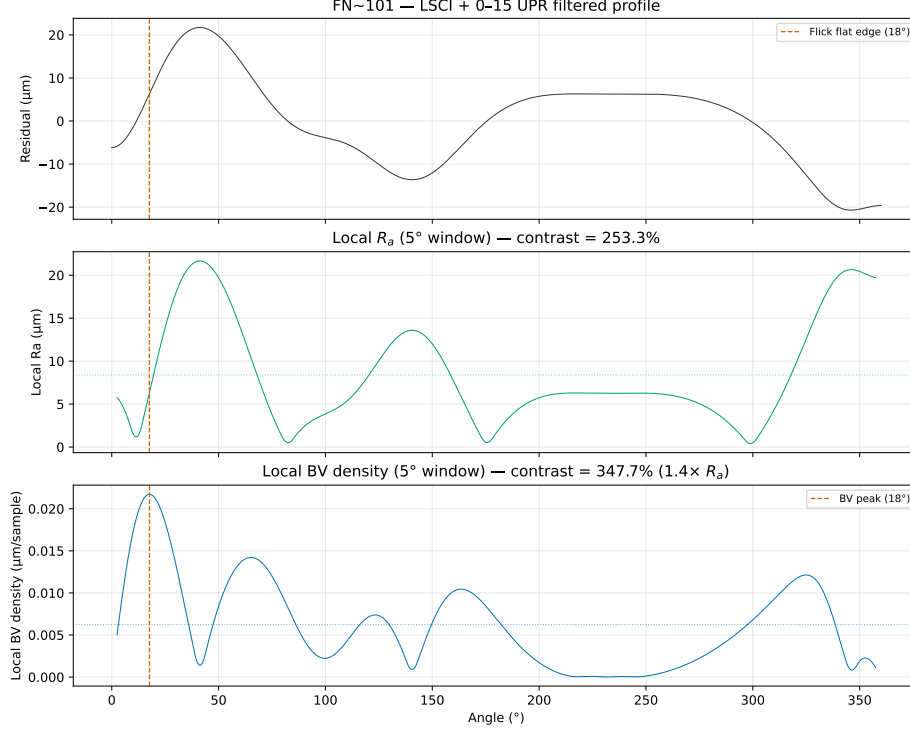


Figure 4: Flick flat detection on the FN 101 magnification standard. BV density (bottom) shows a clear spike at the Flick flat angular position, whereas R_a computed in a sliding window (top) shows no detectable response at the reconstruction resolution. The sliding-window width was matched to the certified angular extent of the Flick flat as specified in the DAkKS-DKD certificate (Art. 532 528); identical window parameters were used for both descriptors.

563 detectable response in a sliding-window R_a analysis at the reconstruction reso-
 564 lution (Fig. 4), illustrating the potential complementary sensitivity of gradient-
 565 based descriptors to localised geometric features.

566 5. Discussion

567 5.1. Confirmed Results

568 The analysis rests on a key metrological distinction: an interferogram is
 569 an intensity measurement, not a phase map and not a height map. The half-
 570 wavelength relation $z = \nu\lambda/2$ becomes valid only after each image has been

571 decoded to a wrapped excess fraction and the ordered excess-fraction sequence
 572 has been unwrapped to the continuous fringe-order coordinate ν . This is why
 573 the reported comparison uses only reconstructed nanometre profiles, not raw
 574 greyscale images and not areal height maps.

575 The most sensitive part of the workflow is the EFM localisation of bright-
 576 ring maxima, with an excess-fraction uncertainty of approximately ± 0.05 fringe
 577 orders (tightened to ± 0.03 by sinusoidal refinement in 72% of FN 111 frames).
 578 A single ϵ_i error of 0.05 fringe corresponds to 13 nm, sub-dominant to the
 579 85 nm residual-profile RMS. The chronological unwrapping criterion rejects
 580 phase jumps exceeding 0.35 fringe. The median number of detected rings is
 581 three for both artefacts within the 240 px central aperture. The five 400° ce-
 582 ramic sweeps require a geometric correction: successive useful 360° intervals are
 583 shifted by 40° because the physical object angle advances continuously; without
 584 this correction, the LSCI fit appears inconsistent even when phase extraction
 585 within each sweep is repeatable.

586 The linear drift of $0.0246 \text{ fringe frame}^{-1}$ in the steel unwrapped phase se-
 587 quence (versus 0.00021 for the FN 111) is attributed to cumulative bias in the
 588 global unwrapping algorithm rather than thermal effects or axial runout [52].
 589 The lower fringe contrast of the FN 101 interferograms — likely due to surface
 590 finish — reduces per-frame EFM quality; the pipeline applies automatic linear
 591 detrending where needed.

592 *5.2. Interpretation*

593 *5.2.1. Eccentricity removal and wobble verification*

594 Roundness descriptors are computed after LSCI reference-circle fitting (Sec. 3.3),
 595 which removes the first harmonic. A shared model across all five sweeps yields
 596 $R^2 = 0.99991$ with per-sweep amplitude variation of 63 nm (0.18%); the manufacturer-
 597 specified wobble ($\pm 12 \mu\text{rad}$) bounds the observed variation an order of magni-
 598 tude below $RONt = 278 \text{ nm}$. The polar representation (Fig. 3) shows five
 599 overlaid sweeps repeatable to $\pm 50 \text{ nm}$, illustrating that the residual is domi-
 600 nated by low-order form deviation rather than random roughness.

5.3. Comparison with ISO Parameters

A central question of this work is whether gradient-based functional descriptors provide additional descriptive sensitivity alongside classical ISO parameters when applied to the same reconstructed profiles. To answer this rigorously, every descriptor was computed on the same reconstructed nanometre residual profiles.

Mathematical equivalences. The L^1 norm is defined as $\frac{1}{N} \sum |p_i - \bar{p}|$, which is identical to the definition of R_a . The L^2 norm is $\sqrt{\frac{1}{N} \sum (p_i - \bar{p})^2}$, identical to R_q . Computing both on the same centred residual yields *exact numerical equality*: $R_a - L^1 = 0$ and $R_q - L^2 = 0$ to machine precision for both artefacts (Table 4). These equalities are not empirical findings; they are definitional consequences. Labelling the arithmetic mean of absolute deviations as L^1 rather than R_a provides no new metrological information and should not be presented as a methodological advance.

It is emphasised that neither the L^p norms nor the Sobolev and BV semi-norms are presented as novel mathematical constructs; they are standard tools whose definitions are restated for completeness. Their value in the present context is threefold. First, the functional-analytic taxonomy places ISO parameters at specific positions (L^1 , L^2 , L^∞) within a larger space of possible descriptors, revealing that descriptors outside the ISO set — BV density, $W^{1,2}$ seminorm — respond differently to the same perturbations. Second, the synthetic-defect injection methodology provides a controlled, like-for-like comparison framework that can be applied to any descriptor computed from the same residual profile; the framework itself, rather than any individual norm, constitutes the methodological contribution. Third, the Flick flat on the certified FN 101 standard provides a concrete existence proof: a real, DAkkS-DKD-certified artefact whose defining geometric feature is detected unambiguously by BV density while remaining below the detection threshold of sliding-window R_a (Fig. 4).

Extrema: R_z versus L^∞ . $R_z/L^\infty \approx 2$ for both artefacts, consistent with symmetric positive and negative excursions. L^∞ captures the single largest one-sided excursion; the ratio serves as a simple symmetry indicator.

631 **Variation-based descriptors.** A controlled sensitivity analysis (Supple-
632 mentary Table S2) examined five synthetic defect types injected into the FN 111
633 residual profile. Amplitude-averaging descriptors (R_a , R_q , R_z) showed no de-
634 tectable change at the reconstruction resolution — a single 100 nm spike changed
635 R_a by less than 0.05%, below the per-frame phase-extraction precision — while
636 BV density increased by +18% and the $W^{1,2}$ gradient seminorm by +622% for
637 the same spike (Fig. 5). ISO shape parameters responded to asymmetry (R_{sk}
638 changed by −1104% for a step) but not to symmetric localised features. R_{sk}
639 and BV density appear complementary in the tested scenarios: R_{sk} responds to
640 asymmetry, BV density responds to localised gradients.

641 Translation of synthetic responses to realistic defects. The injected
642 defects are idealised (isolated spike, uniform scratch, pure sinusoid), whereas
643 real manufacturing defects have complex, random morphologies. The synthetic
644 responses nevertheless translate to other backgrounds through a simple scaling
645 argument. A localised defect adds a total-variation increment ΔTV that depends
646 only on the defect geometry ($\Delta TV \approx 2A$ for an isolated spike of amplitude
647 A), so the relative full-profile BV-density response is $\Delta TV/TV_{\text{background}}$. On
648 the FN 111 background ($TV = 1.137 \mu\text{m}$) a 100 nm spike yields +18%; on
649 the FN 101 background ($TV = 118.4 \mu\text{m}$) the identical spike would yield only
650 +0.17%, below the within-run repeatability. Detectability of a given absolute
651 defect in the full-profile descriptor therefore scales inversely with the background
652 gradient content; on this basis the FN 101 defect-to-background ratio is quantified
653 as roughly 500 times less favourable than in typical smooth-surface applications.
654 Two consequences follow for industrial inspection. First, full-profile BV density
655 is best suited to smooth, finished surfaces — bearing raceways, optical components,
656 precision seals — whose residual amplitudes (tens of nanometres) are comparable
657 to the FN 111 case, and where the synthetic archetypes map onto realistic
658 features (spike $\leftrightarrow$ pit or inclusion edge, scratch $\leftrightarrow$ handling or tooling mark,
659 sinusoid $\leftrightarrow$ chatter or vibration signature). Second, for rougher backgrounds
660 the sliding-window formulation restores local contrast: the certified Flick flat
661 is detected on the FN 101 (Fig. 4) despite the unfavourable full-profile ratio,

precisely because the window localises the comparison. Validation against physical defects of calibrated dimensions on real metallic and ceramic surfaces remains necessary before these scaling arguments can be considered established (Sec. 5.6).

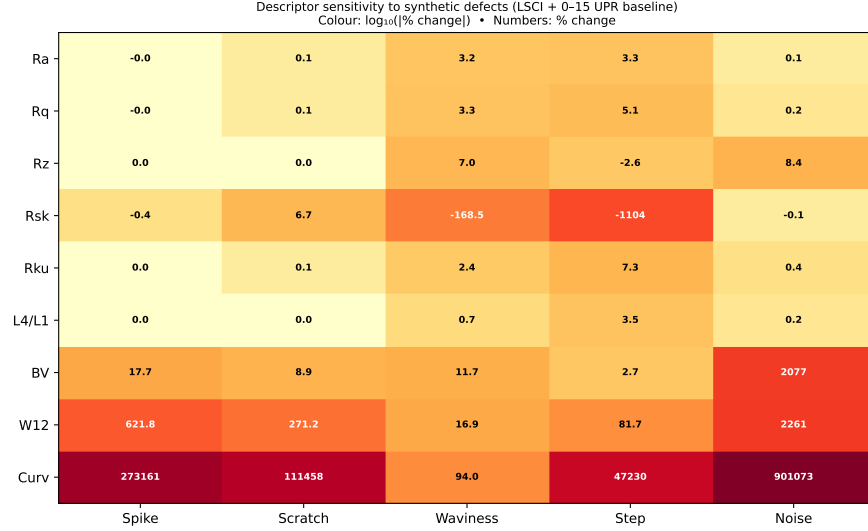


Figure 5: Sensitivity of ISO and gradient-based descriptors to five synthetic defect types injected into the FN 111 residual profile. Percentage change from the unperturbed baseline; bold labels indicate changes exceeding 10%.

Supporting analyses — descriptor correlation matrices, power spectral density comparison, Cohen’s d effect sizes, critical descriptor assessment, and L^p norm convergence — are provided in the Supplementary Materials (Figs. S13–S17). Given the number of descriptors compared (~ 15 across two artefacts), the reported differences should be interpreted as exploratory rather than confirmatory; no formal multiple-comparison correction has been applied.

Practical considerations. A practical suggestion for interferometric profile and roundness metrology is to retain R_a , R_q , R_z , R_{sk} , $RONt$ and $RONq$ as the primary engineering layer compliant with ISO 4287:2019-2, and to consider supplementing them with BV density (in angular units, nm deg^{-1} , Sec. 3.6) as a gradient-sensitive functional-analysis complement. The $W^{1,2}$ gradient semi-

677 norm is strongly correlated with BV density in the present datasets (within the
 678 FN 111: Pearson $r = 0.95$, $n = 5$ sweeps; within the FN 101: $r = 0.93$, $n = 5$).
 679 The pooled $r = 0.94$ (95% CI $[0.72, 0.99]$, $n = 10$) is reported for descriptive pur-
 680 poses only — the sweeps are not independent observations and this pooled corre-
 681 lation should be interpreted with caution. This strong correlation indicates that,
 682 as repeatability metrics across sweeps, BV density and the $W^{1,2}$ may add limited
 683 independent information beyond BV density alone given the small sample. The
 684 seminorm carry largely redundant information, and routine reporting of both is
 685 not warranted. They are strongly correlated but not mathematically equivalent:
 686 BV integrates the first power of the local slope, $TV = \int |p'| ds$, whereas $W^{1,2}$
 687 integrates its square, $\int |p'|^2 ds$, so the two coincide only for profiles whose slope
 688 magnitude is nearly constant and diverge whenever the slope distribution is
 689 uneven. This is exactly what the defect responses show: for the 100 nm
 690 synthetic spike the $W^{1,2}$ seminorm responded with +622% versus +18% for
 691 BV density, because the quadratic weighting amplifies a single steep event far
 692 more strongly than the linear total-variation measure. A practical reading of
 693 the descriptor space in these data is therefore: (i) R_a/R_q (equivalently L^1/L^2)
 694 carry amplitude information; (ii) R_{sk} carries an independent asymmetry axis;
 695 (iii) BV density carries the localised-gradient axis and is recommended as the
 696 primary gradient descriptor; (iv) the $W^{1,2}$ seminorm adds value mainly as a
 697 high-sensitivity alarm for isolated steep features rather than as an independent
 698 information axis; and (v) the L^4/L^1 peakiness ratio provides a supplementary
 699 distribution-shape axis with a direct physical interpretation as the amplification
 700 of dominant profile excursions relative to R_a . These additional descriptors are
 701 computed from the same residual profile without additional hardware or changes
 702 to the EFM pipeline. The cross-instrument validation suggests that gradient-
 703 based descriptors are applicable to any 1D profile, whether from interferometry
 704 or tactile roundness measurement.

705 **Practical value and the known-feature caveat.** It must be acknowledged
 706 that the Flick flat is a certified, deliberately manufactured feature whose presence
 707 and position were known in advance: Fig. 4 is an existence proof under ground-truth

conditions, not a blind detection study. The practical argument for a gradient-sensitive layer is therefore not that it revealed an unknown defect here. It is that it converts what an operator might notice in a visual polar-plot inspection into a quantitative, thresholdable, and automatable indicator computed from data already acquired for ISO reporting — with no operator in the loop, a defined angular position estimate, and a repeatability statement. Whether this indicator reveals defects that routine quality-control reporting would otherwise miss has not been demonstrated; a blind-detection protocol on artefacts with independently characterised defects is outlined in Sec. 5.6 as the decisive next test of practical value.

Planned versus exploratory comparisons. The synthetic-defect responses (Supplementary Table S2, Fig. 5) and the Flick flat detection (Fig. 4) were planned comparisons motivated by the study’s objective of assessing gradient-based descriptor sensitivity. The correlation matrices, power spectral density comparison, Cohen’s d effect sizes, L^p norm convergence analysis, and the cross-descriptor stability comparison (Supplementary Figs. S13–S17) are exploratory and are intended to characterise the descriptor space rather than to test specific hypotheses. This distinction should be borne in mind when interpreting the reported associations. The present study is a proof-of-concept demonstration; generalisability to other artefact types, materials, and measurement instruments remains to be established.

5.4. Limitations

Several limitations should be acknowledged. First, the uncertainty analysis ~~is restricted to~~ combines within-run Type A repeatability from five sweeps ~~in a single continuous rotation,~~ the indicative type-B budget of Sec. 3.8 (including the measured static-session drift bound), and a two-session between-run comparison (Sec. 3.9) that shows agreement within combined uncertainties for identical acquisition parameters; a full multi-session reproducibility campaign with multiple independent setups and thermal cycles remains to be performed. The small $n = 5$ limits statistical power (relative differences below $\sim 30\%$ cannot be re-

solved), and between-run reproducibility (independent setups, thermal cycles, re-centring) has not been assessed. A full GUM-compliant uncertainty budget, incorporating type-B evaluations of laser wavelength stability, refractive-index variations, Abbe error, camera nonlinearity, and form-removal uncertainty, is beyond the scope of this study for the FN 111; the reported expanded uncertainties should be interpreted as lower bounds, and the form-removal systematic (bounded at ≤ 41 nm) is carried outside the quadrature combination.

Second, the validation is restricted to two artefacts from a single manufacturer (JENOPTIK), both of ~ 30 mm diameter;-. The two artefacts do differ substantially in material (Al_2O_3 ceramic versus steel) and in residual amplitude (two orders of magnitude in R_a), which provides some breadth, but generalisability to other sizes, materials, or diameters, materials such as optical glass or tungsten carbide, and other surface finishes has not been tested. Third, the synthetic-defect analysis uses idealised mathematical defects (isolated spike, uniform scratch, pure sinusoid) injected into the FN 111 ceramic profile only; the response to real manufacturing defects with complex morphologies may differ, and the defect-to-background ratio for scaling analysis of Sec. 5.3 shows quantitatively that full-profile detection sensitivity degrades in proportion to background gradient content (the FN 101 is approximately ratio is ~ 500 times smaller, so the detection sensitivity reported here may not generalise to artefacts with substantially larger form deviations less favourable). Fourth, BV density and the $W^{1,2}$ seminorm carry intrinsic sampling-interval dependence requiring conversion to angular units for cross-instrument comparison; the angular-unit convention of Sec. 3.6 standardises reporting, but no inter-laboratory evidence yet exists that the convention transfers across instruments. Fifth, the Flick flat result (Supplementary Fig. S18) is demonstrated on a single artefact with a known, certified macroscopic feature; performance blind-detection performance and performance for subtler, micrometre-scale defects has have not been characterised.

767 5.5. Metrological Implications

768 The results carry several implications for profile and roundness metrology
769 practice. The finding that BV density responds to localised gradients that am-
770 plitude averaging may not capture suggests — subject to further validation —
771 a potential role for gradient-based descriptors in applications where isolated
772 defects are of concern; possible examples include quality control of bearing sur-
773 faces, optical components, or precision seals. Because these descriptors are
774 computed from the same residual profile used for ISO ~~4287~~21920-2 parameters,
775 their adoption does not require changes to existing measurement acquisition
776 protocols.

777 The ISO ~~4287 framework~~21920-2 framework (with ISO 4287 as its predecessor)
778 remains the appropriate baseline for surface texture specification and confor-
779 mity assessment. The gradient-based descriptors discussed here are proposed
780 as optional supplementary indicators, not as replacements for standardised pa-
781 rameters. Their metrological utility would be strengthened by inter-laboratory
782 comparisons, by evaluation on a wider range of artefact types, and by ~~the~~
783 ~~development of agreed procedures for converting sampling-dependent units to~~
784 ~~instrument-independent angular gradient units.~~adoption of the angular-unit reporting
785 convention of Sec. 3.6. Until such steps are taken, BV density and related de-
786 scriptors should be regarded as research-grade tools whose diagnostic value has
787 been observed under controlled laboratory conditions on two specific artefacts.

788 5.6. Future Work

789 The present study suggests several directions for further investigation. (i) A
790 multi-session between-run reproducibility ~~study campaign~~ with independent
791 setups~~and~~, distinct thermal cycles, and physical re-centring ~~would establish~~
792 ~~whether the gradient-based descriptors retain their relative stability under realistic~~
793 ~~laboratory conditions.~~of the artefact would extend the two-session comparison
794 of Sec. 3.9 and would supply the input distributions needed to upgrade the
795 indicative type-B budget of Sec. 3.8 to a complete GUM-compliant evaluation.
796 (ii) Extending the validation to artefacts with different diameters, materials

797 (e.g., ~~glass, optical glass, tungsten~~ carbide), and surface finishes would test the
 798 generalisability of the findings beyond the two ~30 mm JENOPTIK artefacts
 799 studied here. (iii) A systematic characterisation of BV density response to real
 800 manufacturing defects (scratches, pits, inclusions) of ~~controlled dimensions~~ calibrated
 801 dimensions, culminating in a blind-detection protocol in which the analyst does
 802 not know defect presence or position, would bridge the gap between the present
 803 synthetic-defect analysis and industrial inspection ~~scenarios~~ and would provide
 804 the decisive test of practical value. (iv) An inter-laboratory comparison using
 805 a common artefact set and a standardised processing pipeline would provide
 806 the reproducibility data needed to assess whether BV density could eventually
 807 be considered for standardisation. (v) ~~The development of agreed Empirical~~
 808 verification of the angular-unit ~~conventions for sampling dependent gradient~~
 809 ~~descriptors would facilitate cross-instrument comparison and potential inclusion~~
 810 convention of Sec. 3.6 across instruments with different angular resolutions
 811 would support the potential inclusion of gradient descriptors in reference soft-
 812 ware for roundness evaluation. (vi) A systematic study of the speed-accuracy
 813 trade-off (rotation speed, frame rate, fringe contrast) would establish the shortest
 814 acquisition compatible with the reported uncertainty, a prerequisite for industrial
 815 adoption.

816 Data Availability

817 The analysis code, processed results, and all figures are available at [https:](https://github.com/dawidkucharski/banach-profile-metrology)
 818 [//github.com/dawidkucharski/banach-profile-metrology](https://github.com/dawidkucharski/banach-profile-metrology) (release v1.1.0).
 819 The raw interferometric PNG archives (~32 GB), together with the two additional
 820 independent FN 111 sessions used for the between-run comparison of Sec. 3.9
 821 and the static stability recording used for the drift bound in Sec. 3.8 (~7 GB
 822 each), are available from the corresponding author upon reasonable request.

823 References

- 824 [1] L. Zhu, C. Ni, Z. Yang, C. Liu, Investigations of micro-textured surface
 825 generation mechanism and tribological properties in ultrasonic vibration-
 826 assisted milling of Ti-6Al-4V, Precision Engineering 57 (November 2018)
 827 (2019) 229–243. doi:10.1016/j.precisioneng.2019.04.010.
 828 URL <https://doi.org/10.1016/j.precisioneng.2019.04.010https://linkinghub.elsevier.com/retrieve/pii/S0141635918307384>
 829
- 830 [2] R. Leach, Optical Measurement of Surface Topography, Springer Berlin
 831 Heidelberg, Berlin, Heidelberg, 2011. doi:10.1007/978-3-642-12012-1.
 832 URL <http://link.springer.com/10.1007/978-3-642-12012-1>
- 833 [3] D. J. Whitehouse, Handbook of Surface and Nanometrology, 2nd Edition,
 834 CRC Press, Boca Raton, 2010. doi:10.1201/b10415.
- 835 [4] A. Michelson, Light-Waves and their Application to Metrology, Nature
 836 49 (1255) (1893) 56–60. doi:10.1038/049056a0.
 837 URL <https://doi.org/10.1038/049056a0http://10.0.4.14/049056a0http://www.nature.com/articles/049056a0>
 838
- 839 [5] F. A. Jenkins, H. E. White, Fundamentals of Optics, International student
 840 edition, McGraw-Hill, 1976, (accessed 16 August 2026).
 841 URL <https://archive.org/details/fundamentalsop00jenk>
- 842 [6] M. Born, E. Wolf, Principles of Optics: Electromagnetic Theory of
 843 Propagation, Interference and Diffraction of Light, 6th Edition, Pergamon
 844 Press, Oxford, 1980, (accessed 16 August 2026).
 845 URL <https://www.sciencedirect.com/book/monograph/9780080264820/principles-of-optics>
 846
- 847 [7] R. Brodmann, Roughness form and waviness measurement by means of
 848 light-scattering, Precision Engineering 8 (4) (1986) 221–226. doi:10.1016/
 849 0141-6359(86)90063-2.

- [8] Y. Y. Fan, V. M. Huynh, An investigation of light scattering from flat periodic rough surfaces for surface roughness estimation, Precision Engineering 16 (3) (1994) 205–211. doi:10.1016/0141-6359(94)90126-0.
- [9] A. Hertzsch, K. Kröger, H. Truckenbrodt, Microtopographic analysis of turned surfaces by model-based scatterometry, Precision Engineering 26 (3) (2002) 306–313. doi:10.1016/S0141-6359(02)00116-2.
- [10] D. Kucharski, H. Zdunek, A low-cost, simple optical setup for a fast scatterometry surface roughness measurements with nanometric precision, Bulletin of the Polish Academy of Sciences: Technical Sciences 68 (48) (2020) 485–490. doi:10.24425/bpasts.2020.133364.
URL http://journals.pan.pl/Content/116520/PDF/10_485-490_01475_Bpast.No.68-3_30.06.20_K3A_TeX.pdf
- [11] R. Brodmann, T. Gast, G. Thurn, A. Wirtz, O. W. G. Rodenstock, An optical instrument for measuring the surface roughness in production control, CIRP Annals 33 (1) (1984) 403–406. doi:10.1016/S0007-8506(07)61451-6.
URL <https://www.sciencedirect.com/science/article/pii/S0007850607614516>
- [12] R. Benoît, Application des phénomènes d’interférence à des déterminations métrologiques, Journal de Physique Théorique et Appliquée 7 (1) (1898) 57–68. doi:10.1051/jphystap:01898007005700.
URL <http://www.edpsciences.org/10.1051/jphystap:01898007005700%0Apapers3://publication/doi/10.1051/jphystap:01898007005700><http://www.edpsciences.org/10.1051/jphystap:01898007005700>
- [13] G. Xue-fei, X. Sheng-nian, Y. Ye-fei, B. Shan, B. Xing, C. Zhou-jian, C. Ge-rui, D. Peng, G. Tian-shu, G. Wei, H. Shuang-lin, L. Yu-long, L. Ying, L. Zi-ren, S. Ming-xue, S. Bao-san, T. Wen-lin, Y. Pin, X. Peng,

- 878 Z. Yun-long, Z. Hai-peng, L. Yun-kau, Laser Interferometric Gravita-
 879 tional Wave Detection in Space and Structure Formation in the Early
 880 Universe, Chinese Astronomy and Astrophysics 39 (4) (2015) 411–446.
 881 doi:10.1016/j.chinastron.2015.10.001.
 882 URL [http://www.sciencedirect.com/science/article/pii/](http://www.sciencedirect.com/science/article/pii/S0275106215000843)
 883 [S0275106215000843https://linkinghub.elsevier.com/retrieve/](https://linkinghub.elsevier.com/retrieve/pii/S0275106215000843)
 884 [pii/S0275106215000843](https://linkinghub.elsevier.com/retrieve/pii/S0275106215000843)
- 885 [14] P. de Groot, Phase Shifting Interferometry, in: R. K. Leach (Ed.), Optical
 886 Measurement of Surface Topography, Springer Berlin Heidelberg, Berlin,
 887 Heidelberg, 2011, pp. 167–186. doi:10.1007/978-3-642-12012-1_8.
 888 URL http://link.springer.com/10.1007/978-3-642-12012-1_8
- 889 [15] S. Chatterjee, Phase-Shifting Laser Interferometry for Measurement of Sur-
 890 face Form Error, in: P.K.Gupta, R.Khare (Eds.), Springer Proceedings in
 891 Physics, Vol. 160 of Springer Proceedings in Physics, 2015, pp. 209–222.
 892 doi:10.1007/978-81-322-2000-8_10.
 893 URL http://link.springer.com/10.1007/978-81-322-2000-8_10
- 894 [16] P. de Groot, Principles of interference microscopy for the measurement
 895 of surface topography, Advances in Optics and Photonics 7 (2015) 1–65.
 896 doi:10.1364/AOP.7.000001.
- 897 [17] F. Polack, M. Thomasset, S. Brochet, D. Denetiere, Surface shape deter-
 898 mination with a stitching Michelson interferometer and accuracy evalua-
 899 tion, Review of Scientific Instruments 90 (2). doi:10.1063/1.5061930.
- 900 [18] M. Thomasset, M. Idir, F. Polack, M. Bray, J. J. Servant, A new phase-shift
 901 microscope designed for high accuracy stitching interferometry, Nuclear
 902 Instruments and Methods in Physics Research, Section A: Accelerators,
 903 Spectrometers, Detectors and Associated Equipment 710 (2013) 7–12. doi:
 904 10.1016/j.nima.2012.10.123.
- 905 [19] K.-C. Fan, N. Wang, Z.-W. Wang, H. Zhang, Development of a roundness
 906 measuring system for microspheres, Measurement Science and Technology

- 907 25 (6) (2014) 064009. doi:10.1088/0957-0233/25/6/064009.
 908 URL [http://stacks.iop.org/0957-0233/25/i=6/a=064009?key=](http://stacks.iop.org/0957-0233/25/i=6/a=064009?key=crossref.73300f1601df9e917d2e7830f09f45e7)
 909 [crossref.73300f1601df9e917d2e7830f09f45e7](http://stacks.iop.org/0957-0233/25/i=6/a=064009?key=crossref.73300f1601df9e917d2e7830f09f45e7)
- 910 [20] M. Kühnel, V. Ullmann, U. Gerhardt, E. Manske, Automated setup for
 911 non-tactile high-precision measurements of roundness and cylindricity
 912 using two laser interferometers, Measurement Science and Technology
 913 23 (7) (2012) 74016. doi:10.1088/0957-0233/23/7/074016.
 914 URL [http://stacks.iop.org/0957-0233/23/i=7/a=074016?key=](http://stacks.iop.org/0957-0233/23/i=7/a=074016?key=crossref.8429e4ab7d2d23702c0a05dba94b50d5)
 915 [crossref.8429e4ab7d2d23702c0a05dba94b50d5](http://stacks.iop.org/0957-0233/23/i=7/a=074016?key=crossref.8429e4ab7d2d23702c0a05dba94b50d5)[http://stacks.iop.](http://stacks.iop.org/0957-0233/23/i=7/a=074016)
 916 [org/0957-0233/23/i=7/a=074016](http://stacks.iop.org/0957-0233/23/i=7/a=074016)
- 917 [21] M. Takeda, H. Ina, S. Kobayashi, Fourier-transform method of fringe-
 918 pattern analysis for computer-based topography and interferometry, Jour-
 919 nal of the Optical Society of America 72 (1) (1982) 156–160. doi:
 920 10.1364/JOSA.72.000156.
- 921 [22] Q. Kemao, Two-dimensional windowed Fourier transform for fringe pattern
 922 analysis: Principles, applications and implementations, Optics and Lasers
 923 in Engineering 45 (2) (2007) 304–317. doi:10.1016/j.optlaseng.2005.
 924 10.012.
- 925 [23] S. Feng, Q. Chen, G. Gu, T. Tao, L. Zhang, Y. Hu, W. Yin, C. Zuo,
 926 Fringe pattern analysis using deep learning, Advanced Photonics 1 (2)
 927 (2019) 025001. doi:10.1117/1.AP.1.2.025001.
- 928 [24] I. Galaktionov, V. Toporovsky, A Multi-Stage Algorithm of Fringe Map
 929 Reconstruction for Fiber-End Surface Analysis and Non-Phase-Shifting In-
 930 terferometry, Applied System Innovation 9 (2) (2026) 31. doi:10.3390/
 931 asi9020031.
- 932 [25] D. Kucharski, M. Wiczorowski, Radial image processing for phase ex-
 933 traction in rough-surface interferometry, Measurement (2025) 117102doi:
 934 10.1016/j.measurement.2025.117102.

- 935 [26] P. Dumas, J. Fleig, G. Forbes, P. E. Murphy, Extending the range of
 936 interferometry though subaperture stitching, Vol. 10314, 2003, p. 134 –
 937 137. doi:10.1117/12.2284035.
 938 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85016807739&doi=10.1117%2f12.2284035&partnerID=40&md5=8aa04fbb9453cddff6da95df376ffdb6)
 939 [0-85016807739&doi=10.1117%2f12.2284035&partnerID=40&md5=](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85016807739&doi=10.1117%2f12.2284035&partnerID=40&md5=8aa04fbb9453cddff6da95df376ffdb6)
 940 [8aa04fbb9453cddff6da95df376ffdb6](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85016807739&doi=10.1117%2f12.2284035&partnerID=40&md5=8aa04fbb9453cddff6da95df376ffdb6)
- 941 [27] S. Chen, S. Li, Y. Dai, Z. Zheng, Iterative algorithm for subaperture
 942 stitching test with spherical interferometers, Journal of the Optical Society
 943 of America A: Optics and Image Science, and Vision 23 (5) (2006) 1219 –
 944 1226. doi:10.1364/JOSAA.23.001219.
 945 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-33745276550&doi=10.1364%2fJOSAA.23.001219&partnerID=40&md5=4d72b8095c89e81b1ba058a414b7b0c2)
 946 [0-33745276550&doi=10.1364%2fJOSAA.23.001219&partnerID=40&](https://www.scopus.com/inward/record.uri?eid=2-s2.0-33745276550&doi=10.1364%2fJOSAA.23.001219&partnerID=40&md5=4d72b8095c89e81b1ba058a414b7b0c2)
 947 [md5=4d72b8095c89e81b1ba058a414b7b0c2](https://www.scopus.com/inward/record.uri?eid=2-s2.0-33745276550&doi=10.1364%2fJOSAA.23.001219&partnerID=40&md5=4d72b8095c89e81b1ba058a414b7b0c2)
- 948 [28] S. Chen, S. Li, Y. Dai, Z. Zheng, Testing of large optical surfaces
 949 with subaperture stitching, Applied Optics 46 (17) (2007) 3504 – 3509.
 950 doi:10.1364/AO.46.003504.
 951 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-34547536867&doi=10.1364%2fAO.46.003504&partnerID=40&md5=9e100905a834eebb31d582fc8884de99)
 952 [0-34547536867&doi=10.1364%2fAO.46.003504&partnerID=40&md5=](https://www.scopus.com/inward/record.uri?eid=2-s2.0-34547536867&doi=10.1364%2fAO.46.003504&partnerID=40&md5=9e100905a834eebb31d582fc8884de99)
 953 [9e100905a834eebb31d582fc8884de99](https://www.scopus.com/inward/record.uri?eid=2-s2.0-34547536867&doi=10.1364%2fAO.46.003504&partnerID=40&md5=9e100905a834eebb31d582fc8884de99)
- 954 [29] A. S. Iacchetta, J. R. Fienup, D. T. Leisawitz, Rotation and transla-
 955 tion registration of bandlimited interferometric images using a chirp
 956 z-transform, Vol. 9907, 2016. doi:10.1117/12.2232178.
 957 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85006847872&doi=10.1117%2f12.2232178&partnerID=40&md5=25831551d0ae177fef89c421998e31d4)
 958 [0-85006847872&doi=10.1117%2f12.2232178&partnerID=40&md5=](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85006847872&doi=10.1117%2f12.2232178&partnerID=40&md5=25831551d0ae177fef89c421998e31d4)
 959 [25831551d0ae177fef89c421998e31d4](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85006847872&doi=10.1117%2f12.2232178&partnerID=40&md5=25831551d0ae177fef89c421998e31d4)
- 960 [30] J. Burge, S. Ament, J. Beverage, C. Muccianti, C. Zhao, Applications of
 961 computer-generated holograms for measuring x-ray and euv optics, Vol.
 962 13620, 2025. doi:10.1117/12.3067011.
 963 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85006847872&doi=10.1117%2f12.2232178&partnerID=40&md5=25831551d0ae177fef89c421998e31d4)

- 964 0-105024341829&doi=10.1117%2f12.3067011&partnerID=40&md5=
965 92bd5b2fbfd00333a45113efd7a5be87
- 966 [31] H. Quan, H. Xi, W. Fan, Evaluating surface repeatability for in-
967 terferometric measurement: A comparative study, Vol. 9684, 2016.
968 doi:10.1117/12.2243301.
969 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85002262299&doi=10.1117%2f12.2243301&partnerID=40&md5=98a061c8f8cdb6f89be75a953cd88b3f)
970 0-85002262299&doi=10.1117%2f12.2243301&partnerID=40&md5=
971 98a061c8f8cdb6f89be75a953cd88b3f
- 972 [32] L. Zhang, B. Zhang, S. Han, S. Tang, C. Zhuang, Repeatability study on
973 different interference systems, Vol. 10847, 2018. doi:10.1117/12.2505406.
974 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85059070480&doi=10.1117%2f12.2505406&partnerID=40&md5=d2fe726c4d532c3f34340ac03143d343)
975 0-85059070480&doi=10.1117%2f12.2505406&partnerID=40&md5=
976 d2fe726c4d532c3f34340ac03143d343
- 977 [33] A. Pappas, L. Newton, A. Thompson, H. Hooshmand, R. Leach, Un-
978 certainty propagation of field areal surface texture parameters using the
979 metrological characteristics approach, 2023, p. 419 – 422, (accessed 16
980 August 2026).
981 URL [https://www.scopus.com/inward/record.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85165481981&partnerID=40&md5=3c2a4bd283d7a91350fa5adce5f6941b)
982 uri?eid=2-s2.0-85165481981&partnerID=40&md5=
983 3c2a4bd283d7a91350fa5adce5f6941b
- 984 [34] J. Gertheiss, D. Rügamer, B. X. W. Liew, S. Greven, Functional data
985 analysis: An introduction and recent developments, Biometrical Journal
986 66 (7). doi:10.1002/bimj.202300363.
987 URL [https://www.scopus.com/inward/record.uri?eid=2-s2.](https://www.scopus.com/inward/record.uri?eid=2-s2.0-85205152017&doi=10.1002%2fbimj.202300363&partnerID=40&md5=8d9e42e9cd2f23350c0bf0b477169043)
988 0-85205152017&doi=10.1002%2fbimj.202300363&partnerID=40&md5=
989 8d9e42e9cd2f23350c0bf0b477169043
- 990 [35] C. Happ, F. Scheipl, A.-A. Gabriel, S. Greven, A general framework for
991 multivariate functional principal component analysis of amplitude and
992 phase variation, Stat 8 (1). doi:10.1002/sta4.220.

- 993 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
 994 0-85064480543&doi=10.1002%2fst4.220&partnerID=40&md5=
 995 e8d4b76faff42103fe5637961836125d
- 996 [36] G. W. Wolf, Surfaces - topography and topology, Surface Topography:
 997 Metrology and Properties 8 (1). doi:10.1088/2051-672X/ab70e8.
 998 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
 999 0-85084666906&doi=10.1088%2f2051-672X%2fab70e8&partnerID=
 1000 40&md5=006779646e49c4fc727d508bc63eabfa
- 1001 [37] A. Sanner, W. G. Nöhring, L. A. Thimons, T. D. Jacobs, L. Pastewka,
 1002 Scale-dependent roughness parameters for topography analysis, Applied
 1003 Surface Science Advances 7. doi:10.1016/j.apsadv.2021.100190.
 1004 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
 1005 0-85119021594&doi=10.1016%2fj.apsadv.2021.100190&partnerID=
 1006 40&md5=7ad03ad2f796c56f6bec60b5febac199
- 1007 [38] J. Zhao, Z. Wang, L. Zhengminqing, R. Zhu, Fractal simulation of surface
 1008 topography and prediction of its lubrication characteristics, Surface Topog-
 1009 raphy: Metrology and Properties 9 (4). doi:10.1088/2051-672X/ac3f26.
 1010 URL <https://www.scopus.com/inward/record.uri?eid=2-s2.>
 1011 0-85122423109&doi=10.1088%2f2051-672X%2fac3f26&partnerID=
 1012 40&md5=7eb253c5518d5356ead64c22878553ba
- 1013 [39] F. Meijer, D. Kucharski, E. Stachowska, Determination of the phase in
 1014 the center of a circular two-beam interference pattern to determine the
 1015 displacement of a rough surface, Optical Engineering 57 (10) (2018) 1.
 1016 doi:10.1117/1.OE.57.10.104101.
 1017 URL [https://www.spiedigitallibrary.org/journals/
 1018 optical-engineering/volume-57/issue-10/104101/
 1019 Determination-of-the-phase-in-the-center-of-a-circular/10.
 1020 1117/1.OE.57.10.104101.full](https://www.spiedigitallibrary.org/journals/optical-engineering/volume-57/issue-10/104101/Determination-of-the-phase-in-the-center-of-a-circular/10.1117/1.OE.57.10.104101.full)
- 1021 [40] JENOPTIK Industrial Metrology, Unequivocal measurement of form and

1022 positional tolerances using innovative measuring systems, JENOPTIK
1023 Industrial Metrology Germany GmbH, 2018, (accessed 16 August 2026).
1024 URL [https://www.jenoptik.cz/files/products-en/
1025 roundness-measurement/roundness-measurement_10064360_12_2016_
1026 en.pdf](https://www.jenoptik.cz/files/products-en/roundness-measurement/roundness-measurement_10064360_12_2016_en.pdf)

1027 [41] Thorlabs Inc., CPS532 Collimated Laser Diode Module, 532 nm, 4.5 mW,
1028 Round Beam, Ø11 mm Housing, (accessed 16 August 2026) (2019).
1029 URL [https://www.thorlabs.com/thorproduct.cfm?partnumber=
1030 CPS532](https://www.thorlabs.com/thorproduct.cfm?partnumber=CPS532)

1031 [42] FLIR Systems, Software Development Kit, (accessed 16 August 2026)
1032 (2019).
1033 URL [https://www.teledynevisionsolutions.com/support/
1034 support-center/software-firmware-downloads/](https://www.teledynevisionsolutions.com/support/support-center/software-firmware-downloads/)

1035 [43] Newport Corporation, ESP301 Controller GUI Manual, Newport Corpora-
1036 tion, 2017, (accessed 16 August 2026).
1037 URL [https://www.newport.com/medias/sys_master/images/images/
1038 h7e/hfe/9044140982302/ESP301-Controller-GUI-Manual.pdf](https://www.newport.com/medias/sys_master/images/images/h7e/hfe/9044140982302/ESP301-Controller-GUI-Manual.pdf)

1039 [44] R. Ihaka, R. Gentleman, R: A Language for Data Analysis and Graphics,
1040 Journal of Computational and Graphical Statistics 5 (3) (1996) 299–314.
1041 doi:10.1080/10618600.1996.10474713.
1042 URL [http://www.tandfonline.com/doi/abs/10.1080/10618600.1996.
1043 10474713](http://www.tandfonline.com/doi/abs/10.1080/10618600.1996.10474713)

1044 [45] ISO 12181-1:2011, Geometrical product specifications (GPS) — Roundness
1045 — Part 1: Vocabulary and parameters of roundness, Tech. rep., Interna-
1046 tional Organization for Standardization, (accessed 16 August 2026) (2011).
1047 URL <https://www.iso.org/standard/53620.html>

1048 [46] ISO 4291:1985, Methods for the assessment of departure from roundness —
1049 Measurement of variations in radius, Tech. rep., International Organization

1050 for Standardization, withdrawn, replaced by ISO 12181-1:2011. (accessed
1051 16 August 2026) (1985).
1052 URL <https://www.iso.org/standard/10135.html>

1053 [47] ISO 16610-21:2025, Geometrical product specifications (GPS) — Filtration
1054 — Part 21: Linear profile filters: Gaussian filters, Tech. rep., International
1055 Organization for Standardization, (accessed 16 August 2026) (2025).
1056 URL <https://www.iso.org/standard/84786.html>

1057 [48] ISO 21920-2:2021, Geometrical product specifications (GPS) — Surface
1058 texture: Profile — Part 2: Terms, definitions and surface texture param-
1059 eters, Tech. rep., International Organization for Standardization, Geneva,
1060 (accessed 16 August 2026) (2021).
1061 URL <https://www.iso.org/standard/72226.html>

1062 [49] ISO 4287:1997, Geometrical Product Specifications (GPS) — Surface tex-
1063 ture: Profile method — Terms, definitions and surface texture parameters,
1064 Tech. rep., International Organization for Standardization, (accessed 16
1065 August 2026) (1997).
1066 URL <https://www.iso.org/standard/10132.html>

1067 [50] ISO 25178-2:2021, Geometrical Product Specifications (GPS) — Surface
1068 texture: Areal — Part 2: Terms, definitions and surface texture param-
1069 eters, Tech. rep., International Organization for Standardization, (accessed
1070 16 August 2026) (2021).
1071 URL <https://www.iso.org/standard/74591.html>

1072 [51] S. Banach, Théorie des opérations linéaires, Monografie Matematyczne,
1073 Warsaw, 1932, (accessed 16 August 2026).
1074 URL <https://archive.org/details/in.ernet.dli.2015.493033>

1075 [52] Newport Corporation, Precision Motion Control Catalog, Newport Corpo-
1076 ration, 2018, (accessed 16 August 2026).
1077 URL <https://www.newport.com/p/URS100BCC>

1078 [53] JCGM 100:2008, Evaluation of measurement data — Guide to the expres-
1079 sion of uncertainty in measurement (GUM), Tech. rep., Joint Committee
1080 for Guides in Metrology, (accessed 16 August 2026) (2008).
1081 URL [https://www.bipm.org/documents/20126/2071204/JCGM_100_](https://www.bipm.org/documents/20126/2071204/JCGM_100_2008_E.pdf)
1082 [2008_E.pdf](https://www.bipm.org/documents/20126/2071204/JCGM_100_2008_E.pdf)