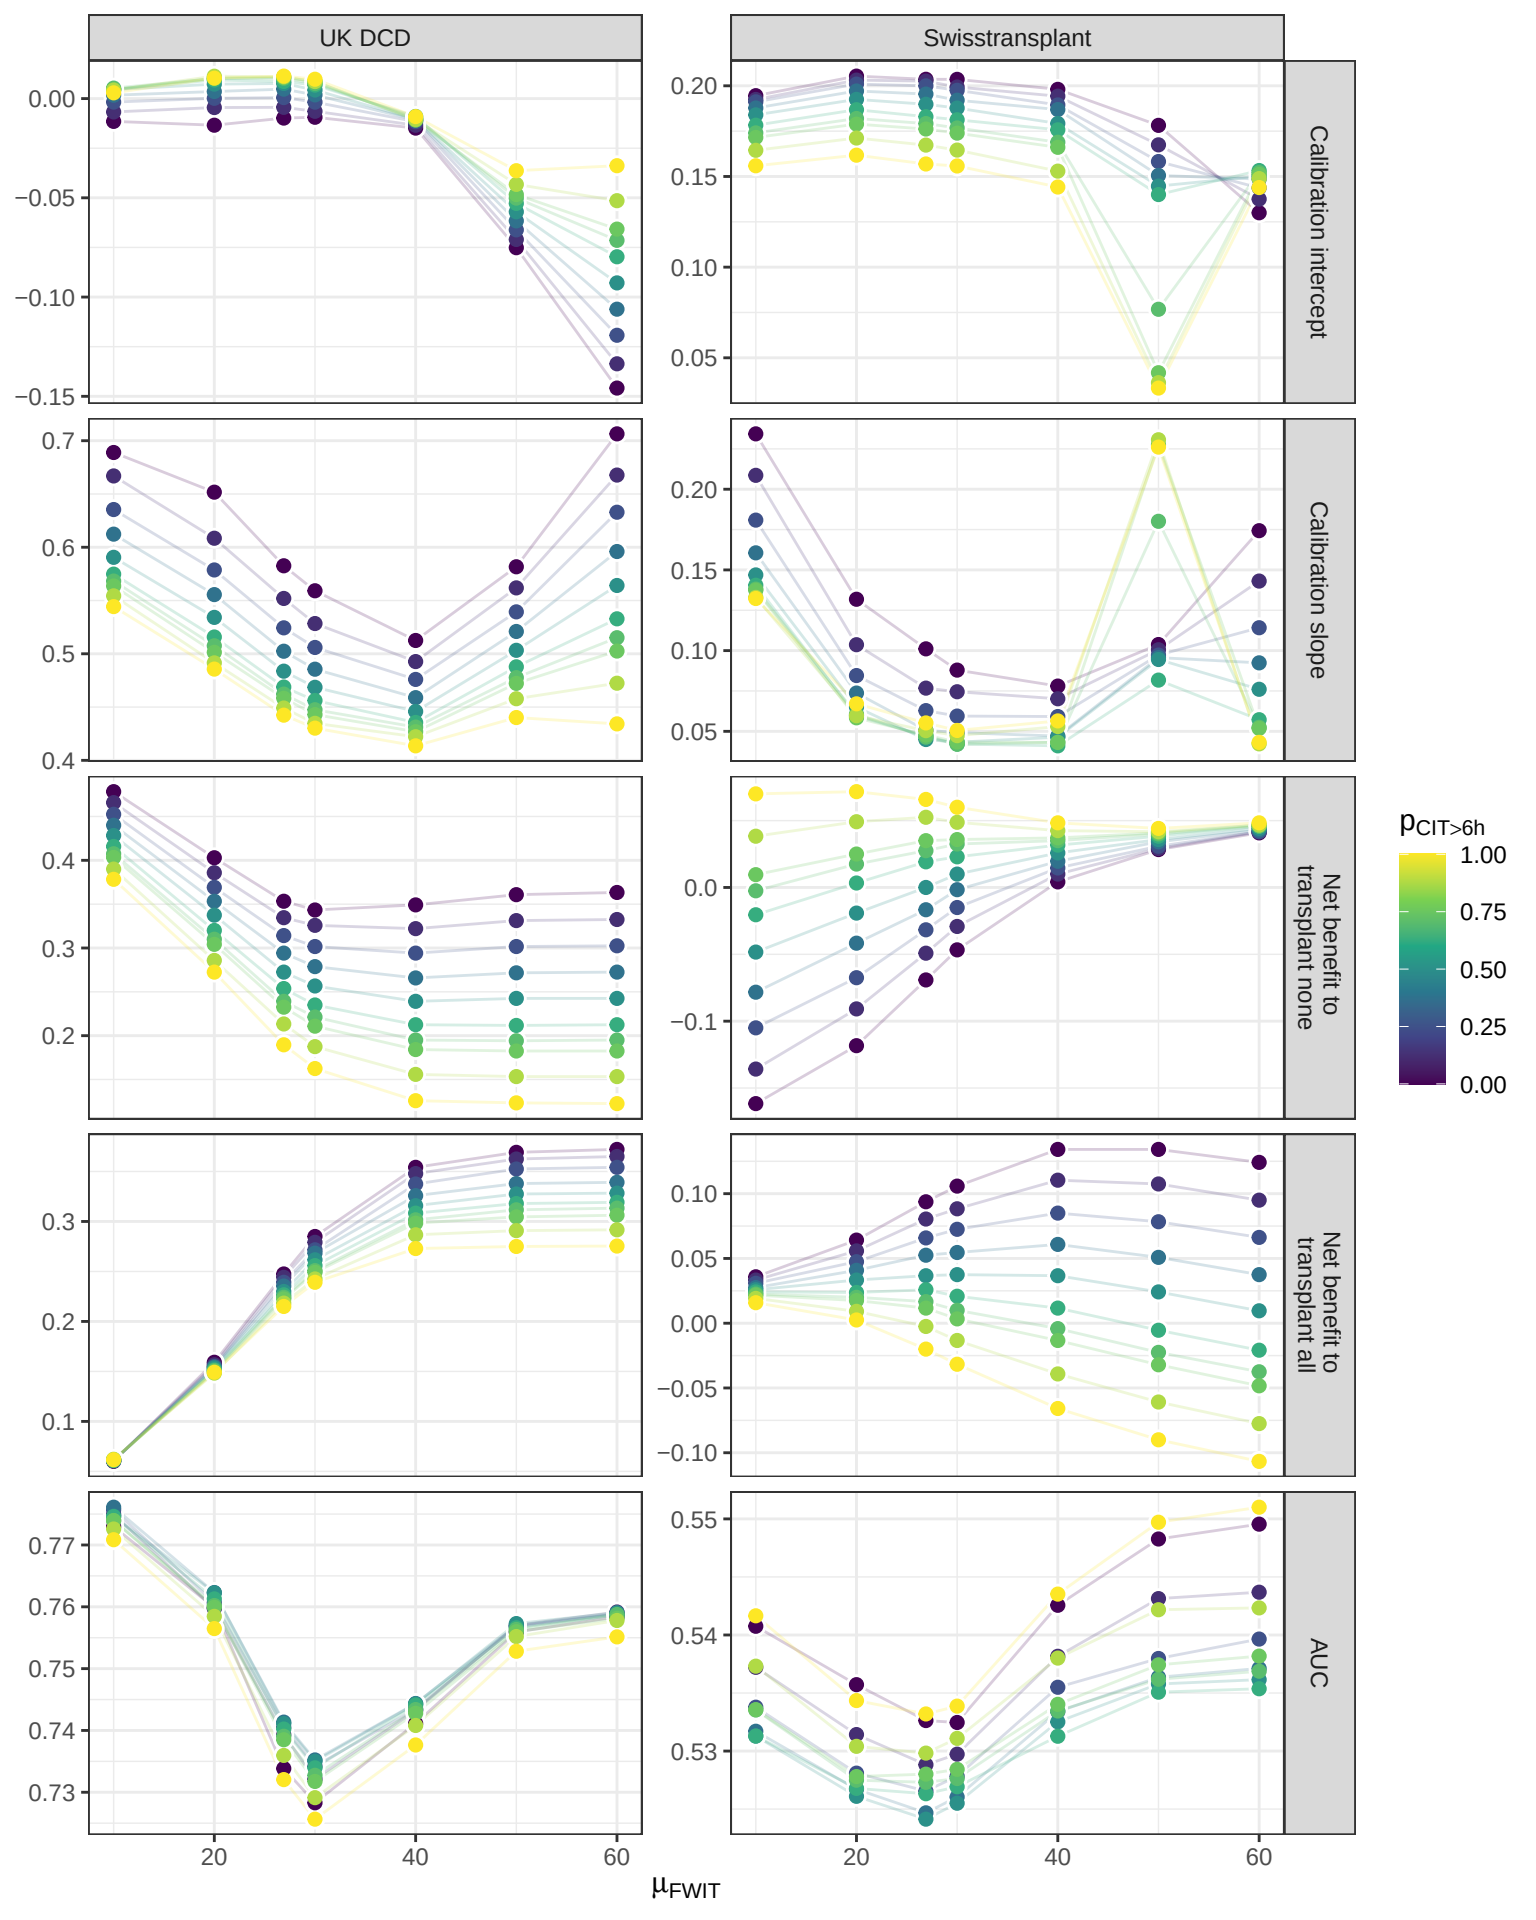

UK DCD
Swisstransplant
Calibration intercept
Calibration slope
Net benefit to transplant none
Net benefit to transplant all
AUC
$p_{CIT>6h}$
1.00
0.75
0.50
0.25
0.00
μ_{FWIT}