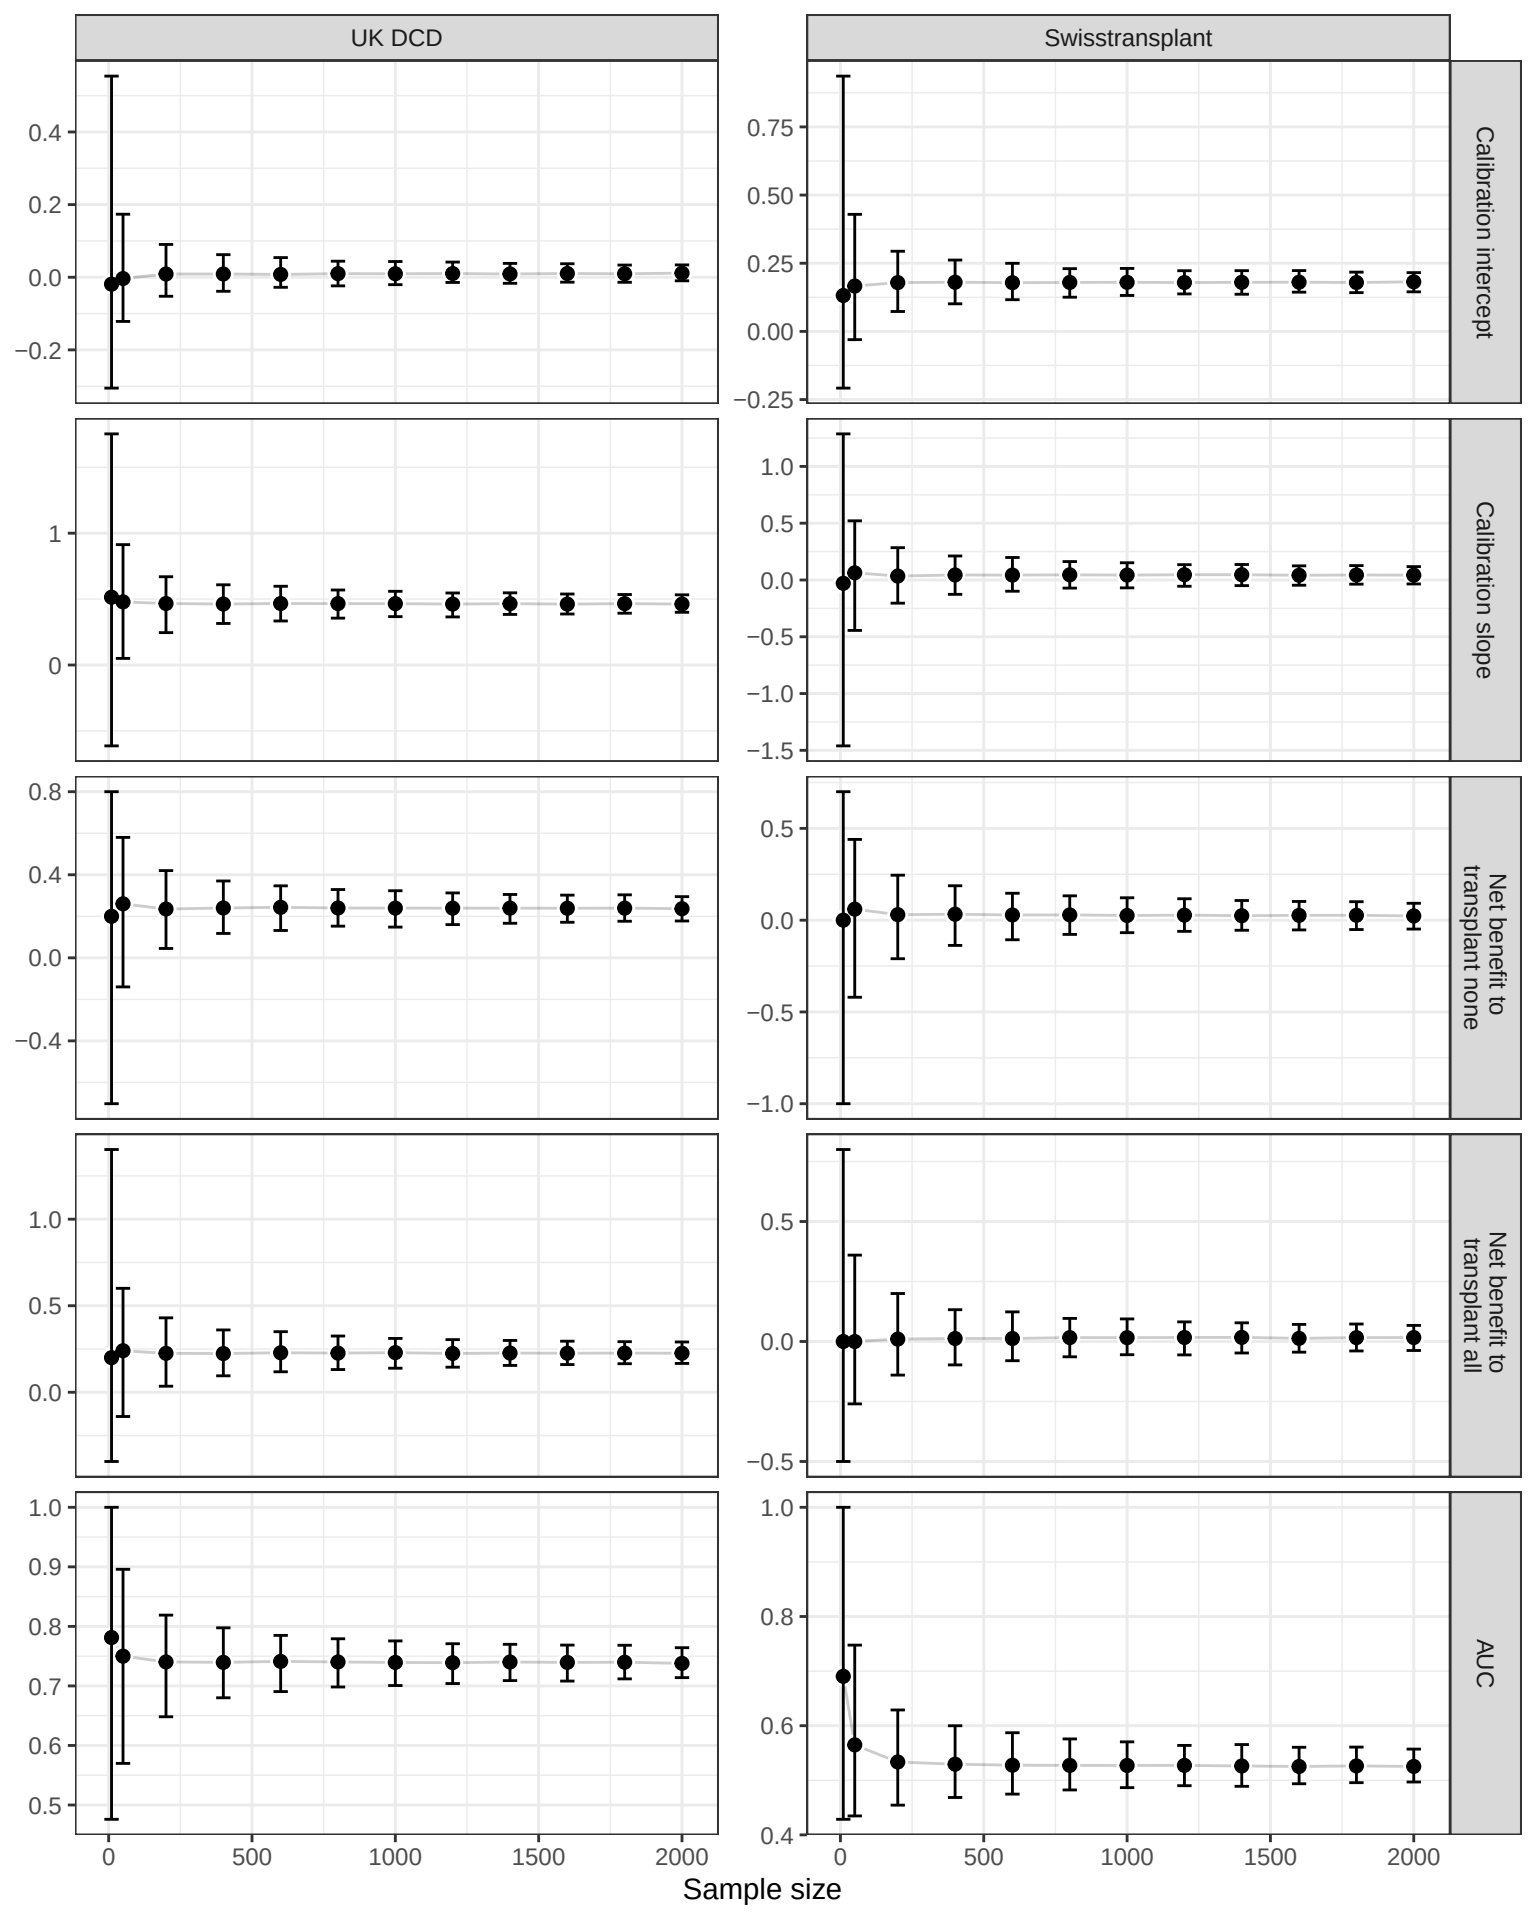
UK DCD
Swisstransplant
Calibration intercept
Calibration slope
Net benefit to transplant none
Net benefit to transplant all
AUC
Sample size