

Rigid-Motion Correction in Head Cone-Beam CT with a 3D Flow-Matching Prior on a Geometry Bridge_by_codex

Sungho Yun
Seungryong Cho

Department of Nuclear and Quantum Engineering,
Korea Advanced Institute of Science and Technology (KAIST), Daejeon 34141, South Korea

Abstract

Blind motion correction in head cone-beam CT (CBCT) requires joint estimation of the image and per-view rigid poses. We propose a 3D flow-matching prior trained on a geometry bridge: FDK reconstructions generated from the same volume as the simulated motion amplitude decreases linearly to zero. The bridge connects the uncorrected reconstruction to its motion-free FDK counterpart, with an analytic velocity target derived from the forward projector’s geometry derivative. At inference, a predictor-corrector loop alternates image updates from the frozen prior, motion fitting with a hash-encoded network, and data-consistency updates. We evaluated the method on simulated projections from 30 held-out CQ500 patients with $10\text{ mm}/10^\circ$ peak-to-peak rigid motion. The final reconstructions achieved 36.66 dB PSNR and 0.978 SSIM, while mean reprojection error decreased from 6.12 to 0.28 mm. Reprojection error was 2.26 mm for learned autofocus and 0.84 mm for JRM-ADM; the proposed reconstructions exceeded JRM-ADM by 7.0 dB and 0.066 SSIM under the same evaluation protocol. Inference took 9.3 minutes per patient on an RTX A6000. Replacing the geometry bridge with a pixel-linear path reduced PSNR by approximately 1.4 dB, supporting the use of a motion-based training path for joint image and motion recovery.

I Introduction

Cone-beam CT is used for head and neck imaging in image-guided radiotherapy, interventional suites and point-of-care settings. Head motion during acquisition violates the static-object assumption of analytic reconstruction, producing streaks and double contours. A six-degree-of-freedom (6-DoF) rigid pose per projection view provides a useful model of skull motion. Recovering these poses from the projections alone is challenging because the image used to estimate the motion is itself corrupted by that motion. The forward model is linear in the volume but nonlinear in the poses, making their joint estimation a non-convex problem.

Autofocus methods estimate motion by optimizing an image-quality measure of the reconstruction. Classical approaches use criteria such as image sharpness [1], while learned approaches predict voxel-wise visual information fidelity (VIF) [2] or a scalar quality score [3]. Image-domain methods instead map corrupted reconstructions directly to corrected images without estimating the acquisition poses [4]. Autofocus provides efficient motion estimation, but the pose search depends on how well its quality metric distinguishes residual motion artifacts from anatomical structure, particularly under severe motion.

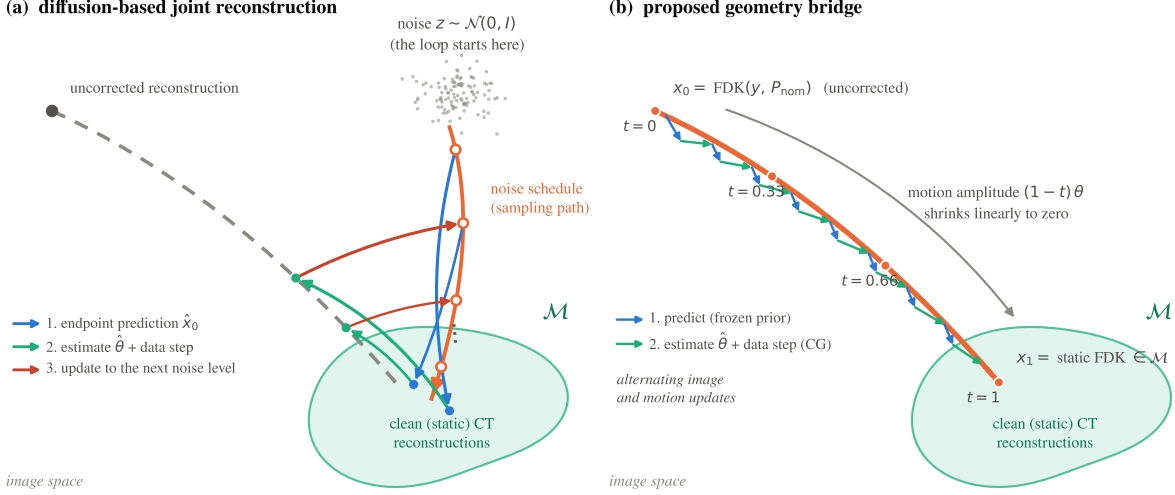


Figure 1: Schematic comparison of training paths and their use in joint reconstruction. (a) A noise-to-clean diffusion prior predicts an image that is combined with motion and data-consistency updates before advancing the sampling schedule. (b) The geometry bridge consists of FDK reconstructions simulated with motion amplitude $(1 - t)\theta$; its tangent dx_t/dt is the training target. The learned velocity guides image updates interleaved with motion fitting and data consistency. The arrows illustrate the update sequence, not measured inference trajectories or projection onto the training bridge.

Generative image priors offer another way to guide joint recovery, building on plug-and-play reconstruction [5] and diffusion-based inverse solvers [6]. JRM-ADM [7] combines a wavelet-domain diffusion prior (W3DM [17]) with weighted-least-squares image updates and B-spline motion estimation. Its prior is trained to recover clean volumes from noisy inputs, and the image and motion updates are incorporated into the diffusion sampling schedule. This training path is defined by noise corruption; it does not explicitly represent the image changes caused by reducing patient motion.

Flow matching [8] allows a velocity field to be learned along a prescribed path between data distributions [9, 10, 11]. We define such a path using FDK reconstructions of a volume simulated with progressively reduced motion. This geometry bridge connects an uncorrected reconstruction to the corresponding motion-free FDK image. Its tangent provides a supervised target for image updates, which we use before each motion fit in a predictor-corrector loop. Fig. 1 illustrates the distinction between this training path and a noise-to-clean path.

The method has two main components: a 3D flow-matching prior on the geometry bridge, with an analytic velocity target derived from the forward projector (Sec. II.B), and a predictor-corrector algorithm combining this prior with hash-encoded motion estimation and conjugate-gradient data consistency (Sec. II.C). We evaluate image and motion recovery on 30 held-out patients against learned autofocus and JRM-ADM, and compare the geometry bridge with a pixel-linear path under the same training and inference settings (Sec. IV.B).¹

¹An earlier version of this work, without the comparative evaluation, was submitted to SPIE Medical Imaging 2027.

II Methods

A Problem formulation

Let x denote an attenuation volume and y the log-transformed projections acquired over V views on a nominal circular orbit P_{nom} . The rigid pose at view v is $\theta_v \in \mathbb{R}^6$, comprising a translation and an axis-angle rotation. Writing its transform as $T(\theta_v)$, the acquisition geometry is $P(\theta)[v] = P_{\text{nom}}[v]T(\theta_v)$ and the forward model is $y = A_{P(\theta)}x$. We abbreviate this projector as A_θ and write $\text{FDK}(\theta) = \text{FDK}(y, P(\theta))$ for analytic reconstruction at a given trajectory.

The image and motion updates are guided by the data-fidelity term


$$\mathcal{D}(x, \theta) = \frac{1}{2} \|A_\theta x - y\|_2^2. \quad (1)$$

We combine these updates with a learned flow velocity and total-variation (TV) denoising. The learned prior enters through its image update, without specifying an explicit regularization functional. The resulting iteration is described in Sec. II.C.

A common change of the object coordinate frame and acquisition geometry leaves the projections unchanged. This SE(3) gauge ambiguity makes the absolute global pose unobservable, so image and trajectory errors are evaluated after removing that offset (Sec. III.B).

B Flow-matching prior on the geometry bridge

(a) Training: a flow-matching prior on the geometry bridge

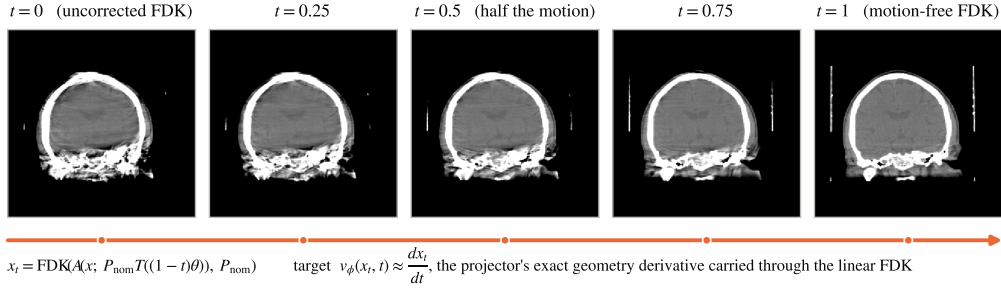

(b) Inference: blind predictor-corrector loop along the bridge

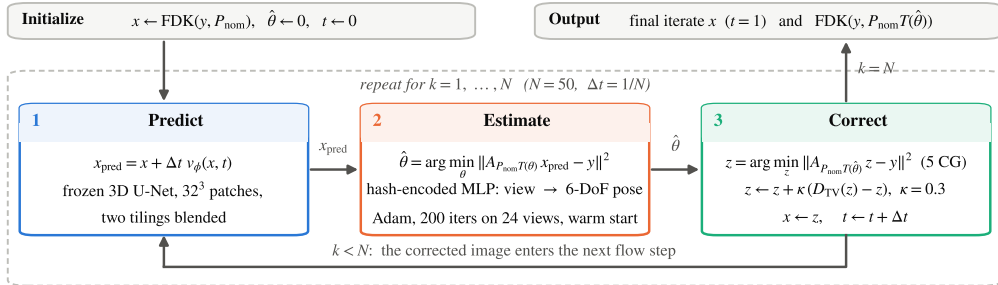


Figure 2: Training and inference. (a) FDK reconstructions of one volume re-simulated with motion amplitude $(1-t)\theta$. The training target is the path tangent, obtained by applying the fixed-geometry FDK operator to the projection derivative. (b) At inference, the frozen prior predicts an image, the motion estimator fits the measured projections to that prediction, and data consistency updates the image at the estimated geometry.

Flow matching learns a velocity field $v_\phi(x, t)$ by regression to the tangent of a prescribed path. For a training volume x and simulated motion θ , we define the geometry bridge by reducing the motion

amplitude and reconstructing each simulated scan at the nominal geometry:

$$P_t = P_{\text{nom}}T((1-t)\theta), \quad y_t = A_{P_t}x, \quad x_t = \text{FDK}(y_t, P_{\text{nom}}). \quad (2)$$

Scaling the translation and axis-angle rotation by $(1-t)$ reduces both to zero as t increases from 0 to 1. The initial state is the uncorrected reconstruction, $x_0 = \text{FDK}(y, P_{\text{nom}})$, for the simulated scan $y = A_{P(\theta)}x$. The endpoint $x_1 = \text{FDK}(A_{P_{\text{nom}}}x, P_{\text{nom}})$ is its motion-free FDK counterpart. Intermediate states are FDK reconstructions simulated at decreasing motion amplitudes (Fig. 2(a)).

Since FDK is linear in its projection input and its reconstruction geometry is fixed, the path tangent is

$$\dot{x}_t = \text{FDK}(\dot{y}_t, P_{\text{nom}}), \quad \dot{y}_t = D_P(A_P x)|_{P=P_t}[\dot{P}_t], \quad \dot{P}_t = P_{\text{nom}} \frac{d}{dt}T((1-t)\theta). \quad (3)$$

Here $D_P(A_P x)[\dot{P}_t]$ is the directional geometry derivative of the forward projector. The rigid-transform derivative is analytic under the translation and axis-angle parameterization, and the projector derivative is evaluated for the same discrete operator used to generate the bridge. We train with the squared loss $\|v_\phi(x_t, t) - \dot{x}_t\|_2^2$, sampling $t \sim \mathcal{U}[0, 1]$.

The velocity field is represented by a 3D U-Net operating on 32^3 patches. Following [12], each patch receives four additional channels: the whole current volume downsampled to 32^3 , and three maps of the patch voxels’ absolute z , y and x coordinates. These channels supply global anatomy and spatial context while retaining the memory cost of patch-wise inference.

C Predictor-corrector inference loop

Inference starts from the uncorrected reconstruction and zero motion. Each of $N = 50$ iterations applies a prior prediction, refits the motion to that prediction, and updates the image using the measured projections (Algorithm 1). The flow time sets the input to the prior; the motion and data updates use the fixed measurement y .

Algorithm 1 Blind rigid-motion correction with the geometry-bridge prior

Require: projections y , nominal geometry P_{nom} , frozen prior v_ϕ , number of steps N

- 1: $x \leftarrow \text{FDK}(y, P_{\text{nom}})$, $\hat{\theta} \leftarrow 0$, $\Delta t \leftarrow 1/N$
 - 2: **for** $k = 0, \dots, N-1$ **do**
 - 3: $t \leftarrow k/N$, $x_{\text{pred}} \leftarrow x + \Delta t v_\phi(x, t)$
 - 4: $\hat{\theta} \leftarrow \text{FitMotion}(x_{\text{pred}}, y; \hat{\theta})$ ▷ warm-started Adam
 - 5: $z \leftarrow \text{CG}_5(A_{\hat{\theta}}, y; z_0 = x_{\text{pred}})$ ▷ five data-update iterations
 - 6: $x \leftarrow z + \kappa(D_{\text{TV}}(z) - z)$ ▷ relaxed TV update
 - 7: **end for**
 - 8: **return** final iterate $x_{\text{final}} = x$ and $\text{FDK}(\hat{\theta})$
-

Predict. The frozen prior takes one Euler step, $x_{\text{pred}} = x + \Delta t v_\phi(x, t)$. Patch predictions are blended over two tilings of the volume.

Estimate. The motion estimator fits the predicted image to the projections by reducing $\|A_\theta x_{\text{pred}} - y\|_2^2$. A multiresolution hash encoding [13] maps the normalized view index to features, and an MLP outputs the 6-DoF pose. We optimize the encoder and MLP with Adam, using the projector’s geometry gradient and retaining the optimizer state between flow steps. No explicit trajectory smoothness penalty is used. Fitting the motion after the prior update allows the estimator to use the current image correction.

Correct. At the updated trajectory $\hat{\theta}$, five conjugate-gradient (CG) iterations reduce the projection residual, initialized at x_{pred} . The resulting image z receives a relaxed TV update, $x = z + \kappa(D_{\text{TV}}(z) - z)$, where D_{TV} denotes TV denoising. This image becomes the input to the next prior prediction. The finite CG and motion updates are not exact minimizations, and the corrected iterates need not lie on the training bridge.

The algorithm returns the final iterate x_{final} and FDK($\hat{\theta}$). The former is the reconstructed image after joint refinement; the latter evaluates the estimated poses through analytic reconstruction. Although FDK applies no learned image update, its poses were estimated with the aid of the prior.

D Implementation details

The U-Net has base width 32, channel multipliers (1, 2, 4), two residual blocks per level, and a time embedding. It has 9.9M parameters and five input channels. We trained it for 500k iterations using AdamW, a cosine learning-rate schedule from 10^{-4} to 10^{-6} , EMA 0.999, fp16, and 64 patches per batch.

Projection and backprojection use LEAP [14]. We implement the geometry derivative of its forward operator for both the bridge target and motion estimation. At each inference step, the motion estimator runs 200 Adam iterations with 24 randomly sampled views per iteration. It uses half volume resolution until $t = 0.5$ and full resolution thereafter. The data update uses five CG iterations, followed by five TV iterations with step size 0.015 and relaxation weight $\kappa = 0.3$. Source code is available at https://github.com/dbstjstod1/Flow_matching_motion_3D.

III Experiments

A Data and simulation setup

We use the CQ500 head CT collection [15], selecting one thin-slice series per patient and removing slice-count outliers following [2]. Of the 343 retained patients, 150 are assigned to training, 50 to validation and 143 to the test split. Reconstructions use a 256^3 grid with 1 mm voxels.

Projections are simulated as noiseless line integrals on a finer 612^3 grid with 0.42 mm voxels to reduce dependence on the reconstruction discretization. The head-CBCT geometry follows [2]: source-isocenter distance 785 mm, source-detector distance 1200 mm, a 700×500 detector with 0.64 mm pixel pitch, and 360 views over a full rotation. Photon noise, scatter and beam hardening are not modeled.

For each motion component, a zero-centered Akima spline [16] is drawn through 10 random nodes. Training samples per-component amplitudes up to 15 mm / 20° ; evaluation uses one fixed 10 mm / 10° pattern per patient. All amplitudes are peak-to-peak. The evaluation uses the same $[-5, 5]$ mm and degree control-point range as [7], with a different spline interpolant, and twice the motion amplitude reported in the evaluation of [2].

B Evaluation protocol

We evaluate 30 patients from the held-out test split, following the cohort size of [2]. Each method receives the same patient, motion realization and sinogram, giving paired comparisons. Before computing PSNR and SSIM, reconstructed volumes are rigidly aligned to the ground truth to account for the global pose ambiguity. Both metrics are evaluated within the measured field of view for all methods.

Motion accuracy is assessed by reprojection error (RPE) [2], the mean detector displacement induced by pose error over a set of points in the head. Trajectories are placed in a zero-mean gauge before comparison. We also report the mean absolute error of each motion component over views and patients, in millimeters for translation and degrees for rotation. These component-wise errors complement RPE, which combines the six pose components into a detector-plane displacement. Analytic reconstructions at the estimated poses provide an additional image-domain assessment. Reported p -values use paired two-sided Wilcoxon signed-rank tests.

C Comparison methods

Learned autofocus [2]. Thies et al. estimate motion by maximizing a learned image-quality metric. A network predicts a voxel-wise VIF map from the reconstruction, and gradient descent adjusts the spline control points through a differentiable backprojector. The method returns an analytic reconstruction at the estimated poses and uses no projection-domain data-fidelity term. We use the authors’ released implementation and reconstruction operator, with the quality network retrained on our 150 training patients.

JRM-ADM [7]. JRM-ADM combines a Haar-wavelet diffusion prior (W3DM [17]) with joint image and motion updates. At each sampling step, the prior predicts a clean volume; weighted-least-squares projection fitting then updates the image and the 6-DoF motion, parameterized by cubic B-spline control points. We use the authors’ released sampler and optimizers, with the prior retrained on our 150 training patients under their noise schedule. For our full-view protocol, the reconstruction grid is extended to 224^3 and the prior weight is rescaled to preserve the data-to-prior balance. The reconstructed volume is placed in the evaluation frame and the poses are converted to our geometry convention for scoring. This evaluates the method under our 360-view protocol, rather than reproducing its published sparse-view experiment.

Bridge ablation (pixel-linear bridge). We train a second prior on the pixel-linear path $x_t = (1 - t)x_0 + tx_1$, with target velocity $x_1 - x_0$. The endpoints, U-Net, conditioning channels, time sampling, 500k training iterations and inference loop are unchanged. This comparison tests the geometry-based path and its tangent against linear interpolation under a fixed training and inference configuration.

IV Results

A Performance of the proposed method

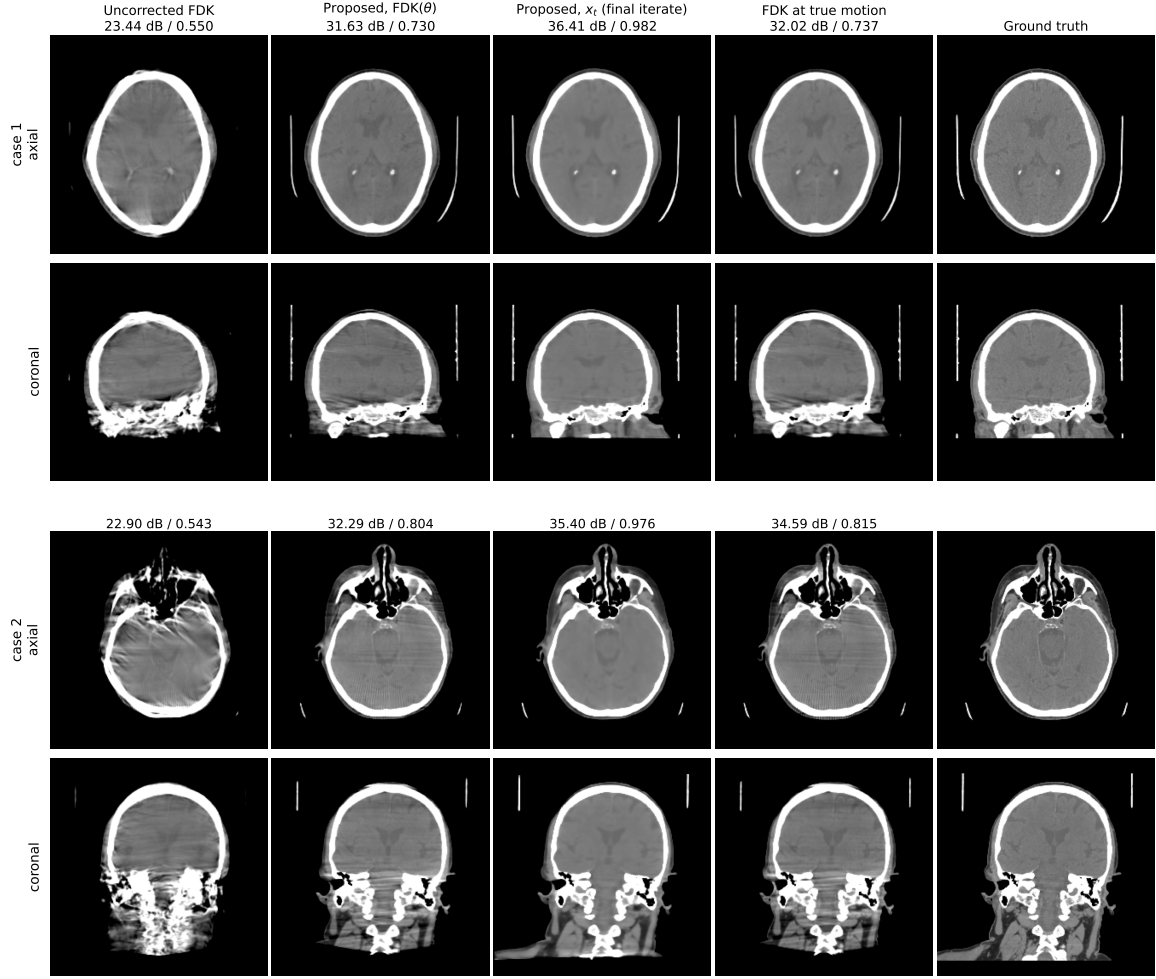


Figure 3: Two representative test patients at 10 mm / 10° motion, brain window (level 40 / width 420 HU); volumes are rigidly aligned to the ground truth before display, and labels give PSNR / SSIM against the ground-truth volume. The fourth column is the FDK of the same scan at the true motion.

Table 1: Performance of the proposed method on 30 held-out CQ500 patients with Akima motion at 10 mm / 10° peak-to-peak. PSNR and SSIM are computed against the ground-truth volume after rigid alignment, within the measured field of view; RPE is the reprojection error of [2] with the mean pose offset removed (mean $\pm$ standard deviation).

Output	PSNR (dB)	SSIM	RPE (mm)
Uncorrected FDK	23.29 $\pm$ 0.93	0.546 $\pm$ 0.035	6.12 $\pm$ 0.66
FDK($\hat{\theta}$)	31.80 $\pm$ 0.76	0.753 $\pm$ 0.032	0.28 $\pm$ 0.09
x_{final} (final iterate)	36.66 $\pm$ 1.58	0.978 $\pm$ 0.008	0.28 $\pm$ 0.09

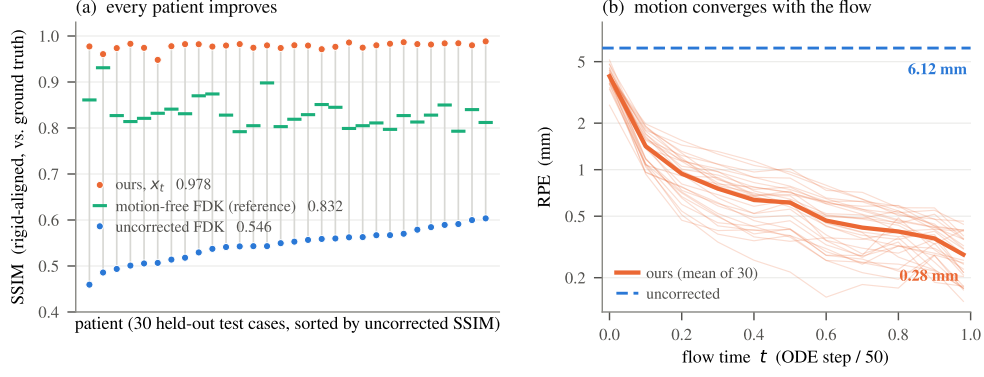


Figure 4: Cohort results over 30 held-out patients. (a) Per-patient SSIM; grey stems join each patient’s uncorrected and corrected score. (b) Reprojection error against flow time (thin: individual patients).

The final iterate achieved 36.66 dB PSNR and 0.978 SSIM, compared with 23.29 dB and 0.546 for the uncorrected FDK (Table 1). Image quality improved in all 30 patients (Fig. 4(a)), and mean RPE decreased from 6.12 to 0.28 mm over the iteration (Fig. 4(b)). Inference took 9.3 minutes per patient on one RTX A6000 GPU (Sec. IV.C).

The analytic reconstruction at the estimated poses reached 31.80 dB and 0.753 SSIM. In the displayed cases, it resembles FDK at the true motion, with residual artifacts in both analytic images (Fig. 3). The final iterate improves on $\text{FDK}(\hat{\theta})$ by 4.9 dB and 0.225 SSIM. It also exceeds the motion-free FDK reference, obtained from a separately simulated static acquisition at the nominal geometry (33.11 dB and 0.832 SSIM), by 3.5 dB and 0.146 SSIM. This gain shows the benefit of iterative reconstruction beyond analytic motion compensation.

B Comparison with other methods

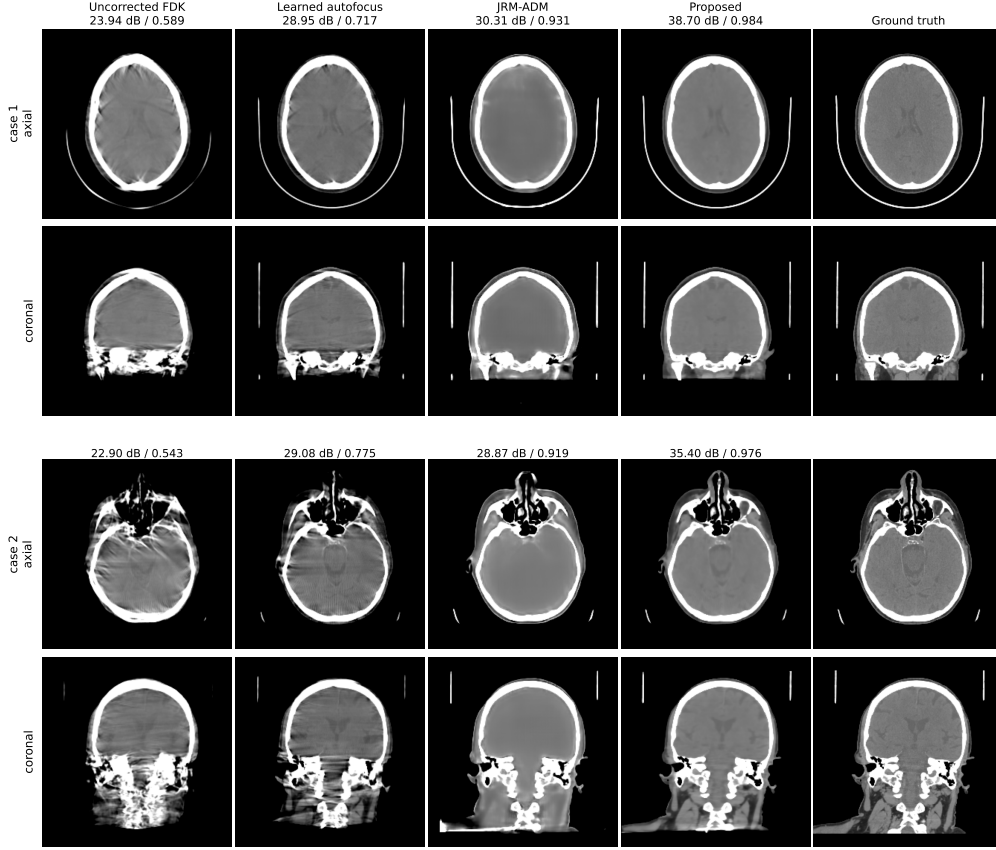


Figure 5: Qualitative comparison on two representative test patients, axial and coronal slices in the brain window; the axial slice of the second case lies at the skull-base level. All volumes are rigidly aligned to the ground truth before slicing, and labels give PSNR / SSIM against the ground truth.

Table 2: Comparison with other methods on the same 30 patients, under the conventions of Table 1. All learned components were retrained on the same 150 training patients and evaluated on identical (patient, motion, sinogram) triples. The pixel-linear row is the bridge ablation discussed at the end of this section.

Method	PSNR (dB)	SSIM	RPE (mm)
Learned autofocus [2]	29.22 ± 1.11	0.727 ± 0.032	2.26 ± 0.52
JRM-ADM [7]	29.64 ± 2.64	0.912 ± 0.038	0.84 ± 0.55
Proposed, FDK($\hat{\theta}$)	31.80 ± 0.76	0.753 ± 0.032	0.28 ± 0.09
Proposed, pixel-linear bridge (ablation)	35.29 ± 2.28	0.966 ± 0.015	0.42 ± 0.17
Proposed, x_{final} (final iterate)	36.66 ± 1.58	0.978 ± 0.008	0.28 ± 0.09

The proposed method reduced RPE relative to learned autofocus in all 30 patients, from a cohort mean of 2.26 to 0.28 mm ($p = 1.7 \times 10^{-6}$; Table 2). Its analytic output also exceeded the autofocus reconstruction: PSNR was higher by 2.6 dB on average and in all 30 patients, while SSIM was higher by 0.026 on average and in 23 patients ($p = 1.5 \times 10^{-4}$ for SSIM). The final iterate exceeded the autofocus output in both image metrics for all patients. In Fig. 5, autofocus reduces the motion artifacts but leaves visible streaks, particularly in the coronal slices.

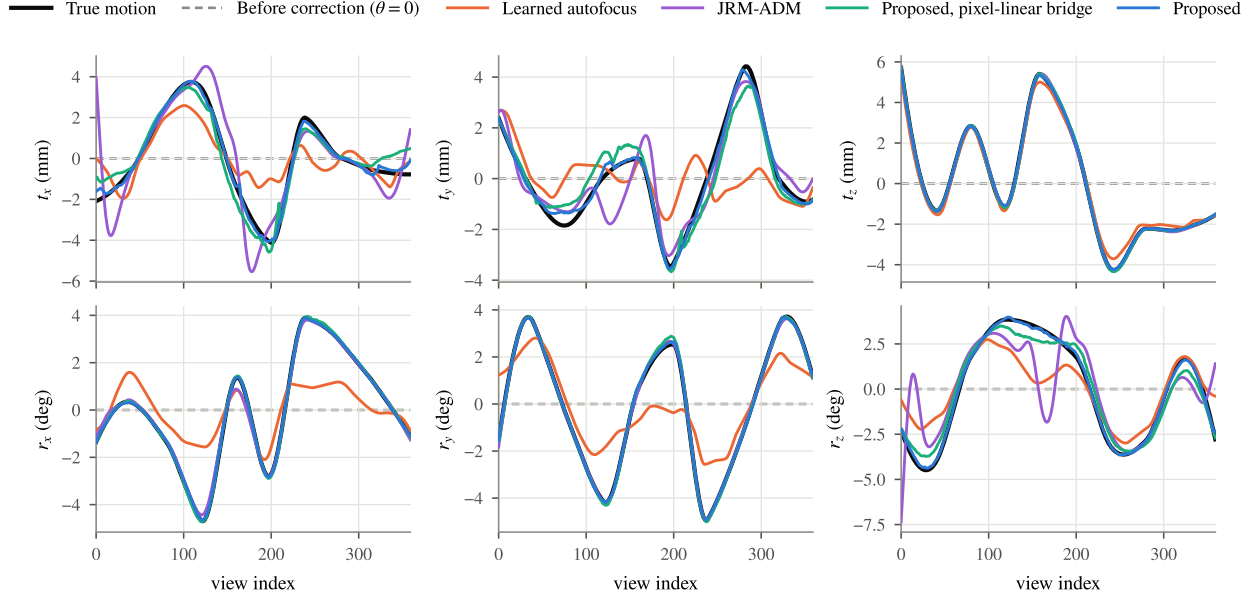


Figure 6: Recovered motion of one test patient (the first case of Fig. 5). Each panel shows one degree of freedom against the view index: the true trajectory, the state before correction ($\theta = 0$), and the trajectory recovered by each method, all on the zero-mean gauge. Translations in mm, rotations in degrees.

Table 3: Per-DoF mean absolute error of the recovered motion over the 30 patients, on the zero-mean gauge. Translations in mm, rotations in degrees. Bold values denote column minima at the reported precision.

Method	t_x	t_y	t_z	r_x	r_y	r_z
Uncorrected	1.93	2.08	1.95	2.01	1.90	2.17
Learned autofocus [2]	1.30	1.33	0.36	0.95	0.98	1.09
JRM-ADM [7]	2.17	1.97	0.06	0.09	0.07	0.68
Proposed, pixel-linear bridge (ablation)	0.71	0.69	0.04	0.04	0.05	0.40
Proposed	0.79	0.78	0.03	0.04	0.04	0.23

The component-wise errors reveal differences that are less apparent in RPE alone (Table 3). The proposed method reduced translation MAE to at most 0.79 mm and rotation MAE to at most 0.23° . Its largest residual errors were in the in-plane translations and gantry-axis rotation. The pixel-linear prior had slightly lower in-plane translation errors, while the geometry bridge had lower gantry-axis rotation error (0.23° versus 0.40°). Fig. 6 shows these trajectories for one patient.

JRM-ADM recovered axial translation and out-of-plane rotations with low error, but its in-plane translation MAEs were 2.17 and 1.97 mm despite an RPE of 0.84 mm. This discrepancy is consistent with drift along directions to which detector-plane displacement is less sensitive. RPE and component-wise pose errors therefore provide complementary assessments of motion recovery.

JRM-ADM’s final reconstruction achieved 29.64 dB and 0.912 SSIM, compared with 36.66 dB and 0.978 for the proposed method. The PSNR gain was present in all 30 patients ($p = 1.9 \times 10^{-9}$). FDK at the JRM-ADM poses reached 29.45 dB and 0.715 SSIM; the proposed analytic output had higher PSNR in 28 patients, with a mean gain of 2.3 dB ($p = 1.6 \times 10^{-7}$). The displayed JRM-ADM reconstructions suppress much of the motion artifact but show more smoothing of soft-tissue contrast than the proposed output (Fig. 5).

With the pixel-linear bridge, final PSNR and SSIM decreased to 35.29 dB and 0.966, and RPE

increased to 0.42 mm (Table 2). The geometry bridge improved PSNR by approximately 1.4 dB and SSIM by 0.012 under the same training and inference settings. This ablation supports the choice of a path defined by simulated motion reduction, while the component-wise results show that the improvement is not uniform across all pose parameters.

C Computational cost

Table 4: Computational cost. Proposed and JRM-ADM runtimes were measured on an RTX A6000 under the 360-view protocol; the autofocus runtime is reported by its authors. Network evaluations count complete prior or quality evaluations, including patch-wise processing for the proposed method. Operator counts are approximate full-view equivalents: an update using 24 views contributes 24/360. Different resolutions and operators give these updates different computational costs.

Method	Network evaluations	Full-view equivalents	Time
Learned autofocus [2]	100	~ 100	< 2 min (reported)
JRM-ADM [7]	100	$\sim 1,600$	4.6 h
Proposed	50	~ 900	9.3 min

The proposed method took 9.3 minutes per patient, with approximately 80% of the runtime spent in motion estimation. Its 10,000 Adam iterations use 24 views each, amounting to roughly 670 full-view equivalents; the 250 CG iterations add another 250. Half-resolution motion fitting during the first half of inference further reduces the cost. The learned autofocus method requires fewer updates and has a published runtime below two minutes (Table 4).

JRM-ADM took 4.6 hours per patient in this implementation. Its 100 sampling steps use 10–15 image updates and 5–10 motion updates per step, each over all 360 views, for approximately 1,600 full-view equivalents. This count is less than twice that of the proposed method, so update counts alone do not explain the runtime difference. The comparison also includes different projector implementations, resolutions and solver costs. In particular, the 360-view protocol increases the work per data update relative to JRM-ADM’s sparse-view setting; the measured runtime difference should be interpreted within this protocol.

V Discussion

The geometry bridge gives the prior a training target tied to a specified reduction in motion. Its advantage over the pixel-linear path, with architecture and inference held fixed, supports using the simulated acquisition model to define the training path. The learned velocity can then guide image updates before motion fitting. The inference iterates also include data-consistency and TV updates, however, so they are not required to follow the prescribed training path exactly.

The two outputs distinguish image reconstruction from evaluation of the recovered poses. FDK at the estimated poses permits comparison through an analytic reconstruction, while the final iterate includes the effects of joint image refinement. The gain over motion-free FDK shows that reconstruction quality can improve beyond that analytic reference. It does not determine how much residual motion still limits the iterative result. Likewise, the comparison with JRM-ADM establishes a difference between complete methods under a common evaluation protocol, without attributing that difference to a single component.

The evidence is limited to noiseless simulated projections, one rigid-motion realization per test patient, and the specified acquisition geometry. Photon noise, scatter, beam hardening and genuine

patient motion require evaluation on measured data. The rigid model is appropriate for the skull but does not describe independent mandibular or neck motion. The baseline comparisons also differ from their published evaluation settings: autofocus is tested at a larger motion amplitude, and JRM-ADM is applied to full-view data. Finally, the 9.3-minute runtime remains longer than the reported autofocus runtime. Reducing the cost of motion fitting is the main opportunity for acceleration in the current implementation.

VI Conclusion

We presented a 3D flow-matching prior trained on FDK reconstructions with progressively reduced motion and integrated it into joint image and pose estimation. On simulated scans from 30 held-out patients, the method achieved 36.66 dB PSNR, 0.978 SSIM and 0.28 mm reprojection error, improving image quality and motion accuracy relative to learned autofocus and JRM-ADM under the tested protocol. The pixel-linear ablation supports the geometry bridge as a training path for this reconstruction problem.

References

- [1] A. Sisniega, J. W. Stayman, J. Yorkston, J. H. Siewerdsen, and W. Zbijewski, “Motion compensation in extremity cone-beam CT using a penalized image sharpness criterion,” *Phys. Med. Biol.* **62**(9), 3712–3734 (2017).
- [2] M. Thies et al., “A gradient-based approach to fast and accurate head motion compensation in cone-beam CT,” *IEEE Trans. Med. Imaging* **44**(2), 1098–1109 (2025).
- [3] H. Huang, J. H. Siewerdsen, W. Zbijewski, C. R. Weiss, T. Ehtiati, and A. Sisniega, “Reference-free learning-based similarity metric for motion compensation in cone-beam CT,” *Phys. Med. Biol.* **67**(12), 125020 (2022).
- [4] Y. Ko, S. Moon, J. Baek, and H. Shim, “Rigid and non-rigid motion artifact reduction in X-ray CT using attention module,” *Med. Image Anal.* **67**, 101883 (2021).
- [5] S. V. Venkatakrishnan, C. A. Bouman, and B. Wohlberg, “Plug-and-play priors for model based reconstruction,” in *IEEE GlobalSIP*, 945–948 (2013).
- [6] H. Chung, S. Lee, and J. C. Ye, “Decomposed diffusion sampler for accelerating large-scale inverse problems,” in *ICLR* (2024).
- [7] A. De Paepe, A. Bousse, C. Phung-Ngoc, Y. Mellak, and D. Visvikis, “Adaptive diffusion models for sparse-view motion-corrected head cone-beam CT,” *IEEE Trans. Radiat. Plasma Med. Sci.* (2025); arXiv:2504.14033.
- [8] Y. Lipman, R. T. Q. Chen, H. Ben-Hamu, M. Nickel, and M. Le, “Flow matching for generative modeling,” in *ICLR* (2023).
- [9] M. Delbracio and P. Milanfar, “Inversion by direct iteration: an alternative to denoising diffusion for image restoration,” *Trans. Mach. Learn. Res.* (2023).
- [10] M. S. Albergo, M. Goldstein, N. M. Boffi, R. Ranganath, and E. Vanden-Eijnden, “Stochastic interpolants with data-dependent couplings,” arXiv:2310.03725 (2023).
- [11] G.-H. Liu, A. Vahdat, D.-A. Huang, E. A. Theodorou, W. Nie, and A. Anandkumar, “I²SB: image-to-image Schrödinger bridge,” in *ICML* (2023).

- [12] T. Yang, J. Hu, J. A. Fessler, and L. Shen, “Local patches meet global context: scalable 3D diffusion priors for computed tomography reconstruction,” arXiv:2512.18161 (2025).
- [13] T. Müller, A. Evans, C. Schied, and A. Keller, “Instant neural graphics primitives with a multiresolution hash encoding,” *ACM Trans. Graph.* **41**(4), 102 (2022).
- [14] H. Kim and K. Champley, “Differentiable forward projector for X-ray computed tomography,” arXiv:2307.05801 (2023); LEAP, <https://github.com/LLNL/LEAP>.
- [15] S. Chilamkurthy et al., “Deep learning algorithms for detection of critical findings in head CT scans: a retrospective study,” *The Lancet* **392**(10162), 2388–2396 (2018).
- [16] H. Akima, “A new method of interpolation and smooth curve fitting based on local procedures,” *J. ACM* **17**(4), 589–602 (1970).
- [17] P. Friedrich, J. Wolleb, F. Bieder, A. Durrer, and P. C. Cattin, “WDM: 3D wavelet diffusion models for high-resolution medical image synthesis,” in *MICCAI Workshop on Deep Generative Models*, 11–21 (2024).