

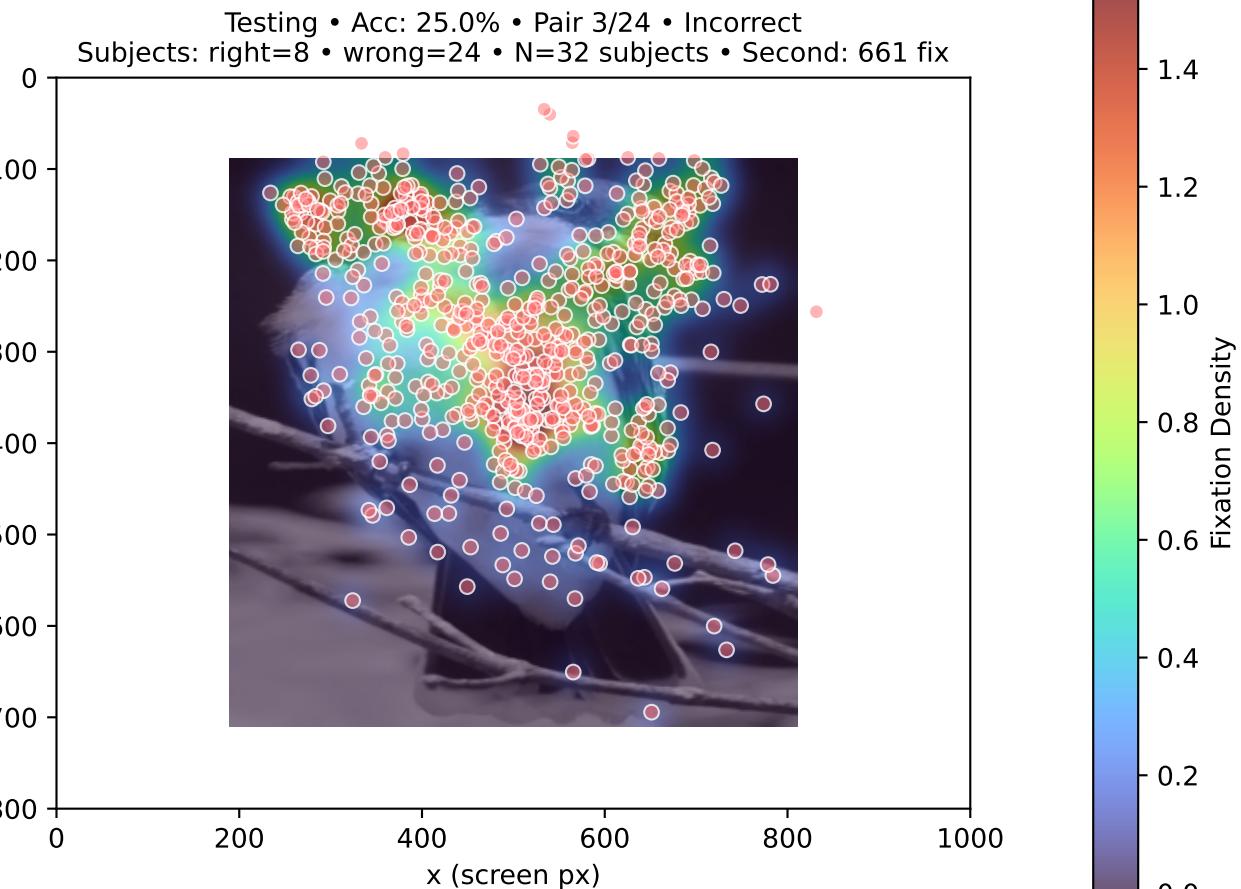
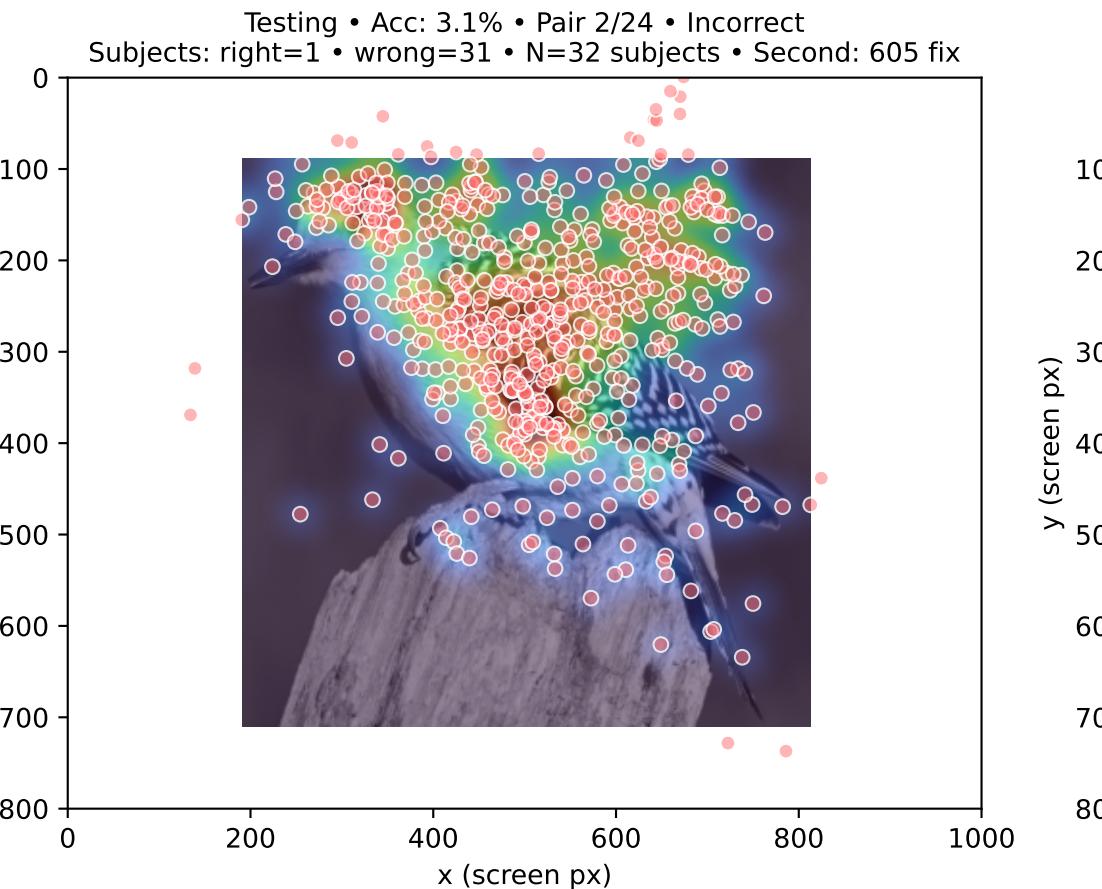
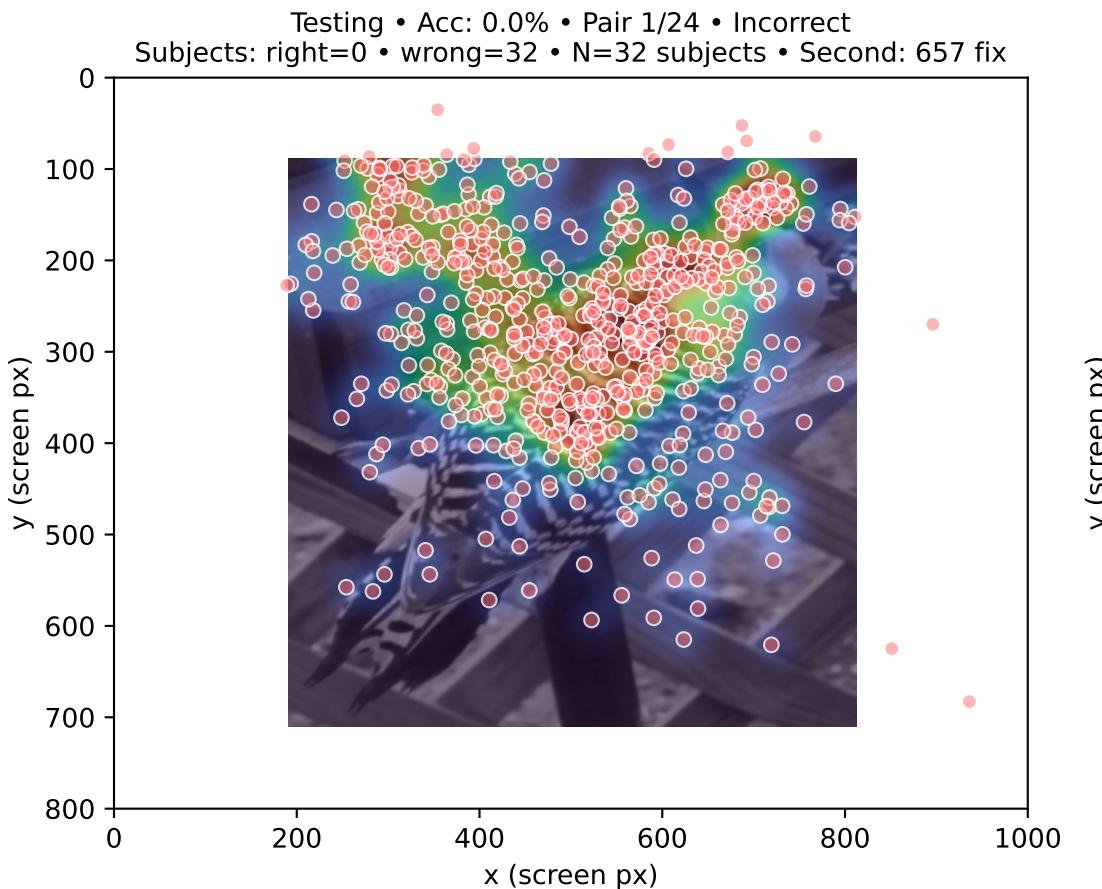
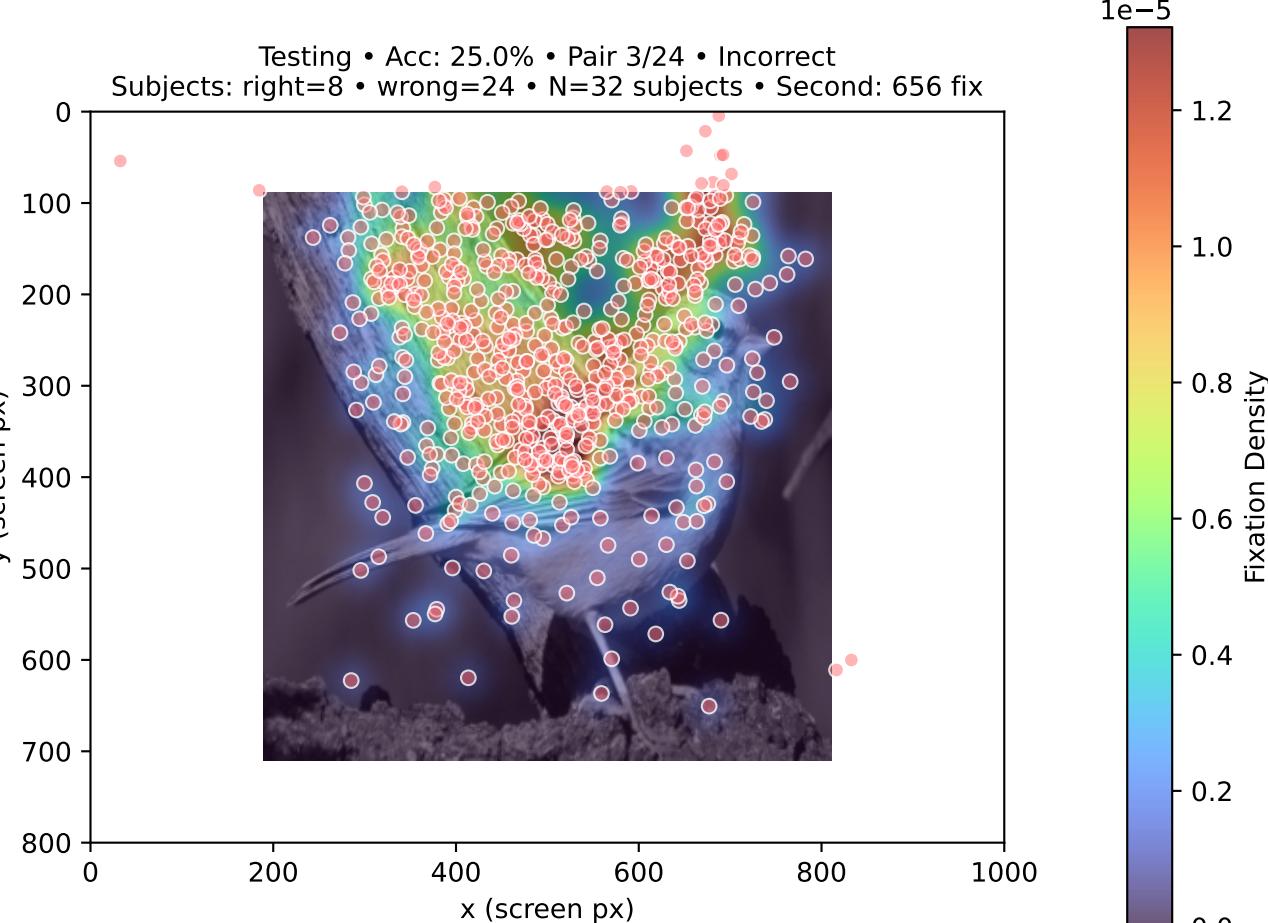





Testing Phase - FULL Viewing Condition
Bottom 3 Trials (Low Accuracy)
Ordered from Most Incorrect → Least Incorrect

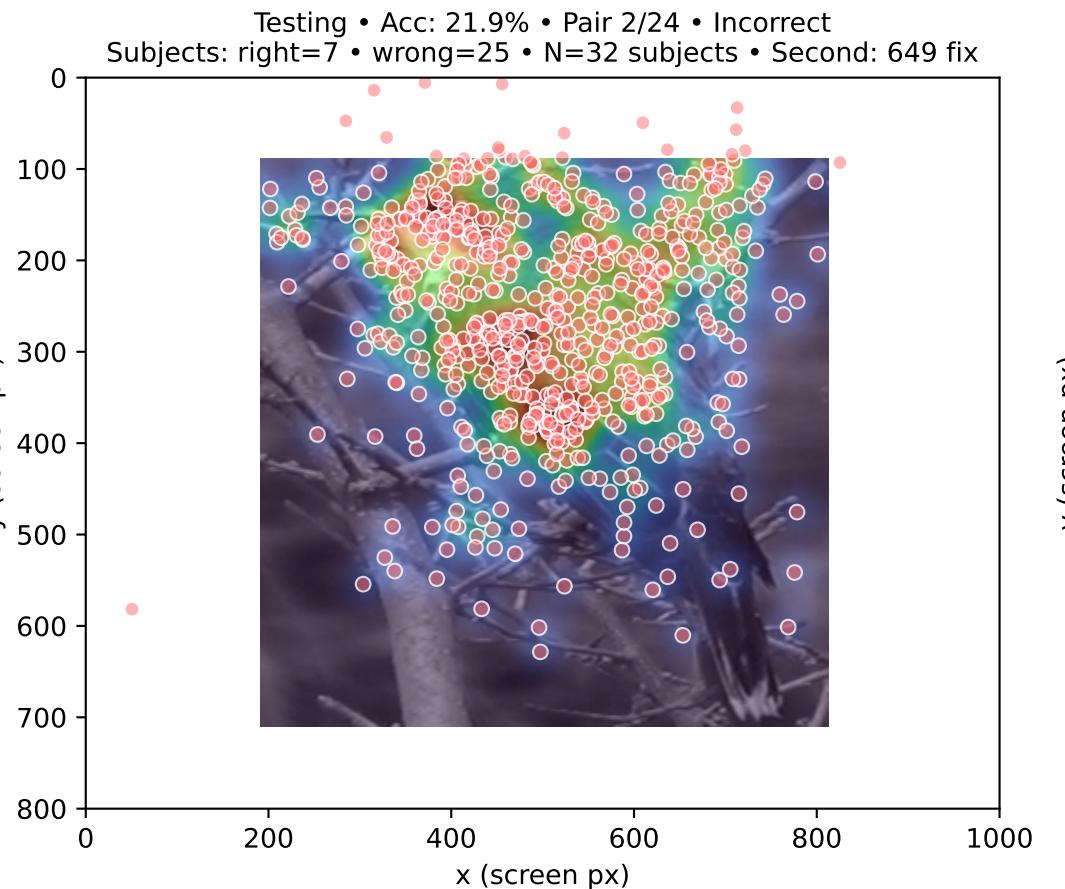

Testing Phase - CENTRAL Viewing Condition
Bottom 3 Trials (Low Accuracy)
Ordered from Most Incorrect → Least Incorrect

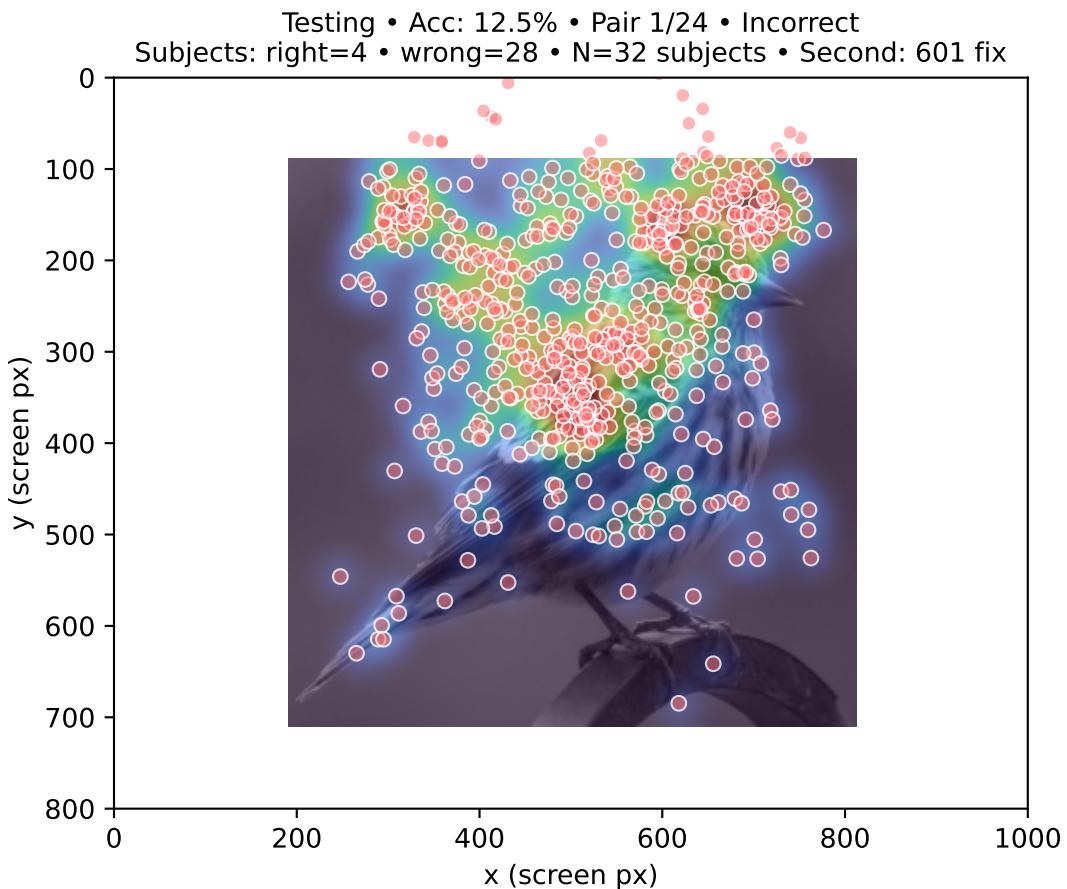

Testing Phase - PERIPHERAL Viewing Condition
Bottom 3 Trials (Low Accuracy)
Ordered from Most Incorrect → Least Incorrect

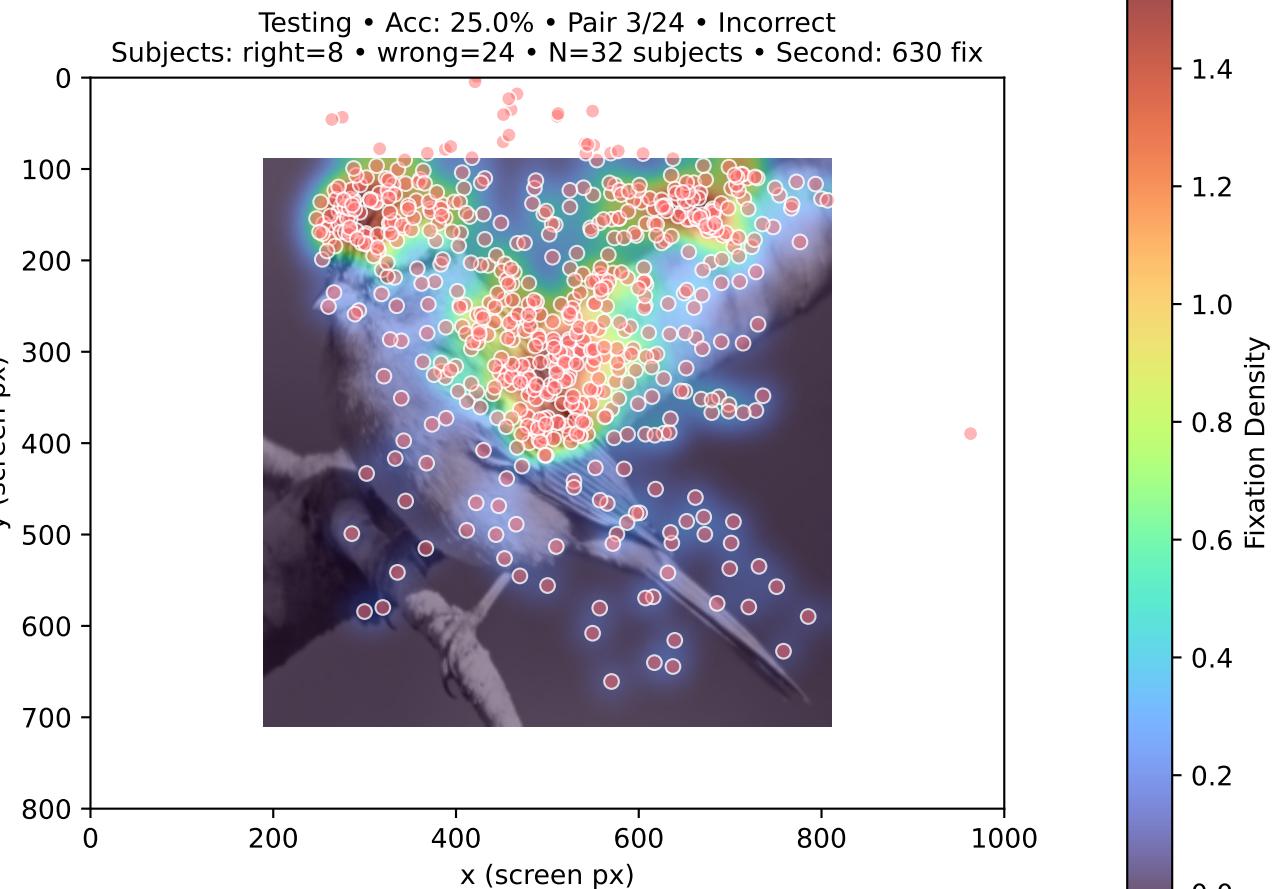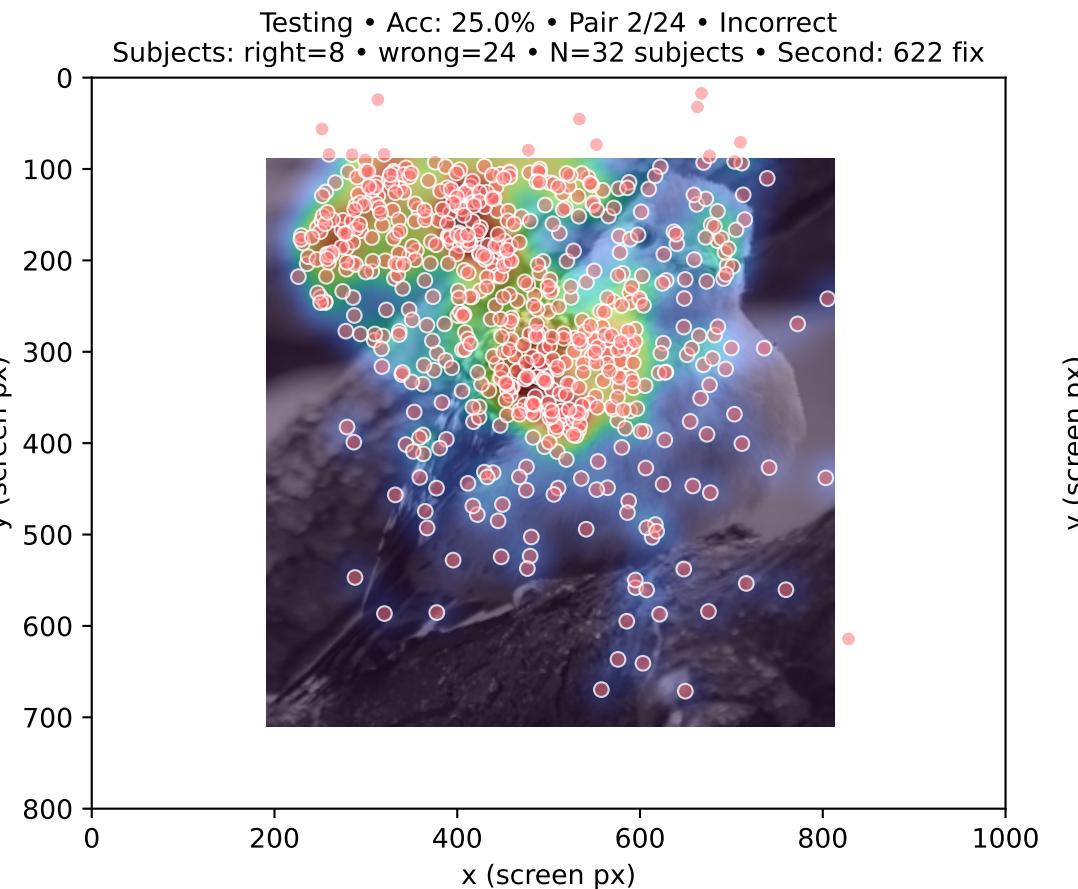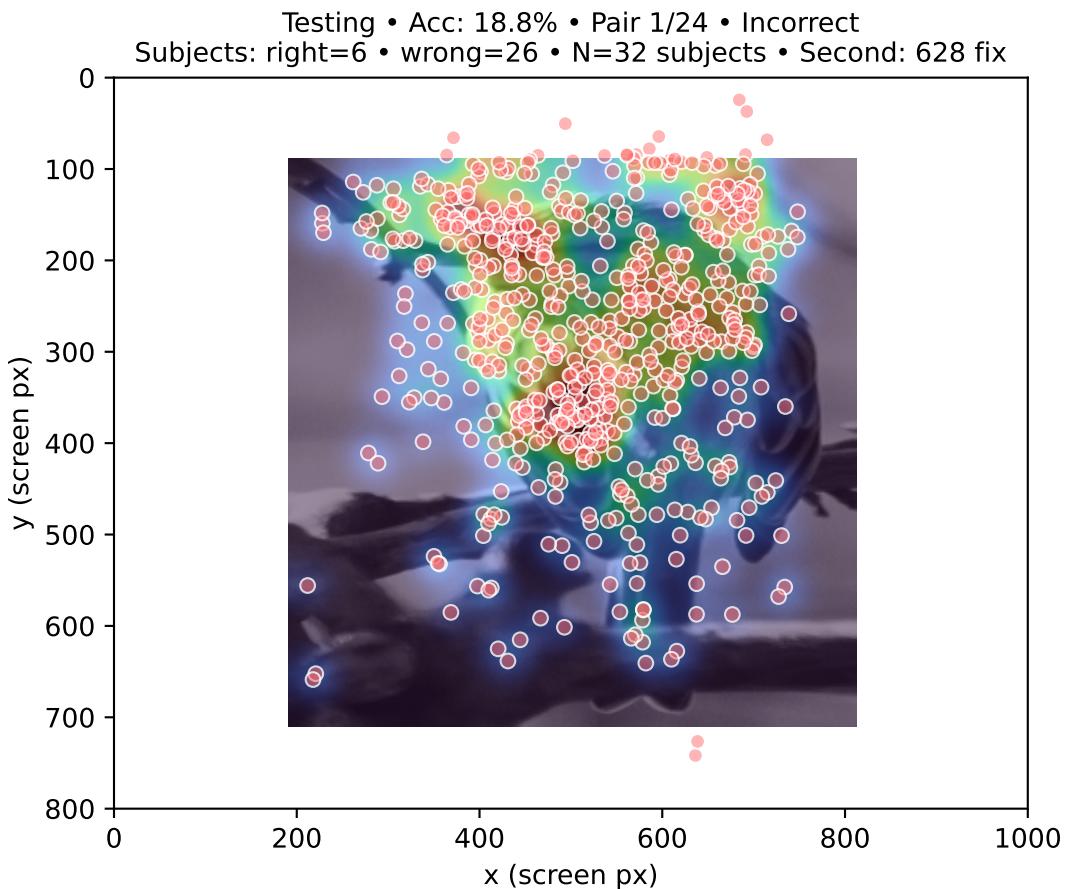

1e-5

A vertical color bar indicating the fixation density scale. The scale ranges from 0.0 (dark purple) to 1.4 (dark red), with a multiplier of 1e-5 applied to the values. The color bar is labeled 'Fixation Density' at the bottom.