


GENERAL IN-PATIENT BED

HDU location available upon request

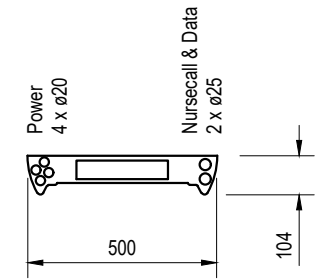

INSTRUCTIONS		
--------------	--	--


For rapid COVID-19 pandemic installation requirements this MEDICOL can be configured using a variety of our standard plates to suit the bedhead application. This enables us to expedite manufacturing for a rapid response outwith standard lead times.

Tick or circle the plate or components required as below to structure the specification.

Where a nurse call is a wireless installation for speed no plate piercing is required. If a bespoke hard wired nurse call system is required this may impact lead times of that component. Please contact us for further information.

NOTES

1. Test & certify in accordance with BS7671 & ISO11197:2016
2. Module factory gassed? YES / NO

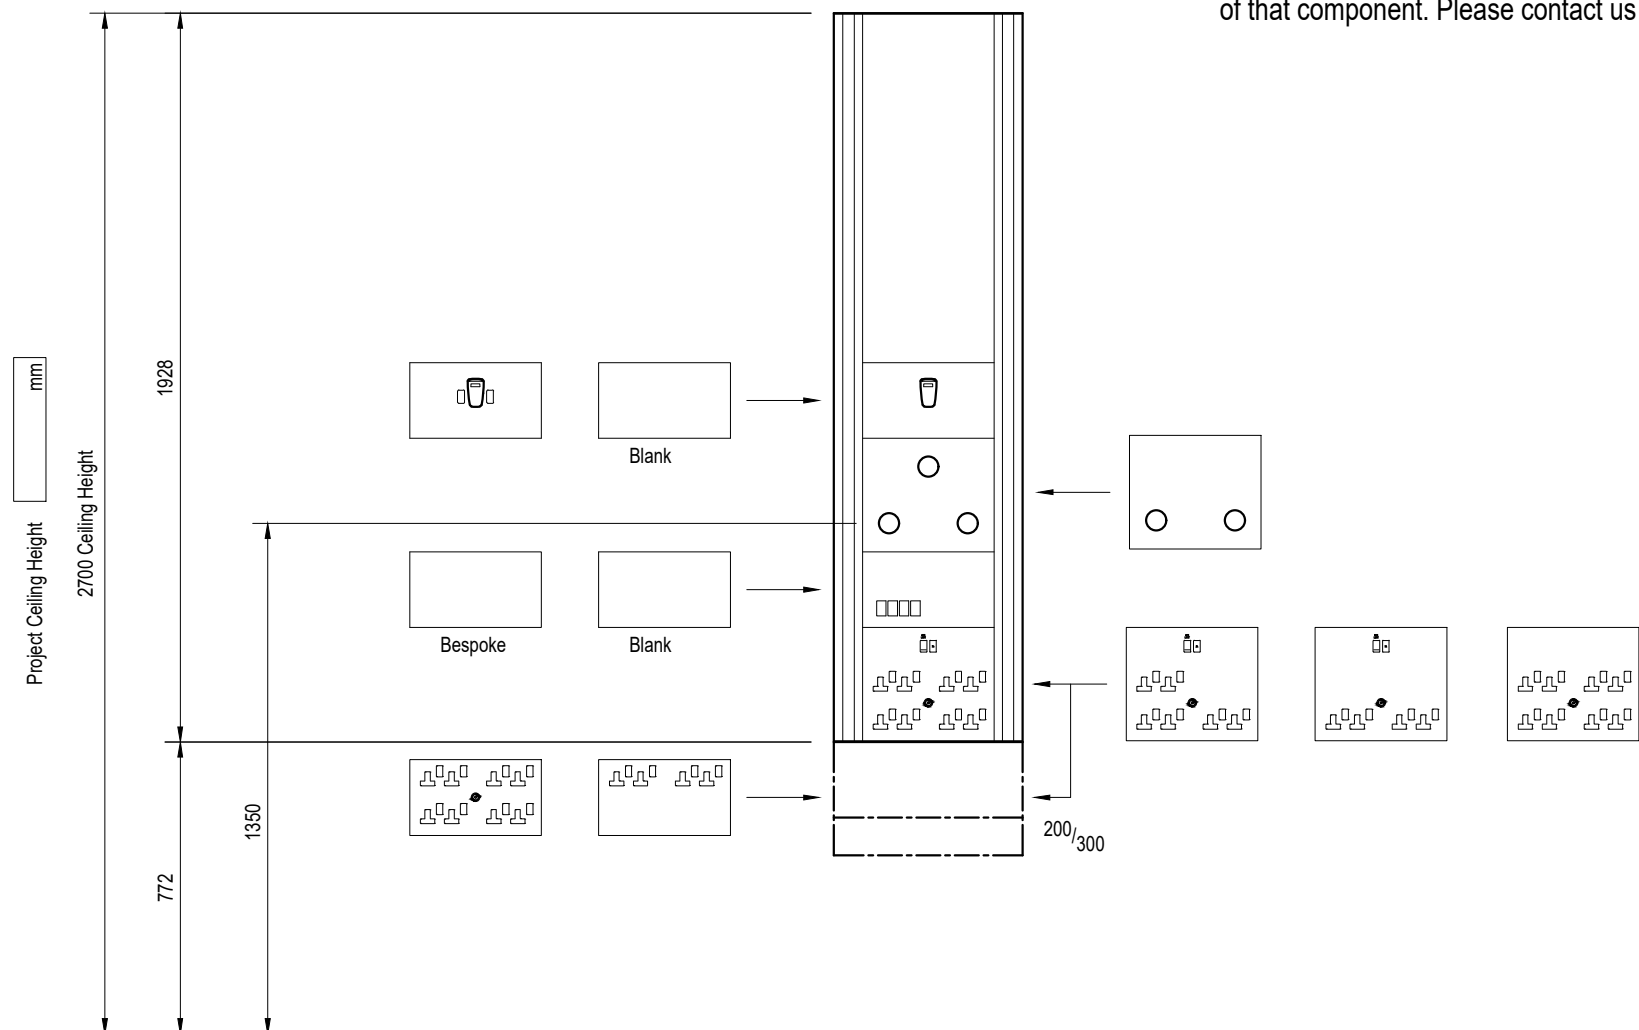

Colour
RAL9010
White
ALL OVER

Iss: A

Iss	Description	Date	Iss	Description	Date	Iss	Description	Date	CABLEFLOW™ Cableflow International Limited Cableflow International Limited Windsor House Abbey Barn Road High Wycombe Buckinghamshire HP11 1NN United Kingdom Tel: +44 (0) 1494 528811 Fax: +44 (0) 1494 531188 E-mail: sales@cableflow.com Web: www.cableflow.com © Copyright CableFlow Intnl Ltd 27/03/2020									
.	.	.	.	.	.	.	.	.	TITLE Medicol std 1 bed COVID-19 Drwn: SRP Date: 27-03-2020 DRG NO: 19870/20 1 OF 1									