


MCMC Diagnostics

Sampler: emcee via ChemEx direct EnsembleSampler
Parameters: 3
Steps: 5000
Walkers: 32
Requested burn: "auto"
Discarded steps: 73
Thin: 1
Retained steps: 4927
Retained samples: 157664
Acceptance fraction: mean=0.64731, min=0.6282, max=0.6674
Autocorrelation status: reliable
Max autocorrelation time: 36.319
Recommended steps (50 tau): 1816
Recommended steps (100 tau): 3632


Posterior summaries:
[DW_AB, NUC->55N]: median=4.6817, 95% ETI=[4.603, 4.7581], ESS=4341.1
[R1_A, NUC->55N, B0->600.3MHZ]: median=1.5966, 95% ETI=[1.5812, 1.6124], ESS=4463.8
[R2_A, NUC->55N, B0->600.3MHZ]: median=10.002, 95% ETI=[9.8477, 10.161], ESS=4408

Correlation threshold: $|r| \geq 0.5$
No parameter pairs exceeded the correlation threshold.


Posterior distribution: [DW_AB, NUC->55N]

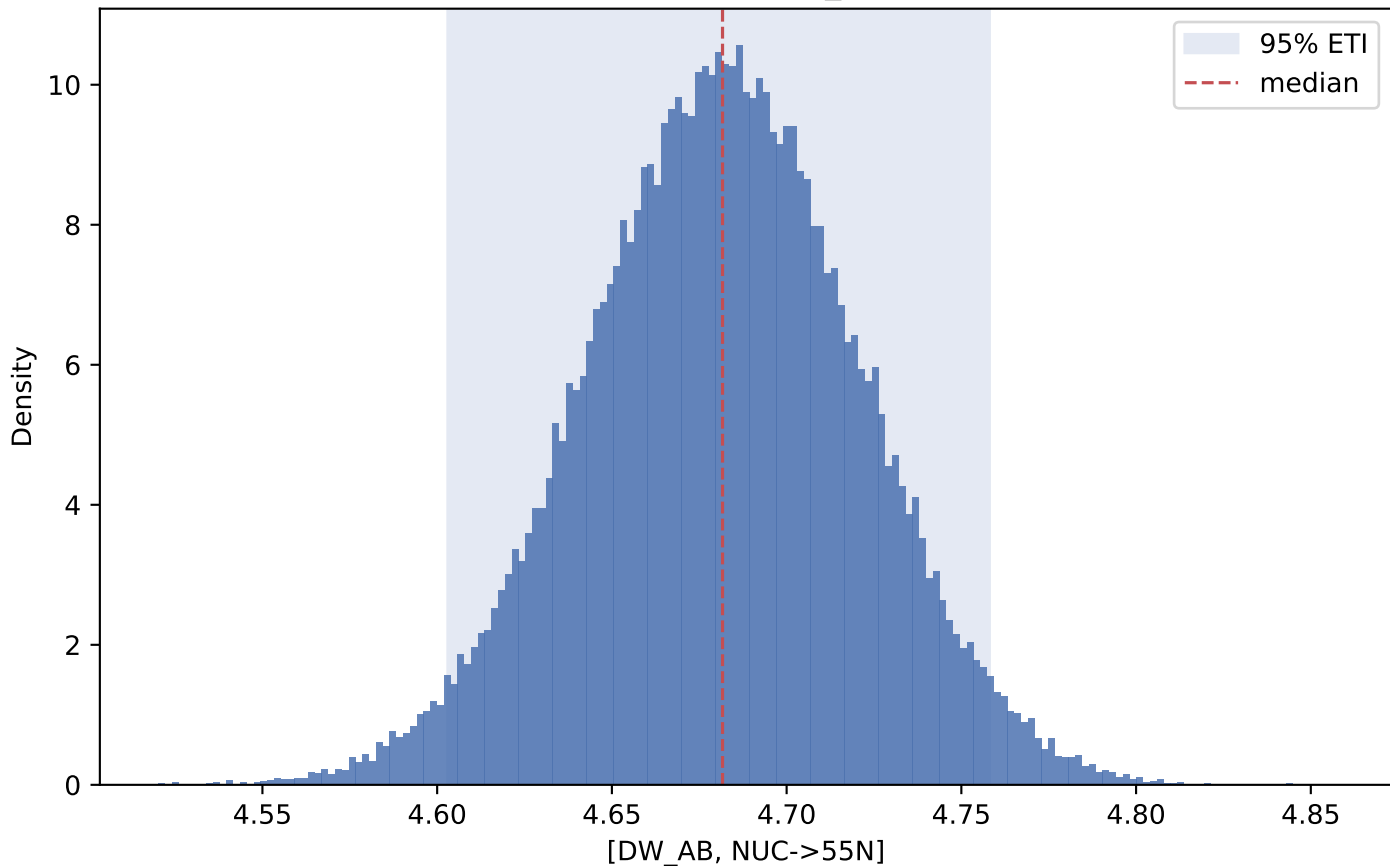


Posterior distribution: [R1_A, NUC->55N, B0->600.3MHZ]

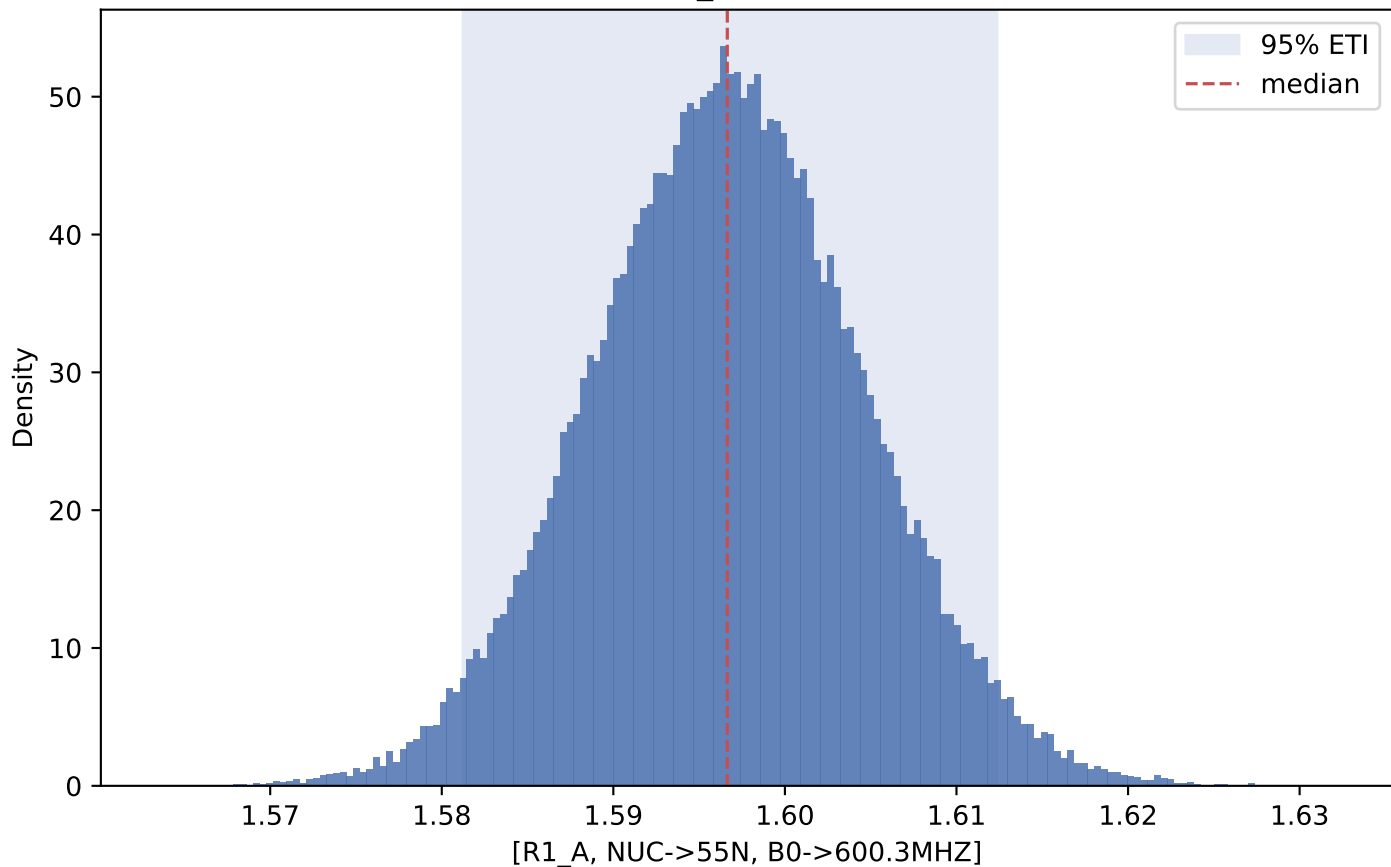


Posterior distribution: [R2_A, NUC->55N, B0->600.3MHZ]

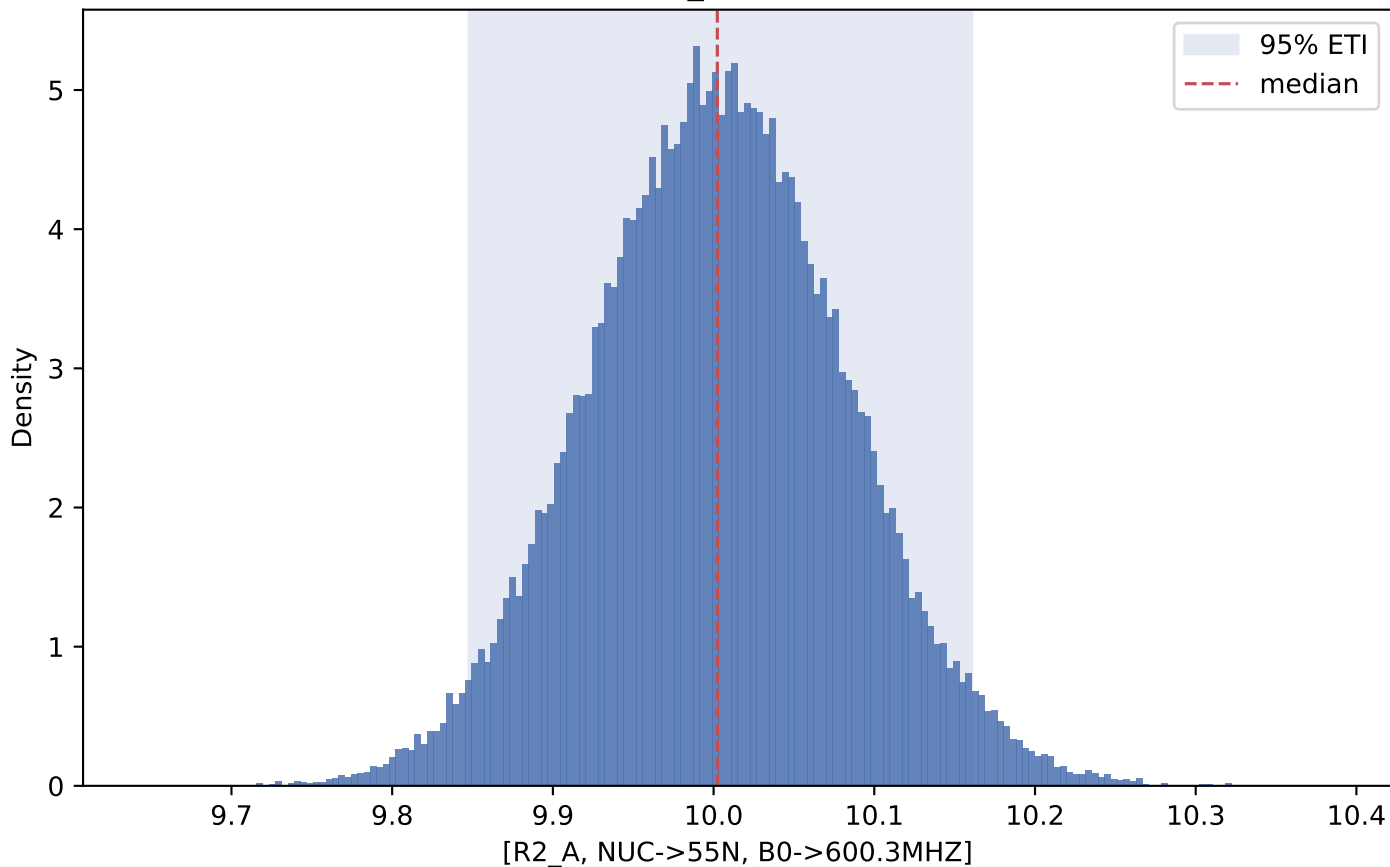


MCMC trace: [DW_AB, NUC->55N]

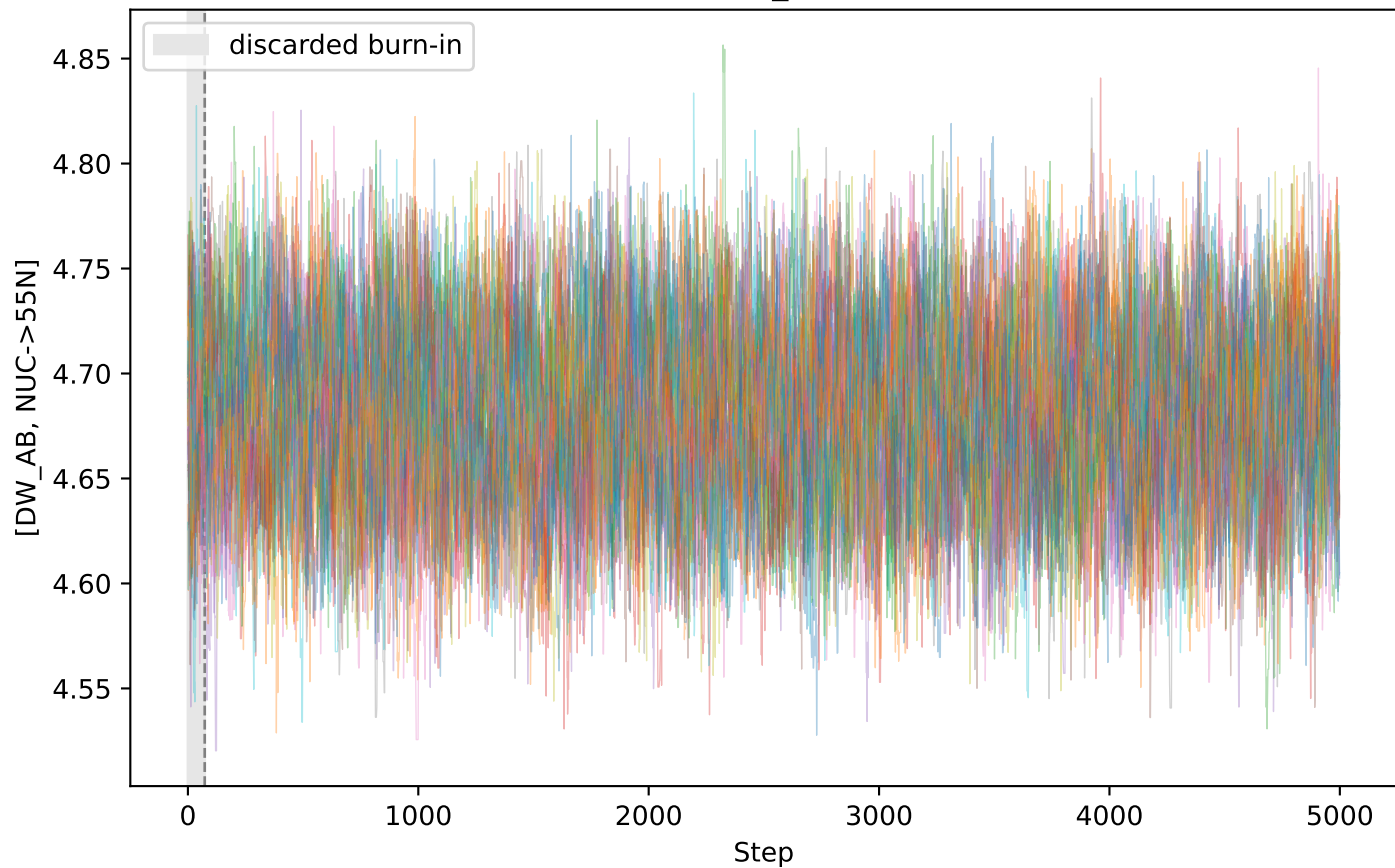


MCMC trace: [R1_A, NUC->55N, B0->600.3MHZ]

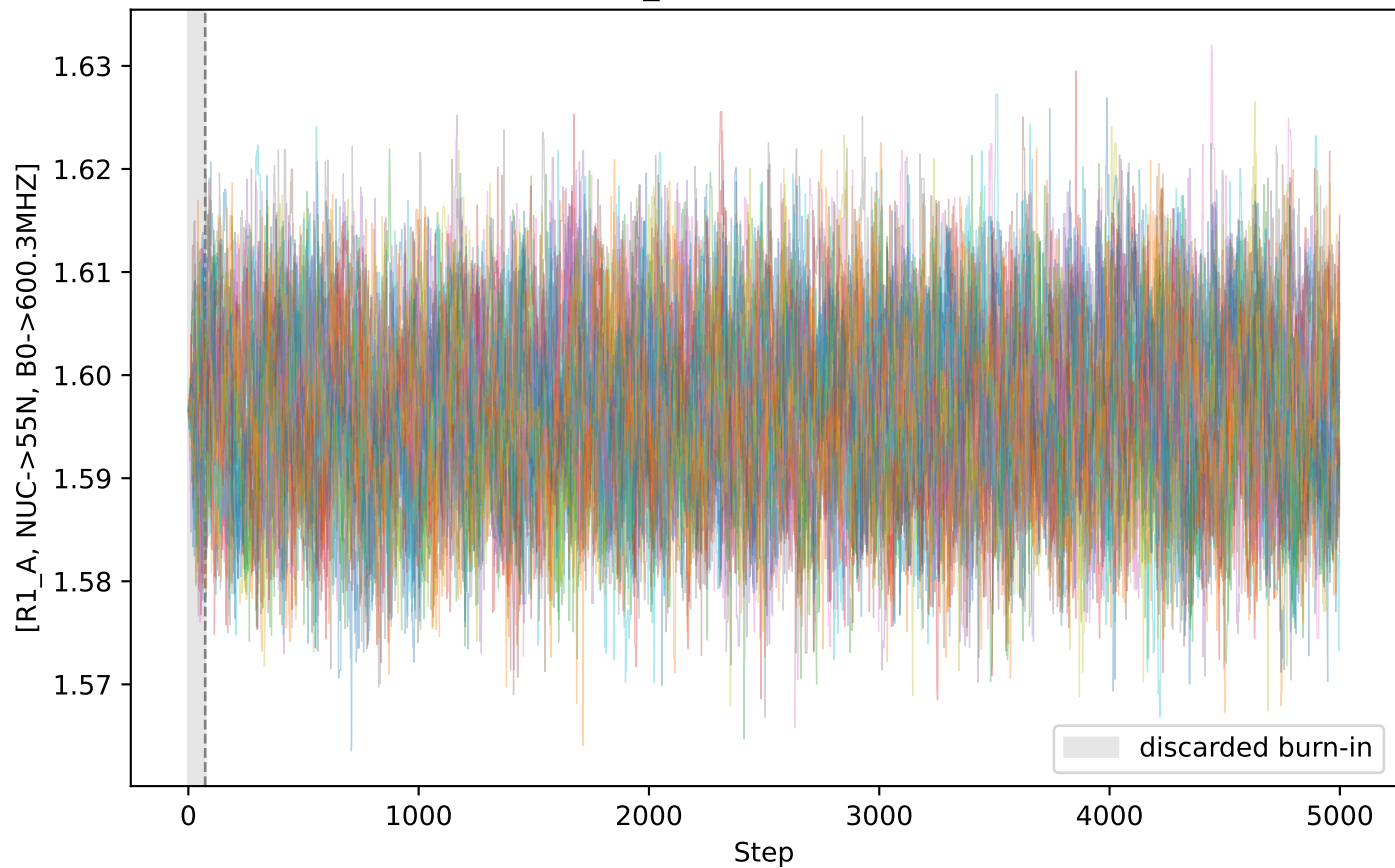

MCMC trace: [R2_A, NUC->55N, B0->600.3MHZ]

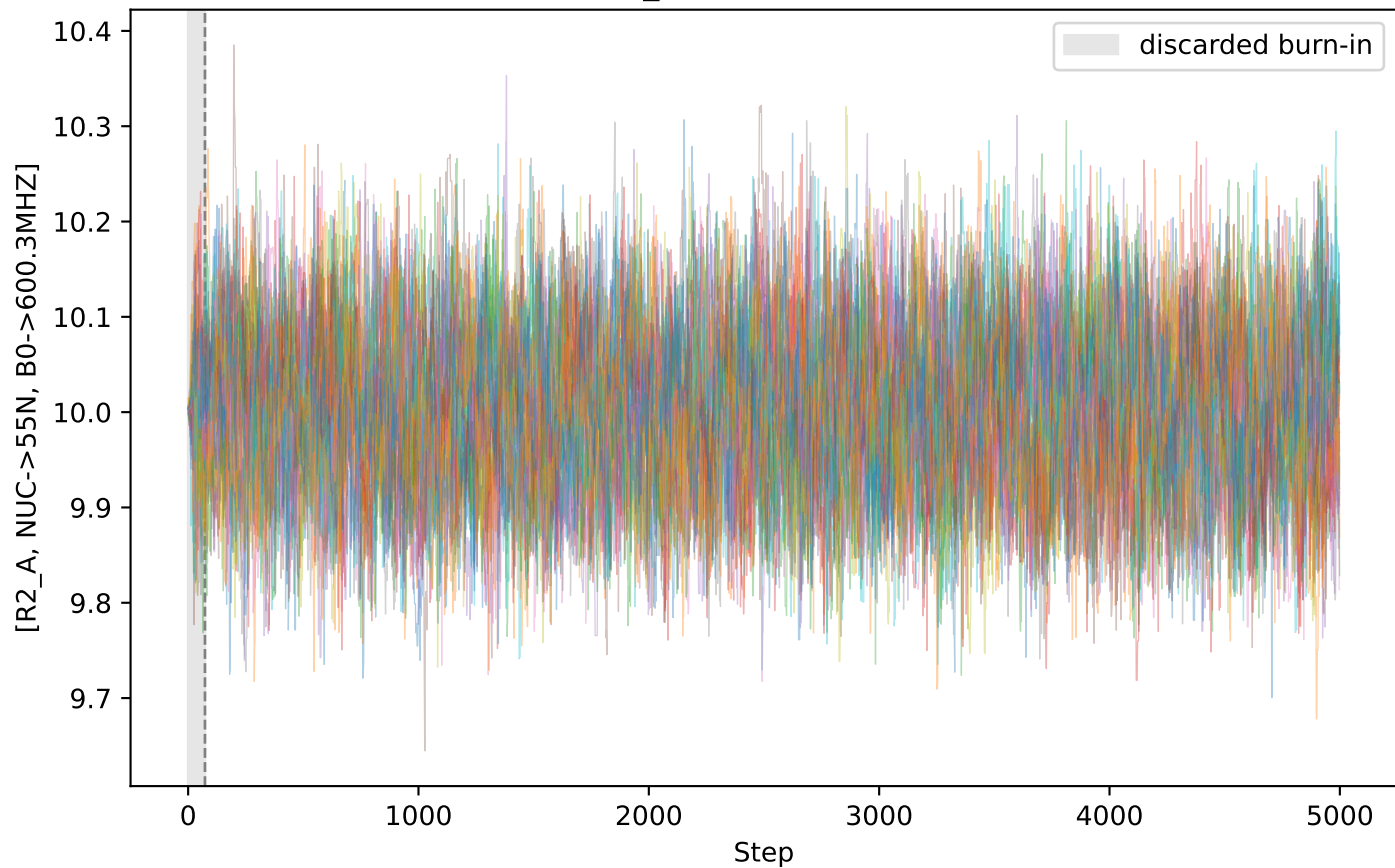

MCMC log-probability trace

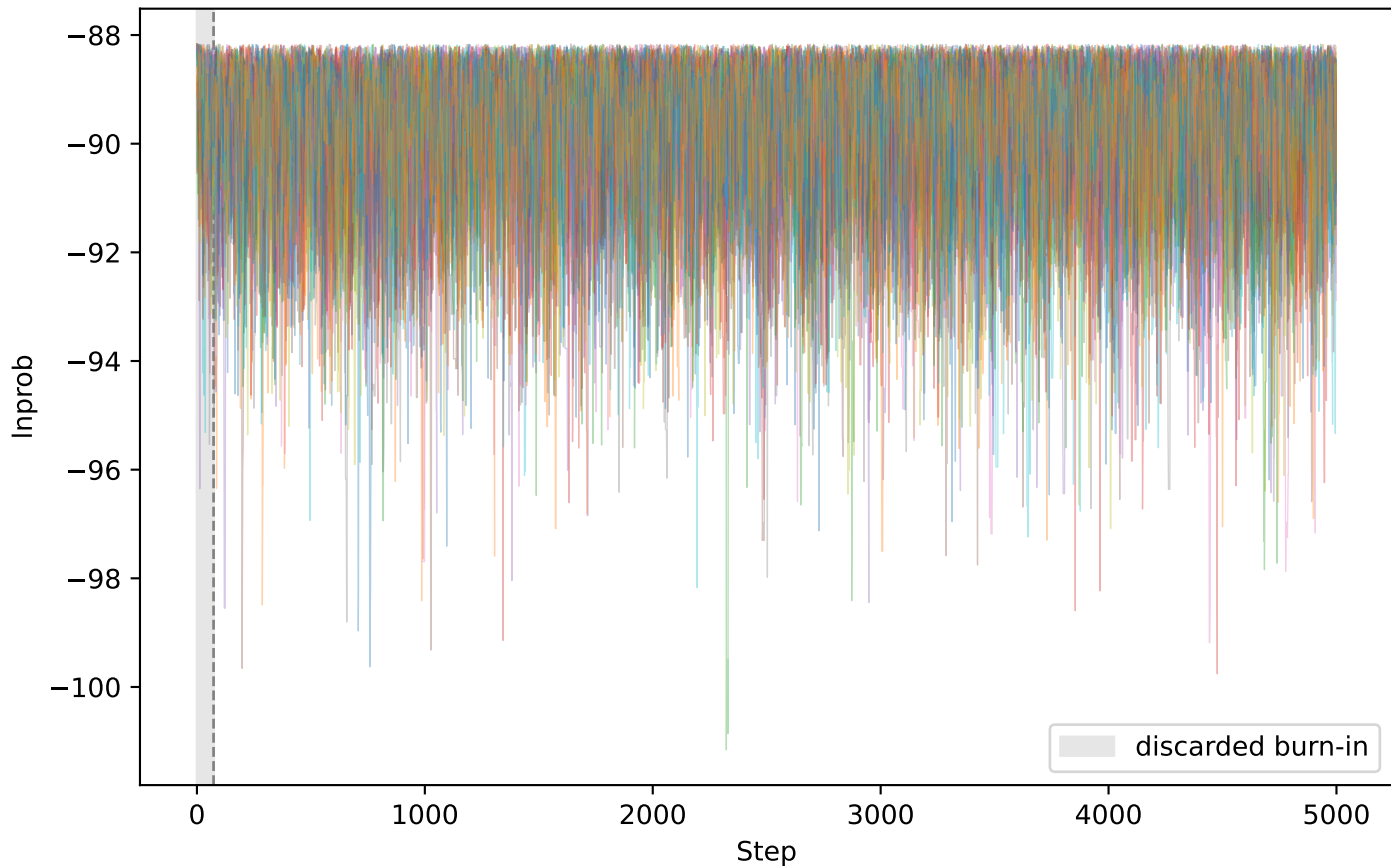

MCMC autocorrelation monitor

