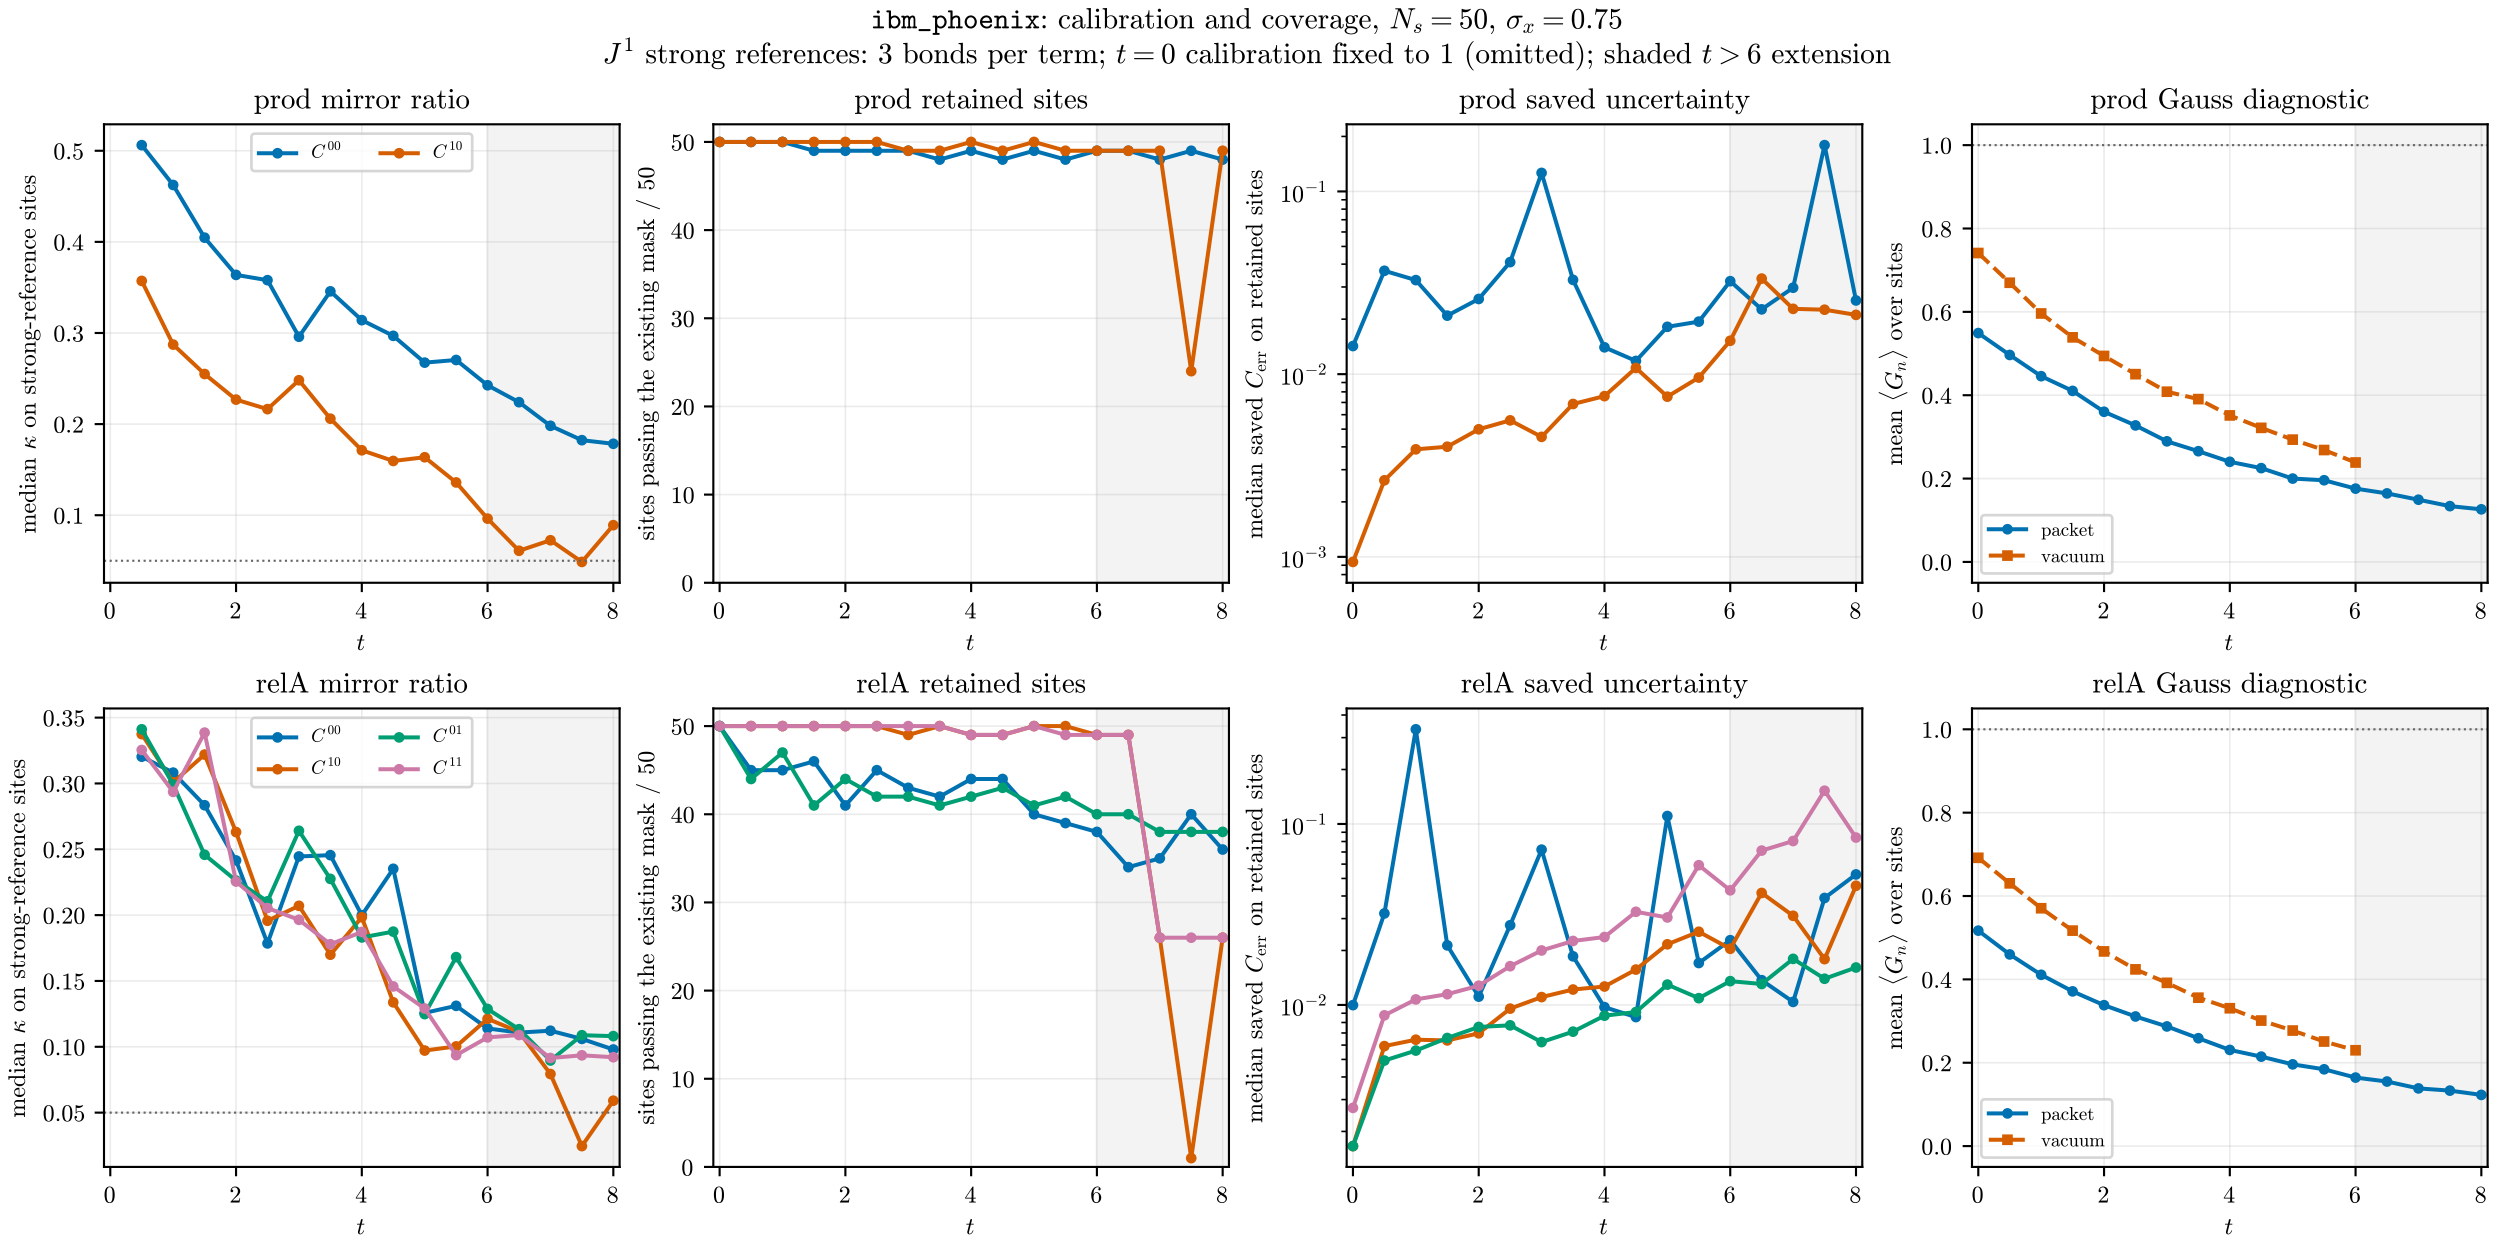

ibm_phoenix: calibration and coverage, $N_s = 50$, $\sigma_x = 0.75$
J^1 strong references: 3 bonds per term; $t = 0$ calibration fixed to 1 (omitted); shaded $t > 6$ extension
prod mirror ratio
prod retained sites
prod saved uncertainty
prod Gauss diagnostic
relA mirror ratio
relA retained sites
relA saved uncertainty
relA Gauss diagnostic
median κ on strong-reference sites
sites passing the existing mask / 50
median saved C_{err} on retained sites
mean $\langle G_n \rangle$ over sites
t
C^{00}
C^{10}
C^{01}
C^{11}
packet
vacuum