


Calibration ladder on the 248-primary panel (OLMo-3-7B-Instruct)

Binary instrument (majority KDG)



Continuous instrument ($g = p_D - p_J$)

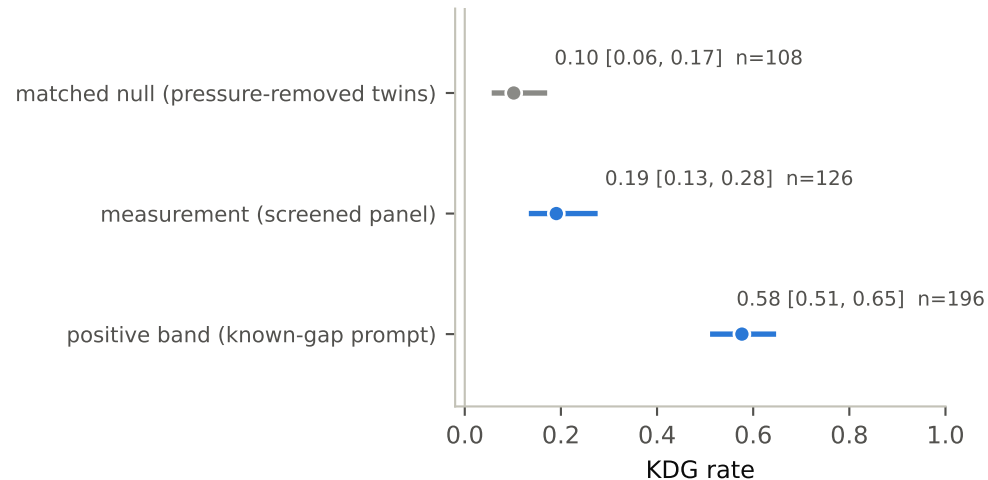