

# Analysis of Toxic Elements in Drinking and Bottled Waters using the Thermo Scientific iCAP 7200 ICP-OES

Patrícia Coelho, Applications Chemist, Thermo Fisher Scientific, Cambridge, UK

## Key Words

Bottled water, Drinking water, Environmental analysis, Toxic elements

## Goal

This application note describes the analysis of several toxic elements in drinking and bottled waters using the Thermo Scientific™ iCAP™ 7200 ICP-OES. The pre-loaded templates provide a simple and effective tool for routine environmental analysis. Additionally the duo plasma enables excellent detection limits for toxic elements using axial view.

## Introduction

The increase in popularity of bottled drinking water has prompted many new regulations which manufacturers must adhere to. These apply to the country in which the water is sold and consumed. China and India have seen a huge increase in the consumption of bottled water in the last decade which has driven the contract analysis of toxic elements in these products to the following regulations in the respective countries (listed below with maximum limits expressed in Table 1).

### Chinese regulations:

- GB 8537–2008 - Drinking natural mineral water
- GB 17324–2003 - Hygienic standard of bottled purified water for drinking
- GB 5749–2006 - Standards for drinking water quality
- GB 3838–2002 - Environmental quality standard for surface water

### Indian regulations:

- IS 10500:2012 - Drinking Water
- IS 13428:2005 - Packaged natural mineral water
- IS 14543:2004 - Packaged drinking water (other than packaged natural mineral water)



Table 1. Maximum permissible levels in ppm.

Element	GB 8537-2008	GB 17324-2003	GB 5749-2006	GB 3838-2002 (I) <sup>1</sup>	IS 10500:2012	IS 13428:2005	IS 14543:2004
Arsenic	0.01	0.01	0.01	0.05	0.01	0.05	0.05
Cadmium	0.003	-	0.005	0.001	0.003	0.003	0.01
Chromium*	0.05	-	0.05	0.01	0.05	0.05	0.05
Copper	1	0.01	1	0.01	0.05	1	0.05
Iron	-	-	0.3	0.3	0.3	-	0.1
Lead	0.01	0.01	0.01	0.01	0.01	0.01	0.01
Mercury	0.001	-	0.001	0.00005	0.001	0.001	0.001
Nickel	0.02	-	0.02	0.02	0.02	0.02	0.02
Zinc	0.2	-	1	0.05	5	5	5

<sup>1</sup> For GB 3838, (I) refers to Class I categories, stated as mainly applicable to the source of water, National Nature Reserve.

\* For Chinese regulations, chromium is defined as hexavalent chromium present.

## Instrumentation

The Thermo Scientific iCAP 7200 ICP-OES was used for the analysis. This is a compact dual view ICP-OES instrument based on the powerful core technologies of the iCAP 7000 Series ICP-OES. The instrument achieves powerful analyte detection and provides a highly cost effective solution for routine analysis of liquids in laboratories with standard sample throughput requirements. The Thermo Scientific™ Qtegra™ Intelligent Scientific Data Solution™ (ISDS) incorporates pre-loaded analysis-ready templates (see Figure 1) to simplify method development.

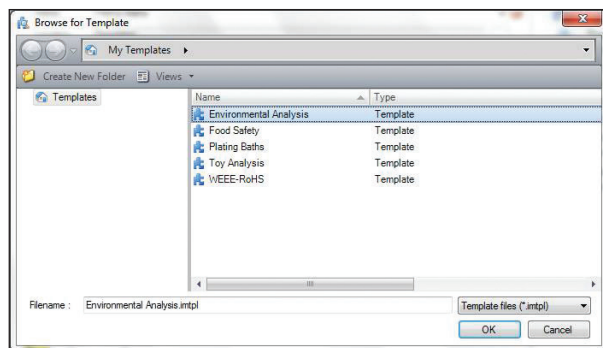


Figure 1. Environmental Analysis template selection.

## Sample and standard preparation

A selection of drinking water samples (tap water and bottled water) were collected in China for analysis. In addition, European bottled water was also tested for comparison. The samples are listed below:

- Tap water sample from Dingpu river area, Shanghai
- Tap water sample from Jinqiao lake area, Shanghai
- Waterman (packaged drinking water)
- Nestle (natural mineral water)
- Evian (natural mineral water)

The samples did not require any pre-treatment and were analyzed directly after preservation in 0.5% analytical grade nitric acid (HNO<sub>3</sub>). Calibration standards were prepared in 0.5% HNO<sub>3</sub> at the following concentrations: 0, 50 and 100 ppb. A QC Check solution was prepared at 10 ppb to check recovery rate and test the stability of the method.

## Method development

The Environmental Analysis template was opened within the Qtegra ISDS – this contains all of the required method parameters and standard concentrations as listed in this note. A standard sample introduction kit was used for the analysis as per the recommendations in the method notes. The method parameters are shown below in Table 2.

Table 2. Methods parameters.

Parameter	Setting
Pump tubing	Sample Tygon® orange/white Drain Tygon® white/white
Pump speed	45 rpm
Nebulizer	Glass concentric
Nebulizer gas flow	0.19 MPa
Spray chamber	Glass cyclonic
Auxiliary gas flow	0.5 L/min
Coolant gas flow	12 L/min
Center tube	2 mm
RF Power	1150 W
Torch orientation	Axial
Exposure time	5 sec

The samples were repeatedly analyzed in a single automated run over a period of 4 hours. Using the functionalities of Qtegra ISDS, a QC check was performed every 10 samples, recalibrating, recalculating and reacquiring from a previous sample whenever this check fails. A calibration was performed every 30 samples as per the requirements of the regulation.

## Results

The samples were analyzed repeatedly in batches of 10 (2 of each of the 5 samples). Table 3 shows the averaged results of samples over the 4 hours and the method detection limits (MDLs). The concentrations found in all the samples were within the values outlined in the Chinese and Indian regulations. The MDLs are shown to be fit for purpose for this application. Nevertheless, the use of hydride generation accessories may be employed to further improve MDLs, particularly for mercury (to achieve sub ppb levels) when required.

Table 3. Averaged results and method detection limits in ppb.

Element and Wavelength nm	MDL	Dingpu River	Jinquiao Lake	Waterman	Nestle	Evian
As 193.759	2.14	<DL	1.27	<DL	<DL	<DL
Cd 214.438	0.07	<DL	<DL	<DL	<DL	<DL
Cr 205.560	0.21	<DL	<DL	<DL	<DL	<DL
Cu 324.754	0.39	<DL	1.52	<DL	<DL	<DL
Fe 259.940	0.25	1.14	1.53	0.41	0.78	0.74
Hg 194.227	0.66	<DL	<DL	<DL	<DL	<DL
Ni 231.604	0.36	1.05	0.57	<DL	<DL	<DL
Pb 220.353	1.06	<DL	<DL	<DL	<DL	<DL
Zn 213.856	0.19	<DL	<DL	<DL	<DL	<DL

The 10 ppb QC check was used to check for recovery rates and drift during the run; which was found to be exceptionally stable as the chart below (see Figure 2) demonstrates. All QC recoveries were within 10% of their expected values throughout the 4 hour run.

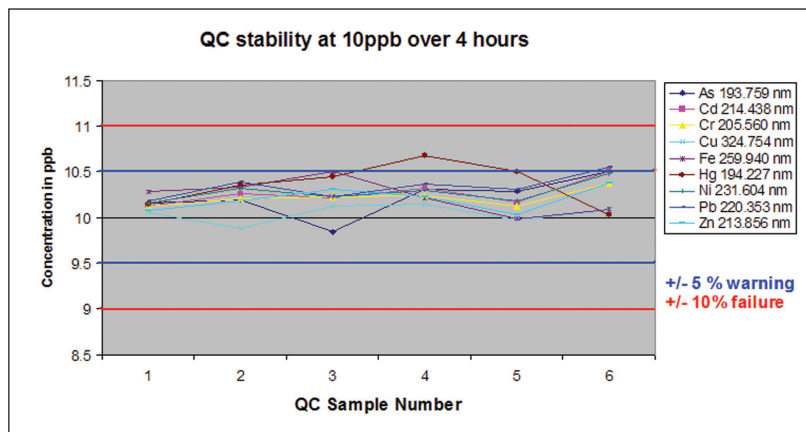


Figure 2. Stability of the 10ppb QC Check over 4 hours.

## Conclusion

The analysis of environmental samples is rapid and analyst friendly using the Thermo Scientific iCAP 7200 ICP-OES with the pre-loaded template. The powerful and innovative design features of this instrument allow both novice and experienced analysts to quickly generate excellent results which allows a highly cost efficient sample analysis regime.

[thermofisher.com](http://thermofisher.com)

©2016 Thermo Fisher Scientific Inc. All rights reserved. Tygon is a registered trademark of Saint-Gobain. All other trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details.

<b>Africa-Other</b> +27 11 570 1840	<b>Europe-Other</b> +43 1 333 50 34 0	<b>Japan</b> +81 45 453 9100	<b>Spain</b> +34 914 845 965
<b>Australia</b> +61 3 9757 4300	<b>Finland/Norway/Sweden</b> +46 8 556 468 00	<b>Latin America</b> +1 561 688 8700	<b>Switzerland</b> +41 61 716 77 00
<b>Austria</b> +43 1 333 50 34 0	<b>France</b> +33 1 60 92 48 00	<b>Middle East</b> +43 1 333 50 34 0	<b>UK</b> +44 1442 233555
<b>Belgium</b> +32 53 73 42 41	<b>Germany</b> +49 6103 408 1014	<b>Netherlands</b> +31 76 579 55 55	<b>USA</b> +1 800 532 4752
<b>Canada</b> +1 800 530 8447	<b>India</b> +91 22 6742 9434	<b>New Zealand</b> +64 9 980 6700	
<b>China</b> +86 10 8419 3588	<b>Italy</b> +39 02 950 591	<b>Russia/CIS</b> +43 1 333 50 34 0	
<b>Denmark</b> +45 70 23 62 60		<b>South Africa</b> +27 11 570 1840	

**Thermo**  
SCIENTIFIC

Part of Thermo Fisher Scientific