

Implant Report

Patient: nikitaben roy
Date of birth: 01/01/2000
Project: nikitaben roy_project1

Patient Information


Name: nikitaben roy
Date of birth: 01/01/2000
Clinician:
Drug therapies:
General health status:

Exam Information


Exam Date: 10/12/2025
Images: 251
Slice thickness: 0.174923
Description:
Project name: nikitaben roy_project1
Last modified:

Planning Information


Implants type: Straumann
Number of implants: 2
Immediate loading: Yes
Type of guide: Mucosa soft tissue supported
Type of fixation: Fixation pins
Flapless surgery: Yes
Bone regeneration: No
Add Sinus Graft/Lift: No
Add Nasal Graft/Lift: No

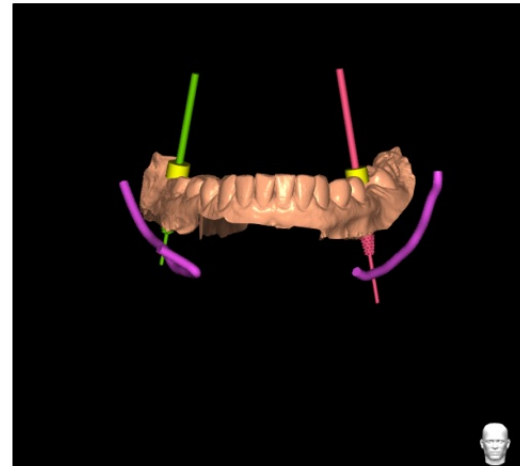


Frontal view

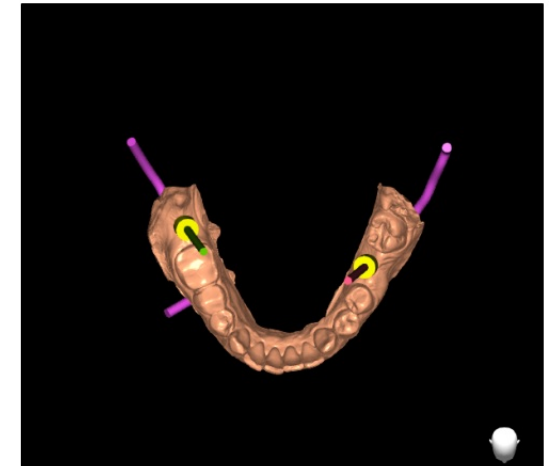

Occlusal view

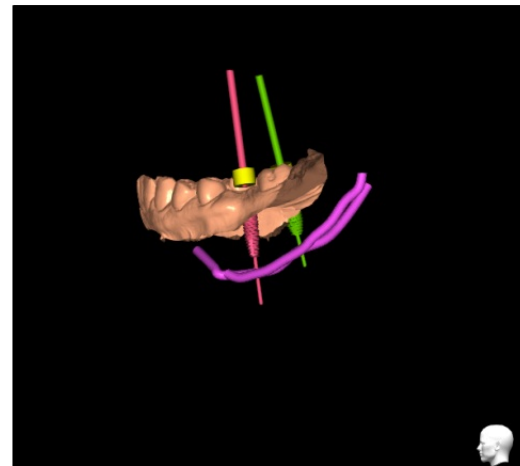


Left view

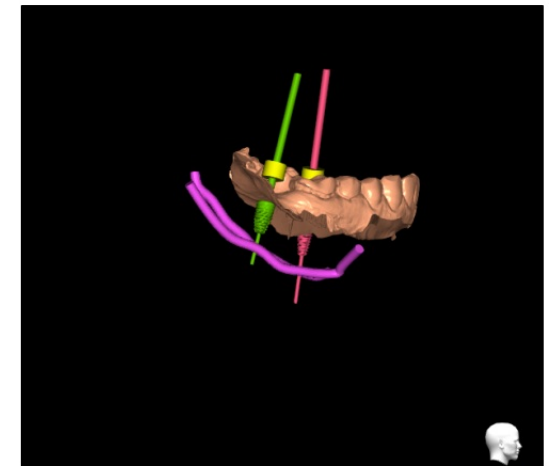

Right view

Planning scheme: Implants

Patient: nikitaben roy
Date of birth: 01/01/2000
Project: nikitaben roy_project1

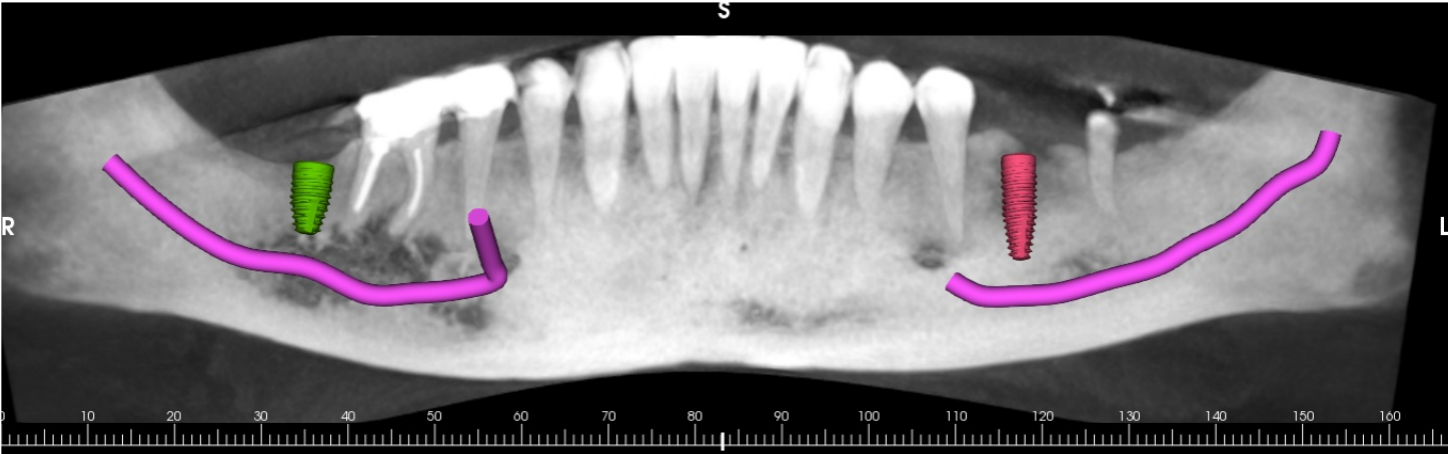

Notes:

Position	Manufacturer	Model	Size	Abutment	Abutment size	Sleeve	Collision warnings
35	Straumann	BLT SLA	RC 4.1 x 12 mm [021.5512]			Hiossen Parametric_OneGuide - D 5.7 mm Closed	No collision
47	Straumann	BLT SLA	RC 4.8 x 8 mm [021.7508]			Hiossen Parametric_OneGuide - D 5.7 mm Closed	No collision



IDDS
3D PRINTING SOLUTIONS

The image scale depends on printer settings and might not be in 1:1 ratio, check rulers on images for reference.
The HU scale depends on acquisition machine calibration, please refer to manufacturer settings and scan settings.
Please refer to the Implant Manufacturer's instructional literature for information on the surgical kit and instrumentation.

Planning scheme: Implants

Implant number: 47

Manufacturer: Straumann

Model: BLT SLA

Size: RC 4.8 x 8 mm

Abutment:

Abt. size:

Implant number: 35


Manufacturer: Straumann

Model: BLT SLA


Size: RC 4.1 x 12 mm

Abutment:


Abt. size:

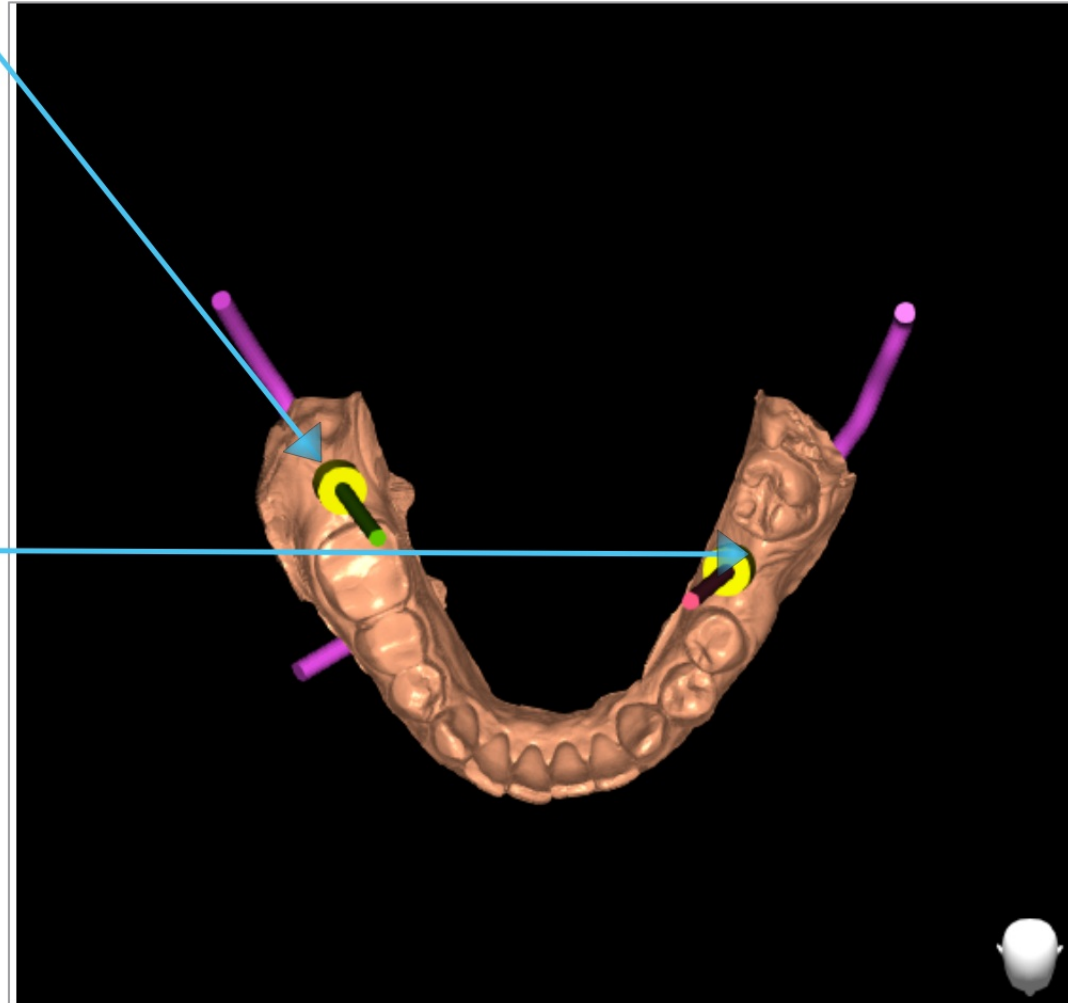




Planning scheme: Implants

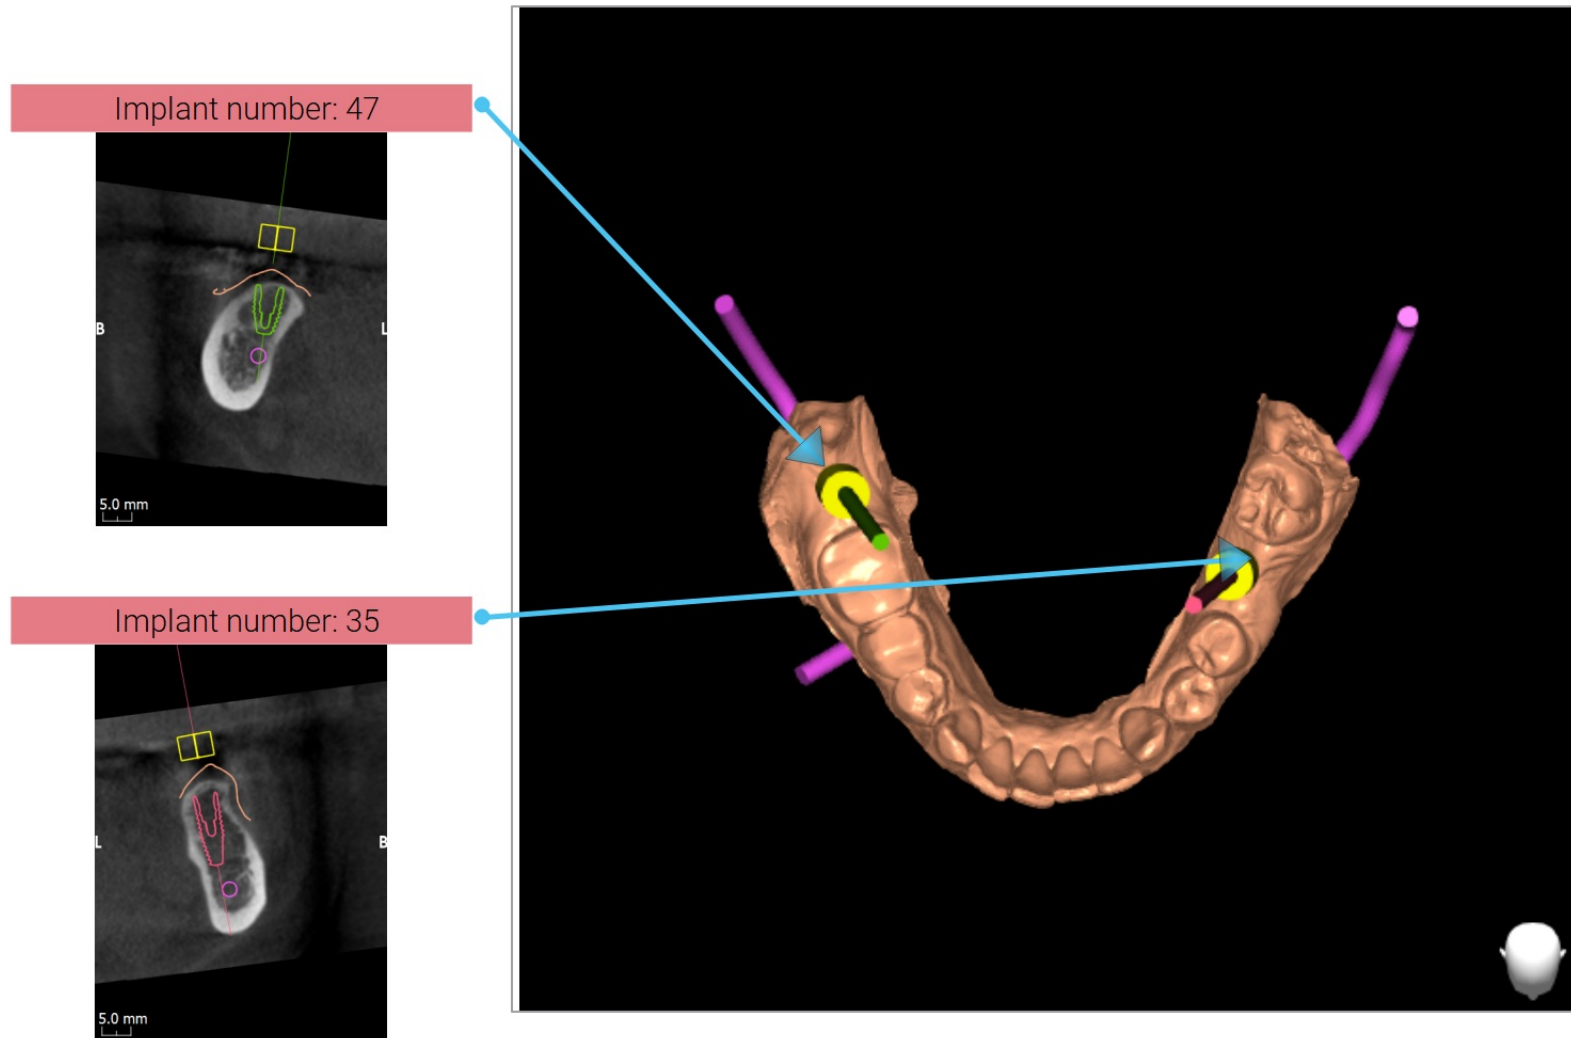


Position	Manufacturer	Model	Size	Abutment	Abutment size	Sleeve	Sleeve top height
35	Straumann	BLT SLA	RC 4.1 x 12 mm [021.5512]			Hiossen Parametric_OneGuide - D 5.7 mm Closed	10.50 mm

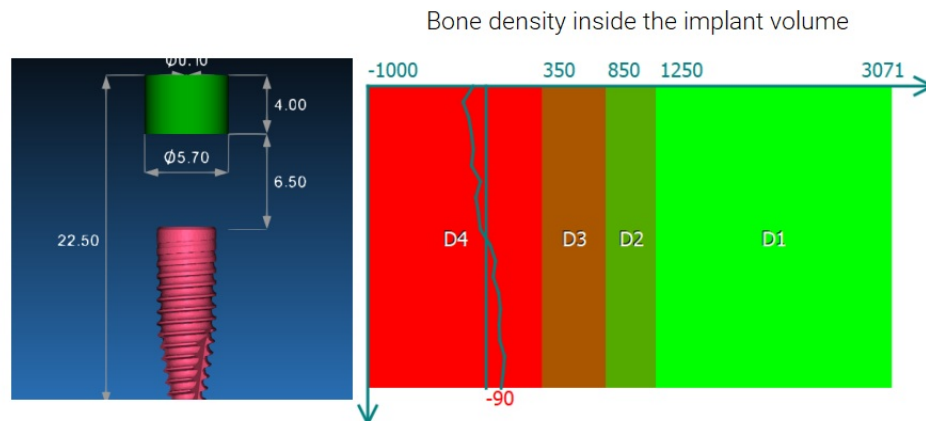

Notes:
 Sleeve Changed

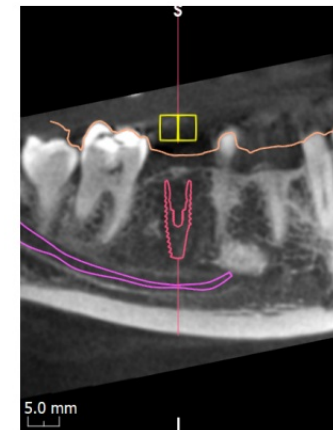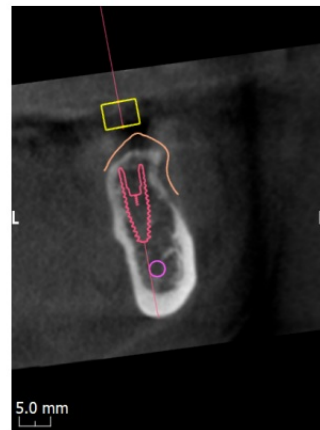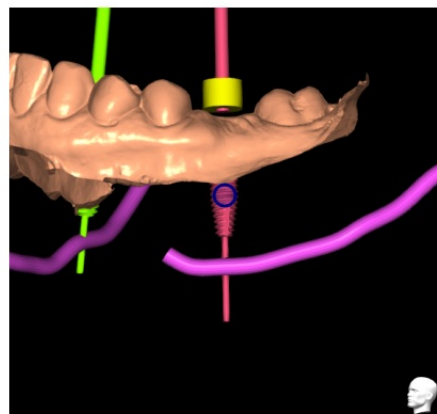

Position	Manufacturer	Model	Size	Abutment	Abutment size	Sleeve	Sleeve top height
47	Straumann	BLT SLA	RC 4.8 x 8 mm [021.7508]			Hiossen Parametric_OneGuide - D 5.7 mm Closed	10.50 mm

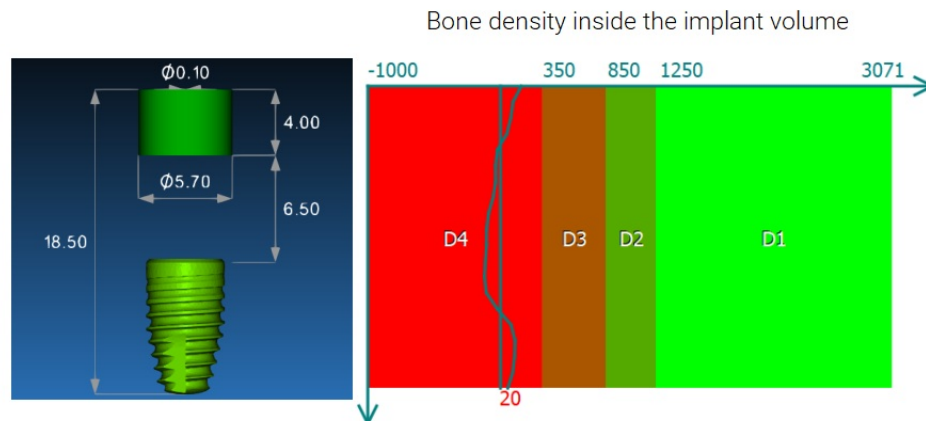

Notes:
 Sleeve Changed

