WATO EX-35(KG-)

Anesthesia Machine

Parts

MINDRAY CONFIDENTIAL

MINDRAY CONFIDENTIAL

Contents

1 Parts..... 4

1.1 WATO EX-35 Main Unit..... 4

1.1.1 Exploded View..... 4

1.1.2 Parts List..... 4

1.2 Gas bench receptacle assembly..... 5

1.2.1 Exploded View..... 5

1.2.2 Parts List..... 5

1.3 Liquid collection bottle assembly..... 6

1.3.1 Exploded View..... 6

1.3.2 Parts List..... 6

1.4 AGSS assembly..... 7

1.4.1 Exploded View..... 7

1.4.2 Parts List..... 7

1.5 Work table assembly..... 8

1.5.1 Exploded View..... 8

1.5.2 Parts List..... 8

1.6 Vaporizer bracket assembly..... 9

1.6.1 Exploded View..... 9

1.6.2 Parts List..... 9

1.7 Hardware box assembly..... 10

1.7.1 Exploded View..... 10

1.7.2 Parts List..... 10

MINDRAY CONFIDENTIAL

1.8 Flow meter and pressure gauge panel assembly.....12

1.8.1 Exploded View.....12

1.8.2 Parts List.....12

1.9 Display assembly.....14

1.9.1 Exploded View.....14

1.9.2 Parts List.....14

1.10 Gas supply inlet assembly.....15

1.10.1 Exploded View.....15

1.10.2 Parts List.....15

1.11 Main body of the patient circuit.....17

1.11.1 Exploded View.....17

1.11.2 Parts List.....17

1.12 Lifting device.....19

1.12.1 Exploded View.....19

1.12.2 Parts List.....19

1.13 Sodalime canister assembly.....20

1.13.1 Exploded View.....20

1.13.2 Parts List.....20

1.14 Others.....21


MINDRAY CONFIDENTIAL

MINDRAY CONFIDENTIAL

1 Parts

1.1 WATO EX-35 Main Unit

1.1.1 Exploded View

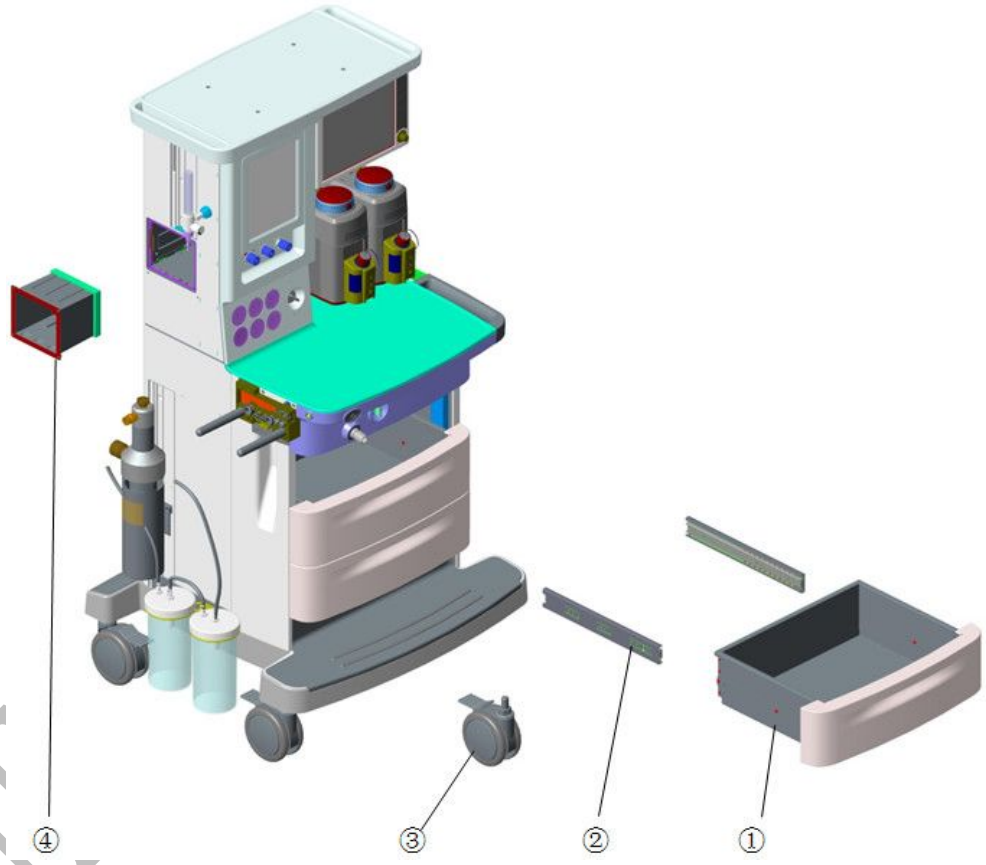

1.1.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	115-025663-00	drawer assembly(0625)	3	Only one in each

				115-025663-00
2	031-000041-00	ball guided.3flod 350mm blue zinc-plated	6	Only one in each 031-000041-00
3	801-0616-00036-00	Caster with brake	4	Only one in each 801-0616-00036-00
4	115-036995-00	Gas bench configure upgrade kit(0619)	1	/

MINDRAY CONFIDENTIAL

1.2 Gas bench receptacle assembly

1.2.1 Exploded View

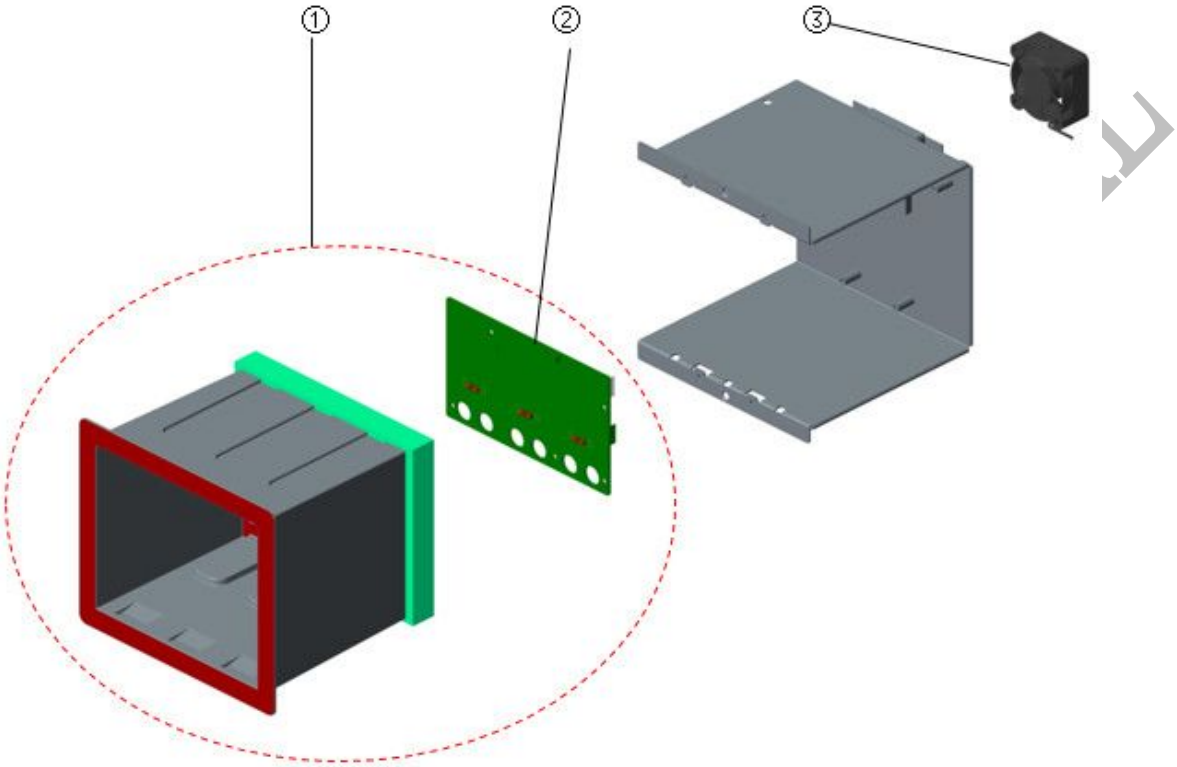


1.2.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	115-016480-00	gas bench receptacle assembly	1	/
2	801-0621-00165-00	0621 Infrared Communication Board	1	/
3	024-000407-00	FAN 12V 40*40*20mm 6.3CFM 18dB typeF	1	/

1.3 Liquid collection bottle assembly

1.3.1 Exploded View

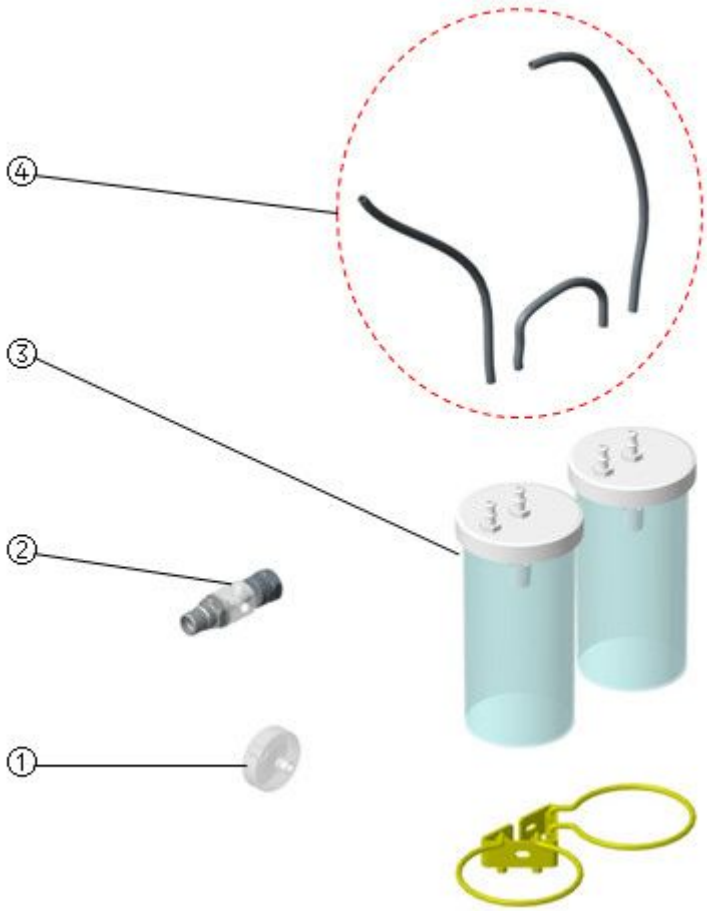

1.3.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	082-001327-00	Disposable Filter.0.45μm	1	/
2	115-020572-00	Suction T-joint air(NIST)check valve	1	/
3	040-001532-00	Vacuum flask	1	w/ overflow protection

	040-001533-00	Vacuum flask(no protection)		w/o overflow protection
	040-001659-00	collecting bottle		w/ overflow protection, icon is printed on the side
4	040-001658-00	tube.pvc	1	/

1.4 AGSS assembly

1.4.1 Exploded View



1.4.2 Parts List

No.	Order Number	Part Description	Qt	Remarks


MINDRAY CONFIDENTIAL

			y	
1	115-042912-00	AGSS 3 ways connector assembly	1	/
2	801-0631-00074-00	AGSS Transfer Tube	1	/

MINDRAY CONFIDENTIAL

1.5 Work table assembly

1.5.1 Exploded View

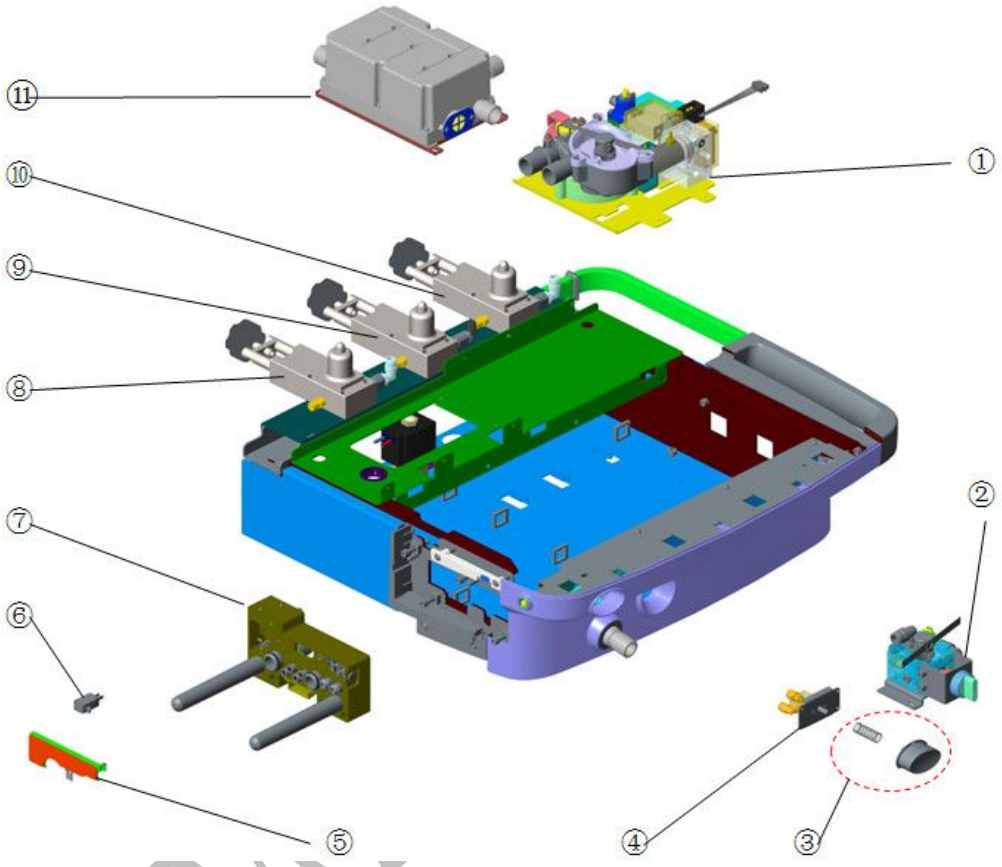

1.5.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	115-011265-01	Ventilation valve assembly(0616)	1	/
2	115-061227-00	mechanical ACGO assembly(0625)	1	/
3	115-037147-00	O2 flush button service kit(0619/0625)	1	/
4	801-0613-00026-00	O2 flush switch assembly	1	/
5	024-000185-00	BC heater for 0616	1	/

6	801-0613-00055-00	Snap action switch (rolling type 200gf)	1	/
7	115-006653-00	assembly of block(No ACGO/No bypass)	1	/
	115-006652-00	assembly of block(No ACGO/bypass)		/
8	115-002250-01	Cylinder Bracket for O2	1	w/ regulator
9	115-002251-02	Cylinder Bracket for N2O(Φ6)	1	w/ regulator
10	115-002728-01	Cylinder Bracket for AIR	1	w/ regulator
11	115-032992-00	Gas reservoir assembly(0625)	1	/

MINDRAY CONFIDENTIAL

1.6 Vaporizer bracket assembly

1.6.1 Exploded View

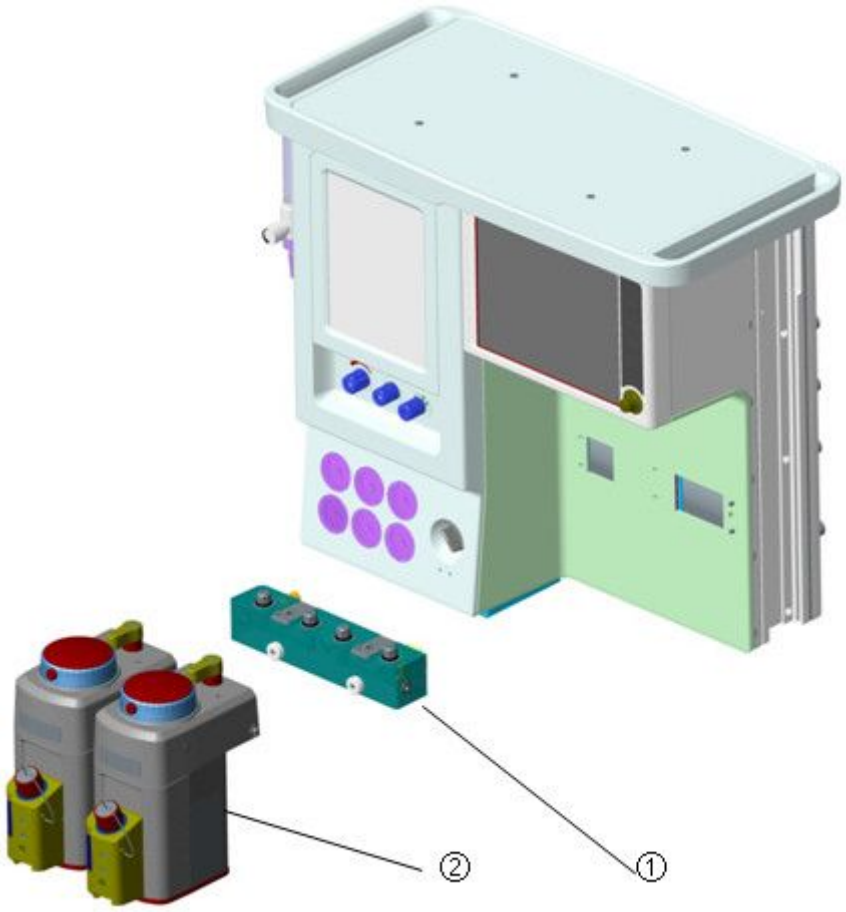

1.6.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	115-030766-00	Single vaporizer assembly(0625)	1	/
	115-032993-00	double vaporizer assembly(0625)		/
	115-017631-00	vaporizer bracket package		/
	115-027692-00	D-vaporizer assembly(plug-in)(0635)		/

2	0621-30-78720	5% Isoflurane Vaporizer(Pour fill)	1	/
	115-005349-00	Sevoflurane Pour Fill Vaporizer		/
	0621-30-78727	5% Isoflurane Vaporizer(Keyed filler)		/
	115-002355-00	8% Sevoflurane Vaporizer(Keyed filler)		/

MINDRAY CONFIDENTIAL

1.7 Hardware box assembly

1.7.1 Exploded View

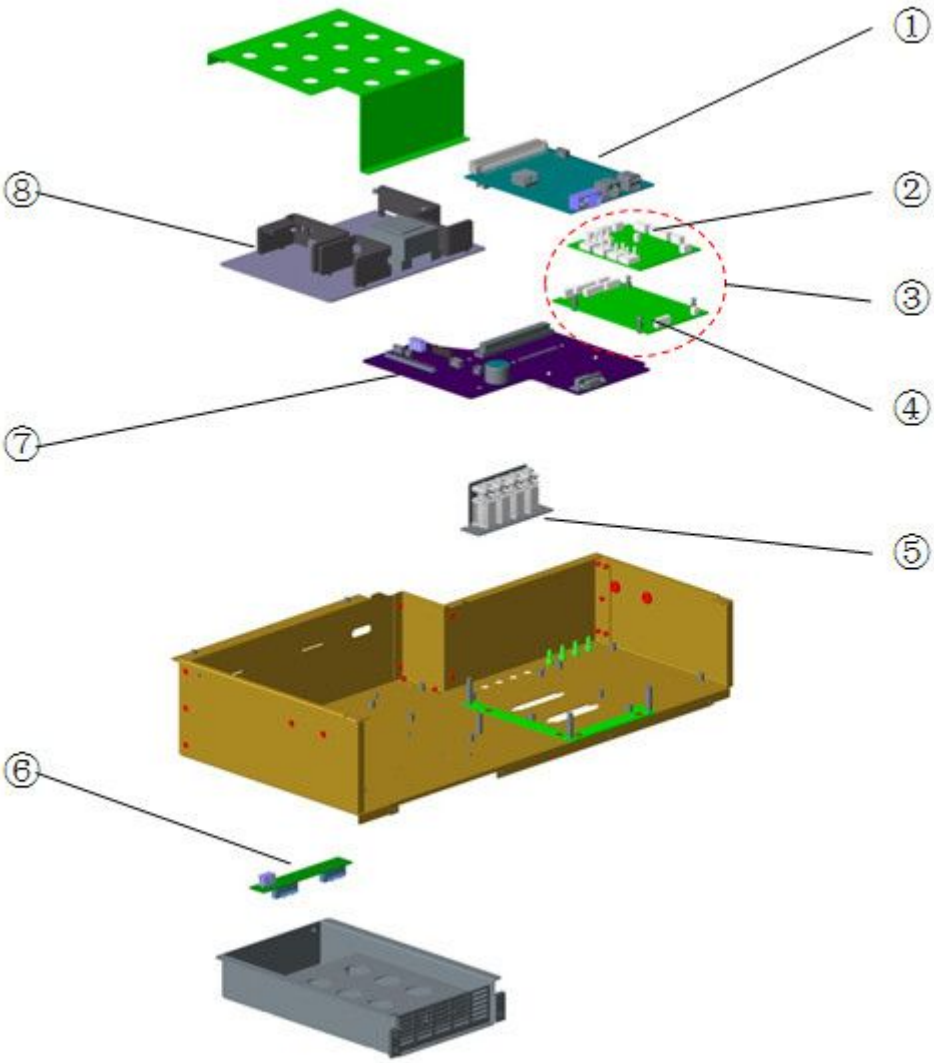

1.7.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	115-043755-00	0619 main control board FRU	1	Factory configuration support VCV mode only. If you want the board support the same

				function with your AM, please provide Machine ID and Function configuration when make Order.
	115-036951-00	0619 main control board FRU(VCV+PCV)		With VCV+PCV mode
2	051-003167-00	0625 Ventilation&Control PCBA	1	Old type, monitoring sensor's nozzle is metal. Compatible with 115-066429-00
	115-066429-00	0625 Ventilation&Control PCBA FRU		New type, monitoring sensor's nozzle is black. Compatible with 051-003167-00
3	115-066431-00	0619 Monitor PCBA FRU	1	115-066429-00+051-002364-00
4	051-002364-00	0619 Ventilater&Protect PCBA(Parker)	1	/
5	115-042876-00	three way valve asm(0625)	1	3 piece of valves, for machine w/o ACGO
	115-042877-00	three way valve asm(0625)		4 piece of valves, for machine w/ ACGO
6	051-000768-00	0623 battery board PCBA	1	/
7	051-002165-00	0619 Mother Board PCBA	1	/
8	051-003469-00	0625 Power board PCBA	1	/

MINDRAY CONFIDENTIAL

1.8 Flow meter and pressure gauge panel assembly

1.8.1 Exploded View

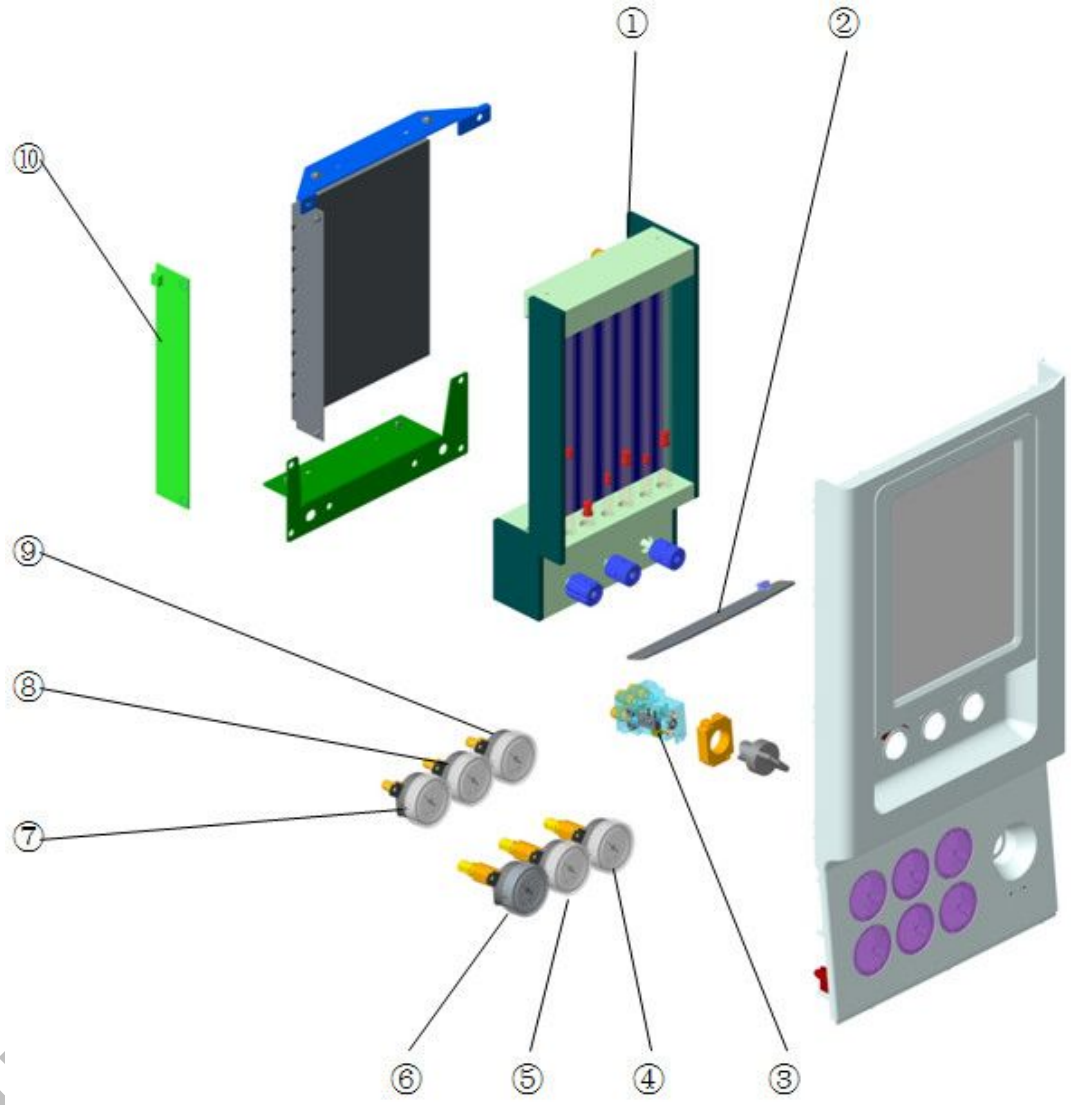

1.8.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	115-036955-00	flowmeter FRU (O2/Air,EU)	1	/
	115-036956-00	flowmeter FRU (O2/N2O,EU)		/


	115-036957-00	flowmeter FRU (O2/N2O/Air,EU)		/
	115-036958-00	flowmeter FRU (O2/Air,US)		/
	115-036959-00	flowmeter FRU (O2/N2O,US)		/
	115-036960-00	flowmeter FRU (O2/N2O/Air,US)		/
	115-036961-00	flowmeter FRU (O2/N2O,Reverse_EU)		/
	115-036962-00	flowmeter FRU (O2/N2O/Air,Reverse_EU)		/
2	051-002386-00	0619 auxiliary lighting board PCBA	1	/
3	801-0611-00044-00	O2&Air system switch	1	for machine w/ O2&Air supply
	801-0613-00021-00	SYSTEM SWITCH		for machine w/o Air supply
4	115-035357-00	High pressure gauge assembly(Air/0619)	1	/
5	115-035358-00	High pressure gauge assembly(N2O/0619)	1	/
6	115-035356-00	High pressure gauge assembly(O2/0619)	1	/
7	115-035353-00	Pressure gauge assembly(O2/0619)	1	/
8	115-035355-00	Pressure gauge assembly(N2O/0619)	1	/
9	115-035354-00	Pressure gauge assembly(Air/0619)	1	/
10	051-000040-00	Flow Meter Lighting Board PCBA	1	/

MINDRAY CONFIDENTIAL

MINDRAY CONFIDENTIAL

1.9 Display assembly

1.9.1 Exploded View

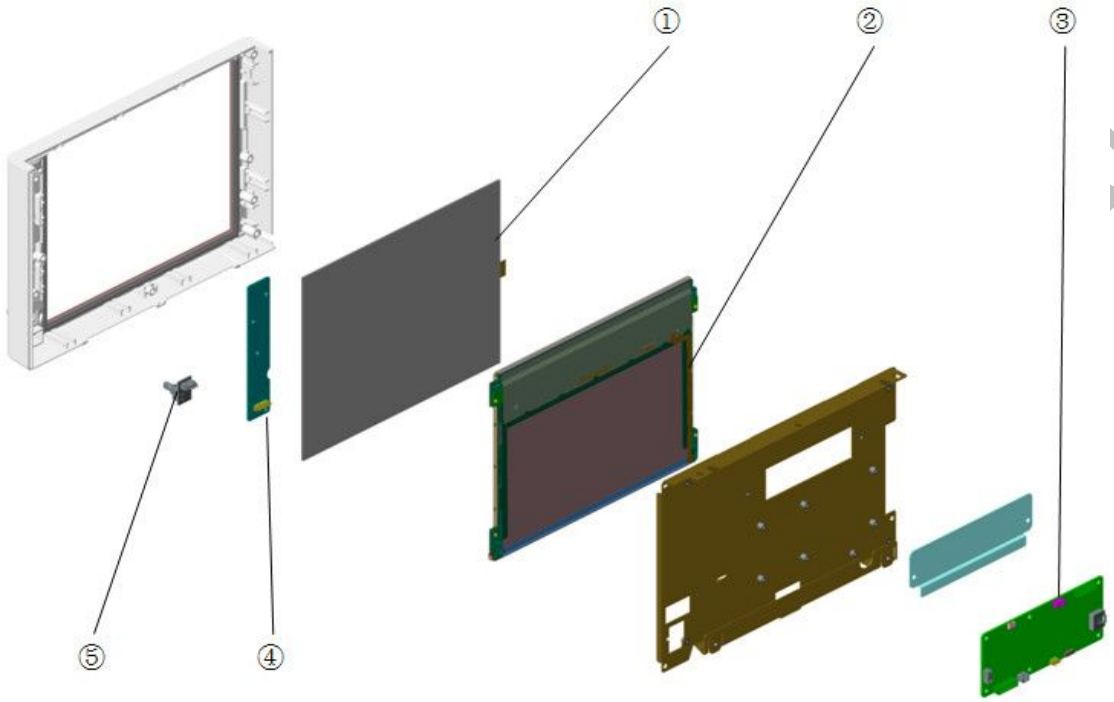


1.9.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	021-000221-00	Touch Panel Five wire 10.4" Narrow Frame	1	/
2	021-000171-00	LCD TFT 10.4" 1024*768 3.3V LED-BL	1	/
3	051-002365-00	0619 Keypad Control Board PCBA	1	/
4	051-002163-00	0619 Key and Alarm Light Board PCBA	1	/
5	801-0613-00035-00	Encoder(FRU)	1	/

MINDRAY CONFIDENTIAL

1.10 Gas supply inlet assembly

1.10.1 Exploded View

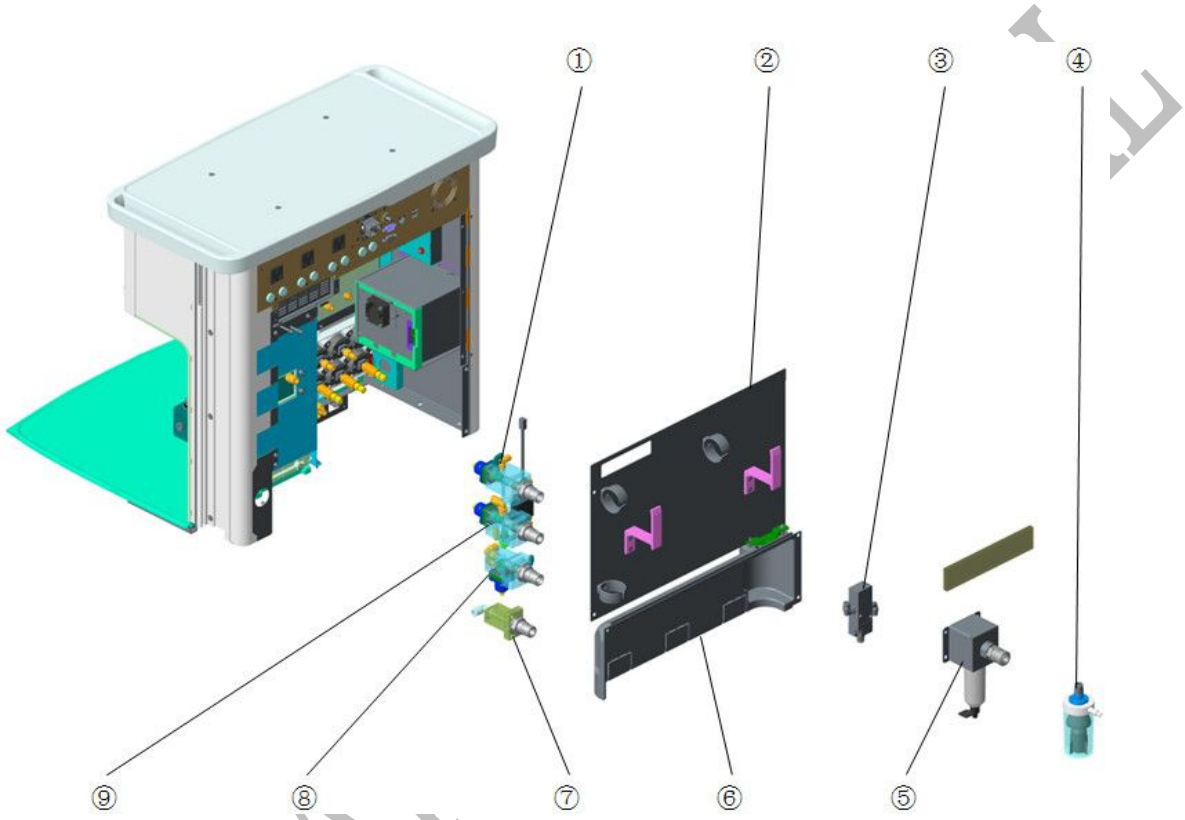

1.10.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	115-033838-01	N2O supply inlet assembly(0615)	1	NIST
	115-034149-01	N2O supply inlet assembly	1	DISS
2	115-030690-00	backcover assembly(0619)	1	/
3	082-001231-00	valve.2-way,air-piloted valves	1	O2-N2O block valve
4	115-018131-00	Overflow Unit	1	/

5	115-048529-00	Air filter (F92G2VNQT1)	1	Only for Air-compressor configuration.
6	115-025552-00	Rear Cover Assembly	1	/
7	115-034706-01	Backup O2 assembly(0615)	1	/
8	115-033837-01	Air supply inlet assembly(0615)	1	NIST
	115-035360-01	Air supply inlet assembly(NIST/0619)	1	w/ pressure switch
	115-034150-01	AIR supply inlet assembly	1	DISS
	115-035359-01	Air supply inlet assembly(DISS/0619)	1	w/ pressure switch
9	115-033836-01	O2 supply inlet assembly(0615)	1	NIST
	115-034148-01	O2 supply inlet assembly	1	DISS

MINDRAY CONFIDENTIAL

1.11 Main body of the patient circuit

1.11.1 Exploded View

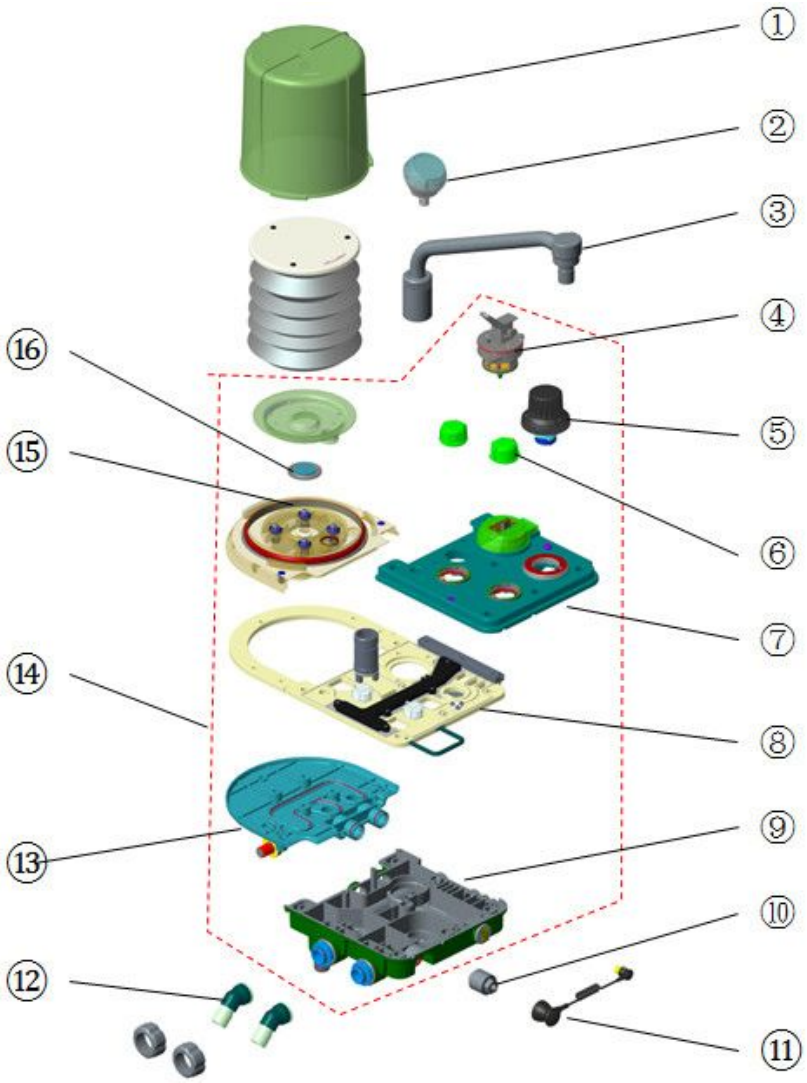

1.11.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	801-0631-00054-00	Bellows Dome A series	1	/

2	115-034210-00	Airway pressure gauge	1	/
3	115-048600-00	Bag arm assembly(silvery/spacing)	1	W/ position limit, refer to TMZ-17026
	801-0601-00005-00	Bag arm assembly		W/O position limit, refer to TMZ-17026
4	801-0601-00017-00	Bag/mechanical ventilation switch	1	/
5	801-0621-00168-00	(New) APL Valve assembly(FRU)	1	Machine before Oct 2017, refer to TMZ-17026
	115-046754-00	APL valve FRU		Machine after Oct 2017, refer to TMZ-17026
6	801-0631-00061-00	Check valve dome A series	2	w/ Seal(O-ring). Only one check valve dome in each 801-0631-00061-00
7	115-034979-00	upper cover assembly FRU	1	Seals and screws are included
8	115-048640-00	mid-plate assembly(0625/prepak)FRU	1	For prepak canister
	115-048642-00	mid-plate assembly(heat/arm)(0619)FRU		For non-prepak canister. Seals are included
9	115-034980-00	lower cover assembly(bag arm)FRU	1	Seals and screws are included
10	0611-10-45654	O2 sensor MedicelMOX-2	1	/


MINDRAY CONFIDENTIAL

	040-000898-00	sensor oxygen		O2 sensor with translucent shell
11	0601-20-78941	O2 sensor cable	1	/
12	801-0631-00057-00	Insp/Exp Connector A series	2	Only connector in each 801-0631-00057-00
13	115-034190-00	lower cover 2 assembly(0615)	1	Seals and screws are included
14	115-034909-00	Circuit main unit(heat/bag arm)	1	For non-prepak canister(spiral interface)
	115-048843-00	patient main unit		For prepak canister
	115-037183-00	Circuit main unit FRU(heat/bag arm/0619)		For non-prepak canister(lifting)
15	115-034189-00	upper cover 2 assembly(0615)	1	Seals and screws are included
16	801-0601-00002-00	Pop-off valve assembly	1	/

MINDRAY CONFIDENTIAL

1.12 Lifting device

1.12.1 Exploded View

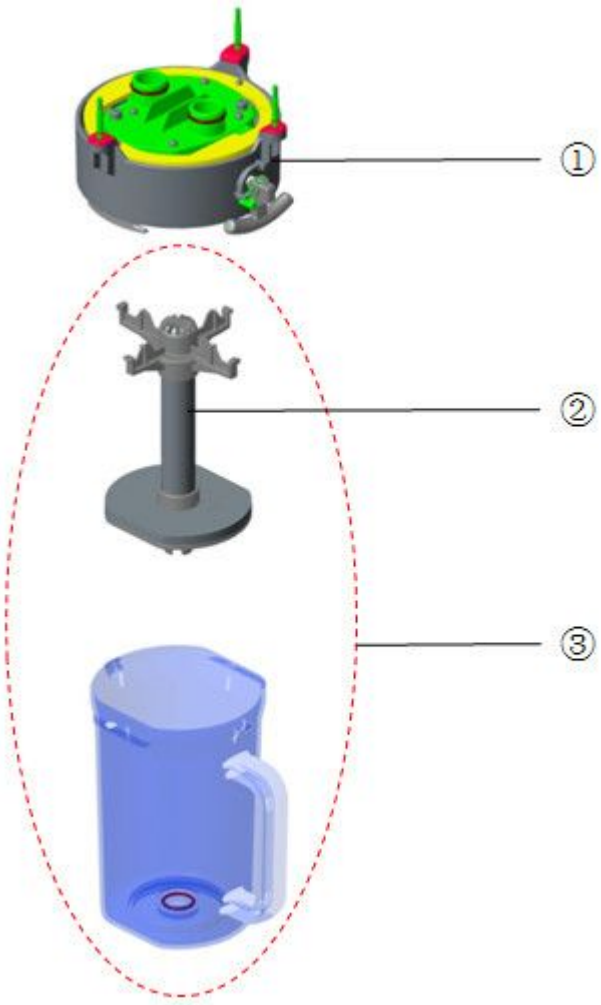

1.12.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	115-034208-00	Lifting device(with bypass/0615)	1	The whole lifting device
2	115-034689-00	Absorb canister shore(0625)	1	/

3	115-030838-00	Canister assembly(0625)	1	/

MINDRAY CONFIDENTIAL

1.13 Sodalime canister assembly

1.13.1 Exploded View

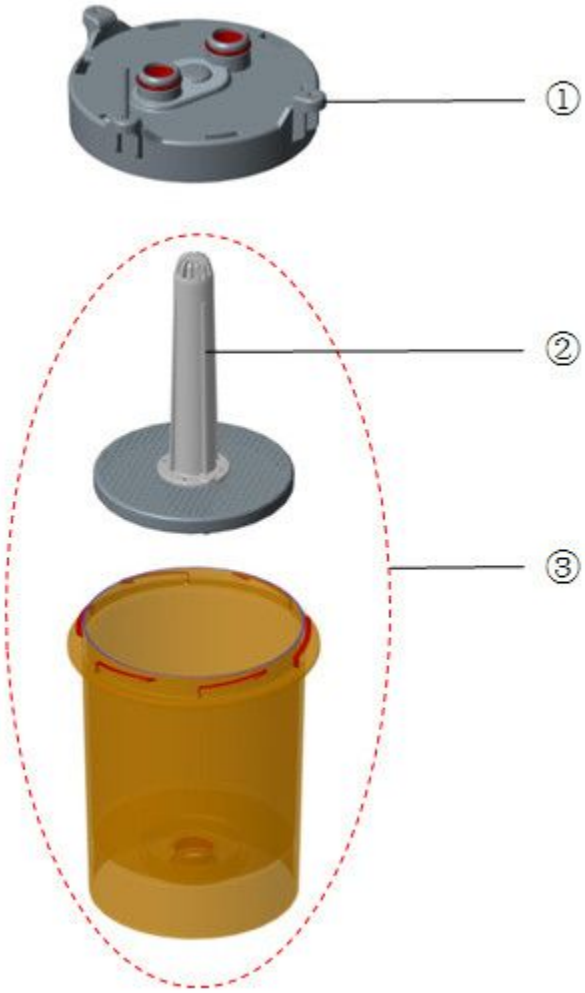

1.13.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	115-034193-00	Canister upper cover assembly(20B)	1	/
2	115-036950-00	Absorber caniste support module FRU(20B)	1	/

3	115-034194-00	Sodalime canister assembly(20B)	1	/

MINDRAY CONFIDENTIAL

1.14 Others

No.	Order Number	Part Description	Qty	Remarks
1	115-036966-00	USB flash memory(SIMV-VC+SIMV-PC)	1	Need to provide machine's SN and machine ID
2	115-033012-00	USB flash memory(PS)	1	Need to provide machine's SN and machine ID
3	115-033014-00	USB flash memory(Loop)	1	Need to provide machine's SN and machine ID
4	115-024461-00	Support arm kit(0634)	1	Mechanical arm, mounted to GCX compatible rail system to fix tube
5	115-035836-00	pendant adapter package(no_sup_cylinder)	1	/
6	115-021015-00	Accessory hook kit(0632)	1	/
7	801-0601-00008-00	Inspiratory/Expiratory flow sensors	1	/
8	115-036963-00	Maintain Kit(0619,Basic,1 yr)	1	No need to replace spiral canister's seal, since this seal is not FRU.
9	115-036964-00	Maintain Kit(0619,Extend,1yr)	1	No need to replace spiral canister's seal, since this seal is not FRU.
10	115-036965-00	Maintain Kit(0619,Advanced,1 yr)	1	No need to replace spiral canister's seal, since this seal is not FRU.
11	115-034694-00	Maintain Kit(0625,Basic,1 yr/Prepark)	1	For prepak canister

MINDRAY CONFIDENTIAL

12	115-034696-00	Maintain Kit(0625,Extend,1yr/Prepark)	1	For prepak canister
13	115-034698-00	Maintain Kit(0625,Advanced,1 yr/Prepark)	1	For prepak canister
14	115-051201-00	0619 Ventilation kit FRU(O2 Drive)	1	115-066431-00(0619 Monitor PCBA FRU) and 115-011265-01(Ventilation valve assembly(0616)) are included
15	115-051202-00	0619 Ventilation kit FRU(Air Drive)	1	115-066431-00(0619 Monitor PCBA FRU) and 115-011265-01(Ventilation valve assembly(0616)) are included
16	115-018429-00	suction tube kit(inner suction)	1	/
17	115-035676-00	Auxiliary O2 Package(0619)	1	Upgrade kit for auxiliary O2 supply
18	115-018012-00	Li-ion Bat Pack (11.1V4500mAh LI23S002A)	1	/
19	801-0631-00132-00	Power Socket 3C (black)(FRU)	1	rear cover
20	801-0631-00028-00	Fan	1	rear cover
21	051-001866-00	0625 toplight board PCBA	1	under screen
22	801-0631-00038-00	Speaker and Connecting Cable	1	/
23	115-002015-00	AGSS passive scavenging tube assembly	1	/
24	082-001372-00	AGSS receiving hosing(35G-WAGD-DS/FG2-3)	1	/
25	115-009073-00	AGSS low-flow Receiving	1	/

MINDRAY CONFIDENTIAL

		hoses assembly		
26	115-020745-00	AGSS connector package(UK)	1	/
27	040-000065-00	Keyed Fill Adaptor for Isoflurane 53453	1	/
28	040-000066-00	Keyed Fill Adaptor for Sevoflurane 53454	1	/
29	115-036182-00	Medicine filler sleeve(0605) FRU	1	/
30	115-036167-00	Filler cap FRU	1	/
31	115-039569-00	Filler cap of ENF(Pour Fill)	1	/
32	115-039571-00	Filler cap of ISO(Pour Fill)	1	/
33	115-039572-00	Filler cap of SEV(Pour Fill)	1	/
34	115-039573-00	Filler cap of SEV(Quik-Fil)	1	/
35	115-039574-00	Filler cap of Hal(Pour Fill)	1	/
36	034-000353-00	Drawer lock	1	/
37	803-011648-00	WATO EX-35 main unit warranty	1	/
38	115-033063-00	gas cylinder wrench assembly	1	/
39	801-0613-00051-00	Gas pressure switch	2/3	There are 2 pressure switches in O2 supply inlet assembly and Ventilation valve assembly. Whether Air supply inlet have 1 pressure switch is depended on AM configuration. Only one pressure switch in each 801-0613-00051-00

MINDRAY CONFIDENTIAL

MINDRAY CONFIDENTIAL