WATO EX-20&30(DW-&DY-)

Anesthesia Machine

Parts

MINDRAY CONFIDENTIAL

MINDRAY CONFIDENTIAL

Contents

1 Parts..... 4

1.1 Main Unit..... 4

1.1.1 Exploded View..... 4

1.1.2 Parts List..... 4

1.2 Flow Meter Assembly..... 6

1.2.1 Exploded View..... 6

1.2.2 Parts List..... 6

1.3 Pressure Gauge Assembly..... 8

1.3.1 Exploded View..... 8

1.3.2 Parts List..... 8

1.4 Work Table..... 10

1.4.1 Exploded View..... 10

1.4.2 Parts List..... 10

1.5 Top Plate Assembly..... 13

1.5.1 Exploded View..... 13

1.5.2 Parts List..... 13

1.6 Hardware Box I..... 14

1.6.1 Exploded View..... 14

1.6.2 Parts List..... 14

1.7 Hardware Box II..... 16

1.7.1 Exploded View..... 16

1.7.2 Parts List..... 16

MINDRAY CONFIDENTIAL

1.8 Display Assembly.....17
1.8.1 Exploded View.....17
1.8.2 Parts List.....17
1.9 Upper Half.....19
1.9.1 Exploded View.....19
1.9.2 Parts List.....19
1.10 Auxiliary Output Assembly.....23
1.10.1 Exploded View.....23
1.10.2 Parts List.....23
1.11 Isolation Transformer Assembly.....24
1.11.1 Exploded View.....24
1.11.2 Parts List.....24
1.12 Heating Control Assembly.....25
1.12.1 Exploded View.....25
1.12.2 Parts List.....25
1.13 Liquid Collection Bottle Assembly.....26
1.13.1 Exploded View.....26
1.13.2 Parts List.....26
1.14 Main Body of the Patient Circuit.....27
1.14.1 Exploded View.....27
1.14.2 Parts List.....27
1.15 Check Valve Assembly.....30
1.15.1 Exploded View.....30
1.15.2 Parts List.....30

MINDRAY CONFIDENTIAL


1.16 Lifting Device Assembly..... 31
1.16.1 Exploded View..... 31
1.16.2 Parts List..... 31
1.17 Sodalime Canister Assembly..... 33
1.17.1 Exploded View..... 33
1.17.2 Parts List..... 33
1.18 Others..... 34

MINDRAY CONFIDENTIAL

1 Parts

1.1 Main Unit

1.1.1 Exploded View

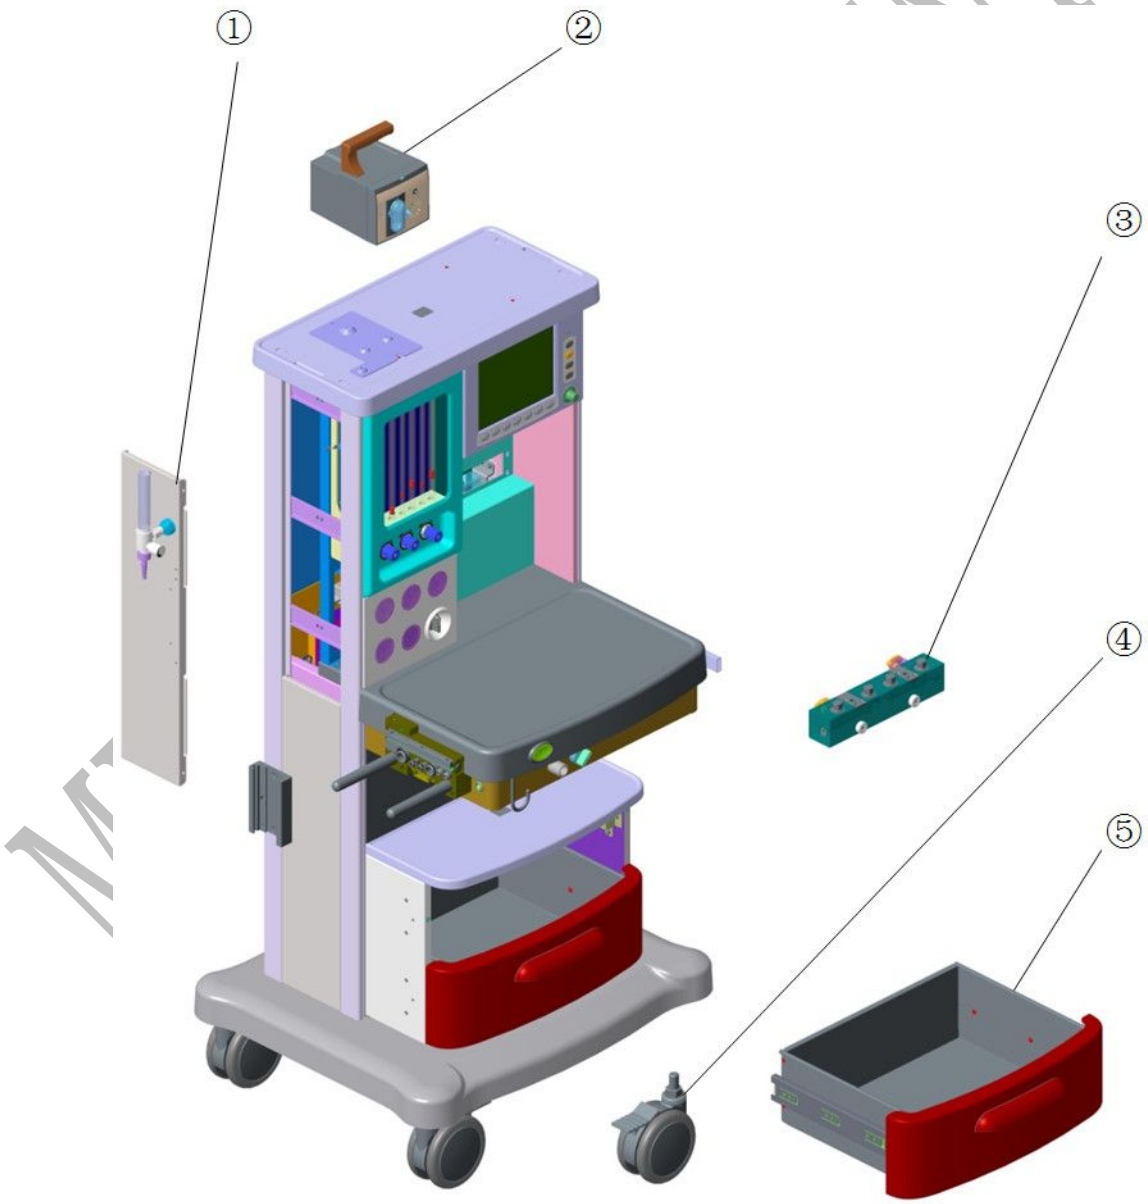


1.1.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	115-002606-00	Auxiliary Gas Outlet Assembly	1	/
2	801-0616-00043-00	Case for CO2 module (FRU)	1	/
3	801-0616-00008-00	Manifold for single-vaporizer	1	/
	801-0616-00009-00	Manifold for dual-vaporizer		/
	115-032600-00	Plug-in Upgrade kit(0616)		/
4	801-0616-00036-00	Caster with brake	4	Only one caster in each 801-0616-00036-00
5	801-0621-00051-00	Drawer	1	26cm height, used for single drawer configuration machine. Refer to TMZ-12012
	115-011667-00	assembly of drawer(0616)	2	15cm height, used for two drawers configuration machine. Refer to TMZ-12012. Only one drawer in each 115-011667-00

MINDRAY CONFIDENTIAL

1.2 Flow Meter Assembly

1.2.1 Exploded View

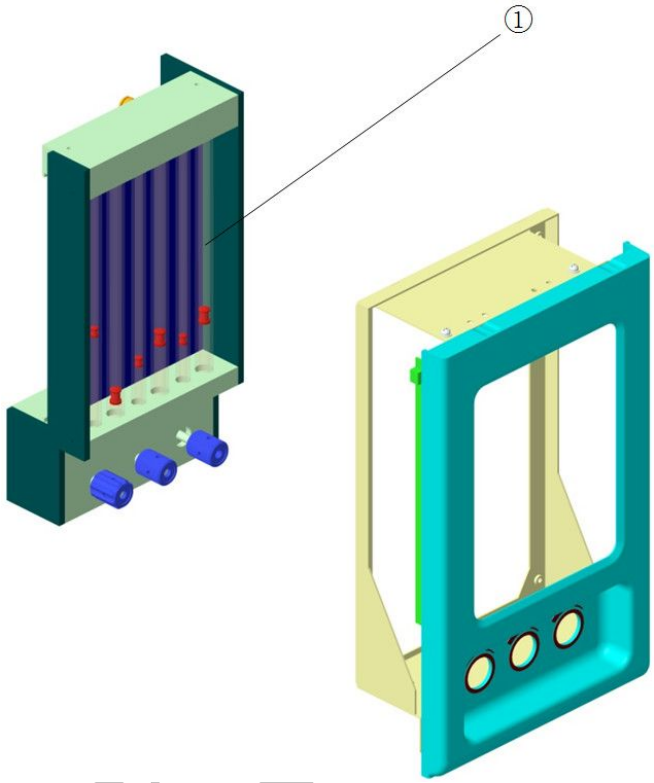

1.2.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	801-0616-00023-00	Flow meter(O2/IEC)	1	Only O2
	801-0616-00026-00	Flow meter(O2/US)		Only O2
	801-0616-00024-00	Flow meter(N2O, O2/IEC)		O2&N2O
	801-0616-00027-00	Flow meter(N2O,O2/US)		O2&N2O
	801-0616-00025-00	Flow meter(Air,N2O,O2/IEC		O2&N2O&Air


MINDRAY CONFIDENTIAL

		)		
	801-0616-00028-00	Flow meter(Air,N2O,O2 / US)		O2&N2O&Air
	115-016501-00	O2 & AIR flowmeter assembly(EN Standard)		O2&Air
	115-016500-00	O2 & AIR flowmeter assembly(US Standard)		O2&Air
	115-062672-00	Flow meter(Sri Lanka) (FRU)		O2&N2O&Air flowmeter assembly(EN Standard)(6 tubes), O2 minimum flow 0.25L/min. Only for EX-30 in Sri Lanka, Refer to TMZ-19013

MINDRAY CONFIDENTIAL

1.3 Pressure Gauge Assembly

1.3.1 Exploded View

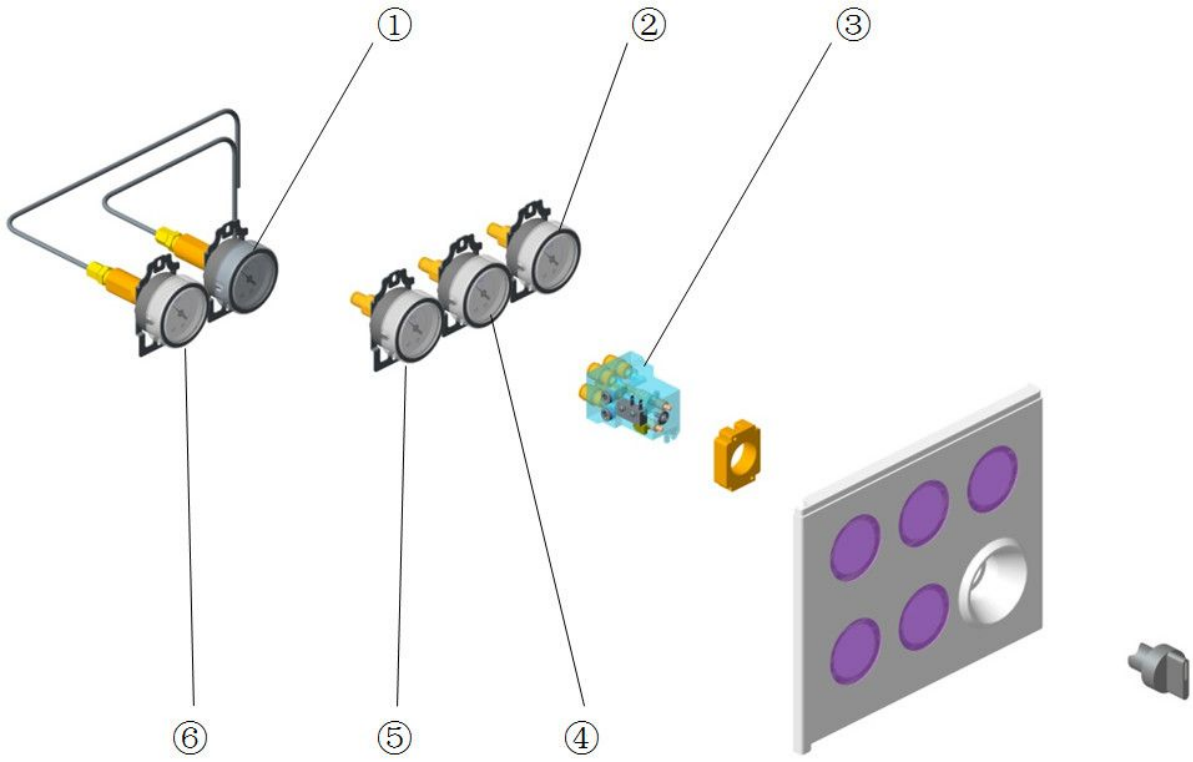

1.3.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	801-0616-00029-00	High Pressure Gauge Assembly(Right)	1	w/o O2/N2O/AIR label
	115-008975-01	high pressure gauge assembly,AIR		/
	115-008976-01	high pressure gauge assembly,N2O		/
2	115-009025-01	pressure gauge assembly,AIR	1	/

	801-0613-00005-00	Pipeline supply gauge		w/o O2/N2O/AIR label
3	801-0611-00044-00	O2&Air system switch	1	/
	801-0613-00021-00	SYSTEM SWITCH		Only O2
4	115-009026-01	pressure gauge assembly,N2O	1	/
	801-0613-00005-00	Pipeline supply gauge		w/o O2/N2O/AIR label
5	115-009024-01	pressure gauge assembly,O2	1	/
	801-0613-00005-00	Pipeline supply gauge		w/o O2/N2O/AIR label
6	801-0616-00030-00	High Pressure Gauge Assembly(Left)	1	w/o O2/N2O/AIR label
	115-008974-01	high pressure gauge assembly,O2		/

MINDRAY CONFIDENTIAL

1.4 Work Table

1.4.1 Exploded View

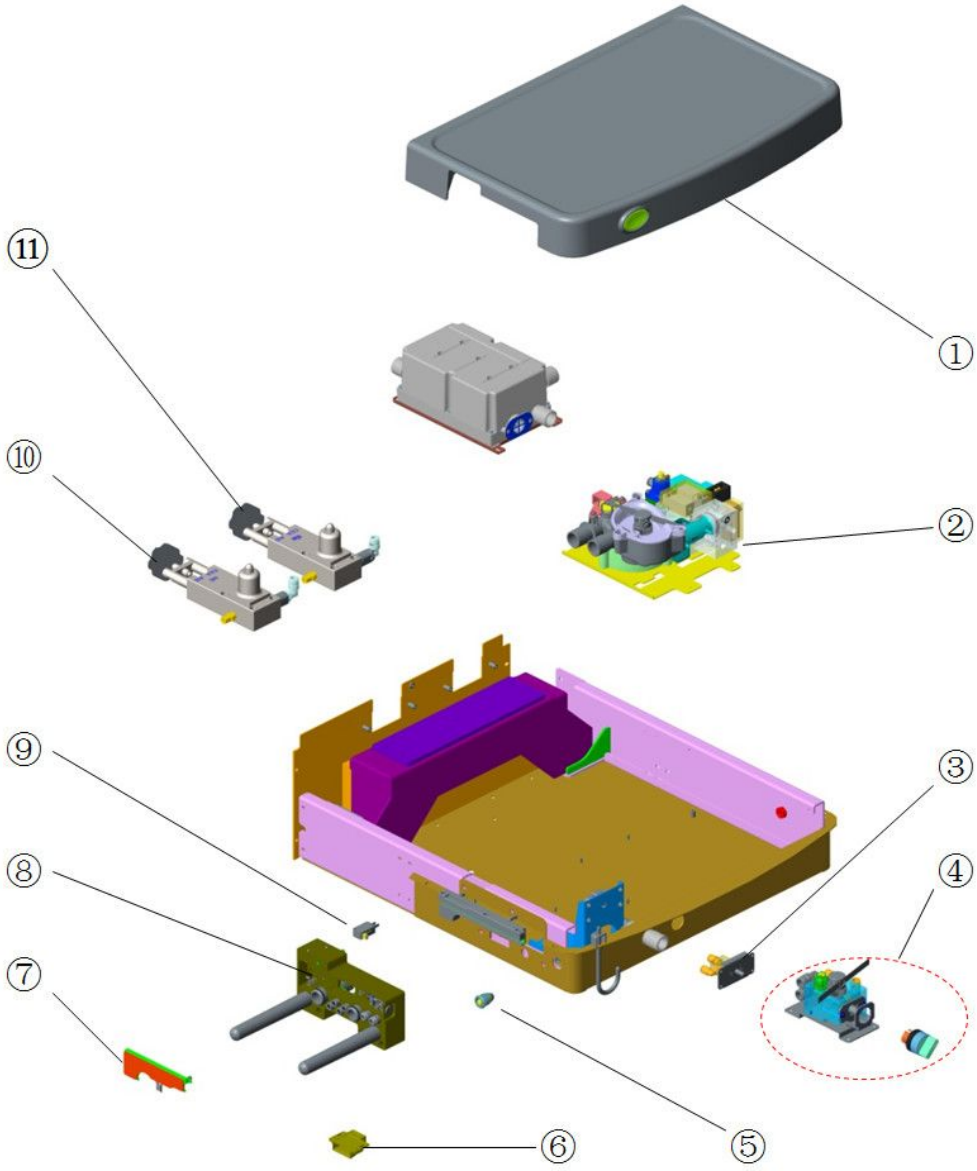

1.4.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	801-0616-00045-00	table cover	1	w/ O2 flush button

		assembly		
2	115-011265-01	Ventilation valve assembly(0616)	1	Proportional valve is Parker, main unit is black. Refer to: TMZ-15053, TMZ-15057
	115-034207-00	Ventilation valve(pressure switch)		Proportional valve is Parker, main unit is white. Refer to: TMZ-15053, TMZ-15057
	801-0621-00047-00	Breathing Valve Assembly		Proportional valve is Norgren, main unit is black
3	801-0611-00026-00	O2 flush button assembly	1	w/o O2 flush button
4	801-0616-00126-00	AGGO assembly(FRU new switch)	1	/
	801-0616-00128-00	ACGO update package,FRU		w/ tubes and fresh gas connector
5	801-0621-00154-00	2Pin Female Socket Assembly (FRU)	1	/
6	801-0613-00053-00	Lock with micro switch(FRU)	1	/
7	024-000185-00	BC heater for 0616	1	/
8	115-034171-00	BS block (ACGO/no bypass/0615)	1	/
	115-034170-00	BS block (no ACGO/no bypass/0615)		/


MINDRAY CONFIDENTIAL

9	801-0613-00055-00	Snap action switch (rolling type 200gf)	1	/
10	801-0616-00013-00	O2 cylinder yoke assembly	1	For machines before 2012.04. Refer to TMZ-12010
	115-002250-01	Cylinder Bracket for O2		For machines after 2012.04. Refer to TMZ-12010. Change to another PN in TMZ-16006, and then change back again in TMZ-16028.
11	115-015027-00	Cylinder Bracket for N2O(Φ6)	1	/
	801-0616-00032-00	Air cylinder yoke assembly		For machines before 2012.04. Refer to TMZ-12010
	115-002728-01	Cylinder Bracket for AIR		For machines after 2012.04. Refer to TMZ-12010. Change to another PN in TMZ-16006, and then change back again in TMZ-16028.

MINDRAY CONFIDENTIAL

1.5 Top Plate Assembly

1.5.1 Exploded View

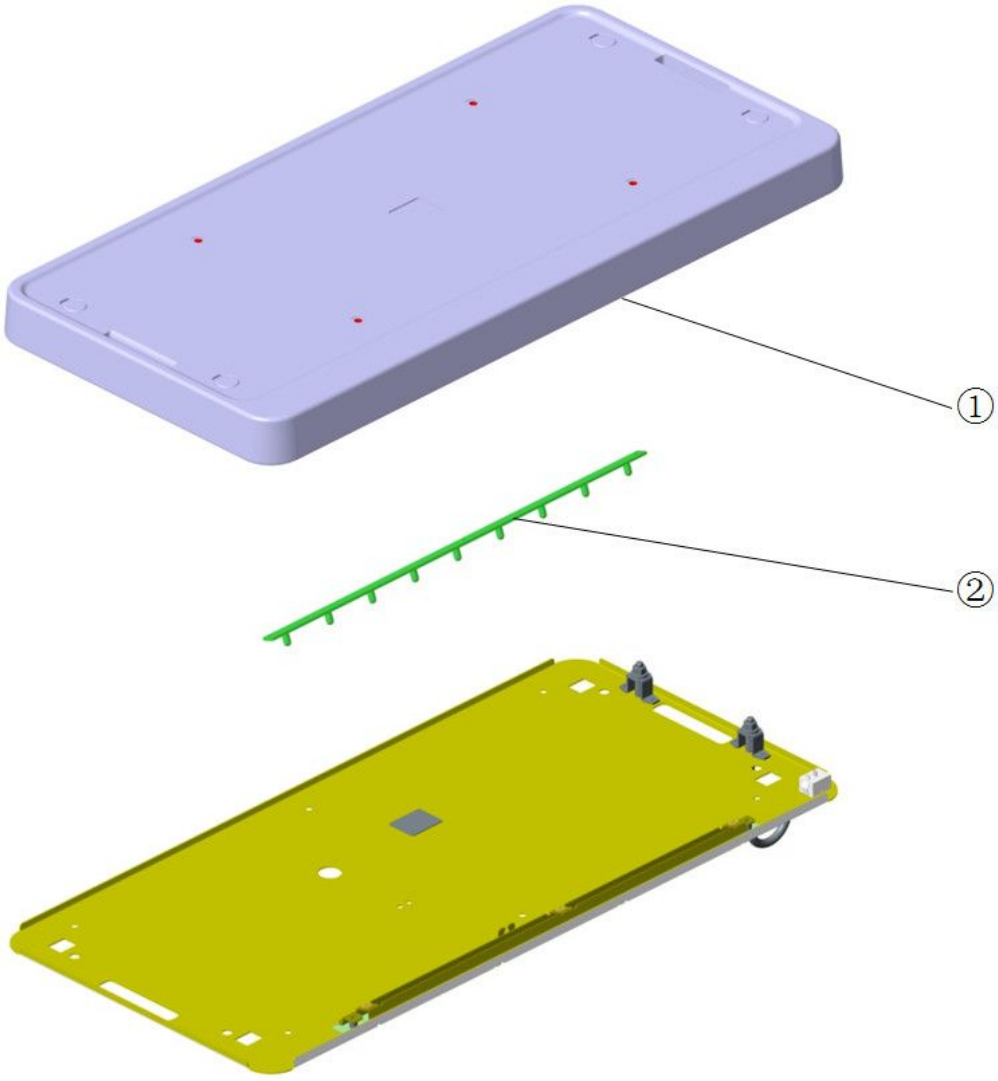


1.5.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	801-0616-00049-00	Top Plate Assembly(FRU) (0616)	1	/
2	801-0621-00026-00	Tabletop light board	1	/

MINDRAY CONFIDENTIAL

1.6 Hardware Box I

1.6.1 Exploded View

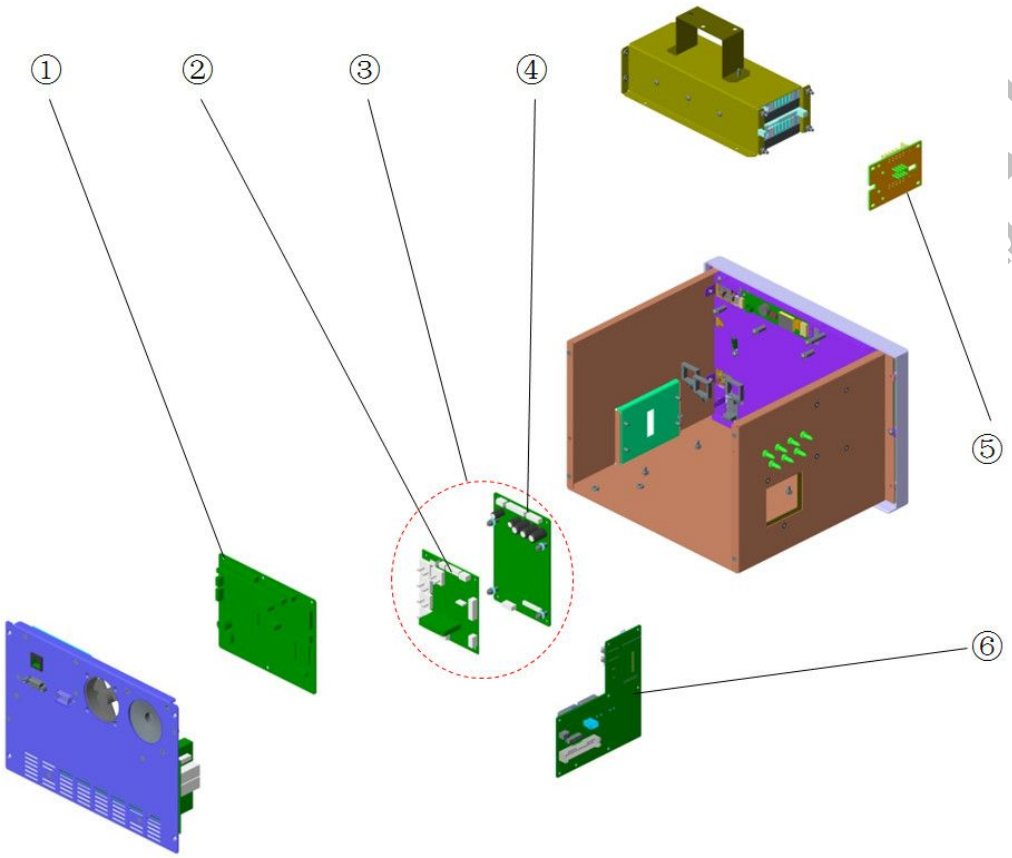

1.6.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	801-0615-00001-00	Main board (VCV, English,0615)	1	For WATO EX-20. Factory configuration support VCV mode only. If you want the board support the same function with your AM, please provide Machine ID and Function configuration when make Order.

	801-0617-00011-00	main board		For WATO EX-30. Factory configuration support VCV+PCV mode only. If you want the board support the same function with your AM, please provide Machine ID and Function configuration when make Order.
2	115-051193-00	Monitored signal detection board (FRU)	1	/
3	115-051195-00	Monitor board assembly	1	/
4	801-0616-00060-00	Drive Board for Monitoring Valve	1	/
5	801-0613-00041-00	lithium battery connection board	1	/
6	115-027184-00	power adapt board FRU	1	Include 024-000582-00

MINDRAY CONFIDENTIAL

1.7 Hardware Box II

1.7.1 Exploded View

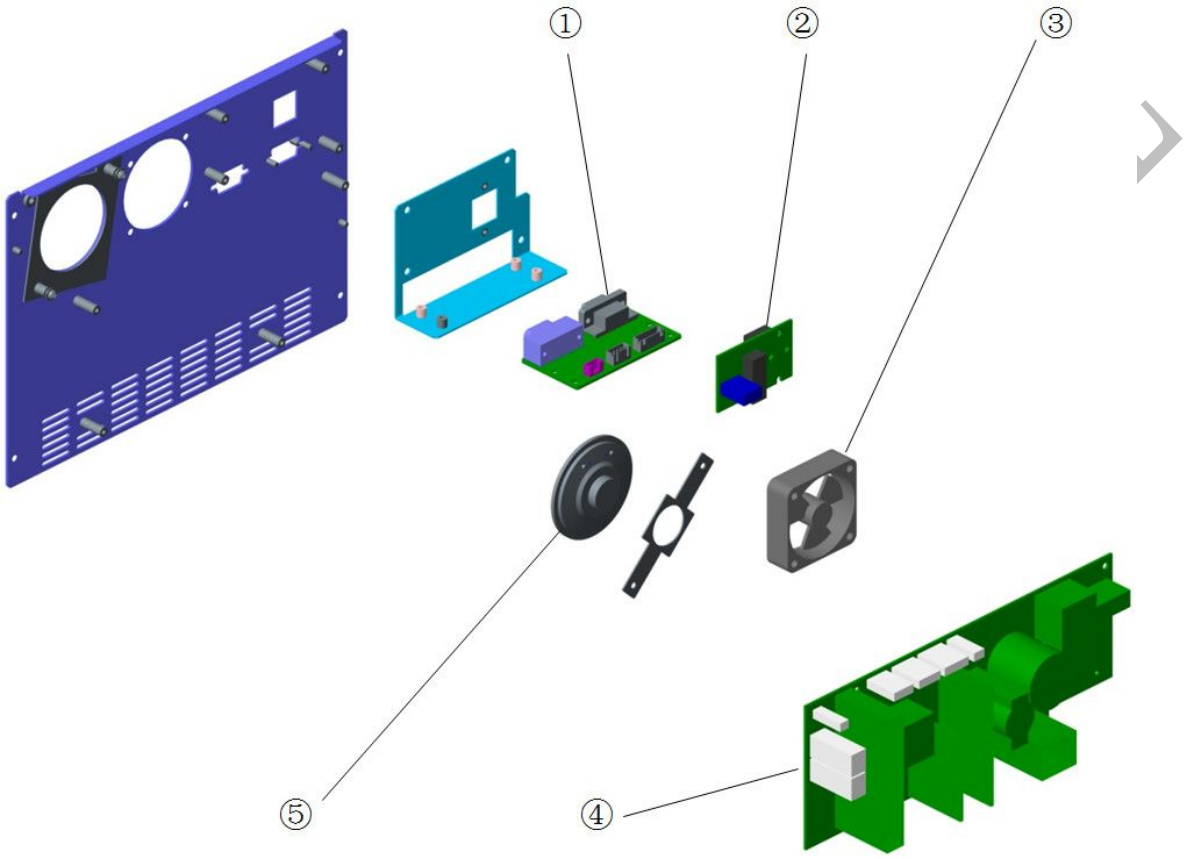

1.7.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	051-000961-00	0616 Calibrating and Communicating PCBA	1	/
2	9210-30-30152	Ntwrk pcb,PM7,8E,9E,MEC12vet	1	/
3	024-000582-00	FAN 12V 9.4CFM 20.1dB 50*50*15*355mm	1	Used in hardware box

4	801-0616-00058-00	0616power board	1	/
5	801-0621-00156-00	2.25 Speaker (w wire, FRU)	1	/

MINDRAY CONFIDENTIAL

1.8 Display Assembly

1.8.1 Exploded View

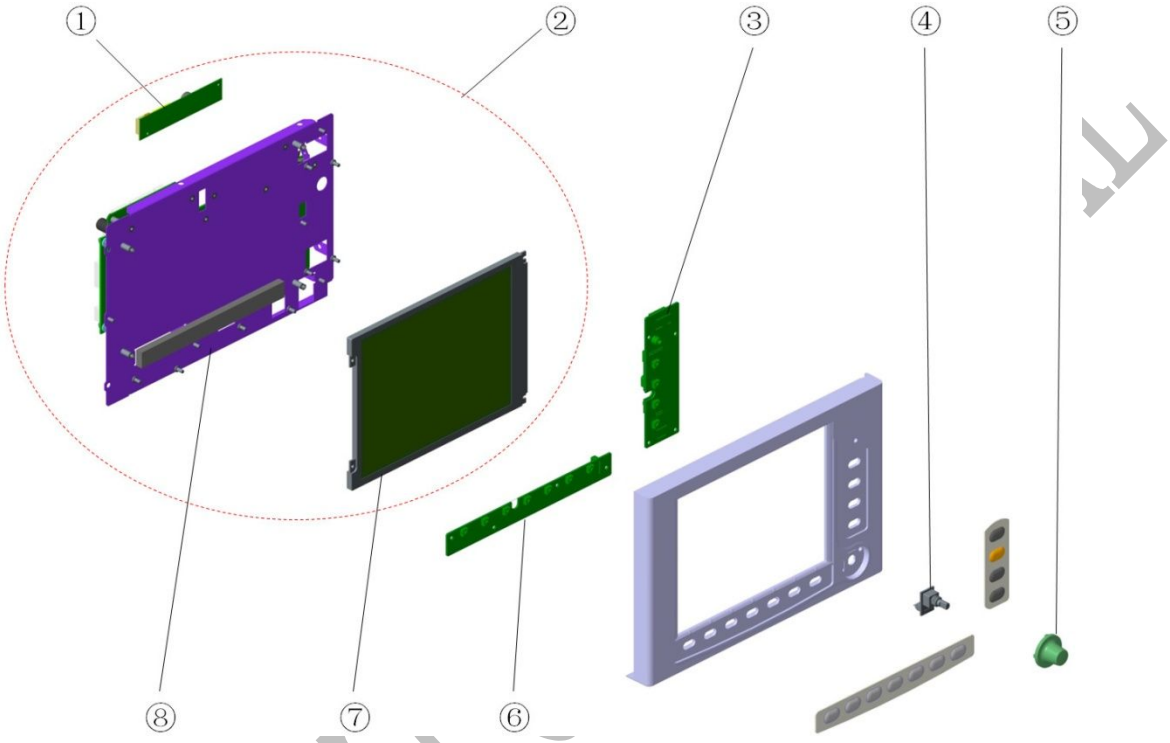

1.8.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	801-0616-00103-00	Adapter brd for 7" Innolux Display	1	For WATO EX-20
	115-030476-00	backlight drive board PCBA		For WATO EX-30, 8" display
2	115-048599-00	Service kit for 8"display(w/ display)	1	/
3	801-0616-00054-00	0616keyboard	1	/
4	801-0613-00035-00	Encoder(FRU)	1	/

5	043-000342-00	Knob	1	/
6	801-0616-00055-00	7" keyboard scan board	1	For WATO EX-20
	801-0616-00056-00	8.4" keyboard scan board		For WATO EX-30
7	115-032939-00	7" screen FRU	1	Refer to TMZ-15045. Including LCD, Silicone Case and Waterproof lens
	115-034741-00	7" screen upgrade kit FRU		Refer to TMZ-15045. Only Silicone Case and Waterproof lens, no LCD
8	115-048598-00	Service kit for 8"display(w/o display)	1	/

MINDRAY CONFIDENTIAL

1.9 Upper Half

1.9.1 Exploded View

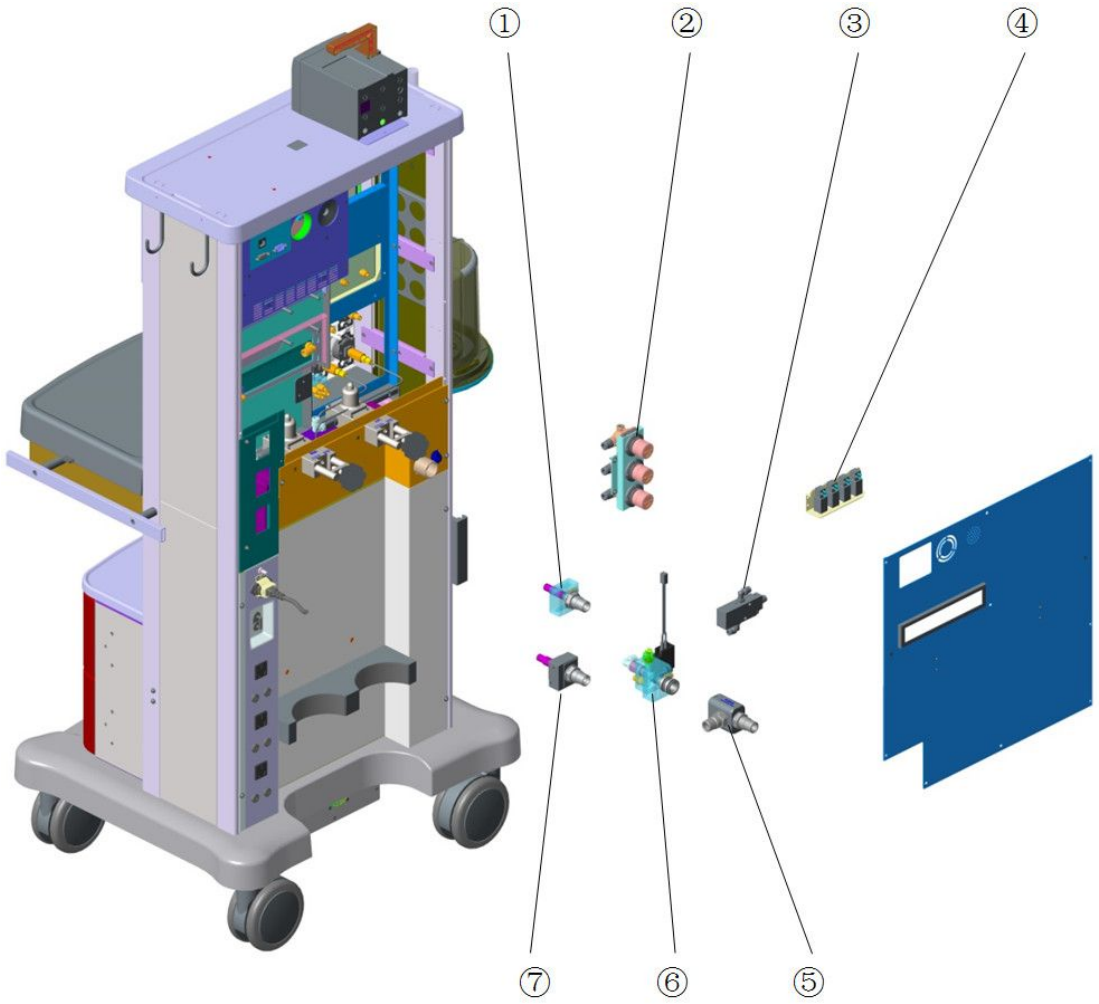

1.9.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	115-003681-00	N2O pipeline inlet assembly (DISS, 0616)	1	DISS, w/ pressure relief valve, w/ pressure regulator. For machines without

				N2O cylinder yoke
	115-003683-00	N2O p-line inlet ass'y, w/yoke DISS 0616		DISS, w/ pressure relief valve, w/ pressure regulator. For machines with N2O cylinder yoke
	115-015025-00	Nitrous oxide inlet assembly (0616,DISS)		DISS, w/o pressure relief valve, w/o pressure regulator
	115-034149-01	N2O supply inlet assembly		DISS, w/o pressure relief valve, w/ pressure regulator
	115-015026-00	Nitrous oxide inlet assembly		NIST, w/o pressure relief valve, w/o pressure regulator
	115-033838-01	N2O supply inlet assembly(0615)		NIST, w/o pressure relief valve, w/ pressure regulator
	115-039044-00	N2O supply inlet assembly FRU(0616)		NIST, w/ pressure relief valve, w/o pressure regulator
	115-038640-00	N2O supply inlet assembly(0615)		NIST, w/ pressure relief valve, w/ pressure regulator
	801-0613-00008-00	N2O supply inlet assembly		NIST, w/ pressure relief valve, w/ pressure regulator(marked "PULLTOADJUST"). For machines without N2O

MINDRAY CONFIDENTIAL

				cylinder yoke
	801-0613-00010-00	N2O supply inlet assembly(with cylinder)		NIST, w/ pressure relief valve, w/ pressure regulator(marked "PULLTOADJUST") . For machines with N2O cylinder yoke
2	115-015124-00	Pressure Regulator Assembly	1	Include 115-007621-00 and tubes
	115-015125-00	Pressure Regulator Assembly		For O2&N2O
	115-007621-00	Regulator assembly(N2O,O2,Air)		For O2&N2O&Air
	115-016549-00	Regulator assembly(O2,Air)		For O2&Air
	801-0631-00087-00	Regulator Assembly for O2 or Air FRU		For O2 or Air
3	082-001231-00	valve.2-way,air-piloted valves	1	/
4	801-0621-00192-00	3-way Valve Assembly (0616/FRU)	1	3 piece of valves, for machine w/o ACGO
	115-034978-00	3 way valve assembly FRU		4 piece of valves, for machine w/ ACGO
5	115-037227-00	oxygen supply T-connection package	1	Used as upgrade kit. Refer to TMZ-16006
	115-036788-00	Reserve O2 Supply Connector(vale)		Square body. Refer to TMZ-16006

MINDRAY CONFIDENTIAL

				16007
6	115-003680-00	O2 Pipeline Inlet Assembly (DISS, 0616)	1	DISS, w/ pressure regulator(marked "PULLTOADJUST")
	115-034148-01	O2 supply inlet assembly		DISS, w/ pressure regulator
	115-036778-00	O2 supply inlet assembly(0623/DISS/vale)		DISS, w/o pressure regulator
	801-0613-00007-00	O2 supply inlet assembly		NIST, w/ pressure regulator(marked "PULLTOADJUST")
	115-033836-01	O2 supply inlet assembly(0615)		NIST, w/ pressure regulator
	115-036781-00	O2 supply inlet assembly(0623/vale)		NIST, w/o pressure regulator
	115-036780-00	Reserve O2 Supply Base(vale)		W/ pressure relief valve, w/ pressure switch, used with 115-036788-00. Refer to TMZ-16006□16007
	115-034706-01	Backup O2 assembly(0615)		W/O pressure relief valve, w/o pressure switch. Refer to TMZ-16006□16007
7	115-003682-00	Air pipeline inlet assembly (DISS, 0616)	1	DISS, w/ pressure relief valve, w/ pressure regulator.

MINDRAY CONFIDENTIAL

				For machines without Air Drive
	115-003684-00	Air p-line inlet ass'y,AirDrive DISS0616		DISS, w/ pressure relief valve, w/ pressure regulator. For machines with Air Drive
	115-011513-00	air inlet assembly (0616,DISS)		DISS, w/o pressure relief valve, w/o pressure regulator
	115-034150-01	AIR supply inlet assembly		DISS, w/o pressure relief valve, w/ pressure regulator
	801-0616-00109-00	AIR supply inlet assembly		NIST, w/o pressure relief valve, w/o pressure regulator
	115-033837-01	Air supply inlet assembly(0615)		NIST, w/o pressure relief valve, w/ pressure regulator
	115-037712-00	Air supply inlet assembly(0616)		NIST, w/ pressure relief valve, w/o pressure regulator
	115-038641-00	Air supply inlet assembly(0615)		NIST, w/ pressure relief valve, w/ pressure regulator
	801-0613-00009-00	Air supply inlet assembly		NIST, w/ pressure relief valve, w/ pressure regulator(marked "PULLTOADJUST"). For machines


MINDRAY CONFIDENTIAL

				without Air Drive
	801-0616-00004-00	Air supply inlet assembly(Air drive)		NIST, w/ pressure relief valve, w/ pressure regulator(marked "PULLTOADJUST"). For machines with Air Drive

MINDRAY CONFIDENTIAL

1.10 Auxiliary Output Assembly

1.10.1 Exploded View

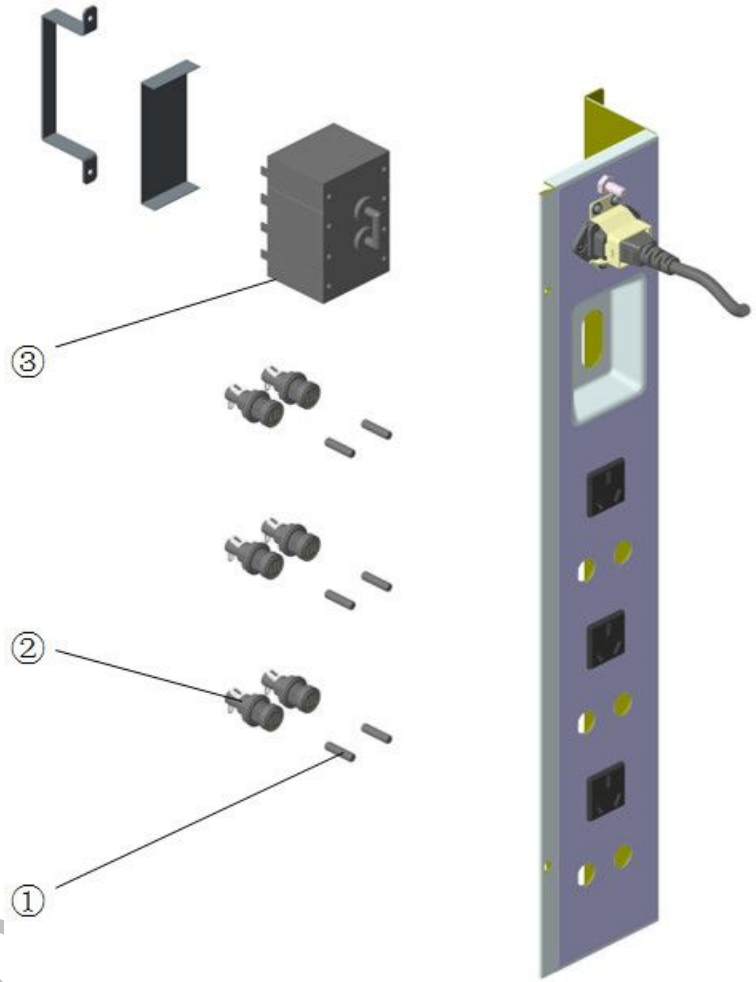

1.10.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	801-0613-00068-00	FUSE time-lag250V2AGLS5*20mm	6	Only one fuse in each 801-0613-00068-00
2	801-0611-00102-00	HEADER Fuse Holder φ5*20 (FRU)	6	Only one holder in each 801-0611-

				00102-00
3	801-0613-00030-00	Breaker 250V 7.5A welded terminal	1	For machines with power outlet breaker

MINDRAY CONFIDENTIAL

1.11 Isolation Transformer Assembly

1.11.1 Exploded View

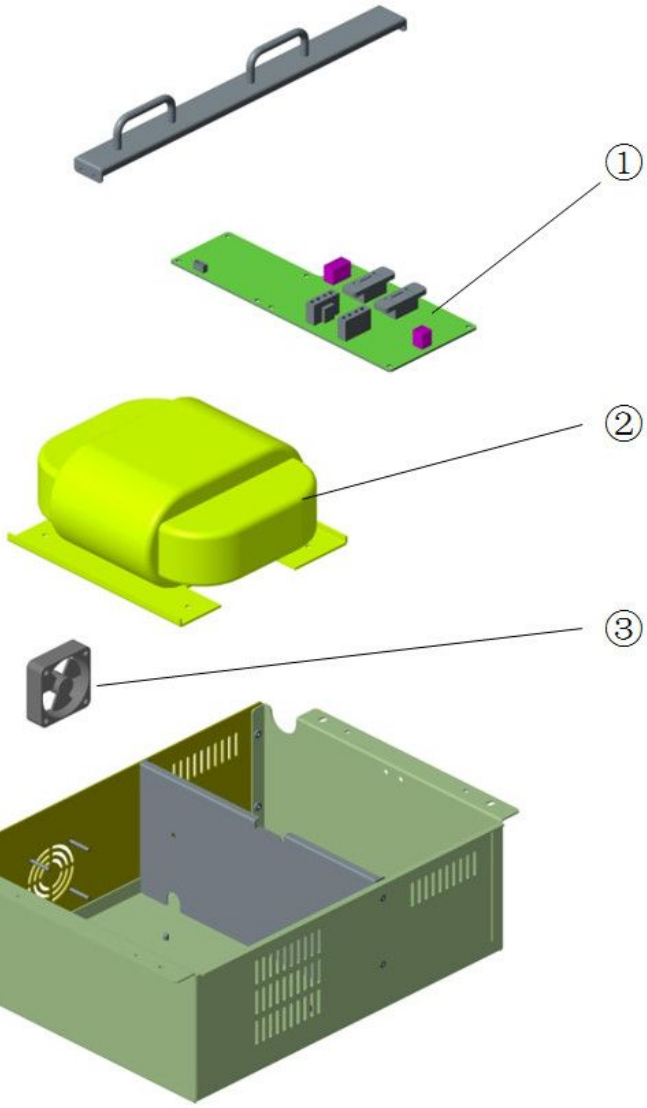

1.11.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	801-0616-00051-00	isolation power drive board	1	/
2	801-0611-00005-00	Isolation transformer R800	1	/

		620VA(FRU)		
3	801-0611-00006-00	Fan for Isolation transformer (w wire)	1	Used in isolation transformer box

MINDRAY CONFIDENTIAL

1.12 Heating Control Assembly

1.12.1 Exploded View

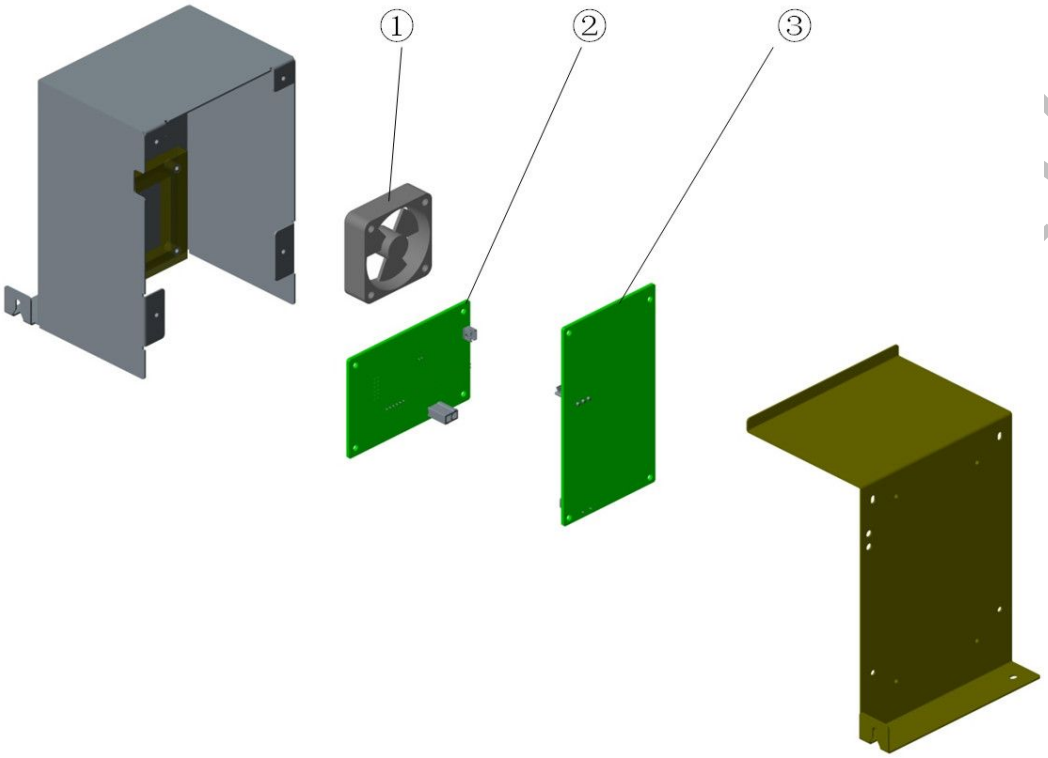


1.12.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	801-0616-00061-00	Fan	1	Used in heating control box
2	051-000152-00	AC-DC power board PCBA	1	/
3	801-0616-00118-00	Heating control Board(FRU)	1	/

1.13 Liquid Collection Bottle Assembly

1.13.1 Exploded View

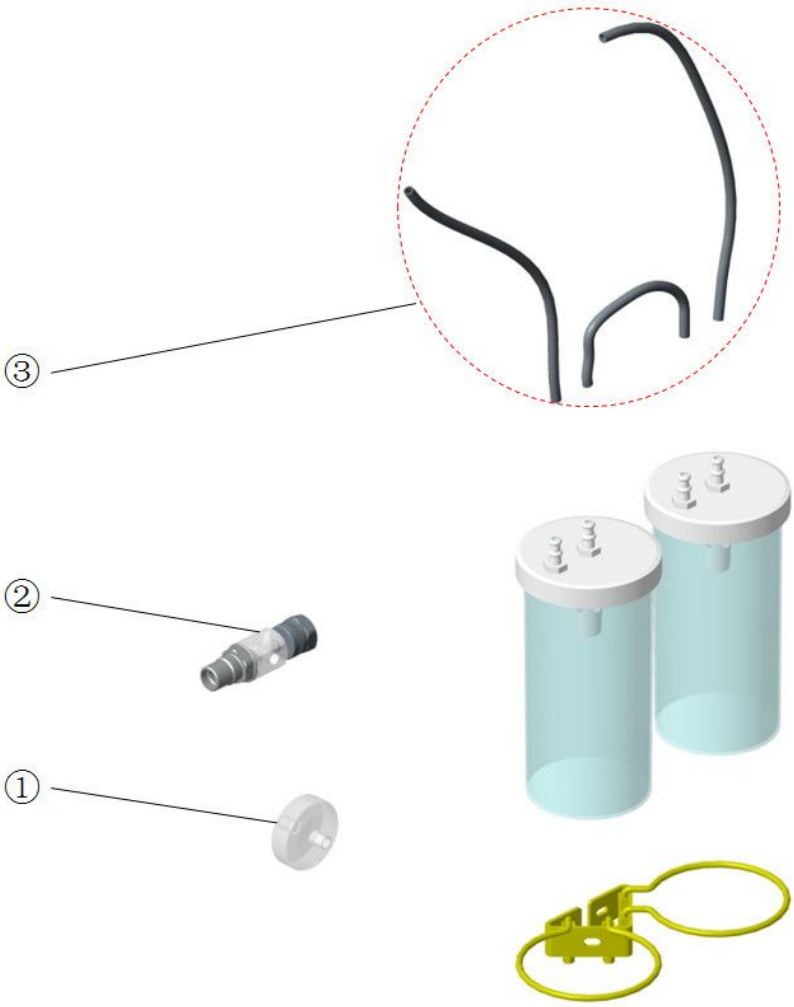

1.13.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	082-001327-00	Disposable Filter.0.45μm	1	/
2	115-020571-00	Suction T-joint air(DISS)check valve	1	/
	115-020572-00	Suction T-joint air(NIST)check valve		/

	115-020573-00	Suction T-joint O2(NIST)check valve		/
	115-020574-00	Suction T-joint O2(DISS)check valve		/
3	040-001658-00	tube.pvc	1	4 meters

MINDRAY CONFIDENTIAL

1.14 Main Body of the Patient Circuit

1.14.1 Exploded View

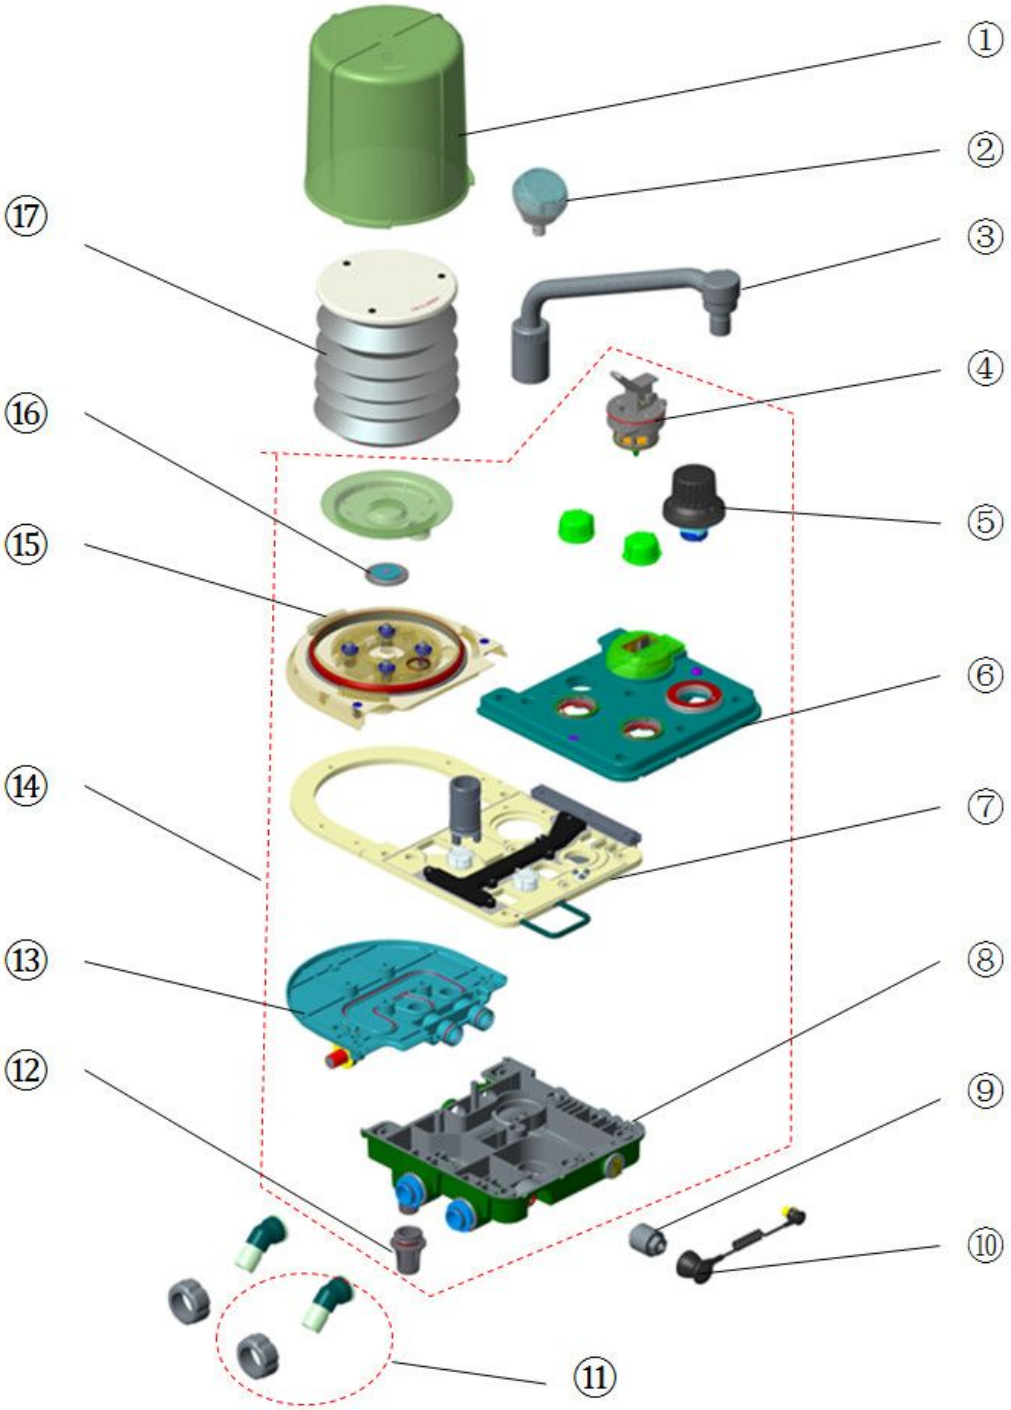

1.14.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	801-0616-00001-00	Bellows housing	1	/
2	115-025563-00	Airway pressure gauge	1	/
3	801-0601-00005-00	Bag arm assembly	1	/
4	801-0601-00017-00	Bag/mechanical ventilation switch	1	/
5	801-0621-00168-00	(New) APL Valve assembly(FRU)	1	/
6	115-015126-00	Upper cover FRU(0616)	1	/
7	115-048634-00	mid-plate assembly(no heat/no arm)FRU	1	/
	115-048635-00	mid-plate assembly(no heat/arm)FRU		/
	115-048636-00	mid-plate assembly(heat/no arm)FRU		/
	115-048638-00	mid-plate assembly(heat/arm)FRU		/
8	115-002370-00	Lower cover assembly(0616)	1	For BC with bag arm. PSU
	115-002377-00	Lower cover assembly (optional)(0616)		For BC without bag arm. PSU
	115-034981-00	lower cover assembly(no bag arm)FRU		For BC without bag arm. Nylon. Refer to

MINDRAY CONFIDENTIAL

				TMZ-15053
9	0611-10-45654	O2 sensor,MedicelMOX-2	1	/
	040-000898-00	sensor oxygen		The same type with factory configuration
10	0601-20-78941	O2 sensor cable	1	/
11	0621-30-78446	Inspiration / expiration connectors asse	2	One connector and one rotary cap in each 0621-30-78446
12	801-0631-00058-00	Water Collection Cup, A series	1	Include colorless O-ring
	801-0616-00005-00	Water collection cup assembly		Include red O-ring
13	043-000121-00	Lower cover 2(PSU)	1	/
14	115-015359-00	Patient circuit (no bag arm/no BYPASS)	1	/
	115-015358-00	Patient circuit(bag arm/no BYPASS)		/
	801-0616-00020-00	Breathing circuit(with arm/BYPASS/PS)		PSU
	801-0616-00021-00	Breath circuit(with arm,w/o BYPASS,PS)		PSU
	801-0616-00018-00	Breath circuit(w/o arm,with BYPASS,PS)		PSU
	801-0616-00019-00	Breathing circuit(w/o arm/BYPASS,PS)		PSU


MINDRAY CONFIDENTIAL

	115-034910-00	Circuit main unit(no heat/bag arm)		Nylon. Refer to TMZ-15053
	115-034909-00	Circuit main unit(heat/bag arm)		Nylon. Refer to TMZ-15053
	115-034908-00	Circuit main unit(no heat/no bag arm)		Nylon. Refer to TMZ-15053
	115-034907-00	Circuit main unit(no heat/bag arm)		Nylon. Refer to TMZ-15053
15	043-000119-00	Upper cover 2(PSU)	1	/
16	801-0601-00002-00	Pop-off valve assembly	1	/
17	801-0601-00001-00	Folding bag assembly	1	/

MINDRAY CONFIDENTIAL

1.15 Check Valve Assembly

1.15.1 Exploded View

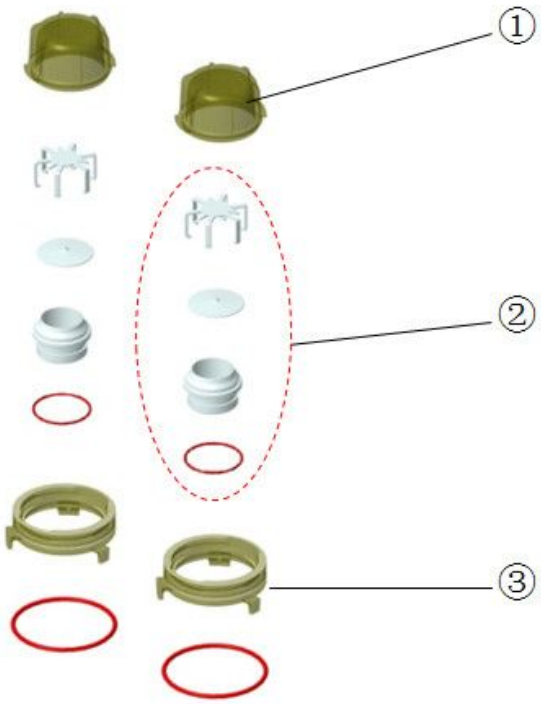

1.15.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	801-0616-00002-00	Check valve cover	2	Only one cover in each 801-0616-00002-00
2	801-0616-00003-00	In&ex-piration check valve assembly	2	Only one check valve assembly in each 801-0616-00003-00
3	043-000127-00	Check Valve bracket(PSU)	2	For PSU BC. Only one bracket in each 043-000127-00


MINDRAY CONFIDENTIAL

	0613-20-87681	Check valve bracket (mold MR87681)		For Nylon BC. Refer to TMZ-15030. Only one bracket in each 0613-20-87681

MINDRAY CONFIDENTIAL

1.16 Lifting Device Assembly

1.16.1 Exploded View

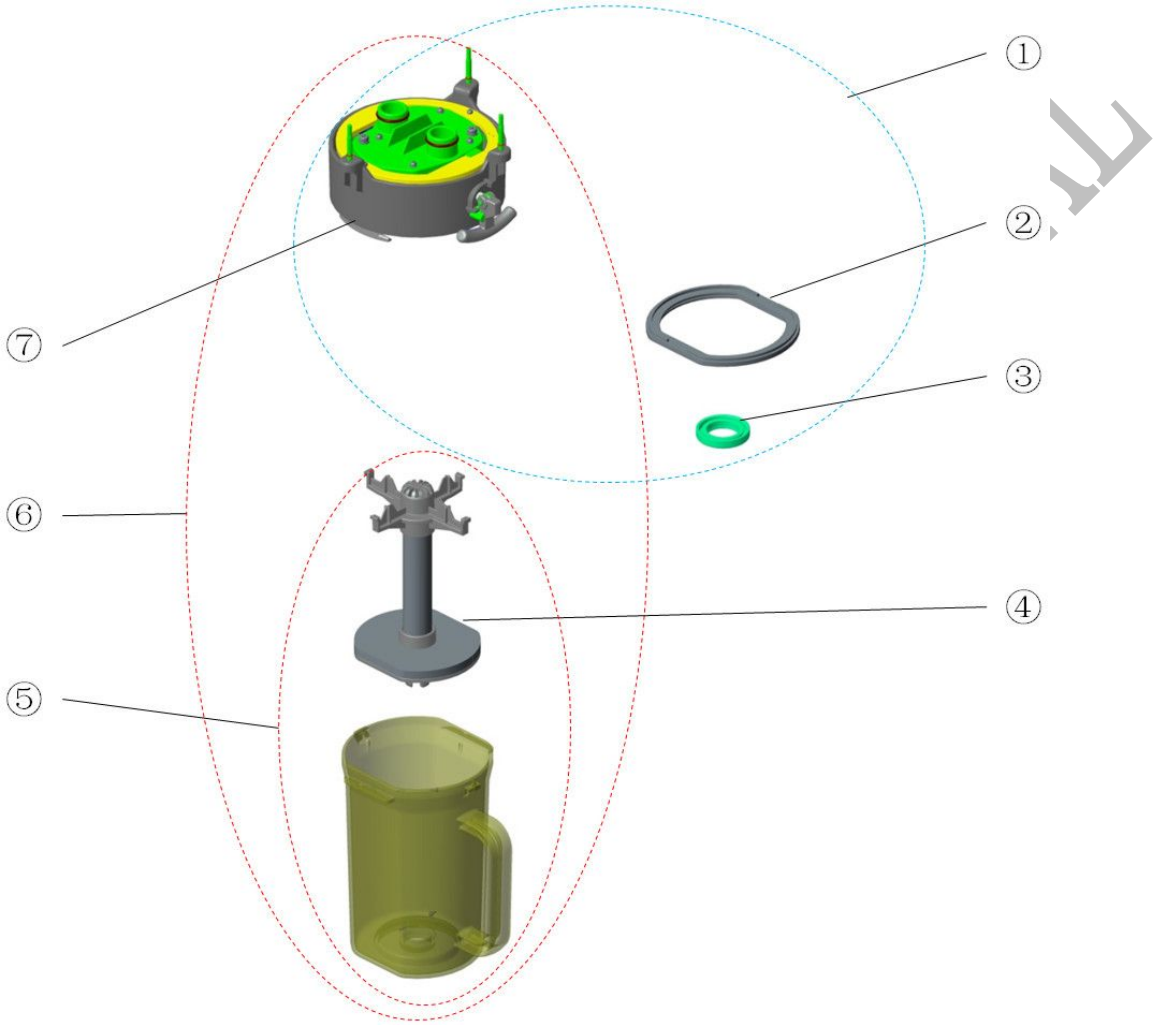

1.16.2 Parts List


No.	Order Number	Part Description	Qty	Remarks
1	115-034208-00	Lifting device(with bypass/0615)	1	For Nylon BC. Refer to TMZ-15053
	115-034209-00	Lifting device(no bypass/0615)		For Nylon BC. Refer to TMZ-15053

2	0601-20-78842	Seal for sodalime canister	1	Only for lifting canister
3	049-000154-00	sealed tray of exit	1	/
4	801-0601-00014-00	Absorber support assembly	1	/
5	115-002374-00	Sodalime canister assembly	1	PSU
	115-030838-00	Canister assembly(0625)		For Nylon BC. Refer to TMZ-15053
6	801-0616-00017-00	Lifting device (with BYPASS)	1	For PSU BC. Include 115-023264-00 & 115-002374-00
	801-0616-00022-00	Lifting device(without BYPASS)		For PSU BC. Include 115-023265-00 & 115-002374-00
7	115-023264-00	Lifting device FRU(with bypass/0616)	1	For PSU BC
	115-023265-00	Lifting device FRU(0616)		For PSU BC. Without BYPASS

MINDRAY CONFIDENTIAL

1.17 Sodalime Canister Assembly

1.17.1 Exploded View

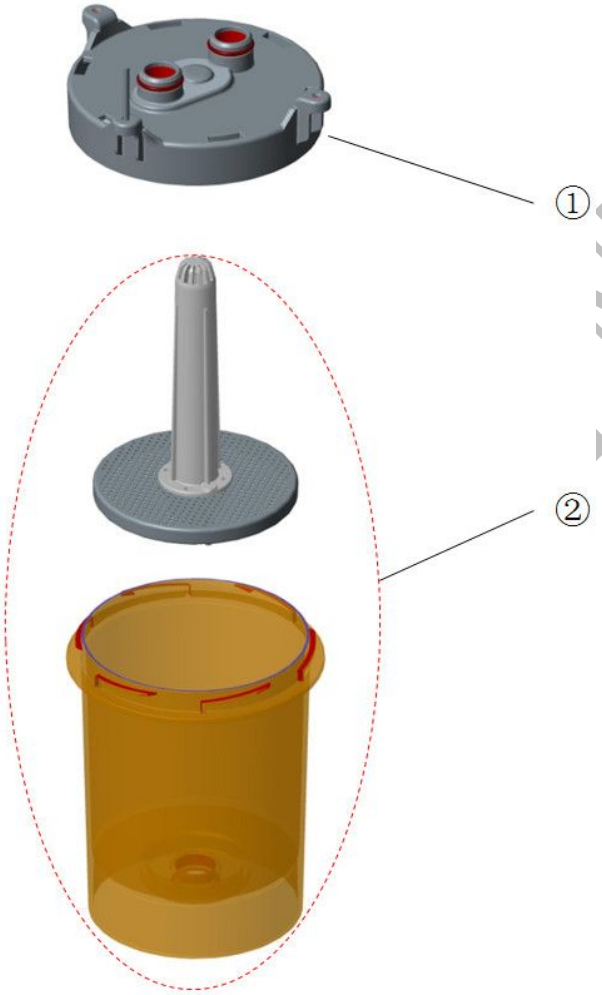

1.17.2 Parts List

No.	Order Number	Part Description	Qty	Remarks
1	115-014605-00	Canister upper cover assembly(20L)	1	/
	115-034193-00	Canister upper cover		For Nylon BC. Refer

		assembly(20B)		to TMZ-15053
2	115-014606-00	Sodalime canister assembly(20L)	1	/
	115-034194-00	Sodalime canister assembly(20B)		For Nylon BC. Refer to TMZ-15053

MINDRAY CONFIDENTIAL

1.18 Others

No.	Order Number	Part Description	Qty	Remarks
1	115-034982-00	circuit screw Kits	1	Refer to TMZ-15053
2	115-034999-00	Heating Module Package 0615)	1	Include heater box assembly and BC heater(not the whole BS block). Refer to TMZ-15053
	801-0616-00132-00	Heating Module Package (ACGO and bypass)		Include heater box assembly and BS block
	801-0616-00129-00	Heating Module Package (ACGO Only)		Include heater box assembly and BS block
	801-0616-00131-00	Heating Module Package (bypass Only)		Include heater box assembly and BS block
	801-0616-00130-00	Heating Module Package(Neither)		Include heater box assembly and BS block
3	115-004332-01	Pendant assembly(0616)	1	/
4	0621-30-78719	quick connector	1	/
5	801-0621-00109-00	USB Disk with Activation Code (PCV)	1	Sys software Ver Higher than 04.08.00, need to provide machine's SN and machine ID

MINDRAY CONFIDENTIAL

6	801-0621-00110-00	USB Disk with Activation Code (SIMV)	1	Sys software Ver Higher than 04.08.00, need to provide machine's SN and machine ID
7	115-021121-00	Maintain Kit(0616/0625,Basic,1 yr)	1	/
8	115-021122-00	Maintain Kit(0616/0625,Extend,1 yr)	1	/
9	115-021123-00	Maintain Kit(0616/0625,Advanced, 1 yr)	1	/
10	095-000031-00	wrench 6700-0020-300	1	/
11	115-036182-00	Medicine filler sleeve(0605) FRU	1	/
12	115-036167-00	Filler cap FRU	1	/
13	115-039569-00	Filler cap of ENF(Pour Fill)	1	/
14	115-039571-00	Filler cap of ISO(Pour Fill)	1	/
15	115-039572-00	Filler cap of SEV(Pour Fill)	1	/
16	115-039573-00	Filler cap of SEV(Quik-Fil)	1	/
17	115-039574-00	Filler cap of Hal(Pour Fill)	1	/
18	115-051200-00	ventilator(AIR drive)	1	Include 115-034207-00 and 115-051195-00

MINDRAY CONFIDENTIAL

	115-051199-00	ventilator(O2 drive)		Include 115-034207-00 and 115-051195-00
19	801-0631-00107-00	spring of Vaporizer Mounting Manifold	1	/
20	801-0611-00094-00	Gas inlet Filter	1	/
21	801-0613-00051-00	Gas pressure switch	1	/
22	801-0616-00099-00	Pipeline Gas Inlet Regulator (FRU)	1	/
23	801-0621-00164-00	Drawer Lock.LA-W613 (FRU)	1	For machines before 2014.01
	115-023320-00	LOCK FRU		For machines after 2014.01. Refer to TMZ-14002
24	115-003706-00	Common Gas Outlet(No ACGO Switch)	1	/
25	115-009073-00	AGSS low-flow Receiving hoses assembly	1	/
	115-009097-00	AGSS high-flow Receiving hoses assembly		/
26	115-020745-00	AGSS connector package(UK)	1	/
27	801-0621-00169-00	(New) APL valve cover assembly(FRU)	1	Used with grey APL
28	049-000243-00	Gasket,Bellows Canister Base	1	/
29	115-037748-00	Nylon circuit(w/ arm,w/o	1	Refer to TMZ-16024

MINDRAY CONFIDENTIAL

		bypass)		
	115-037749-00	Nylon circuit(w/o arm,w/o bypass)		Refer to TMZ-16024
	115-037750-00	Nylon circuit(w/ arm,w/ bypass)		Refer to TMZ-16024
	115-037751-00	Nylon circuit(w/o arm,w/ bypass)		Refer to TMZ-16024
	115-037752-00	Nylon circuit(w/arm,w/o bypass,w/o Lift)		Refer to TMZ-16024
	115-037753-00	Nylon circuit(w/o arm&bypass,w/o Lift)		Refer to TMZ-16024
30	M40-A00027---	TBD	1	Filter power 250VAC 10A panel mount
31	115-051197-00	Ventilator assembly (Air drive)	1	/
32	115-051198-00	Ventilator assembly (O2 drive)	1	/
33	803-010170-00	WATO EX-30 main unit warranty	1	/
34	803-010171-00	WATO EX-20 main unit warranty	1	/

MINDRAY CONFIDENTIAL