
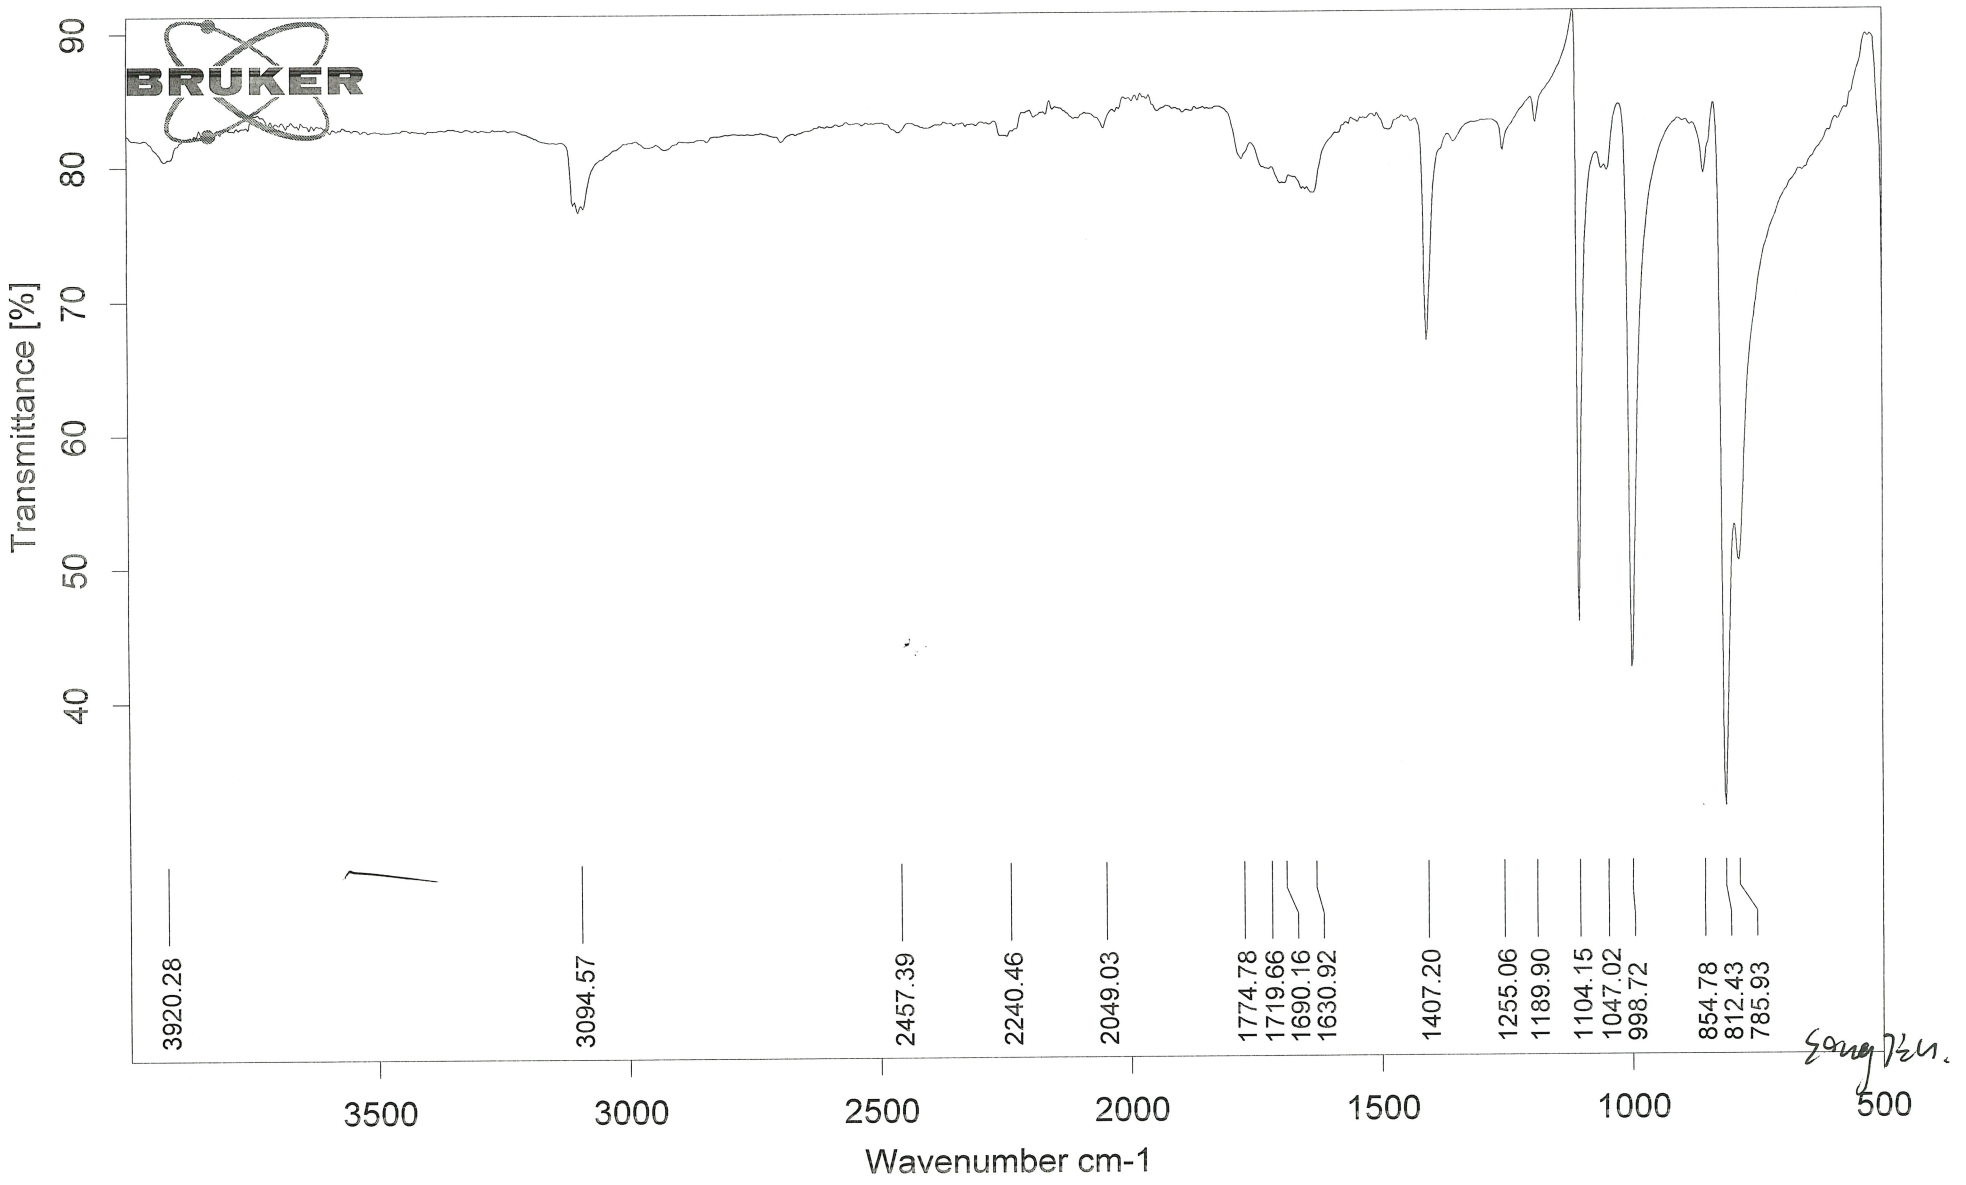


D:\CM3191\17Sep2026\Ferrocene_Kim_donghwan.0	Ferrocene_Kim_donghwan	Solid	17/9/2026

Spectrum Peak Pick Report

09/17/2026 03:09:58 PM

Data Set: KIM DONGHWAN_Ferrocene_150815.spc - RawData

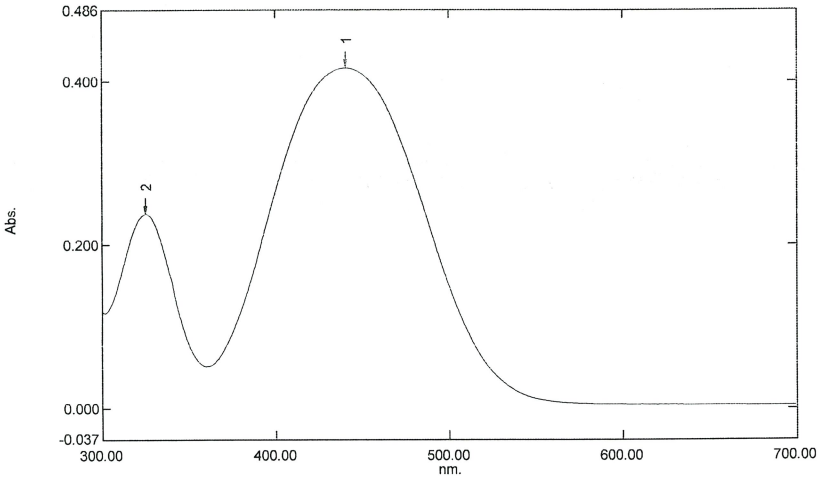

No.	P/V	Wavelength	Abs.	Description
1		440.50	0.416	
2		325.00	0.239	

[Measurement Properties]
Wavelength Range (nm.): 300.00 to 700.00
Scan Speed: Fast
Sampling Interval: 0.5
Auto Sampling Interval: Enabled
Scan Mode: Auto

[Instrument Properties]
Instrument Type: UV-1800 Series
Measuring Mode: Absorbance
Slit Width: 1.0 nm
Light Source Change Wavelength: 340.0 nm
S/R Exchange: Normal

[Attachment Properties]
Attachment: None

[Operation]
Threshold: 0.0010000
Points: 4
InterPolate: Disabled
Average: Disabled

[Sample Preparation Properties]
Weight:
Volume:
Dilution:
Path Length:
Additional Information: