

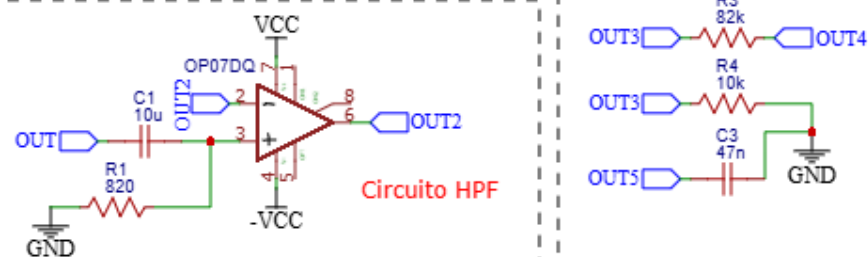
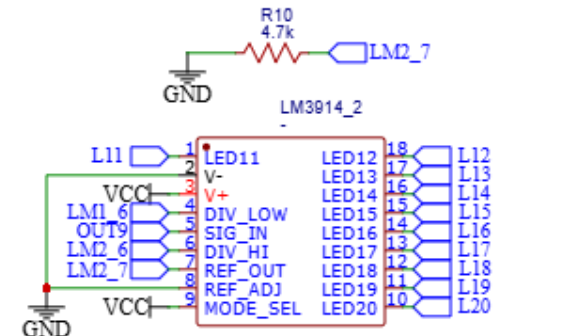
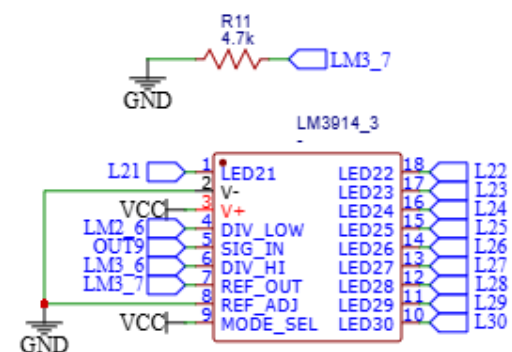
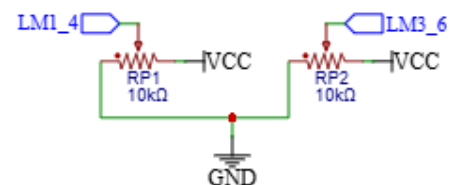
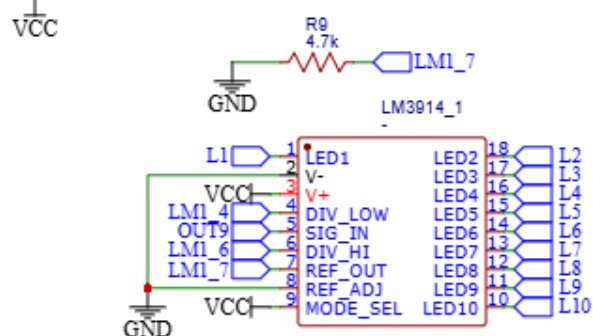


Detector de pico y amplificador no inversor

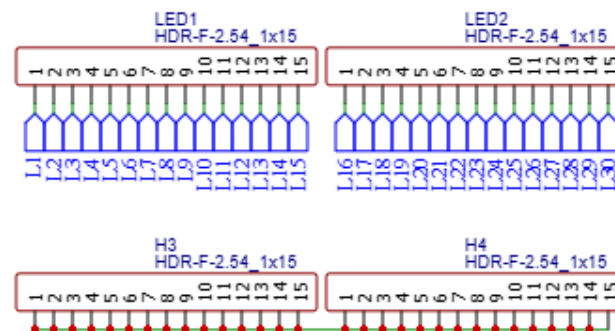

Circuito HPF

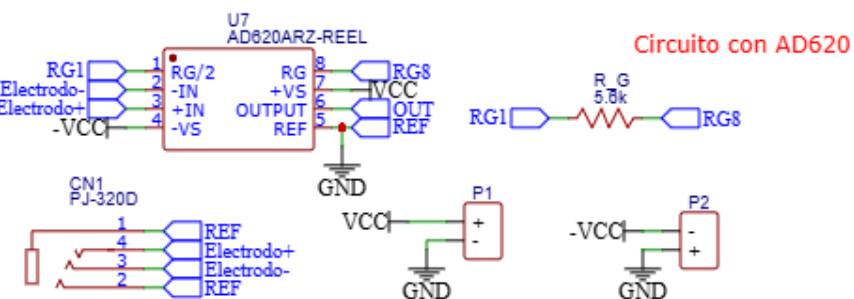

Led Bar Display y LM3914 en cascada

TITLE: Dispositivo de EMG		REV: 1.0
Company: Tec CEM		Sheet: 1/1
Date: 2025-08-18	Drawn By: Diego Roque Gómez	