equipment_type	Sum of max_capacity_hrs	Sum of planned_maintenance_hrs
incubator	69,190.00	242.97
Microscope	45,726.00	141.66
ICSI_Workstation	45,760.00	156.28
Total	**1,60,676.00**	**540.91**

equipment_type	Sum of total_cases_day_lab	Sum of workflow_delay_events	Sum of utilization_pct
Microscope	24685	301.00	1,452.15
ICSI_Workstation	24706	893.00	1,736.38
incubator	37326	1,354.00	3,041.56
Total	**86717**	**2,548.00**	**6,230.09**

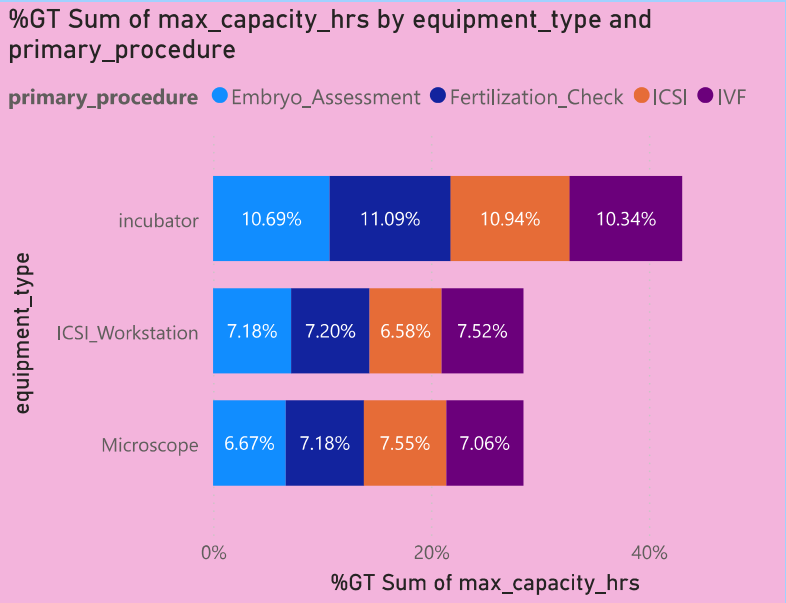

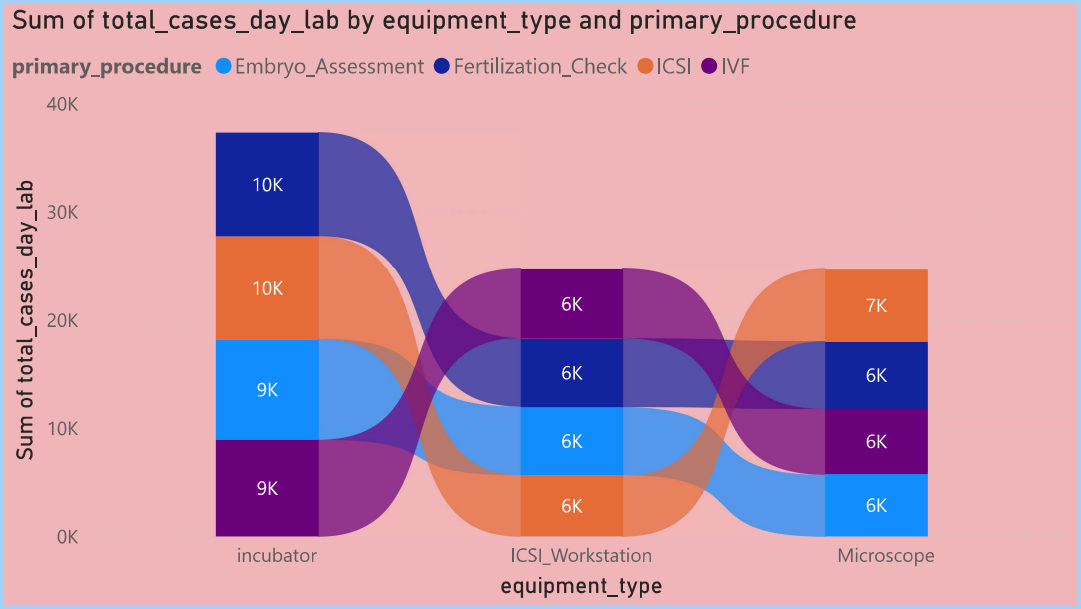

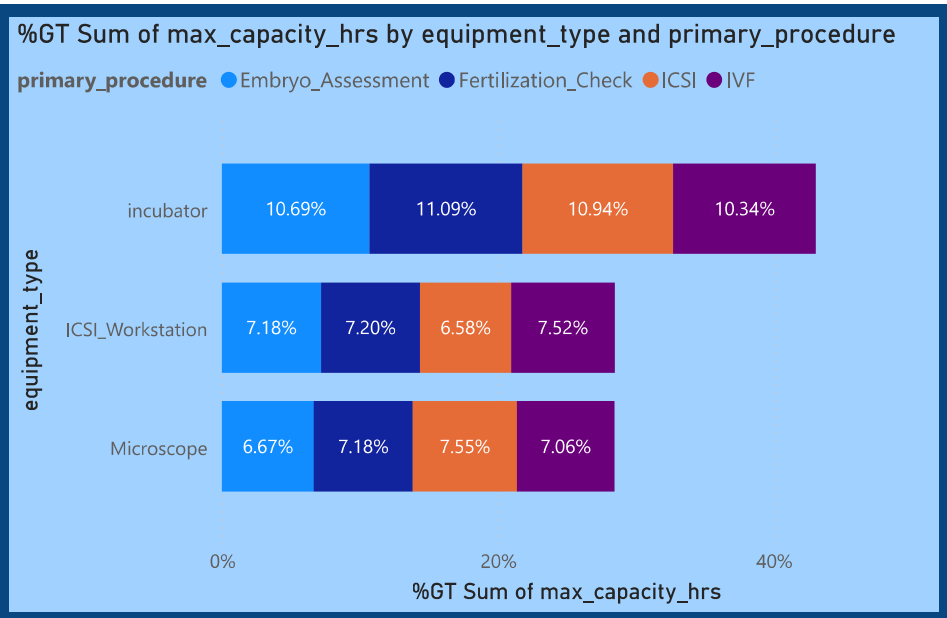
%GT Sum of max_capacity_hrs by equipment_type and primary_procedure
primary_procedure
Embryo_Assessment
Fertilization_Check
ICSI
IVF
equipment_type
incubator
ICSI_Workstation
Microscope
10.69%
11.09%
10.94%
10.34%
7.18%
7.20%
6.58%
7.52%
6.67%
7.18%
7.55%
7.06%
0%
20%
40%
%GT Sum of max_capacity_hrs

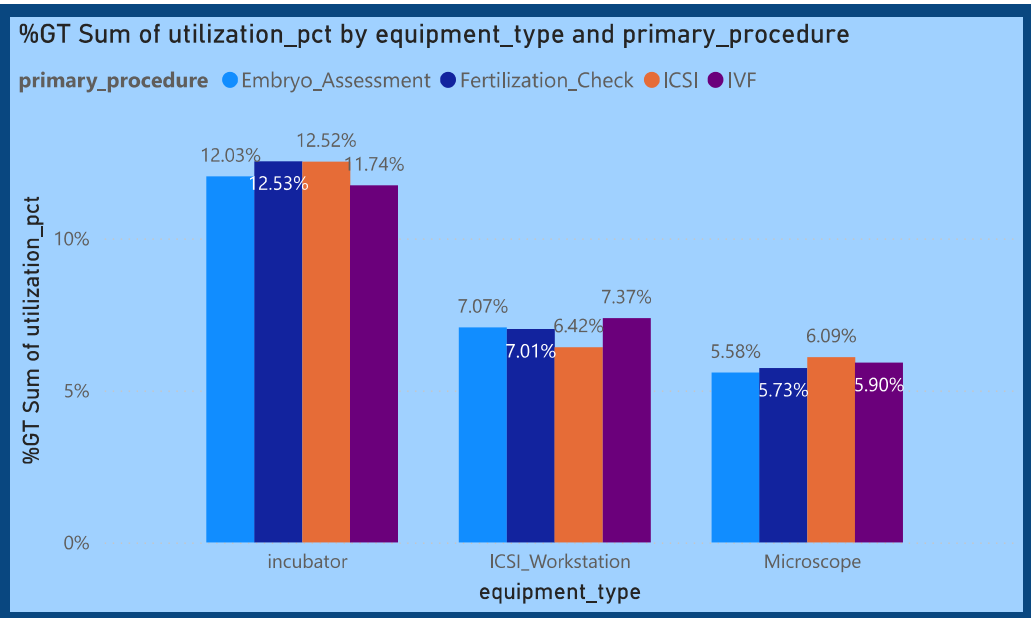
%GT Sum of utilization_pct by equipment_type and primary_procedure
primary_procedure
Embryo_Assessment
Fertilization_Check
ICSI
IVF
%GT Sum of utilization_pct
10%
5%
0%
12.03%
12.53%
12.52%
11.74%
7.07%
7.01%
6.42%
7.37%
5.58%
5.73%
6.09%
5.90%
incubator
ICSI_Workstation
Microscope
equipment_type

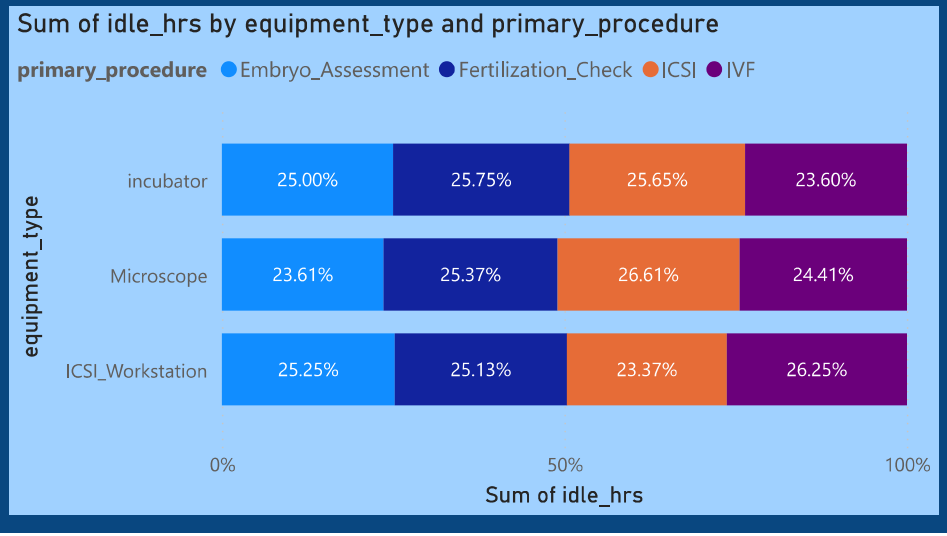
Sum of idle_hrs by equipment_type and primary_procedure
primary_procedure
Embryo_Assessment
Fertilization_Check
ICSI
IVF
equipment_type
incubator
Microscope
ICSI_Workstation
25.00%
25.75%
25.65%
23.60%
23.61%
25.37%
26.61%
24.41%
25.25%
25.13%
23.37%
26.25%
0%
50%
100%
Sum of idle_hrs

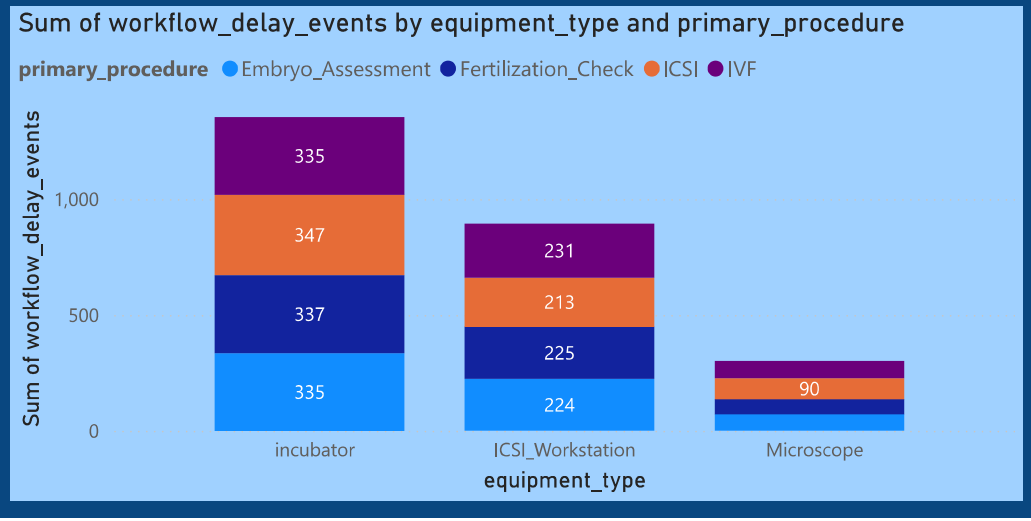
Sum of workflow_delay_events by equipment_type and primary_procedure
primary_procedure
Embryo_Assessment
Fertilization_Check
ICSI
IVF
Sum of workflow_delay_events
1,000
500
0
335
347
337
335
231
213
225
224
90
incubator
ICSI_Workstation
Microscope
equipment_type

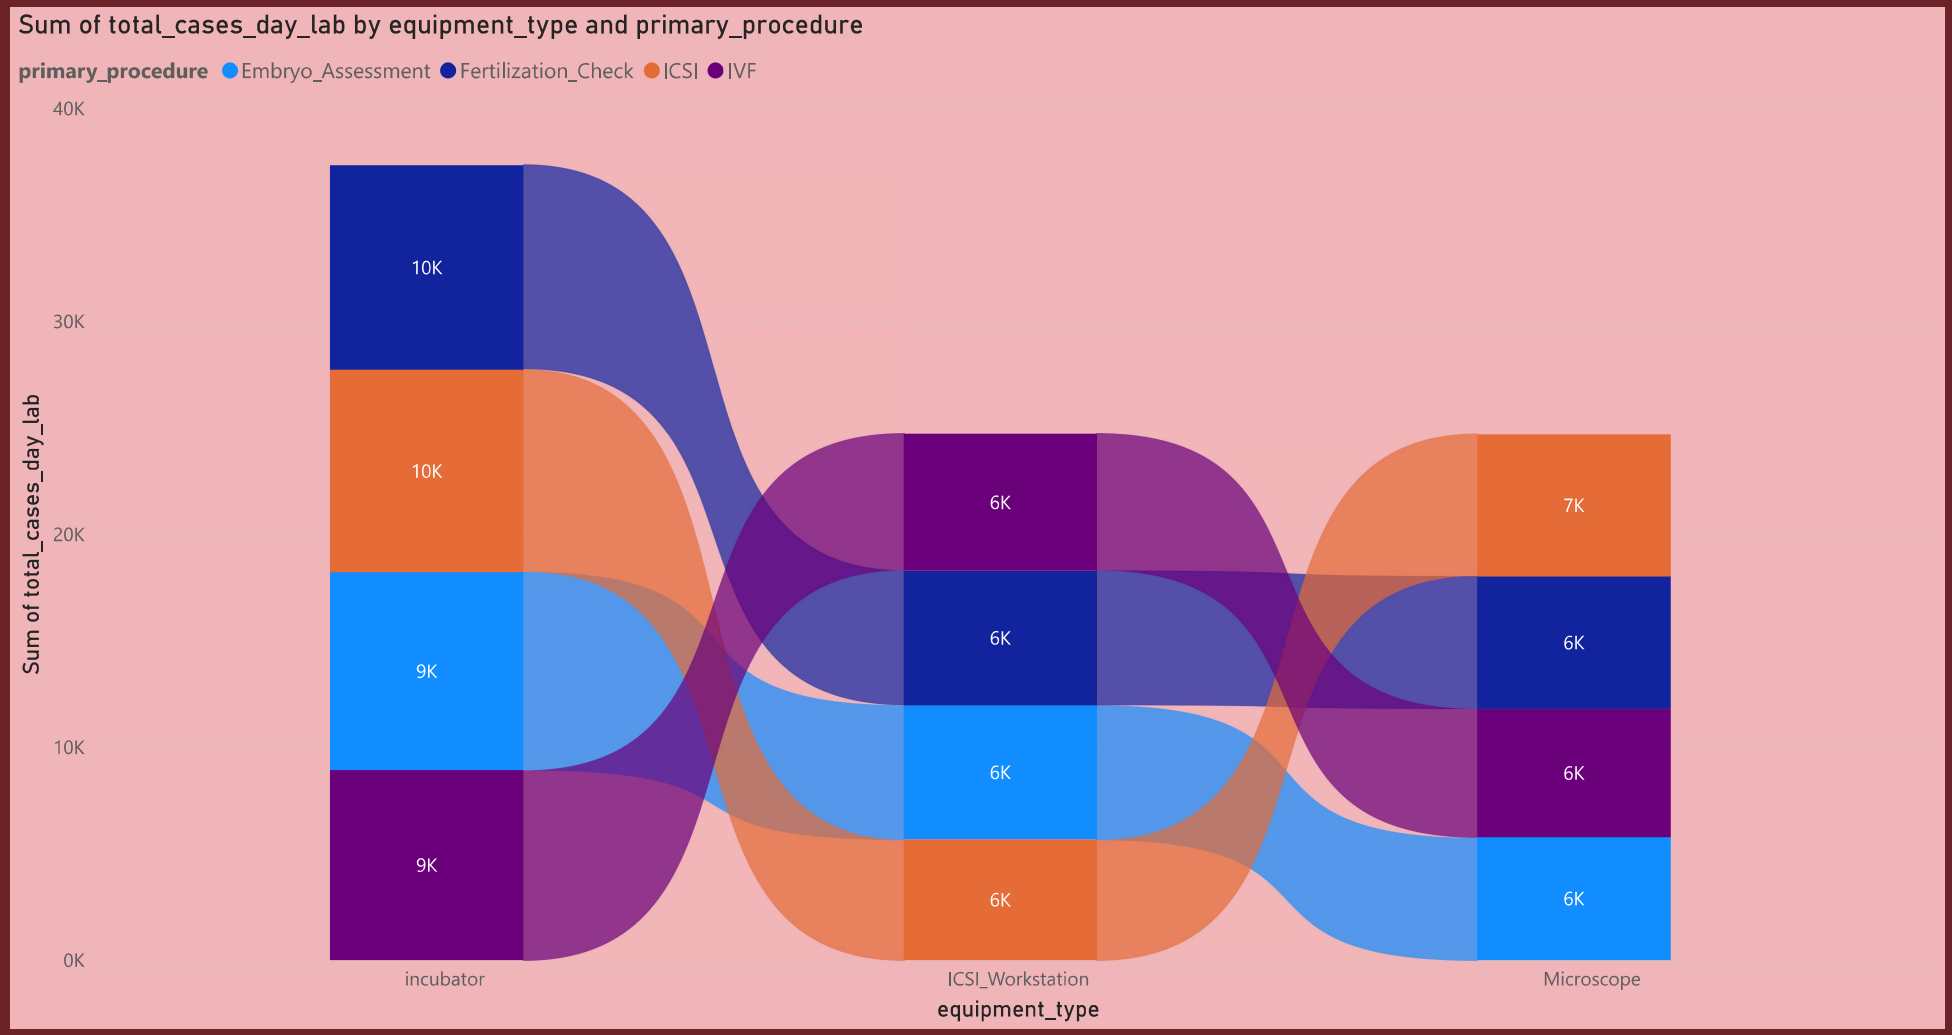
Sum of total_cases_day_lab by equipment_type and primary_procedure
primary_procedure
Embryo_Assessment
Fertilization_Check
ICSI
IVF
40K
30K
20K
10K
0K
Sum of total_cases_day_lab
10K
10K
9K
9K
6K
6K
6K
6K
7K
6K
6K
6K
incubator
ICSI_Workstation
Microscope
equipment_type

Sum of avg_delay_minutes by equipment_type and More / less

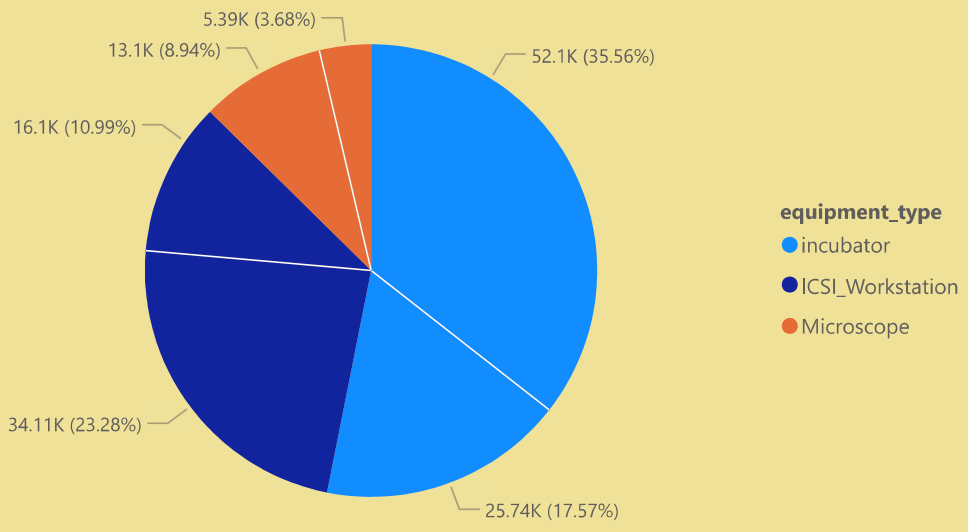

Sum of avg_delay_minutes by primary_procedure and redundancy_available

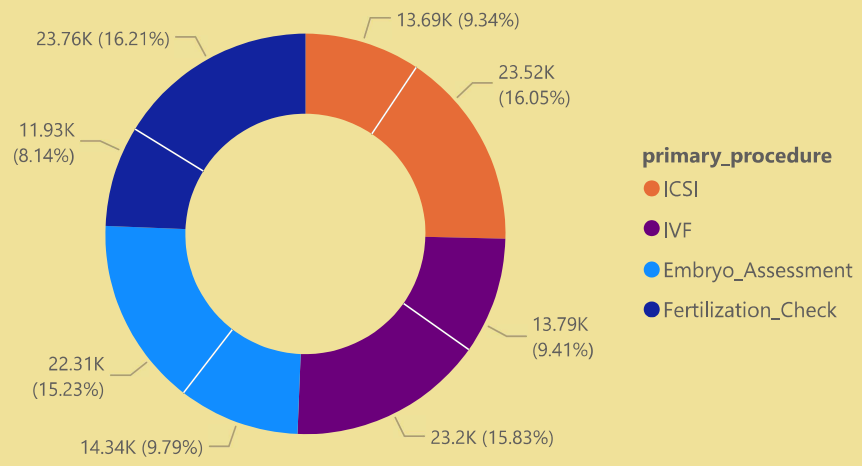

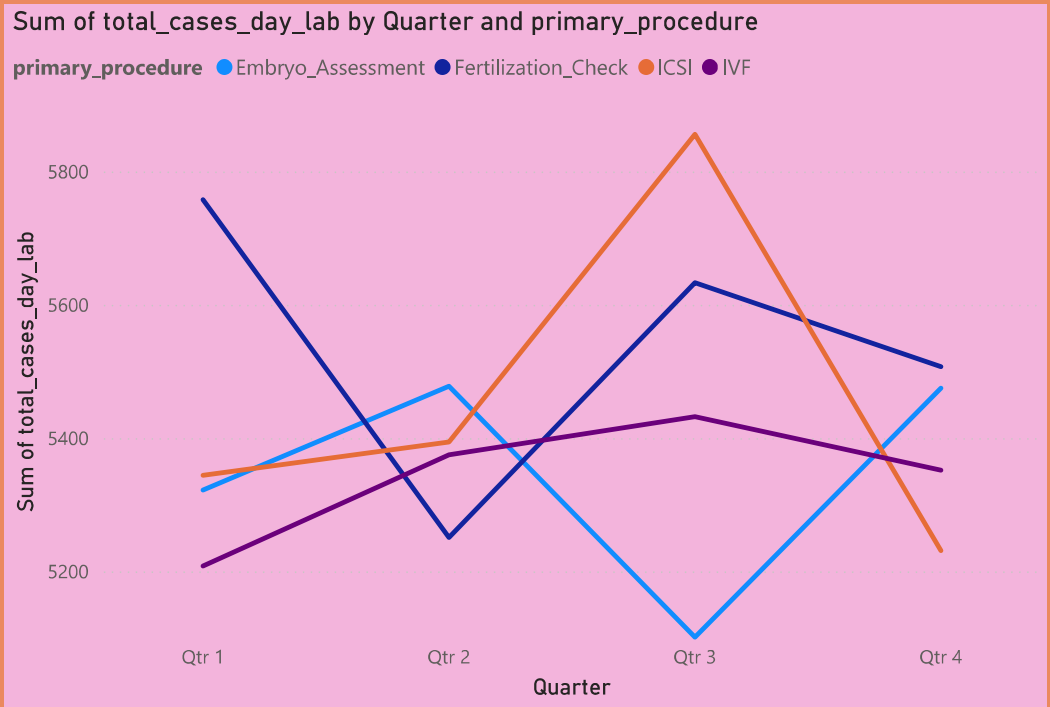
Sum of total_cases_day_lab by Quarter and primary_procedure
primary_procedure
Embryo_Assessment
Fertilization_Check
ICSI
IVF
5800
5600
5400
5200
Sum of total_cases_day_lab
Qtr 1
Qtr 2
Qtr 3
Qtr 4
Quarter

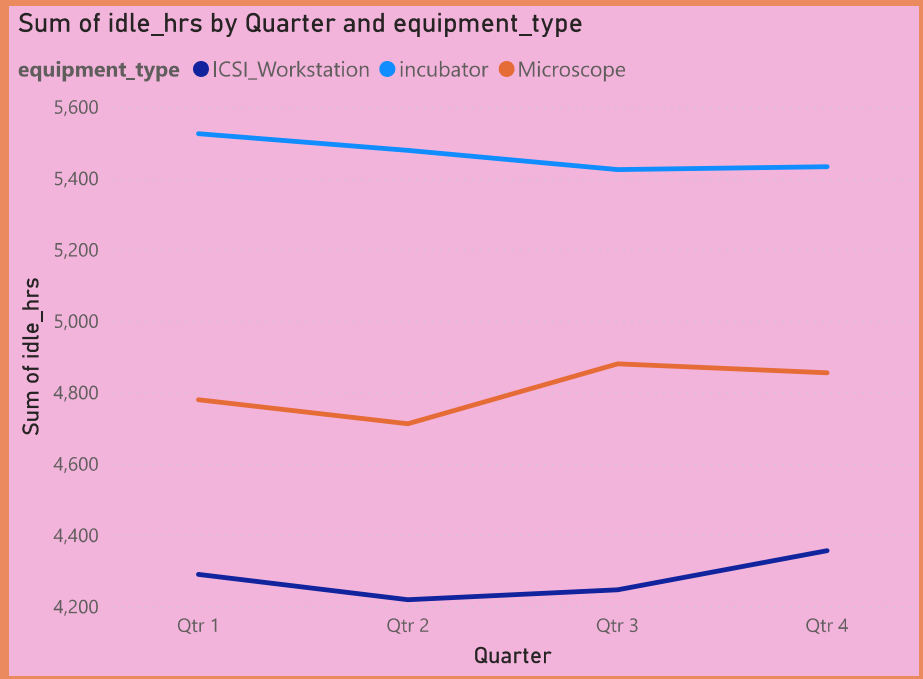
Sum of idle_hrs by Quarter and equipment_type
equipment_type
ICSI_Workstation
incubator
Microscope
5,600
5,400
5,200
5,000
4,800
4,600
4,400
4,200
Sum of idle_hrs
Qtr 1
Qtr 2
Qtr 3
Qtr 4
Quarter

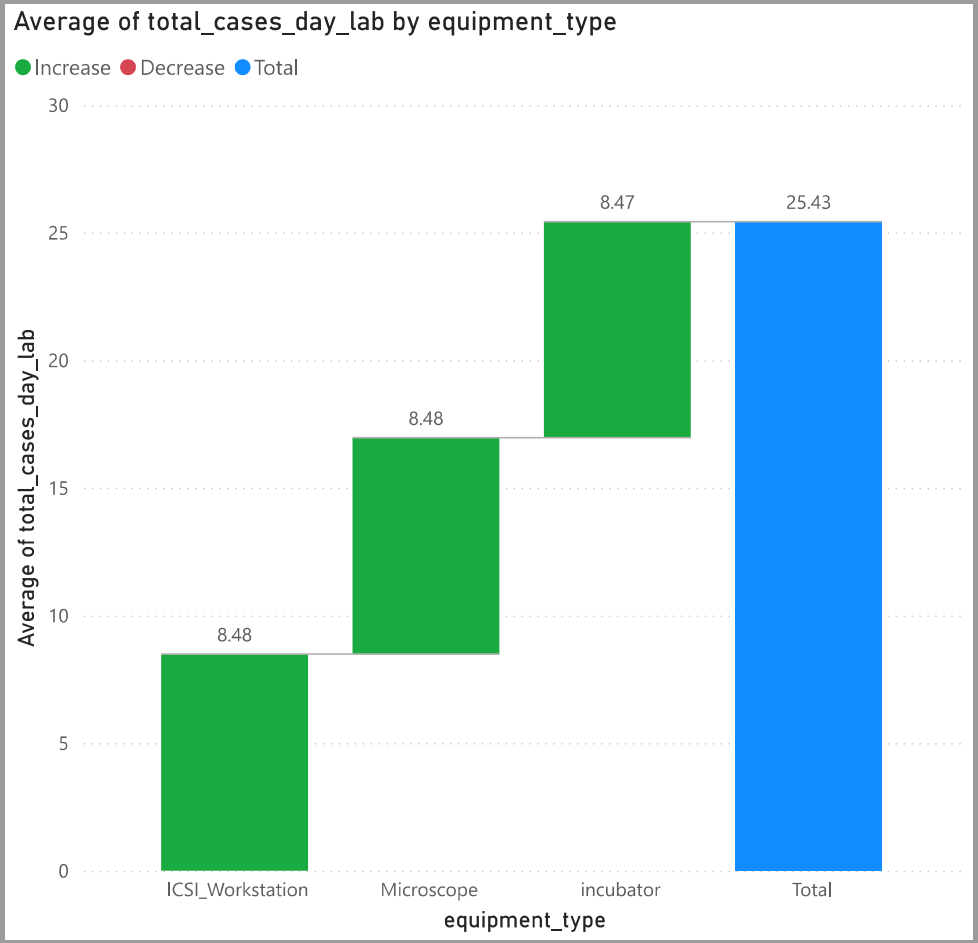
Average of total_cases_day_lab by equipment_type
Increase
Decrease
Total
30
25
20
15
10
5
0
Average of total_cases_day_lab
8.48
8.48
8.47
25.43
ICSI_Workstation
Microscope
incubator
Total
equipment_type

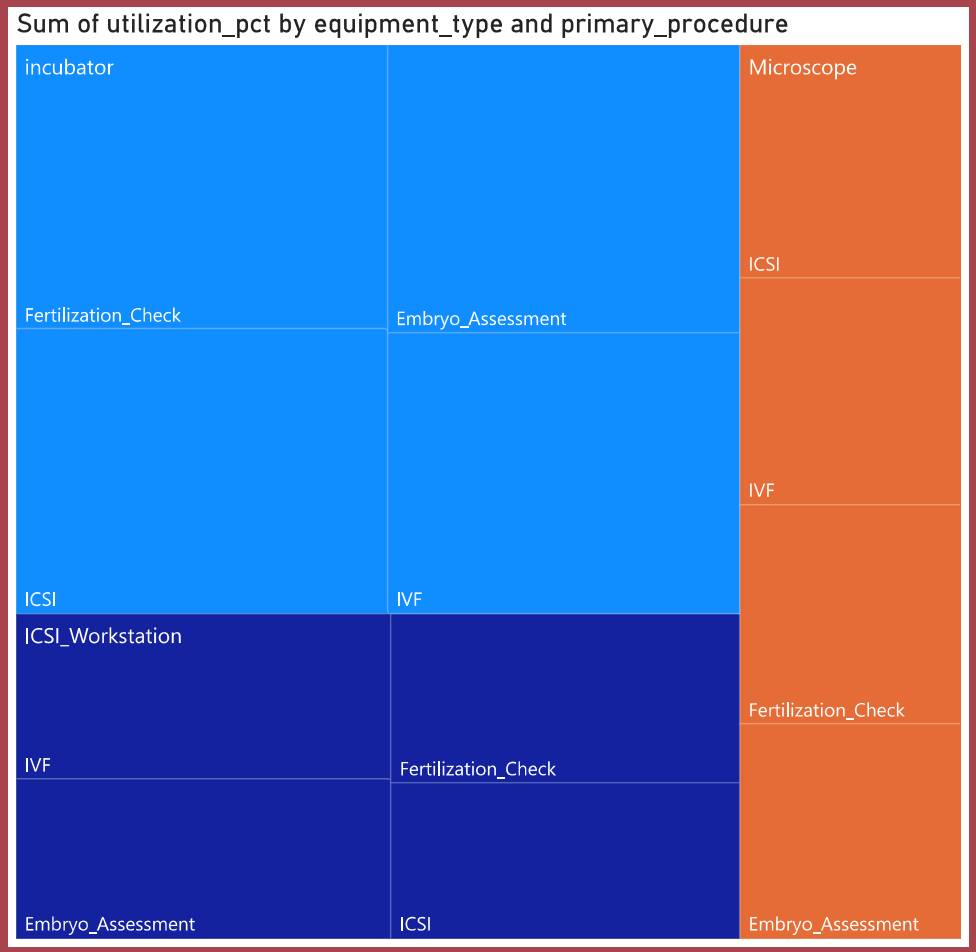
Sum of utilization_pct by equipment_type and primary_procedure
incubator
Fertilization_Check
ICSI
Embryo_Assessment
IVF
ICSI_Workstation
IVF
Embryo_Assessment
Fertilization_Check
ICSI
Microscope
ICSI
IVF
Fertilization_Check
Embryo_Assessment

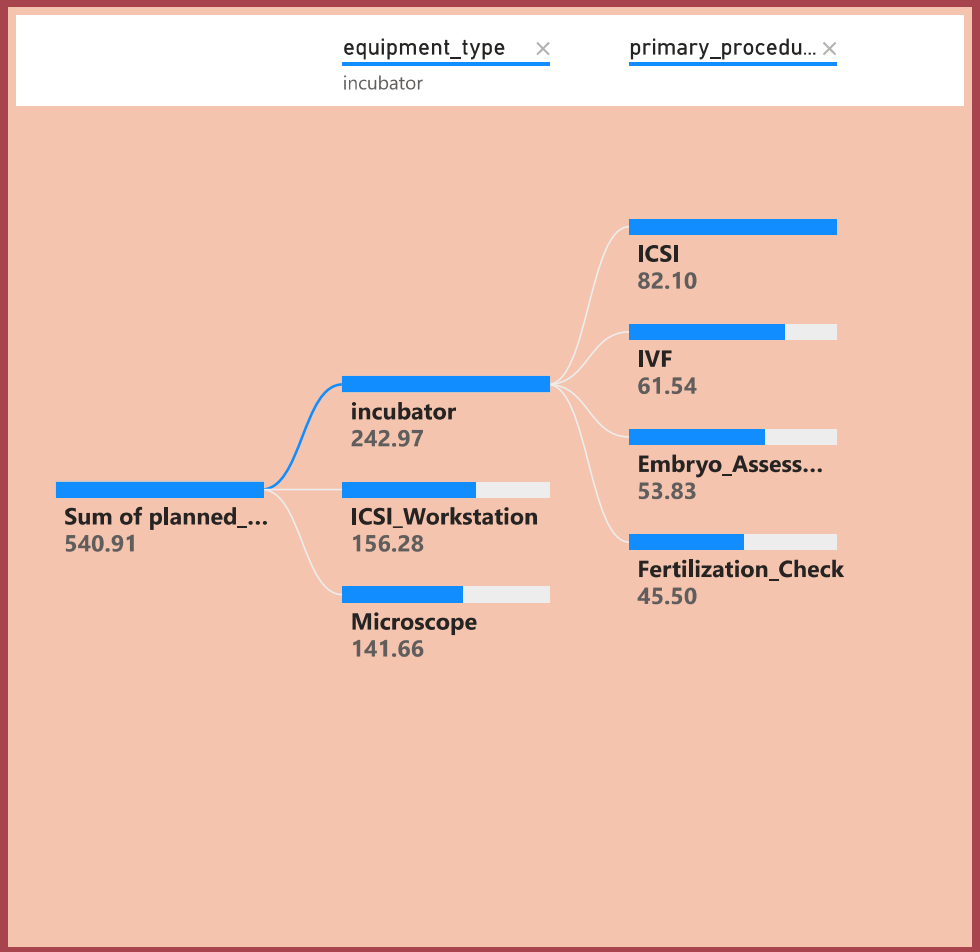
equipment_type
incubator
primary_procedu...
Sum of planned_...
540.91
incubator
242.97
ICSI_Workstation
156.28
Microscope
141.66
ICSI
82.10
IVF
61.54
Embryo_Assess...
53.83
Fertilization_Check
45.50

primary_procedure

- [ ] Embryo_Assessment
- [ ] Fertilization_Check
- [ ] ICSI
- [ ] IVF

Sum of utilization_hrs

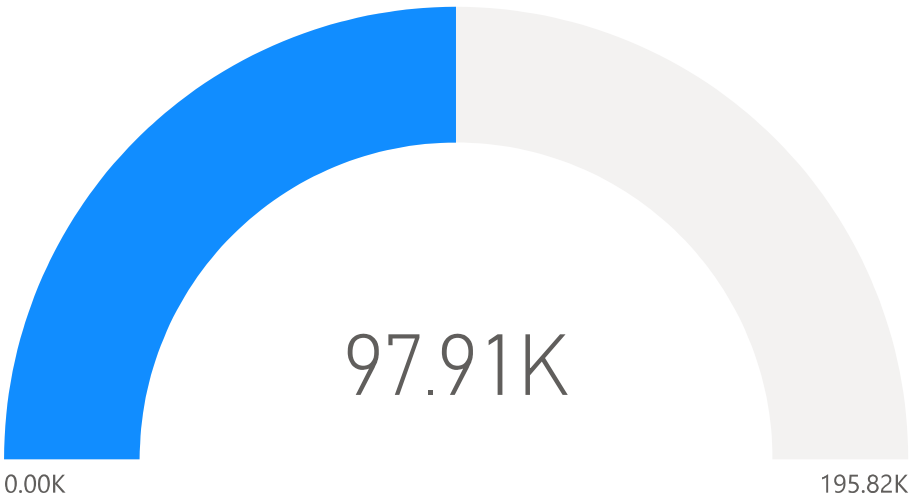

Sum of utilization_hrs and Sum of utilization_pct by primary_procedure