

Medical Physics

AVAILABLE ONLINE—See <http://www.medphys.org>


June 2014

Volume 41, Number 6

The International Journal of Medical Physics Research and Practice

2014 AAPM Annual Meeting Program

Austin, TX

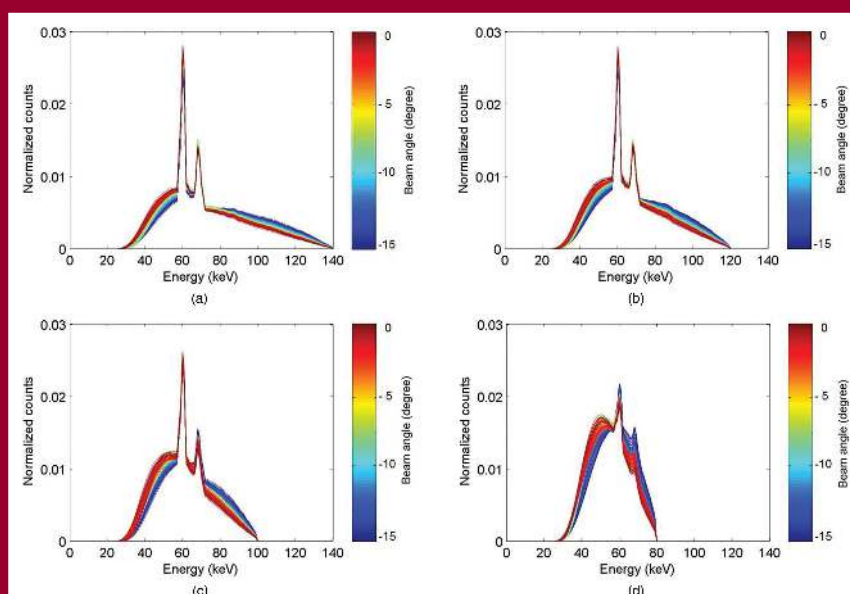

Plot of x-ray spectra from a commercial CT scanner as a function of off-axis angle (ranging from -15° to 1° , as indicated by the color bar), relative to central axis (0°) spectra in the transverse plane, clearly demonstrating beam hardening due to the bow-tie filter. Panels (a)–(d) show spectra for 140, 120, 100, and 80 kVp respectively. Spectra were reconstructed from experimentally-acquired narrow-beam transmission measurements through an off-center polyethylene cylinder.

[Figure 12 from Lin, Ramirez-Giraldo, Gauthier, Stierstorfer, and Samei, “An angle-dependent estimation of CT x-ray spectrum from rotational transmission measurements,” *Med. Phys.* 41, 062104 (12pp.) (2014)].

Published by the American Association of Physicists in Medicine (AAPM) with the association of the Canadian Organization of Medical Physicists (COMP), the Canadian College of Physicists in Medicine (CCPM), and the International Organization for Medical Physics (IOMP) through the AIP Publishing LLC. *Medical Physics* is an official science journal of the AAPM and of the COMP/CCPM/IOMP.

Medical Physics is a hybrid gold open-access journal.