

CALIBRATION

A STUDY IN THE PATIENT TUNING OF A SYSTEM

297 × 420 MM

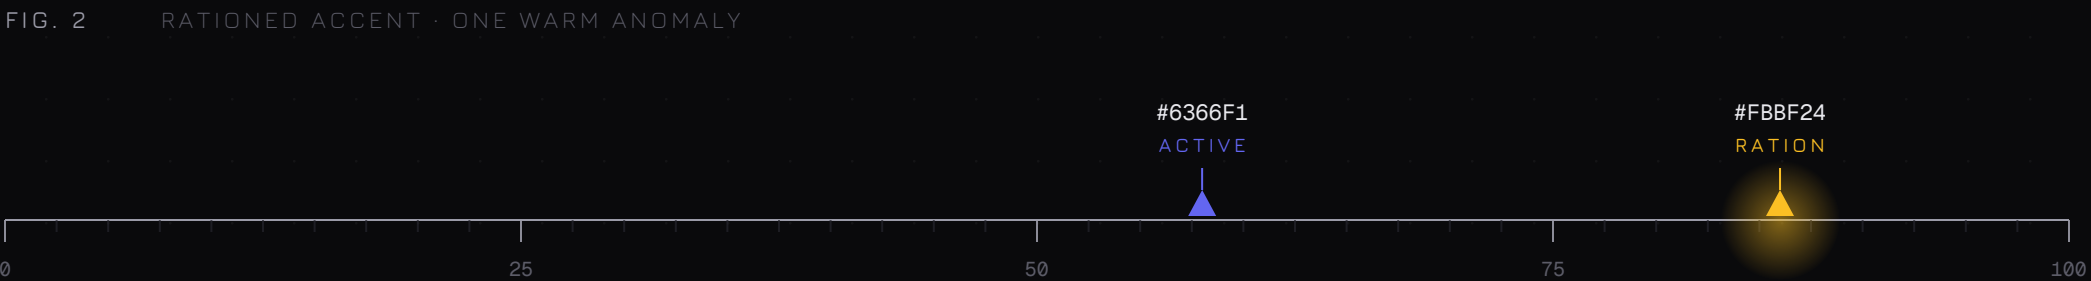
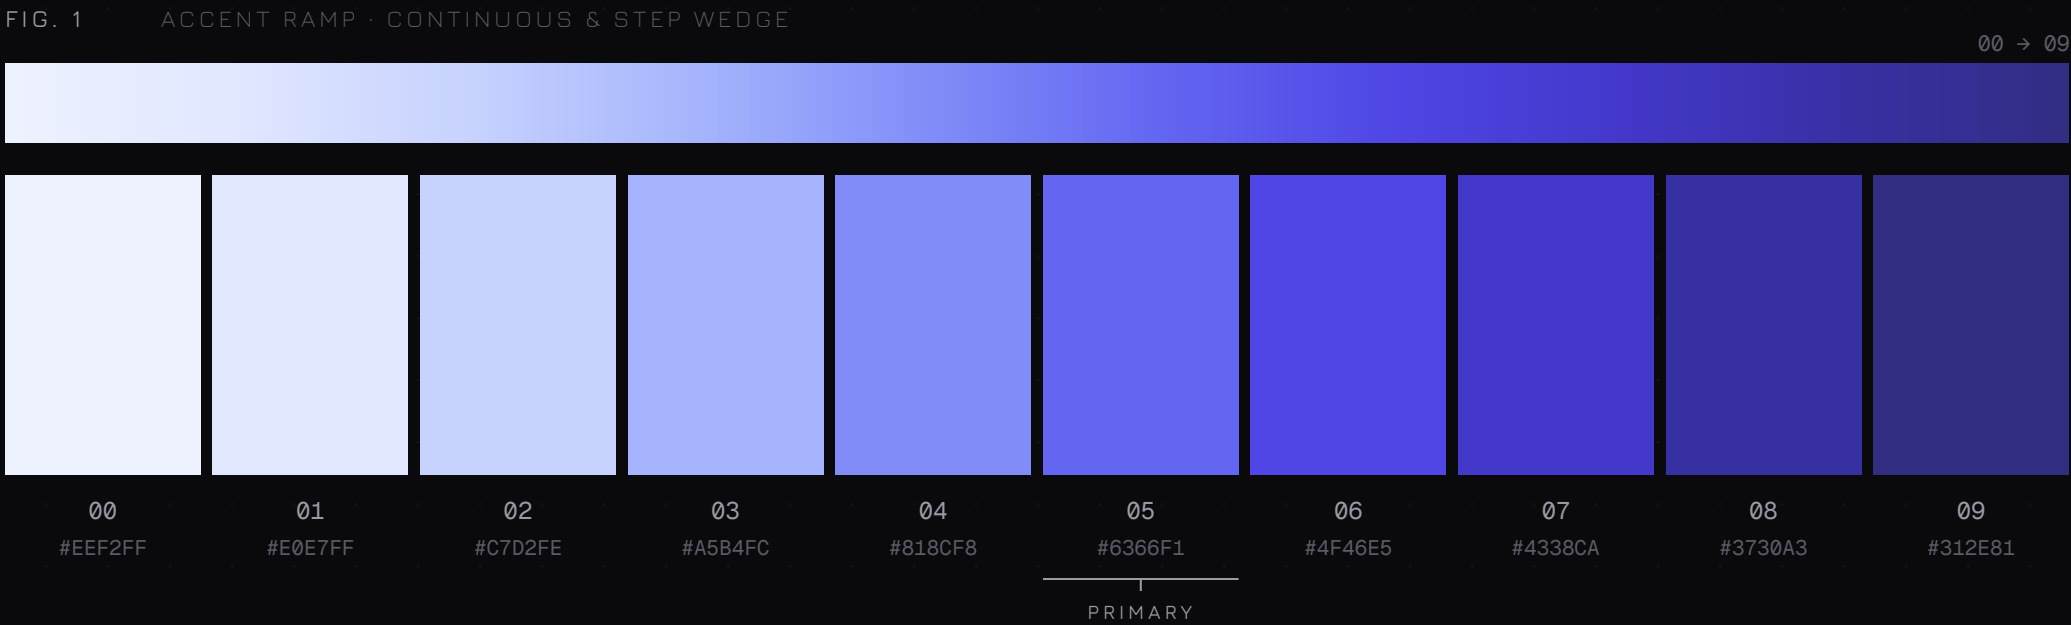


FIG. 3 SYSTEM REGISTER

TOKEN	VALUE	ROLE
GROUND	#0A0A0C	field / page
SURFACE	#1C1C22	card
BASE	#14141A	recessed
INK	#E9E9EE	text · primary
MUTED	#8A8A99	text · muted
ACCENT	#6366F1	active · cta
ACCENT · L	#4F46E5	active (light)
RATION	#FBBF24	rating

“The improvement is the silence between two values.”