

## **Varian OSMS Clinical Report**

**Patient Name: TB2871 ZZUWQA\_Daily (Other)**

**Patient Number: 20170308**


**Treatment Date: 27, March, 2017**

**Treatment Site: Chest**

### **OSMS Positioning Report prior to the Delivery of Treatment**

The OSMS system was used to position the patient immediately prior to treatment and to track the patient during treatment in 3D mode. The patient was monitored for 00:11:51.

The following parameters are the couch shifts which were computed by OSMS in the treatment position, in order to assess the accuracy of patient set-up and to prevent geographical miss with the radiation beam, in standard couch coordinates.

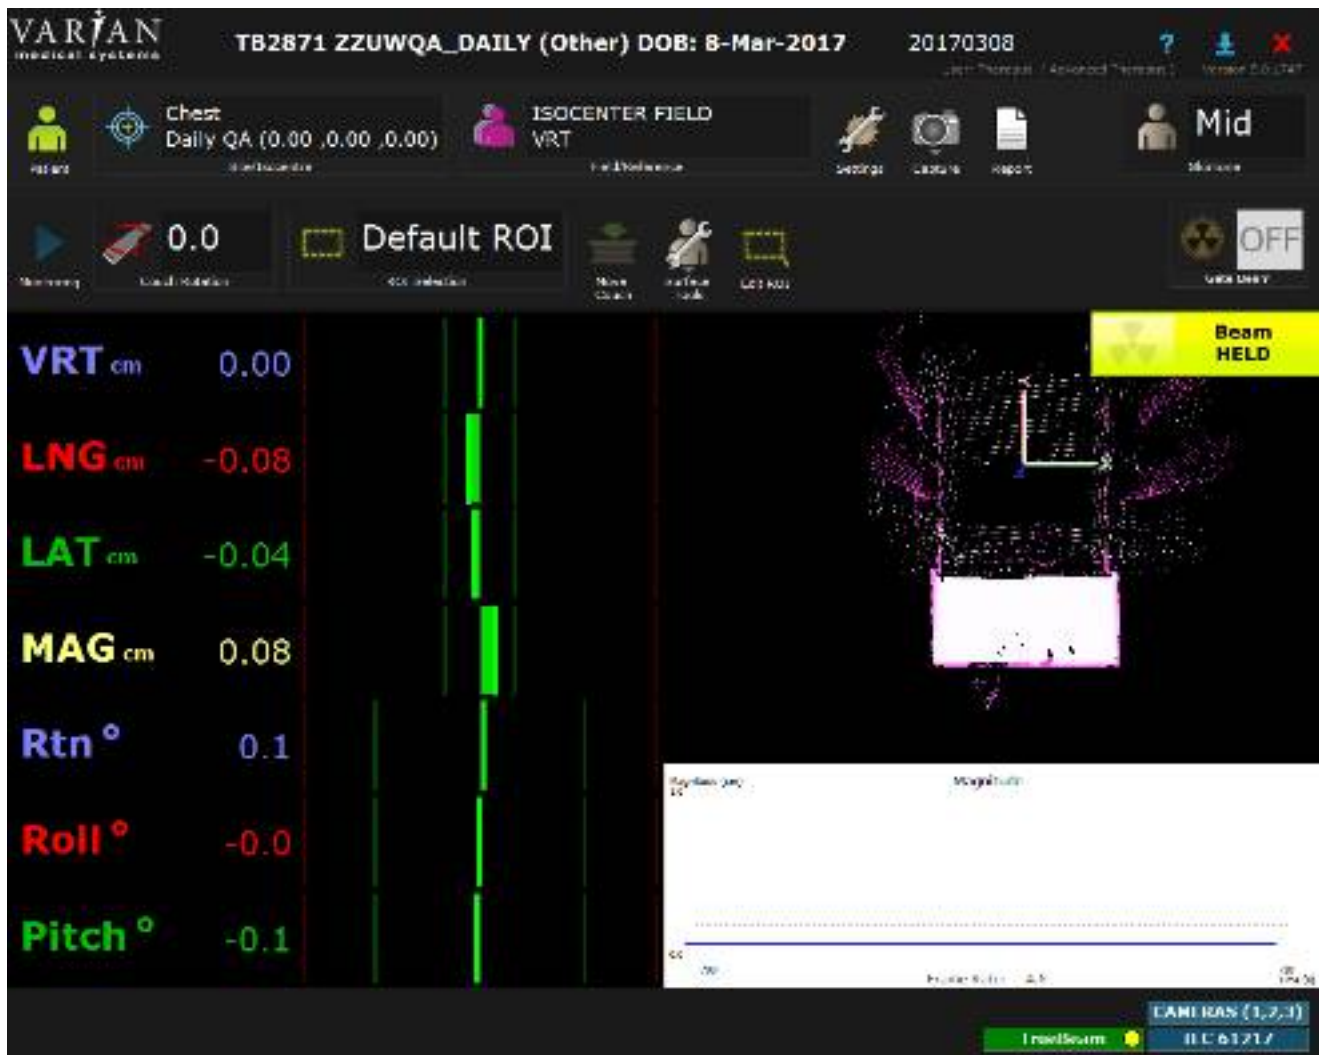

## Couch Angle: 0 Shifts

D\_VRT (cm): 0.00  
 D\_LNG (cm): -0.08  
 D\_LAT (cm): -0.04  
 D\_Rtn (degrees): 0.10  
 D\_Roll (degrees): -0.03  
 D\_Pitch (degrees): -0.12

The patient was aligned properly prior to treatment initiation and the patient position was tracked during treatment delivery. Imaging using the OSMS system was performed by the radiation therapist.

**RTT   Name: Therapist (Therapist)**

**Signature**

**MD   Name:**

**Signature**