

## **Varian OSMS Clinical Report**

**Patient Name: TB2871 ZZUWQA\_Daily (Other)**

**Patient Number: 20170308**


**Treatment Date: 16, May, 2017**

**Treatment Site: Chest**

### **OSMS Positioning Report prior to the Delivery of Treatment**

The OSMS system was used to position the patient immediately prior to treatment and to track the patient during treatment in 3D mode. The patient was monitored for 00:13:03.

The following parameters are the couch shifts which were computed by OSMS in the treatment position, in order to assess the accuracy of patient set-up and to prevent geographical miss with the radiation beam, in standard couch coordinates.

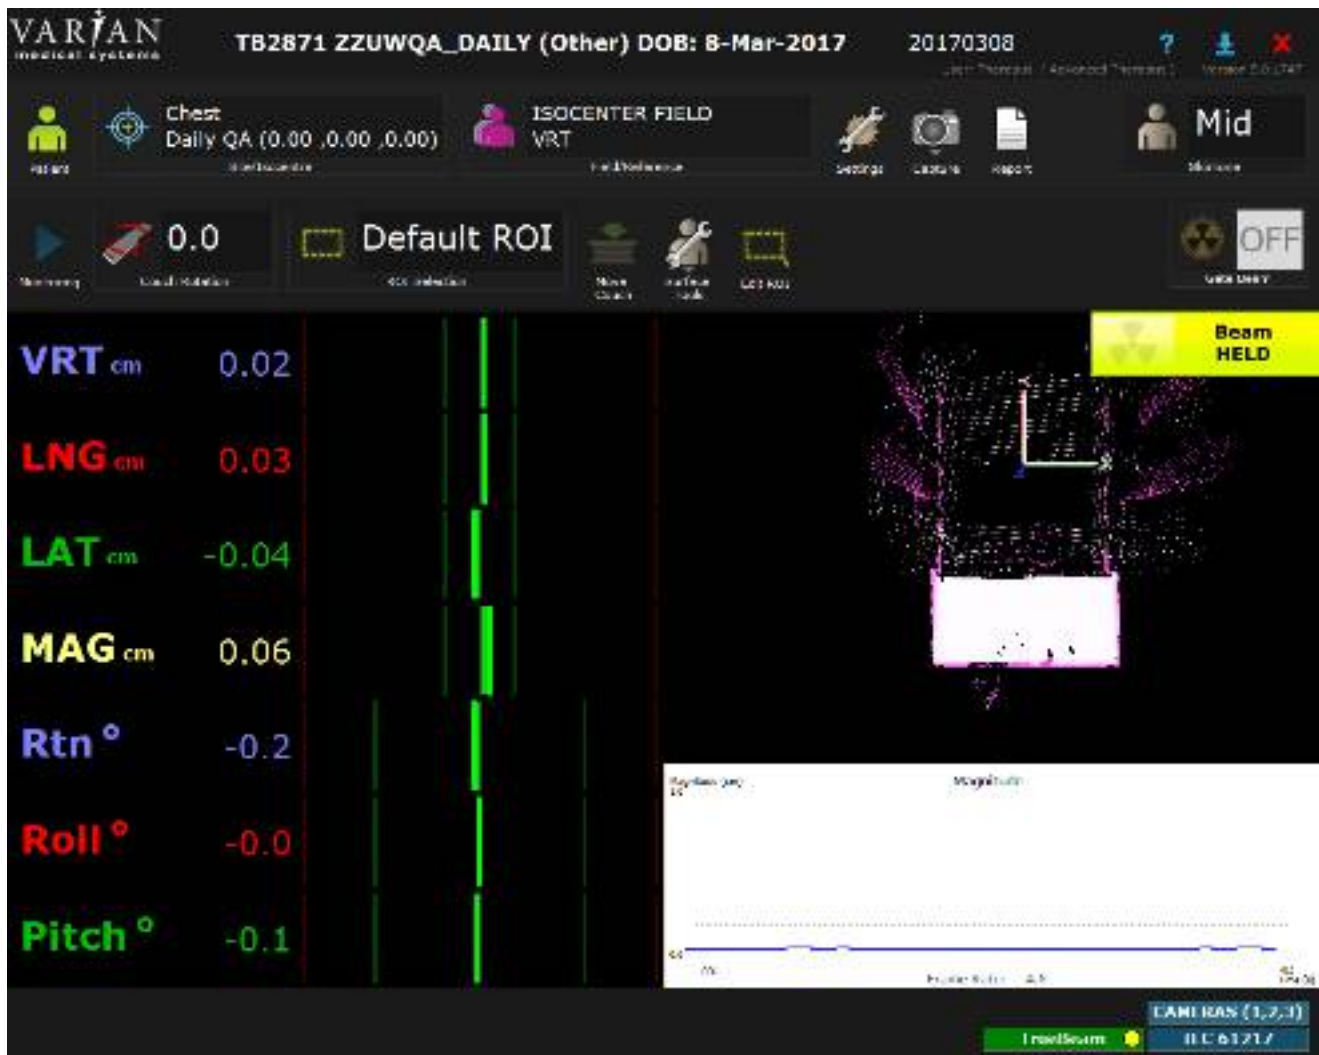

## Couch Angle: 0 Shifts

|                    |       |
|--------------------|-------|
| D_VRT (cm):        | 0.02  |
| D_LNG (cm):        | 0.03  |
| D_LAT (cm):        | -0.04 |
| D_Rtn (degrees):   | -0.19 |
| D_Roll (degrees):  | -0.03 |
| D_Pitch (degrees): | -0.10 |

The patient was aligned properly prior to treatment initiation and the patient position was tracked during treatment delivery. Imaging using the OSMS system was performed by the radiation therapist.

**RTT   Name: Therapist (Therapist)**

**Signature**

**MD   Name:**

**Signature**