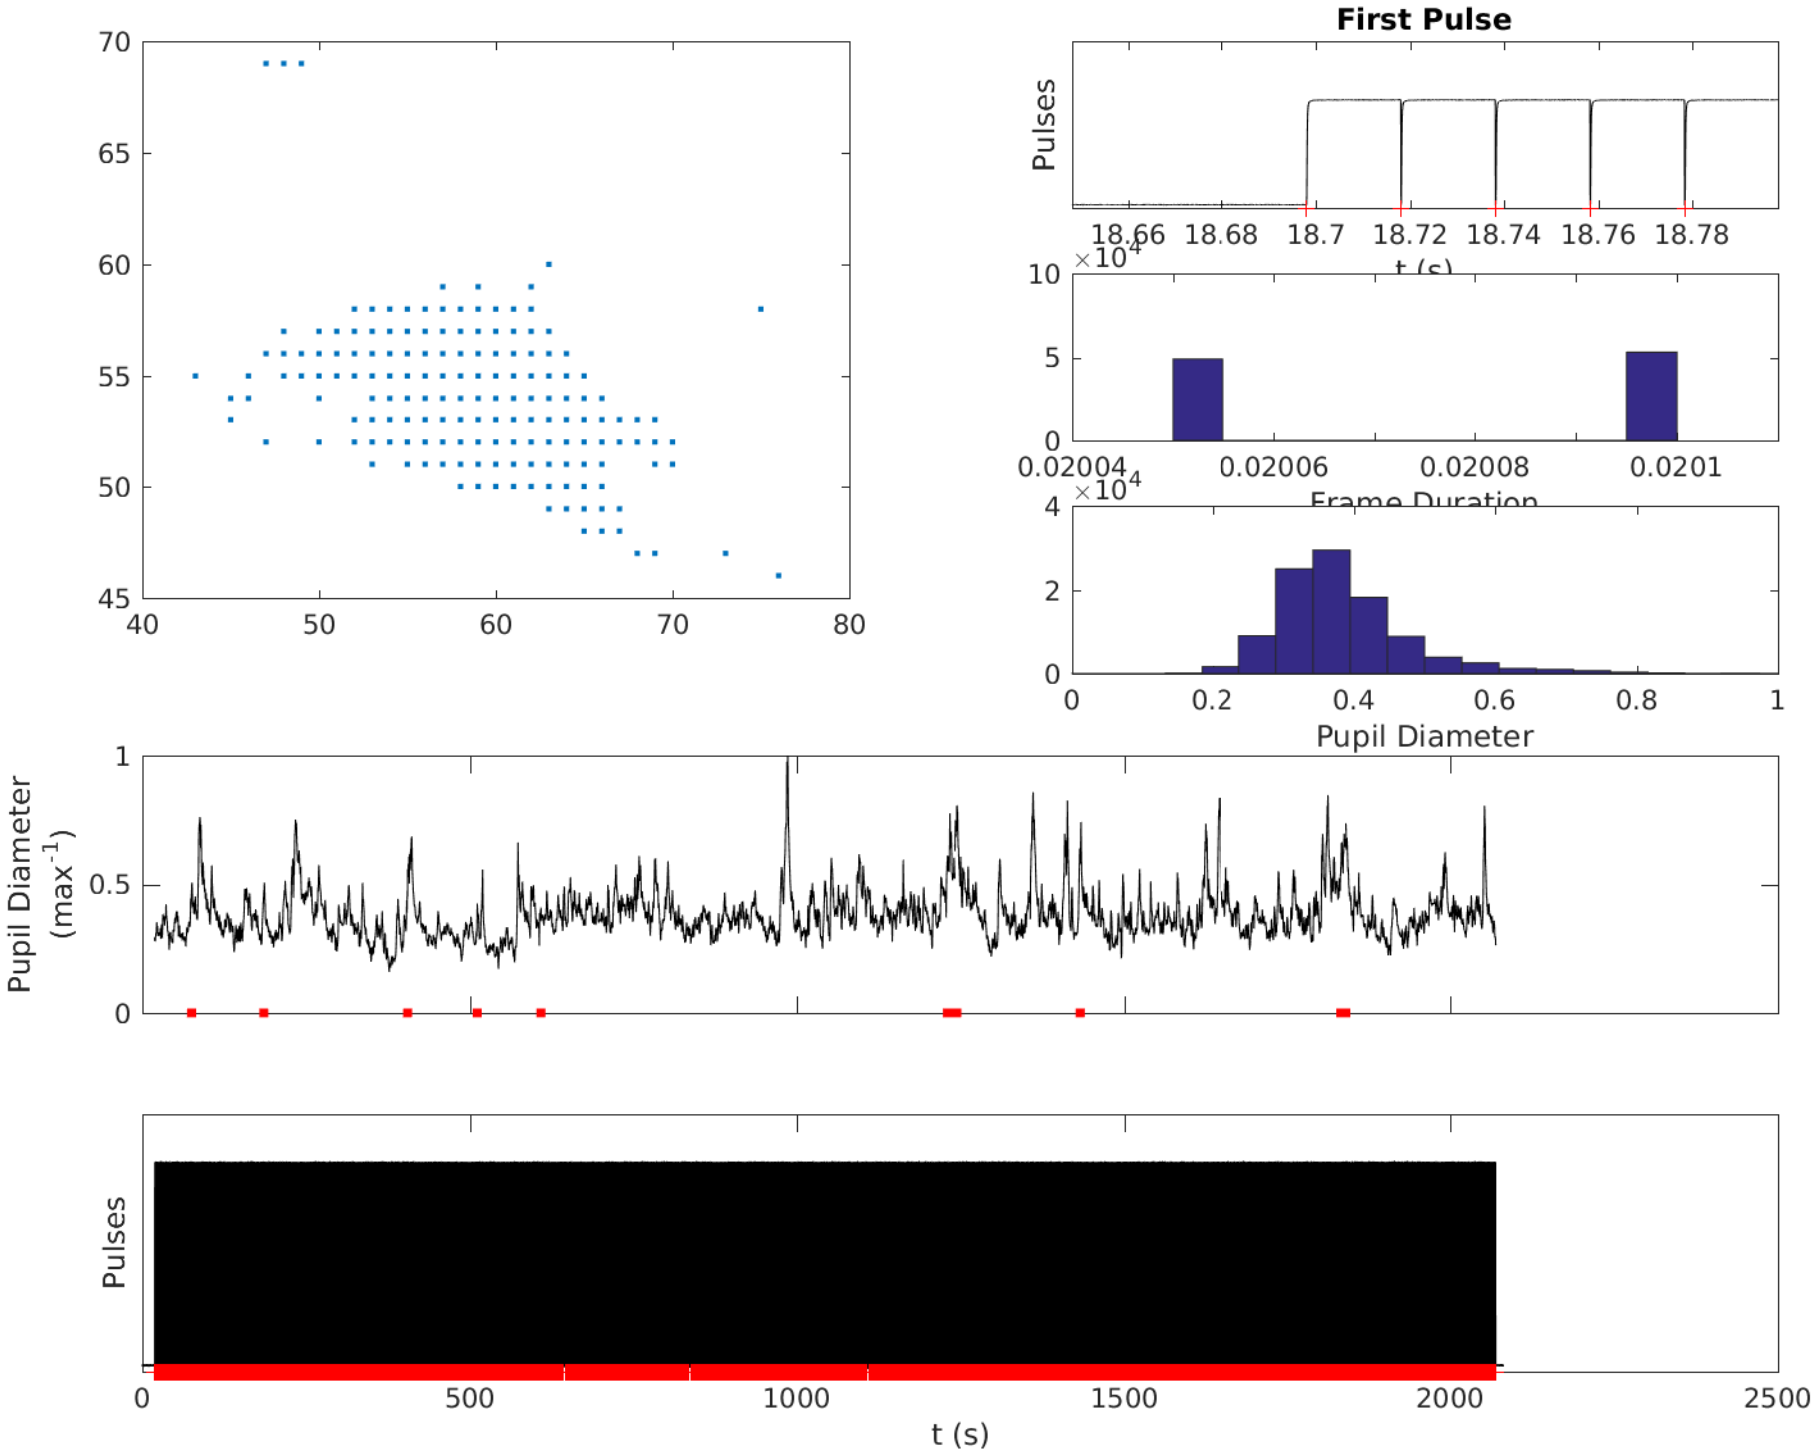
First Pulse
Pulses
18.66
18.68
18.7
18.72
18.74
18.76
18.78
t (s)
×10^4
0.02004
0.02006
0.02008
0.0201
Frame Duration
Pupil Diameter
Pupil Diameter (max^-1)
Pulses
t (s)

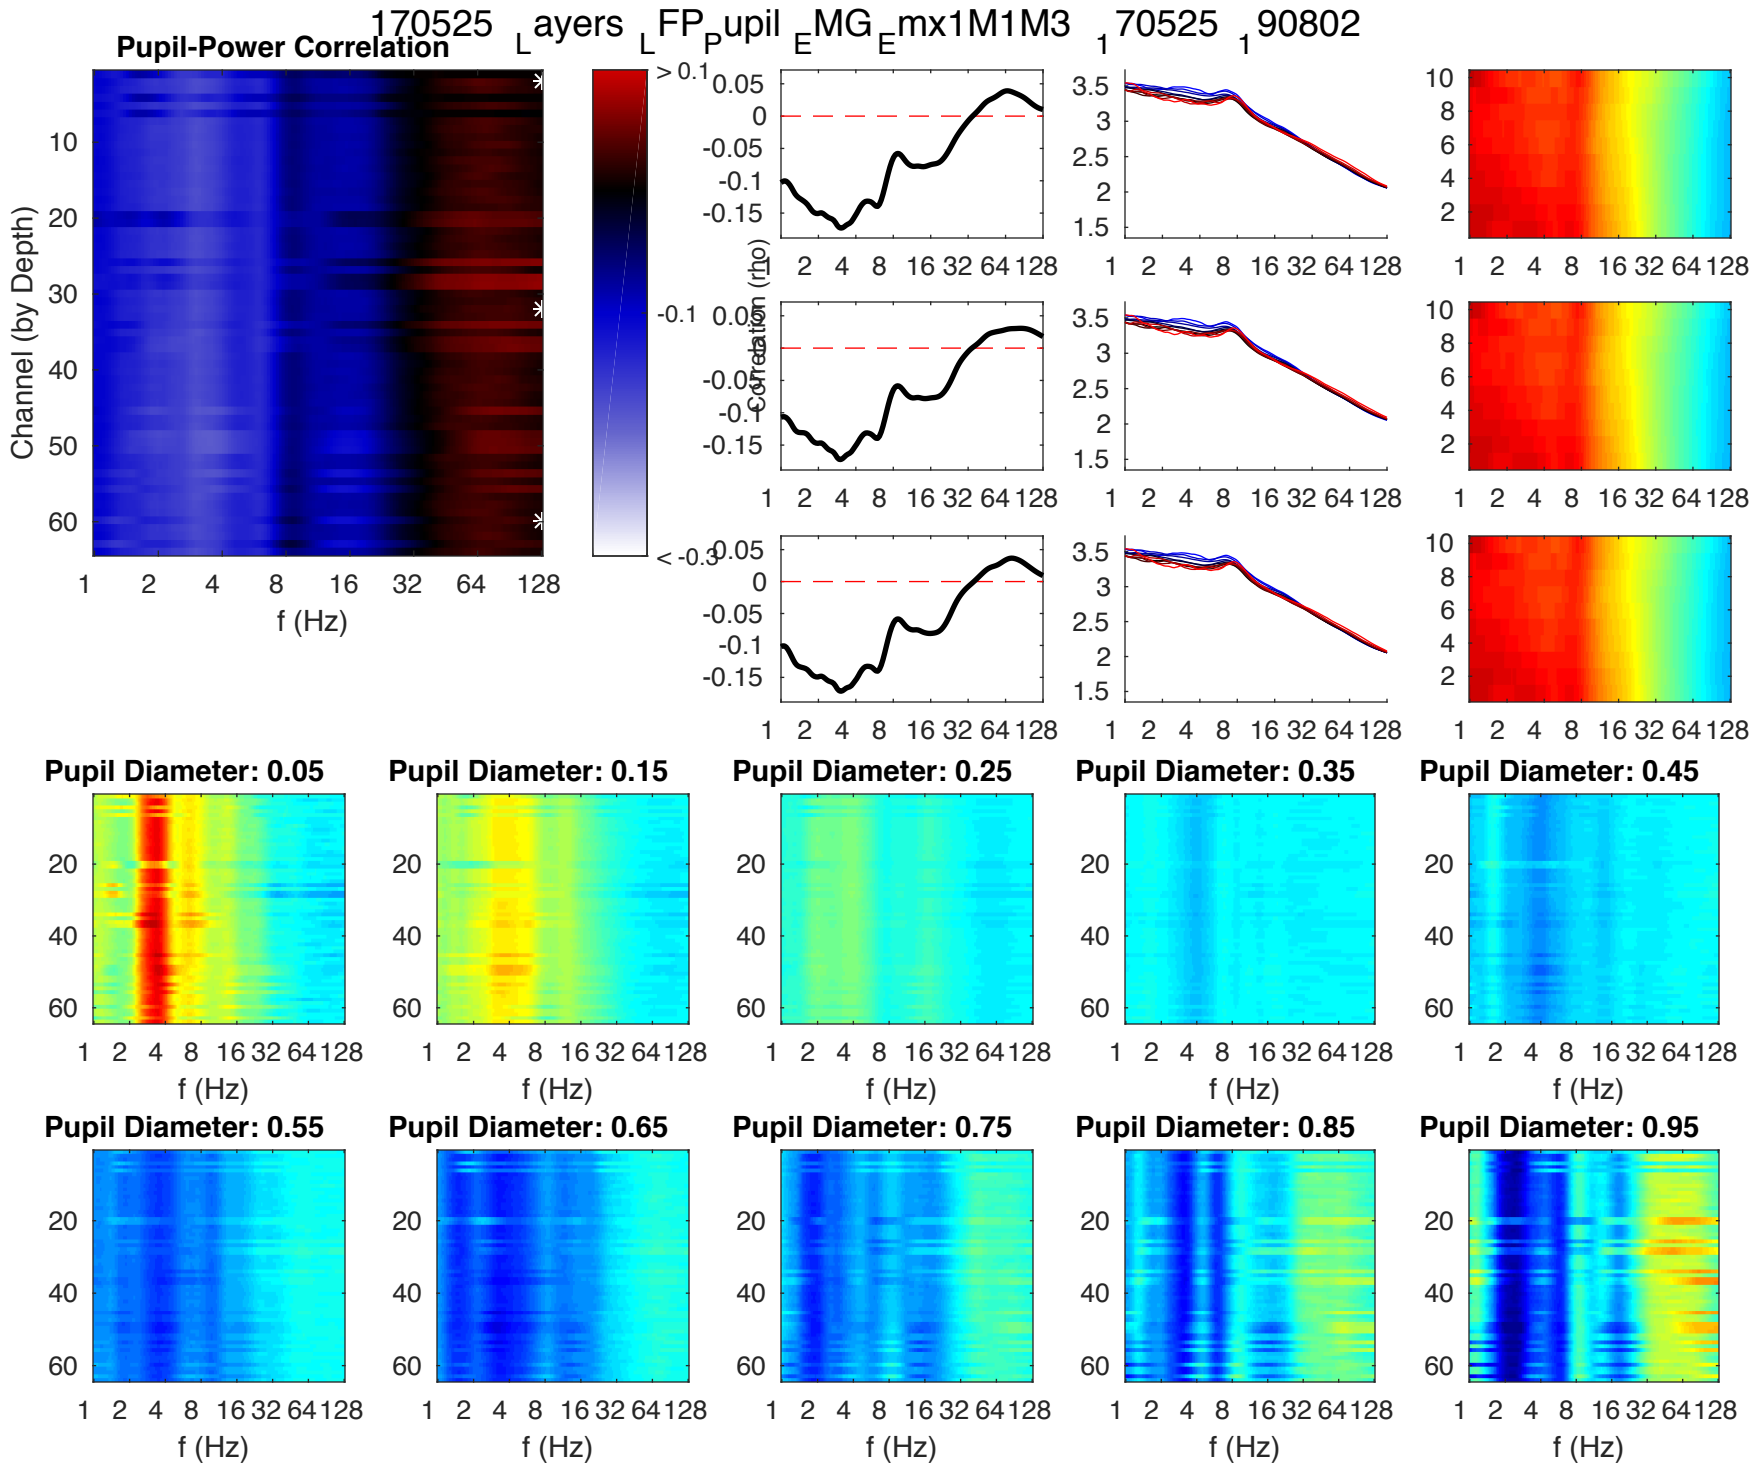
170525 Layers LFP pupil EMG Emx1M1M3 170525 190802
Pupil-Power Correlation
Channel (by Depth)
f (Hz)
> 0.1
-0.1
< -0.3
Correlation (rho)
Pupil Diameter: 0.05
Pupil Diameter: 0.15
Pupil Diameter: 0.25
Pupil Diameter: 0.35
Pupil Diameter: 0.45
Pupil Diameter: 0.55
Pupil Diameter: 0.65
Pupil Diameter: 0.75
Pupil Diameter: 0.85
Pupil Diameter: 0.95