UMOYA	DEVICE DESCRIPTION AND SPECIFICATIONS, INCLUDING VARIANTS AND ACCESSORIES
PRODUCT:	**MATERNAWELL TRAY**

Authorised by:	D J Morris	Date: November 2025	

1. DESCRIPTION OF THE PRODUCT

The MaternaWell PPH Tray is an injection moulded plastic tray of external dimensions height: 47.00 mm, width: 335.00 mm, length: 451.00 mm, and with two 500ml wells intended to receive and estimate post-partum fluids. The sides of the reservoirs are marked to indicate volumetric increments (300ml and 100ml intermediate indicators). A pouring spout facilitates emptying of the tray for accurate measurement or disposal of fluids. The device measures approximately 340mm by 450mm and weighs approximately 485g.

The tray should be washed after use to remove any residual blood or products and should sterilised in a suitable disinfectant before for use on the next patient. Alternatively, it may be sterilised by autoclave at a temperature not exceeding 121oC for 20 minutes. See IFU and training video for full instructions.

When supplied it is not sterile. The device is non-invasive.

The design promotes patient comfort, ease of use for health care practitioners and minimises soiling of linen.

The MaternaWell PPH Tray is manufactured from polypropylene which provides the necessary light weight, strength, durability, reusability and patient comfort and safety. The product is fully recyclable.

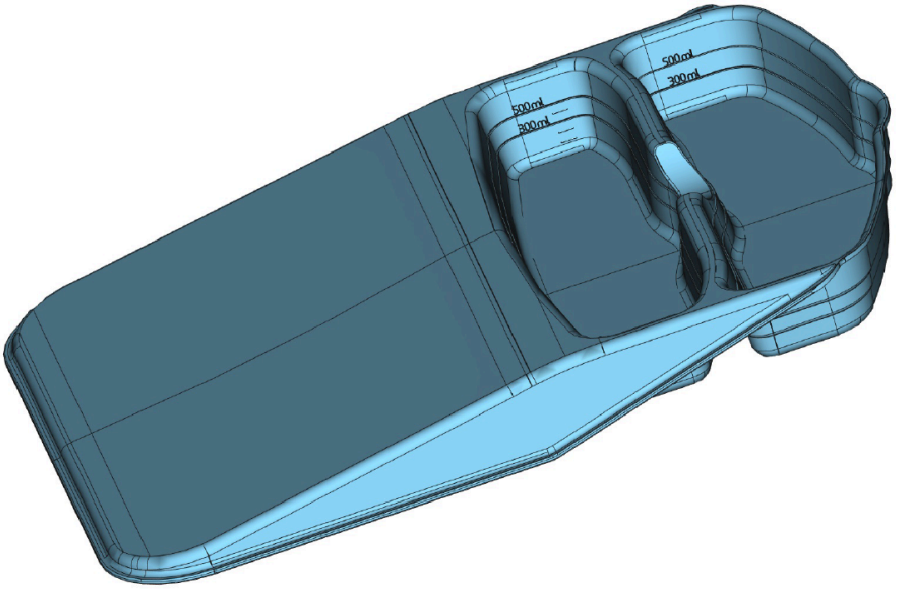

MaternaWell Tray

2. MEDICAL INDICATIONS

Post partum Haemorrhage (PPH) is a major cause of death and morbidity in women of child-bearing age in the developing world. Recognising PPH early is key to managing this largely preventable condition. By WHO definition, PPH is the loss of 500ml of blood or more following delivery of the placenta. Clear protocols exist that define actions to be taken when this critical threshold of blood loss is recorded to attempt to stop the bleeding and provide circulatory support for the mother and, when implemented timeously, lives are saved.

Assessing blood loss adequately has been difficult to achieve practically. Midwives often are left estimating blood loss based on the degree of blood soaking of the linen they observe but this is inherently inaccurate and can be considerably underestimated. Commercial drapes are available that can be weighed to quantify blood loss but they are expensive and create a waste and procurement burden which is especially problematic in low resourced settings. Using the Maternawell Tray provides a means of estimating blood loss as it happens (real time) which can promote rapid medical intervention if necessary.

The MaternaWell Tray provides an indication of blood loss. If an accurate measurement is required, the contents should be emptied into a measuring cylinder via the pouring spout. Alternatively, the tray may be weighed, and the empty weight subtracted.

3. NOVEL FEATURES

The MaternaWell Tray provides a means of instantaneous estimation blood loss with improved reliability in most situations which enables more timely medical support.

4. PATIENT POPULATION

Women in childbirth

5. CLINICAL USE

The tray is placed on the bed under the buttocks of the new mother in a recumbent position after birth of the baby. The tray is designed to catch any vaginal bleeding in the first well that has a maximum volume of 500ml before overflowing into the second well. Graduations allow for progressive real-time estimation of the contents before overflow. The tray remains in place until the birth attendant is satisfied that bleeding has stopped.

This provides a visual indication of both the rate and quantity of bleeding that is occurring as well as indication when the critical volume of 300ml/500ml has been reached which would trigger the PPH protocols. Continuing to monitor bleeding allows further for more accurate estimation of blood transfusion and resuscitation fluid volumes.

The device can be used in theatres, maternity wards, and for clinic and home births.

On the underside of the tray users can find diagrammatic information on how to position the product.

6. LIMITATIONS

None known.

7. CONTRAINDICATIONS

None known.

8. PRECAUTIONS

The device should be clean and sanitary prior to first use and cleaned and sterilised after use and before storage. The device is robust but should be routinely visually inspected for physical damage and recycled or disposed of if such damage has occurred (See 10 below).

9. MATERIAL OF CONSTRUCTION, METHOD OF MANUFACTURE AND PACKAGING

The device is manufactured from polypropylene using injection moulding.

When packaged the device is not sterile and should be cleaned and sterilised prior to first and subsequent uses.

The device is packaged in recyclable cardboard boxes of 20 units. Each box having the dimensions 470mm x 420mm x 350mm and weighing 12kg.

10. USEFUL LIFE AND INSTRUCTIONS FOR DISPOSAL

If used according to the instructions the device should have a working life of many cycles.

If the product is damage or showing signs of excessive wear it should be cleaned and sterilised and can then be safely disposed of or recycled under plastic recycling code PP or 5.

The MaternaWell Tray has a shelf life of 10 years when stored in clean and dry conditions at temperatures below 55°C.