INSTRUCTIONS FOR USE

STEP 1

Remove the clean MaternaWell Tray™ from the delivery pack (or sterilize as per option 1 or 2 if being removed from storage).



STEP 2

Handle all bodily fluids with gloves and appropriate protective equipment.. After the baby is born, place the MaternaWell Tray™ with the ramp under the mother and her perineum over the first well.

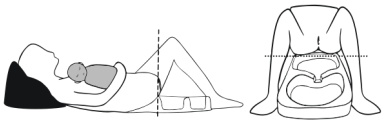

STEP 3

When the placenta is delivered, it may be placed in the second well and then removed.



STEP 4

Continue to monitor the following:
Volume of blood in the wells.
Blood captured in other places (swabs, gauze, mops, etc.)
Note if urine or other fluids collect in the wells
Calibrations are for estimation only.

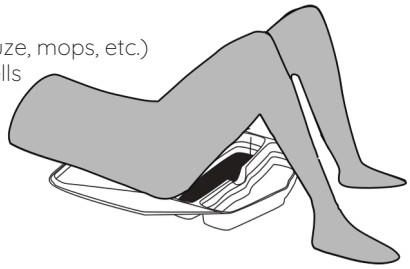

STEP 5

If blood spills over from the first to the second well, the volume is about 500mL - the volume that defines postpartum haemorrhage.

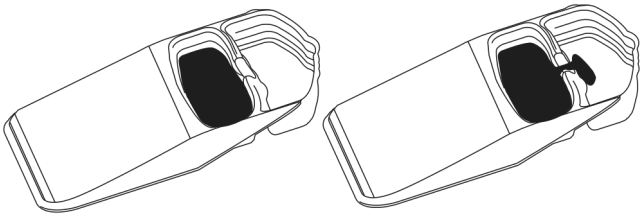

STEP 6

Remove the MaternaWell Tray™ when active bleeding stops. If more accurate measurement is needed, pour contents into measuring jar. Replace the MaternaWell Tray™ if active bleeding resumes.

ALTERNATIVE USES

The device may also be used in a reversed orientation.

ALTERNATIVE USES

With lithotomy position, the wedge of the tray may be inserted under the mattress.

Caution: be mindful of excessive tipping

REMOVE THE DEVICE IN ANY OF THE FOLLOWING SITUATIONS

- If the patient complains of discomfort related to the device. (in this case, the reverse orientation may be tried).
- If the patient needs an intervention that cannot accommodate the device.
- For routine or necessary practices, e.g. encouraging the mother to use the toilet.

MATERIAL

Plastic (polypropylene)

REPROCESSING

Immediately after each use, dispose of contents of the MaternaWell Tray™. Wash thoroughly with soap and warm water to remove all visible soiling. The MaternaWell Tray™ may then be chemically cleaned by immersion in a high-level disinfectant according to the supplier's instruction. After sterilisation, the MaternaWellTray™ should be air-dried. Store per facility guidelines.

MATERNOVA.NET
UMOYA.ORG.ZA

MATERNAWELL TRAY™

UMOYA

maternova

MATERNAWELL TRAY™

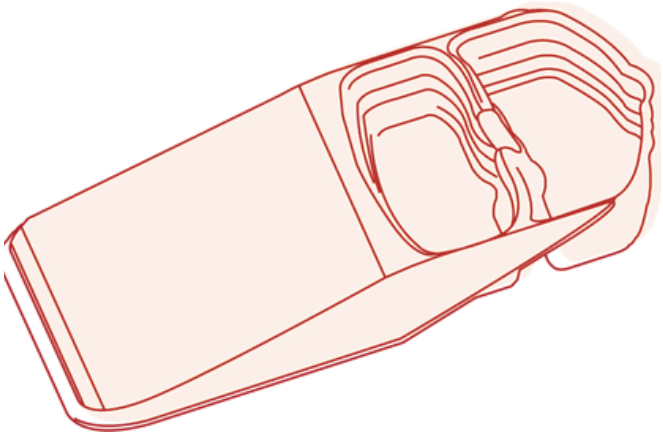

STERILISATION

The MaternaWell Tray™ is designed to be used many times and this requires the tray to be thoroughly cleaned and sterilised after use.

Immediately after use the product should be washed with a detergent and rinsed with clean water so that all visible blood and soiling is removed.

There are two means of sterilising the MaternaWell Tray™ depending on the resources available at the facility.

Option 1: Autoclave Sterilisation

The recommended autoclave sterilisation temperature is 121 degrees C for 20 minutes. A higher termperature or a longer process may degrade the tray more quickly.

Option 2: Wet Chemical Sterilisation

If autoclaving is not available, the MaternaWell Tray™ can be wet chemically sterilised using a commercial sterilising solution. We recommend using the sterilising solution commonly used at each facility such as Cidex, PrimeSafe Sterilit, or other agents such peracetic acid solution, etc. Some of these products can be hazardous and it is important to follow the manufacturer's safety instructions and directions for use. The cleaned MaternaWell Tray™ should be completely immersed in the solution for the time prescribed by the manufacturer of the sterilising agent. After sterilisation the tray should be rinsed and dried prior to storage and reuse.