


Predictive power of the uncalibrated simulator

Every preregistered point (blue, orange, red) was committed before measurement

measured ratio

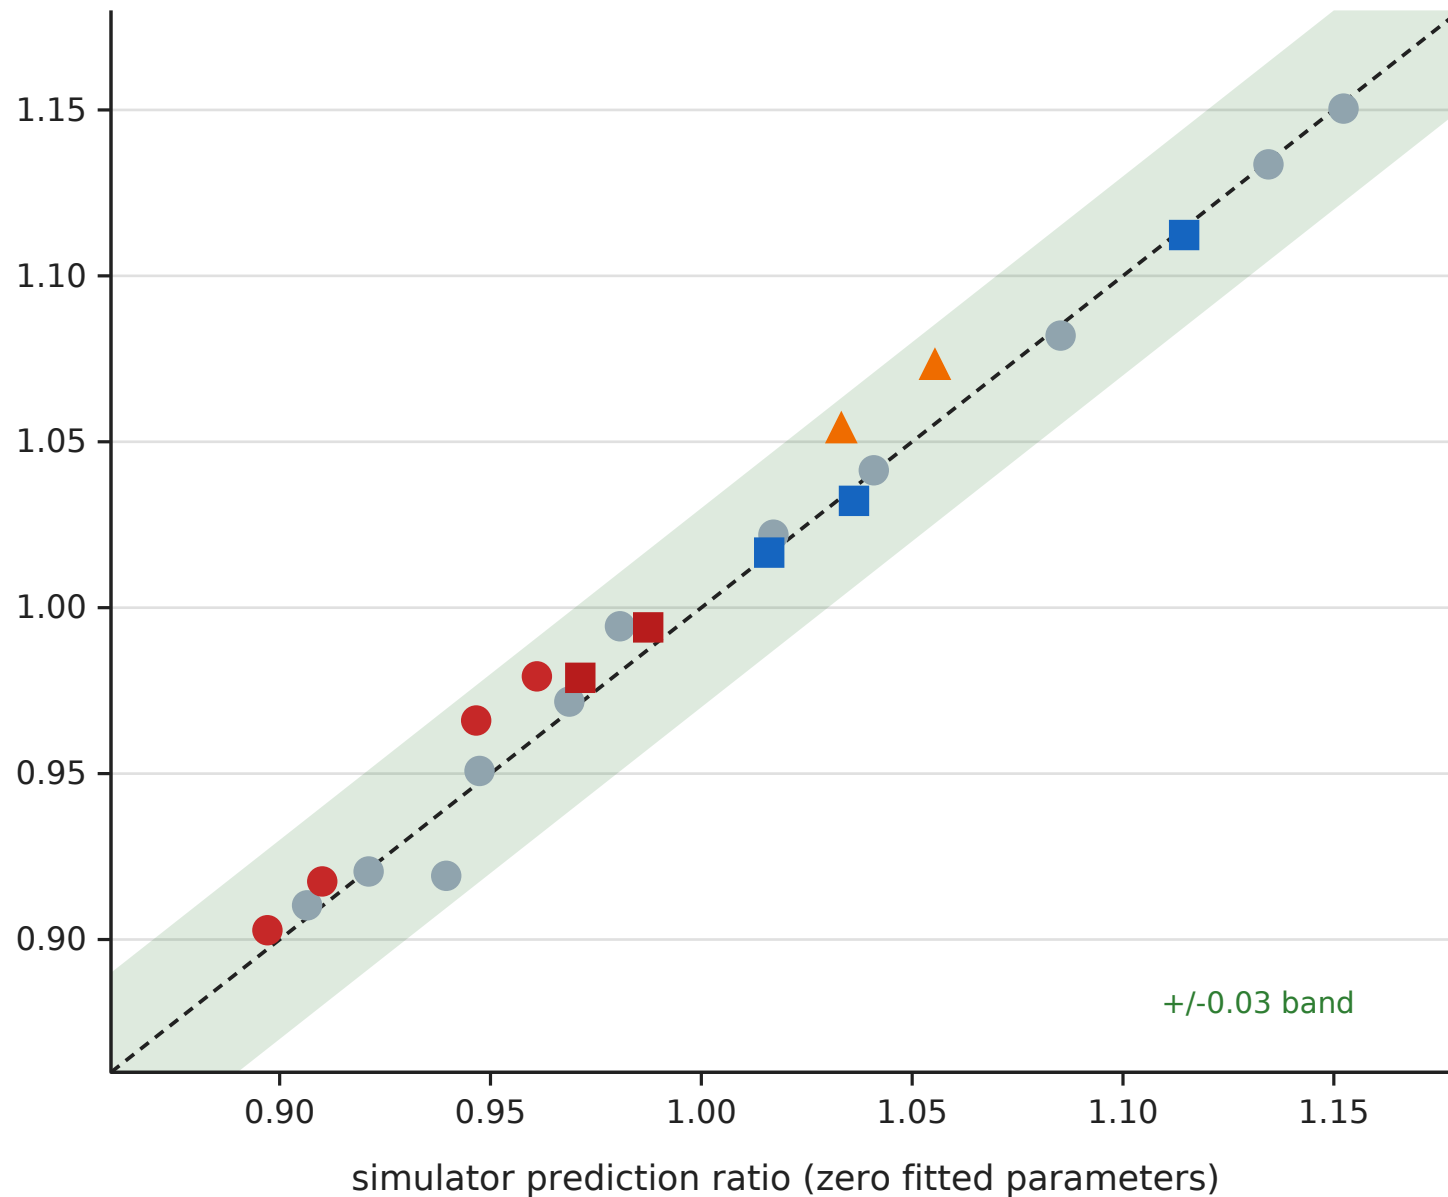

- in-sample (TASK24, 11 pts)
- out-of-sample prereg. (TASK25, 3 pts)
- device + policy (TASK28, 2 pts)
- device + compile cfg (TASK35, 4 pts)
- N=6 reconfirm (TASK36, 2 pts)